


Data Path : U:\HPCHEM1\BNA E\Data\BE012518\  
 Data File : BE095106.D  
 Acq On : 25 Jan 2018 8:47  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_E\METHODS\8270-SIM-BE012318.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Jan 23 15:47:25 2018

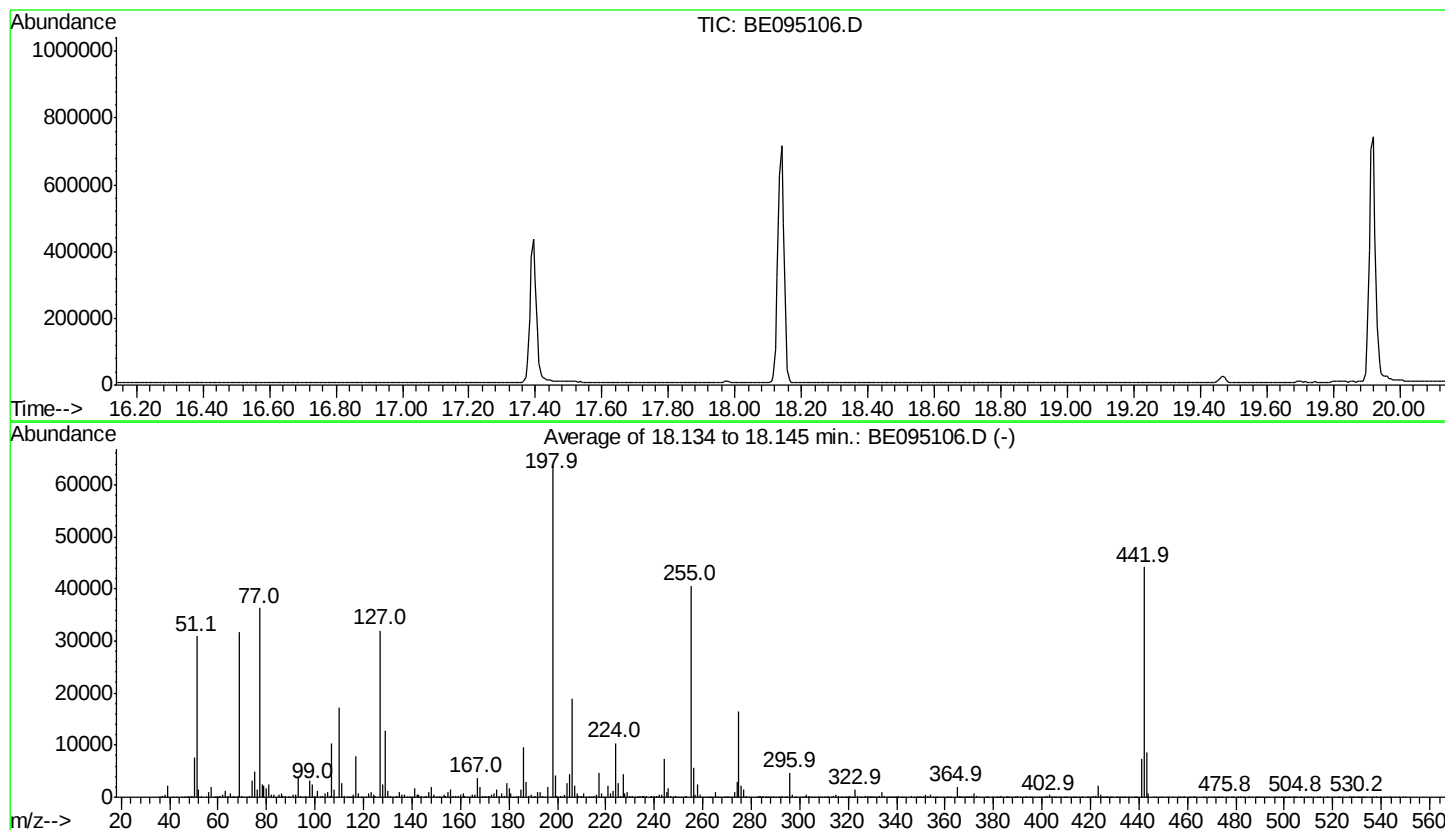

AutoFind: Scans 2646, 2647, 2648; Background Corrected with Scan 2639

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 48.5      | 30882   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.8       | 259     | PASS             |
| 69          | 198          | 0.00         | 100          | 49.8      | 31695   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.5       | 147     | PASS             |
| 127         | 198          | 10           | 80           | 50.3      | 32032   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 63651   | PASS             |
| 199         | 198          | 5            | 9            | 6.7       | 4271    | PASS             |
| 275         | 198          | 10           | 60           | 25.8      | 16423   | PASS             |
| 365         | 198          | 1            | 100          | 3.1       | 2000    | PASS             |
| 441         | 442          | 0.01         | 24           | 16.5      | 7296    | PASS             |
| 442         | 198          | 50           | 100          | 69.4      | 44146   | PASS             |
| 443         | 442          | 15           | 24           | 19.3      | 8529    | PASS             |