

Data Path : Z:\HPCHEM1\BNA E\DATA\BE012618\
 Data File : BE095129.D
 Acq On : 26 Jan 2018 15:59
 Operator : SJ/JU
 Sample : PB105822BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK22

Quant Time: Jan 26 17:41:21 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 26 13:41:10 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	3103	0.40	ng/ul	0.00
2) Naphthalene-d8	11.27	136	9694	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	6106	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.71
16) Chrysene-d12	21.80	240	14913	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	19031	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.82	152	5713	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	17687	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	20.05	202	2427	0.048	ng/ul#	1
23) Benzo(a)pyrene	24.27	252	5436	0.091	ng/ul#	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE012618\
Data File : BE095129.D
Acq On : 26 Jan 2018 15:59
Operator : SJ/JU
Sample : PB105822BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK22

Quant Time: Jan 26 17:41:21 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 26 13:41:10 2018
Response via : Initial Calibration




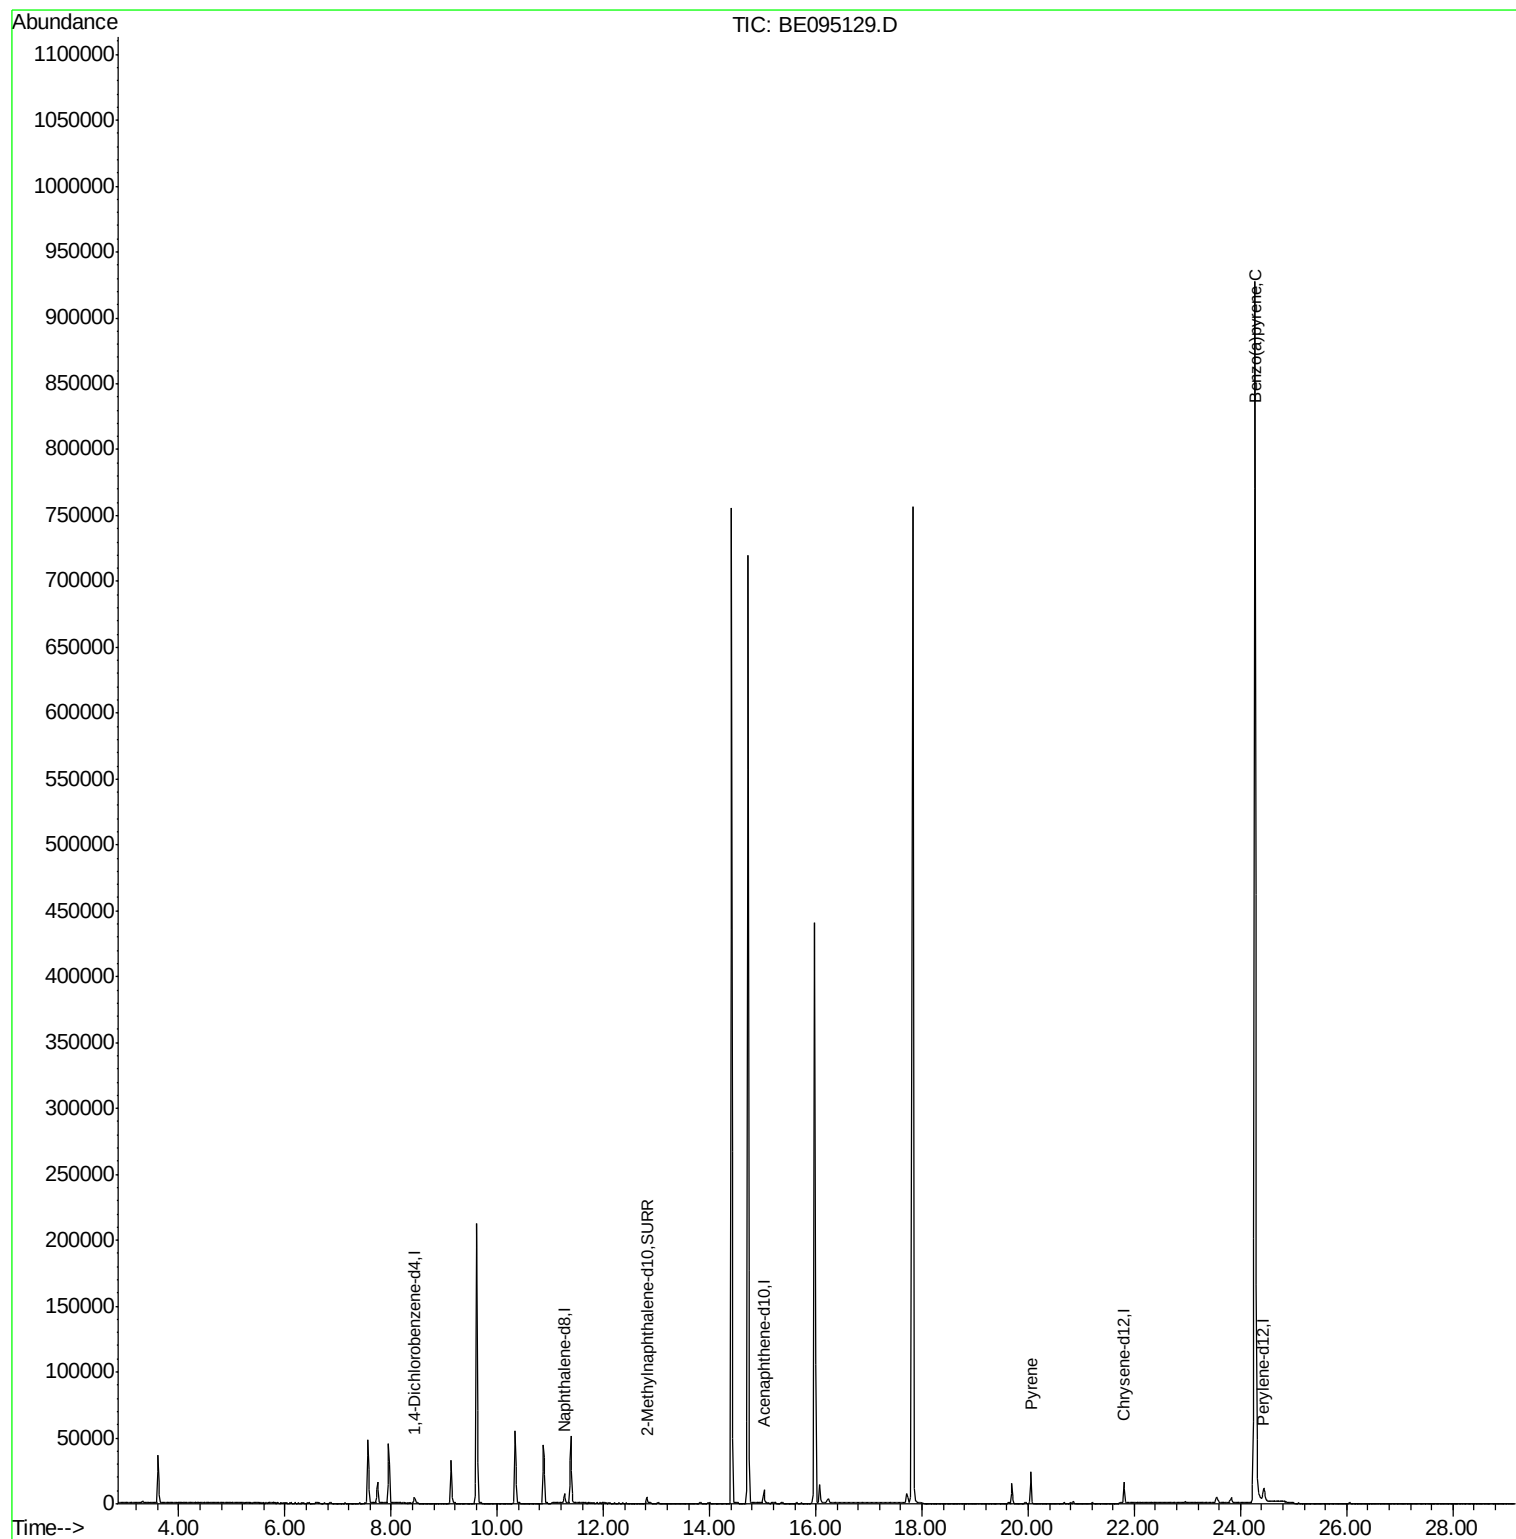


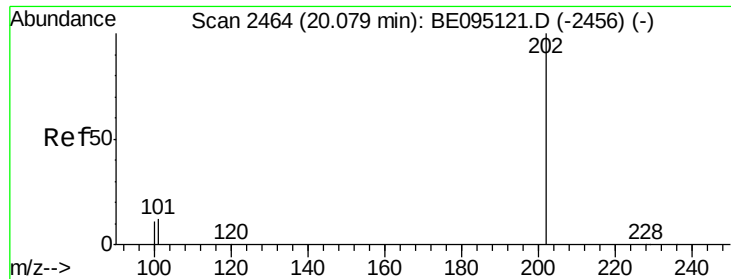

#17
Pvrene
Concen: 0.048 ng/ul
RT: 20.05 min Scan# 2460
Delta R.T. -0.03 min
Lab File: BE095129.D
Acq: 26 Jan 2018 15:59

Instrument :
BNA_E
ClientSampleId :
SBLK22

Tot Ion:202 Resp: 2427
Ion Ratio Lower Upper
202 100
101 165.9 18.2 27.4#
100 1174.3 15.6 23.4#

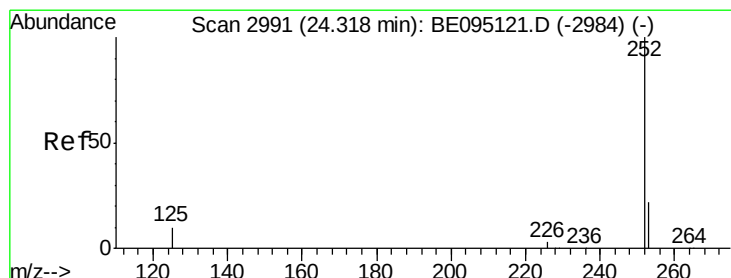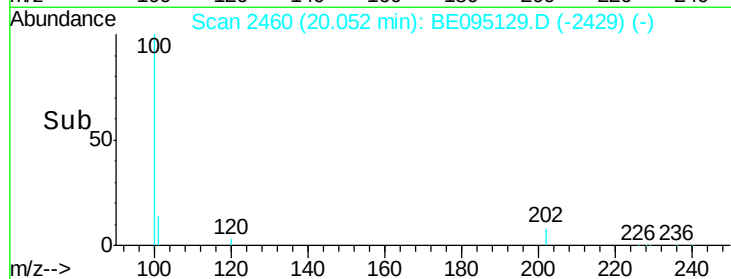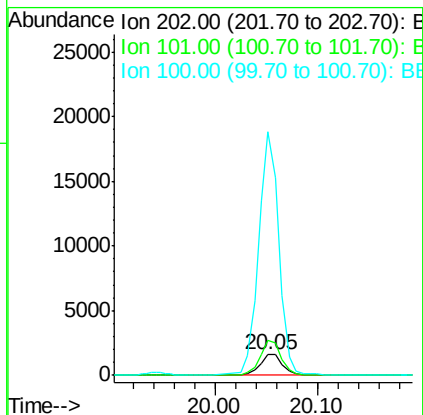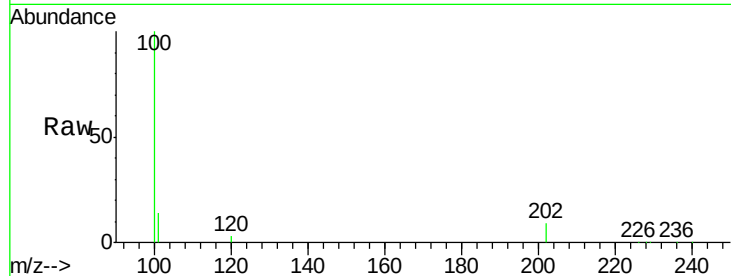

#23
Benzo(a)pyrene
Concen: 0.091 ng/ul
RT: 24.27 min Scan# 2986
Delta R.T. -0.04 min
Lab File: BE095129.D
Acq: 26 Jan 2018 15:59

Tgt Ion:252 Resp: 5436
Ion Ratio Lower Upper
252 100
253 39.5 28.5 42.7
125 48.4 18.1 27.1#

