

Data Path : Z:\HPCHEM1\BNA E\DATA\BE012618\
 Data File : BE095130.D
 Acq On : 26 Jan 2018 16:35
 Operator : SJ/JU
 Sample : PB105816BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK16

Quant Time: Jan 26 17:41:28 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 26 13:41:10 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	3109	0.40	ng/ul	0.00
2) Naphthalene-d8	11.27	136	9542	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	5901	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.71
16) Chrysene-d12	21.81	240	14965	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	20087	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.82	152	5662	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	17340	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	20.06	202	2586	0.051	ng/ul#	1
23) Benzo(a)pyrene	24.27	252	5368	0.085	ng/ul#	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE012618\
Data File : BE095130.D
Acq On : 26 Jan 2018 16:35
Operator : SJ/JU
Sample : PB105816BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK16

Quant Time: Jan 26 17:41:28 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 26 13:41:10 2018
Response via : Initial Calibration




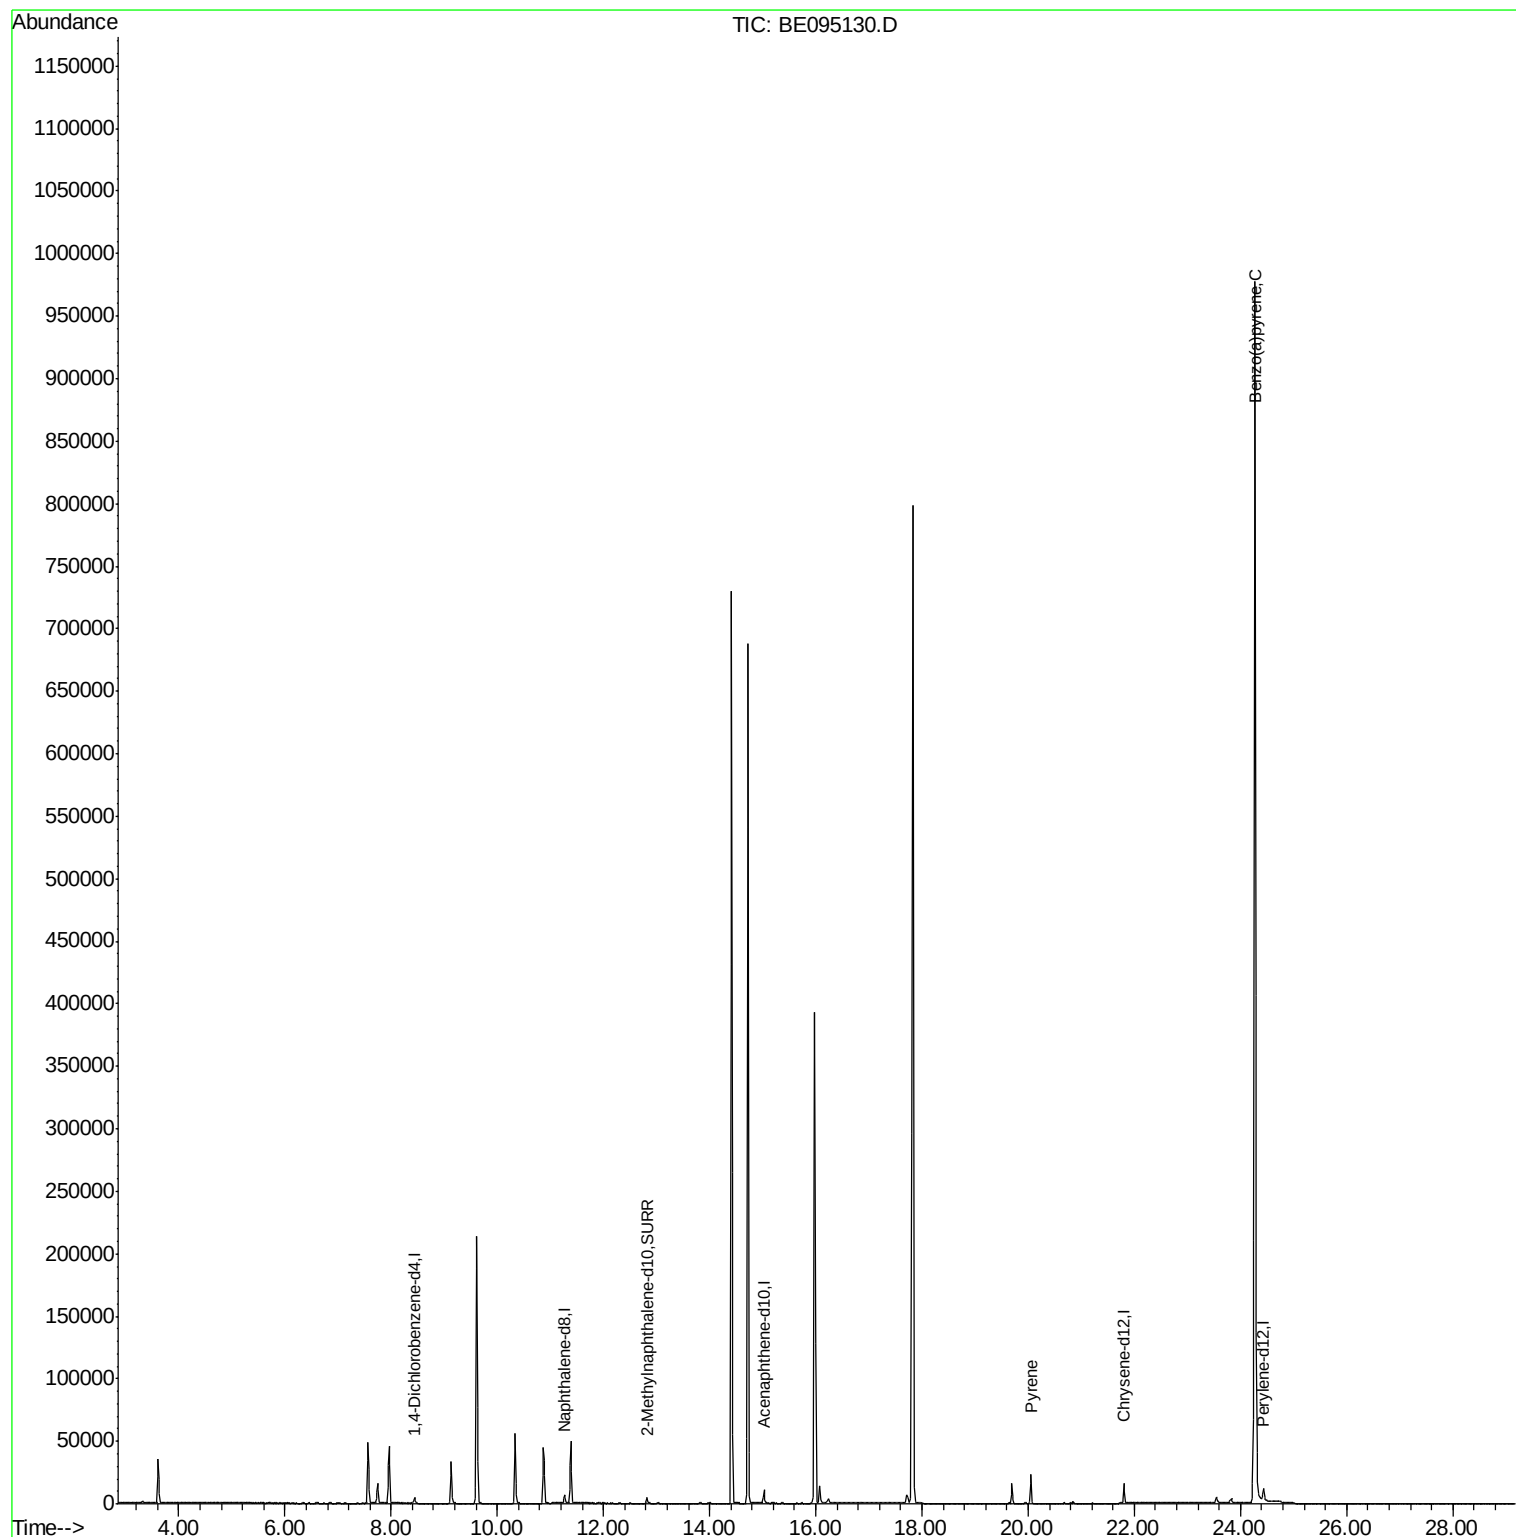


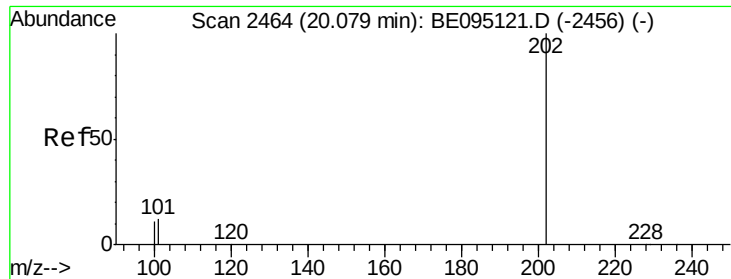

#17
Pvrene
Concen: 0.051 ng/ul
RT: 20.06 min Scan# 2461
Delta R.T. -0.02 min
Lab File: BE095130.D
Acq: 26 Jan 2018 16:35

Instrument :
BNA_E
ClientSampleId :
SBLK16

Tot Ion:202 Resp: 2586
Ion Ratio Lower Upper
202 100
101 151.3 18.2 27.4#
100 931.8 15.6 23.4#

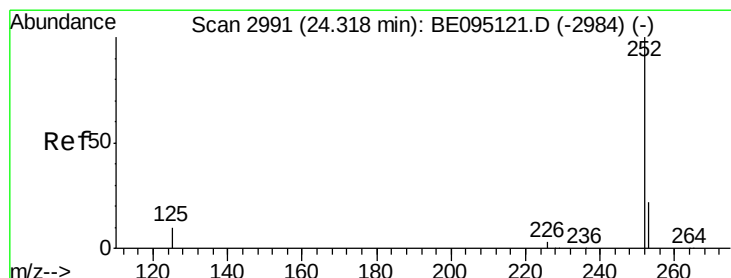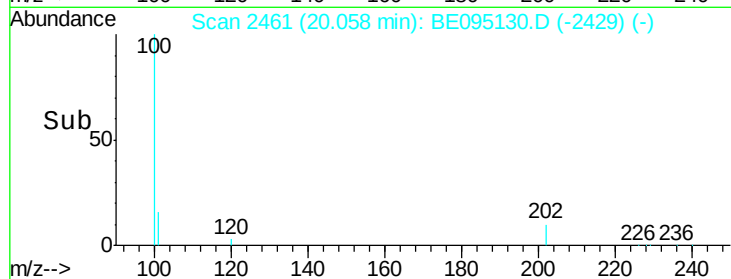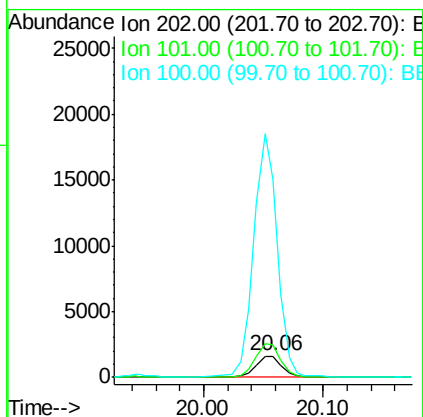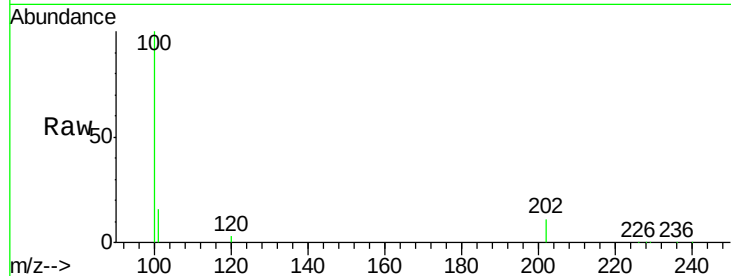

#23
Benzo(a)pyrene
Concen: 0.085 ng/ul
RT: 24.27 min Scan# 2986
Delta R.T. -0.04 min
Lab File: BE095130.D
Acq: 26 Jan 2018 16:35

Tgt Ion:252 Resp: 5368
Ion Ratio Lower Upper
252 100
253 42.0 28.5 42.7
125 37.4 18.1 27.1#

