

Data Path : Z:\HPCHEM1\BNA E\DATA\BE012618\
 Data File : BE095137.D
 Acq On : 26 Jan 2018 20:46
 Operator : SJ/JU
 Sample : J1174-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Jan 27 00:37:33 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 27 00:35:54 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	3300	0.40	ng/ul	0.00
2) Naphthalene-d8	11.27	136	10207	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	6335	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.73
16) Chrysene-d12	21.80	240	15849	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	803873	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.82	152	4642	0.28	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	14191	0.00	ng/ul	0.00
Target Compounds						
8) Acenaphthene	15.08	153	675	0.029	ng/ul	94
17) Pyrene	20.05	202	2362	0.044	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE012618\
Data File : BE095137.D
Acq On : 26 Jan 2018 20:46
Operator : SJ/JU
Sample : J1174-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Jan 27 00:37:33 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 00:35:54 2018
Response via : Initial Calibration

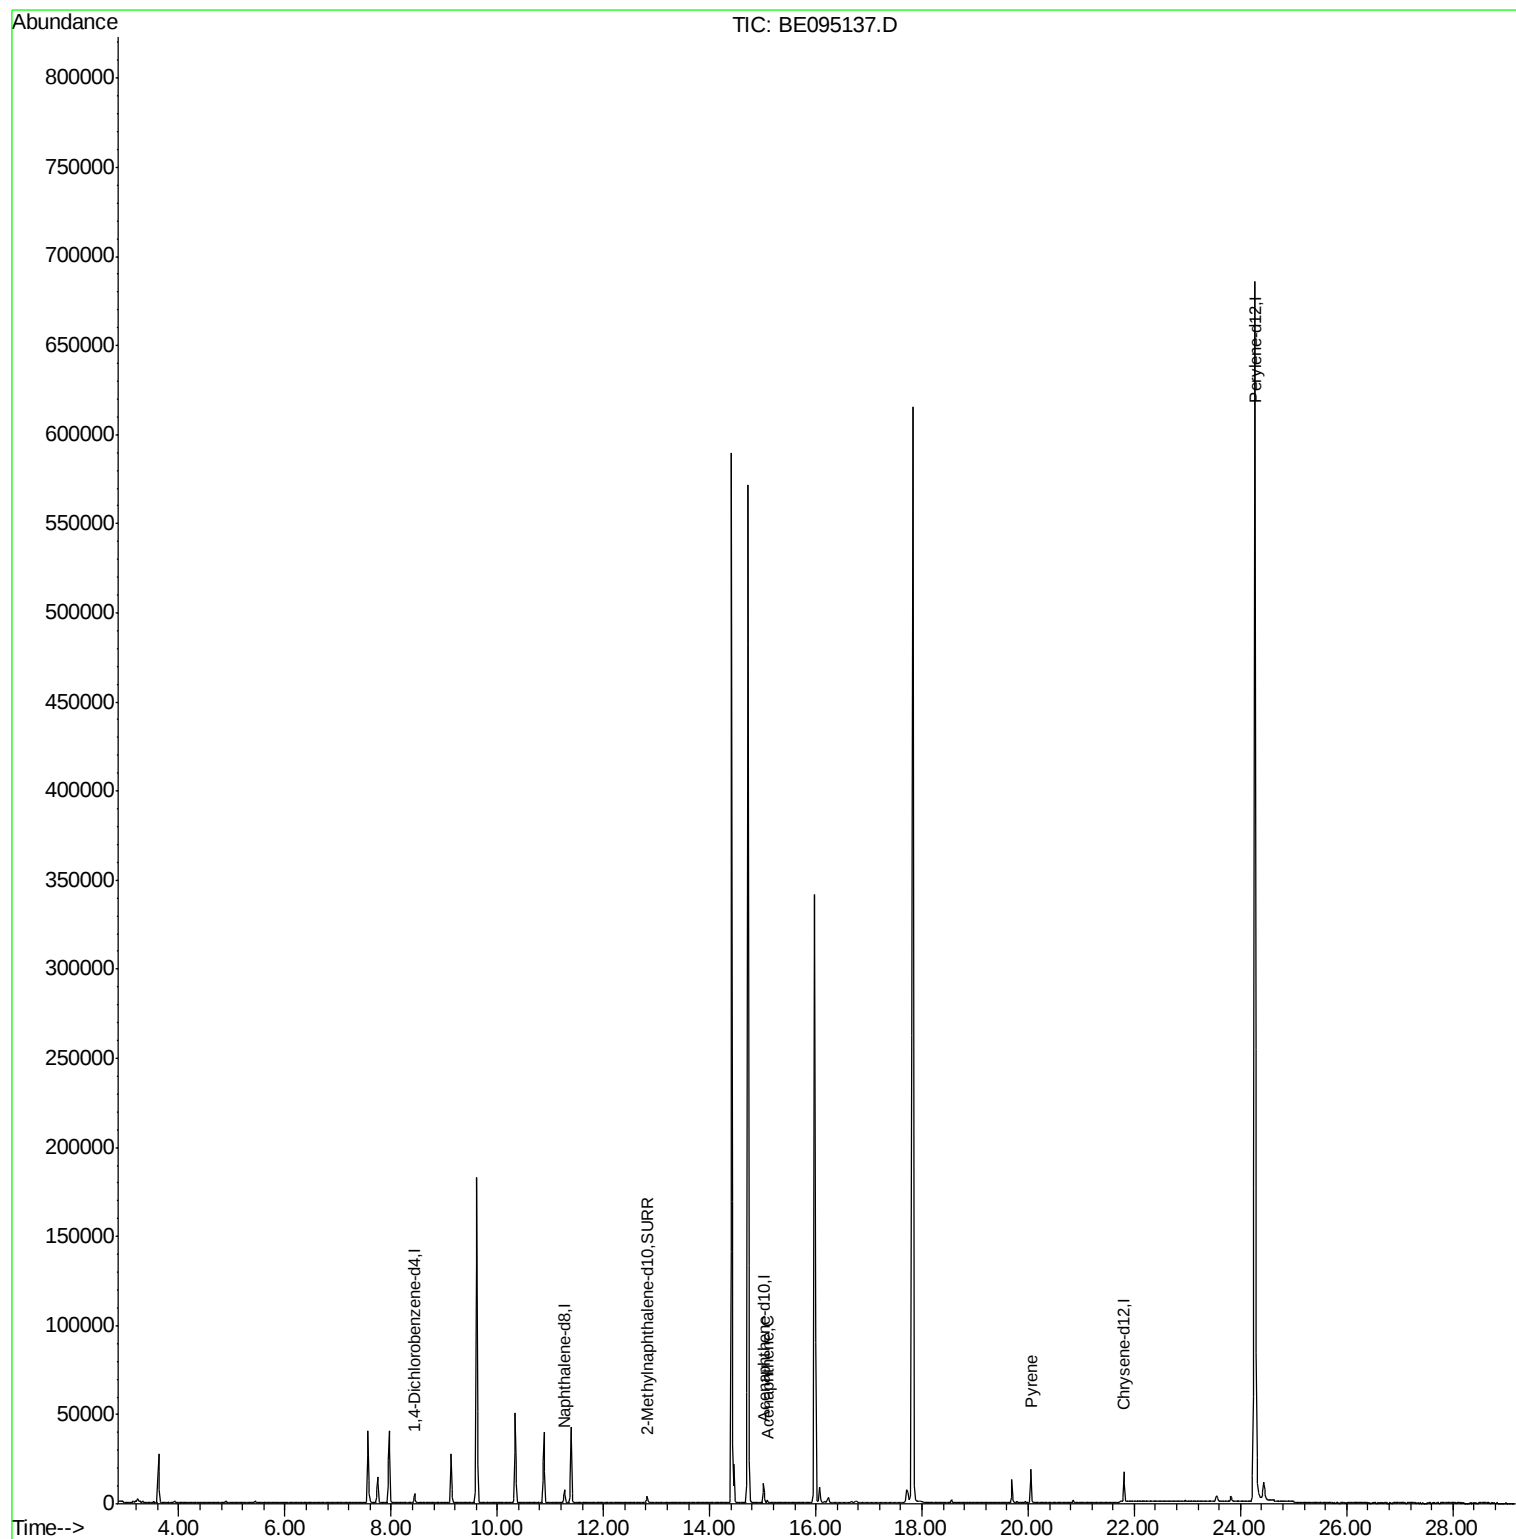

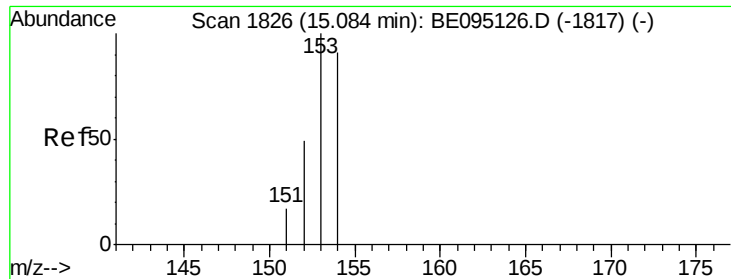

#8

Acenaphthene

Concen: 0.029 ng/ul

RT: 15.08 min Scan# 1826

Delta R.T. 0.00 min

Lab File: BE095137.D

Acq: 26 Jan 2018 20:46

Instrument :

BNA_E

ClientSampleId :


Tot Ion:153 Resp: 675

Ion Ratio Lower Upper

153 100

152 53.8 36.0 54.0

154 88.2 72.0 108.0

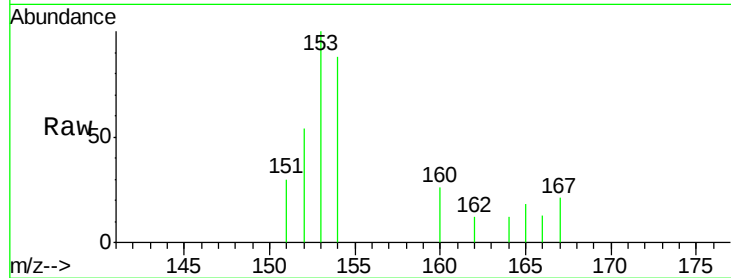

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

15.08



400

200

0

15.05 15.10

Time-->

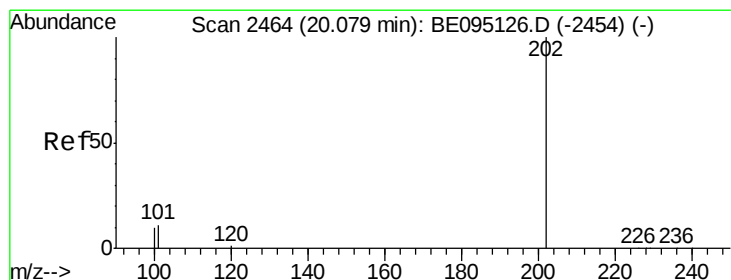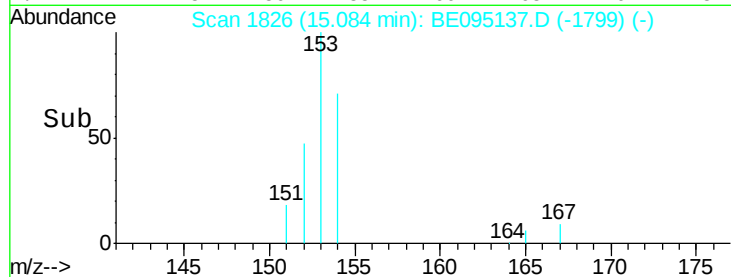

#17

Pyrene

Concen: 0.044 ng/ul

RT: 20.05 min Scan# 2460

Delta R.T. -0.03 min

Lab File: BE095137.D

Acq: 26 Jan 2018 20:46


Tgt Ion:202 Resp: 2362

Ion Ratio Lower Upper

202 100

101 159.2 18.2 27.4#

100 1092.1 15.6 23.4#

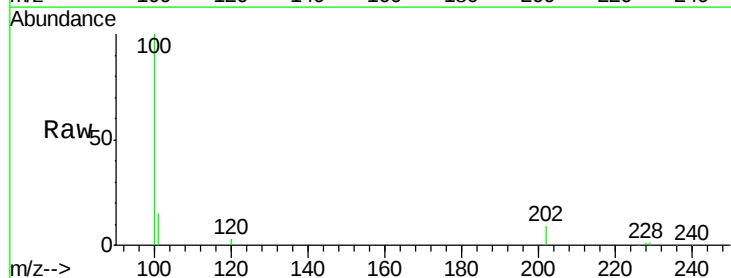

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

20.05

15000

10000

5000

0

20.00 20.10

Time-->

