

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
 Data File : BE095156.D
 Acq On : 27 Jan 2018 8:03
 Operator : SJ/JU
 Sample : J1174-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6A58

Quant Time: Jan 27 22:36:28 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 27 03:18:43 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.45	152	3579	0.40	ng/ul	0.00
2) Naphthalene-d8	11.27	136	11592	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	7502	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.71
16) Chrysene-d12	21.81	240	17991	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	997252	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.82	152	6013	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	17940	0.00	ng/ul	0.00
Target Compounds						
8) Acenaphthene	15.08	153	1293	0.046	ng/ul	92
17) Pyrene	20.06	202	2705	0.045	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
Data File : BE095156.D
Acq On : 27 Jan 2018 8:03
Operator : SJ/JU
Sample : J1174-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6A58

Quant Time: Jan 27 22:36:28 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

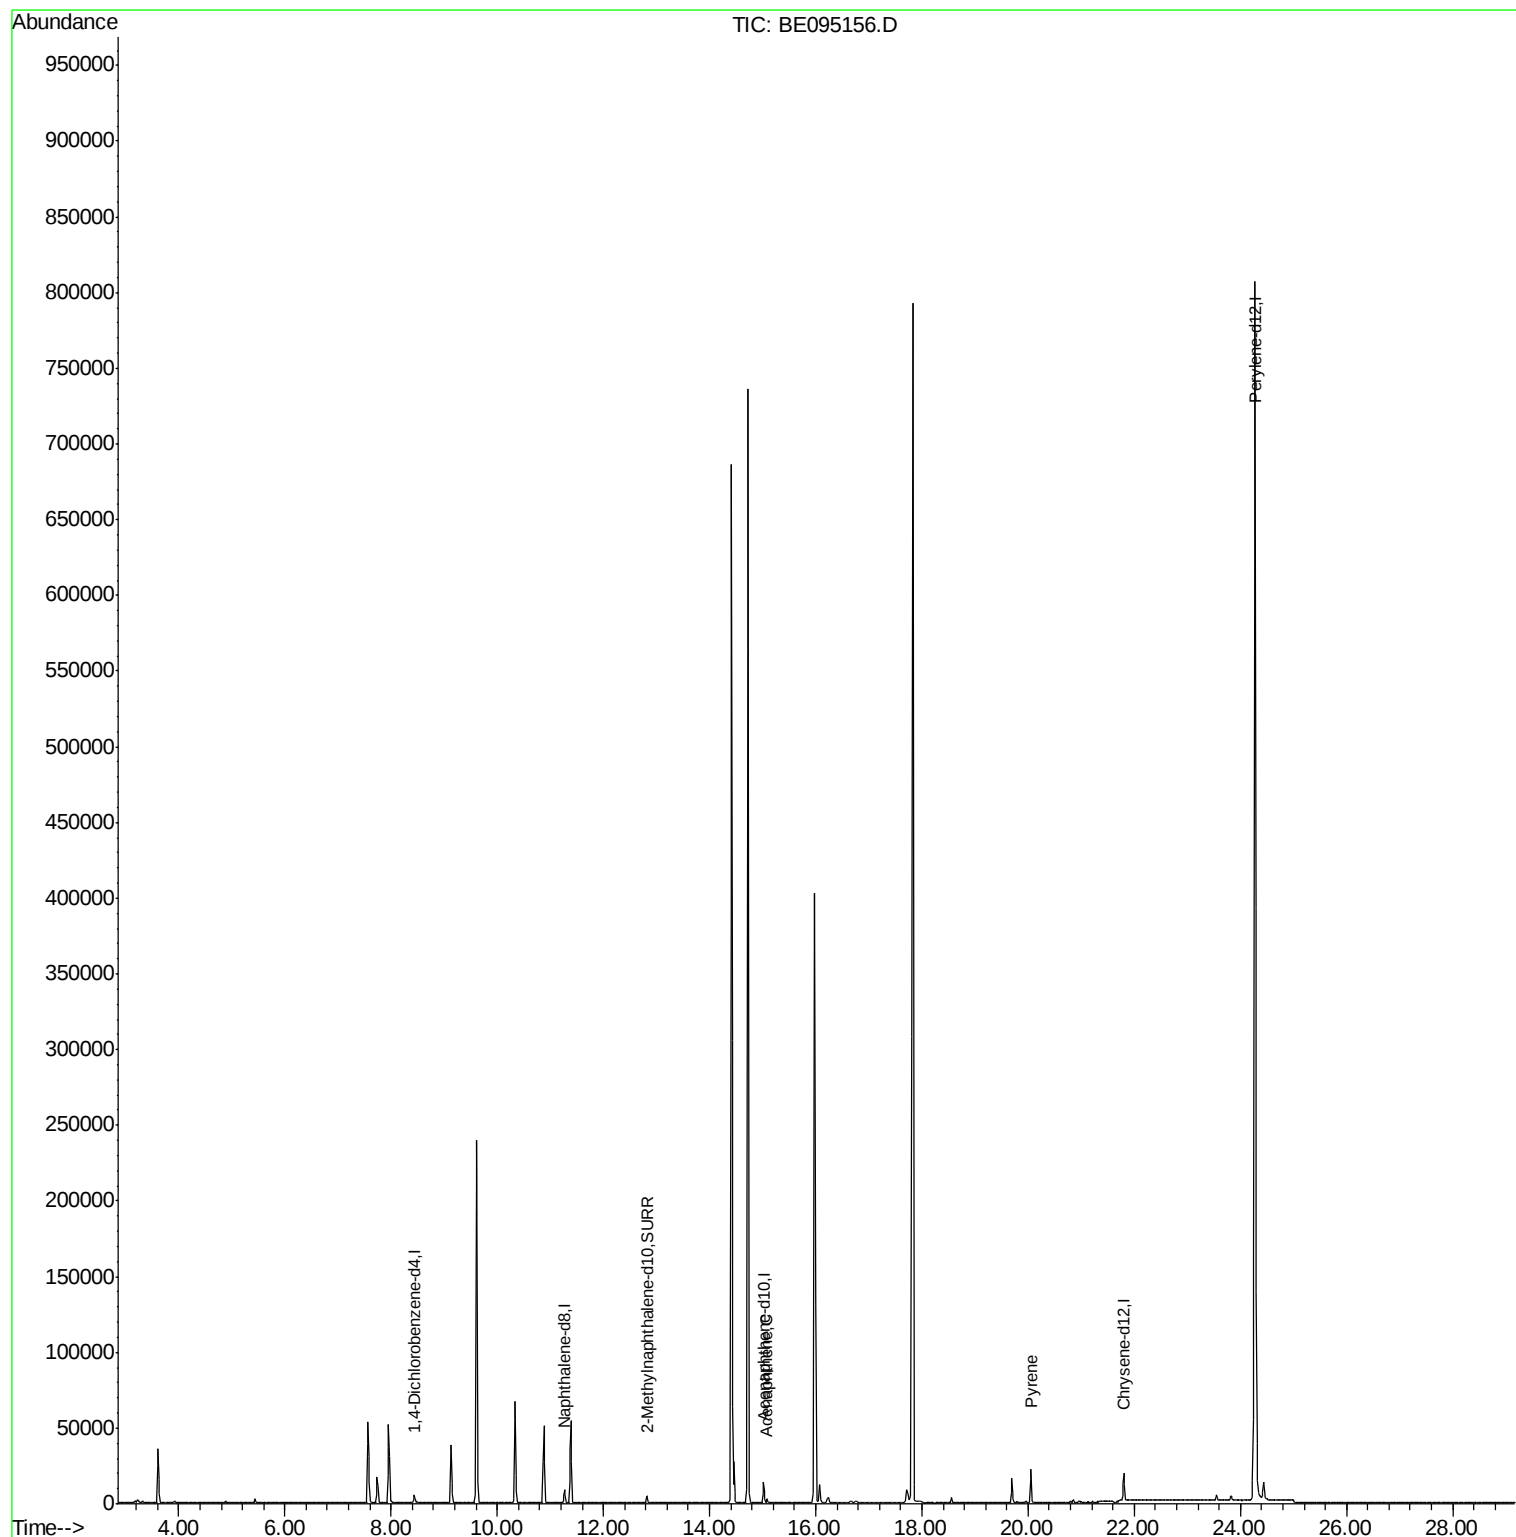

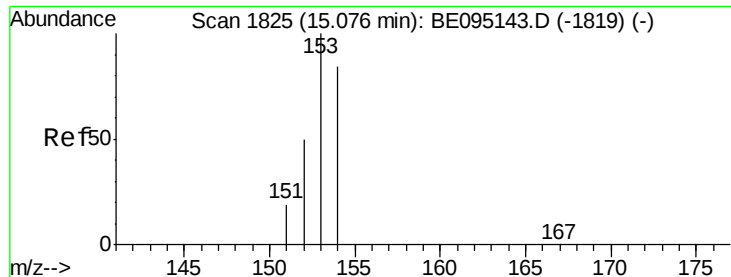

#8

Acenaphthene

Concen: 0.046 ng/ul

RT: 15.08 min Scan# 1826

Delta R.T. 0.01 min

Lab File: BE095156.D

Acq: 27 Jan 2018 8:03

Instrument :

BNA_E

ClientSampleId :

F6A58


Tgt Ion:153 Resp: 1293

Ion Ratio Lower Upper




153 100

152 53.0 36.0 54.0

154 94.9 72.0 108.0

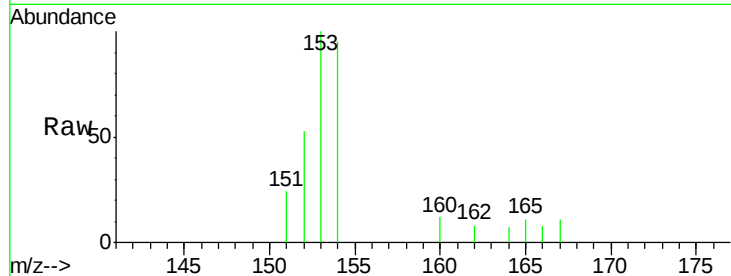

Abundance Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E
Ion 154.00 (153.70 to 154.70): E

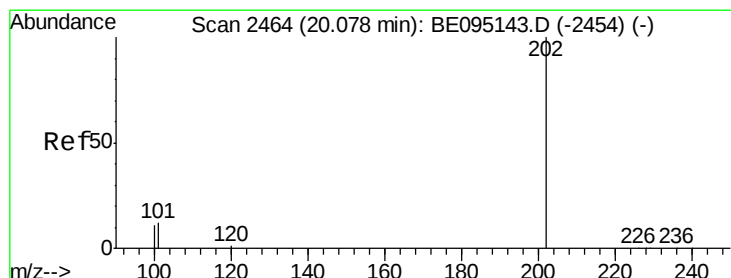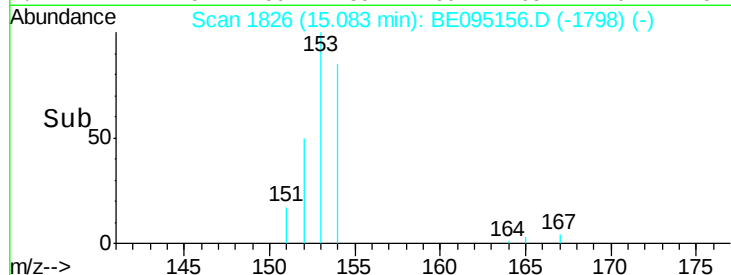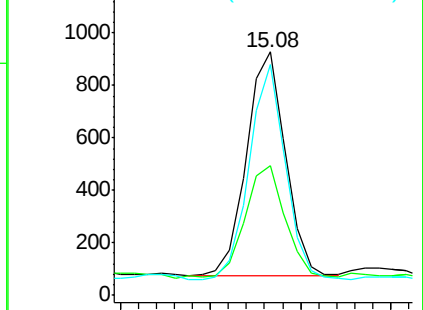

#17

Pyrene

Concen: 0.045 ng/ul

RT: 20.06 min Scan# 2461

Delta R.T. -0.02 min

Lab File: BE095156.D

Acq: 27 Jan 2018 8:03


Tgt Ion:202 Resp: 2705

Ion Ratio Lower Upper

202 100

101 153.8 18.2 27.4#

100 927.1 15.6 23.4#

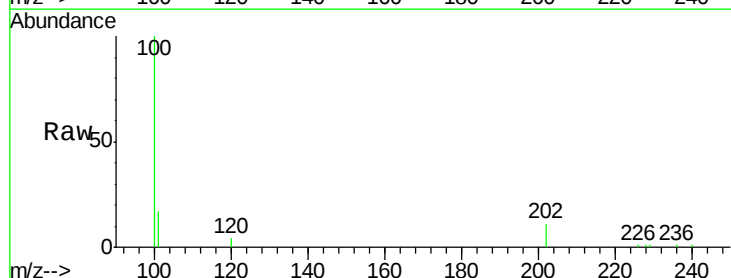

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): E

