

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA E\Data\BE012618\
Data File : BE095129.D
Acq On : 26 Jan 2018 15:59
Operator : SJ/JU
Sample : PB105822BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
SBLK22

Manual Integrations
APPROVED

Sohil
1/29/2018 6:29:52 PM

Quant Time: Jan 29 10:25:24 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 26 13:41:10 2018
Response via : Initial Calibration

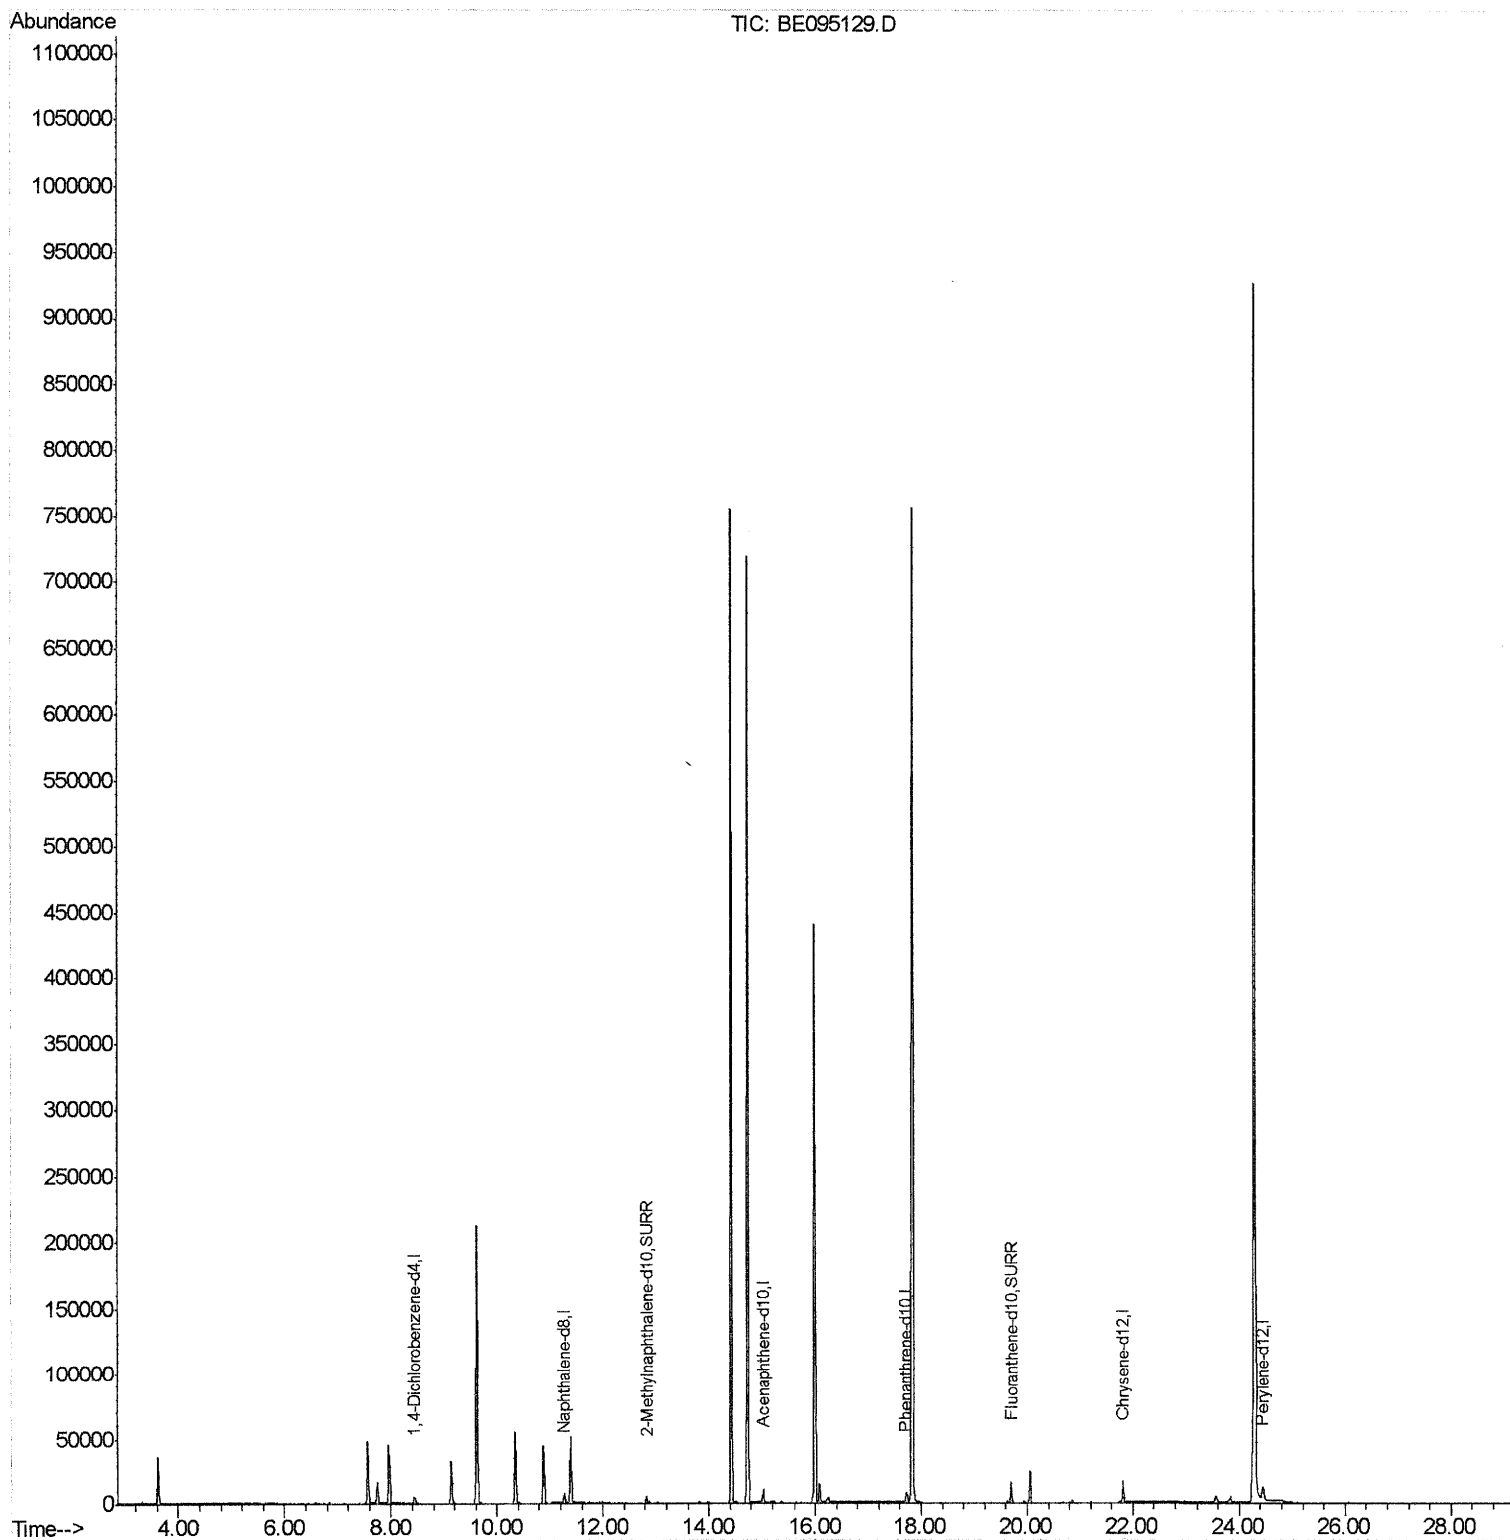

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE012618\
 Data File : BE095129.D
 Acq On : 26 Jan 2018 15:59
 Operator : SJ/JU
 Sample : PB105822BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 SBLK22

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:29:52 PM

Quant Time: Jan 26 18:02:49 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 26 13:41:10 2018
 Response via : Initial Calibration

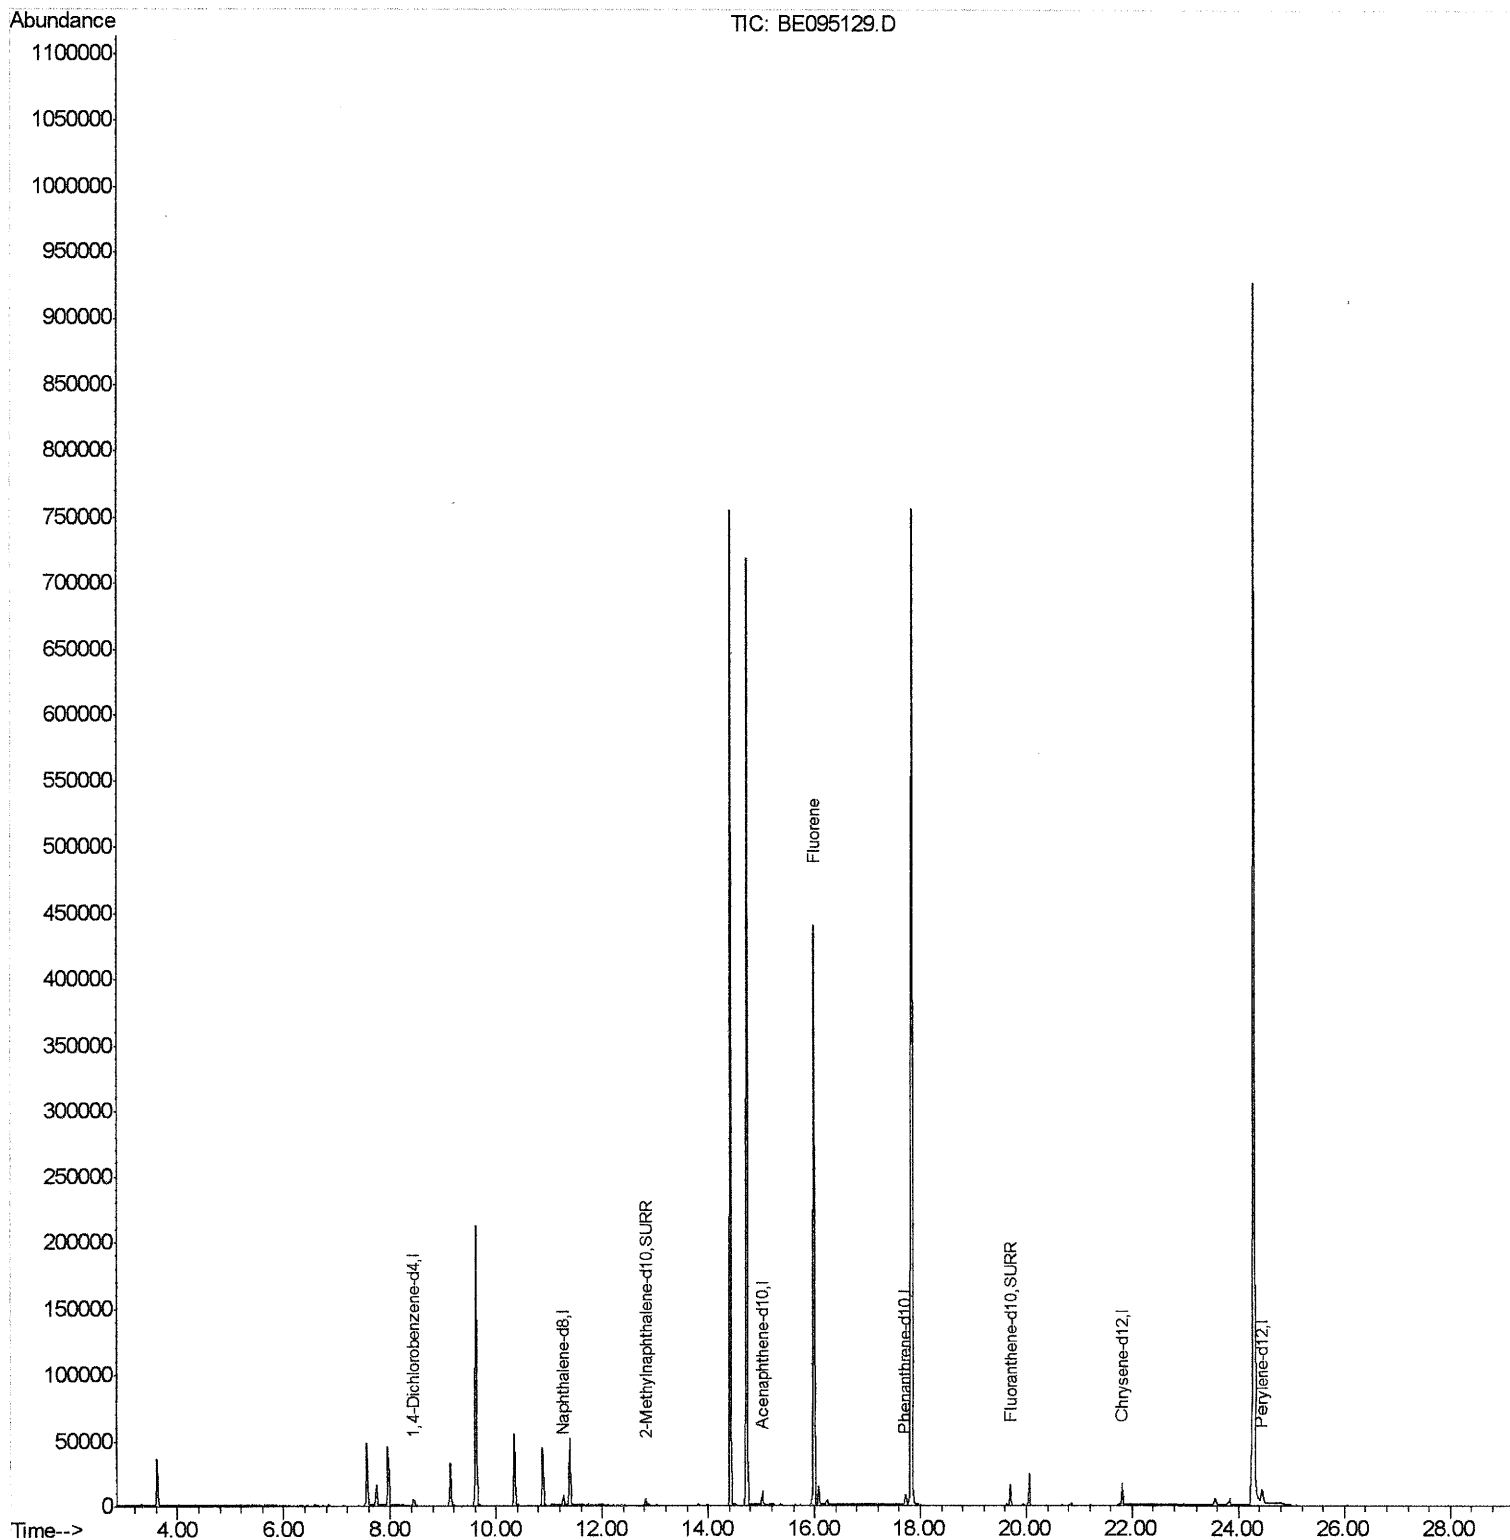

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE012618\
 Data File : BE095129.D
 Acq On : 26 Jan 2018 15:59
 Operator : SJ/JU
 Sample : PB105822BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 SBLK22

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:29:52 PM

Quant Time: Jan 26 17:41:21 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 26 13:41:10 2018
 Response via : Initial Calibration

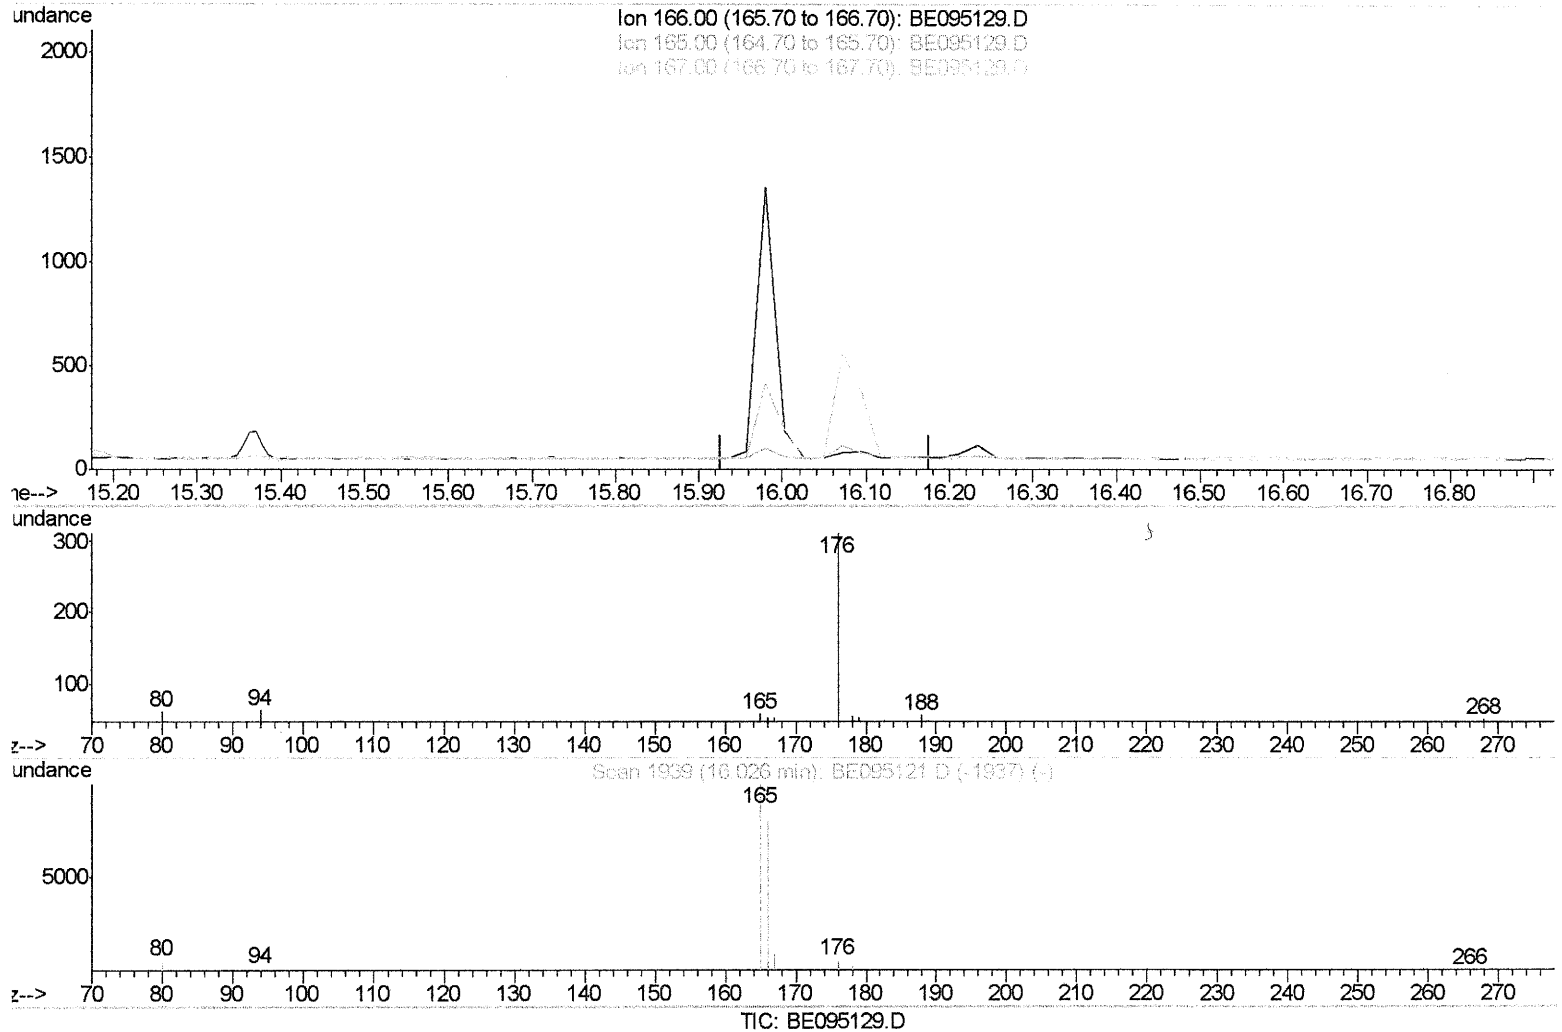

(9) Fluorene

16.026min (-16.026) 0.00ng/ul

response 0

Ion	Exp%	Act%
166.00	100	0.00
165.00	91.80	0.00#
167.00	18.30	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE012618\
 Data File : BE095129.D
 Acq On : 26 Jan 2018 15:59
 Operator : SJ/JU
 Sample : PB105822BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 SBLK22

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:29:52 PM

Quant Time: Jan 26 17:41:21 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 26 13:41:10 2018
 Response via : Initial Calibration

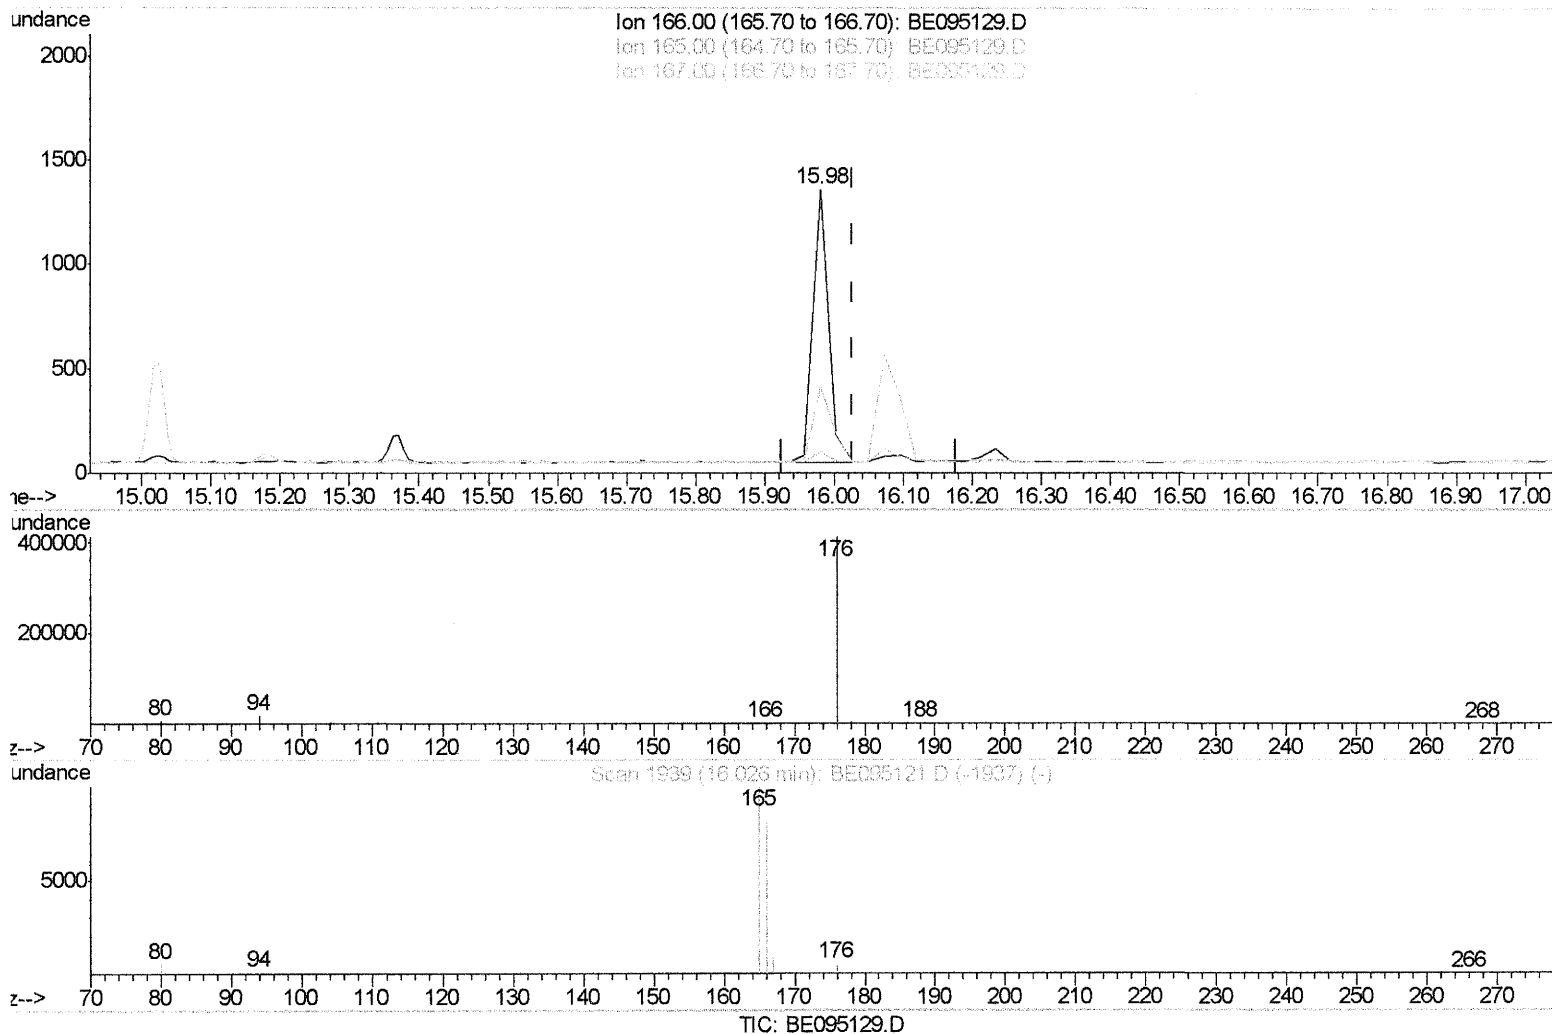

(9) Fluorene

15.980min (-0.047) 0.09ng/ul m

response 2062

Ion	Exp%	Act%
166.00	100	100
165.00	91.80	7.58#
167.00	18.30	31.13#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE012618\
 Data File : BE095129.D
 Acq On : 26 Jan 2018 15:59
 Operator : SJ/JU
 Sample : PB105822BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleID :
 SBLK22

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:29:52 PM

Quant Time: Jan 26 17:41:21 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 26 13:41:10 2018
 Response via : Initial Calibration

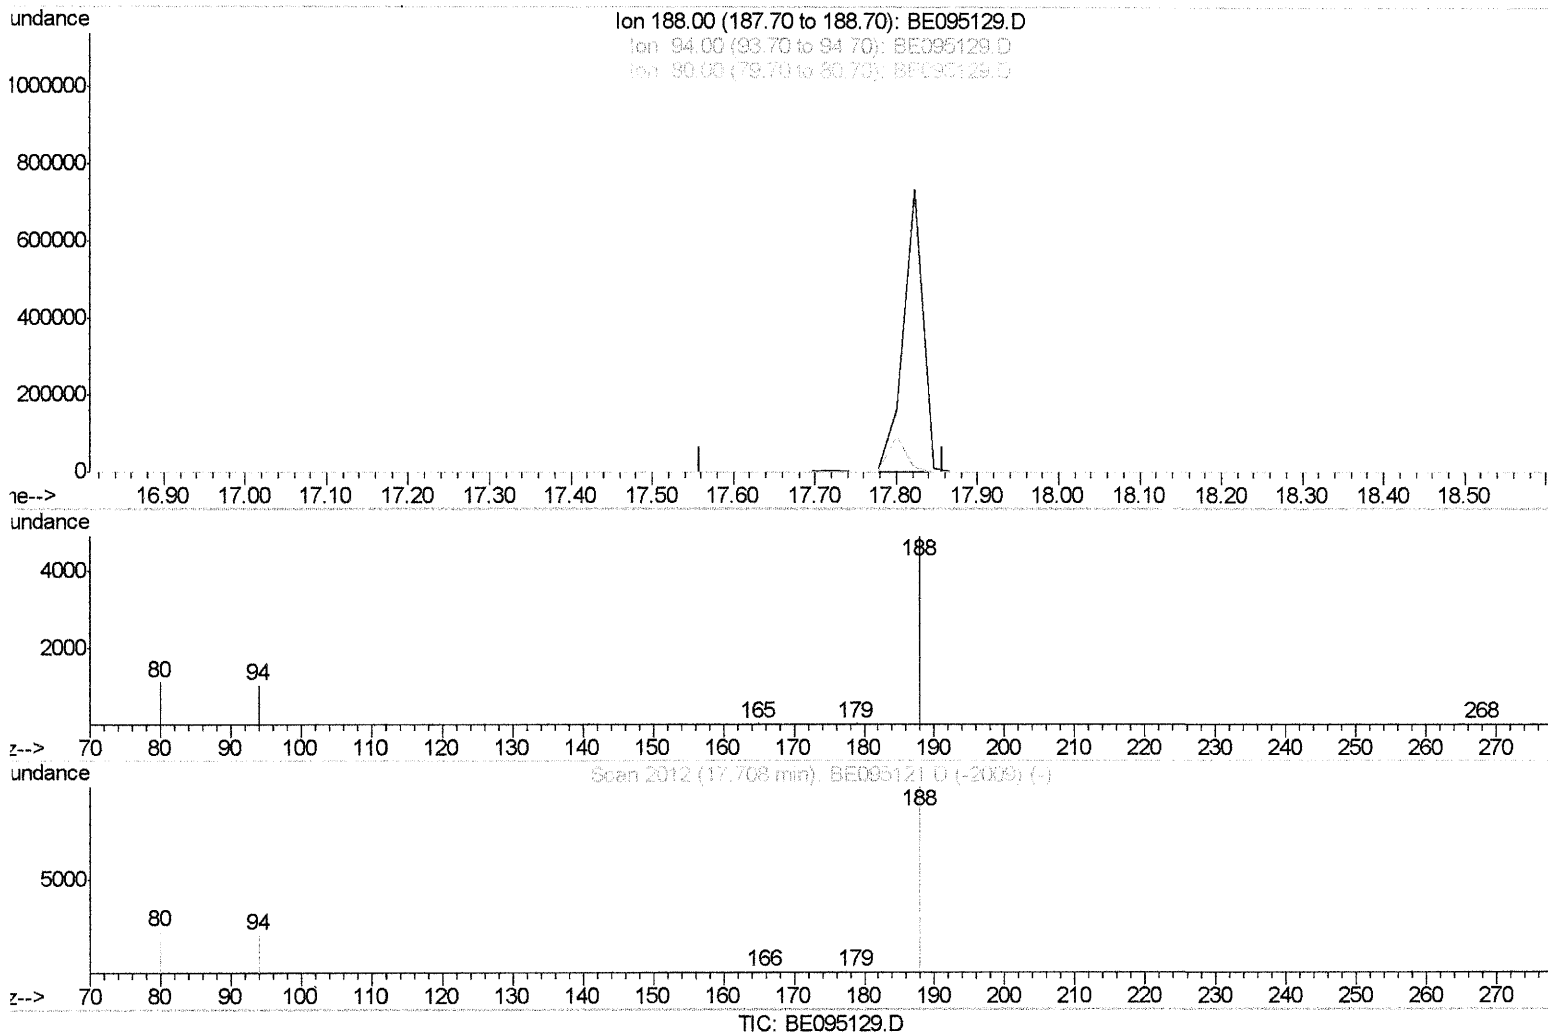

(10) Phenanthrene-d10 (I)

17.708min (-17.708) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE012618\
 Data File : BE095129.D
 Acq On : 26 Jan 2018 15:59
 Operator : SJ/JU
 Sample : PB105822BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 Client Sampled :
 SBLK22

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:29:52 PM

Quant Time: Jan 26 17:41:21 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 26 13:41:10 2018
 Response via : Initial Calibration

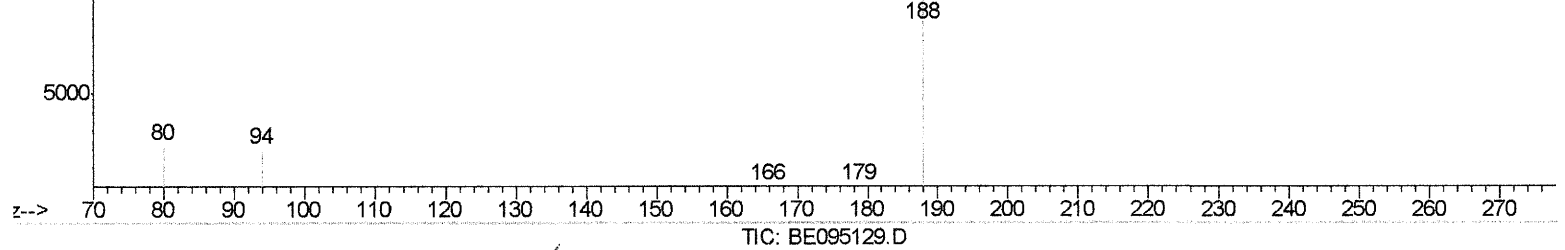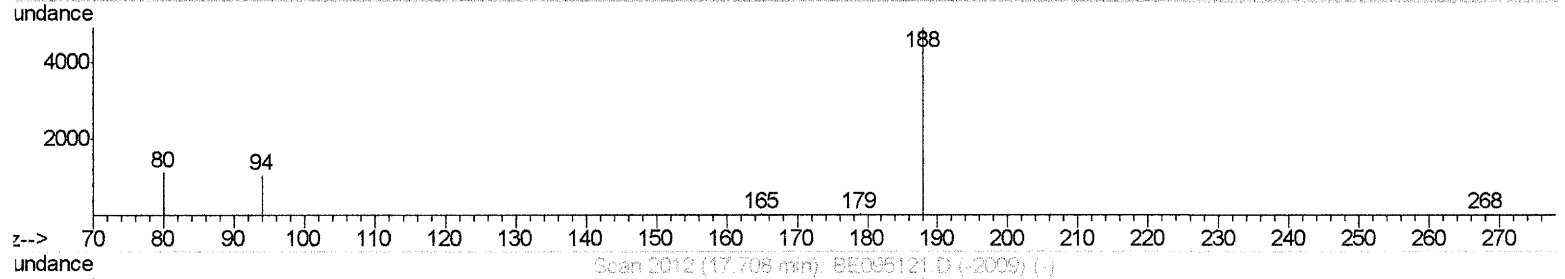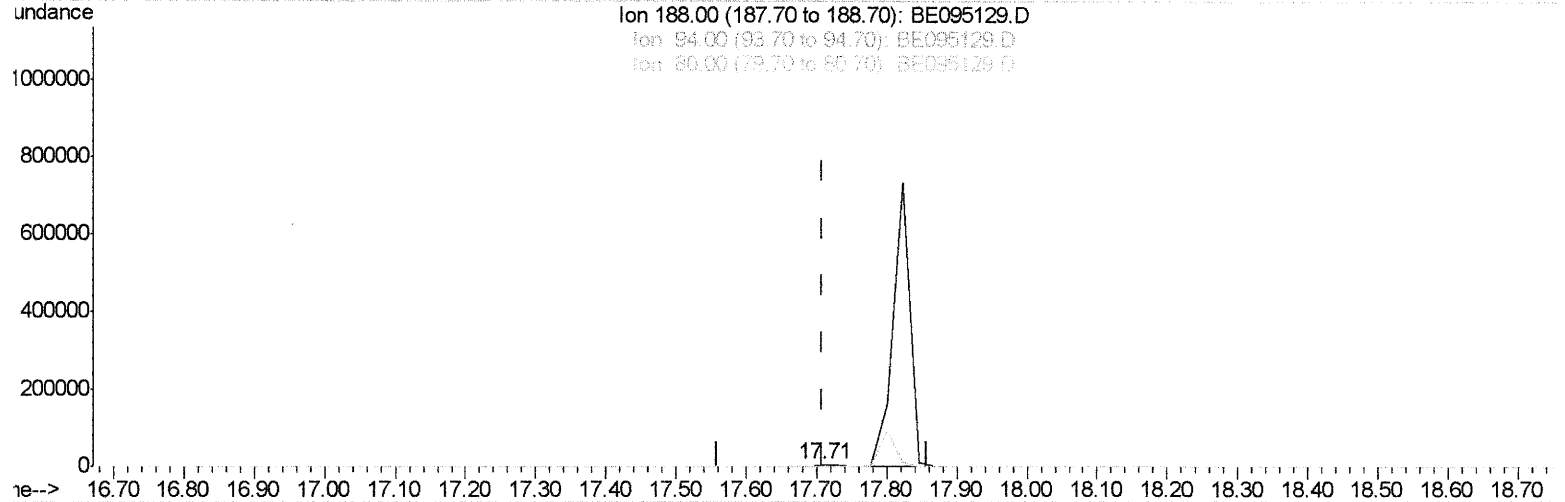

(10) Phenanthrene-d10 (I)

17.708min (-0.001) 0.40ng/ul

response 12975

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	21.33#
80.00	11.80	23.11#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE012618\
Data File : BE095129.D
Acq On : 26 Jan 2018 15:59
Operator : SJ/JU
Sample : PB105822BL
Disc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
Client Sampled :
SBLK22

Manual Integrations
APPROVED

Sohil
1/29/2018 6:29:52 PM

Quant Time: Jan 26 18:02:49 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 26 13:41:10 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	3103	0.40	ng/ul	0.00
2) Naphthalene-d8	11.27	136	9694	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	6106	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	12975m	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	14913	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	19031	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.82	152	5713	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	17687	0.36	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
9) Fluorene	15.98	166	2062m	0.088	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA E\Data\BE012618\
 Data File : BE095129.D
 Acq On : 26 Jan 2018 15:59
 Operator : SJ/JU
 Sample : PB105822BL
 Disc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 Client Sample ID :
 SBLK22

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:29:52 PM

Quant Time: Jan 29 10:25:24 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 26 13:41:10 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	3103	0.40	ng/ul	0.00
2) Naphthalene-d8	11.27	136	9694	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	6106	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	12975m	0.40	ng/ul	>0.00
16) Chrysene-d12	21.80	240	14913	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	19031	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.82	152	5713	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	17687	0.36	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed