

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA_E\Data\BE012618\
 Data File : BE095153.D
 Acq On : 27 Jan 2018 6:16
 Operator : SJ/JU
 Sample : J1174-16
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6A51

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:34:13 PM

Quant Time: Jan 29 16:41:00 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 27 03:18:43 2018
 Response via : Initial Calibration

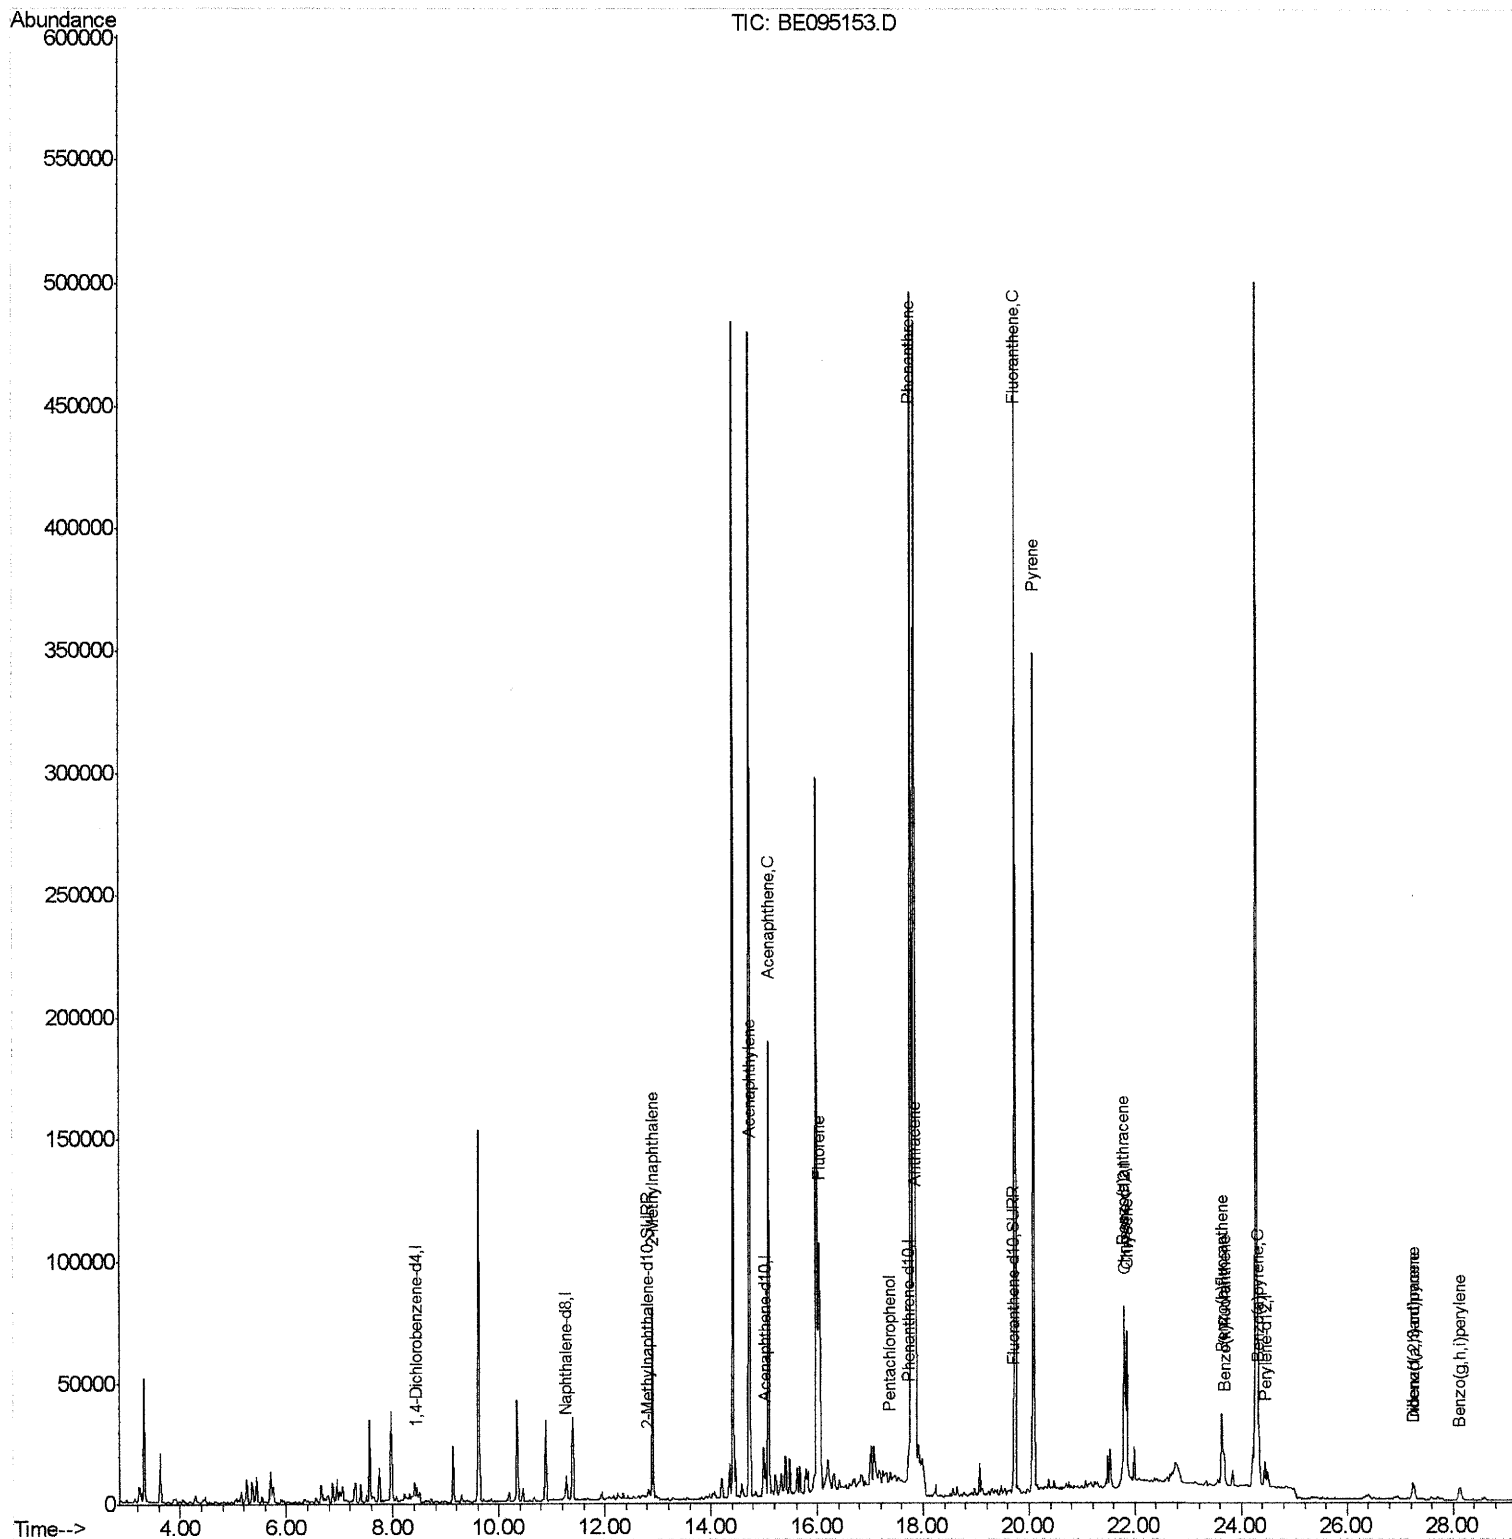

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
 Data File : BE095152.D
 Acq On : 27 Jan 2018 5:40
 Operator : SJ/JU
 Sample : J1174-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6A51

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:34:13 PM

Quant Time: Jan 27 22:45:04 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 27 03:18:43 2018
 Response via : Initial Calibration

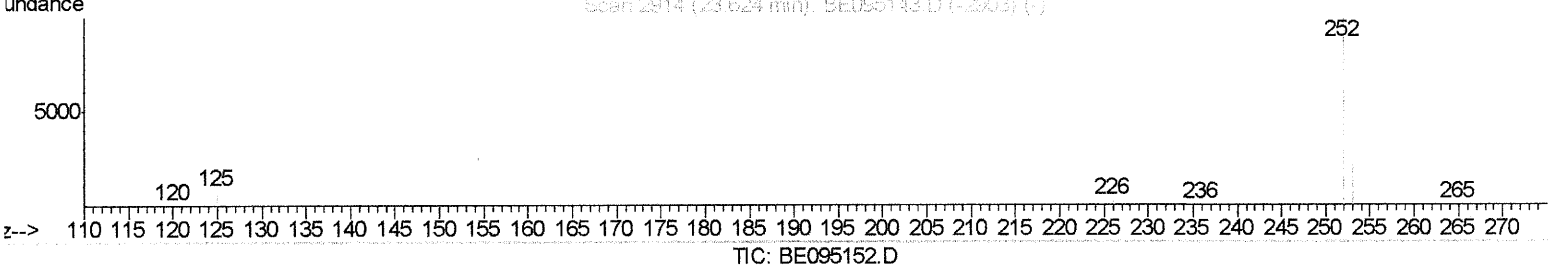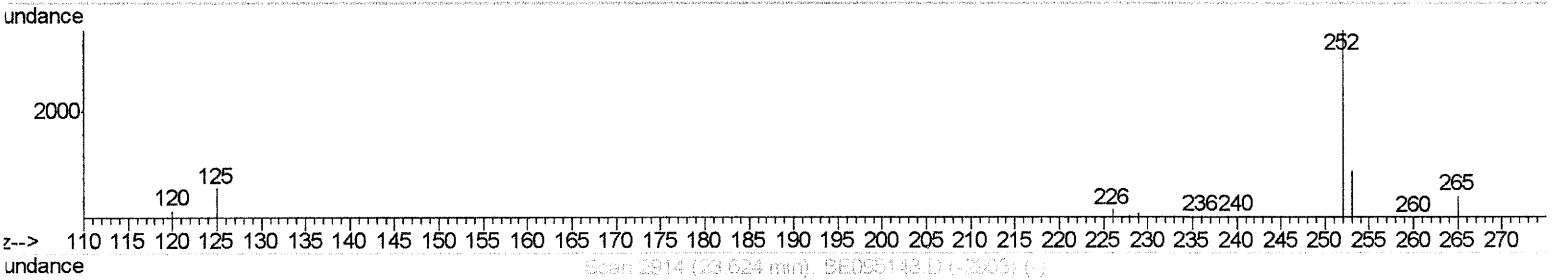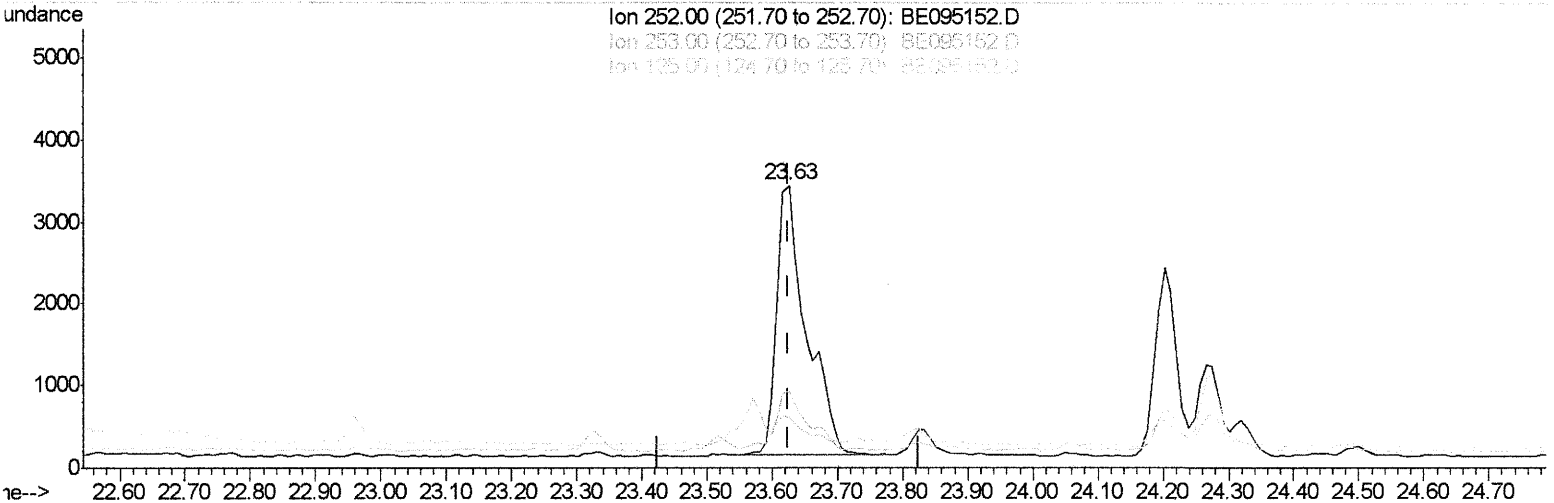

(21) Benzo(b)fluoranthene

23.625min (+0.001) 0.16ng/ul

response 10482

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	26.89
125.00	17.50	17.95
0.00	0.00	0.00

Quantitation Report (Qedit)

Instrument :

BNA_E

Client Sample ID :

F6A51




Manual Integrations
APPROVED

Sohil

1/29/2018 6:34:13 PM

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
Data File : BE095152.D
Acq On : 27 Jan 2018 5:40
Operator : SJ/JU
Sample : J1174-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Jan 27 22:45:04 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

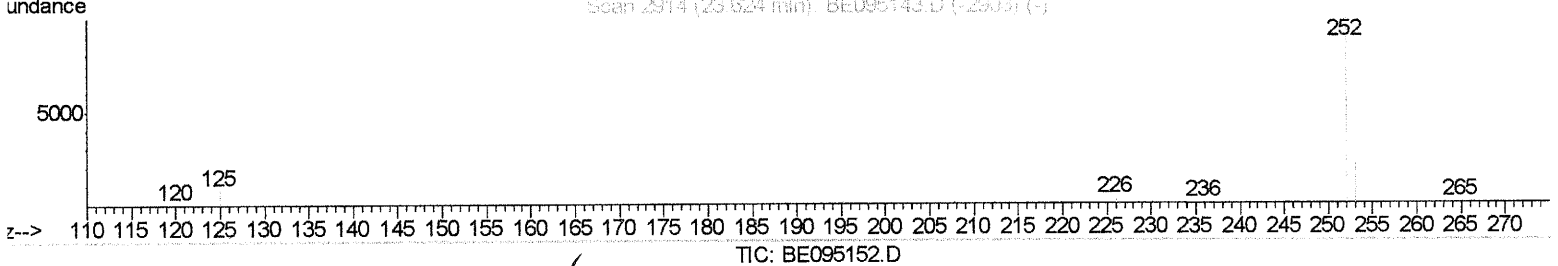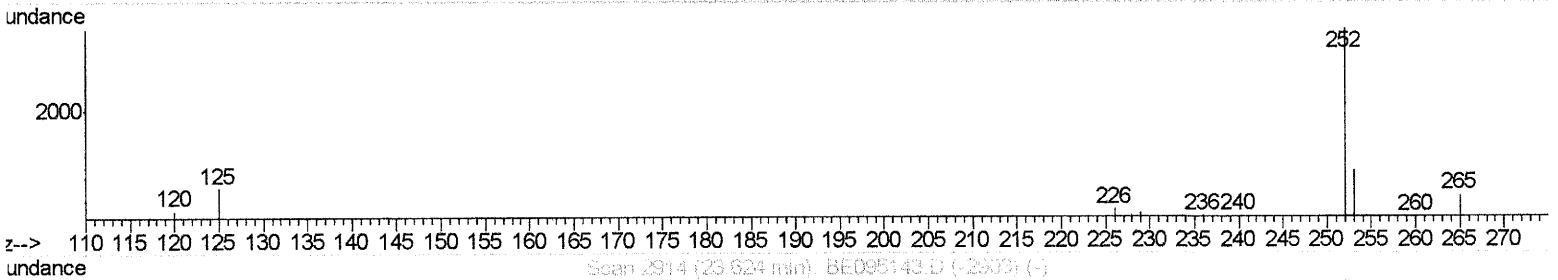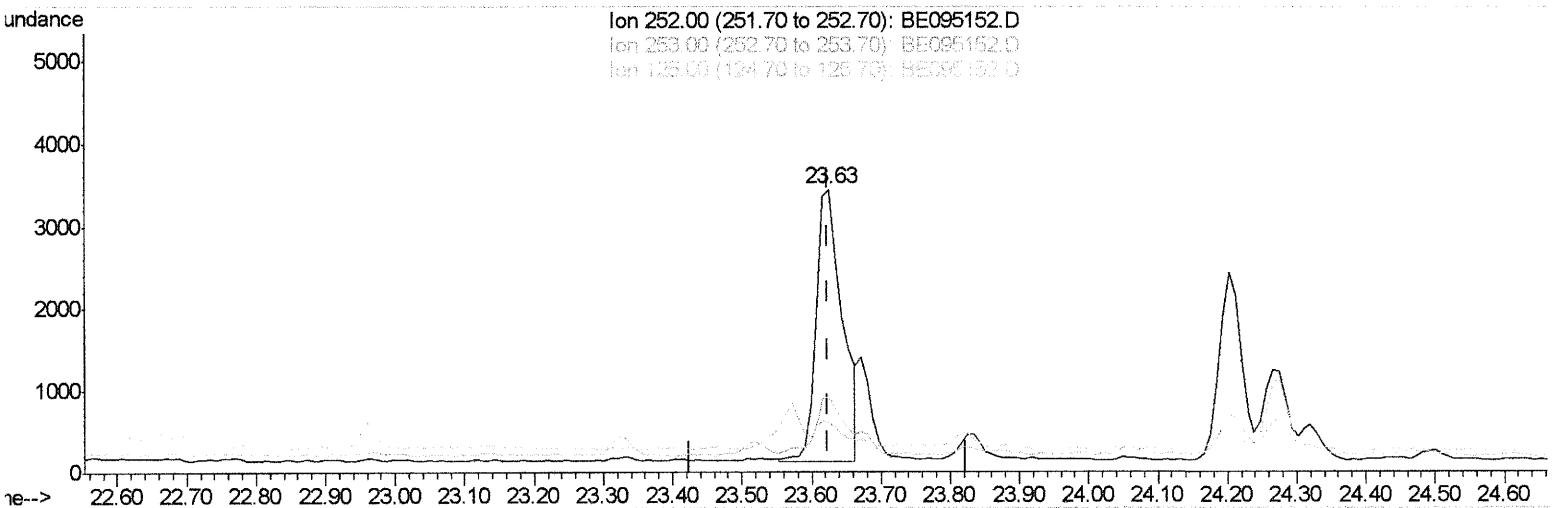

(21) Benzo(b)fluoranthene

23.625min (+0.001) 0.14ng/ul m

response 8866

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	26.89
125.00	17.50	17.95
0.00	0.00	0.00

me 1/27/18

Quantitation Report (Qedit)


Instrument :
BNA_E
ClientSampled :
F6A51

Manual Integrations
APPROVED

Sohil
1/29/2018 6:34:13 PM

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
Data File : BE095152.D
Acq On : 27 Jan 2018 5:40
Operator : SJ/JU
Sample : J1174-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Jan 27 22:45:04 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

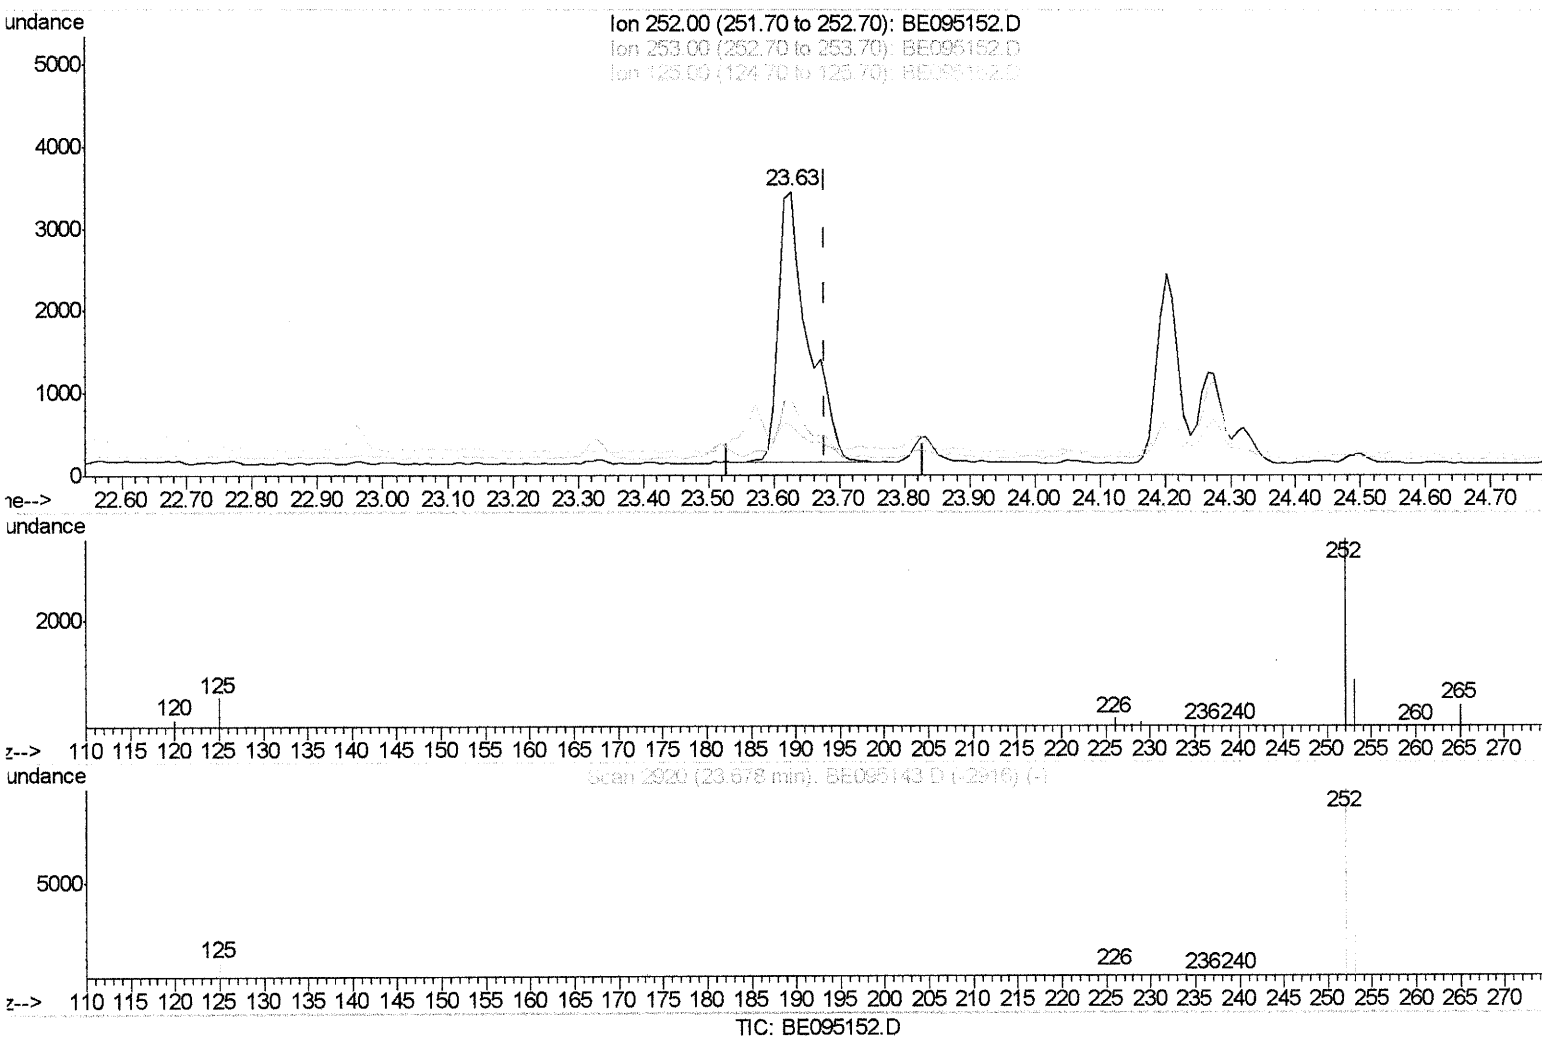

(22) Benzo(k)fluoranthene

23.625min (-0.053) 0.18ng/ui

response 10482

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	26.89
125.00	17.10	17.95
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
Data File : BE095152.D
Acq On : 27 Jan 2018 5:40
Operator : SJ/JU
Sample : J1174-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
F6A51

Manual Integrations
APPROVED

Sohil
1/29/2018 6:34:13 PM

Quant Time: Jan 27 22:45:04 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

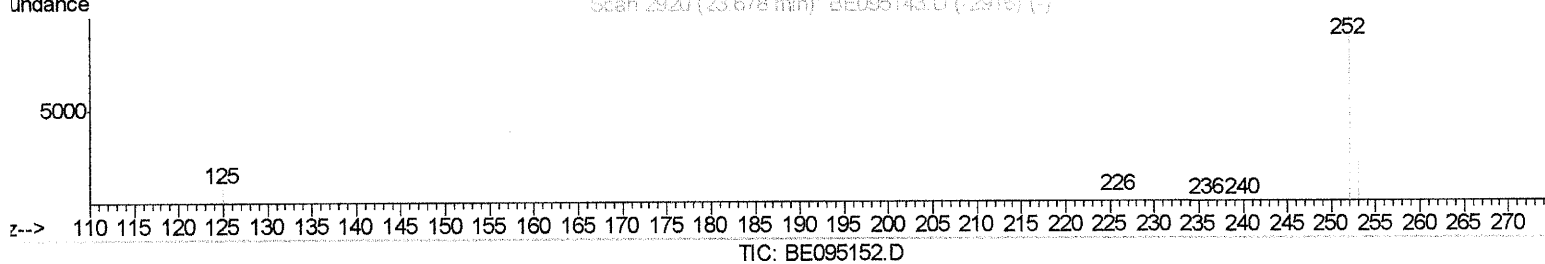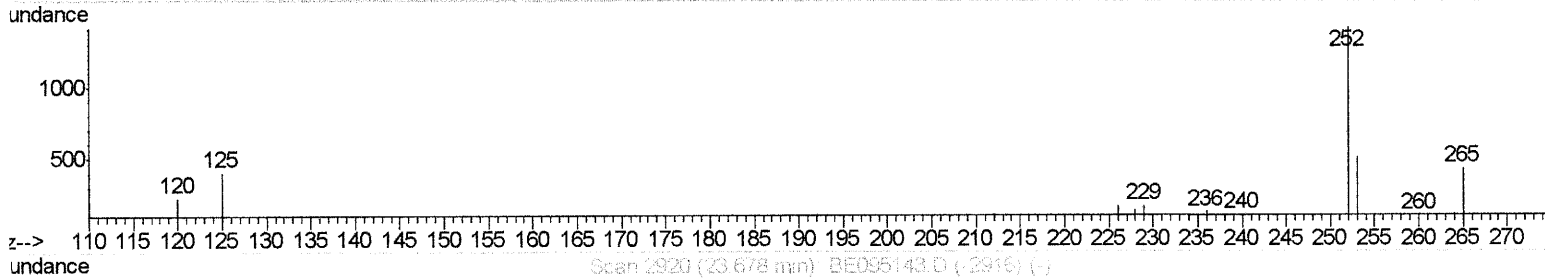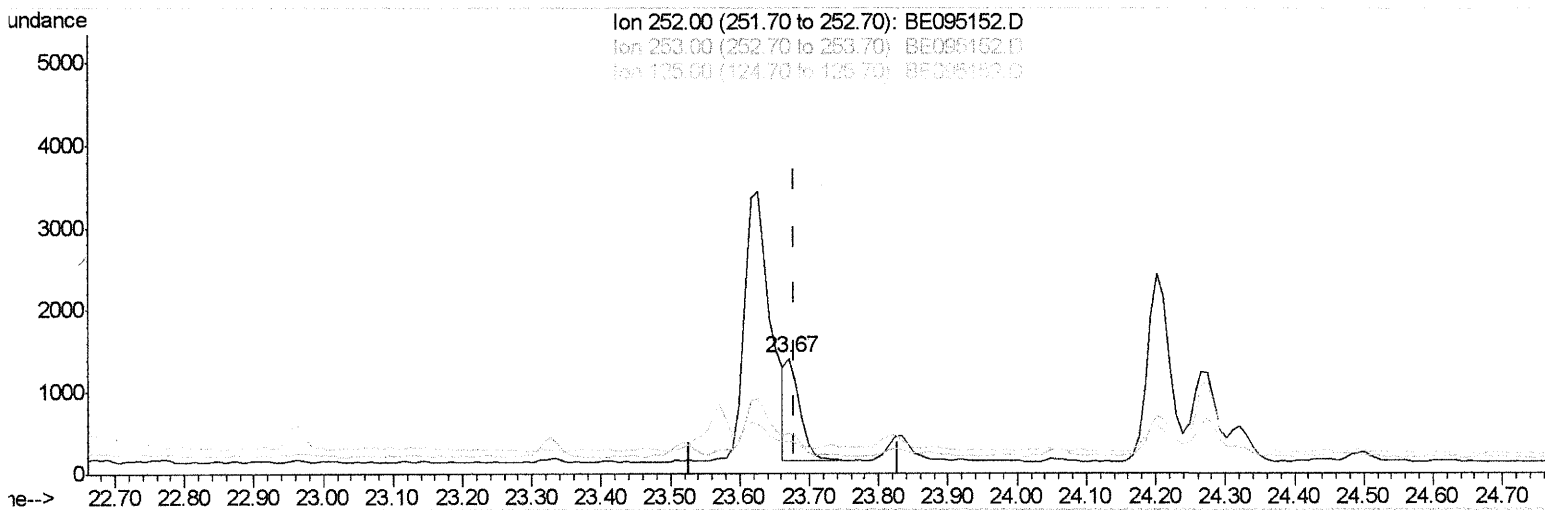

(22) Benzo(k)fluoranthene

23.670min (-0.008) 0.03ng/ul m

response 1726

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	35.88
125.00	17.10	28.73#
0.00	0.00	0.00

Jan 27/18

Quantitation Report (Qedit)




Instrument :
BNA_E
ClientSampleId :
F6A51

Manual Integrations
APPROVED

Sohil
1/29/2018 6:34:13 PM

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
Data File : BE095152.D
Acq On : 27 Jan 2018 5:40
Operator : SJ/JU
Sample : J1174-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Jan 27 23:49:55 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

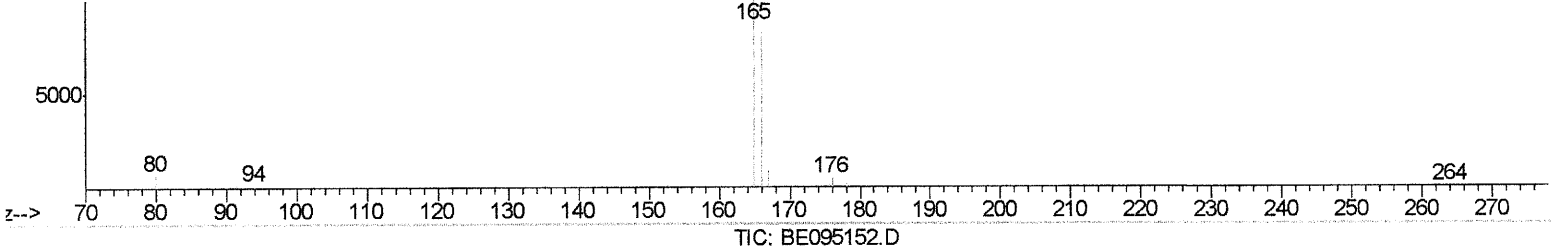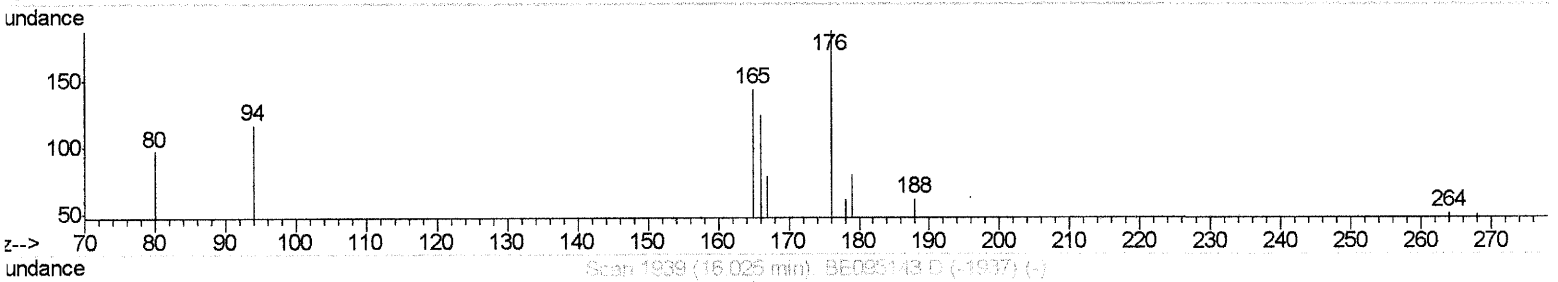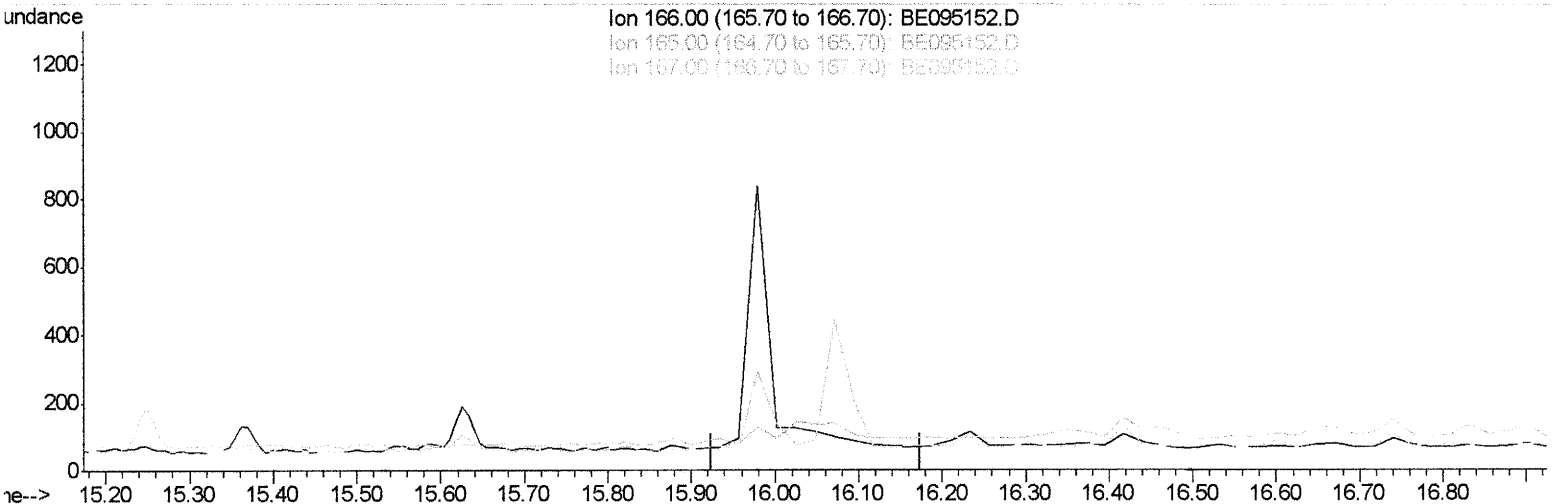

(9) Fluorene

16.025min (-16.025) 0.00ng/ul d

response 0

Ion	Exp%	Act%
166.00	100	0.00
165.00	91.80	0.00
167.00	18.30	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Instrument :
BNA_E
ClientSampleId :
F6A51

Manual Integrations
APPROVED

Sohil
1/29/2018 6:34:13 PM

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
Data File : BE095152.D
Acq On : 27 Jan 2018 5:40
Operator : SJ/JU
Sample : J1174-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Jan 27 23:49:55 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

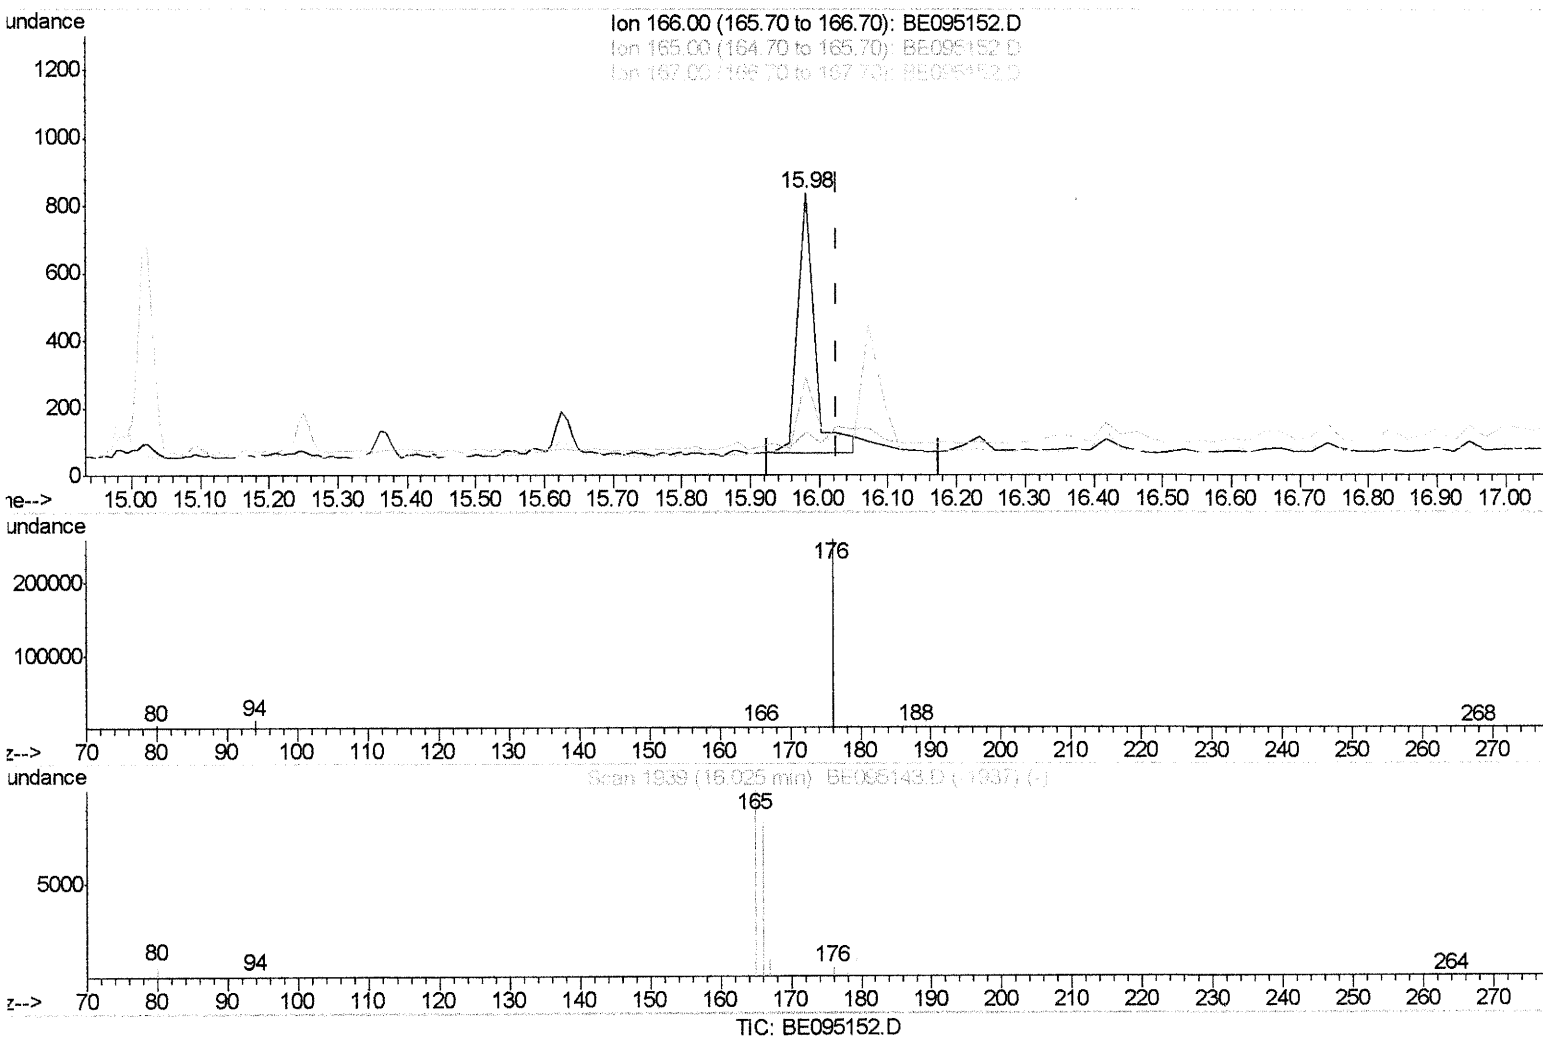

(9) Fluorene

15.979min (-0.046) 0.05ng/ul m

response 1344

Ion	Exp%	Act%
166.00	100	100
165.00	91.80	15.63#
167.00	18.30	35.20#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
 Data File : BE095153.D
 Acq On : 27 Jan 2018 6:16
 Operator : SJ/JU
 Sample : J1174-16
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6A51

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:34:13 PM

Quant Time: Jan 27 22:36:00 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 27 03:18:43 2018
 Response via : Initial Calibration

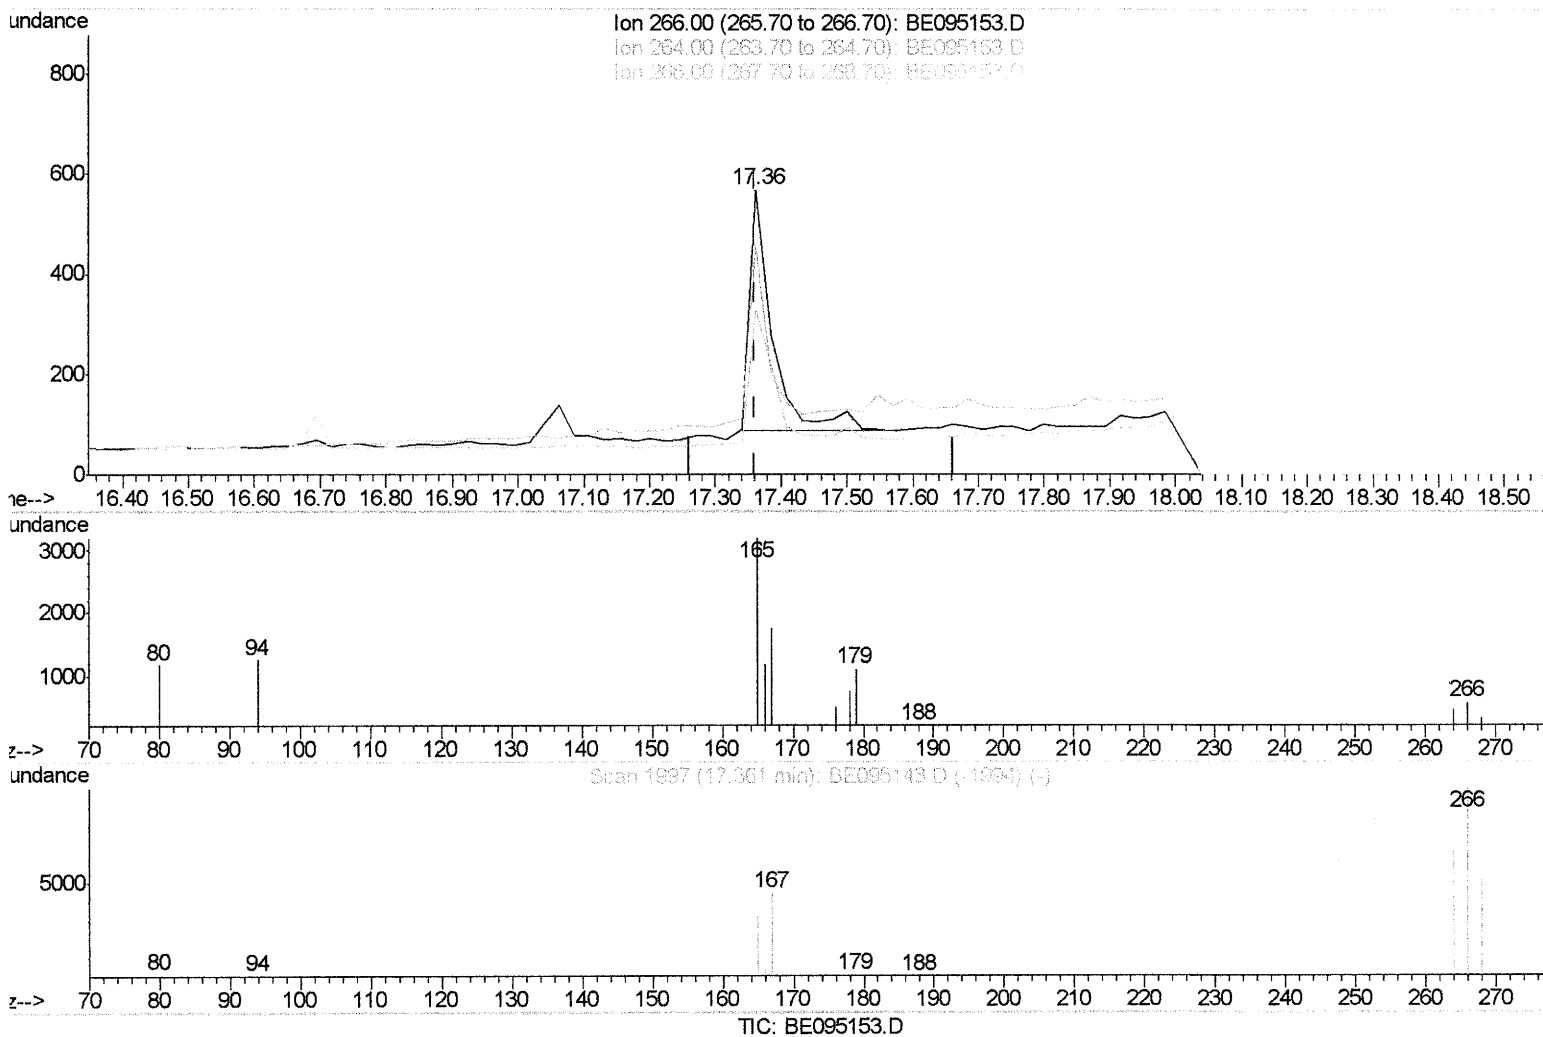

(11) Pentachlorophenol

17.362min (+0.001) 0.40ng/ul

response 1177

Ion	Exp%	Act%
266.00	100	100
264.00	59.90	56.50
268.00	62.30	57.01
0.00	0.00	0.00

Quantitation Report (Qedit)




Instrument :
BNA_E
ClientSampled :
F6A51

Manual Integrations
APPROVED

Sohil
1/29/2018 6:34:13 PM

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
Data File : BE095153.D
Acq On : 27 Jan 2018 6:16
Operator : SJ/JU
Sample : J1174-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Jan 27 22:36:00 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

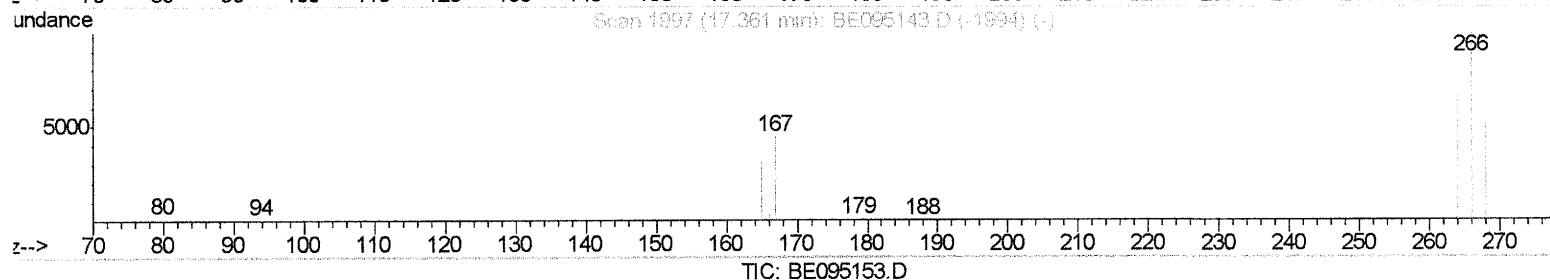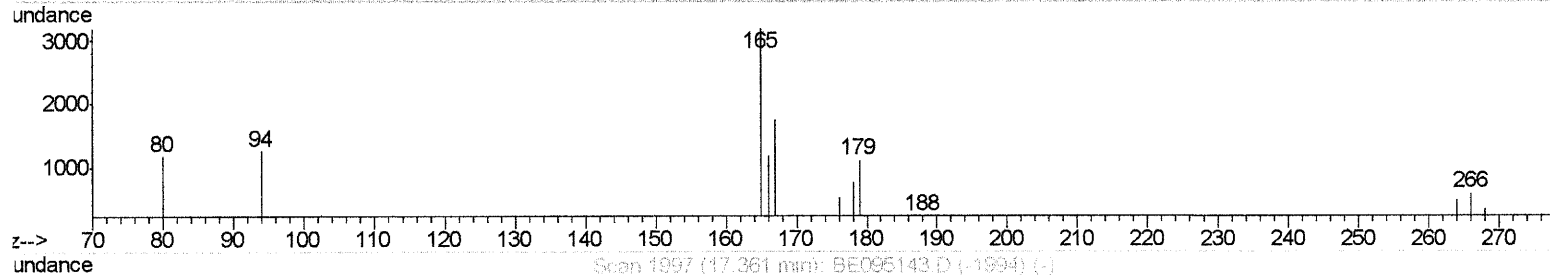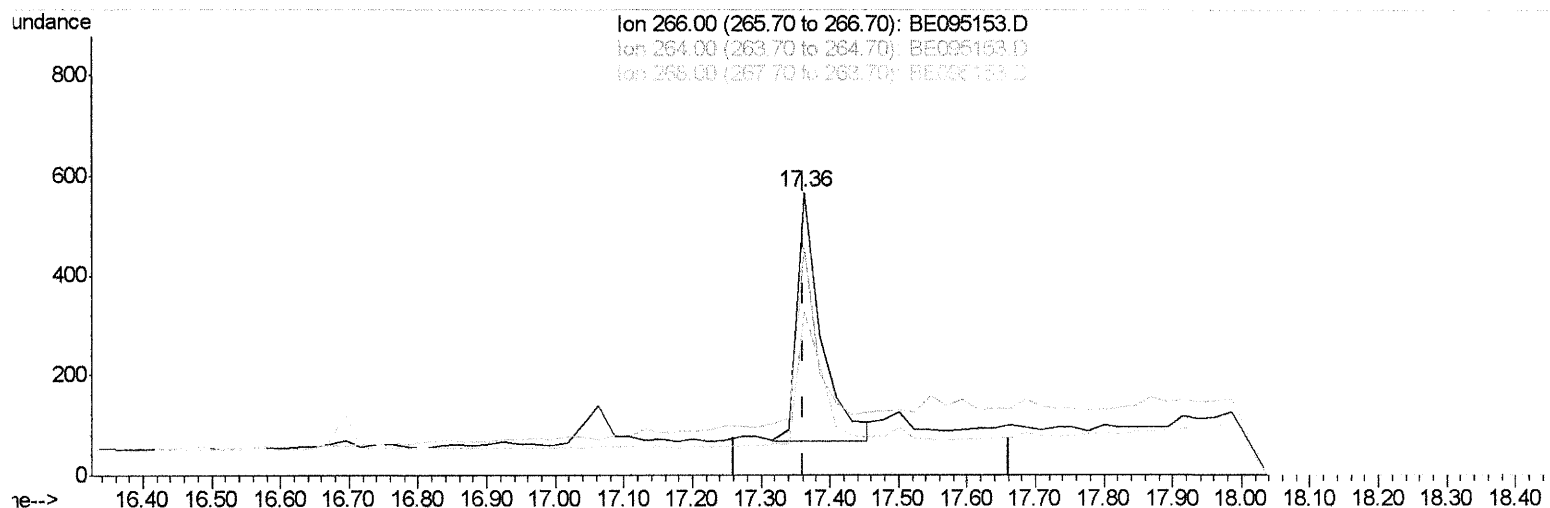

(11) Pentachlorophenol

17.362min (+0.001) 0.42ng/ul m

response 1239

Ion	Exp%	Act%
266.00	100	100
264.00	59.90	53.67
268.00	62.30	54.16
0.00	0.00	0.00

201/27/18

Quantitation Report (Qedit)


Instrument :
BNA_E
ClientSampleId :
F6A51

Manual Integrations
APPROVED

Sohil
1/29/2018 6:34:13 PM

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
Data File : BE095153.D
Acq On : 27 Jan 2018 6:16
Operator : SJ/JU
Sample : J1174-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Jan 27 22:36:00 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

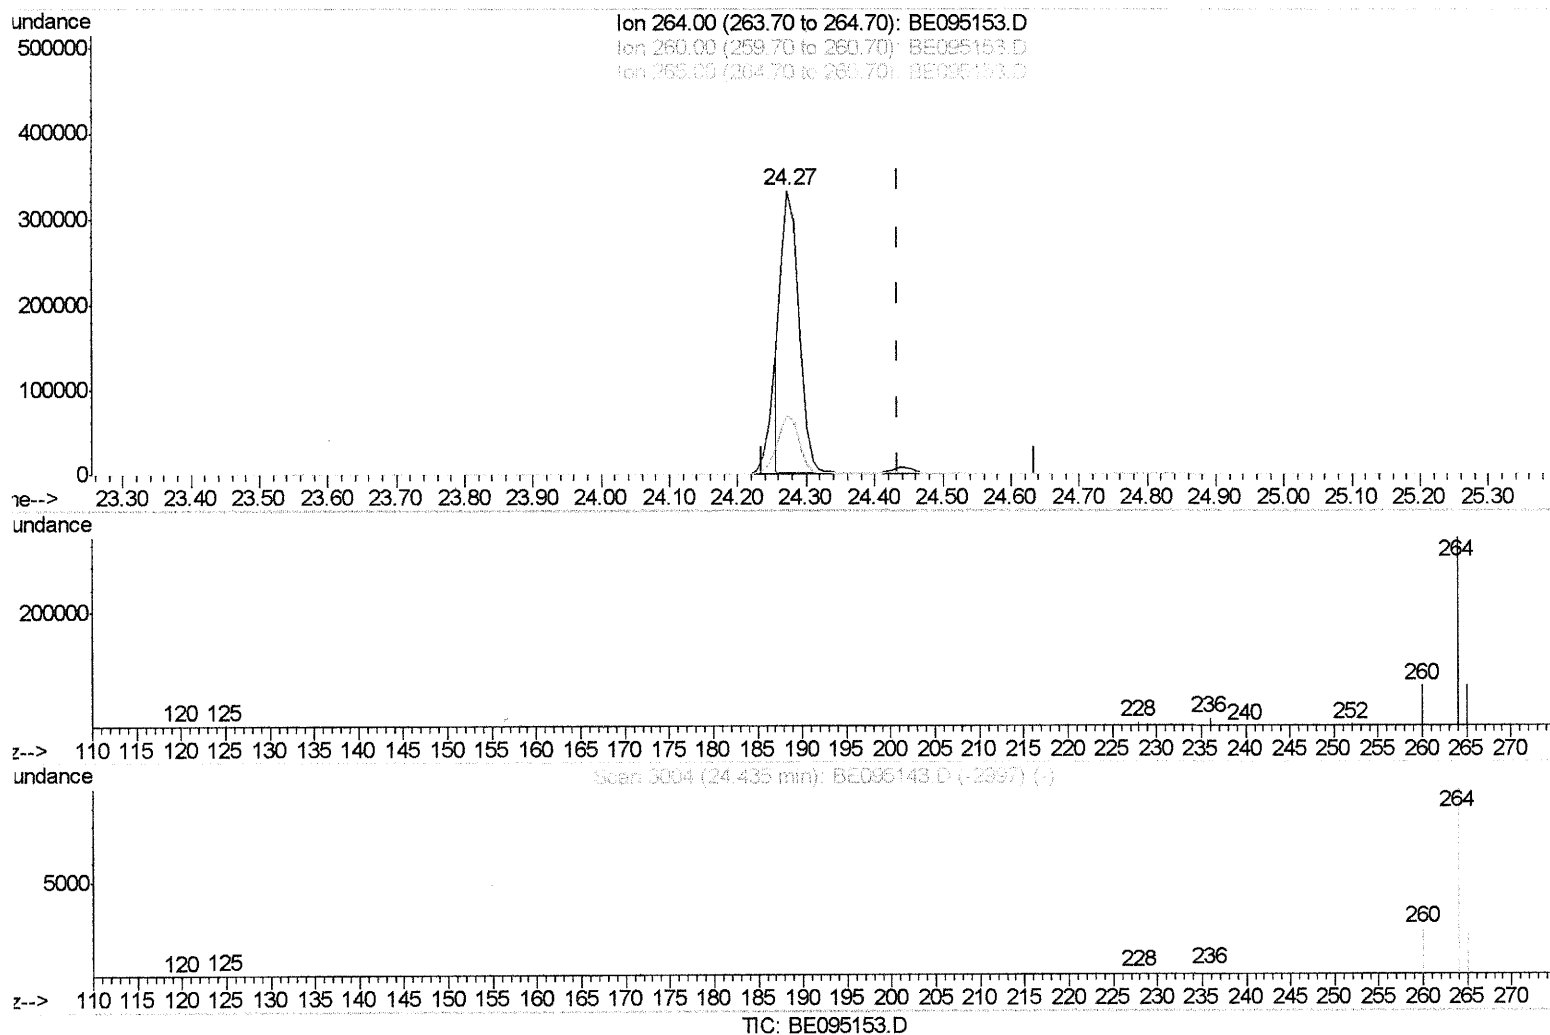

(20) Perylene-d12 (I)

24.273min (-0.162) 0.40ng/ul

response 605221

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.27#
265.00	103.50	21.36#
0.00	0.00	0.00

Quantitation Report (Qedit)


Instrument :
BNA_E
ClientSampleId :
F6A51

Manual Integrations
APPROVED

Sohil
1/29/2018 6:34:13 PM

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
Data File : BE095153.D
Acq On : 27 Jan 2018 6:16
Operator : SJ/JU
Sample : J1174-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Jan 27 22:36:00 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

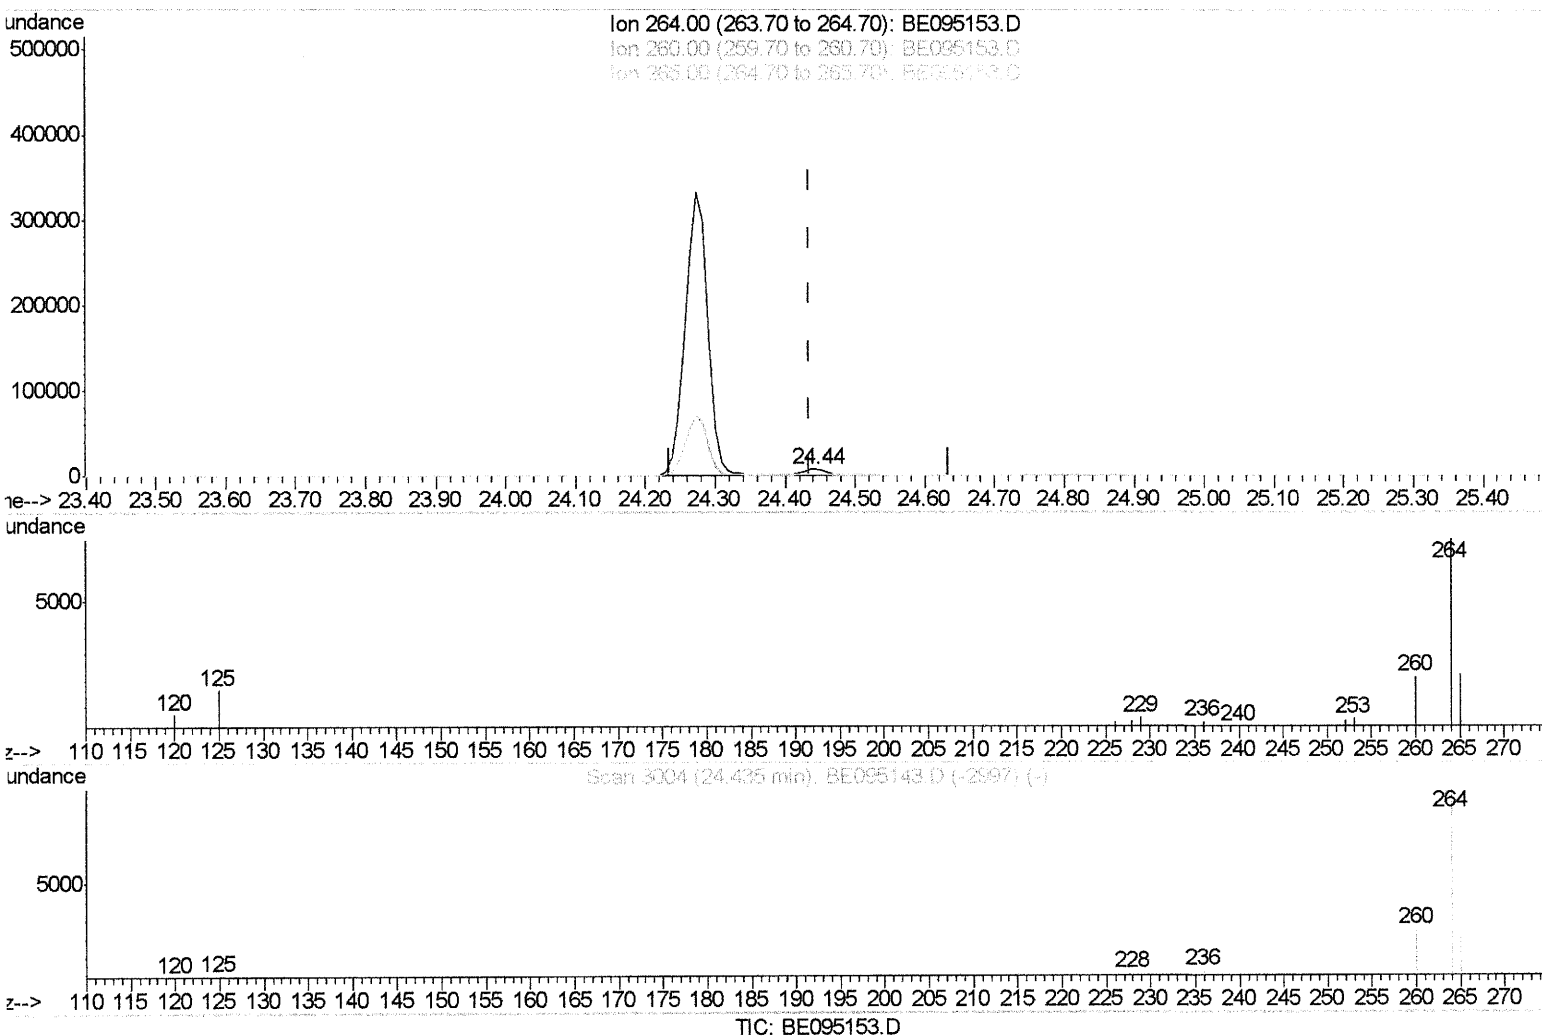

(20) Perylene-d12 (I)

24.444min (+0.009) 0.40ng/ul m

response 14789

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	28.52
265.00	103.50	29.54#
0.00	0.00	0.00

see 1/27/18

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
 Data File : BE095153.D
 Acq On : 27 Jan 2018 6:16
 Operator : SJ/JU
 Sample : J1174-16
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_E
 Client Sample ID :
 F6A51

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:34:13 PM

Quant Time: Jan 27 22:56:33 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 27 03:18:43 2018
 Response via : Initial Calibration

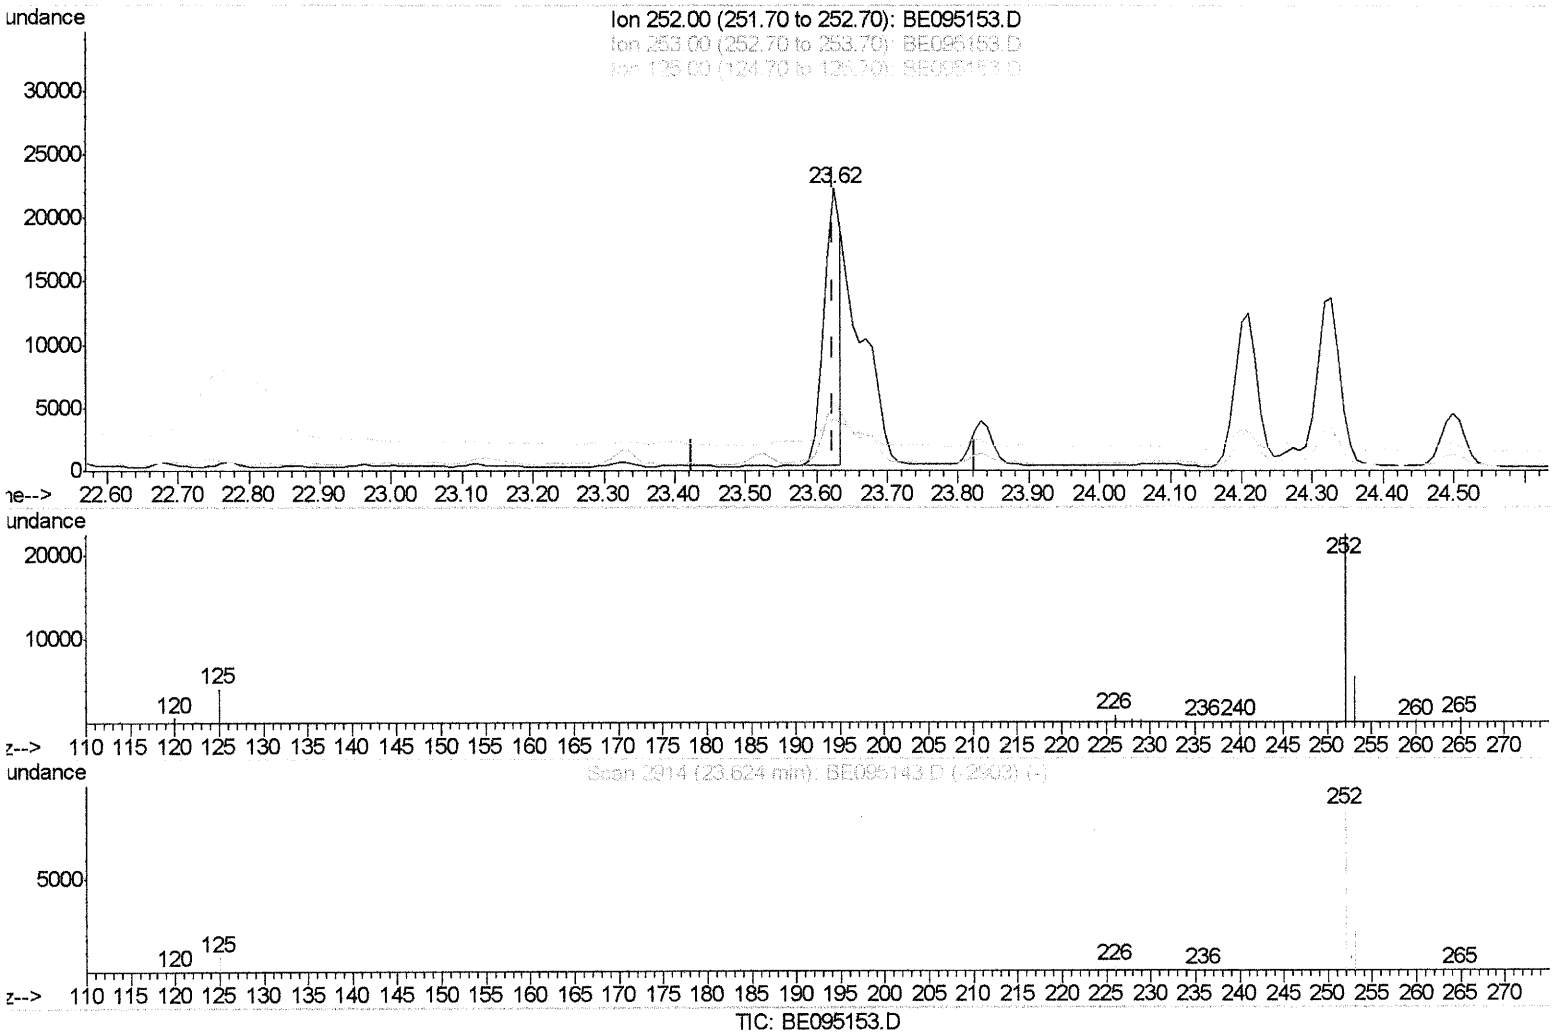

(21) Benzo(b)fluoranthene

23.624min (+0.000) 0.71ng/ul

response 37041

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	24.59
125.00	17.50	18.58
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
 Data File : BE095153.D
 Acq On : 27 Jan 2018 6:16
 Operator : SJ/JU
 Sample : J1174-16
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6A51

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:34:13 PM

Quant Time: Jan 27 22:56:33 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 27 03:18:43 2018
 Response via : Initial Calibration

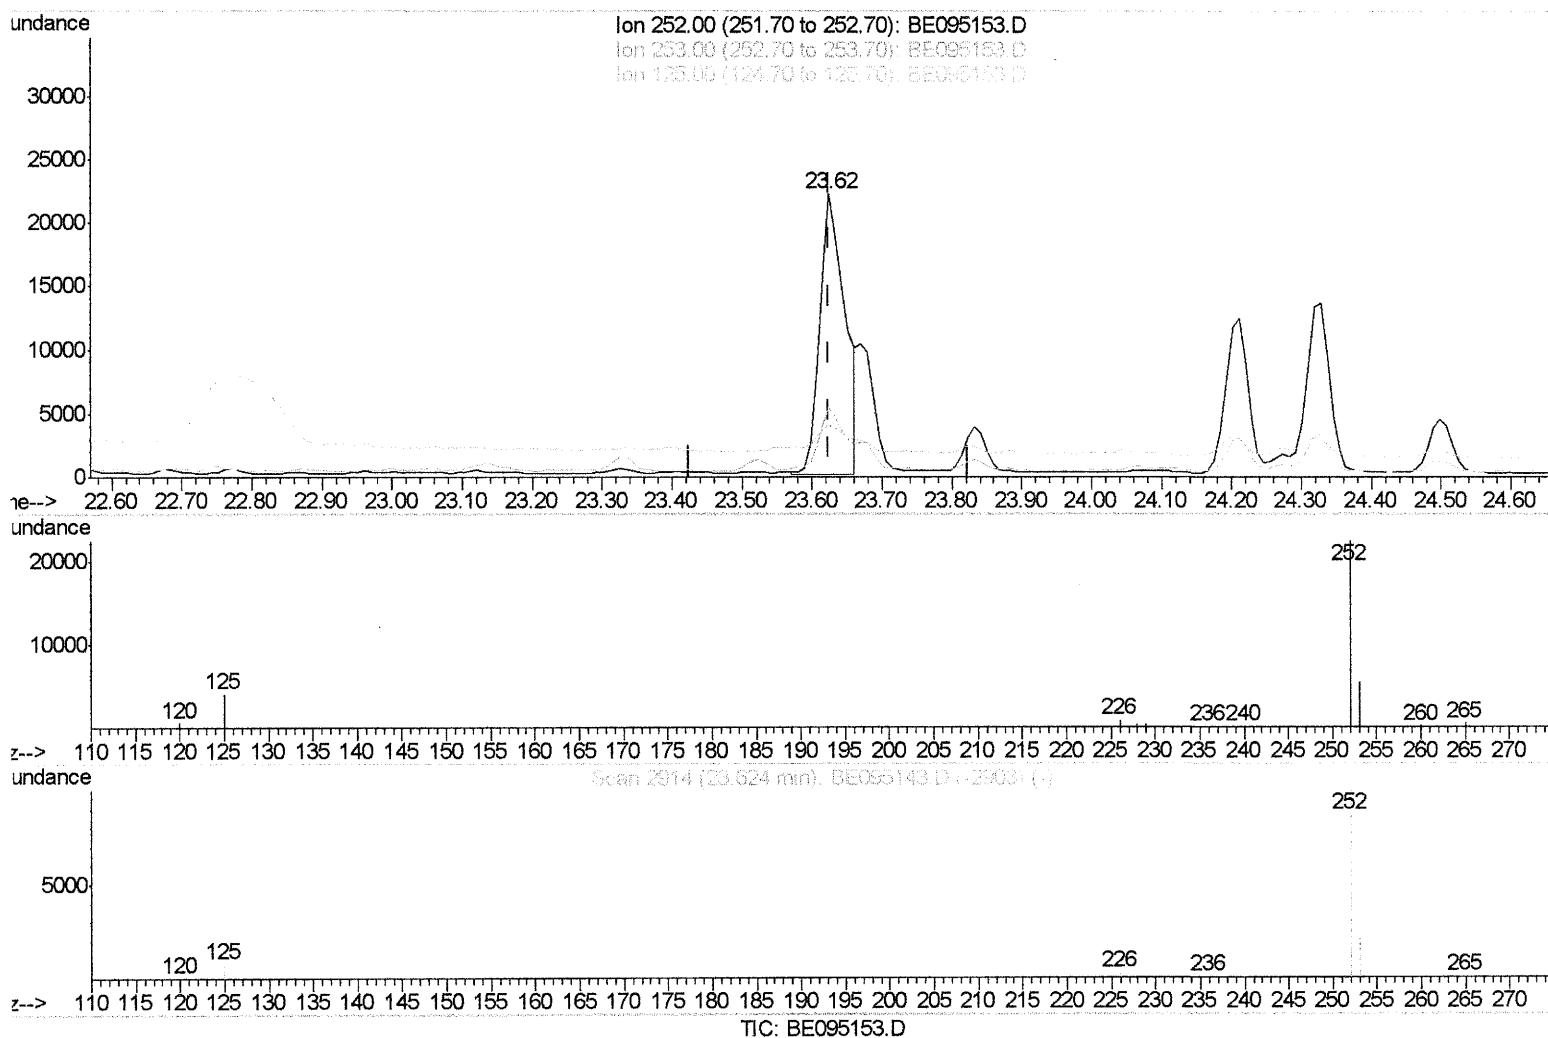

(21) Benzo(b)fluoranthene

23.624min (+0.000) 1.10ng/ul m

response 57155

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	24.59
125.00	17.50	18.58
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
Data File : BE095153.D
Acq On : 27 Jan 2018 6:16
Operator : SJ/JU
Sample : J1174-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
F6A51

Manual Integrations
APPROVED

Sohil
1/29/2018 6:34:13 PM

Quant Time: Jan 27 22:56:33 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

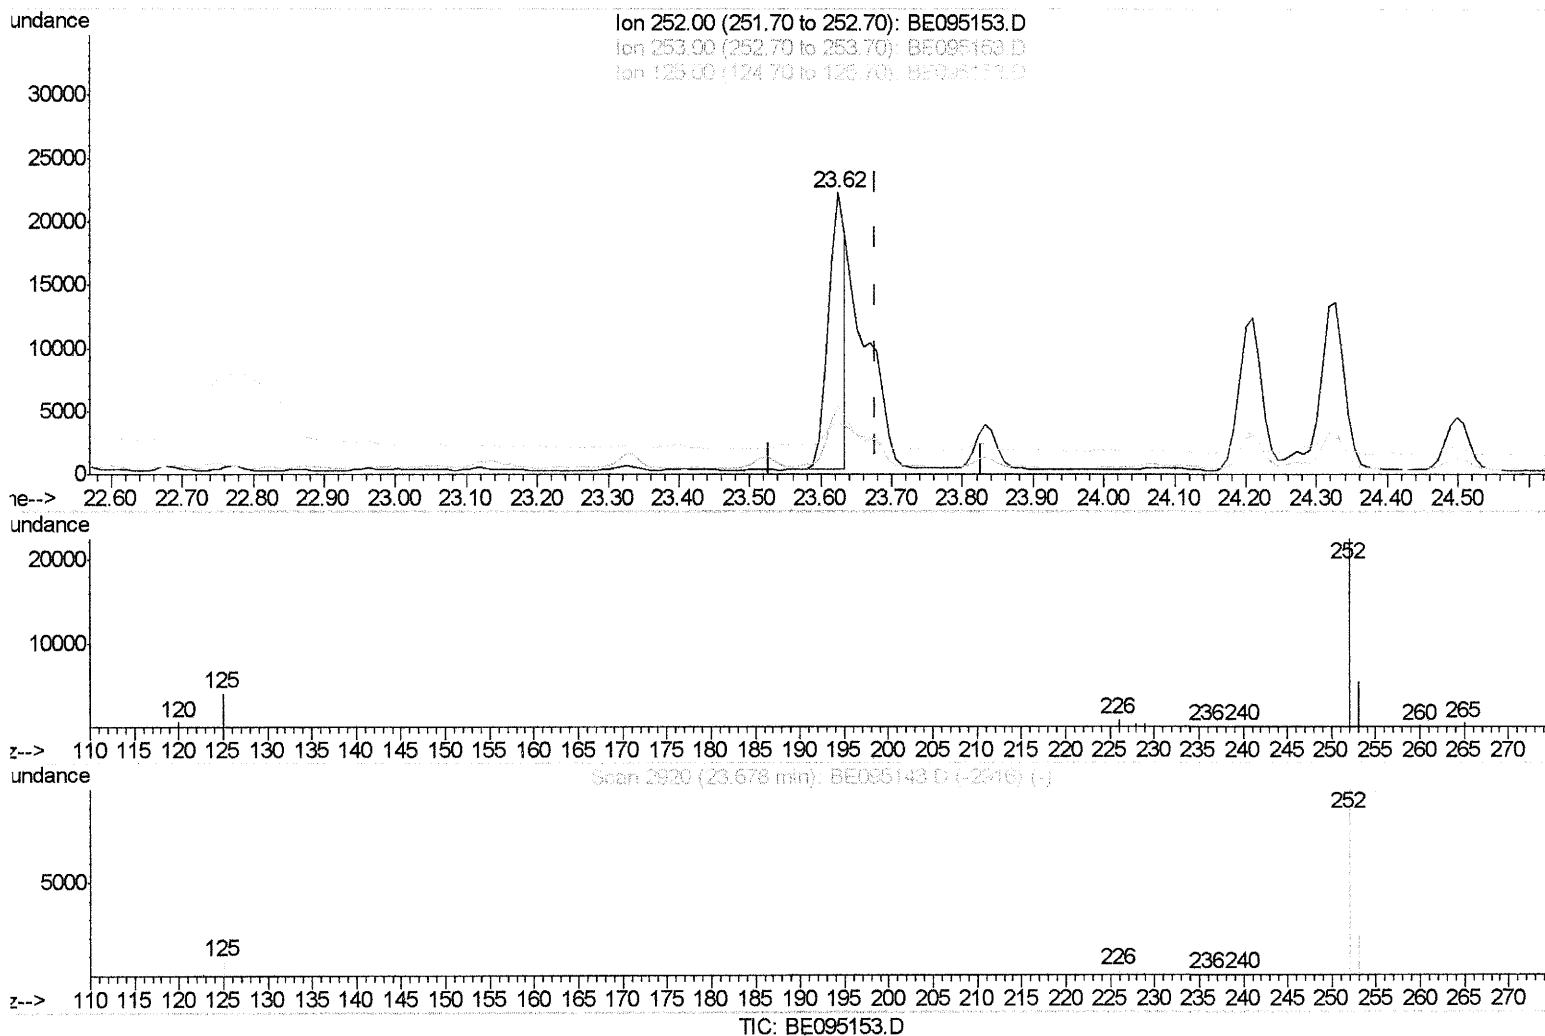

(22) Benzo(k)fluoranthene

23.624min (-0.054) 0.78ng/ul

response 37041

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	24.59
125.00	17.10	18.58
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
 Data File : BE095153.D
 Acq On : 27 Jan 2018 6:16
 Operator : SJ/JU
 Sample : J1174-16
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6A51

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:34:13 PM

Quant Time: Jan 27 22:56:33 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 27 03:18:43 2018
 Response via : Initial Calibration

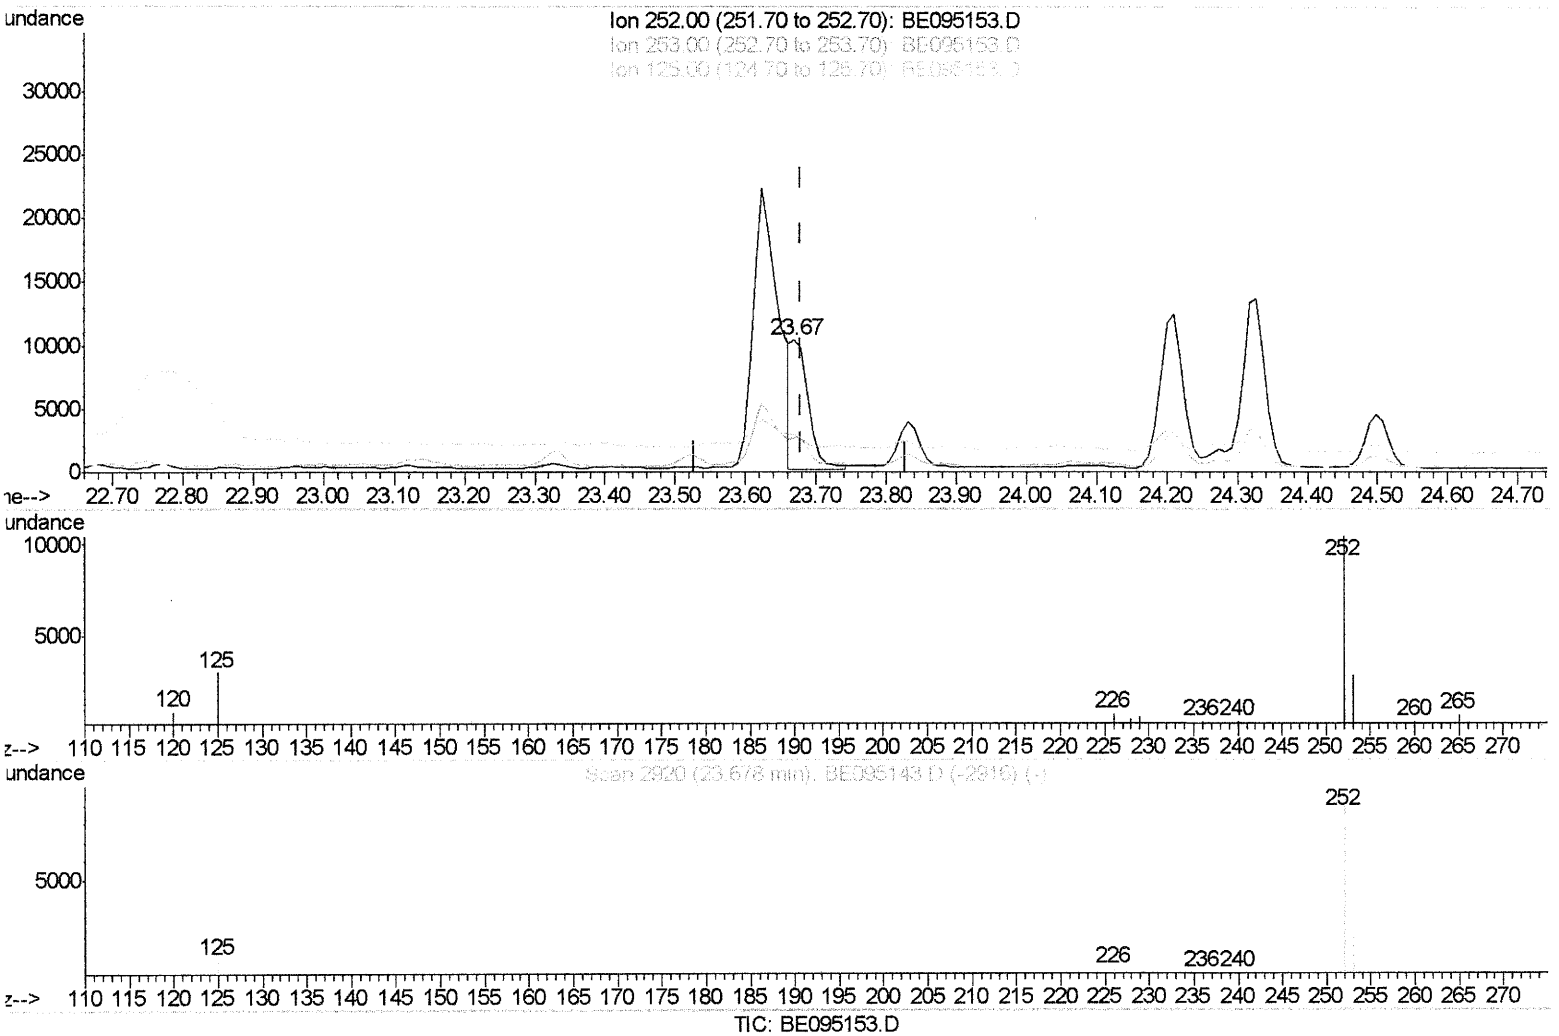

(22) Benzo(k)fluoranthene

23.669min (-0.009) 0.35ng/ul m

response 16844

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	26.44
125.00	17.10	28.48#
0.00	0.00	0.00

229/27/18

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
 Data File : BE095153.D
 Acq On : 27 Jan 2018 6:16
 Operator : SJ/JU
 Sample : J1174-16
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6A51

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:34:13 PM

Quant Time: Jan 27 22:58:19 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 27 03:18:43 2018
 Response via : Initial Calibration

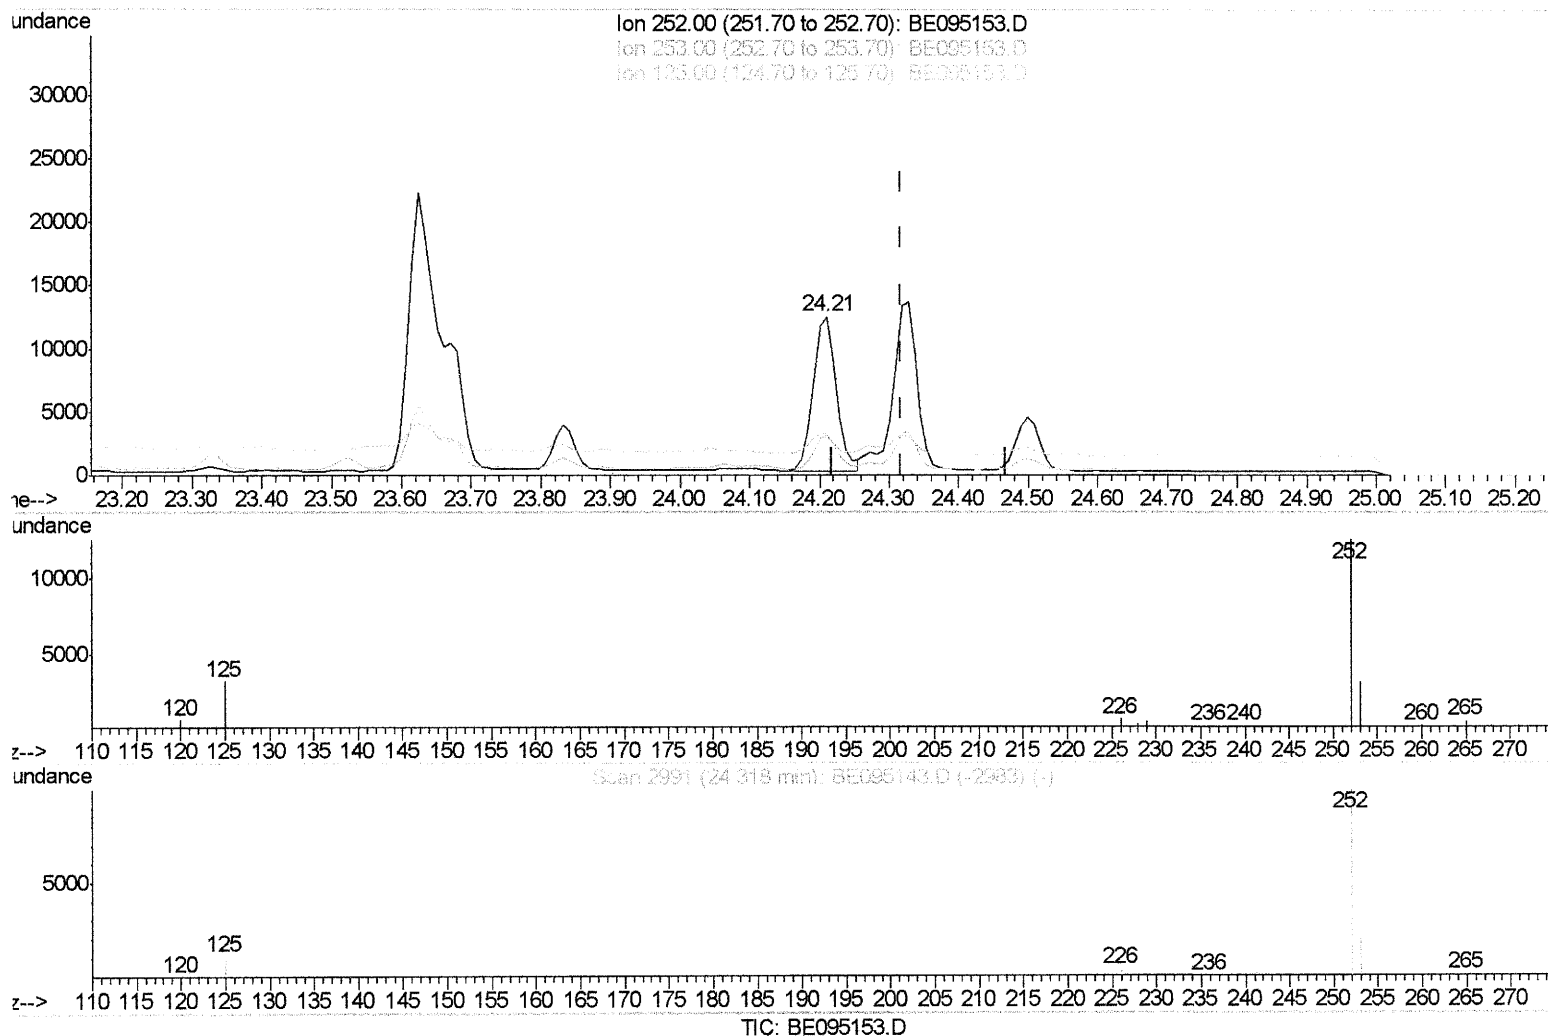

(23) Benzo(a)pyrene (C)

24.210min (-0.108) 0.59ng/ul

response 27701

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	25.07#
125.00	22.60	25.85
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
 Data File : BE095153.D
 Acq On : 27 Jan 2018 6:16
 Operator : SJ/JU
 Sample : J1174-16
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6A51

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:34:13 PM

Quant Time: Jan 27 22:58:19 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 27 03:18:43 2018
 Response via : Initial Calibration

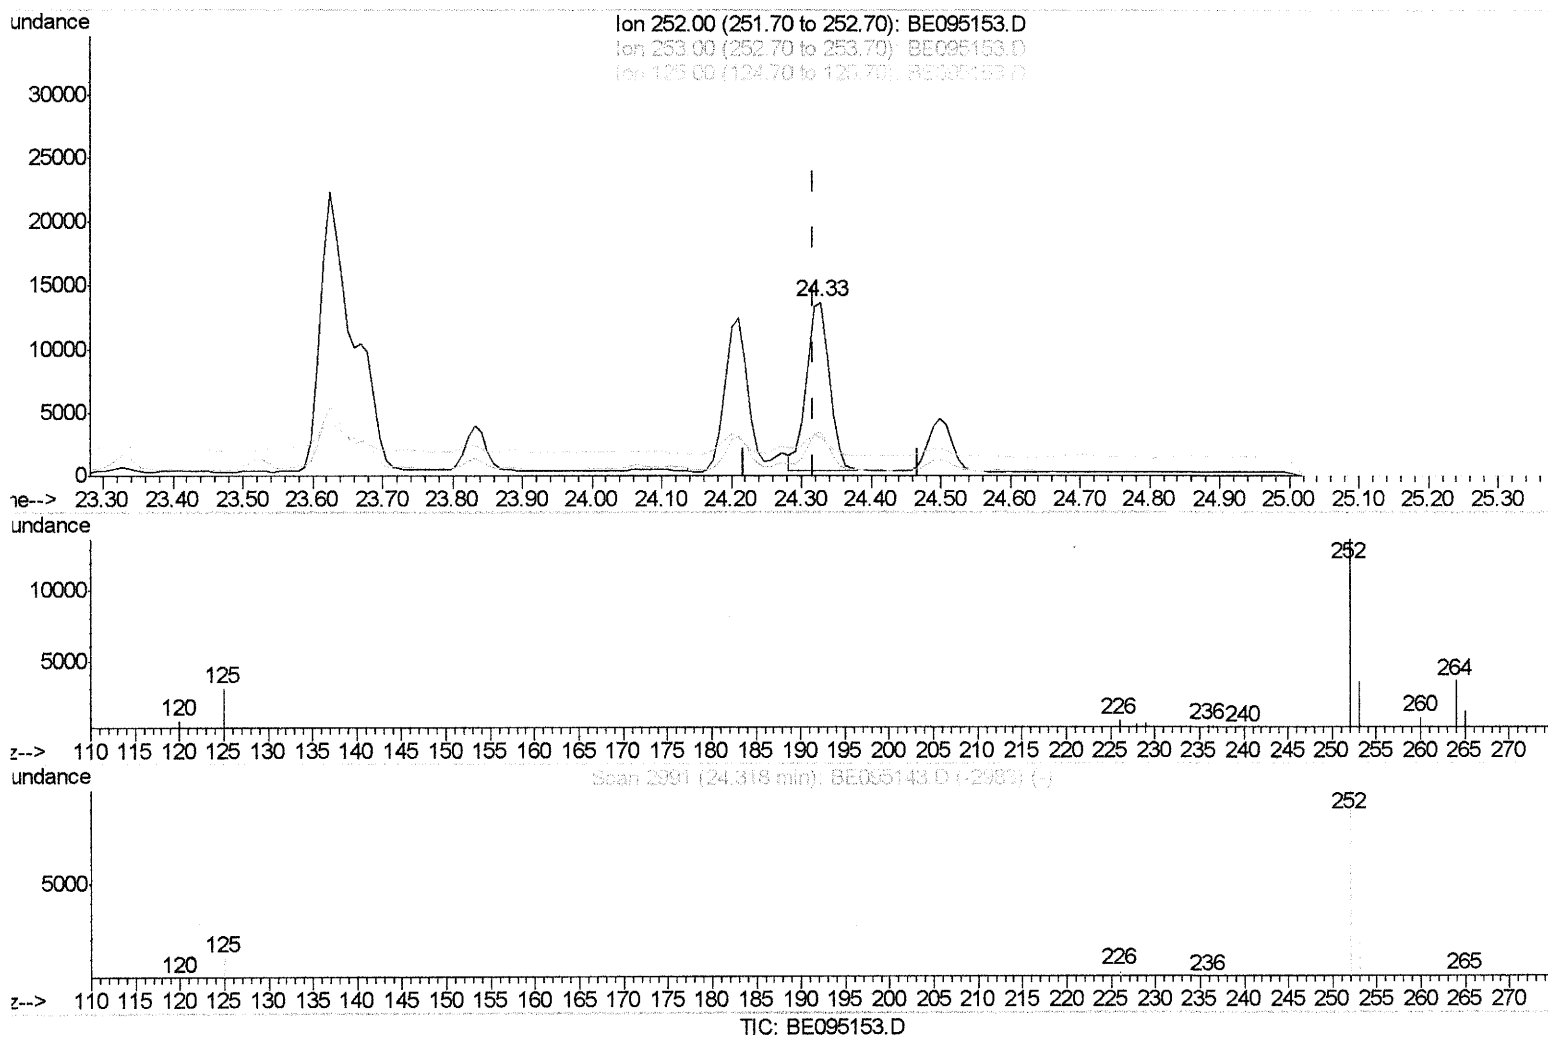

(23) Benzo(a)pyrene (C)

24.327min (+0.009) 0.65ng/ul m

response 30276

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	25.22#
125.00	22.60	22.34
0.00	0.00	0.00

24.327min

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
 Data File : BE095153.D
 Acq On : 27 Jan 2018 6:16
 Operator : SJ/JU
 Sample : J1174-16
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6A51

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:34:13 PM

Quant Time: Jan 27 23:05:05 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 27 03:18:43 2018
 Response via : Initial Calibration

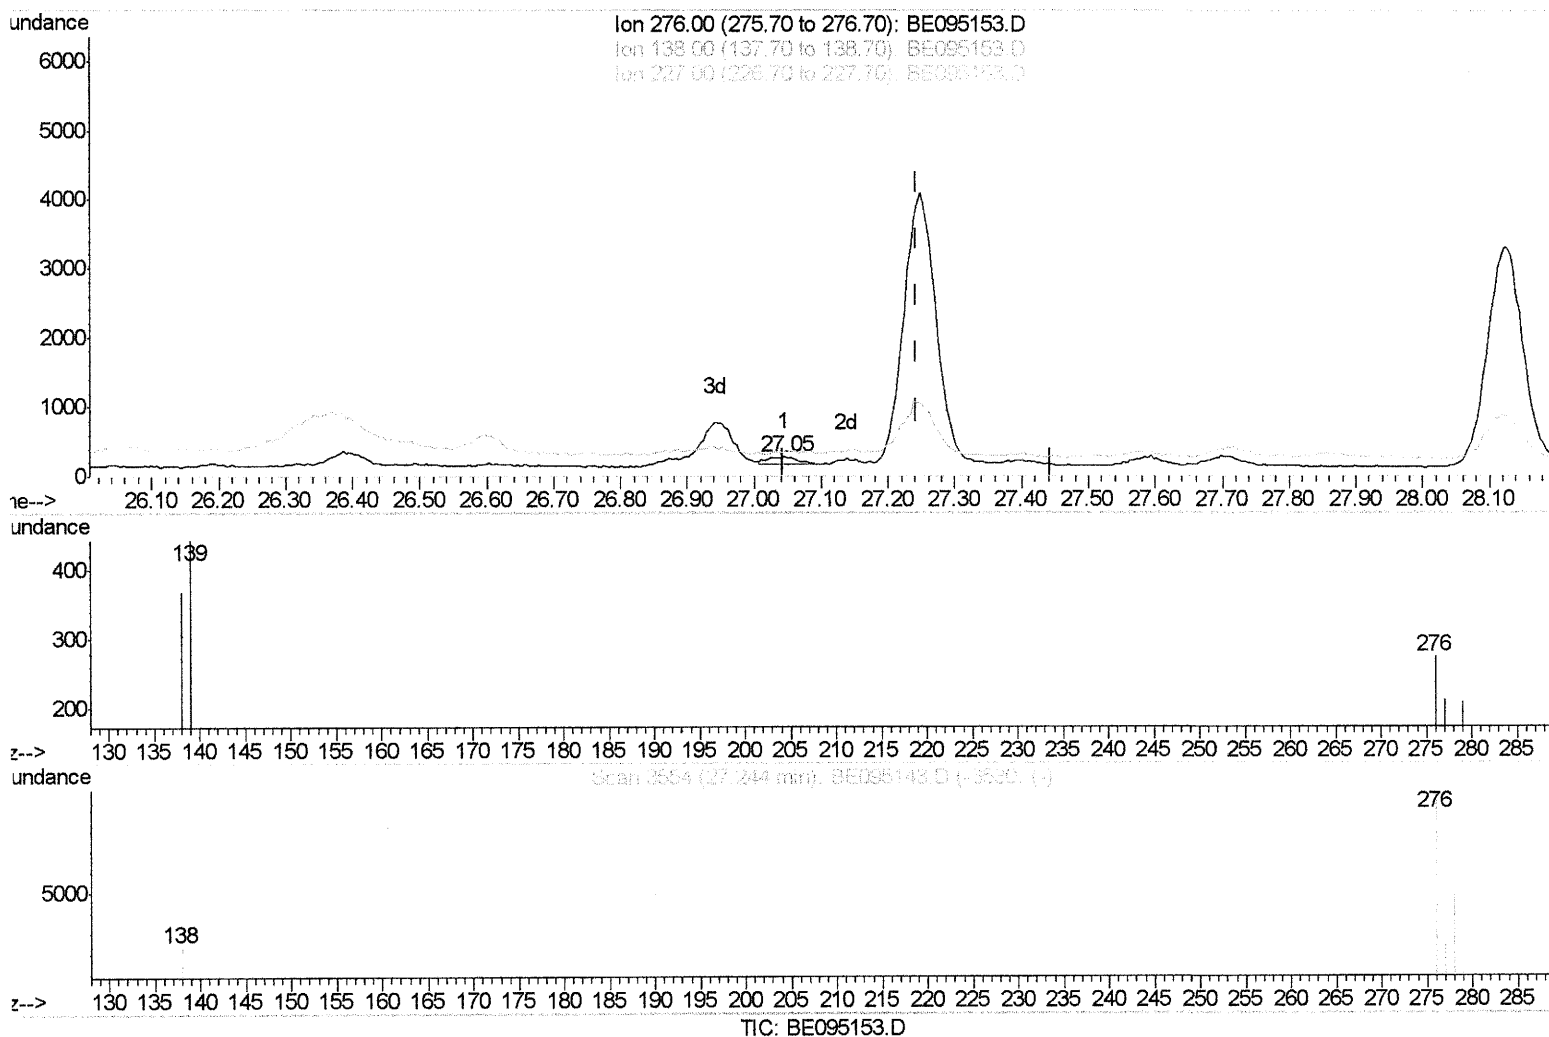

(24) Indeno(1,2,3-cd)pyrene

27.046min (-0.197) 0.01ng/ul

response 303

Ion	Exp%	Act%
276.00	100	100
138.00	35.00	9.24#
227.00	10.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Instrument :
BNA_E
ClientSampled :
F6A51

Manual Integrations
APPROVED

Sohil
1/29/2018 6:34:13 PM

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
Data File : BE095153.D
Acq On : 27 Jan 2018 6:16
Operator : SJ/JU
Sample : J1174-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Jan 27 23:05:05 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

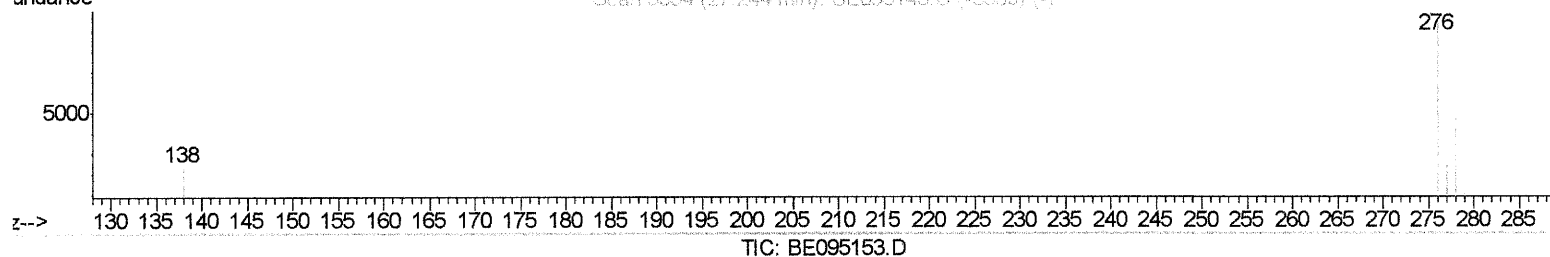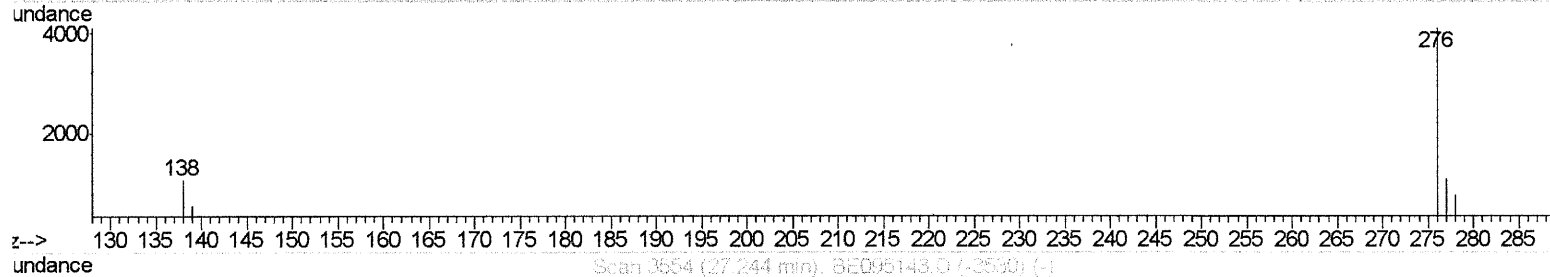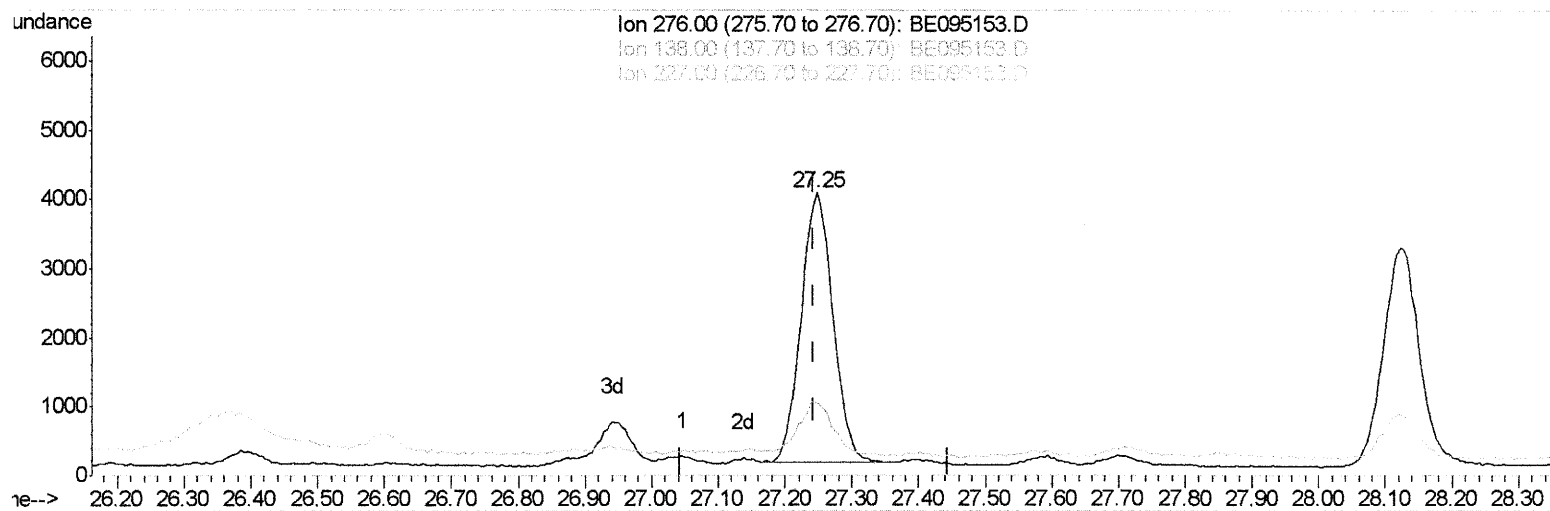

(24) Indeno(1,2,3-cd)pyrene

27.247min (+0.003) 0.25ng/ul m

response 13029

Ion	Exp%	Act%
276.00	100	100
138.00	35.00	0.21#
227.00	10.00	0.00#
0.00	0.00	0.00

3001/30/12

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
 Data File : BE095153.D
 Acq On : 27 Jan 2018 6:16
 Operator : SJ/JU
 Sample : J1174-16
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6A51

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:34:13 PM

Quant Time: Jan 27 23:07:18 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 27 03:18:43 2018
 Response via : Initial Calibration

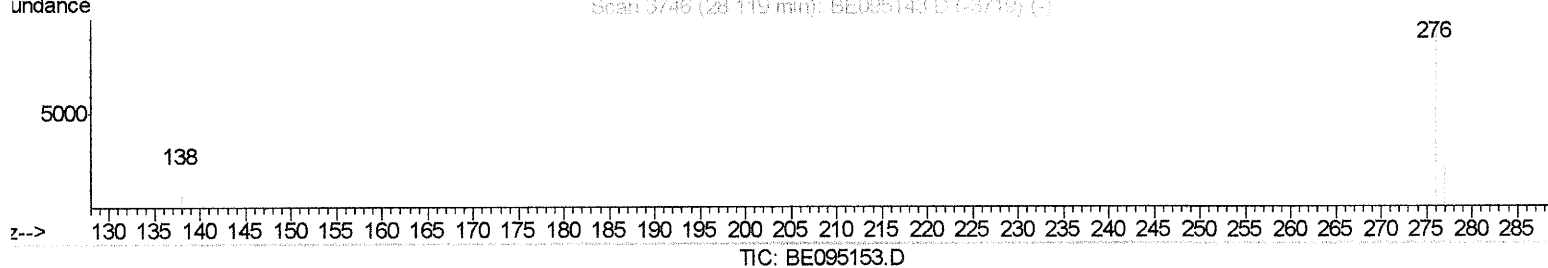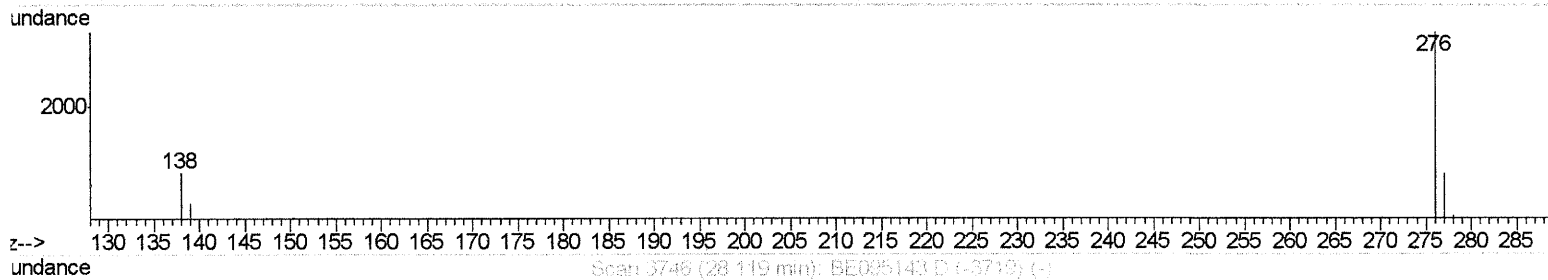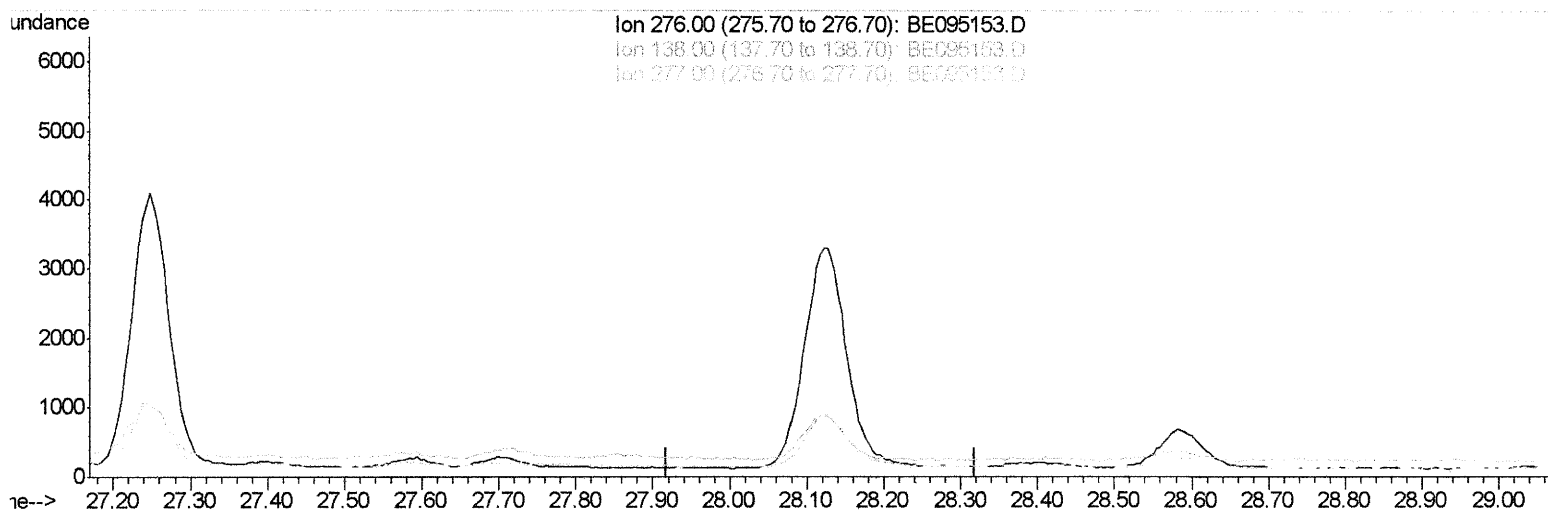

(26) Benzo(g,h,i)perylene

28.119min (-28.119) 0.00ng/ul

response 0

Ion	Exp%	Act%
276.00	100	0.00
138.00	27.30	0.00#
277.00	25.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
 Data File : BE095153.D
 Acq On : 27 Jan 2018 6:16
 Operator : SJ/JU
 Sample : J1174-16
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6A51

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:34:13 PM

Quant Time: Jan 27 23:07:18 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 27 03:18:43 2018
 Response via : Initial Calibration

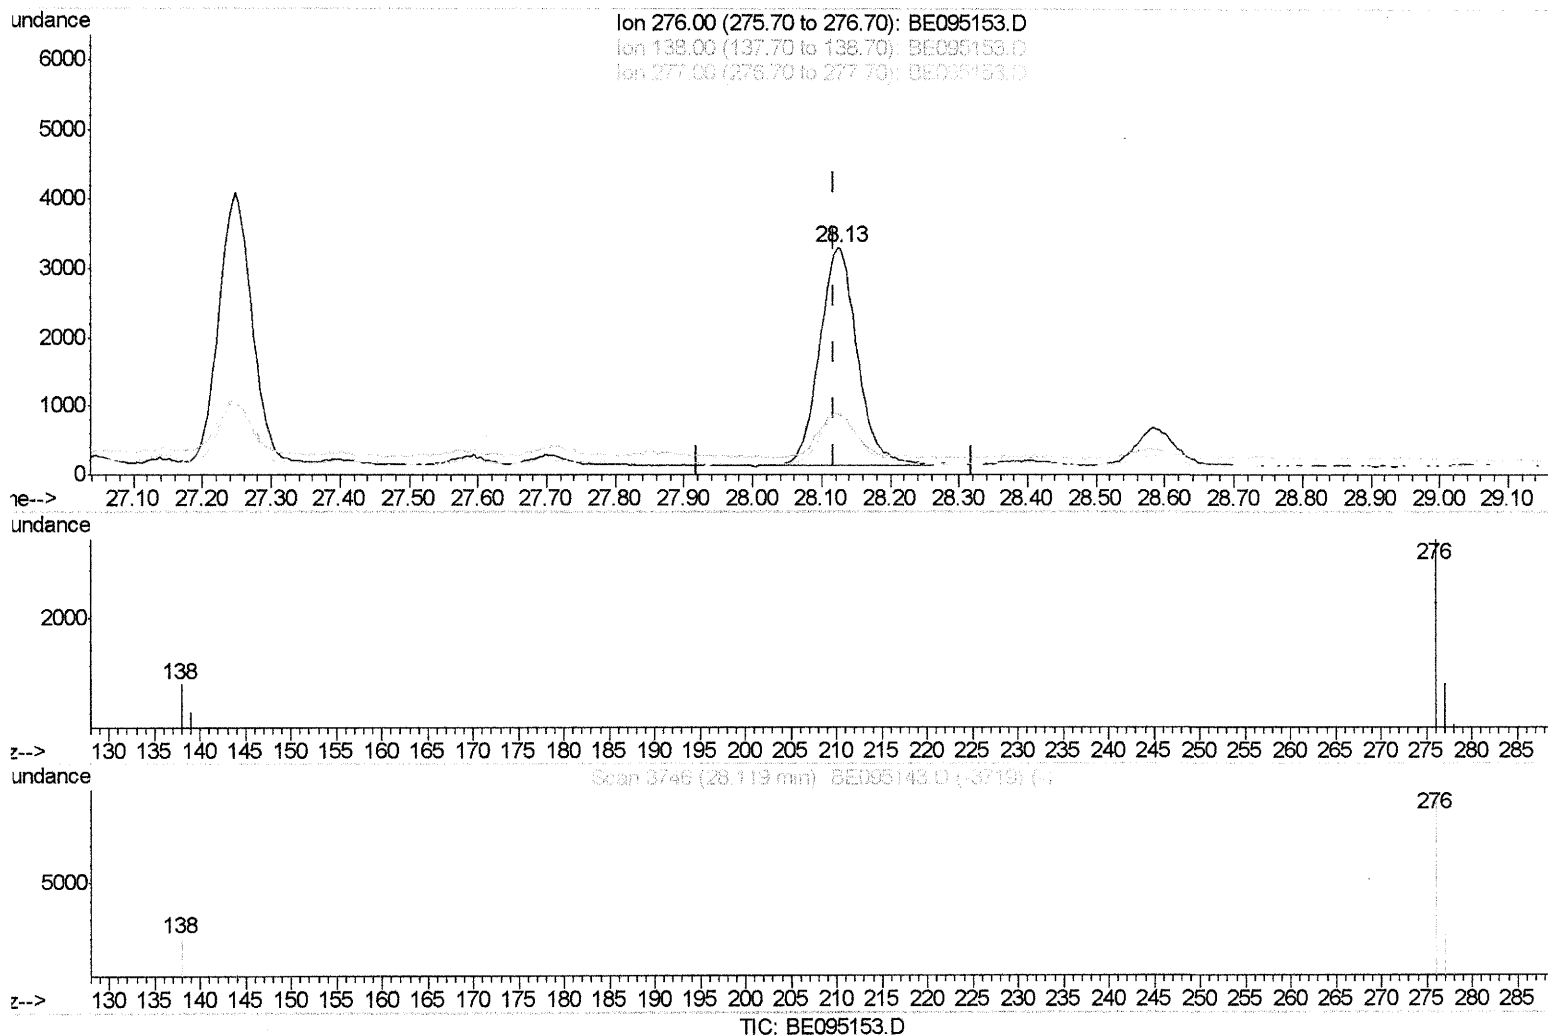

(26) Benzo(g,h,i)perylene

28.126min (+0.008) 0.28ng/ul m

response 12212

Ion	Exp%	Act%
276.00	100	100
138.00	27.30	26.77
277.00	25.60	27.28
0.00	0.00	0.00

JU 1/27/18

Quantitation Report (Qedit)




Instrument :
BNA_E
ClientSampled :
F6A51

Manual Integrations
APPROVED

Sohil
1/29/2018 6:34:13 PM

Data Path : Z:\HPCHEM1\BNA_E\Data\BE012618\
Data File : BE095153.D
Acq On : 27 Jan 2018 6:16
Operator : SJ/JU
Sample : J1174-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Jan 27 23:36:07 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

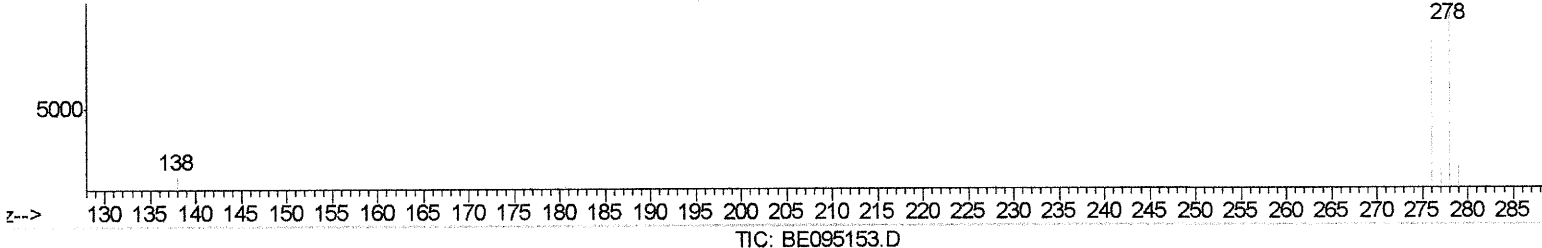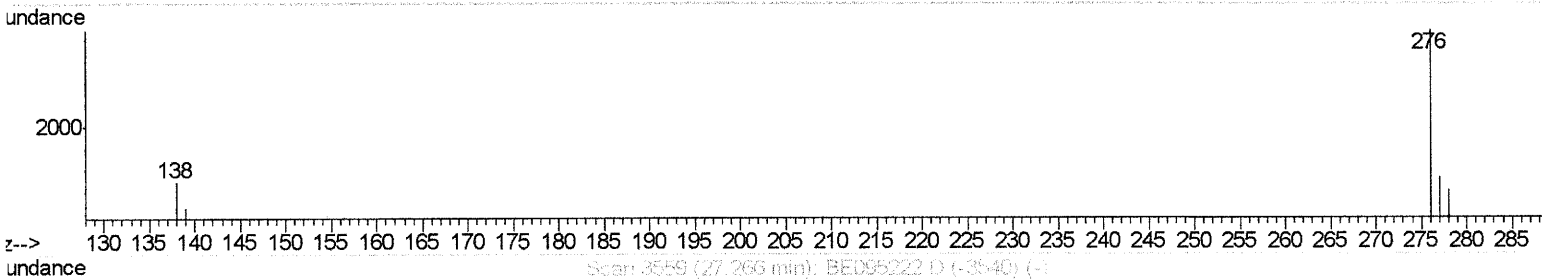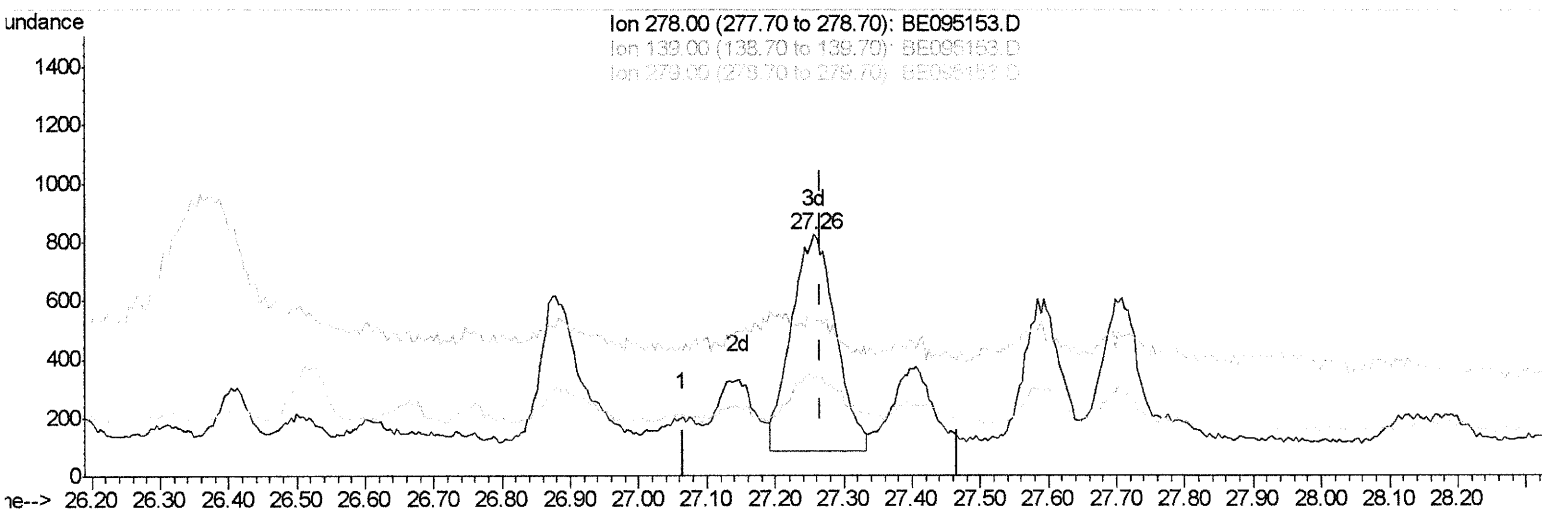

(25) Dibenzo(a,h)anthracene

27.256min (-0.010) 0.08ng/ul m

response 3347

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	64.04#
279.00	32.40	40.68#
0.00	0.00	0.00

ju 1/27/18

Quantitation Report (QT Reviewed)

Instrument :
BNA_E
ClientSampled :
F6A51

Manual Integrations
APPROVED

Sohil
1/29/2018 6:34:13 PM

Data Path : Z:\HPCHEM1\BNA_E\Data\BE012618\
Data File : BE095153.D
Acq On : 27 Jan 2018 6:16
Operator : SJ/JU
Sample : J1174-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Jan 29 16:41:00 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	3856	0.40	ng/ul	0.00
2) Naphthalene-d8	11.27	136	12249	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	8474	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.73	188	15252	0.40	ng/ul	0.02
16) Chrysene-d12	21.80	240	16646	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	14789m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.82	152	4190	0.21	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	11134	0.19	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
5) 2-Methylnaphthalene	12.89	142	63239	2.761	ng/ul	99
7) Acenaphthylene	14.75	152	4904	0.120	ng/ul#	26
8) Acenaphthene	15.08	153	110339	3.488	ng/ul	97
9) Fluorene	16.03	166	103743	3.180	ng/ul#	71
11) Pentachlorophenol	17.36	266	1239m	0.419	ng/ul	85
12) Phenanthrene	17.75	178	584733	11.399	ng/ul#	85
13) Anthracene	17.85	178	97107	2.068	ng/ul#	91
15) Fluoranthene	19.73	202	525612	7.914	ng/ul	83
17) Pyrene	20.08	202	398267	7.130	ng/ul#	80
18) Benzo(a)anthracene	21.79	228	78933	1.517	ng/ul#	87
19) Chrysene	21.84	228	74602	1.380	ng/ul	96
21) Benzo(b)fluoranthene	23.62	252	57155m	1.095	ng/ul	}
22) Benzo(k)fluoranthene	23.67	252	16844m	0.353	ng/ul	
23) Benzo(a)pyrene	24.33	252	30276m	0.650	ng/ul	
24) Indeno(1,2,3-cd)pyrene	27.25	276	13029m	0.255	ng/ul	
25) Dibenzo(a,h)anthracene	27.26	278	3347m	0.080	ng/ul	
26) Benzo(g,h,i)perylene	28.13	276	12212m	0.282	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed