

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA_E\Data\BE012618\
 Data File : BE095154.D
 Acq On : 27 Jan 2018 6:52
 Operator : SJ/JU
 Sample : J1174-11
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_E
 Client Sample ID :
 F6A46

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:34:23 PM

Quant Time: Jan 29 16:45:06 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 27 03:18:43 2018
 Response via : Initial Calibration

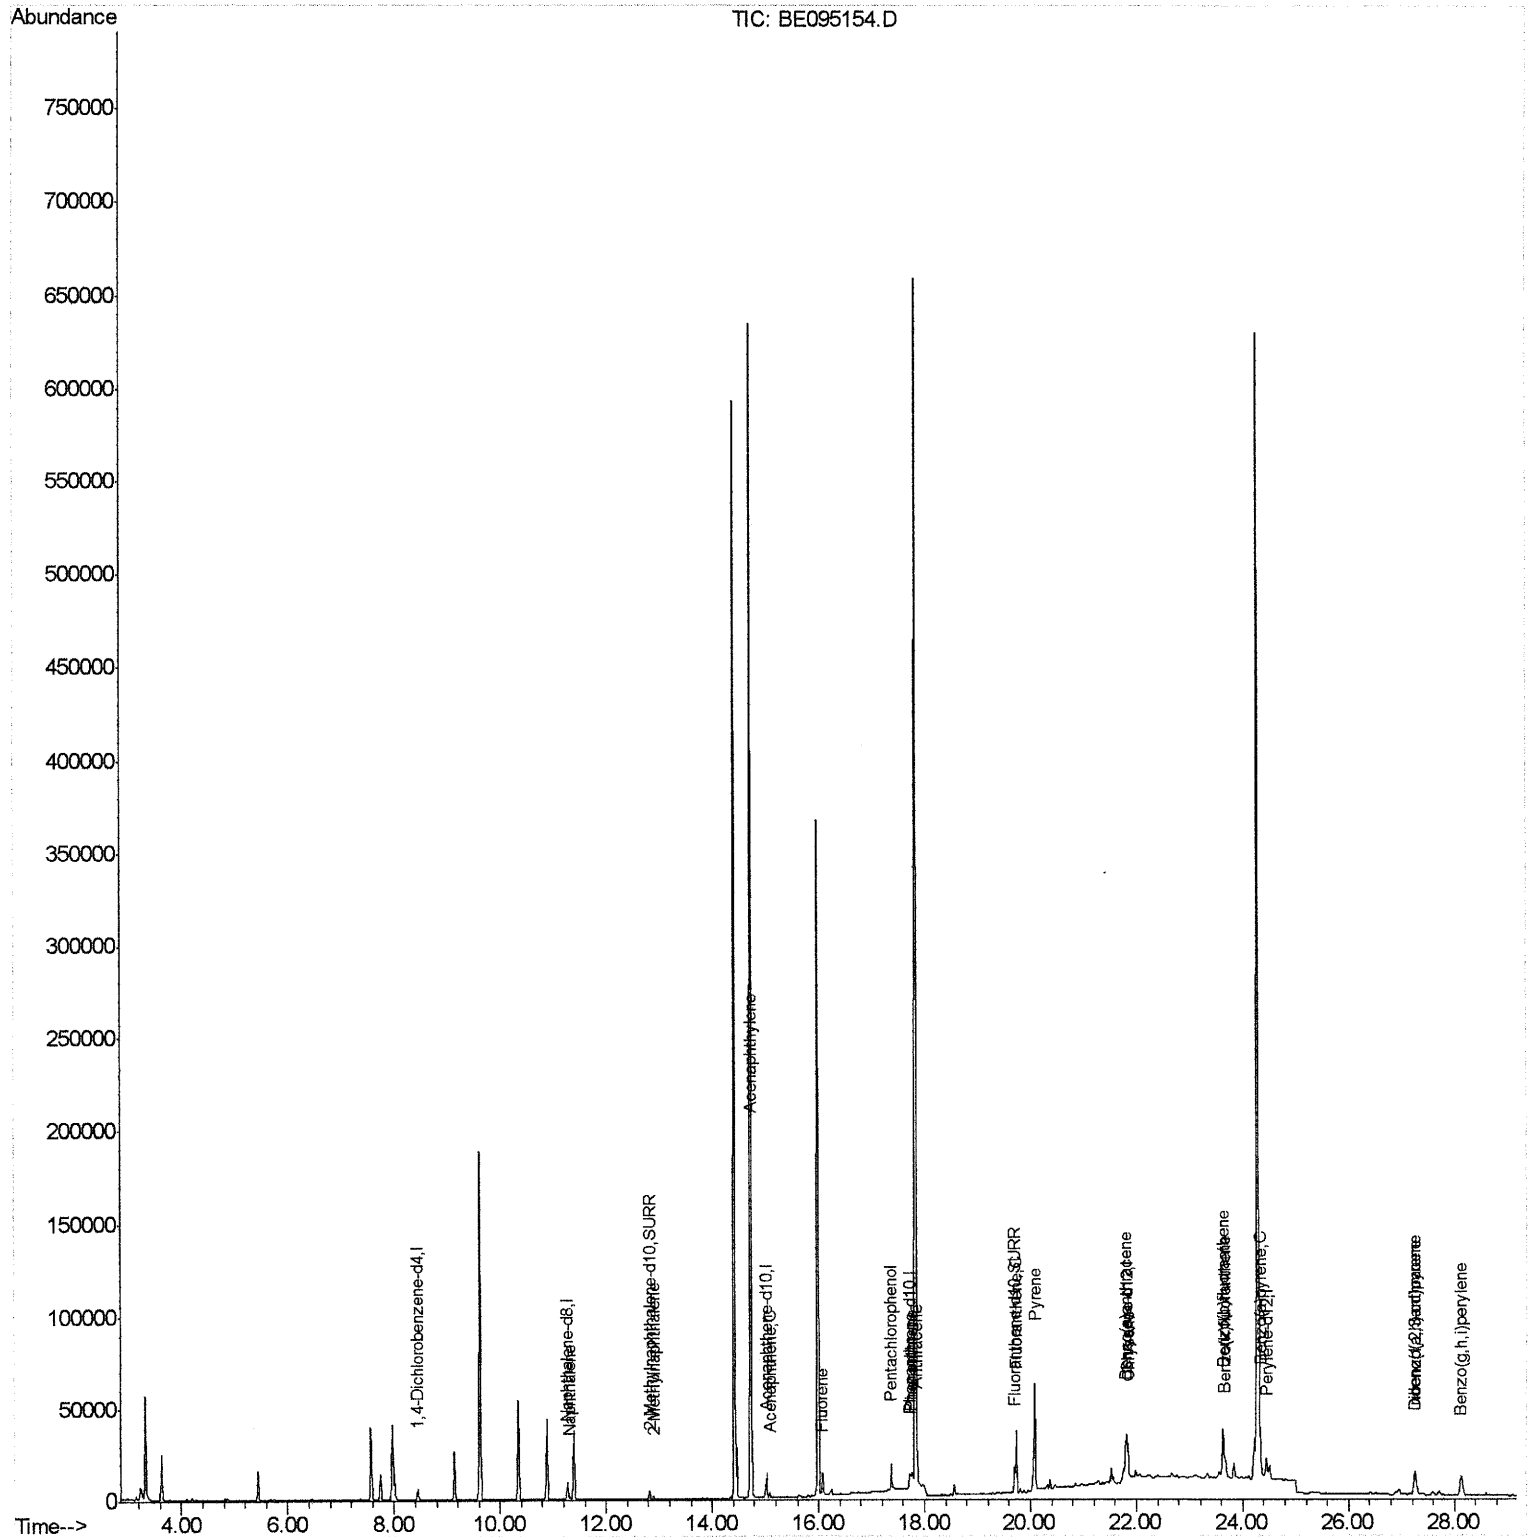

Quantitation Report (Qedit)


Instrument :
BNA_E
ClientSampled :
F6A46

Manual Integrations
APPROVED

Sohil
1/29/2018 6:34:23 PM

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
Data File : BE095154.D
Acq On : 27 Jan 2018 6:52
Operator : SJ/JU
Sample : J1174-11
Misc :
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Jan 28 00:42:51 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

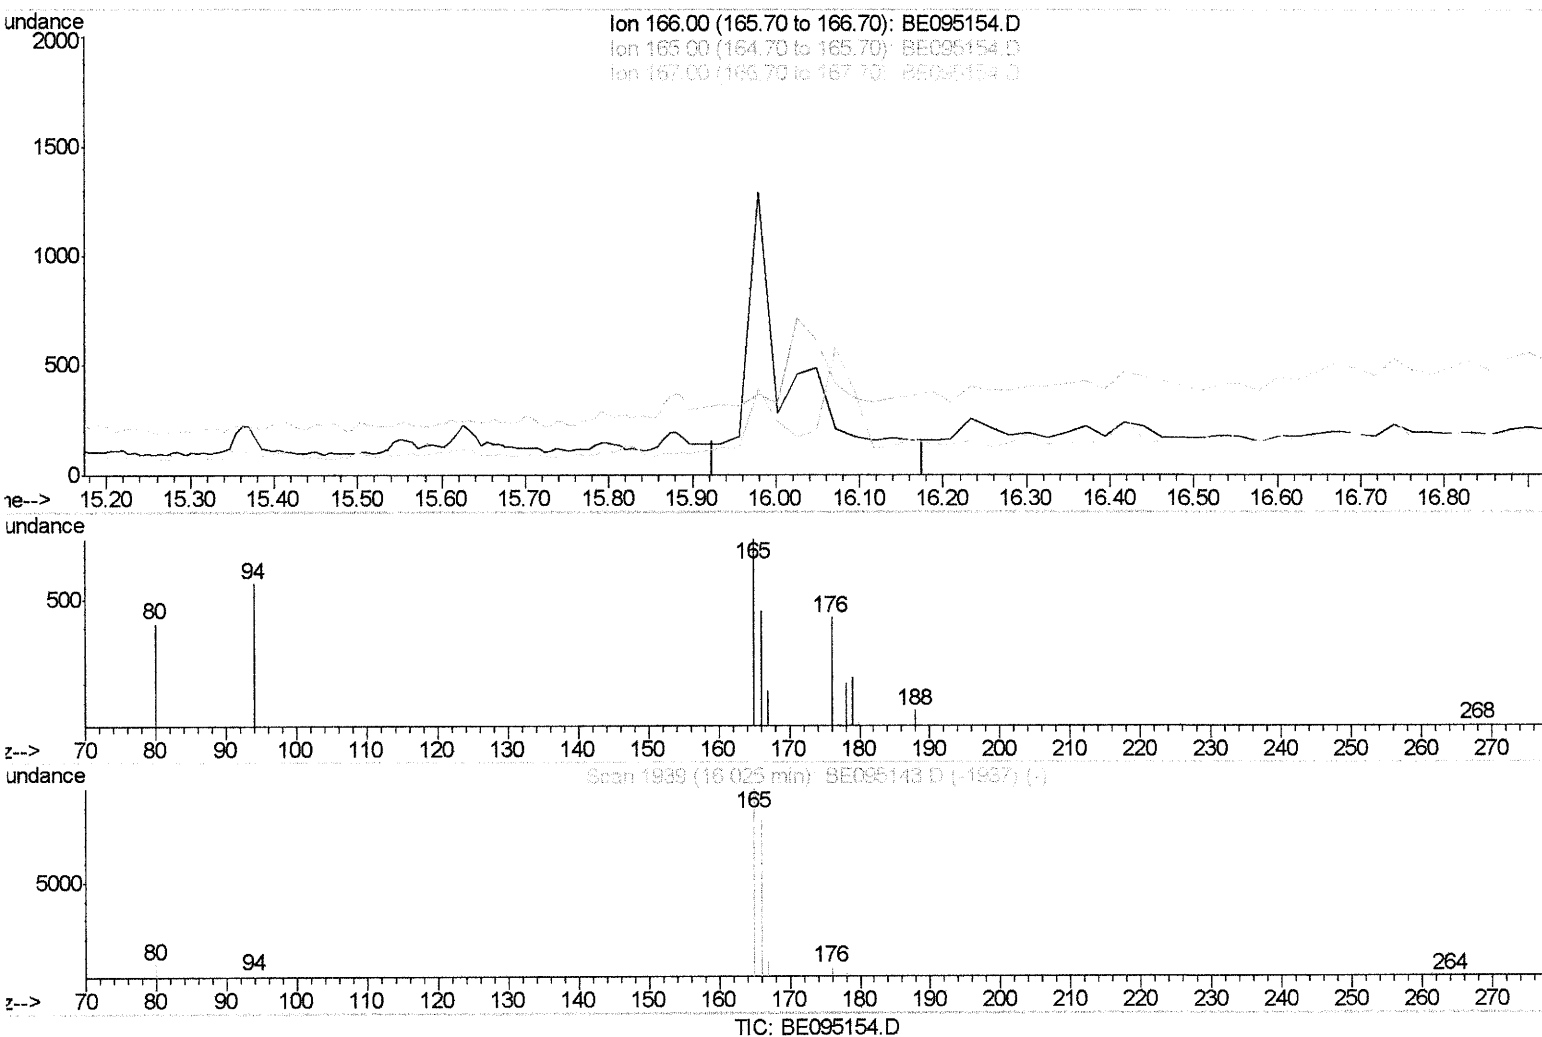

(9) Fluorene

16.025min (-16.025) 0.00ng/ul

response 0

Ion	Exp%	Act%
166.00	100	0.00
165.00	91.80	0.00#
167.00	18.30	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Instrument :
BNA_E
ClientSampled :
F6A46

Manual Integrations
APPROVED

Sohil
1/29/2018 6:34:23 PM

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
Data File : BE095154.D
Acq On : 27 Jan 2018 6:52
Operator : SJ/JU
Sample : J1174-11
Misc :
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Jan 28 00:42:51 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

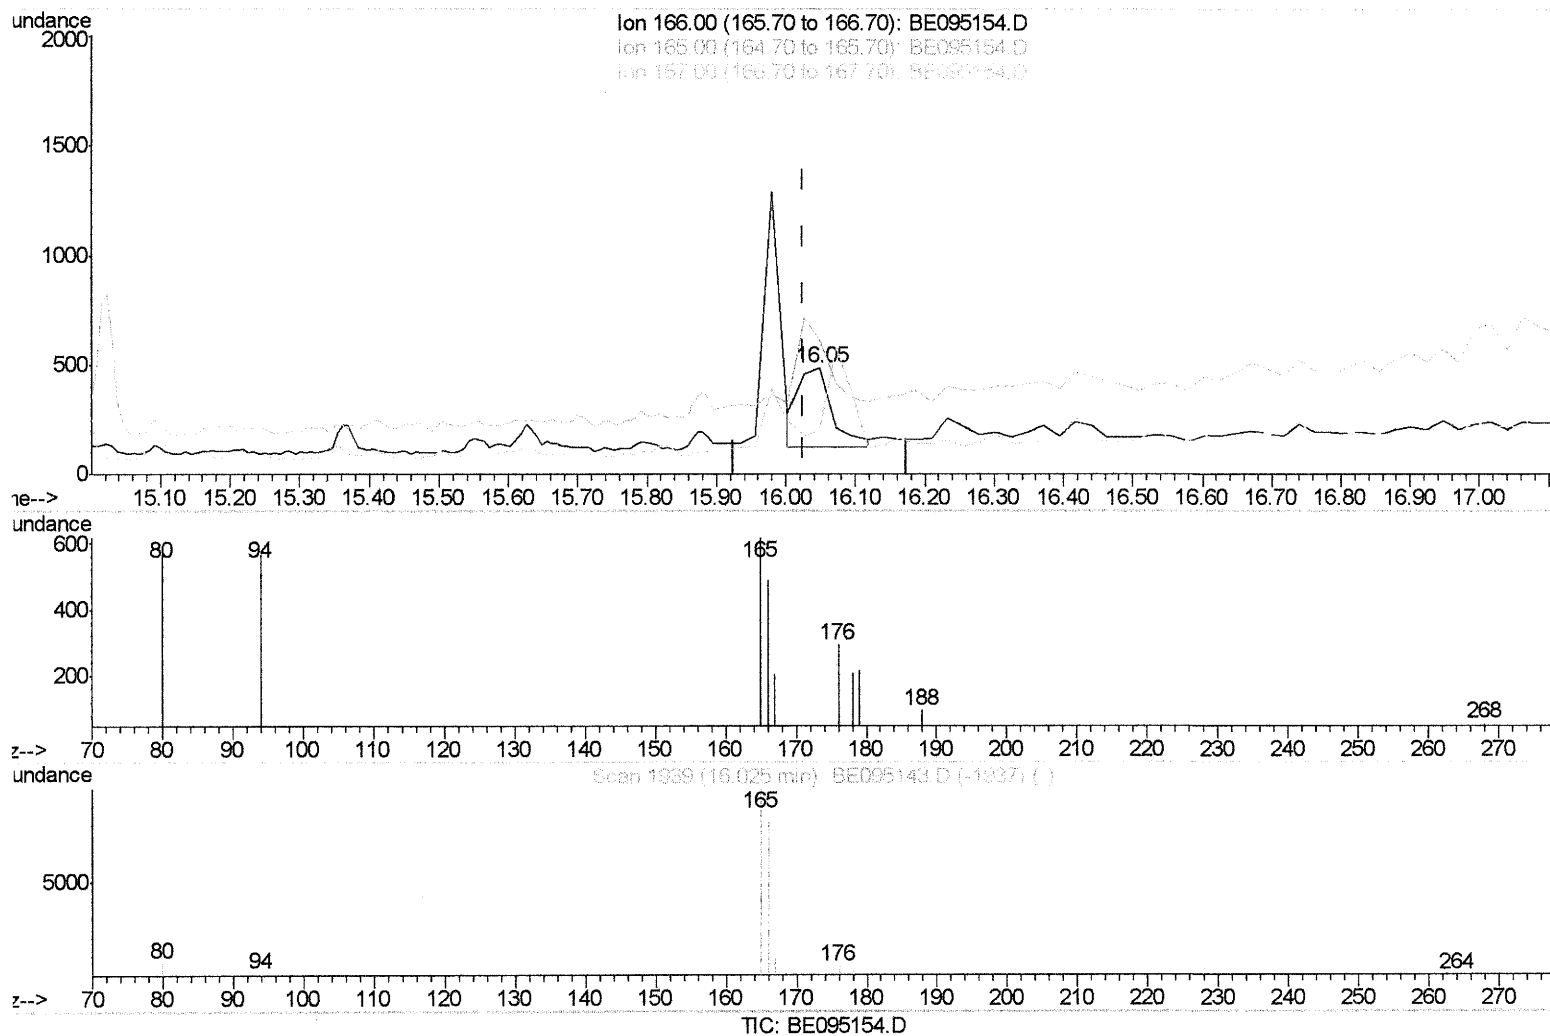

(9) Fluorene

16.048min (+0.023) 0.04ng/ul m

response 1211

Ion	Exp%	Act%
166.00	100	100
165.00	91.80	126.69#
167.00	18.30	41.89#
0.00	0.00	0.00

Handwritten signature/initials

Quantitation Report (Qedit)


Instrument :
BNA_E
ClientSampleId :
F6A46

Manual Integrations
APPROVED

Sohil
1/29/2018 6:34:23 PM

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
Data File : BE095154.D
Acq On : 27 Jan 2018 6:52
Operator : SJ/JU
Sample : J1174-11
Misc :
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Jan 28 00:42:51 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

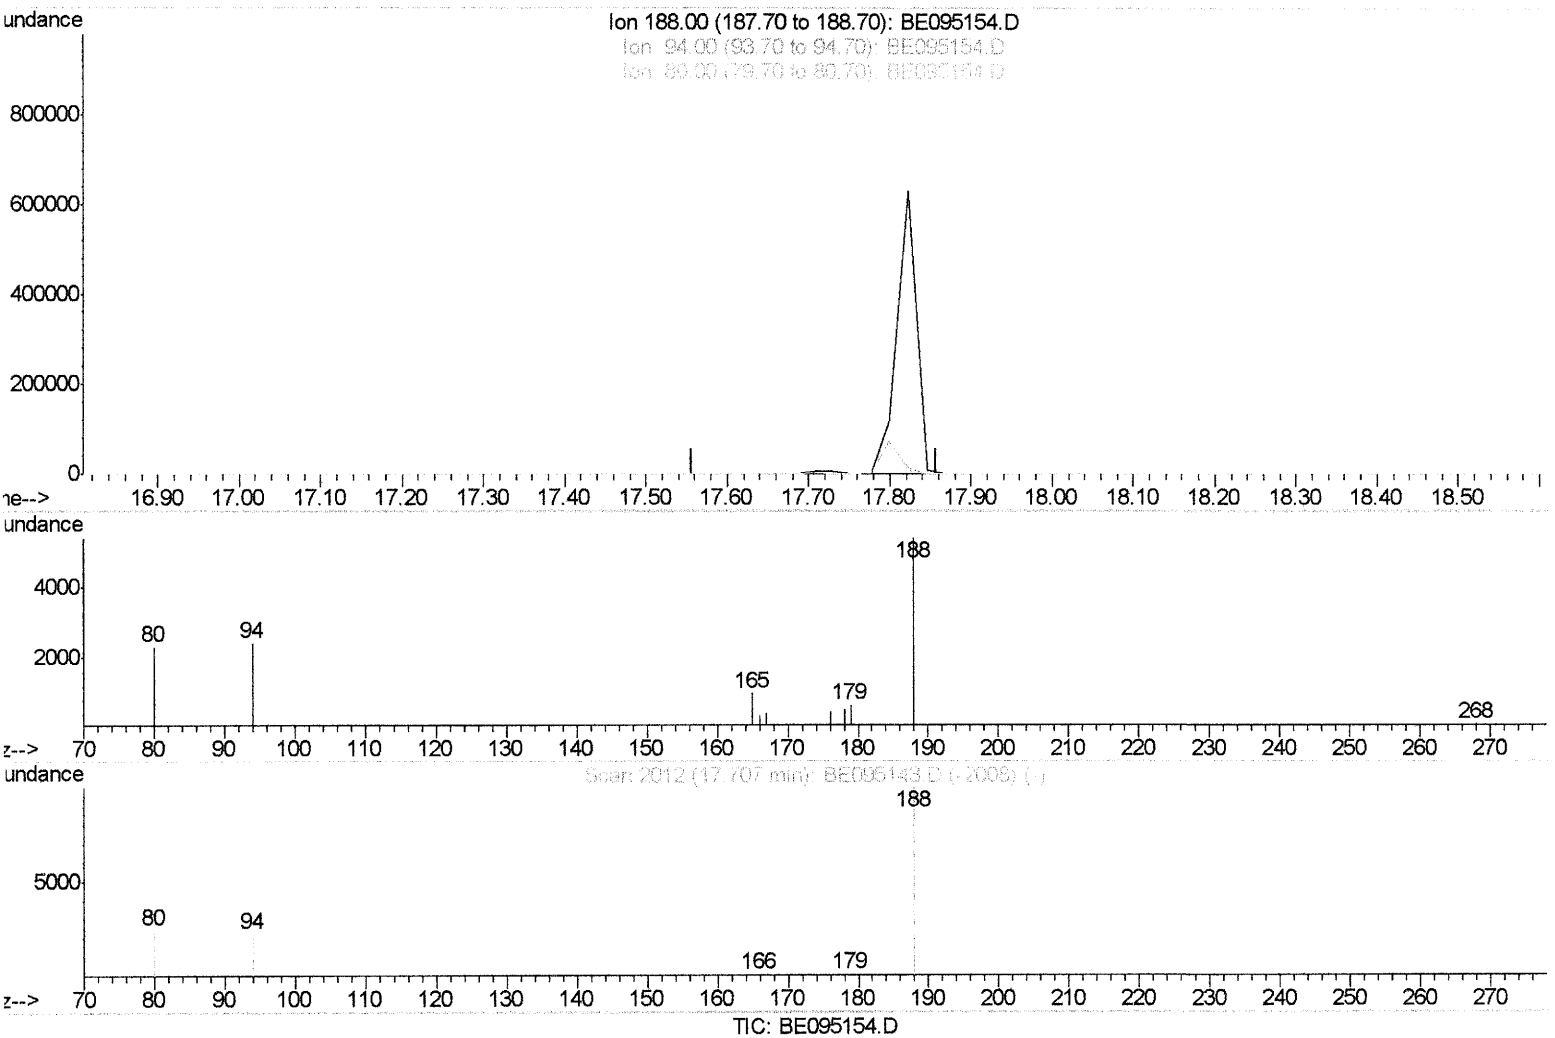

(10) Phenanthrene-d10 (I)

17.707min (-17.707) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Instrument :
BNA_E
ClientSampled :
F6A46

Manual Integrations
APPROVED

Sohil
1/29/2018 6:34:23 PM

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
Data File : BE095154.D
Acq On : 27 Jan 2018 6:52
Operator : SJ/JU
Sample : J1174-11
Misc :
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Jan 28 00:42:51 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

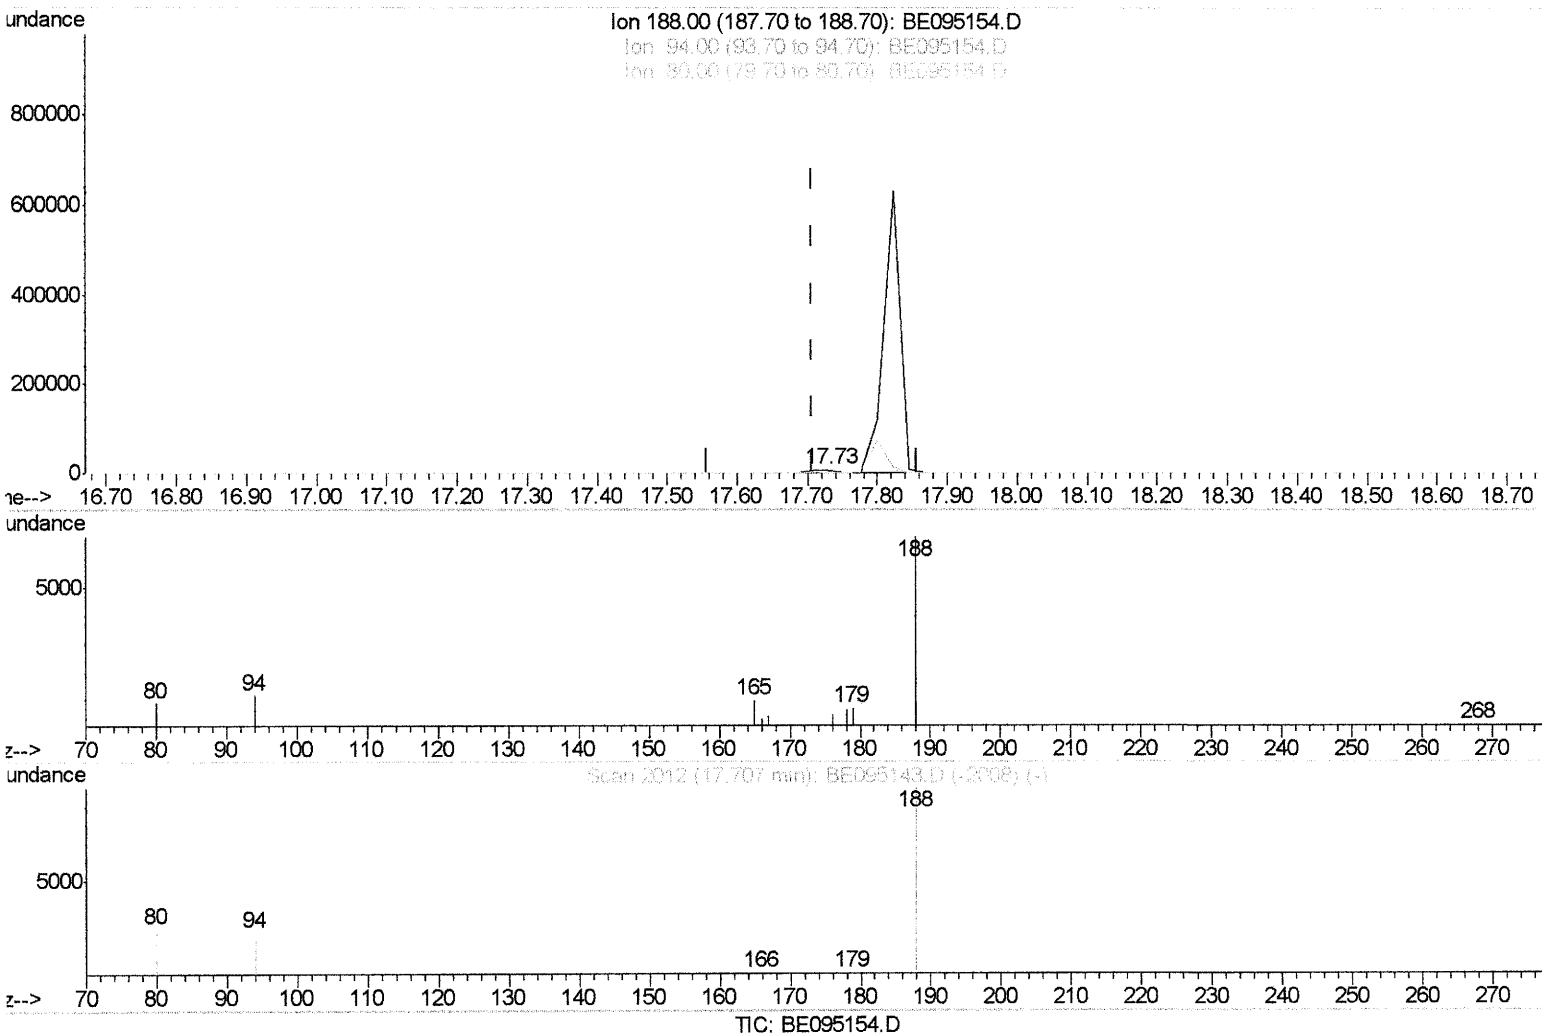

(10) Phenanthrene-d10 (I)

17.730min (+0.023) 0.40ng/ul m

response 17581

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	17.58#
80.00	11.80	13.48
0.00	0.00	0.00

Handwritten signature: JU-1/31/18

Quantitation Report (Qedit)


Instrument :
BNA_E
ClientSampled :
F6A46

Manual Integrations
APPROVED

Sohil
1/29/2018 6:34:23 PM

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
Data File : BE095154.D
Acq On : 27 Jan 2018 6:52
Operator : SJ/JU
Sample : J1174-11
Misc :
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Jan 28 00:43:58 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

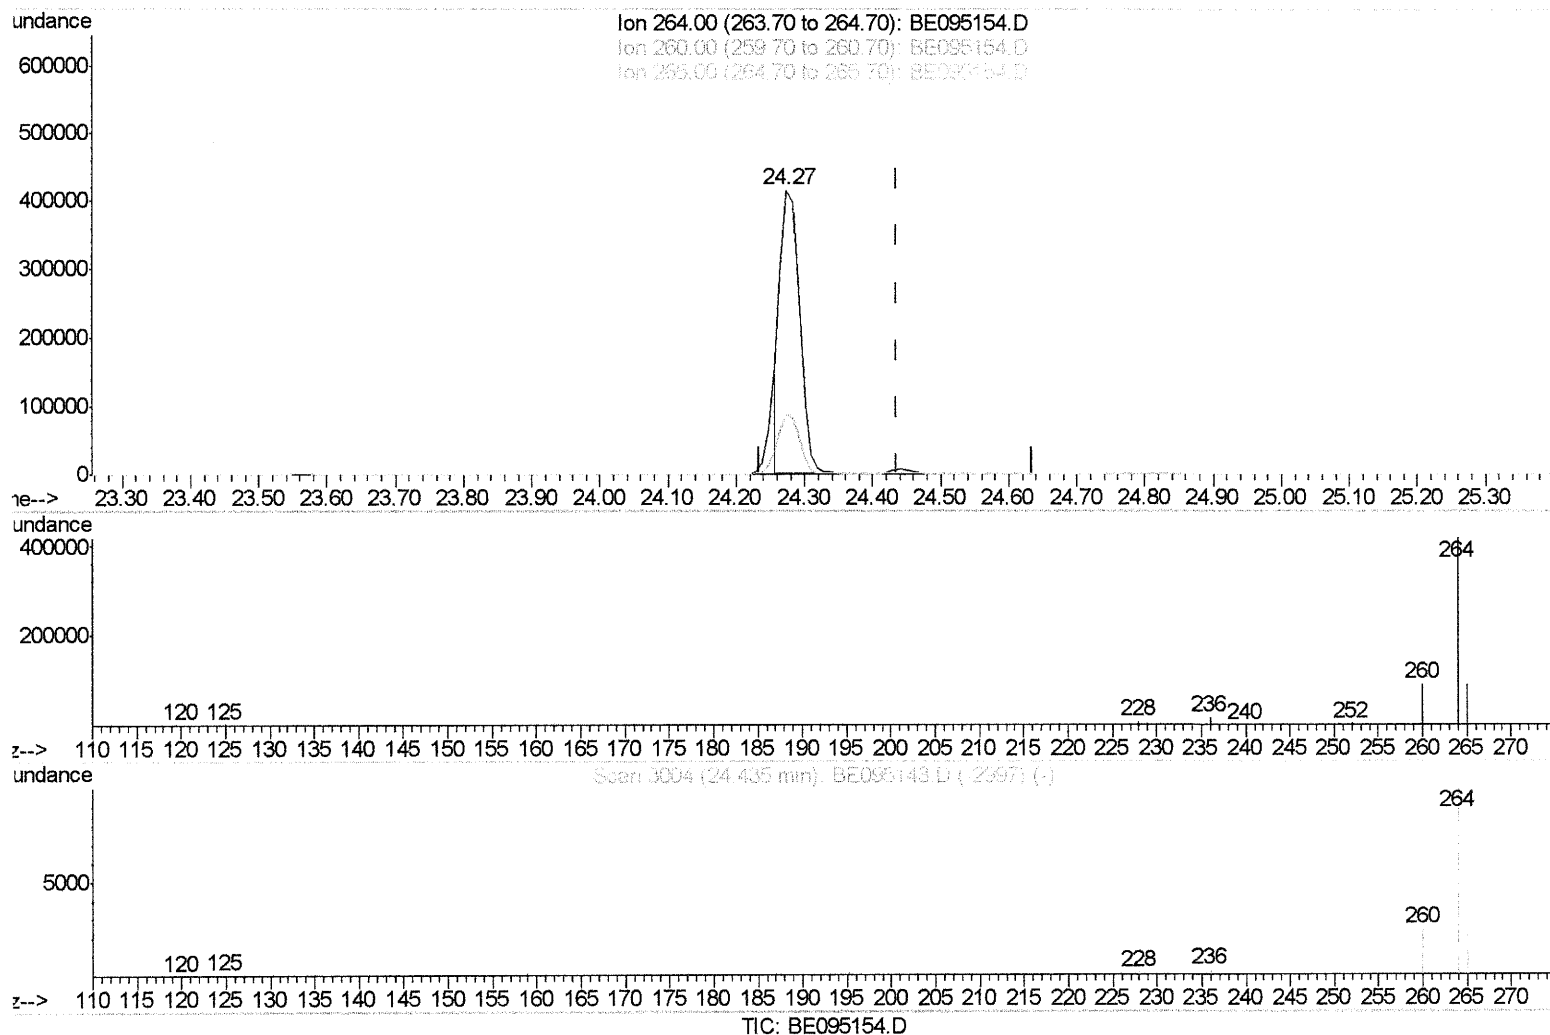

(20) Perylene-d12 (I)

24.274min (-0.161) 0.40ng/ul

response 807280

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.50#
265.00	103.50	21.37#
0.00	0.00	0.00

Quantitation Report (Qedit)

Instrument :

BNA_E

ClientSampled :

F6A46


Manual Integrations
APPROVED

Sohil

1/29/2018 6:34:23 PM

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
Data File : BE095154.D
Acq On : 27 Jan 2018 6:52
Operator : SJ/JU
Sample : J1174-11
Misc :
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Jan 28 00:43:58 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

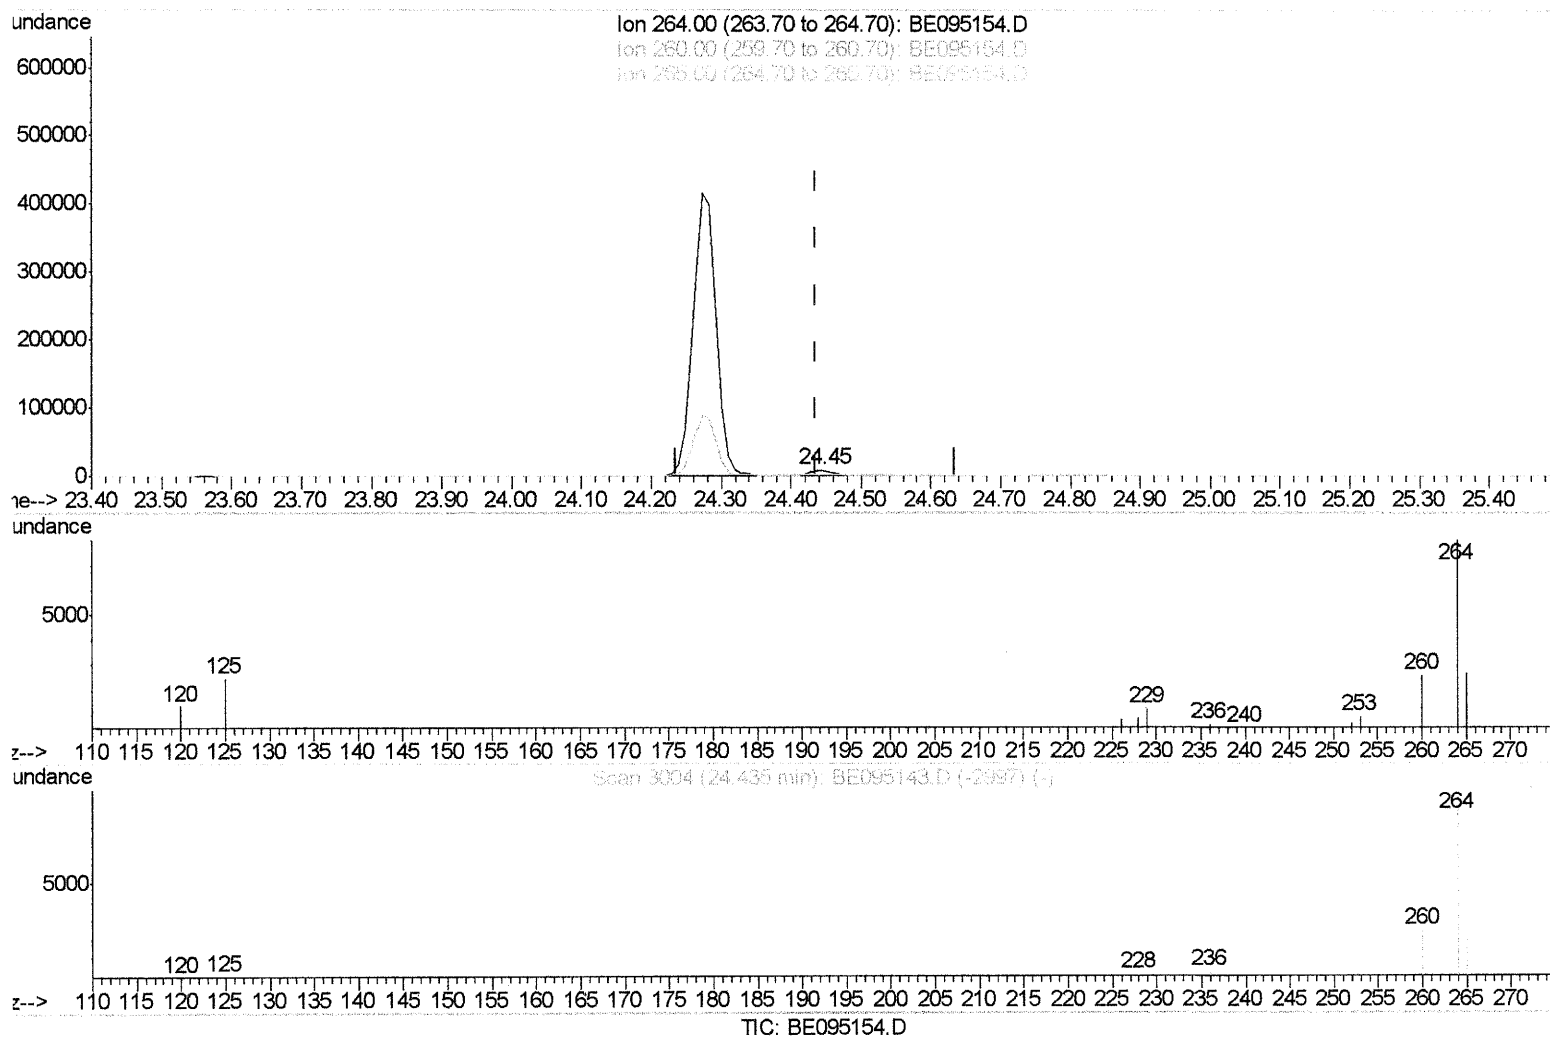

(20) Perylene-d12 (I)

24.445min (+0.010) 0.40ng/ul m

response 15392

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	31.76
265.00	103.50	32.73#
0.00	0.00	0.00

see 1/31/18

Quantitation Report (Qedit)




Instrument :
BNA_E
ClientSampled :
F6A46

Manual Integrations
APPROVED

Sohil
1/29/2018 6:34:23 PM

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
Data File : BE095154.D
Acq On : 27 Jan 2018 6:52
Operator : SJ/JU
Sample : J1174-11
Misc :
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Jan 28 00:44:46 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

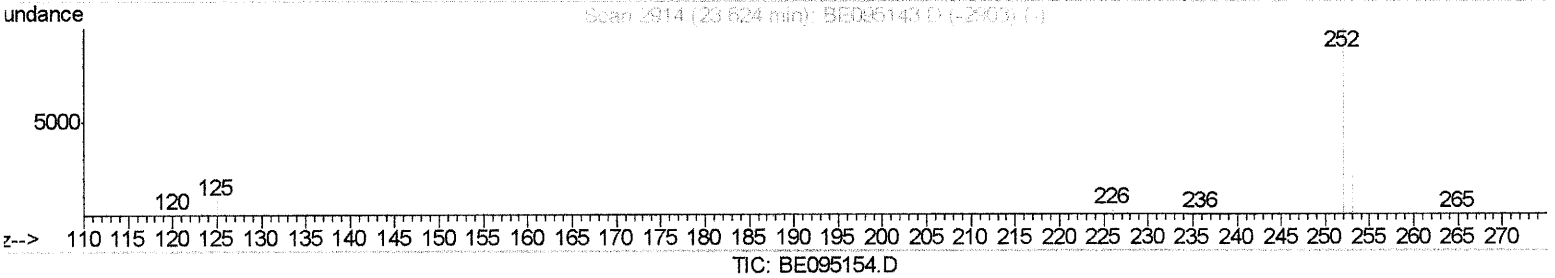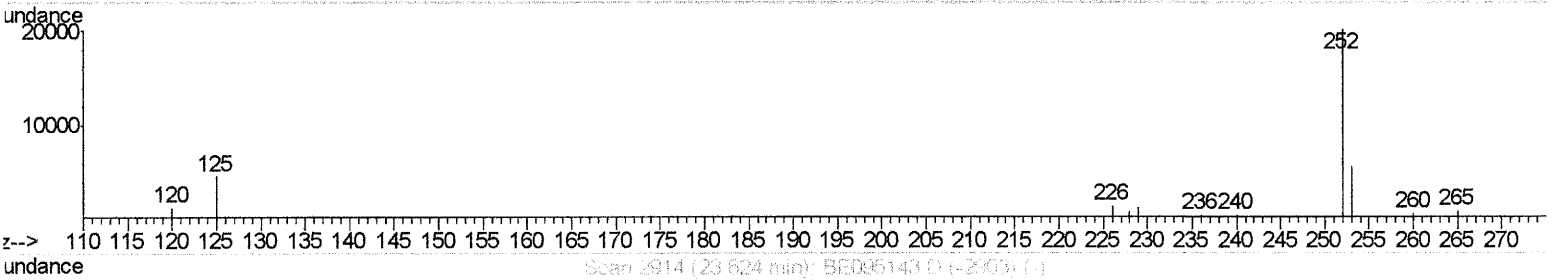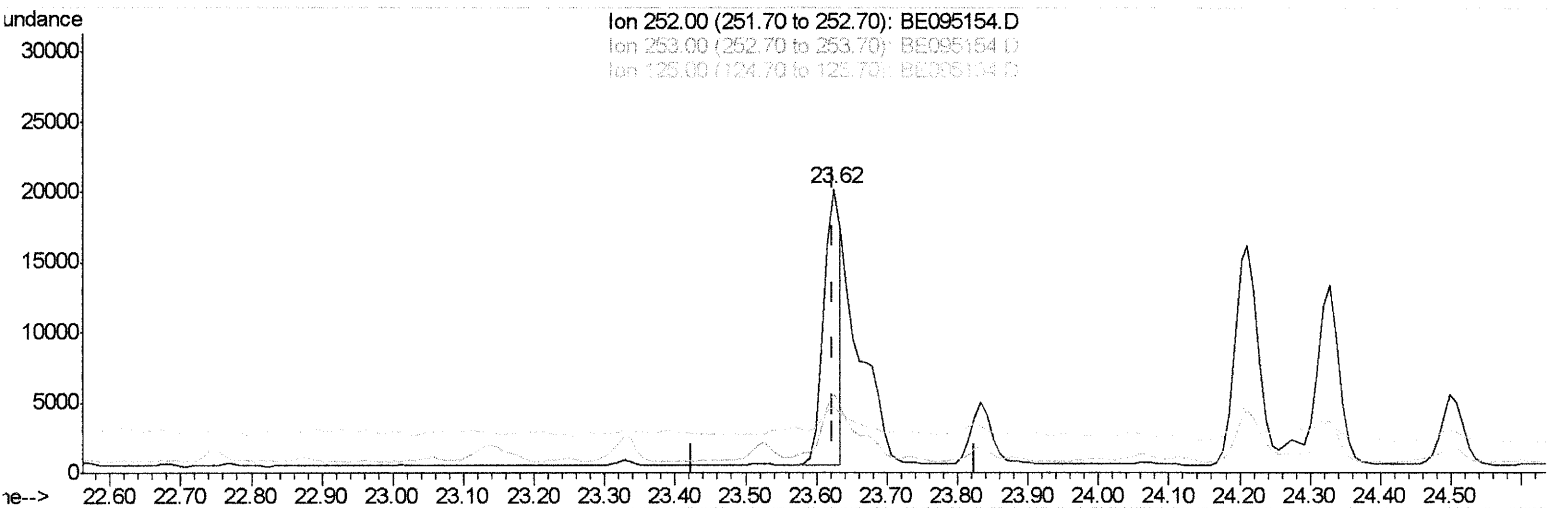

(21) Benzo(b)fluoranthene

23.625min (+0.001) 0.63ng/ul

response 34212

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	28.04
125.00	17.50	22.99
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
 Data File : BE095154.D
 Acq On : 27 Jan 2018 6:52
 Operator : SJ/JU
 Sample : J1174-11
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6A46

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:34:23 PM

Quant Time: Jan 28 00:44:46 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 27 03:18:43 2018
 Response via : Initial Calibration

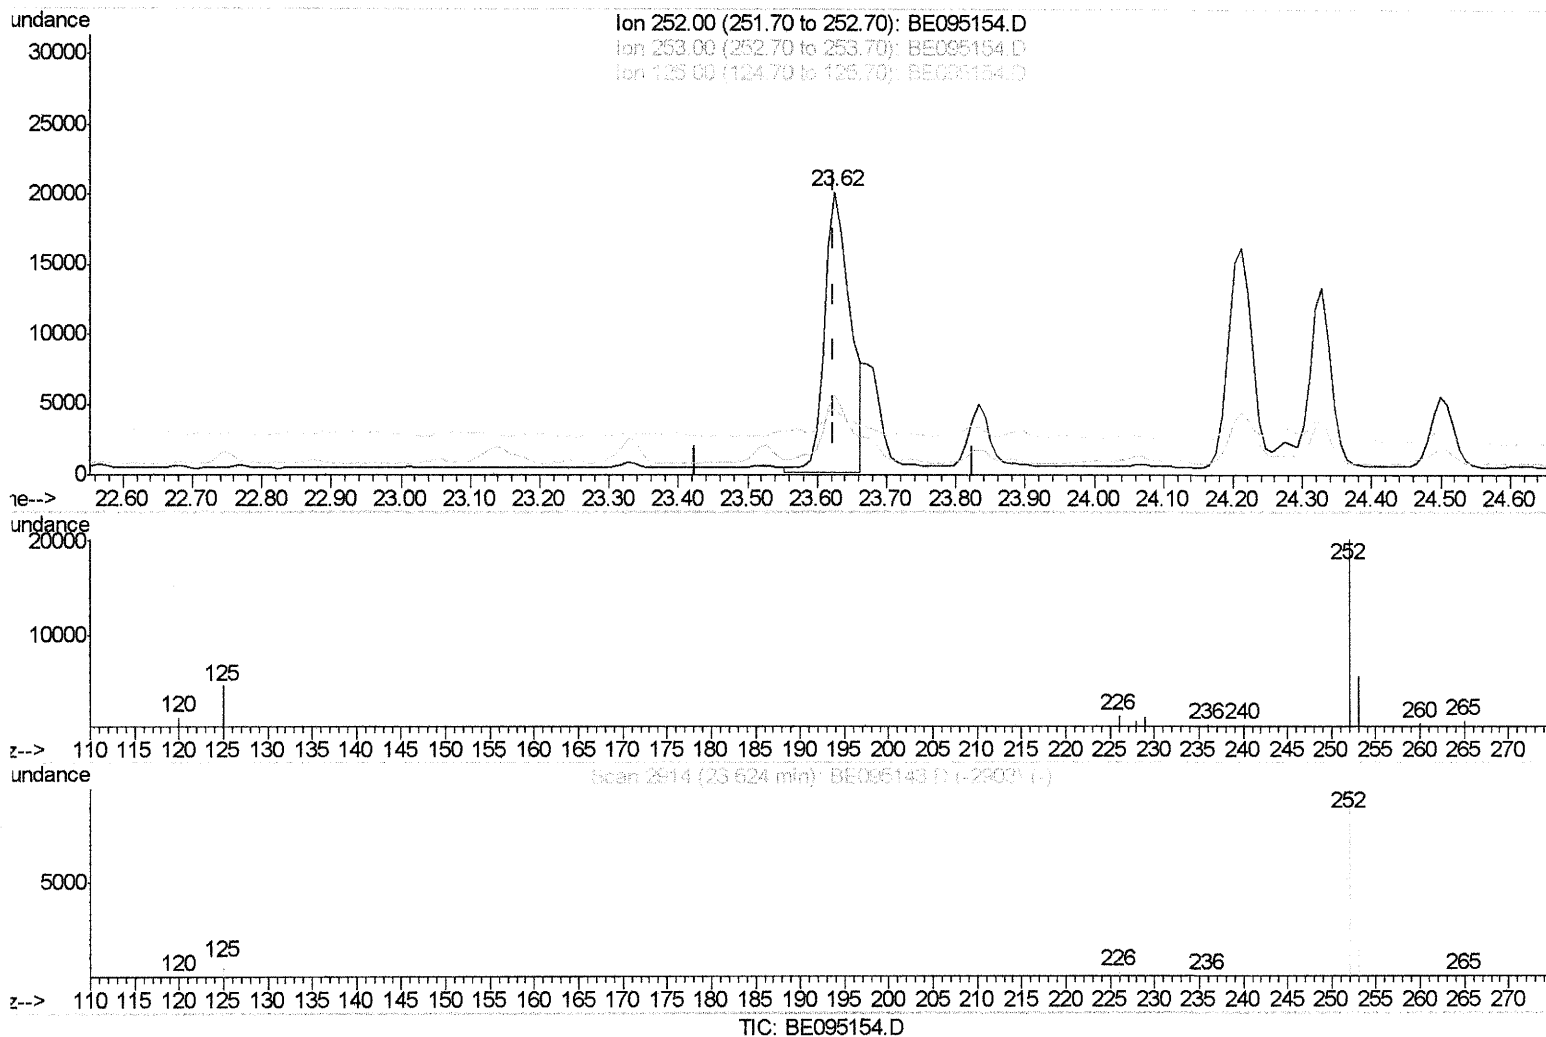

(21) Benzo(b)fluoranthene

23.625min (+0.001) 0.96ng/ul m

response 52316

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	28.04
125.00	17.50	22.99
0.00	0.00	0.00

SJ 1/31/18

Quantitation Report (Qedit)


Instrument :
BNA_E
ClientSampled :
F6A46

Manual Integrations
APPROVED

Sohil
1/29/2018 6:34:23 PM

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
Data File : BE095154.D
Acq On : 27 Jan 2018 6:52
Operator : SJ/JU
Sample : J1174-11
Misc :
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Jan 28 00:44:46 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

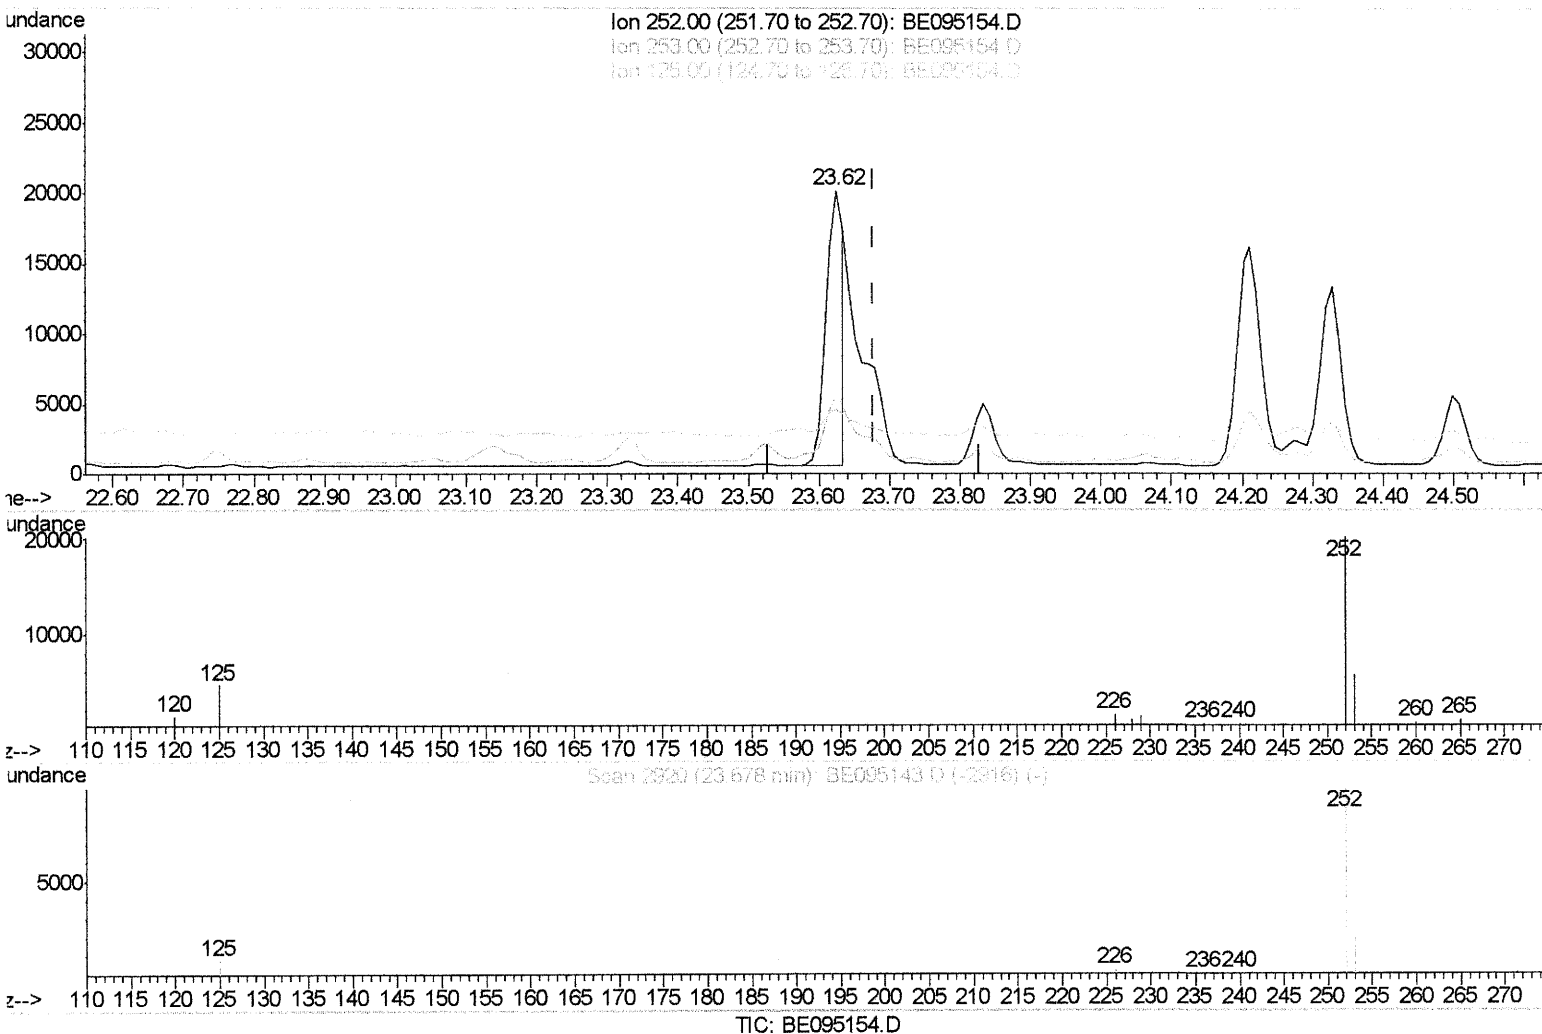

(22) Benzo(k)fluoranthene

23.625min (-0.053) 0.69ng/ui

response 34212

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	28.04
125.00	17.10	22.99#
0.00	0.00	0.00

Quantitation Report (Qedit)




Instrument :
BNA_E
ClientSampleId :
F6A46

Manual Integrations
APPROVED

Sohil
1/29/2018 6:34:23 PM

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
Data File : BE095154.D
Acq On : 27 Jan 2018 6:52
Operator : SJ/JU
Sample : J1174-11
Misc :
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Jan 28 00:44:46 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

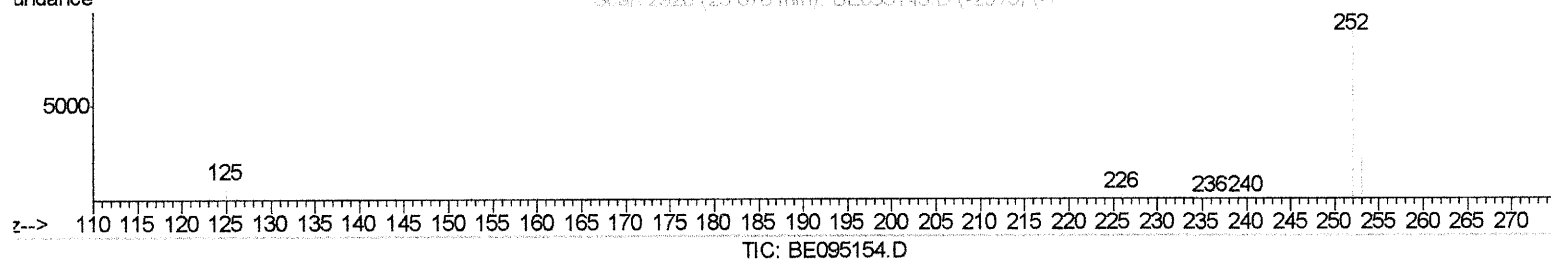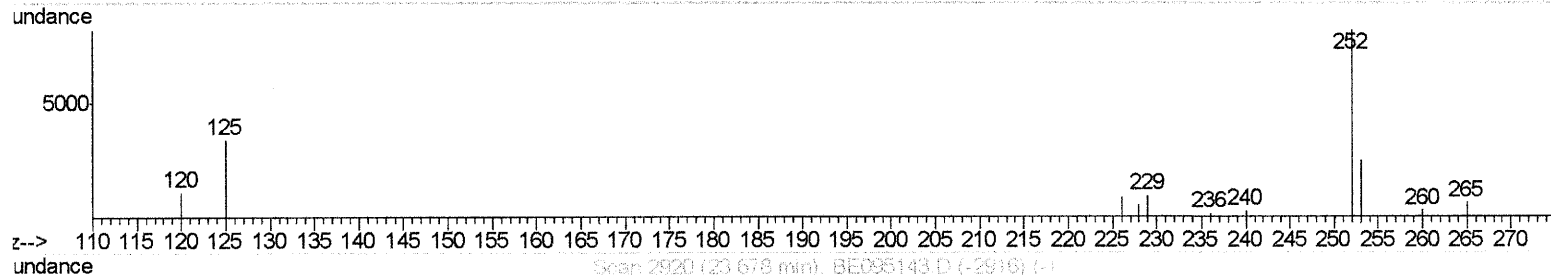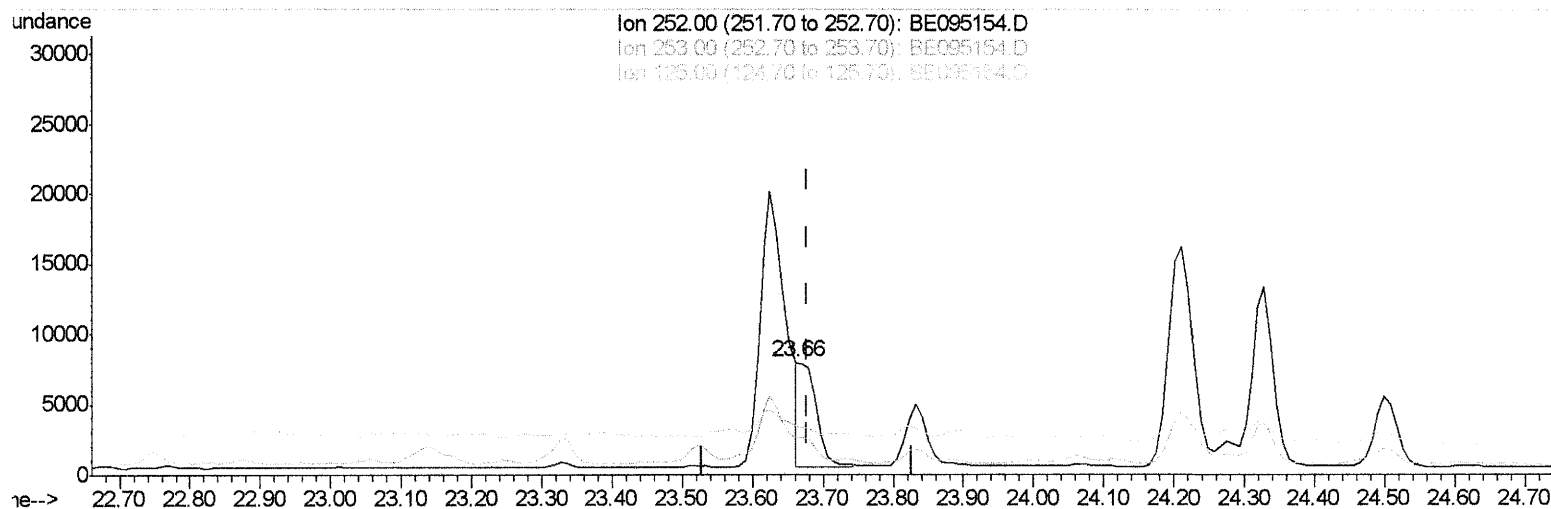

(22) Benzo(k)fluoranthene

23.661min (-0.017) 0.25ng/ul m

response 12363

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	33.22
125.00	17.10	43.90#
0.00	0.00	0.00

201/31/18

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
 Data File : BE095154.D
 Acq On : 27 Jan 2018 6:52
 Operator : SJ/JU
 Sample : J1174-11
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6A46

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:34:23 PM

Quant Time: Jan 28 00:44:46 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 27 03:18:43 2018
 Response via : Initial Calibration

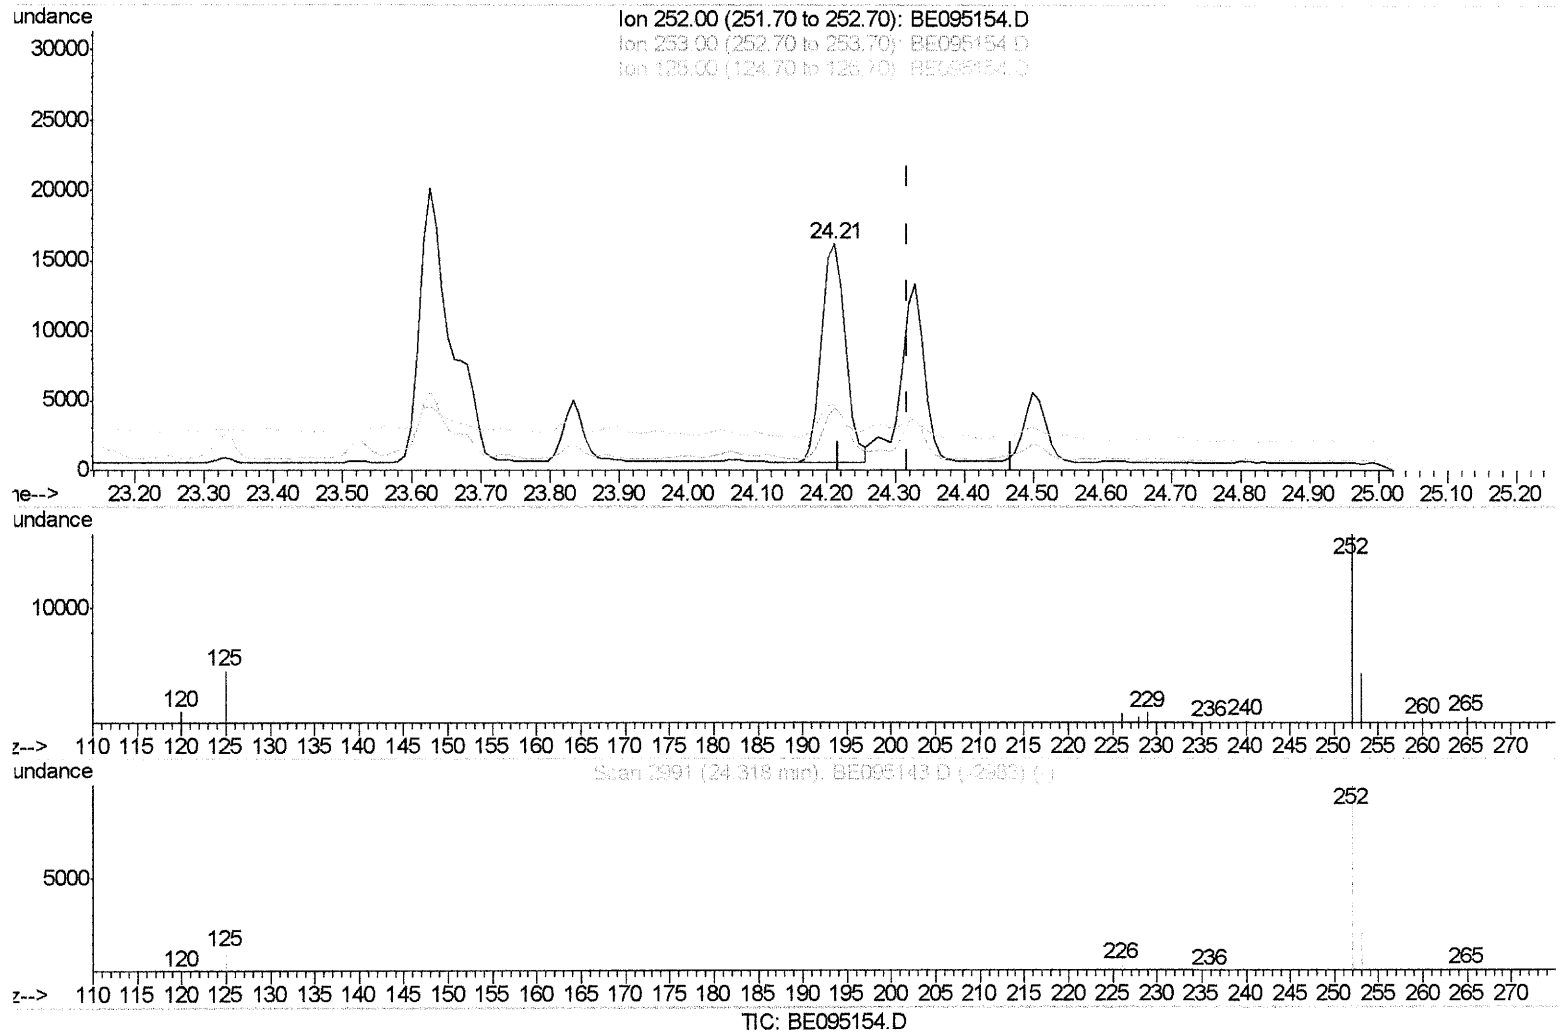

(23) Benzo(a)pyrene (C)

24.211min (-0.107) 0.78ng/ul

response 37902

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	27.54#
125.00	22.60	29.05#
0.00	0.00	0.00

Quantitation Report (Qedit)


Instrument :
BNA_E
ClientSampled :
F6A46

Manual Integrations
APPROVED

Sohil
1/29/2018 6:34:23 PM

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
Data File : BE095154.D
Acq On : 27 Jan 2018 6:52
Operator : SJ/JU
Sample : J1174-11
Misc :
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Jan 28 00:44:46 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

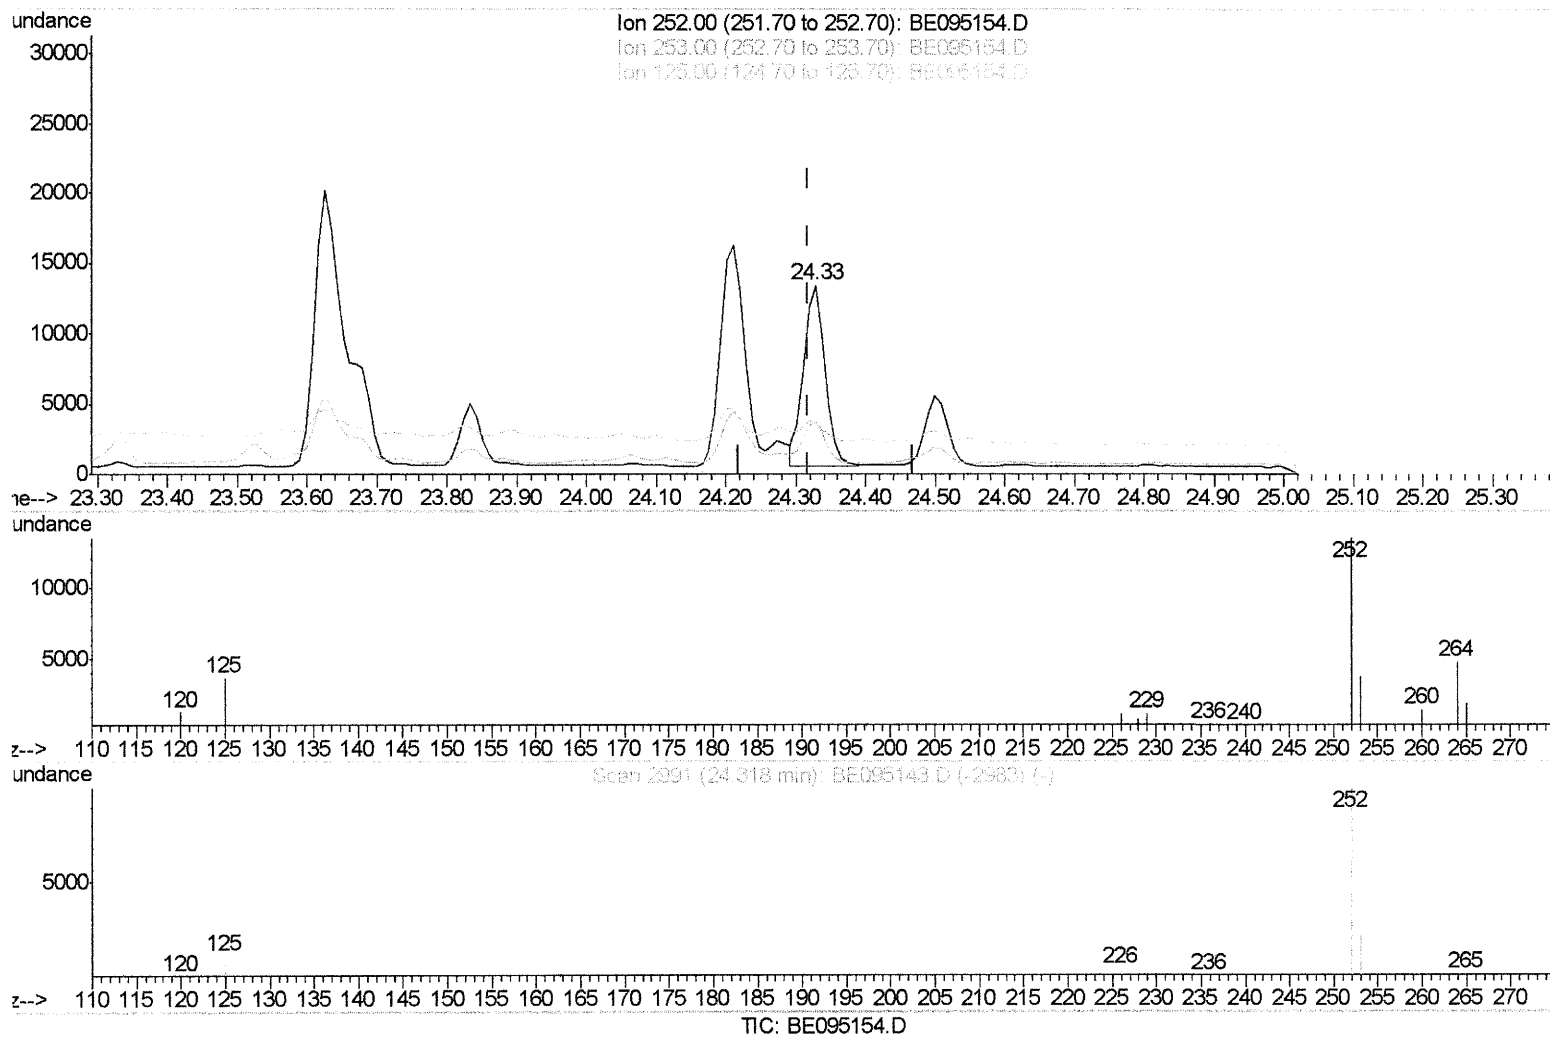

(23) Benzo(a)pyrene (C)

24.328min (+0.010) 0.56ng/ul m

response 27057

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	28.12#
125.00	22.60	27.71#
0.00	0.00	0.00

just 1/31/18

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
 Data File : BE095154.D
 Acq On : 27 Jan 2018 6:52
 Operator : SJ/JU
 Sample : J1174-11
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6A46

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:34:23 PM

Quant Time: Jan 28 00:44:46 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 27 03:18:43 2018
 Response via : Initial Calibration

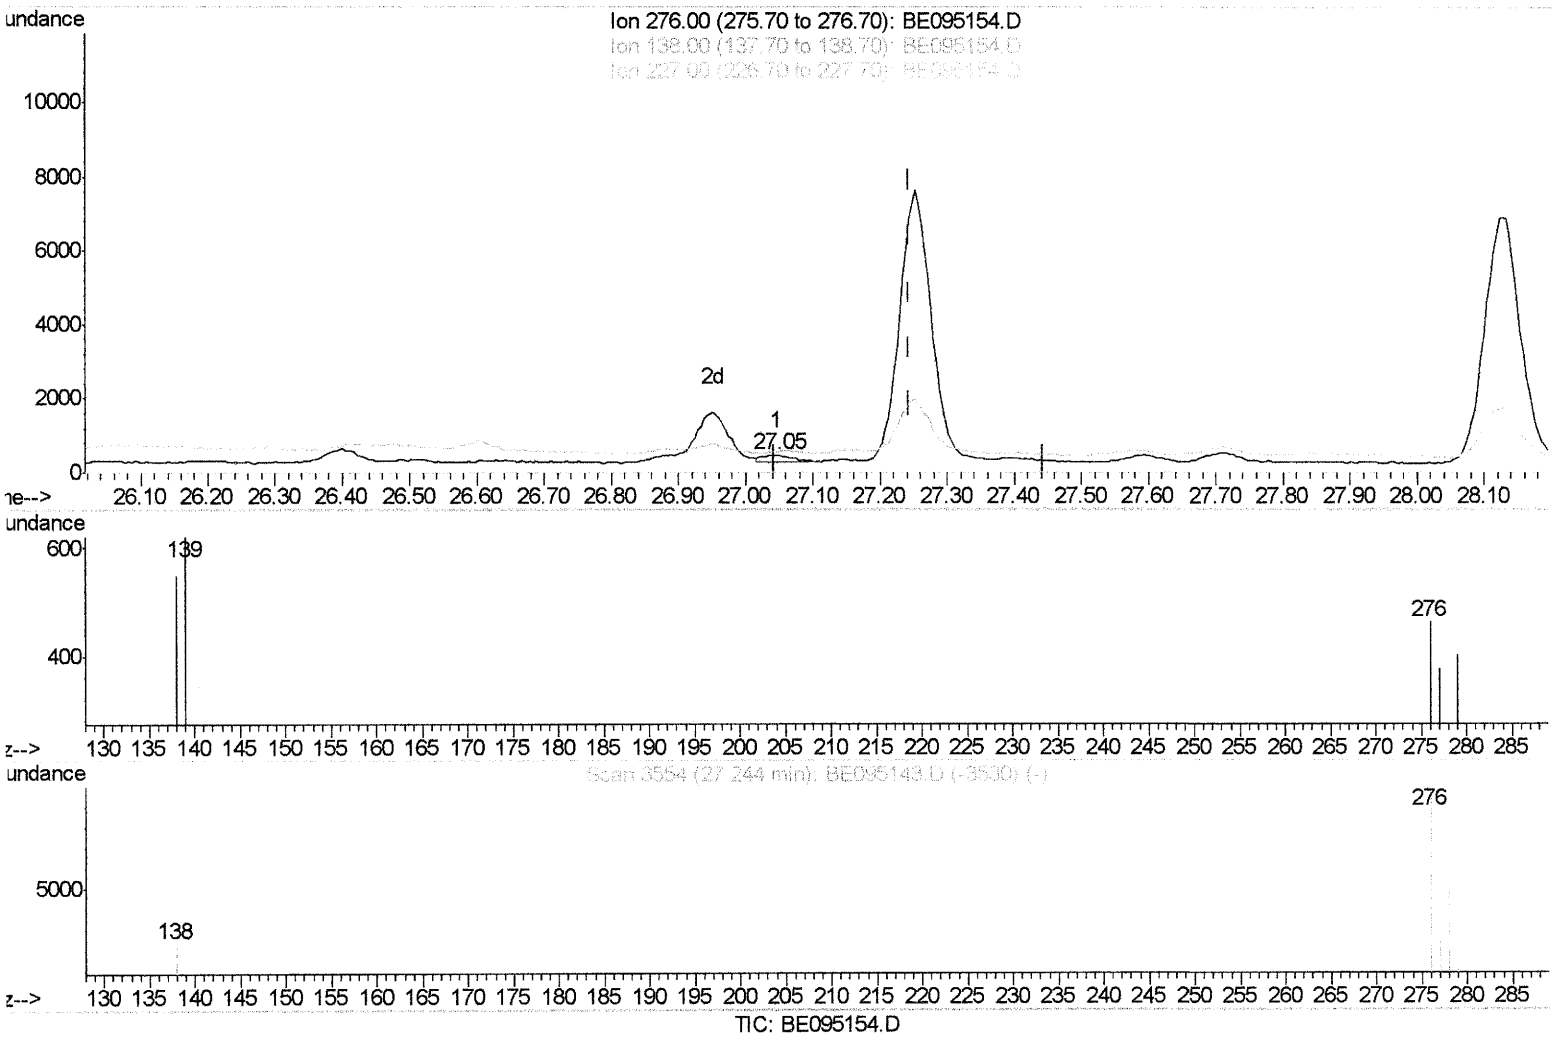

(24) Indeno(1,2,3-cd)pyrene

27.047min (-0.197) 0.01ng/ui

response 482

Ion	Exp%	Act%
276.00	100	100
138.00	35.00	52.28#
227.00	10.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
 Data File : BE095154.D
 Acq On : 27 Jan 2018 6:52
 Operator : SJ/JU
 Sample : J1174-11
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6A46

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:34:23 PM

Quant Time: Jan 28 00:44:46 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 27 03:18:43 2018
 Response via : Initial Calibration

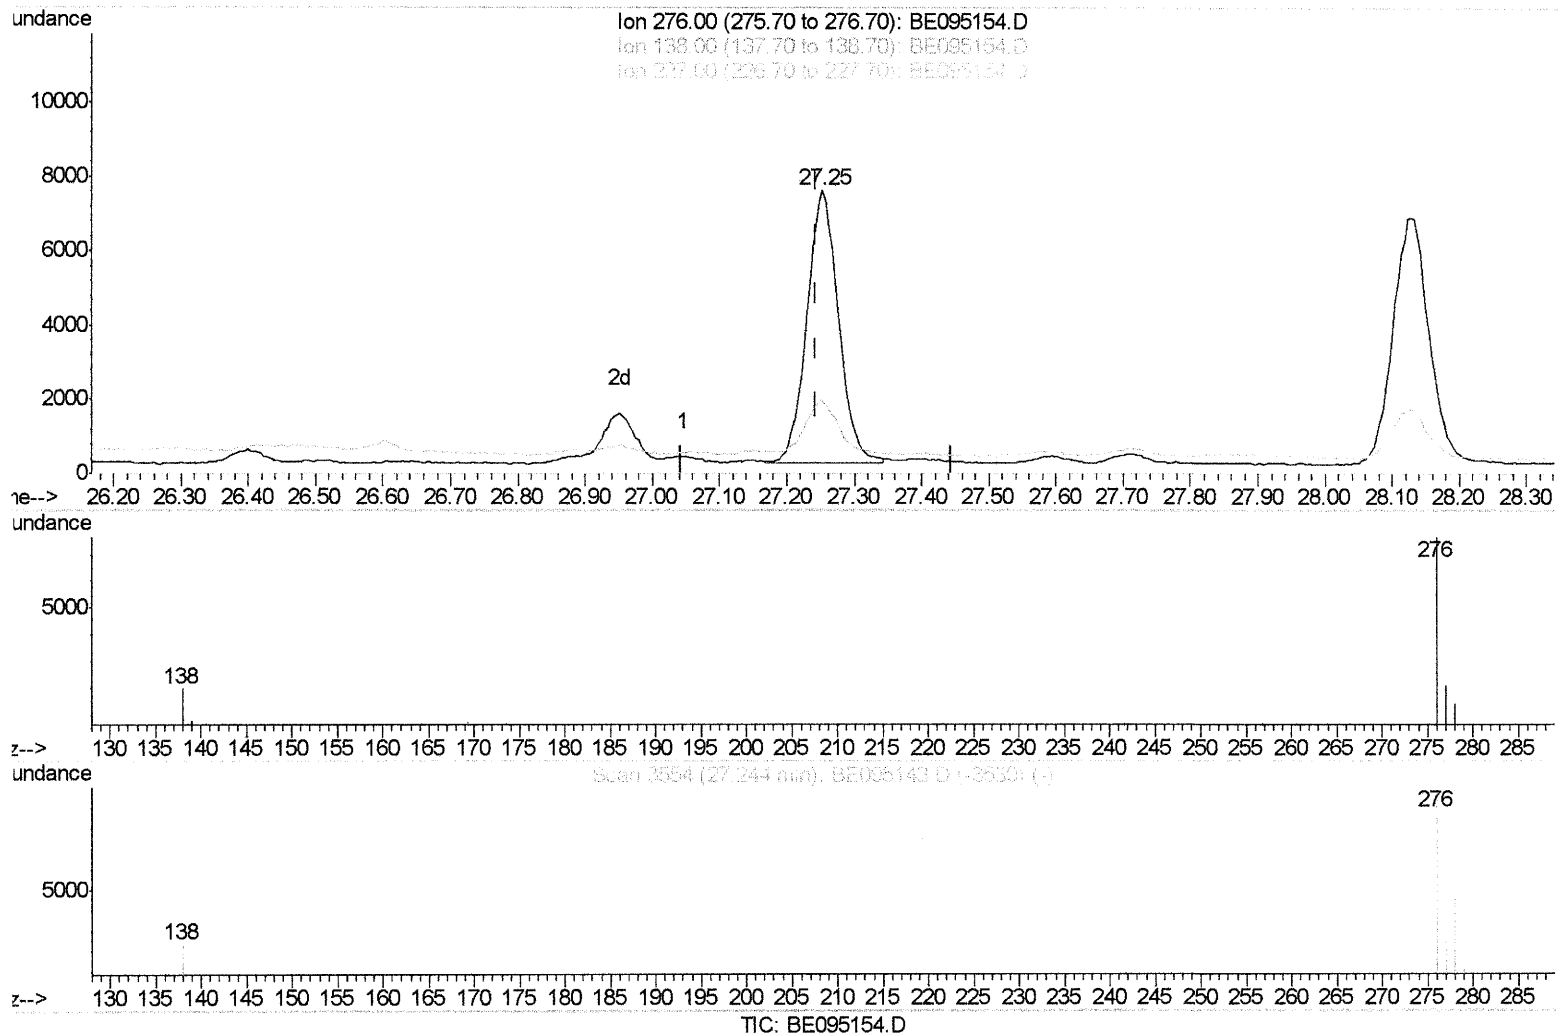

(24) Indeno(1,2,3-cd)pyrene

27.252min (+0.008) 0.45ng/ul m

response 24164

Ion	Exp%	Act%
276.00	100	100
138.00	35.00	1.04#
227.00	10.00	0.00#
0.00	0.00	0.00

27.01/31/18

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
 Data File : BE095154.D
 Acq On : 27 Jan 2018 6:52
 Operator : SJ/JU
 Sample : J1174-11
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6A46

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:34:23 PM

Quant Time: Jan 28 00:44:46 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 27 03:18:43 2018
 Response via : Initial Calibration

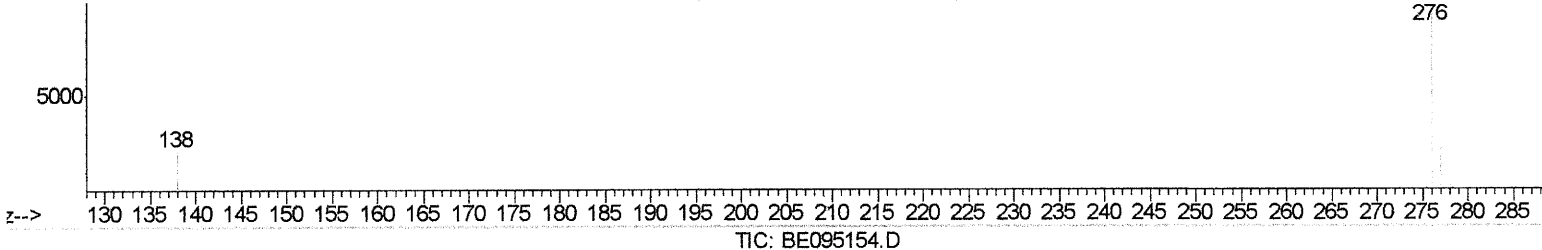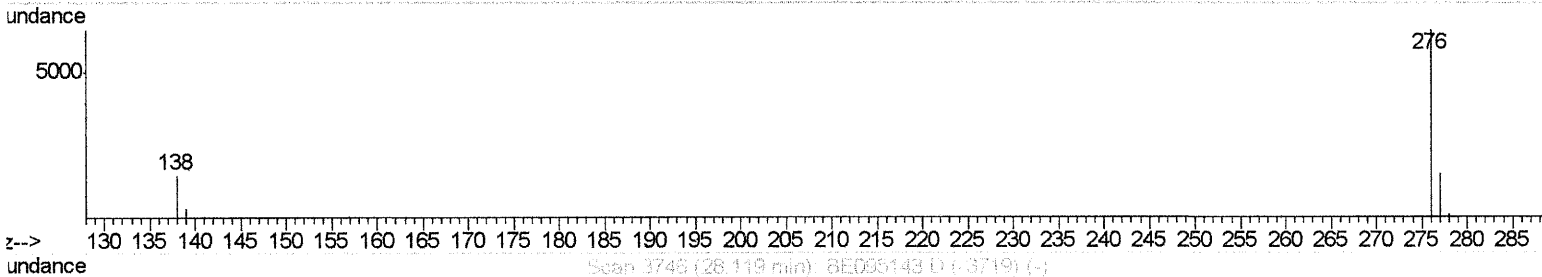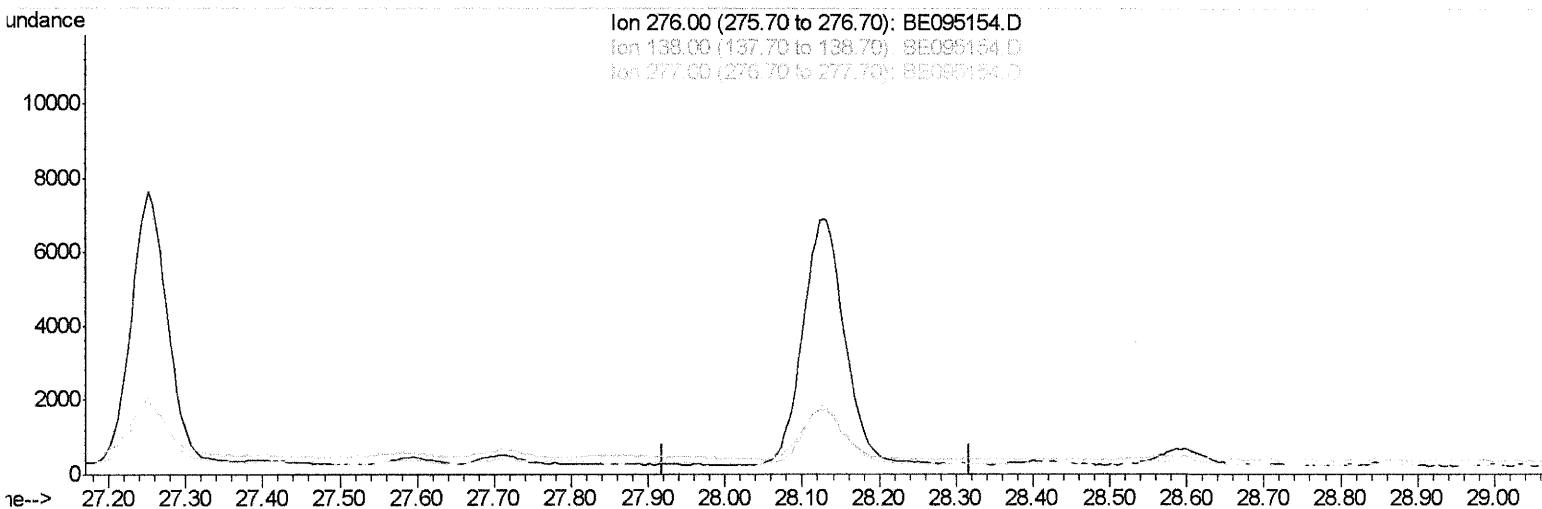

(26) Benzo(g,h,i)perylene

28.119min (-28.119) 0.00ng/ul

response 0

Ion	Exp%	Act%
276.00	100	0.00
138.00	27.30	0.00#
277.00	25.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012618\
 Data File : BE095154.D
 Acq On : 27 Jan 2018 6:52
 Operator : SJ/JU
 Sample : J1174-11
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6A46

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:34:23 PM

Quant Time: Jan 28 00:44:46 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 27 03:18:43 2018
 Response via : Initial Calibration

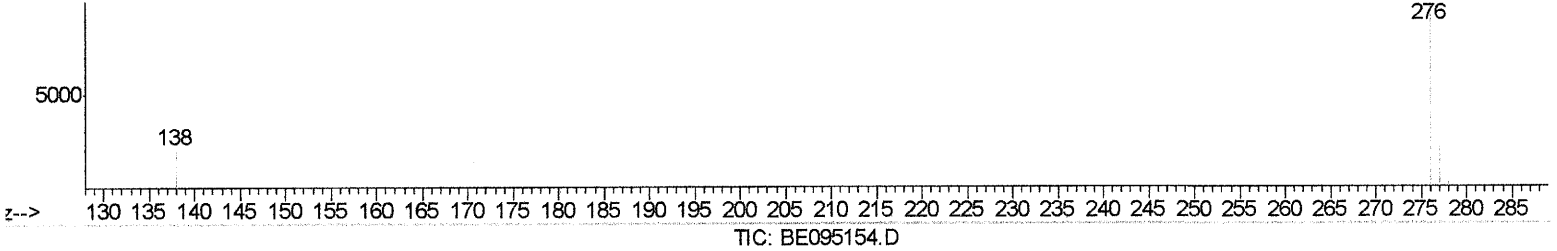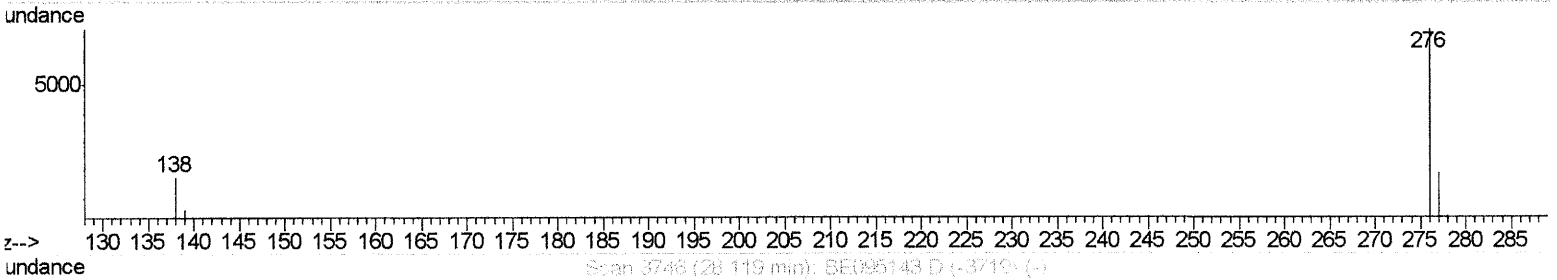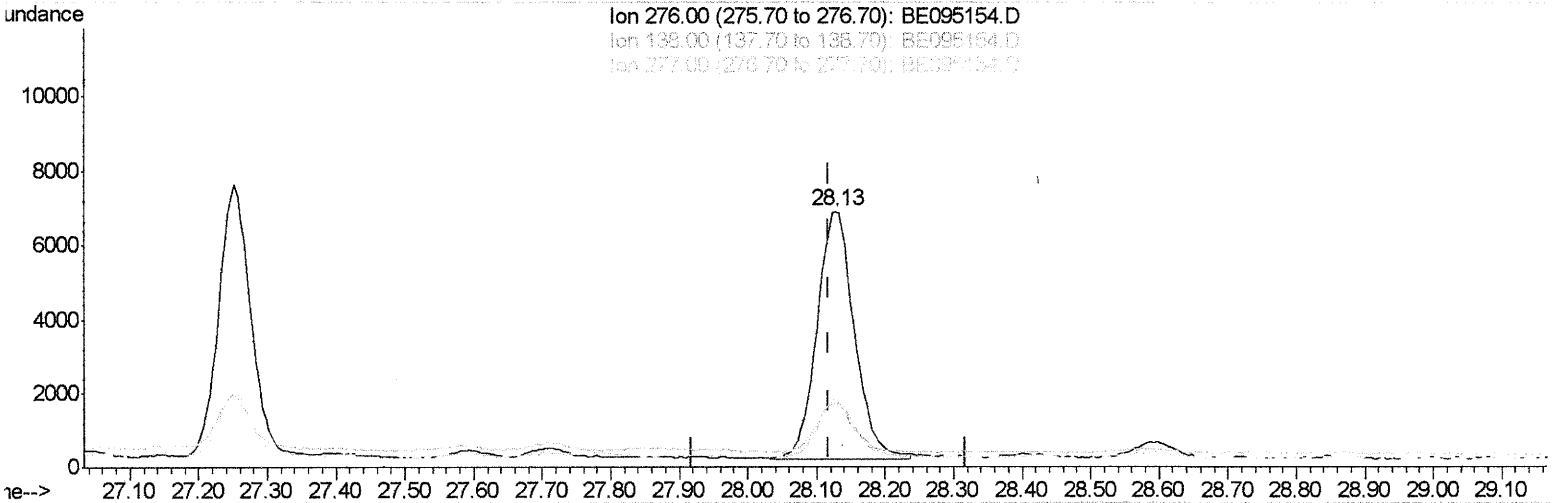

(26) Benzo(g,h,i)perylene

28.127min (+0.008) 0.57ng/ul m

response 25614

Ion	Exp%	Act%
276.00	100	100
138.00	27.30	25.35
277.00	25.60	26.92
0.00	0.00	0.00

28.127min

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE012618\
 Data File : BE095154.D
 Acq On : 27 Jan 2018 6:52
 Operator : SJ/JU
 Sample : J1174-11
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6A46

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:34:23 PM

Quant Time: Jan 28 00:47:37 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 27 03:18:43 2018
 Response via : Initial Calibration

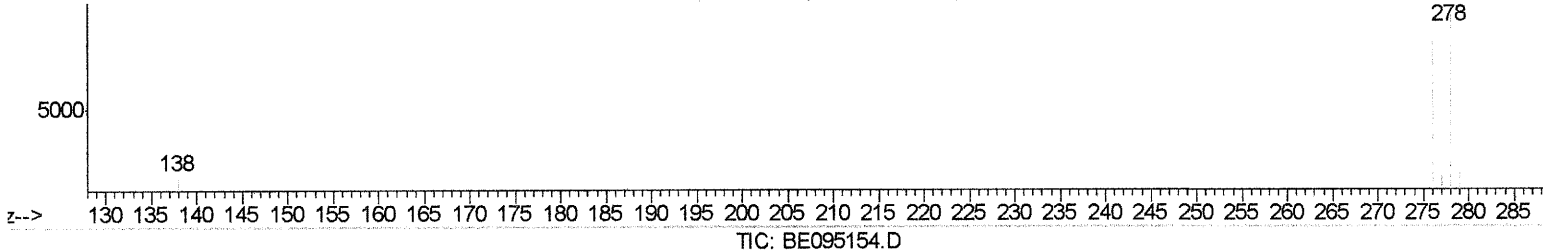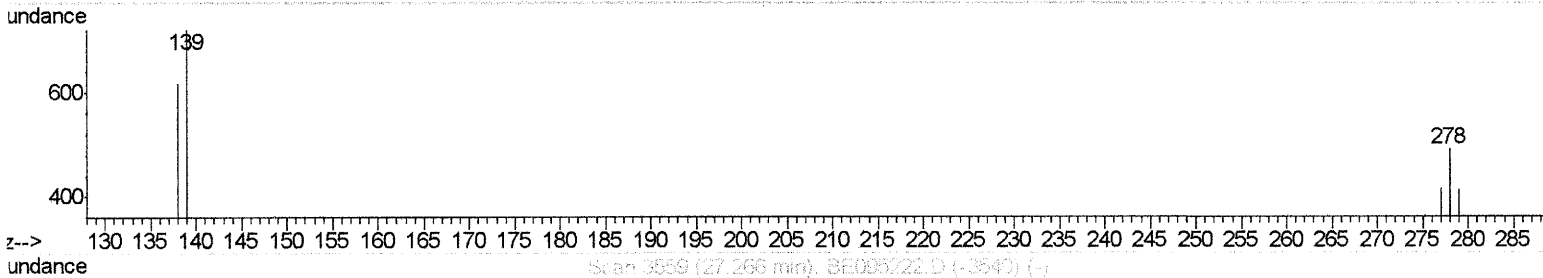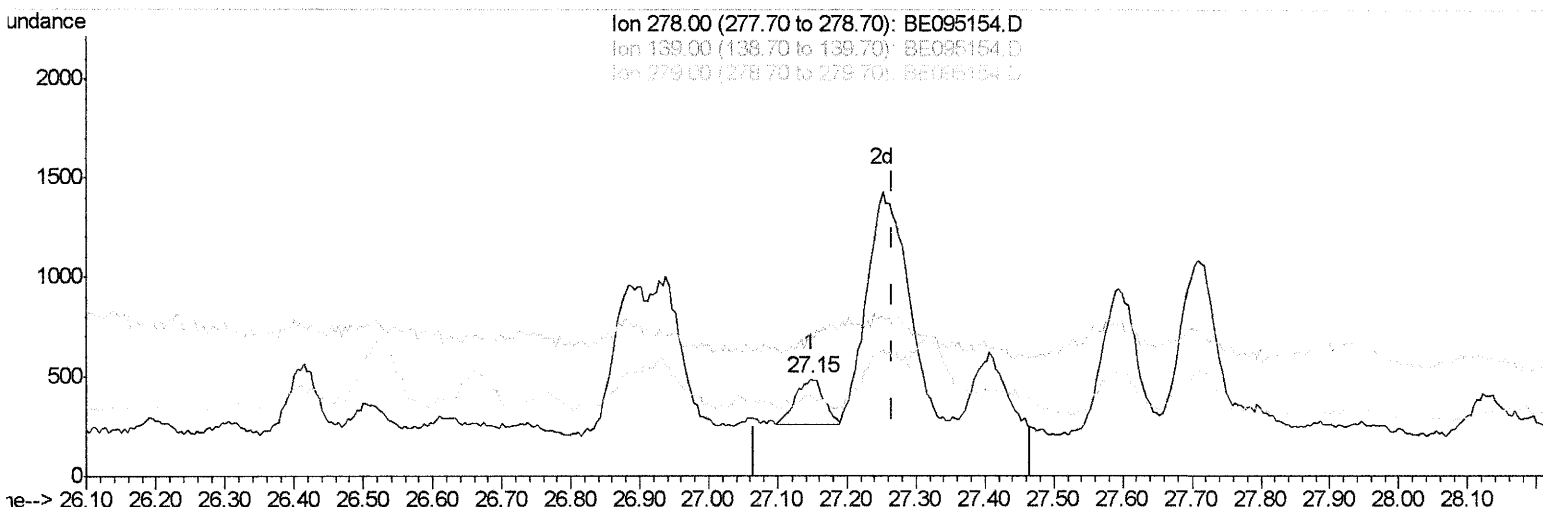

(25) Dibenzo(a,h)anthracene

27.147min (-0.119) 0.01ng/ul

response 645

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	147.05#
279.00	32.40	83.71#
0.00	0.00	0.00

Quantitation Report (Qedit)




Instrument :
BNA_E
ClientSampleId :
F6A46

Manual Integrations
APPROVED

Sohil
1/29/2018 6:34:23 PM

Data Path : Z:\HPCHEM1\BNA_E\Data\BE012618\
Data File : BE095154.D
Acq On : 27 Jan 2018 6:52
Operator : SJ/JU
Sample : J1174-11
Misc :
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Jan 28 00:47:37 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

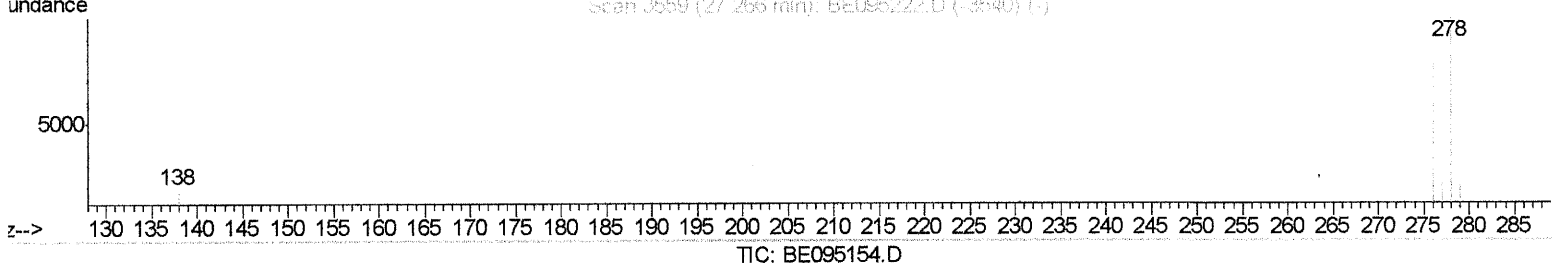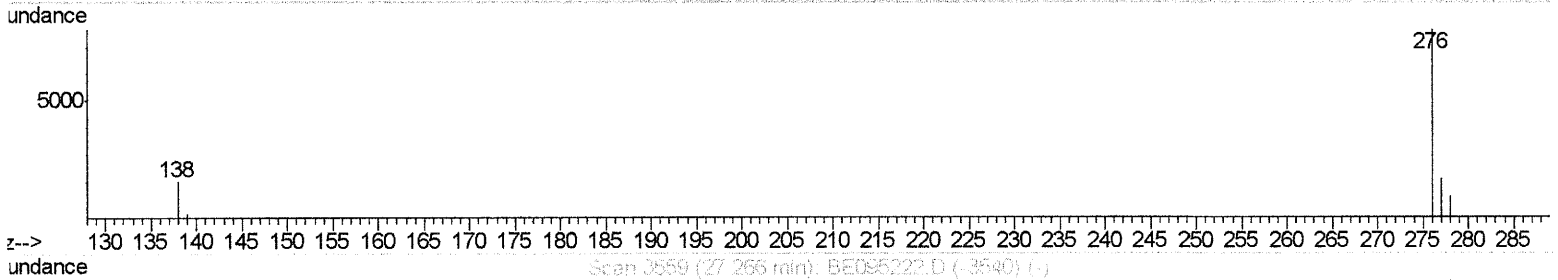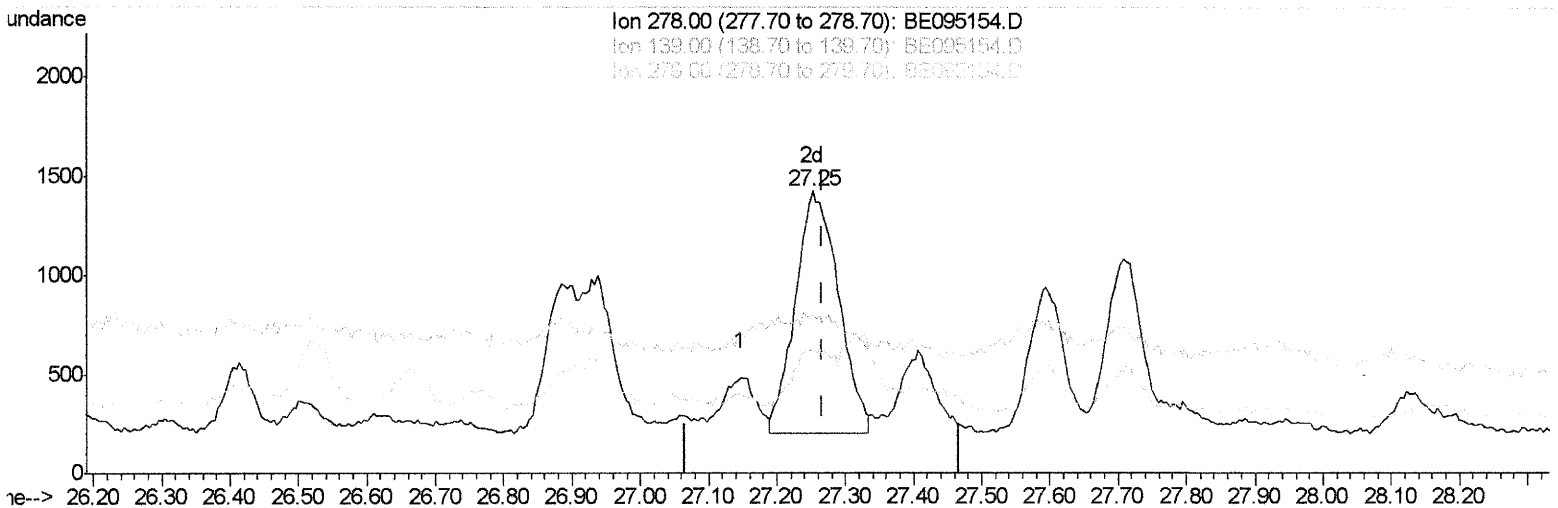

(25) Dibenzo(a,h)anthracene

27.252min (-0.014) 0.12ng/ul m

response 5384

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	56.29#
279.00	32.40	44.69#
0.00	0.00	0.00

27.252min

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE012618\
Data File : BE095154.D
Acq On : 27 Jan 2018 6:52
Operator : SJ/JU
Sample : J1174-11
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6A46

Manual Integrations
APPROVED

Sohil
1/29/2018 6:34:23 PM

Quant Time: Jan 28 00:47:37 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

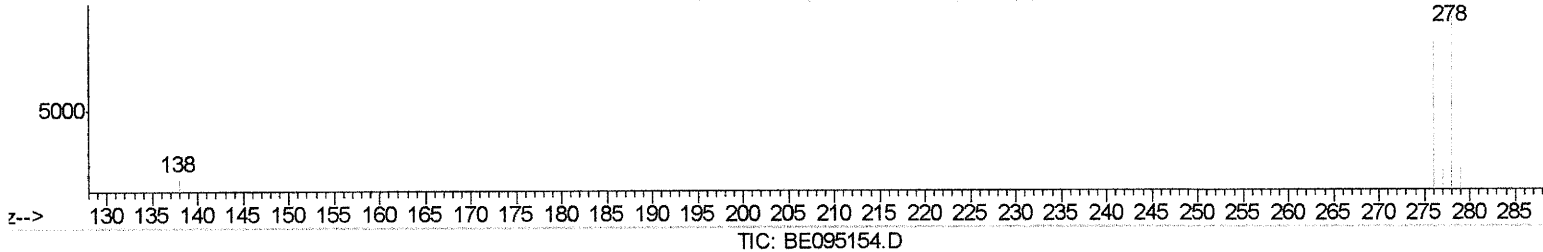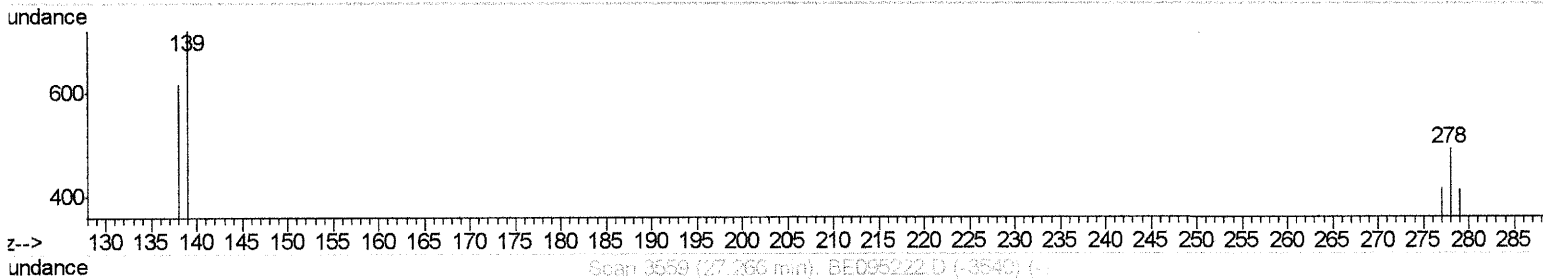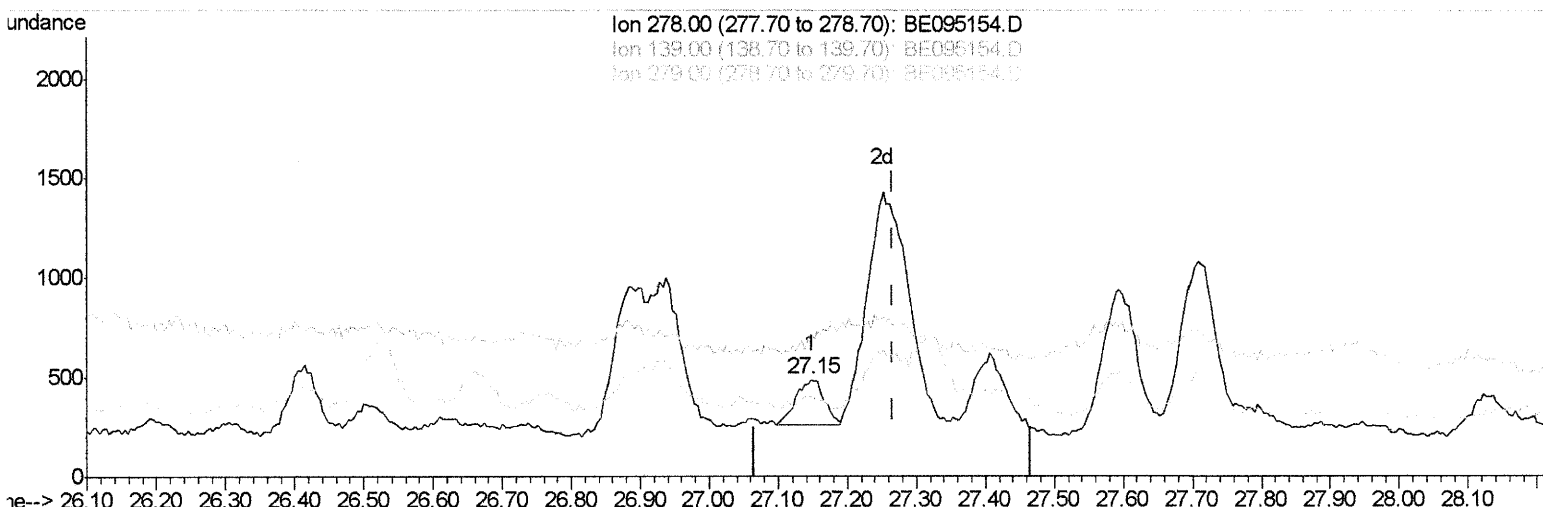

(25) Dibenzo(a,h)anthracene

27.147min (-0.119) 0.01ng/ul

response 645

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	147.05#
279.00	32.40	83.71#
0.00	0.00	0.00

Quantitation Report (Qedit)


Instrument :
BNA_E
ClientSampled :
F6A46

Manual Integrations
APPROVED

Sohil
1/29/2018 6:34:23 PM

Data Path : Z:\HPCHEM1\BNA_E\Data\BE012618\
Data File : BE095154.D
Acq On : 27 Jan 2018 6:52
Operator : SJ/JU
Sample : J1174-11
Misc :
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Jan 28 00:47:37 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

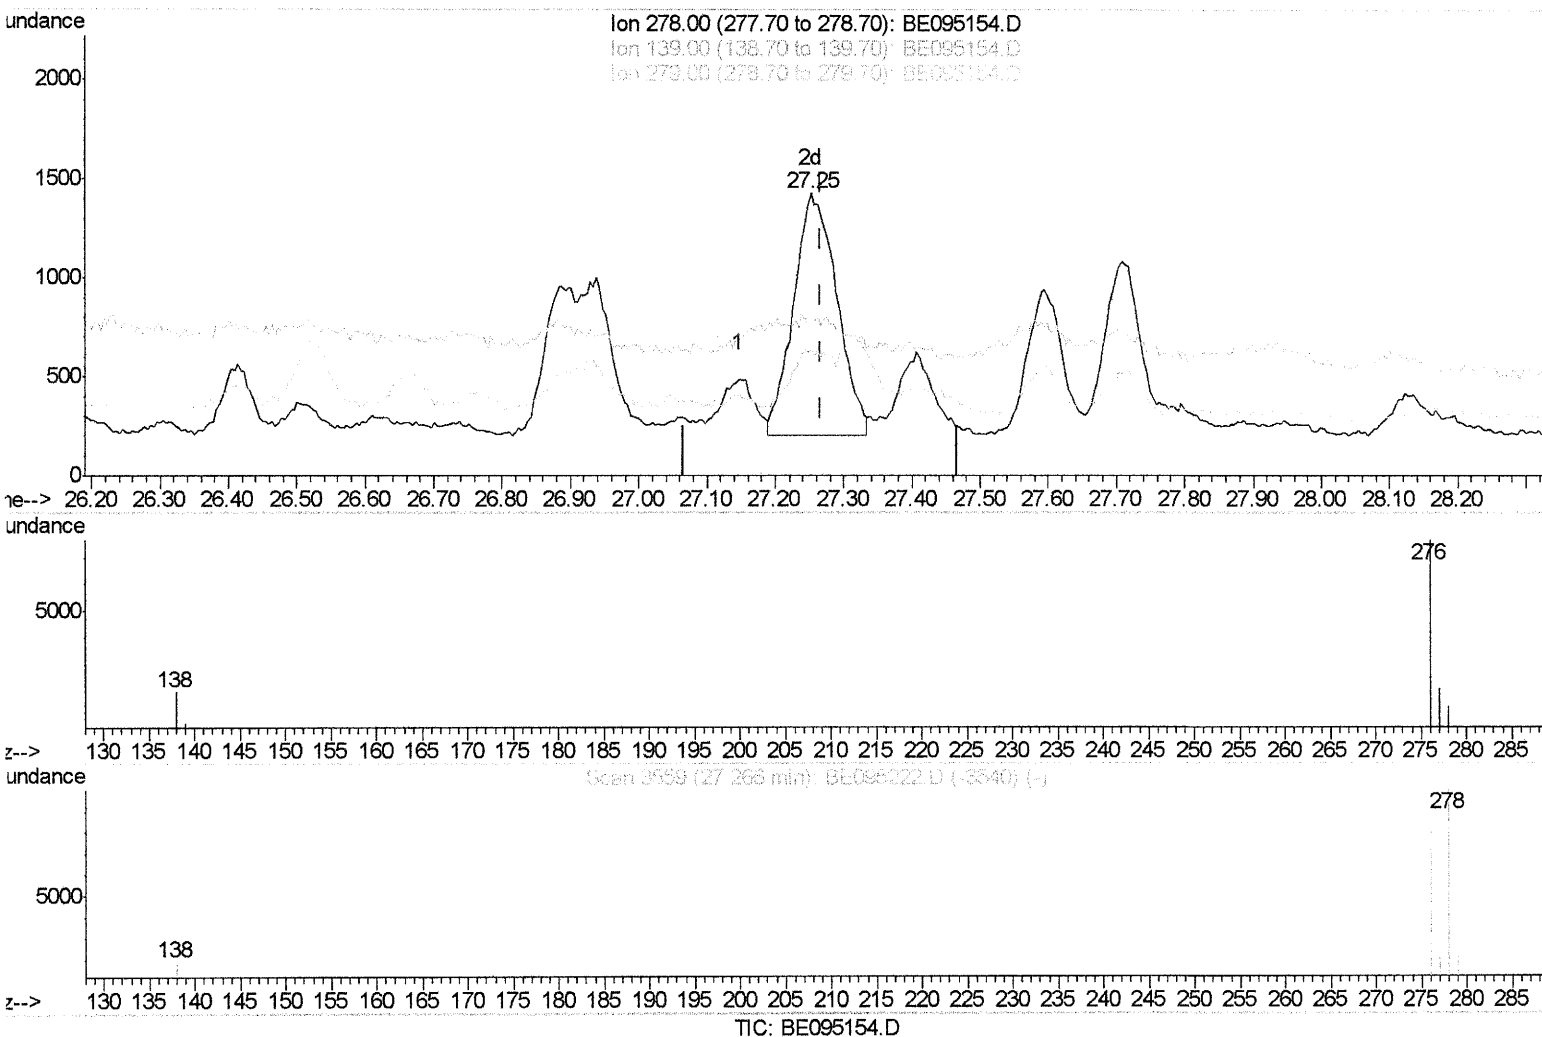

(25) Dibenzo(a,h)anthracene

27.252min (-0.014) 0.12ng/ul m

response 5384

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	56.29#
279.00	32.40	44.69#
0.00	0.00	0.00

See 1/31/18

Quantitation Report (QT Reviewed)

Instrument :
BNA_E
Client Sampled :
F6A46

Manual Integrations
APPROVED

Sohil
1/29/2018 6:34:23 PM

Data Path : Z:\HPCHEM1\BNA_E\Data\BE012618\
Data File : BE095154.D
Acq On : 27 Jan 2018 6:52
Operator : SJ/JU
Sample : J1174-11
Misc :
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Jan 29 16:45:06 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	3691	0.40	ng/ul	0.00
2) Naphthalene-d8	11.27	136	12161	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	8003	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.73	188	17581m	0.40	ng/ul	>0.02
16) Chrysene-d12	21.80	240	16968	0.40	ng/ul	0.00
20) Perylene-d12	24.45	264	15392m	0.40	ng/ul	>0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.82	152	5210	0.26	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	14640	0.22	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Naphthalene	11.32	128	1530	0.045	ng/ul#	85
5) 2-Methylnaphthalene	12.89	142	1138	0.050	ng/ul	96
7) Acenaphthylene	14.74	152	7419	0.193	ng/ul#	94
8) Acenaphthene	15.08	153	1018	0.034	ng/ul#	82
9) Fluorene	16.05	166	1211m	0.039	ng/ul	> 97
11) Pentachlorophenol	17.36	266	10571	3.104	ng/ul	97
12) Phenanthrene	17.75	178	9963	0.168	ng/ul#	89
13) Anthracene	17.85	178	14287	0.264	ng/ul#	91
15) Fluoranthene	19.73	202	38489	0.503	ng/ul	83
17) Pyrene	20.08	202	61839	1.086	ng/ul#	80
18) Benzo(a)anthracene	21.79	228	19880	0.375	ng/ul#	84
19) Chrysene	21.84	228	29015	0.527	ng/ul#	86
21) Benzo(b)fluoranthene	23.62	252	52316m	0.963	ng/ul	} Re-1/3/18
22) Benzo(k)fluoranthene	23.66	252	12363m	0.249	ng/ul	
23) Benzo(a)pyrene	24.33	252	27057m	0.558	ng/ul	
24) Indeno(1,2,3-cd)pyrene	27.25	276	24164m	0.454	ng/ul	
25) Dibenzo(a,h)anthracene	27.25	278	5384m	0.124	ng/ul	
26) Benzo(g,h,i)perylene	28.13	276	25614m	0.569	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed