

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012718\
 Data File : BE095171.D
 Acq On : 27 Jan 2018 17:46
 Operator : SJ/JU
 Sample : J1220-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6A08

Quant Time: Jan 28 02:35:22 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 27 03:18:43 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2920	0.40	ng/ul	0.00
2) Naphthalene-d8	11.27	136	9588	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	6125	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.71
16) Chrysene-d12	21.80	240	13237	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	1009764	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.82	152	6377	0.41	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	18361	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	20.06	202	2873	0.065	ng/ul#	Qvalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012718\
Data File : BE095171.D
Acq On : 27 Jan 2018 17:46
Operator : SJ/JU
Sample : J1220-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6A08

Quant Time: Jan 28 02:35:22 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

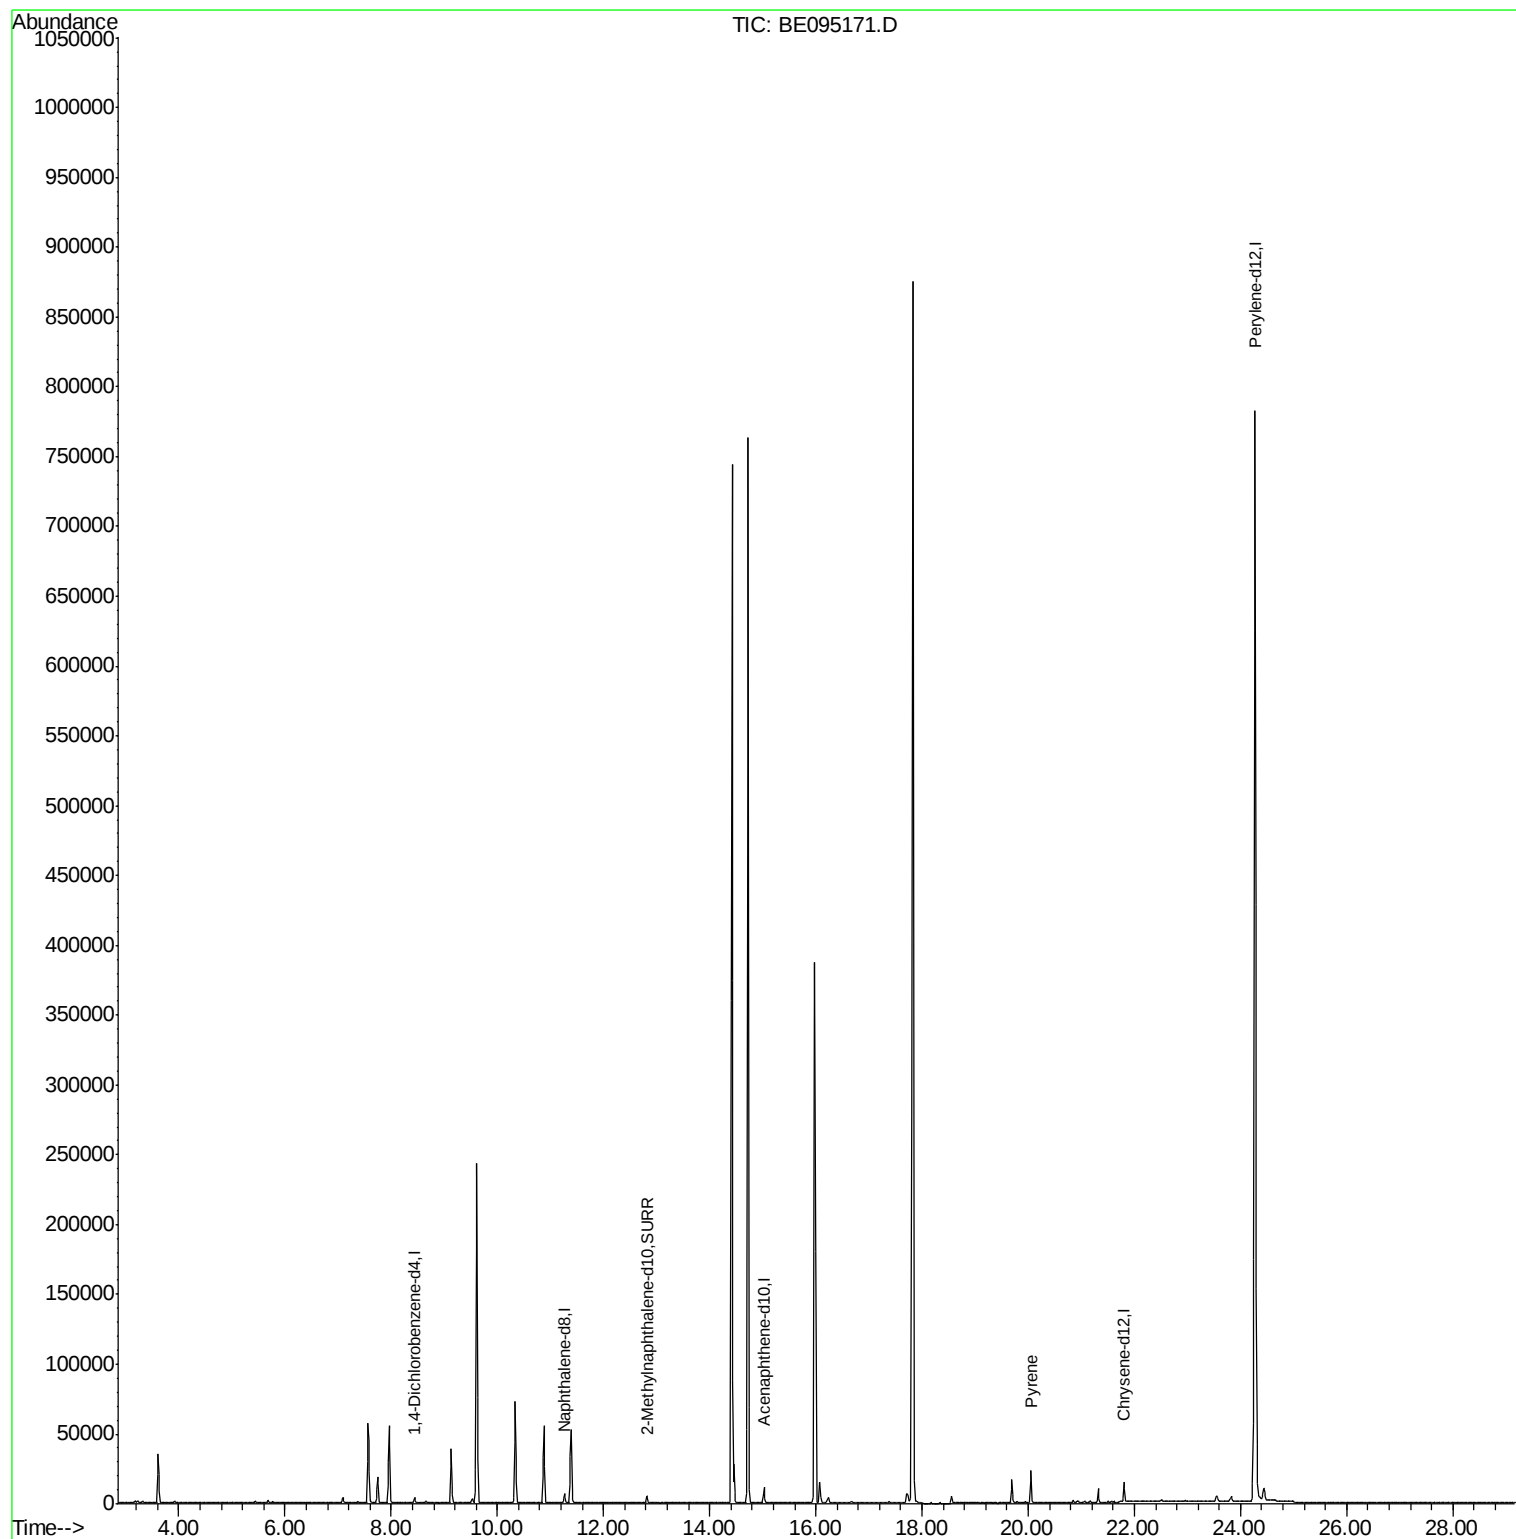

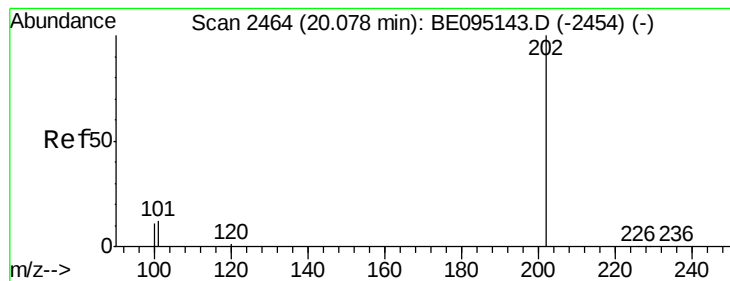

#17

Pyrene

Concen: 0.065 ng/ul

RT: 20.06 min Scan# 2461

Delta R.T. -0.02 min

Lab File: BE095171.D

Acq: 27 Jan 2018 17:46

Instrument :

BNA_E

ClientSampleId :

F6A08


Tgt Ion: 202 Resp: 2873

Ion Ratio Lower Upper

202 100

101 154.8 18.2 27.4#

100 935.6 15.6 23.4#

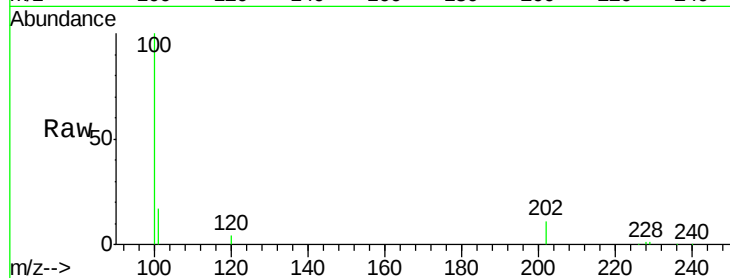

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BE

