

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012718\
 Data File : BE095175.D
 Acq On : 27 Jan 2018 20:10
 Operator : SJ/JU
 Sample : J1220-17
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6A17

Quant Time: Jan 28 02:35:47 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 27 03:18:43 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	3039	0.40	ng/ul	0.00
2) Naphthalene-d8	11.27	136	9730	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	6403	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.71
16) Chrysene-d12	21.80	240	14283	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	799303	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.82	152	4900	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	14648	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	20.05	202	2506	0.052	ng/ul#	Qvalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012718\
Data File : BE095175.D
Acq On : 27 Jan 2018 20:10
Operator : SJ/JU
Sample : J1220-17
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6A17

Quant Time: Jan 28 02:35:47 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

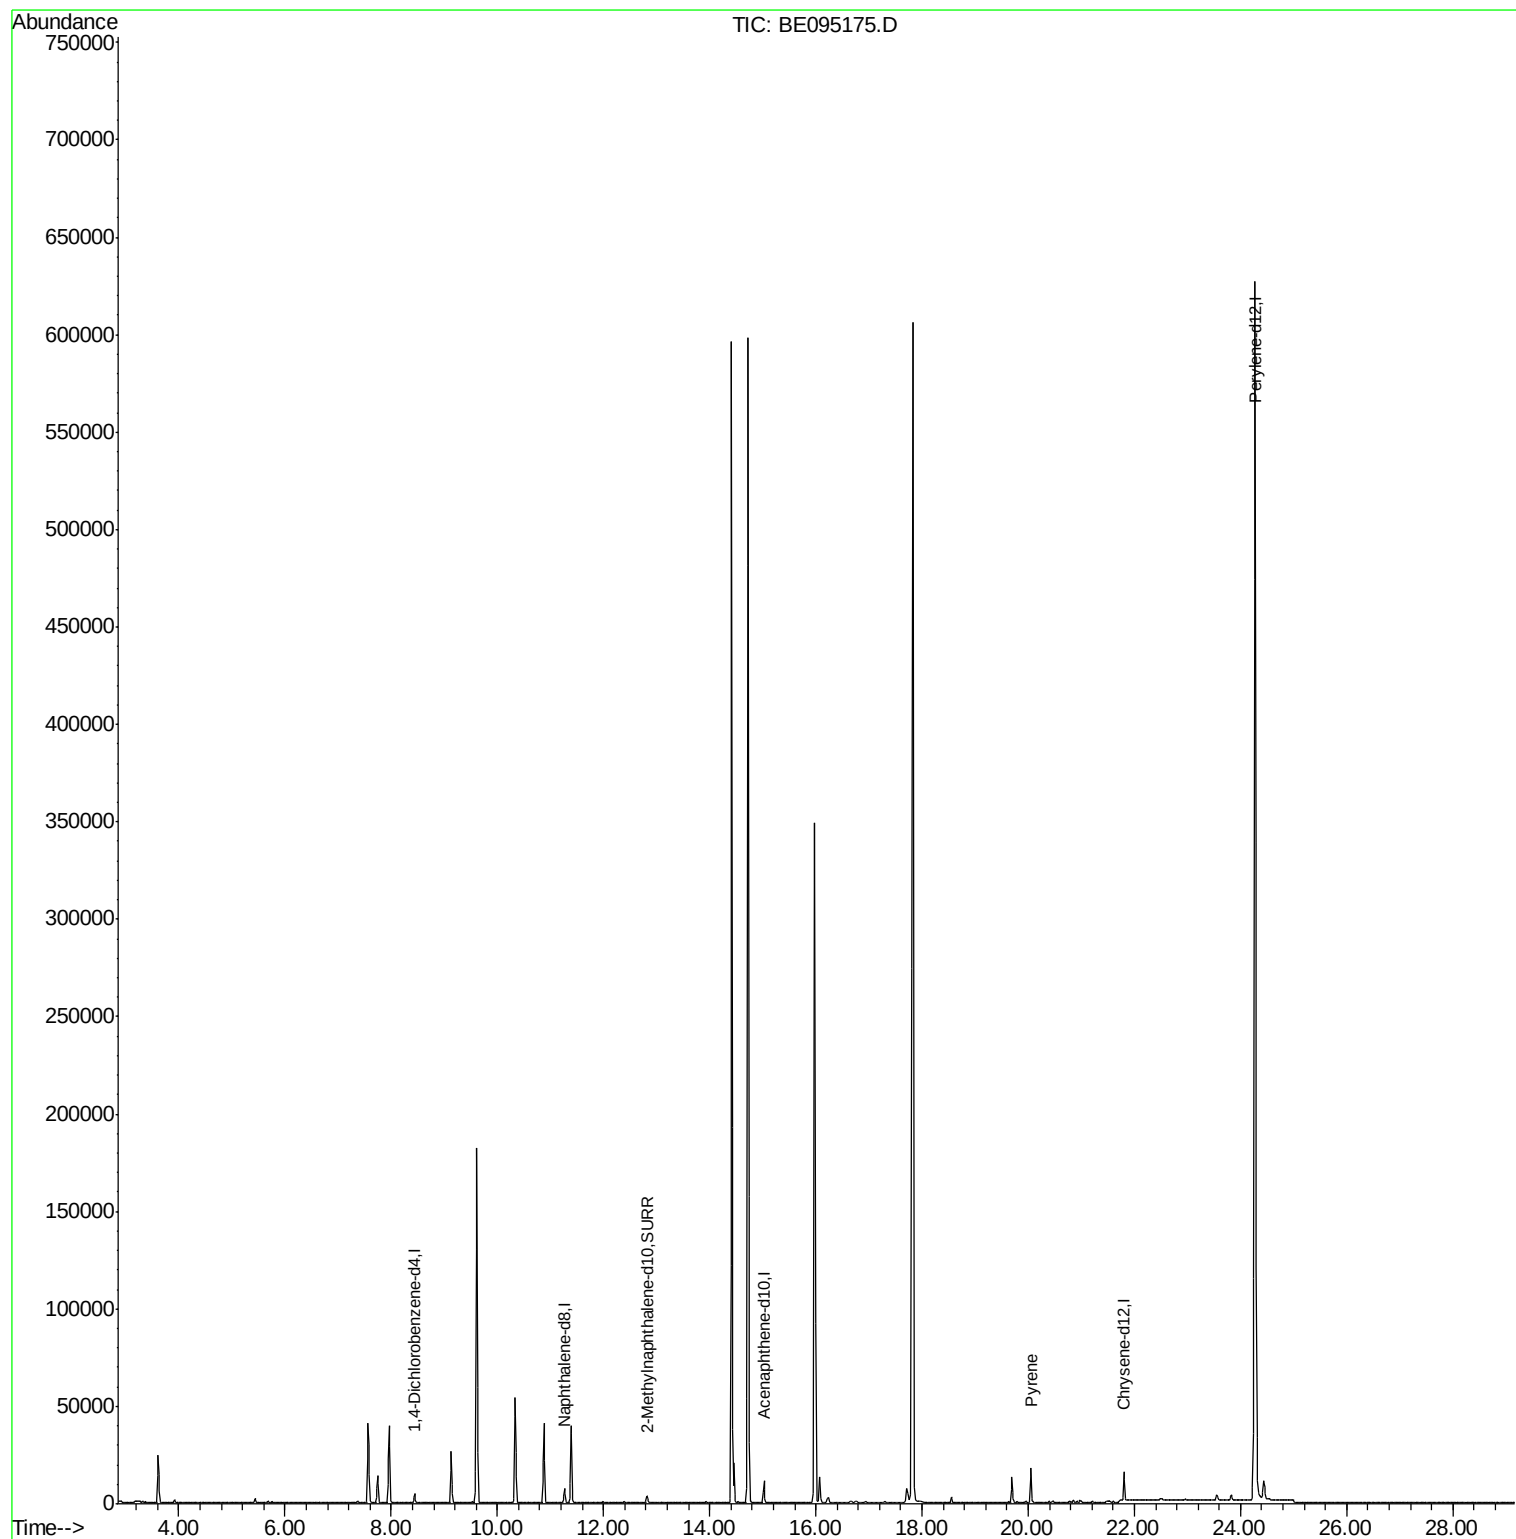

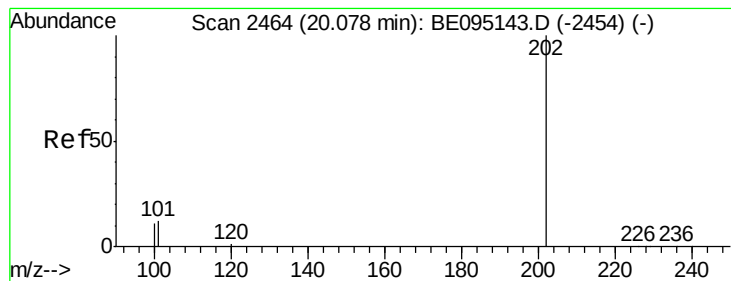

#17
 Pyrene
 Concen: 0.052 ng/ul
 RT: 20.05 min Scan# 2460
 Delta R.T. -0.03 min
 Lab File: BE095175.D
 Acq: 27 Jan 2018 20:10

Instrument :
 BNA_E
 ClientSampleId :
 F6A17

Tgt Ion: 202 Resp: 2506
 Ion Ratio Lower Upper
 202 100
 101 168.9 18.2 27.4#
 100 1152.6 15.6 23.4#

