

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012718\
 Data File : BE095183.D
 Acq On : 28 Jan 2018 00:56
 Operator : SJ/JU
 Sample : J1220-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6A12

Quant Time: Jan 28 04:03:58 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 27 03:18:43 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	3176	0.40	ng/ul	0.00
2) Naphthalene-d8	11.27	136	10508	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	6938	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.71
16) Chrysene-d12	21.80	240	14770	0.40	ng/ul	0.00
20) Perylene-d12	24.28	264	993218	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.82	152	6402	0.37	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	18550	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	20.06	202	3569	0.072	ng/ul#	Qvalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012718\
Data File : BE095183.D
Acq On : 28 Jan 2018 00:56
Operator : SJ/JU
Sample : J1220-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6A12

Quant Time: Jan 28 04:03:58 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

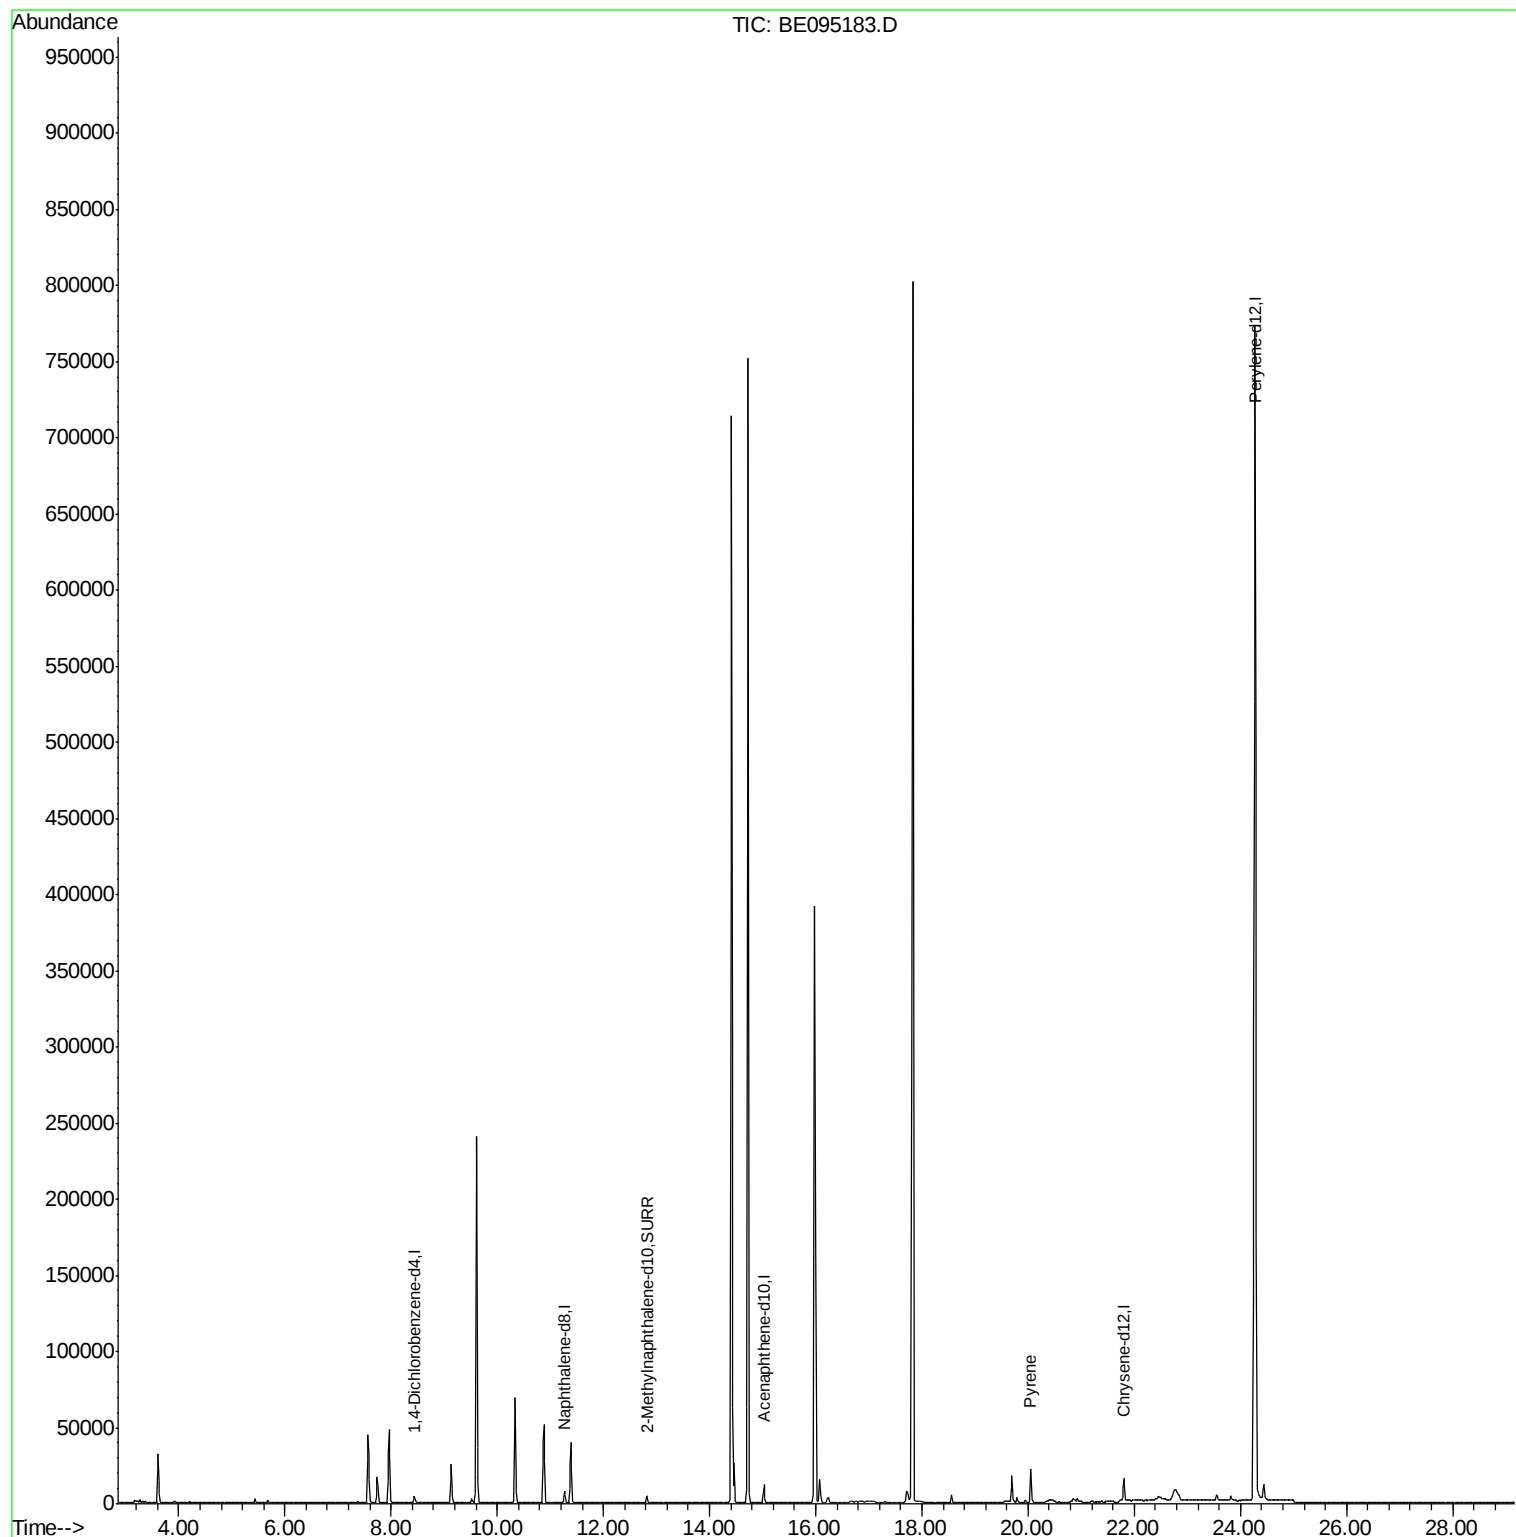

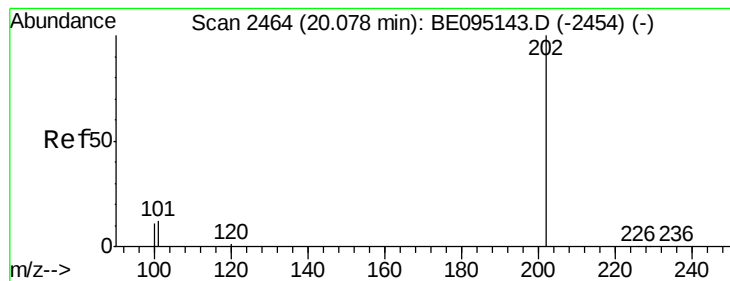

#17

Pyrene

Concen: 0.072 ng/ul

RT: 20.06 min Scan# 2461

Delta R.T. -0.02 min

Lab File: BE095183.D

Acq: 28 Jan 2018 00:56

Instrument :

BNA_E

ClientSampleId :

F6A12


Tgt Ion: 202 Resp: 3569

Ion Ratio Lower Upper

202 100

101 159.4 18.2 27.4#

100 975.1 15.6 23.4#

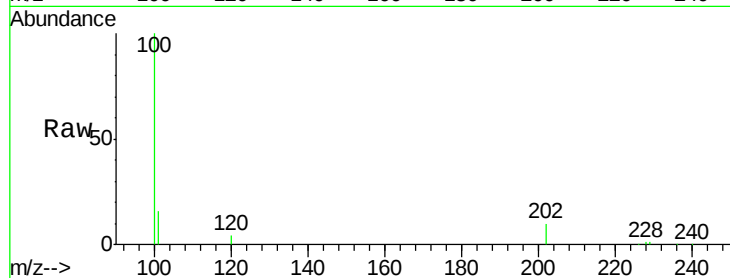

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BE

