

Data Path : Z:\HPCHEM1\BNA E\DATA\BE012718\
 Data File : BE095188.D
 Acq On : 28 Jan 2018 3:55
 Operator : SJ/JU
 Sample : J1220-16
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Jan 29 00:16:06 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 29 00:15:32 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	3375	0.40	ng/ul	0.00
2) Naphthalene-d8	11.27	136	11037	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	7320	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.71
16) Chrysene-d12	21.80	240	15581	0.40	ng/ul	0.00
20) Perylene-d12	24.28	264	1265354	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.82	152	7817	0.43	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	22562	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	20.06	202	4354	0.083	ng/ul#	1
18) Benzo(a)anthracene	21.79	228	1366	0.028	ng/ul#	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE012718\
Data File : BE095188.D
Acq On : 28 Jan 2018 3:55
Operator : SJ/JU
Sample : J1220-16
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Jan 29 00:16:06 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 29 00:15:32 2018
Response via : Initial Calibration

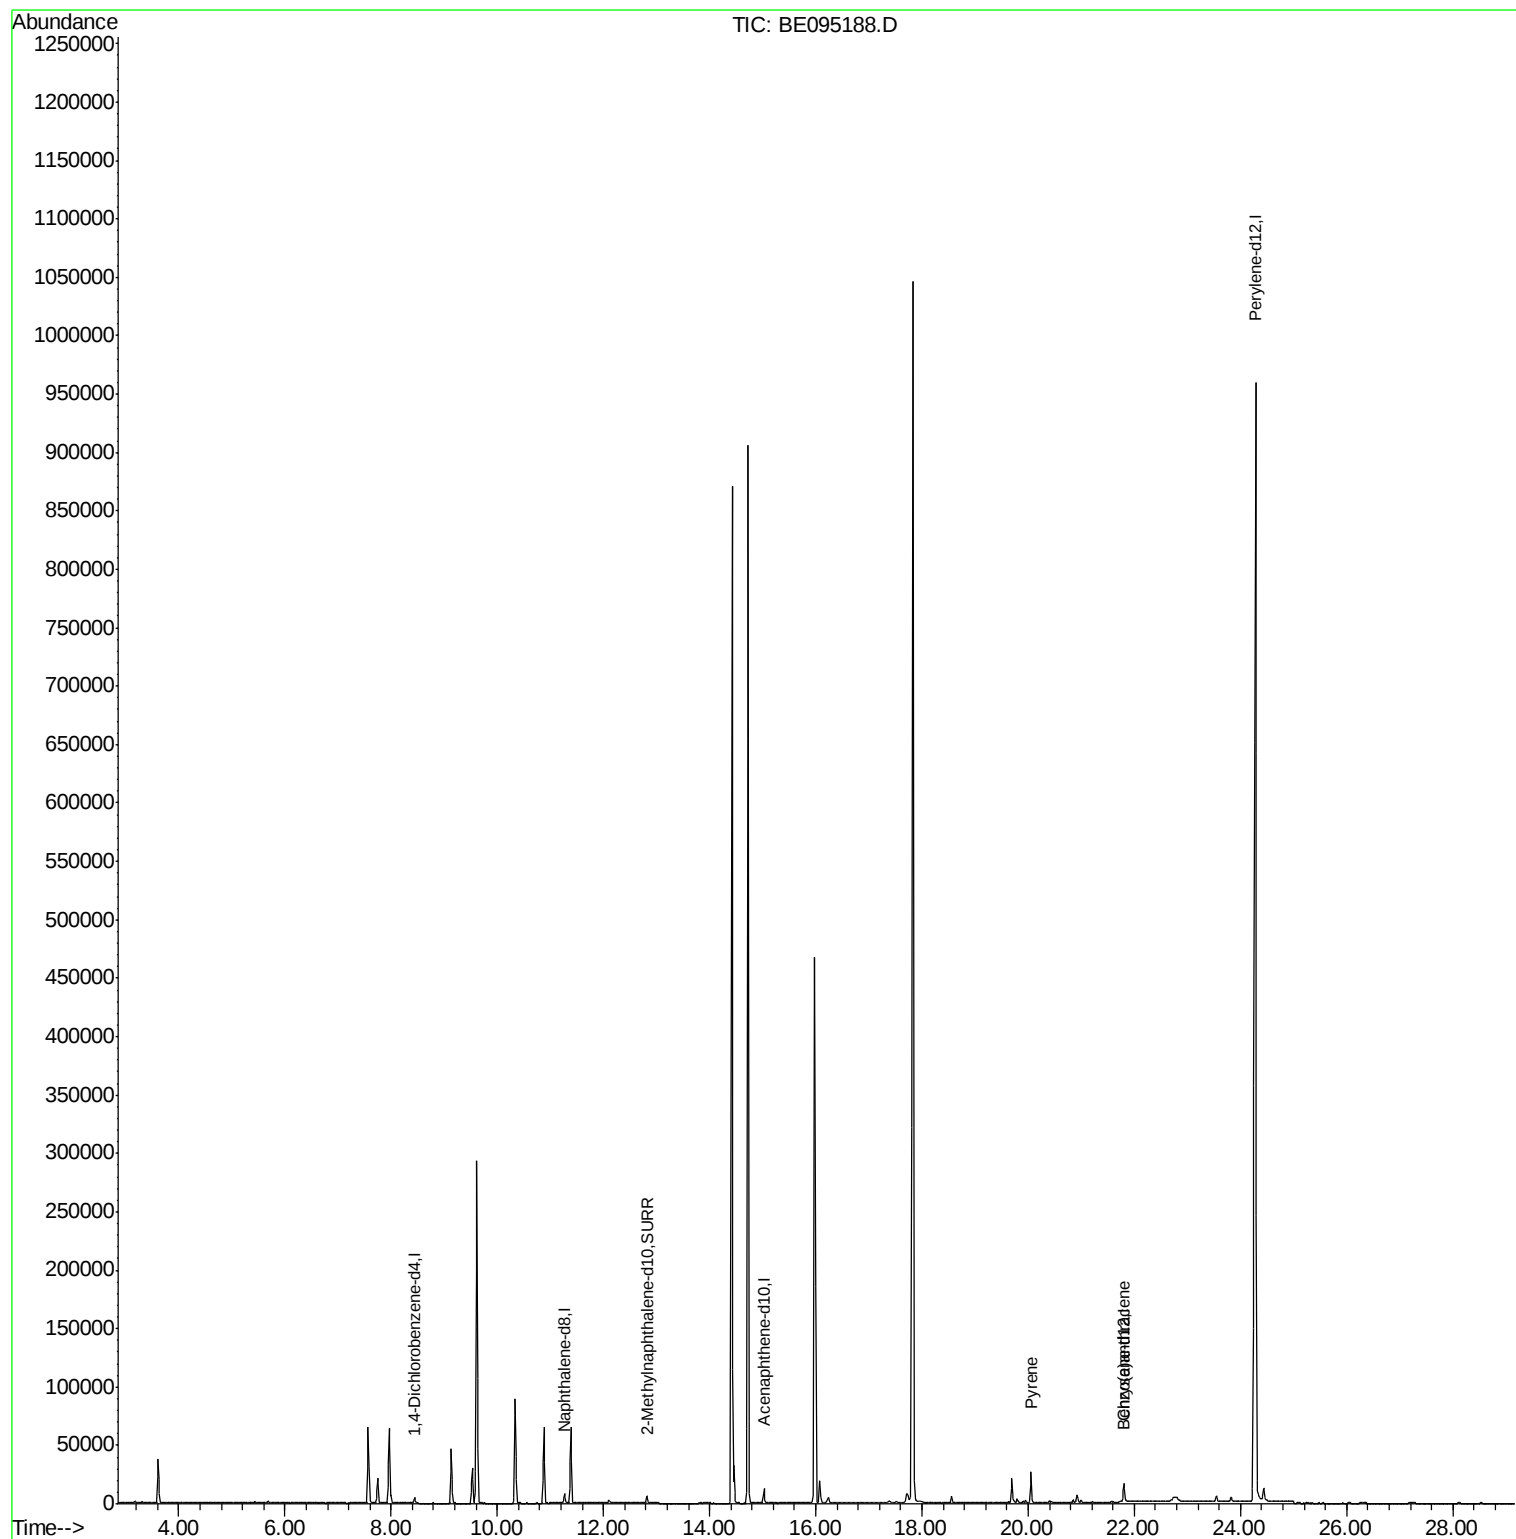

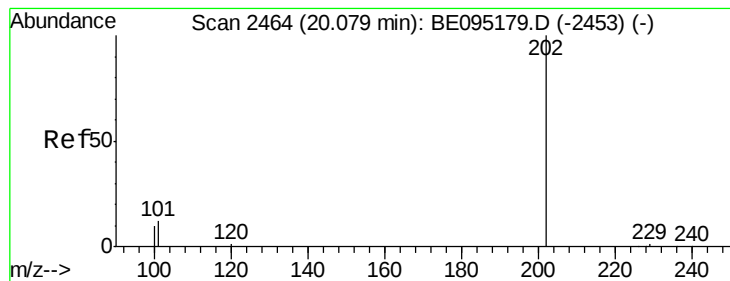

#17

Pvrene

Concen: 0.083 ng/ul

RT: 20.06 min Scan# 2461

Delta R.T. -0.02 min

Lab File: BE095188.D

Acq: 28 Jan 2018 3:55


Instrument :

BNA_E

ClientSampleId :

Tot Ion:202 Resp: 4354




Ion	Ratio	Lower	Upper
202	100		
101	158.3	18.2	27.4#
100	1022.5	15.6	23.4#

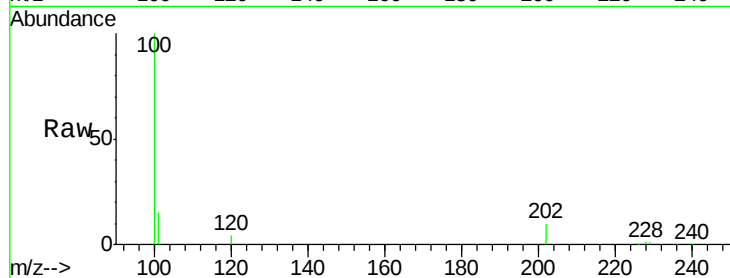

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BE

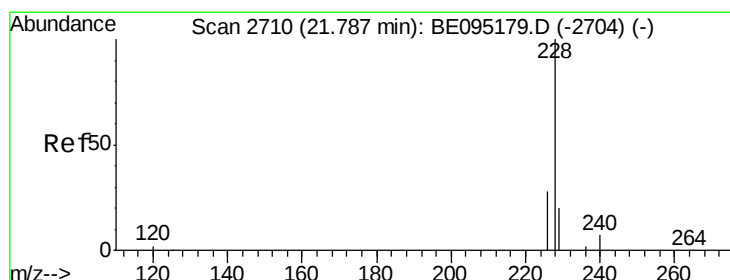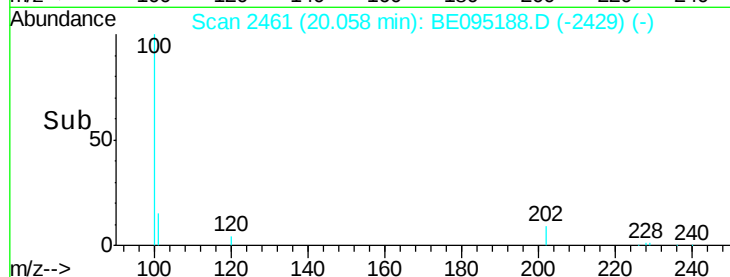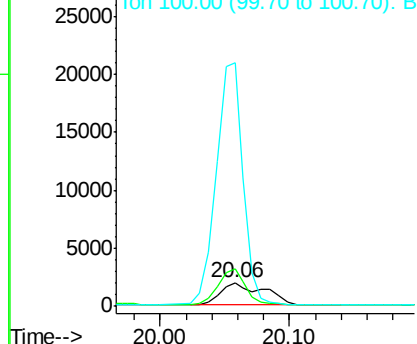

#18

Benzo(a)anthracene

Concen: 0.028 ng/ul

RT: 21.79 min Scan# 2710


Delta R.T. -0.00 min

Lab File: BE095188.D

Acq: 28 Jan 2018 3:55

Tgt Ion:228 Resp: 1366

Ion	Ratio	Lower	Upper
228	100		
229	39.6	22.8	34.2#
226	35.3	17.0	25.6#

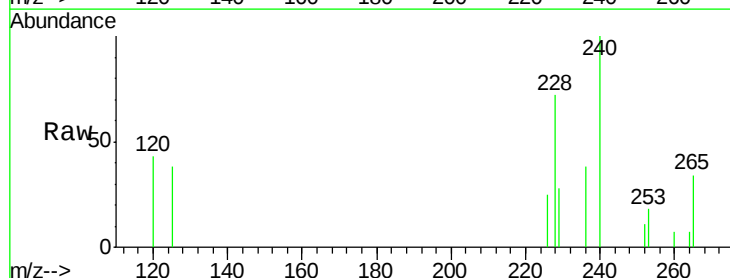

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

