

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012718\
 Data File : BE095185.D
 Acq On : 28 Jan 2018 2:08
 Operator : SJ/JU
 Sample : J1220-12
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6A14

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:22:06 PM

Quant Time: Jan 28 04:42:26 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 27 03:18:43 2018
 Response via : Initial Calibration

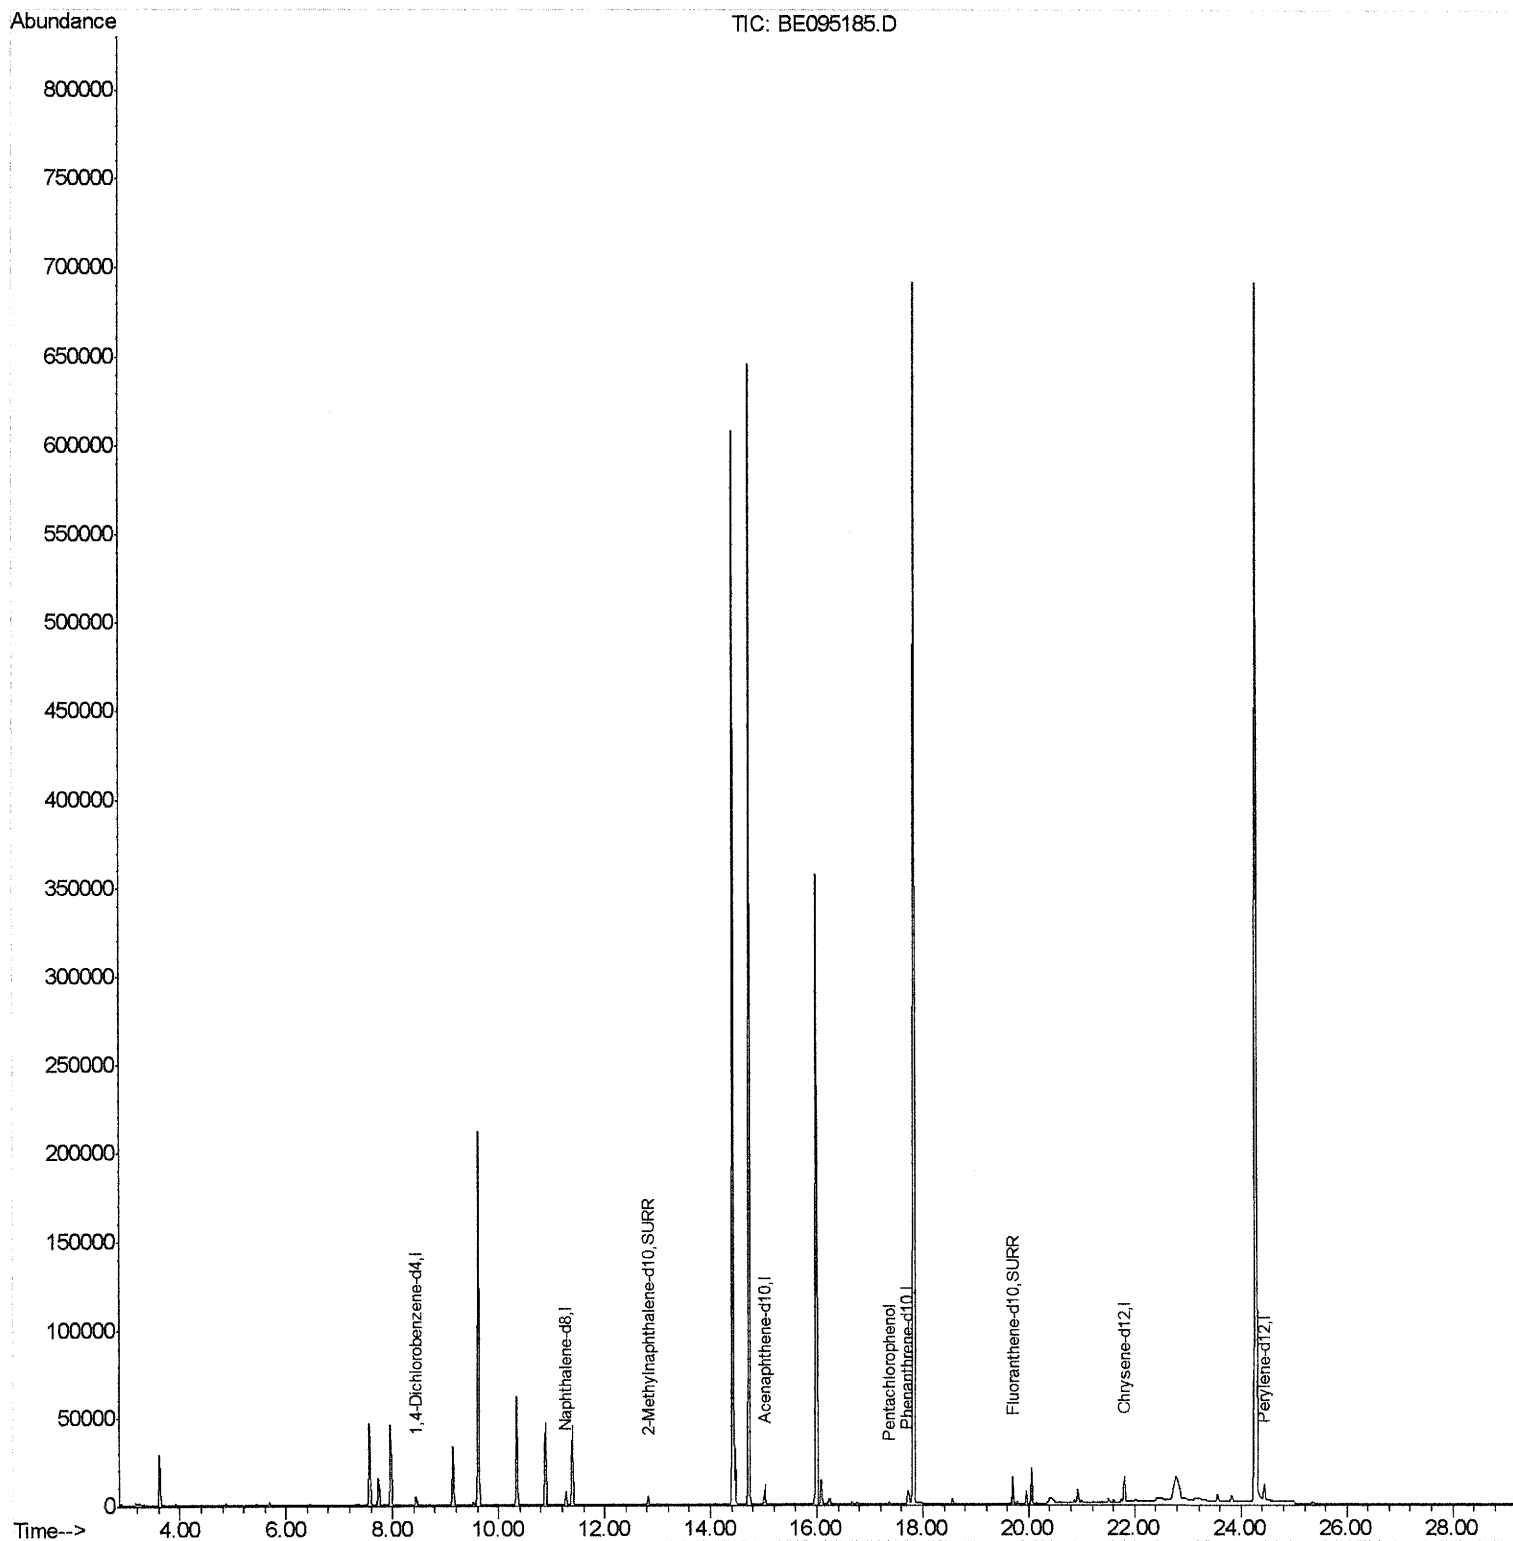

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012718\
Data File : BE095185.D
Acq On : 28 Jan 2018 2:08
Operator : SJ/JU
Sample : J1220-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
F6A14

Manual Integrations
APPROVED

Sohil
1/29/2018 6:22:06 PM

Quant Time: Jan 28 04:04:13 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

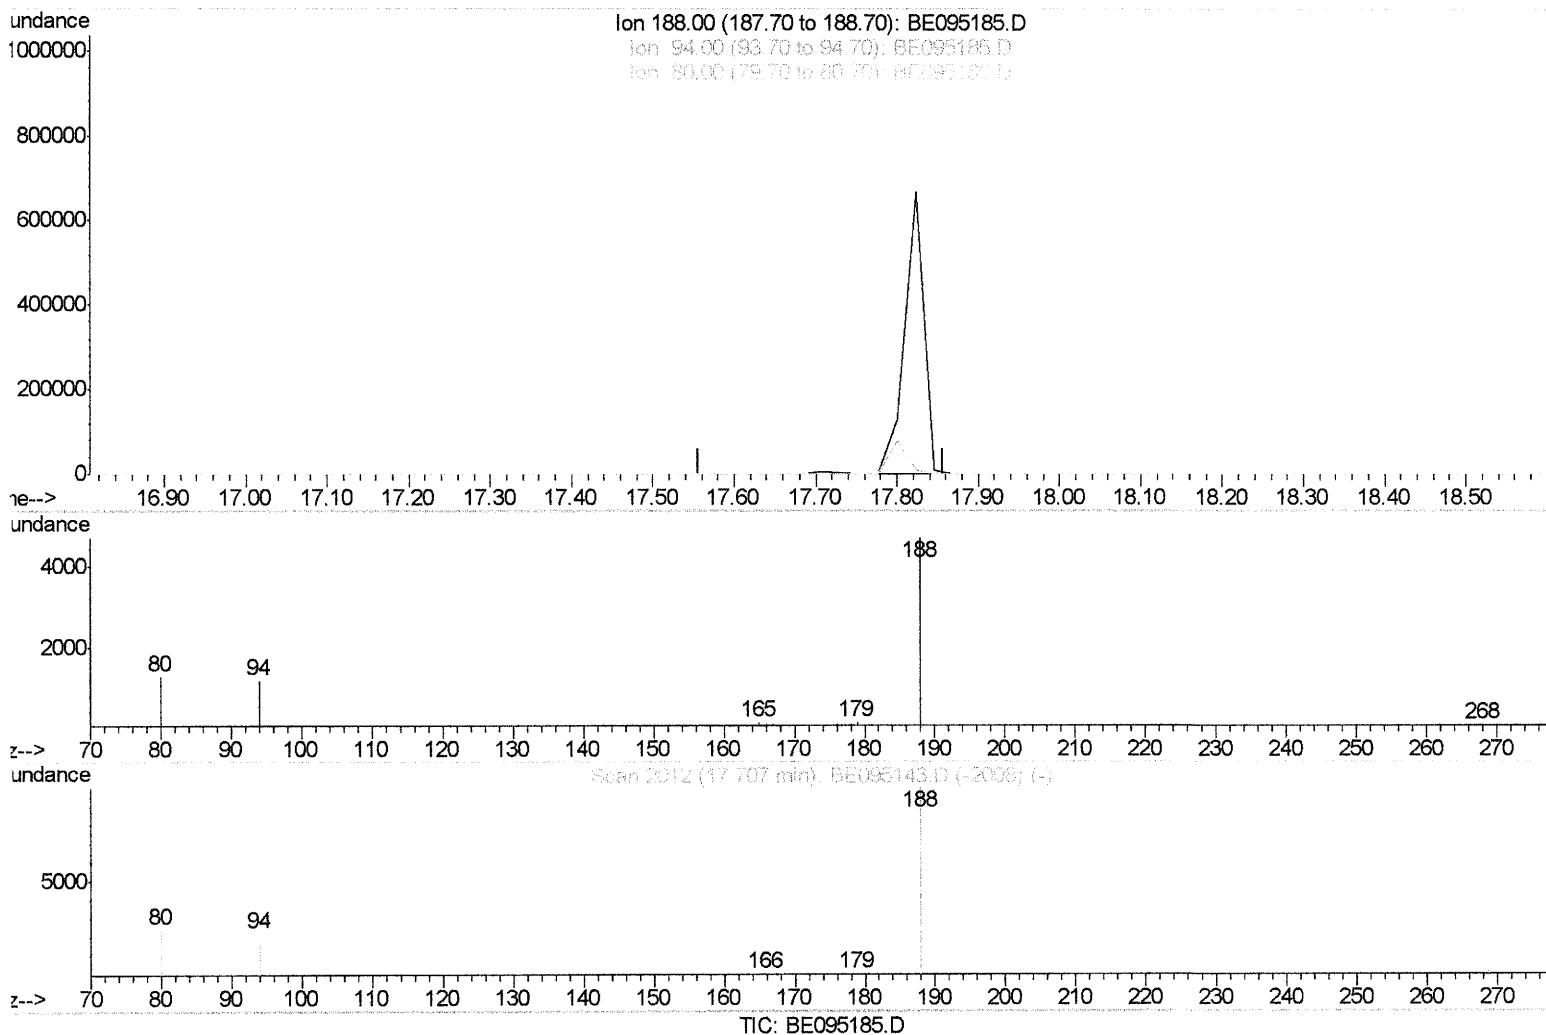

(10) Phenanthrene-d10 (I)

17.707min (-17.707) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Instrument :
BNA_E
ClientSampled :
F6A14

Manual Integrations
APPROVED

Sohil
1/29/2018 6:22:06 PM

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012718\
Data File : BE095185.D
Acq On : 28 Jan 2018 2:08
Operator : SJ/JU
Sample : J1220-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Jan 28 04:04:13 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

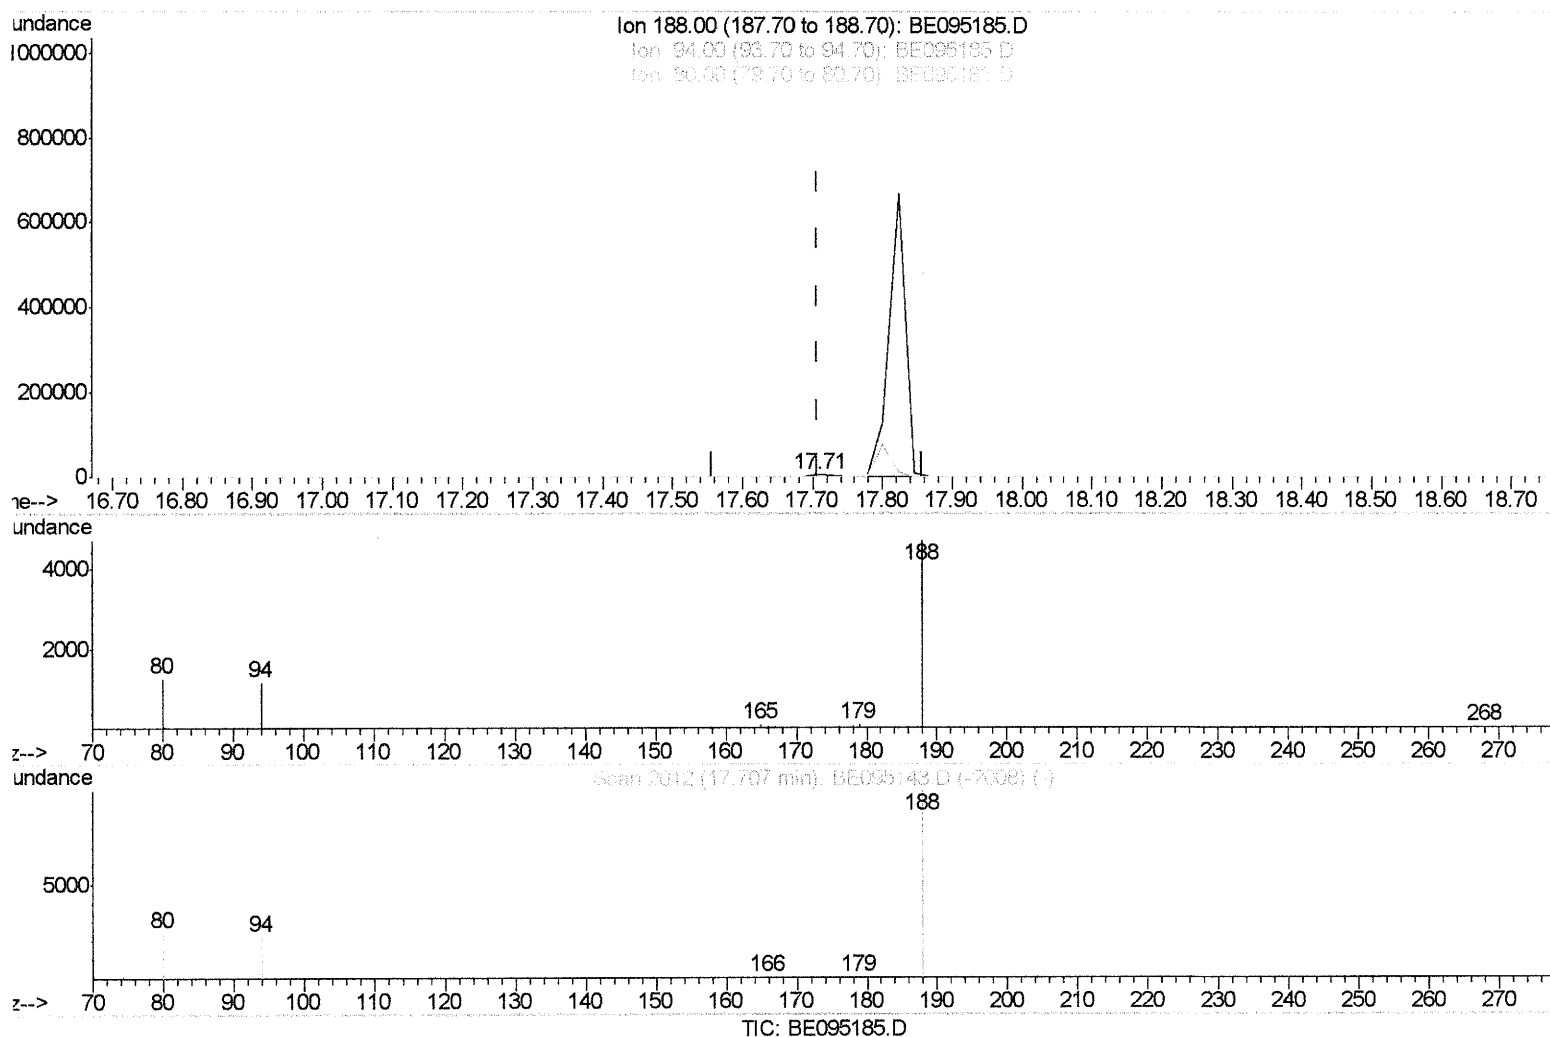

(10) Phenanthrene-d10 (I)

17.707min (+0.000) 0.40ng/ul m

response 13040

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	25.07#
80.00	11.80	26.98#
0.00	0.00	0.00

SJ/JU 1/29/18

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012718\
 Data File : BE095185.D
 Acq On : 28 Jan 2018 2:08
 Operator : SJ/JU
 Sample : J1220-12
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6A14

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:22:06 PM

Quant Time: Jan 28 04:40:55 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 27 03:18:43 2018
 Response via : Initial Calibration

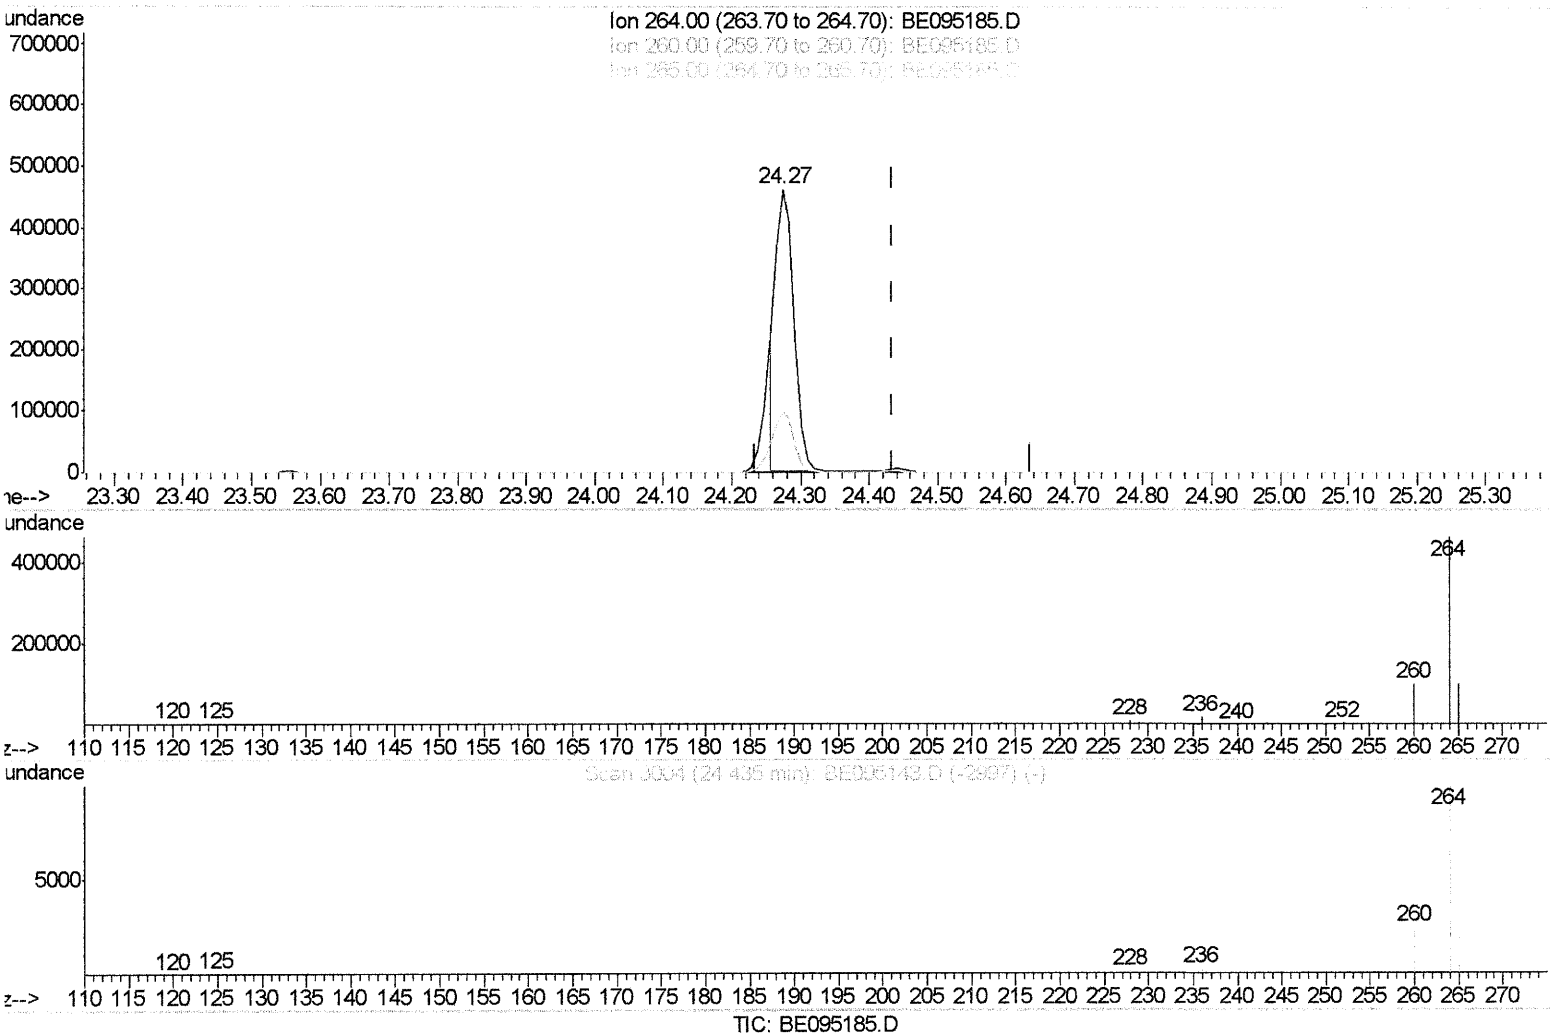

(20) Perylene-d12 (I)

24.274min (-0.161) 0.40ng/ul

response 841452

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.48#
265.00	103.50	21.50#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012718\
 Data File : BE095185.D
 Acq On : 28 Jan 2018 2:08
 Operator : SJ/JU
 Sample : J1220-12
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 Client Sample ID :
 F6A14

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:22:06 PM

Quant Time: Jan 28 04:42:26 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 27 03:18:43 2018
 Response via : Initial Calibration

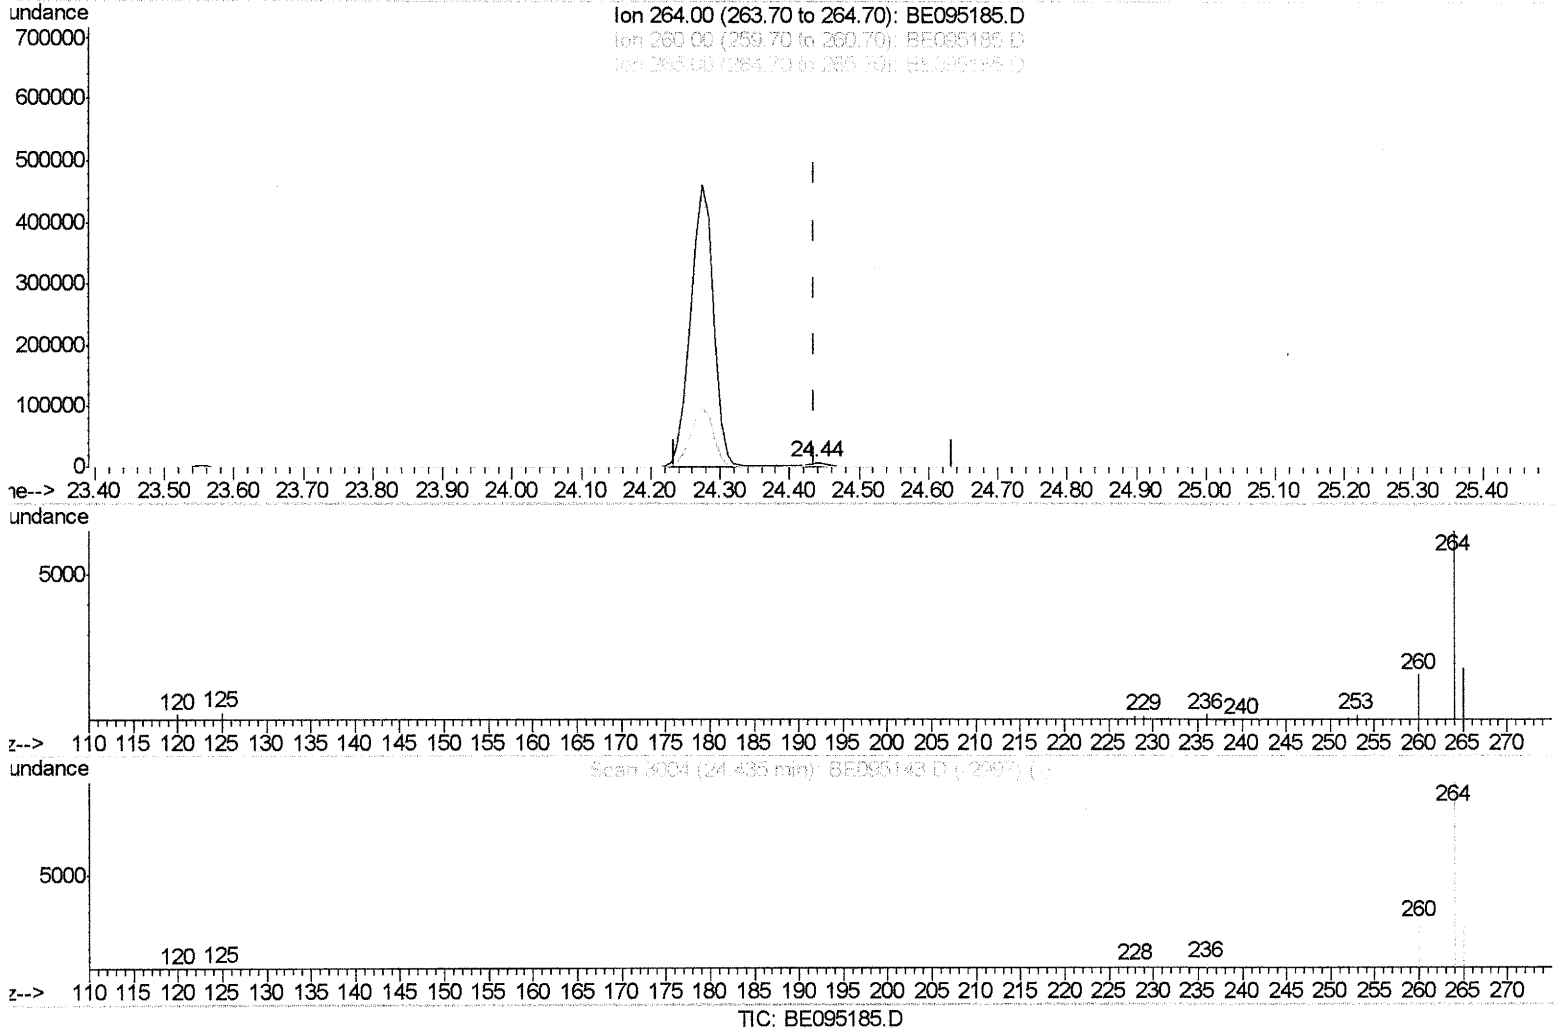

(20) Perylene-d12 (I)

24.436min (+0.001) 0.40ng/ul m

response 12331

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.05
265.00	103.50	28.37#
0.00	0.00	0.00

SJ 1/31/18

Quantitation Report (QT Reviewed)

Instrument :
BNA_E
ClientSampleId :
F6A14

Manual Integrations
APPROVED

Sohil
1/29/2018 6:22:06 PM

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012718\
Data File : BE095185.D
Acq On : 28 Jan 2018 2:08
Operator : SJ/JU
Sample : J1220-12
Disc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Jan 28 04:42:26 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	3066	0.40	ng/ul	0.00
2) Naphthalene-d8	11.27	136	9990	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	6243	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	13040m	0.40	ng/ul	>0.00
16) Chrysene-d12	21.80	240	14025	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	12331m	0.40	ng/ul	>0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.82	152	5522	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	16243	0.33	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	245	0.097	ng/ul	Qvalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed