

Data Path : Z:\HPCHEM1\BNA E\DATA\BE012718\
 Data File : BE095166.D
 Acq On : 27 Jan 2018 14:47
 Operator : SJ/JU
 Sample : J1243-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6D45

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:19:58 PM

Quant Time: Jan 28 01:53:19 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 27 03:18:43 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2964	0.40	ng/ul	0.00
2) Naphthalene-d8	11.27	136	9257	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	6238	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.73	188	12920m	0.40	ng/ul	0.02
16) Chrysene-d12	21.80	240	14103	0.40	ng/ul	0.00
20) Perylene-d12	24.45	264	12336m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.82	152	5084	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	15686	0.32	ng/ul	0.00
Target Compounds						
					Ovalue	
3) Naphthalene	11.32	128	993	0.038	ng/ul#	76
8) Acenaphthene	15.08	153	2414	0.104	ng/ul#	25

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA E\DATA\BE012718\
Data File : BE095166.D
Acq On : 27 Jan 2018 14:47
Operator : SJ/JU
Sample : J1243-02
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
F6D45

Manual Integrations
APPROVED

Sohil
1/29/2018 6:19:58 PM

Quant Time: Jan 28 01:53:19 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

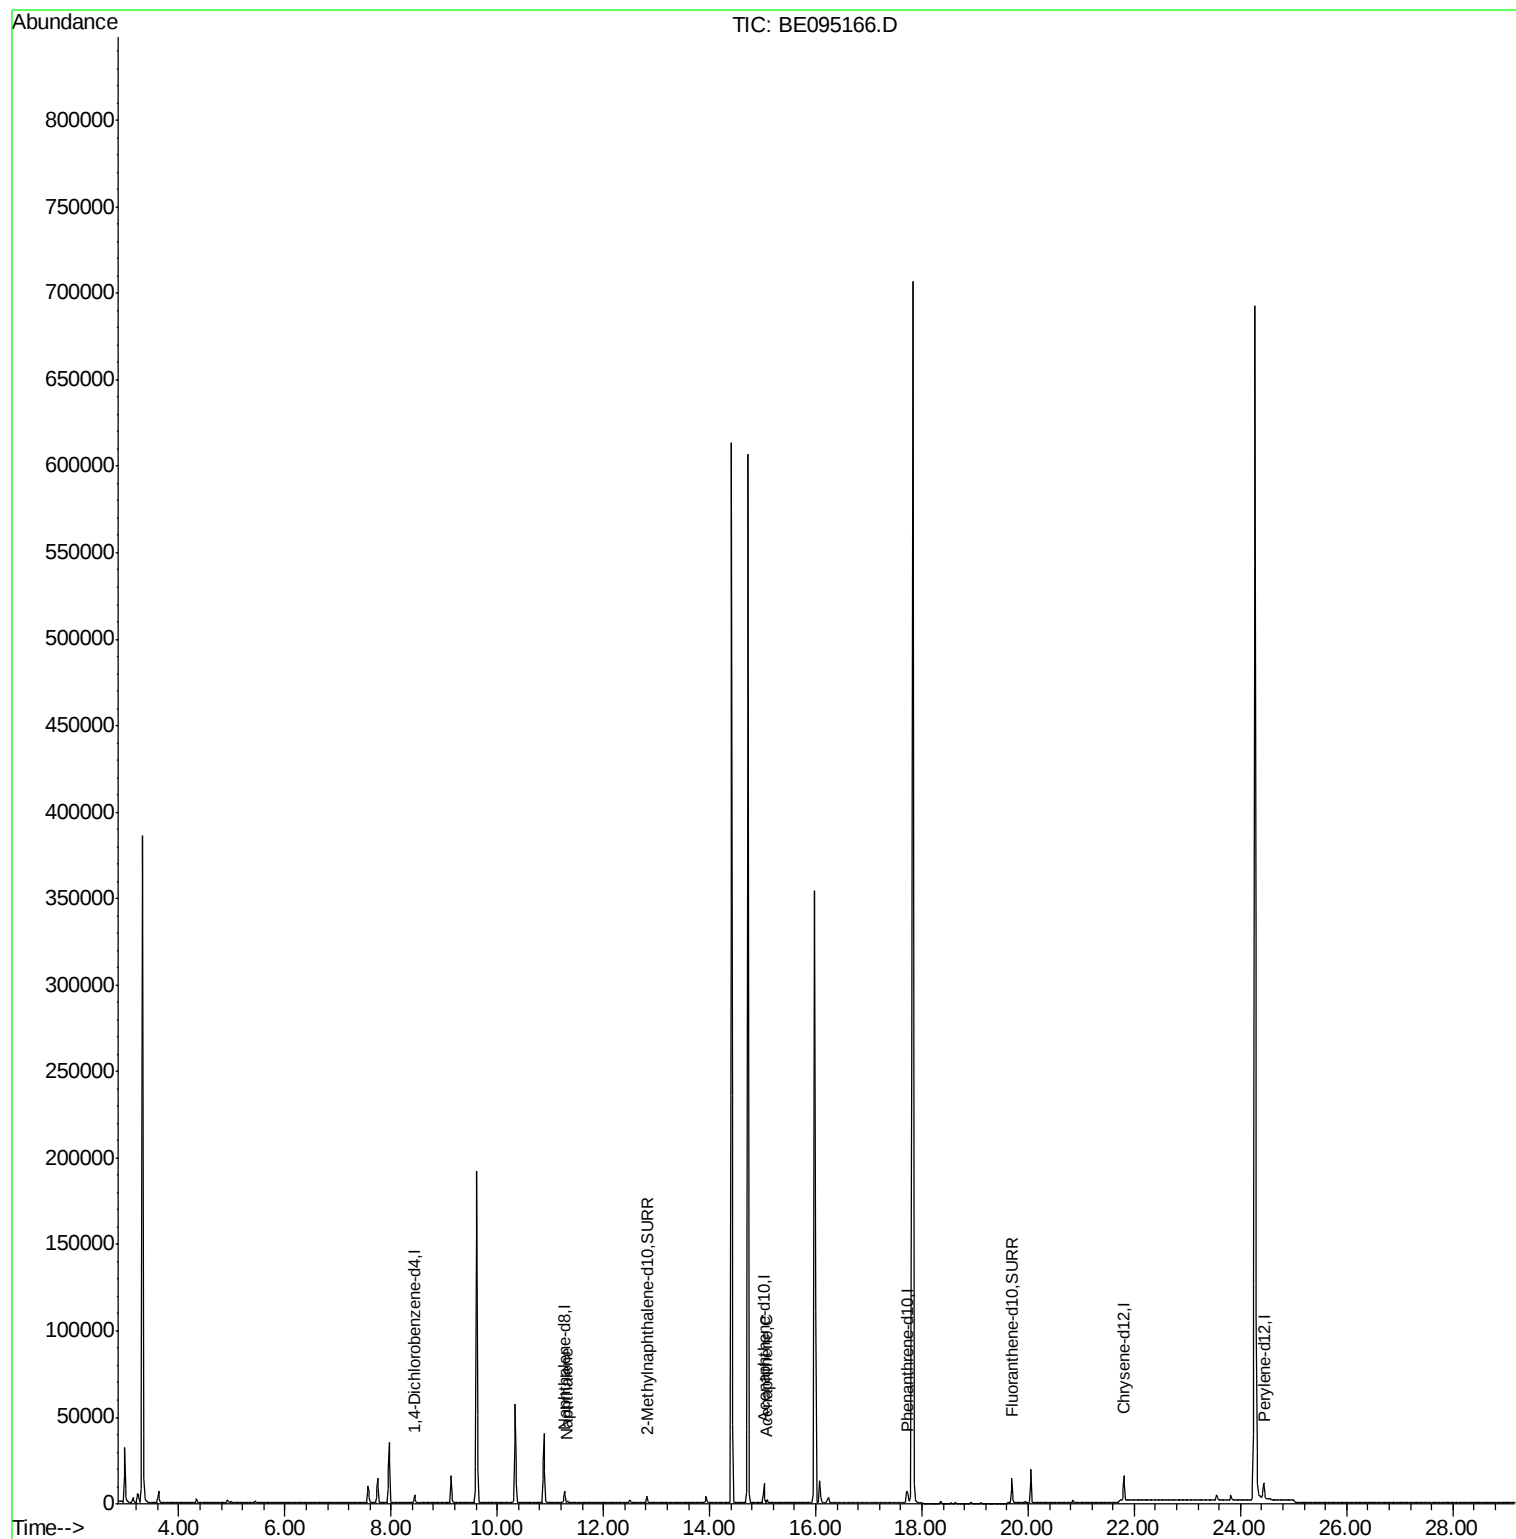

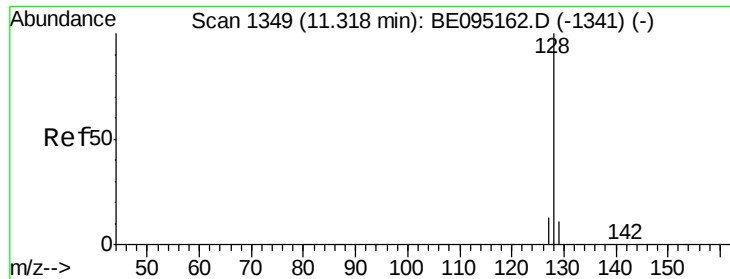

#3

Naphthalene

Concen: 0.038 ng/ul

RT: 11.32 min Scan# 1349

Delta R.T. -0.00 min

Lab File: BE095166.D

Acq: 27 Jan 2018 14:47

Instrument :

BNA_E

ClientSampleId :


F6D45

Tot Ion:	128	Resp:	993
Ion Ratio	Lower	Upper	
128	100		
129	20.6	11.3	16.9#
127	20.3	4.0	6.0#


Manual Integrations
APPROVED

Sohil



1/29/2018 6:19:58 PM

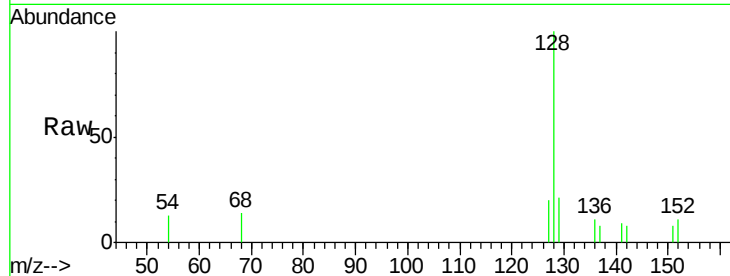

Abundance Ion 128.00 (127.70 to 128.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 127.00 (126.70 to 127.70): E

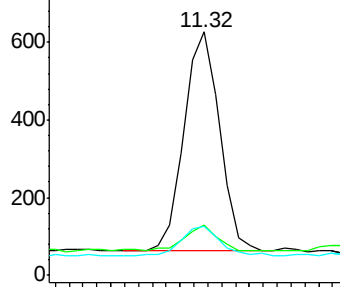

Time-->

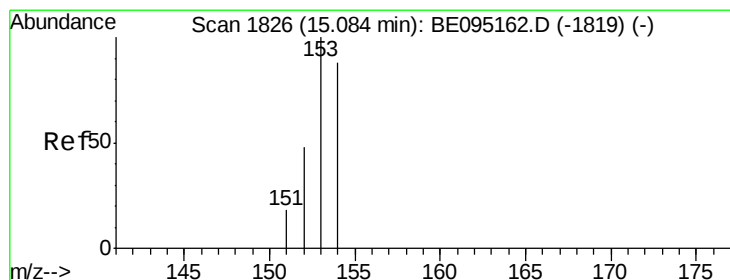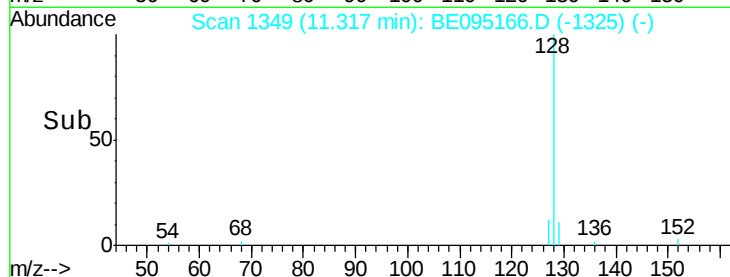

#8

Acenaphthene

Concen: 0.104 ng/ul


RT: 15.08 min Scan# 1825

Delta R.T. -0.00 min


Lab File: BE095166.D

Acq: 27 Jan 2018 14:47

Tgt Ion:	153	Resp:	2414
Ion Ratio	Lower	Upper	
153	100		
152	5.0	36.0	54.0#
154	12.5	72.0	108.0#

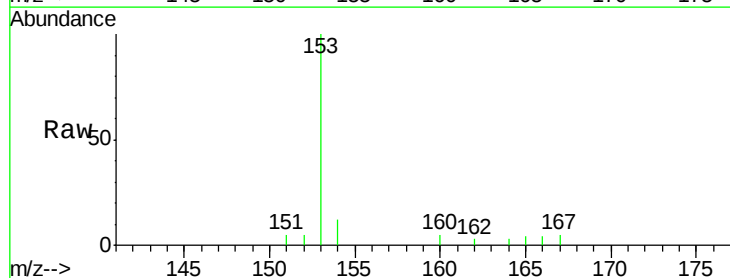

Abundance Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E
Ion 154.00 (153.70 to 154.70): E

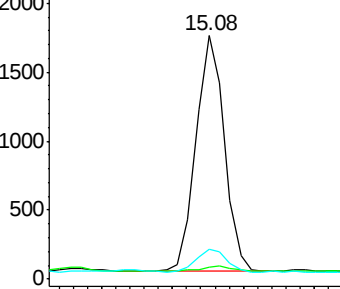

Time-->

