

Data Path : Z:\HPCHEM1\BNA E\DATA\BE012718\
 Data File : BE095168.D
 Acq On : 27 Jan 2018 15:59
 Operator : SJ/JU
 Sample : J1221-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6D43

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:20:01 PM

Quant Time: Jan 28 02:03:37 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 27 03:18:43 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2812	0.40	ng/ul	0.00
2) Naphthalene-d8	11.27	136	8730	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	5908	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.73	188	12104m	0.40	ng/ul	0.02
16) Chrysene-d12	21.80	240	12848	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	11438m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.82	152	5234	0.37	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	15621	0.34	ng/ul	0.00
Target Compounds						
3) Naphthalene	11.32	128	682	0.028	ng/ul#	68
8) Acenaphthene	15.08	153	2745	0.124	ng/ul#	24

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA E\DATA\BE012718\
Data File : BE095168.D
Acq On : 27 Jan 2018 15:59
Operator : SJ/JU
Sample : J1221-04
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
F6D43

Manual Integrations
APPROVED

Sohil
1/29/2018 6:20:01 PM

Quant Time: Jan 28 02:03:37 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 03:18:43 2018
Response via : Initial Calibration

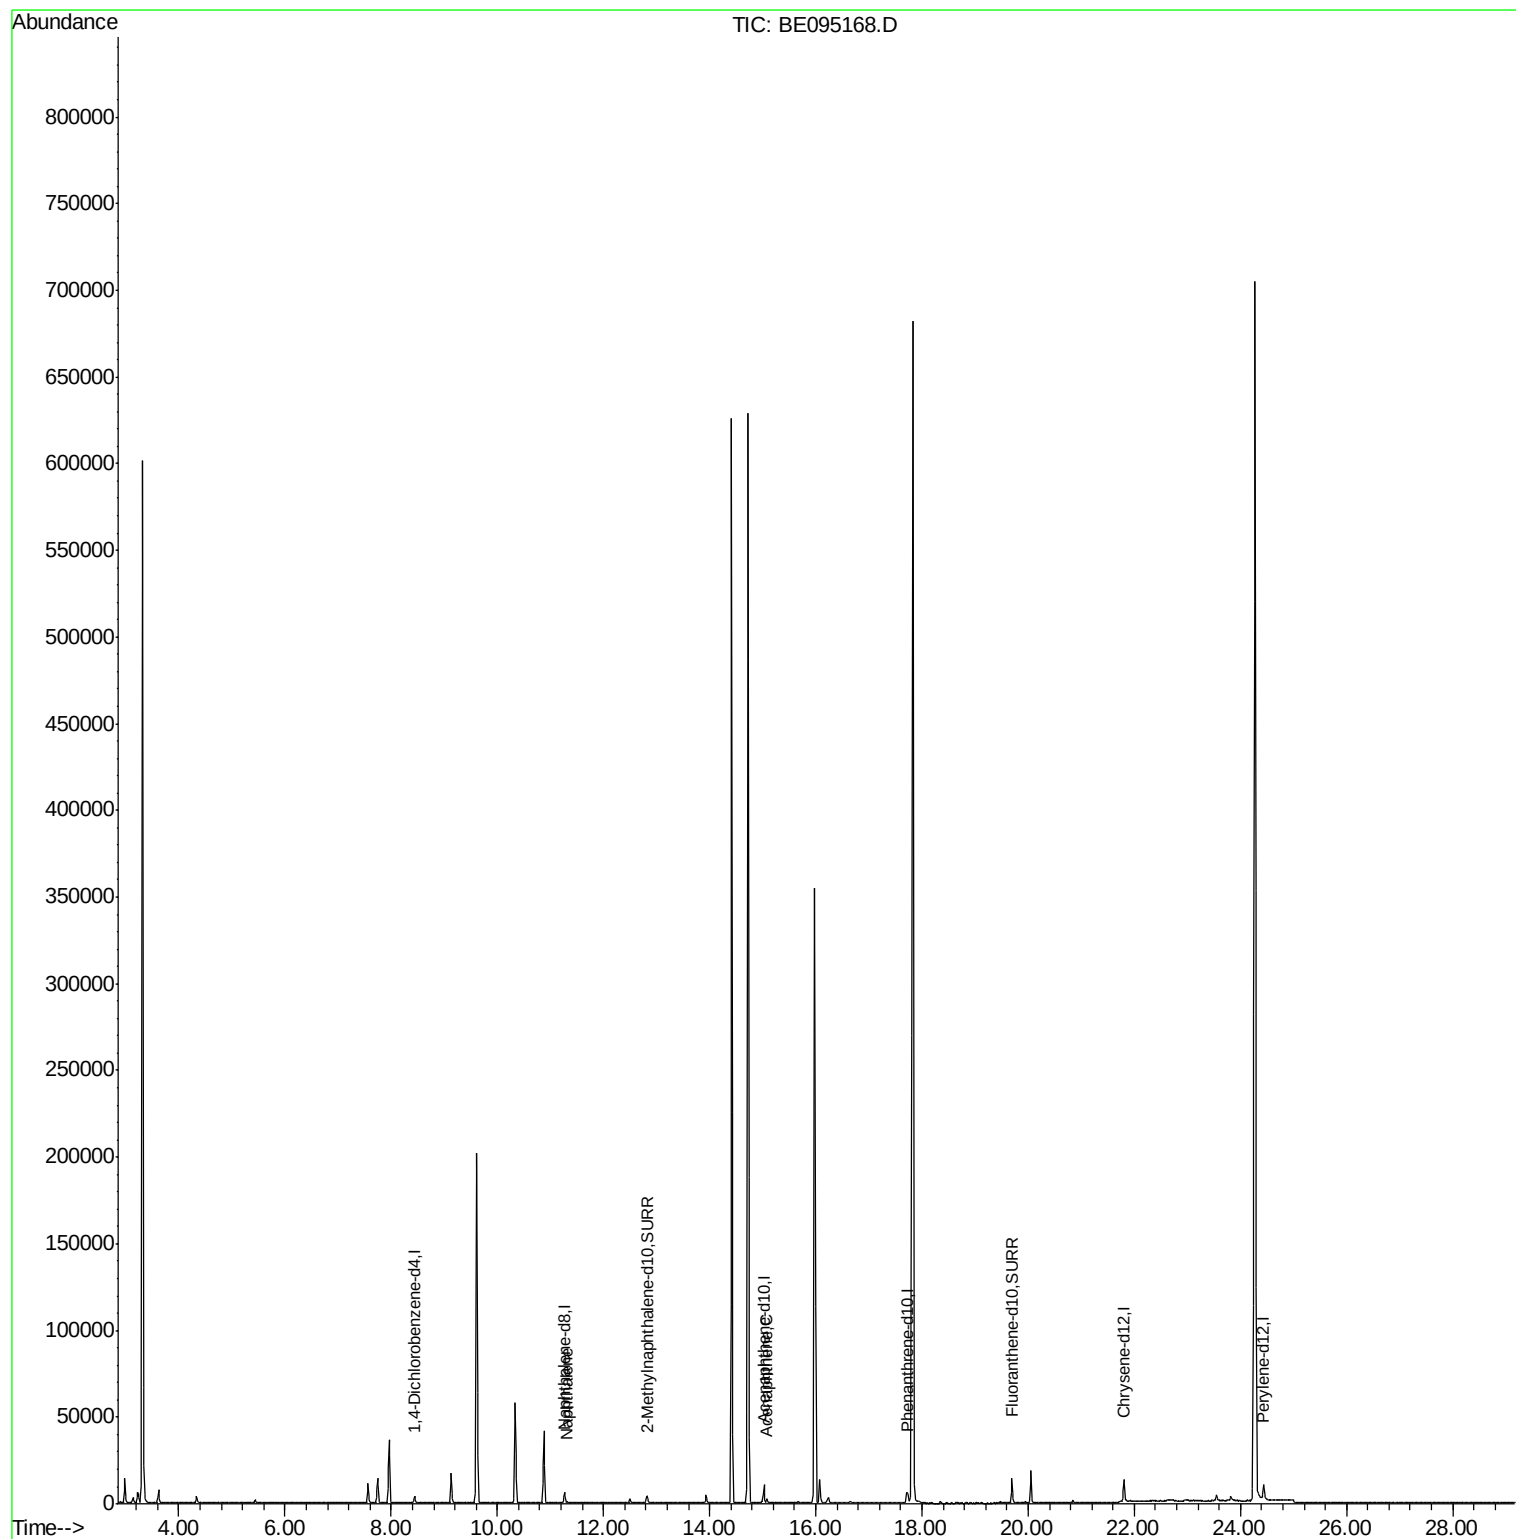

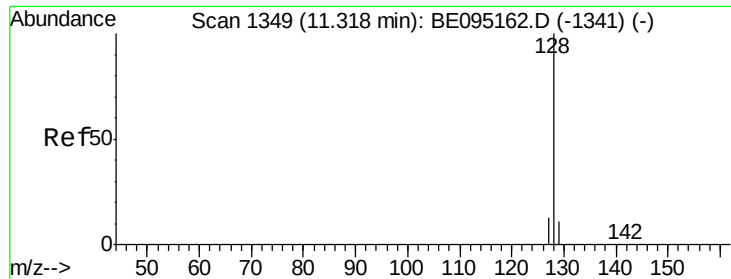

#3

Naphthalene

Concen: 0.028 ng/ul

RT: 11.32 min Scan# 1349

Delta R.T. 0.00 min

Lab File: BE095168.D

Acq: 27 Jan 2018 15:59

Instrument :

BNA_E





ClientSampleId :

F6D43

Tot Ion:128	Resp:	682
Ion Ratio	Lower	Upper
128	100	
129	23.3	11.3 16.9#
127	24.4	4.0 6.0#

Manual Integrations
APPROVED

Sohil
1/29/2018 6:20:01 PM

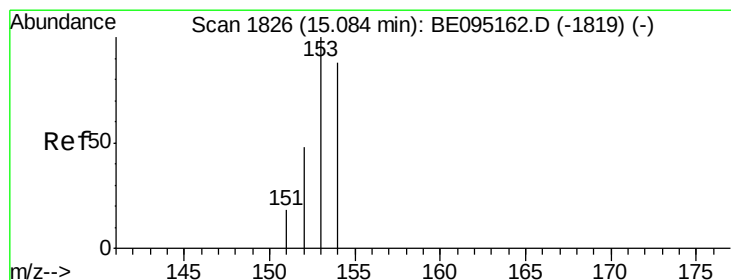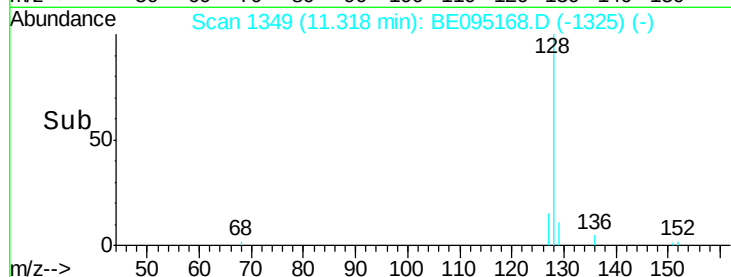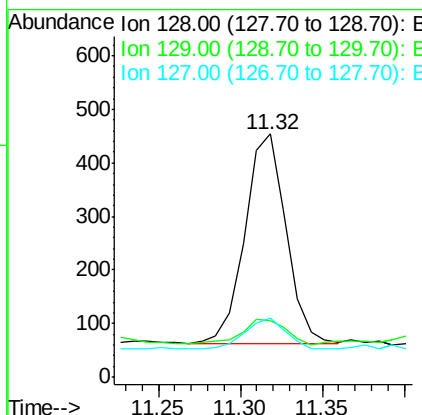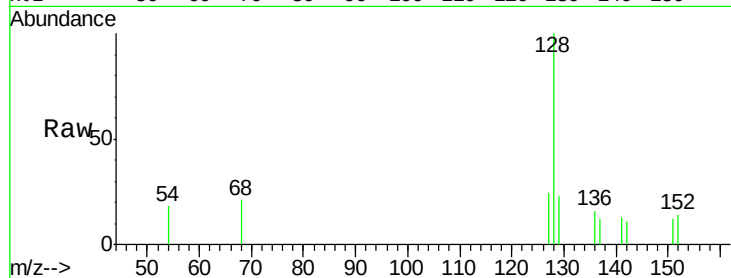

#8

Acenaphthene

Concen: 0.124 ng/ul

RT: 15.08 min Scan# 1825

Delta R.T. 0.00 min

Lab File: BE095168.D

Acq: 27 Jan 2018 15:59

Tgt Ion:153	Resp:	2745
Ion Ratio	Lower	Upper
153	100	
152	4.7	36.0 54.0#
154	12.0	72.0 108.0#

