

Data Path : Z:\HPCHEM1\BNA E\DATA\BE012718\
 Data File : BE095201.D
 Acq On : 28 Jan 2018 11:41
 Operator : SJ/JU
 Sample : J1174-07DL 5X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6A57DL

Manual Integrations
 APPROVED

Sohil
 1/29/2018 6:22:50 PM

Quant Time: Jan 29 01:42:54 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 29 01:25:04 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	3090	0.40	ng/ul	0.00
2) Naphthalene-d8	11.27	136	9931	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	6393	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	13359	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	14271	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	14465	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.82	152	1916	0.12	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	5370	0.11	ng/ul	0.00
Target Compounds				Ovalue		
3) Naphthalene	11.32	128	7089	0.255	ng/ul#	89
5) 2-Methylnaphthalene	12.89	142	9634	0.519	ng/ul	99
8) Acenaphthene	15.08	153	1396	0.059	ng/ul	92
9) Fluorene	16.02	166	814	0.033	ng/ul#	68
11) Pentachlorophenol	17.36	266	5949	2.299	ng/ul	95
12) Phenanthrene	17.75	178	2831	0.063	ng/ul#	89
15) Fluoranthene	19.72	202	2050	0.035	ng/ul	86
17) Pyrene	20.08	202	1240m	0.026	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA E\DATA\BE012718\
Data File : BE095201.D
Acq On : 28 Jan 2018 11:41
Operator : SJ/JU
Sample : J1174-07DL 5X
Misc :
ALS Vial : 40 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
F6A57DL

Manual Integrations
APPROVED

Sohil
1/29/2018 6:22:50 PM

Quant Time: Jan 29 01:42:54 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 29 01:25:04 2018
Response via : Initial Calibration

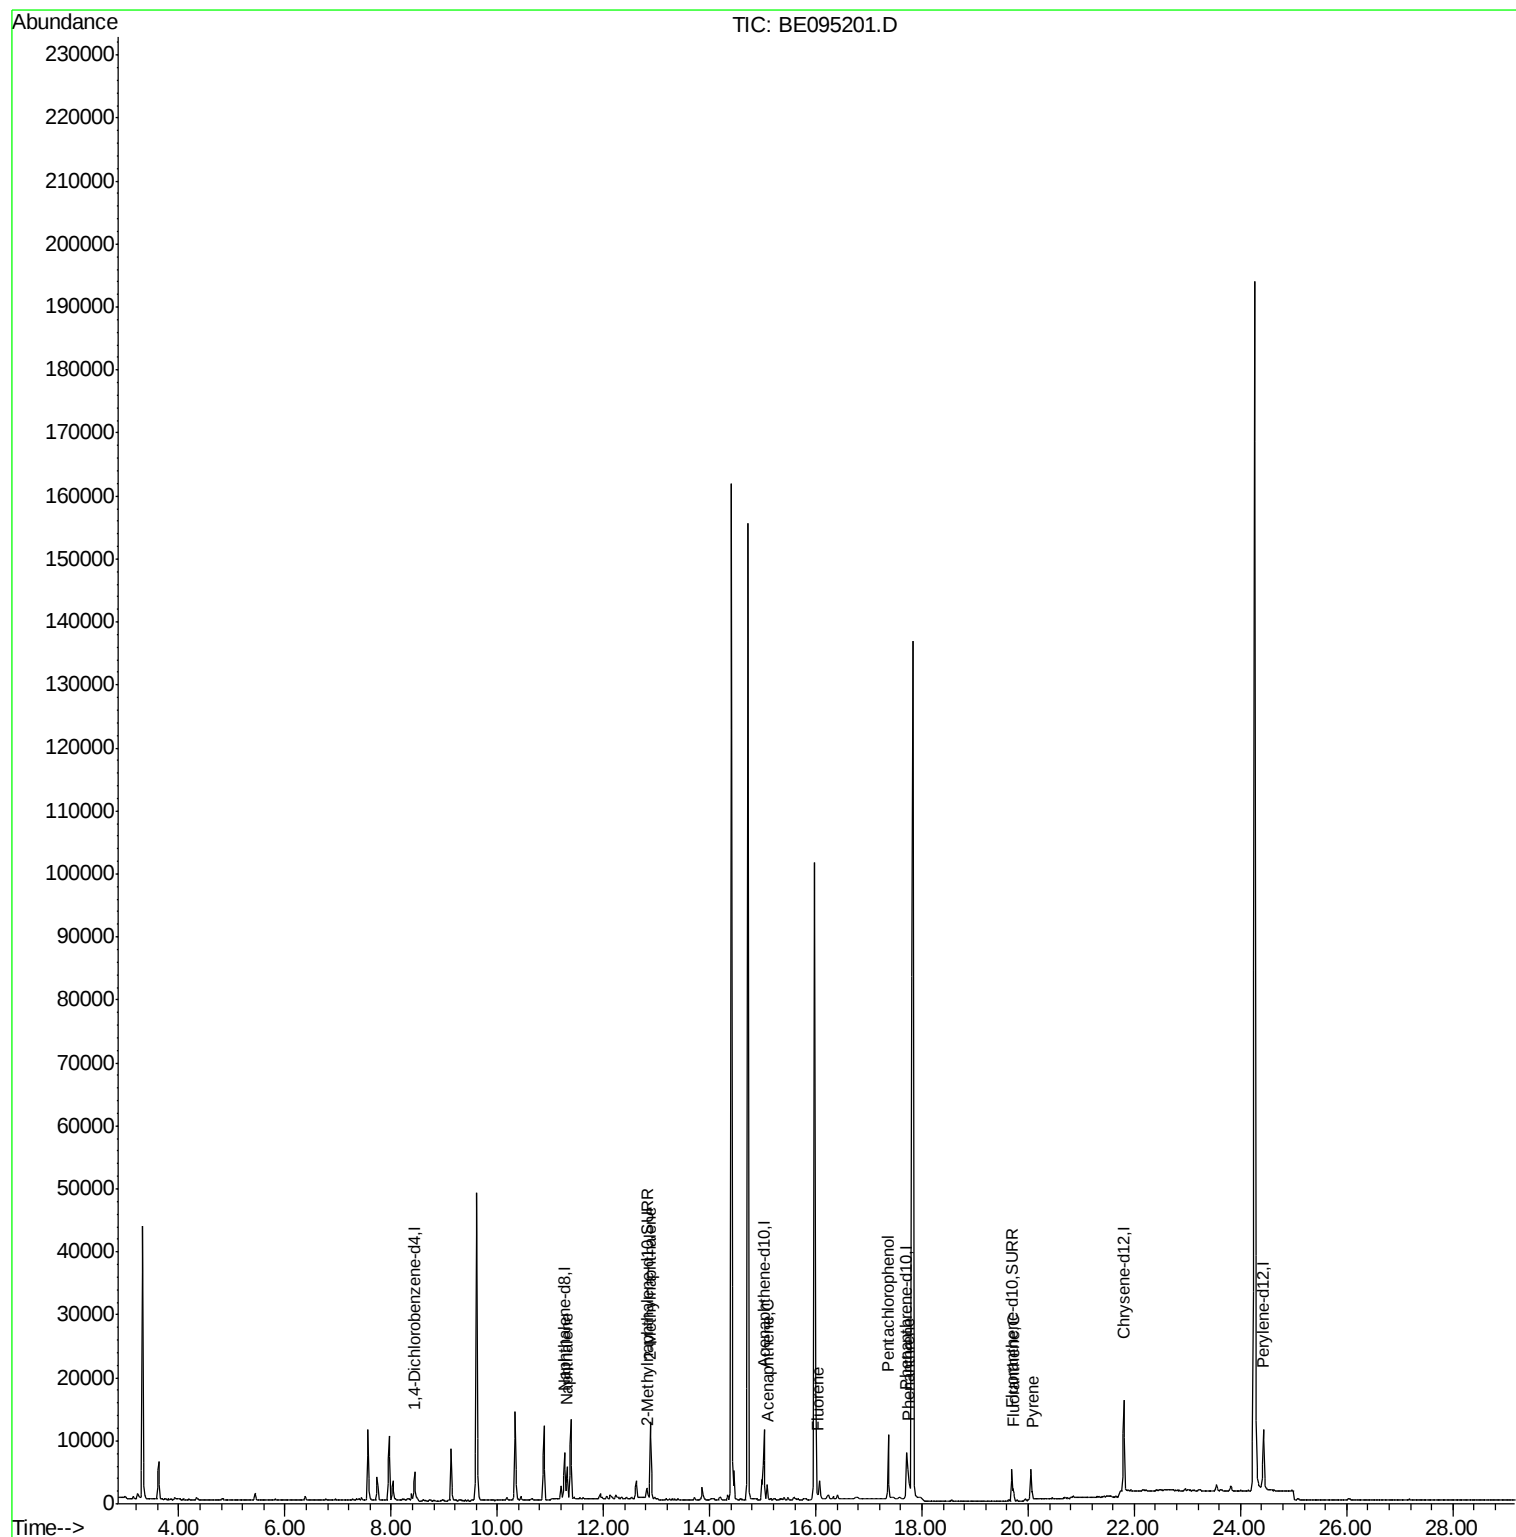

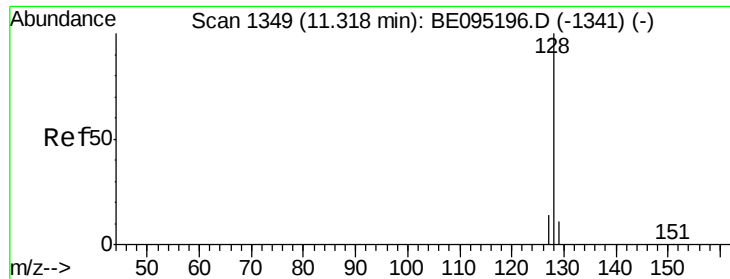

#3

Naphthalene

Concen: 0.255 ng/ul

RT: 11.32 min Scan# 1349

Delta R.T. -0.00 min

Lab File: BE095201.D

Acq: 28 Jan 2018 11:41

Instrument :

BNA_E





ClientSampled :

F6A57DL

Tot Ion:128	Resp:	7089
Ion Ratio	Lower	Upper
128	100	
129	12.6	11.3 16.9
127	15.2	4.0 6.0#

Manual Integrations
APPROVED

Sohil
1/29/2018 6:22:50 PM

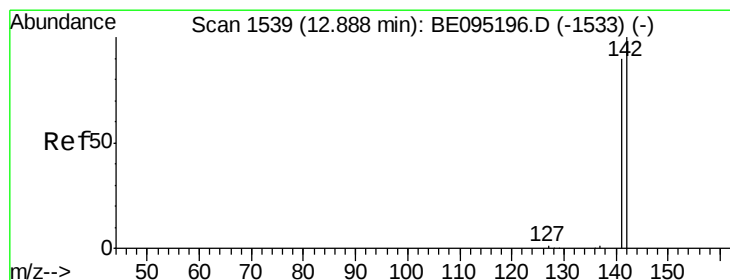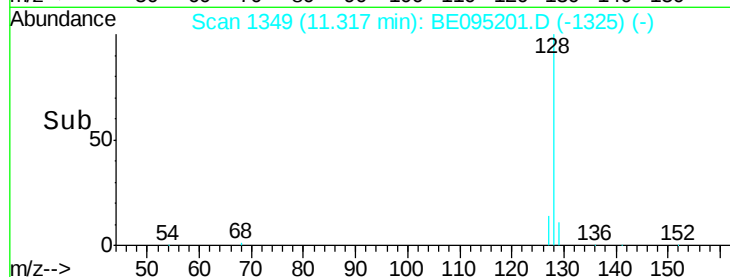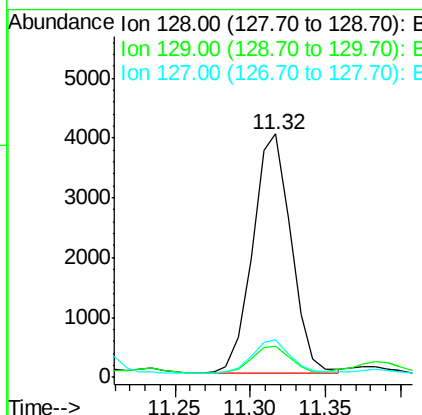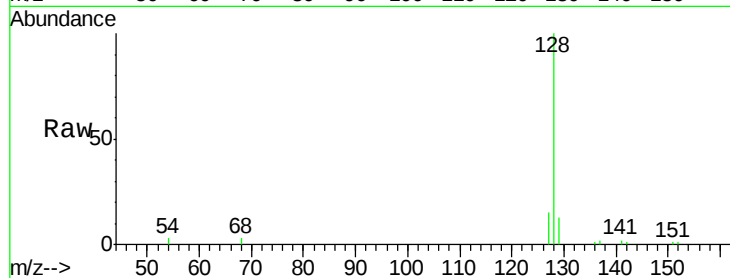

#5

2-Methylnaphthalene

Concen: 0.519 ng/ul




RT: 12.89 min Scan# 1539


Delta R.T. -0.00 min

Lab File: BE095201.D

Acq: 28 Jan 2018 11:41

Tgt Ion:142	Resp:	9634
Ion Ratio	Lower	Upper
142	100	
141	91.8	72.6 108.8

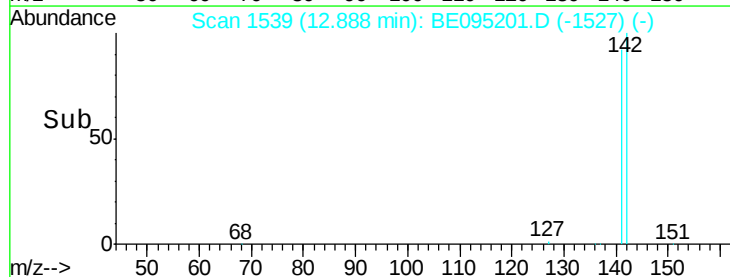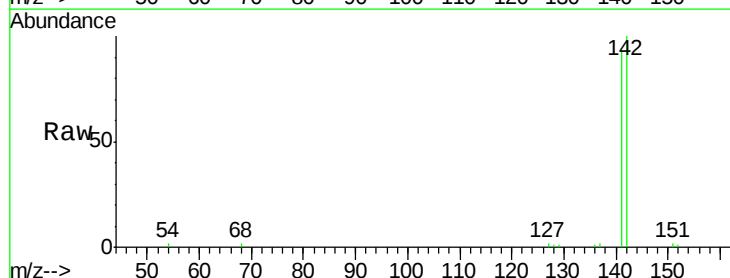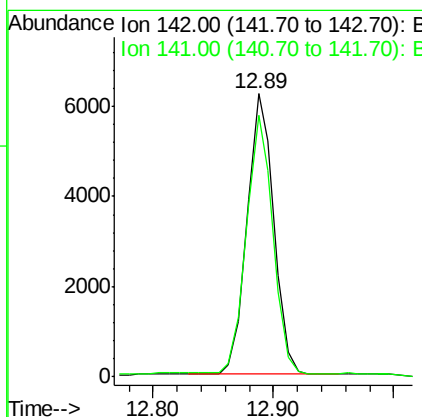

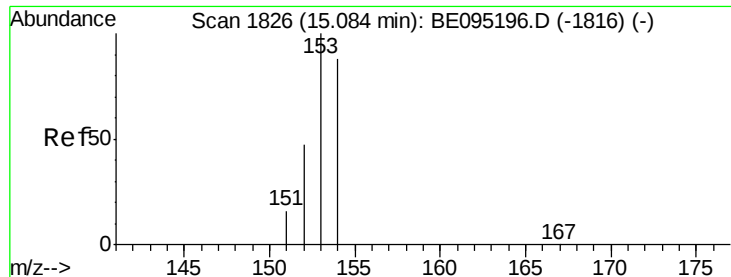

#8

Acenaphthene

Concen: 0.059 ng/ul

RT: 15.08 min Scan# 1826

Delta R.T. -0.00 min

Lab File: BE095201.D

Acq: 28 Jan 2018 11:41

Instrument :

BNA_E





ClientSampled :

F6A57DL

Tot Ion:	153	Resp:	1396
Ion Ratio	Lower	Upper	
153	100		
152	53.8	36.0	54.0
154	85.1	72.0	108.0

Manual Integrations
APPROVED

Sohil
1/29/2018 6:22:50 PM

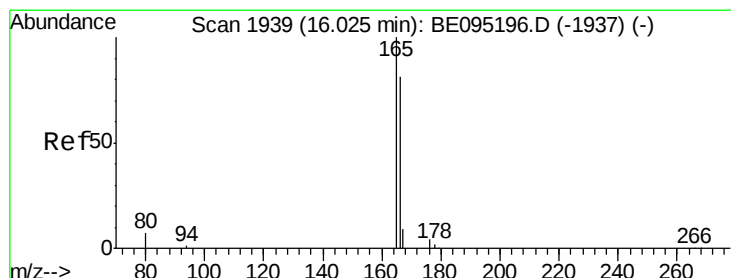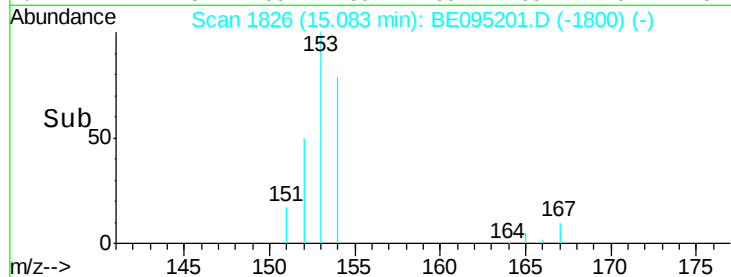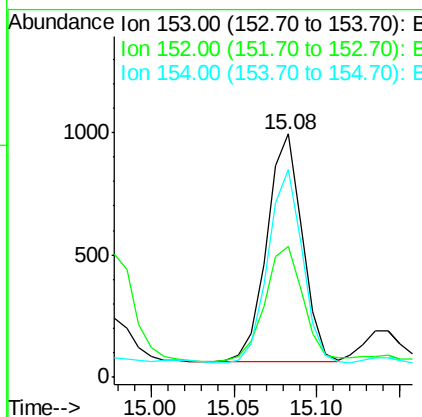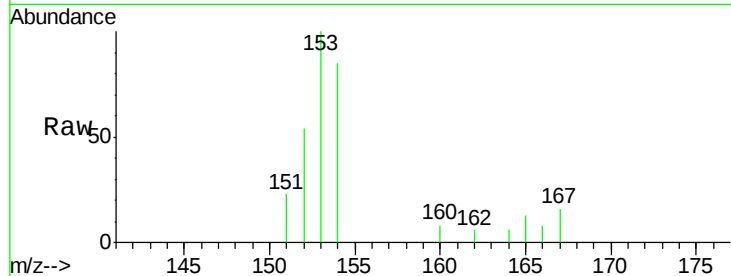

#9

Fluorene

Concen: 0.033 ng/ul




RT: 16.02 min Scan# 1939


Delta R.T. -0.00 min

Lab File: BE095201.D

Acq: 28 Jan 2018 11:41

Tgt Ion:	166	Resp:	814
Ion Ratio	Lower	Upper	
166	100		
165	123.2	73.4	110.2#
167	29.9	14.6	22.0#

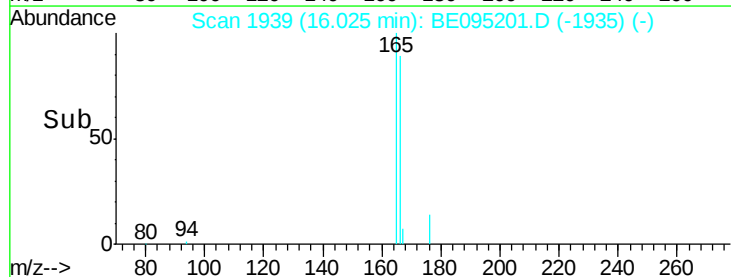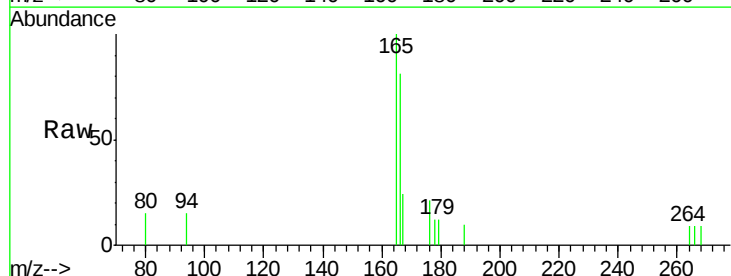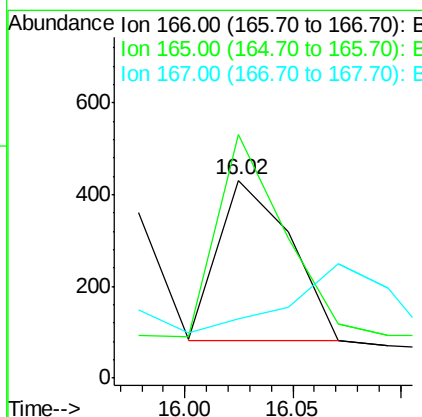

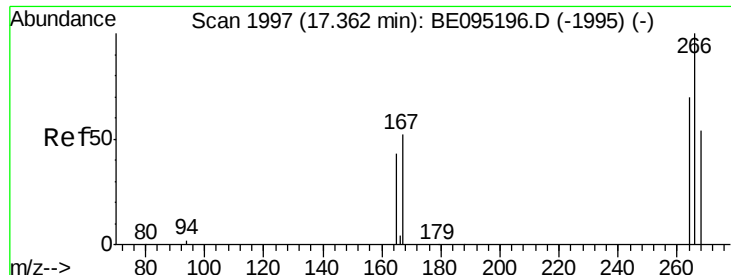





#11
 Pentachlorophenol
 Concen: 2.299 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. -0.00 min
 Lab File: BE095201.D
 Acq: 28 Jan 2018 11:41

Instrument :
 BNA_E
 ClientSampled :
 F6A57DL

Tot Ion	Ratio	Lower	Upper
266	100		
264	65.4	47.9	71.9
268	60.1	49.8	74.8




Manual Integrations
 APPROVED


Sohil
 1/29/2018 6:22:50 PM

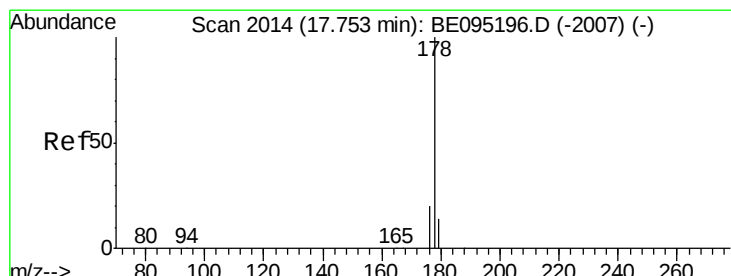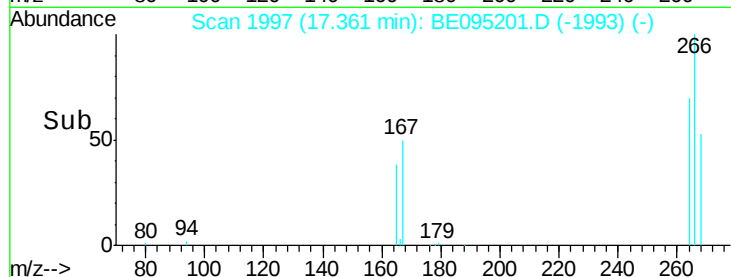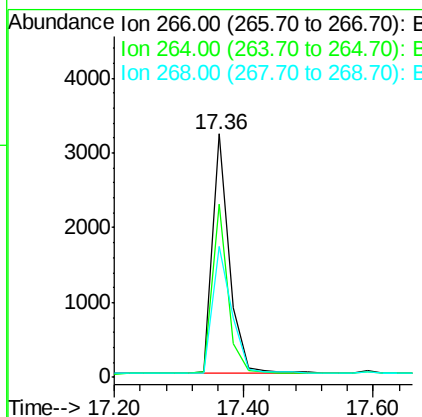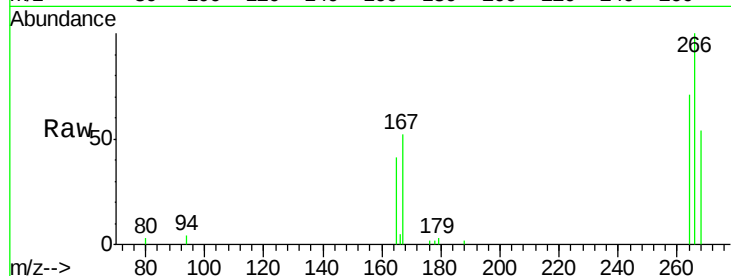

#12
 Phenanthrene
 Concen: 0.063 ng/ul
 RT: 17.75 min Scan# 2014
 Delta R.T. -0.00 min
 Lab File: BE095201.D
 Acq: 28 Jan 2018 11:41

Tgt Ion	Ratio	Lower	Upper
178	100		
179	18.3	18.4	27.6#
176	22.4	13.6	20.4#

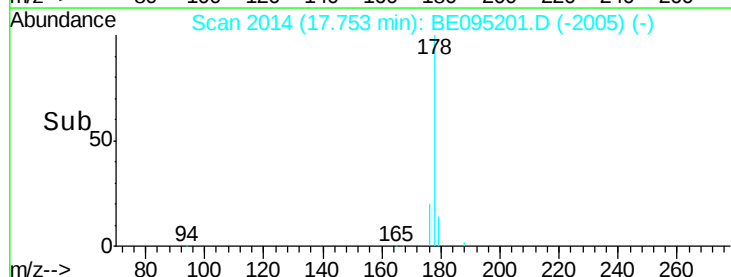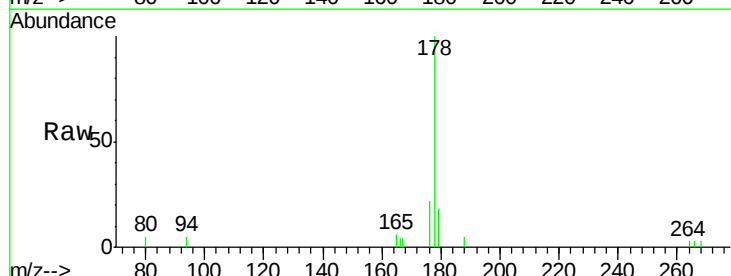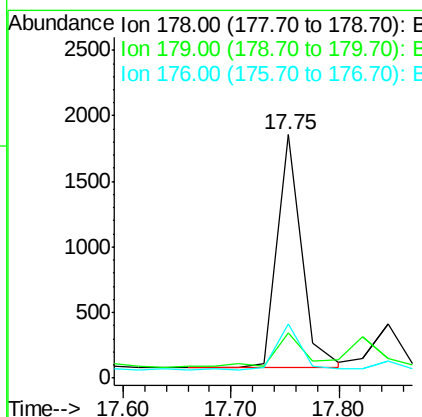

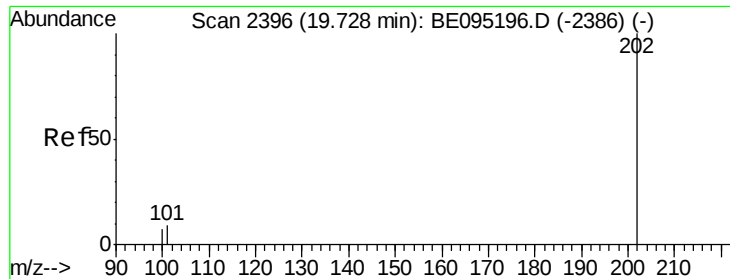





#15
Fluoranthene
Concen: 0.035 ng/ul
RT: 19.72 min Scan# 2395
Delta R.T. -0.00 min
Lab File: BE095201.D
Acq: 28 Jan 2018 11:41

Instrument :
BNA_E
ClientSampleId :
F6A57DL

Tot Ion	Ratio	Lower	Upper
202	100		
101	14.2	0.0	30.3
100	12.0	0.0	39.5

Manual Integrations
APPROVED

Sohil
1/29/2018 6:22:50 PM

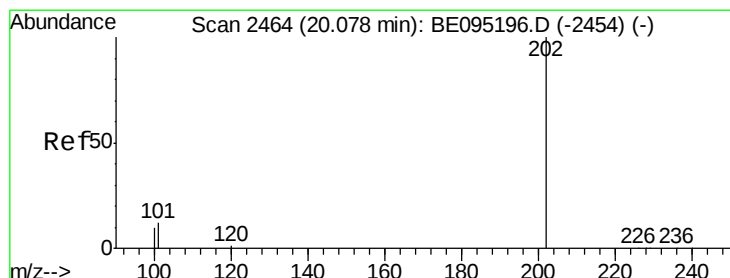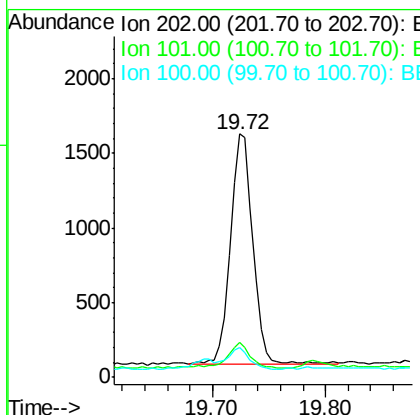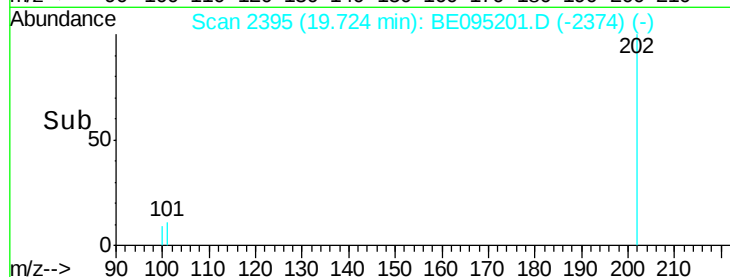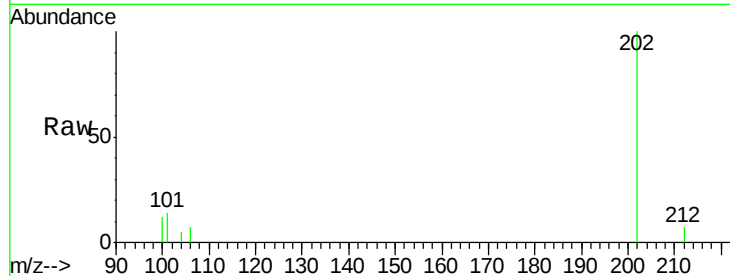

#17
Pyrene
Concen: 0.026 ng/ul m
RT: 20.08 min Scan# 2464
Delta R.T. -0.00 min
Lab File: BE095201.D
Acq: 28 Jan 2018 11:41

Tgt Ion	Ratio	Lower	Upper
202	100		
101	17.5	18.2	27.4#
100	17.2	15.6	23.4

