

Data Path : Z:\HPCHEM1\BNA_E\Data\BE012815\
 Data File : BE089407.D
 Acq On : 29 Jan 2015 3:02
 Operator : TP/IZ
 Sample : SSTDCCC001
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTDCCC001

Quant Time: Jan 29 05:35:55 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-BE012815.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 29 04:21:19 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.58	152	134351	5.00	ng	0.00
7) Naphthalene-d8	12.50	136	469028	5.00	ng	0.00
13) Acenaphthene-d10	12.21	164	13436	5.00	ng	0.00
17) Phenanthrene-d10	19.99	188	371458	5.00	ng	0.00
20) Chrysene-d12	23.84	240	476823	5.00	ng	0.00
27) Perylene-d12	25.55	264	550235	5.00	ng	0.00

System Monitoring Compounds						
3) 2-Fluorophenol	6.74	112	40229	0.96	ng	0.00
4) Phenol-d6	8.85	99	49368	0.95	ng	0.01
8) Nitrobenzene-d5	10.85	82	31290	0.95	ng	0.00
14) 2,4,6-Tribromophenol	18.58	330	4222	0.37	ng	0.00
15) 2-Fluorobiphenyl	15.13	172	52862	0.37	ng	0.00
22) Terphenyl-d14	22.48	244	55510	1.05	ng	0.00


Target Compounds				Qvalue		
2) n-Nitrosodimethylamine	3.58	42	21949	0.91	ng	96
5) Phenol	8.87	94	52785	0.96	ng	# 78
6) bis(2-Chloroethyl)ether	9.06	93	38677	0.94	ng	# 99
9) Nitrobenzene	10.89	77	35361	0.95	ng	99
10) 2,4-Dimethylphenol	11.82	122	27856	0.98	ng	91
11) 2,4-Dichlorophenol	12.21	162	21203	0.97	ng	92
12) Hexachlorobutadiene	12.89	225	14188	0.91	ng	99
16) 2,4-Dinitrophenol	16.90	184	674	0.96	ng	89
18) Hexachlorobenzene	19.23	284	15782	0.92	ng	98
19) Pentachlorophenol	19.65	266	2588	0.78	ng	97
21) Benzidine	22.14	184	45101	0.80	ng	99
23) Benzo(a)anthracene	23.83	228	461240	1.04	ng	100
24) 3,3'-Dichlorobenzidine	23.81	252	42751	1.22	ng	97
25) Chrysene	23.87	228	504799	0.93	ng	99
26) Indeno(1,2,3-cd)pyrene	27.06	276	145951	1.16	ng	# 100
28) Benzo(b)fluoranthene	25.10	252	93925	1.30	ng	98
29) Benzo(k)fluoranthene	25.13	252	162986	0.93	ng	99
30) Benzo(a)pyrene	25.48	252	103428	1.22	ng	99
31) Dibenzo(a,h)anthracene	27.09	278	112829	1.25	ng	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\Data\BE012815\
Data File : BE089407.D
Acq On : 29 Jan 2015 3:02
Operator : TP/IZ
Sample : SSTDCCC001
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SSTDCCC001

Quant Time: Jan 29 05:35:55 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-BE012815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 29 04:21:19 2015
Response via : Initial Calibration

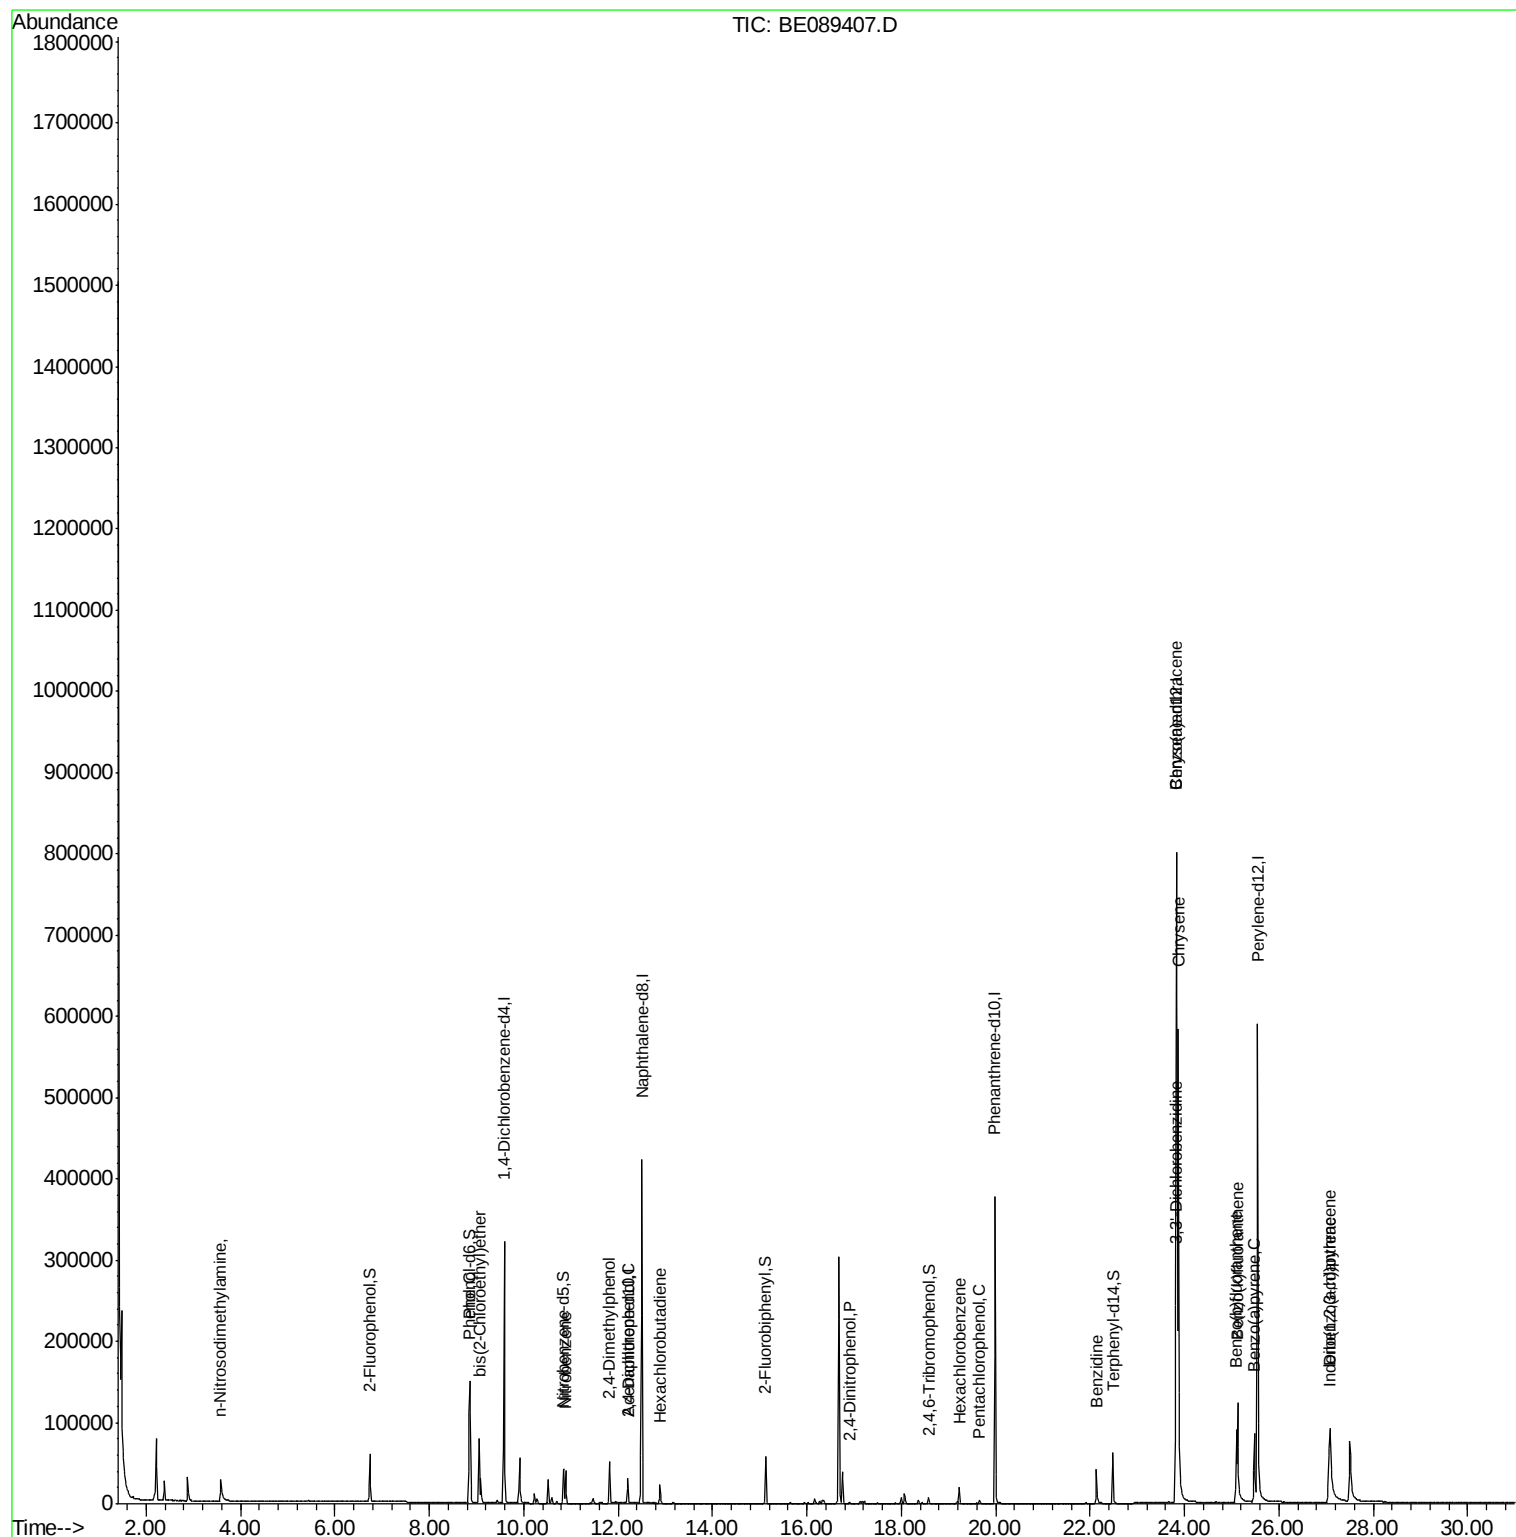

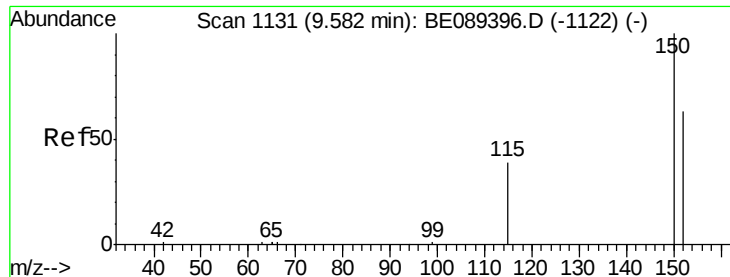

#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 9.58 min Scan# 1131

Delta R.T. 0.00 min

Lab File: BE089407.D

Acq: 29 Jan 2015 3:02

Instrument :

BNA_E

ClientSampleId :

SSTDCCC001


Tgt Ion:152 Resp: 134351

Ion Ratio Lower Upper

152 100

150 156.0 127.2 190.8




115 60.9 49.3 73.9

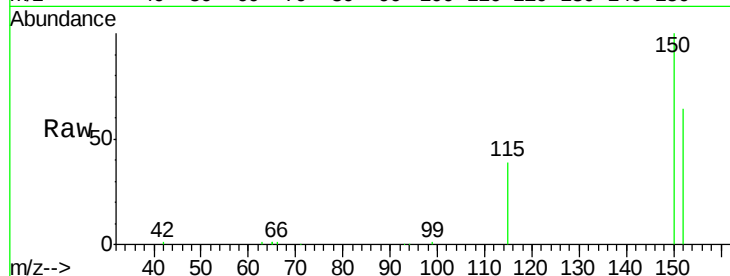

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

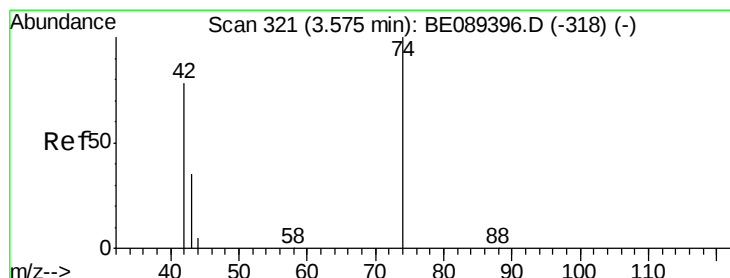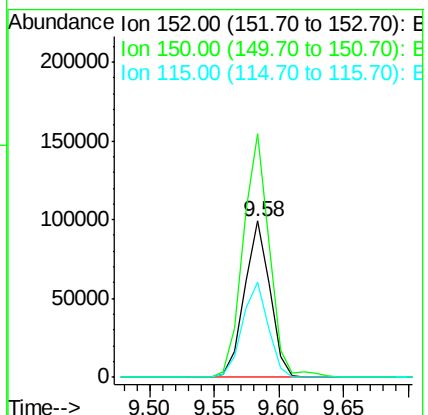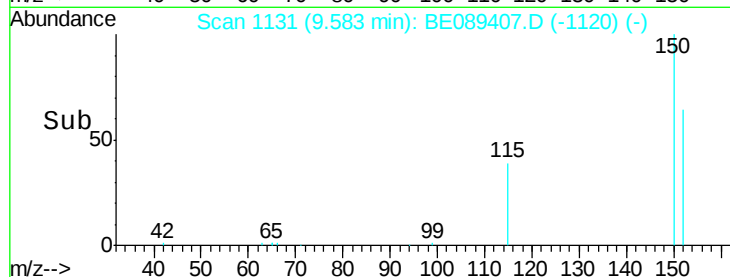

#2

n-Nitrosodimethylamine

Concen: 0.91 ng

RT: 3.58 min Scan# 321

Delta R.T. 0.00 min

Lab File: BE089407.D

Acq: 29 Jan 2015 3:02


Tgt Ion: 42 Resp: 21949

Ion Ratio Lower Upper

42 100

74 121.4 101.2 151.8



44 32.6 26.4 39.6

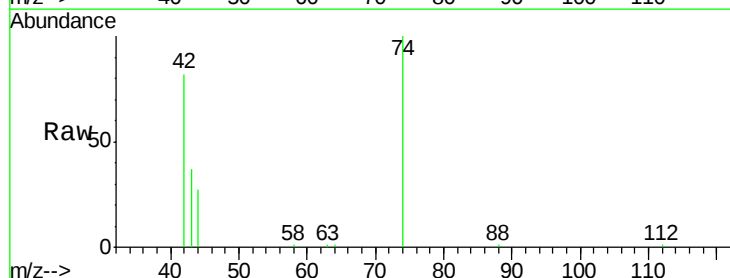


Abundance Ion 42.00 (41.70 to 42.70): BE0

Ion 74.00 (73.70 to 74.70): BE0

Ion 44.00 (43.70 to 44.70): BE0

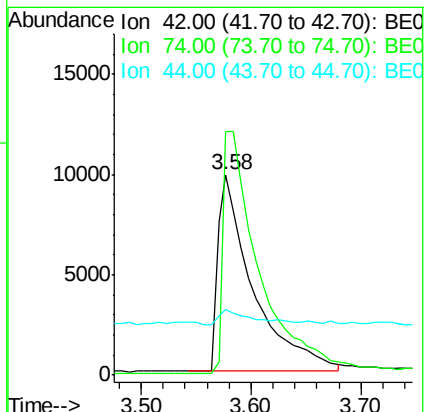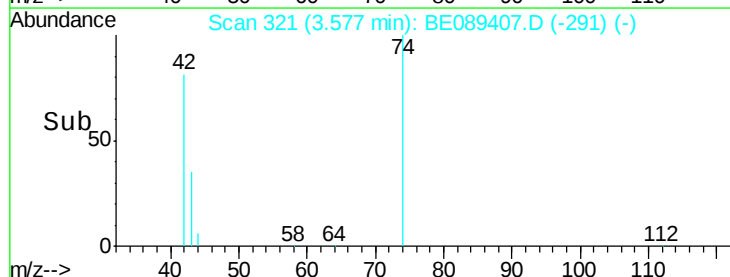


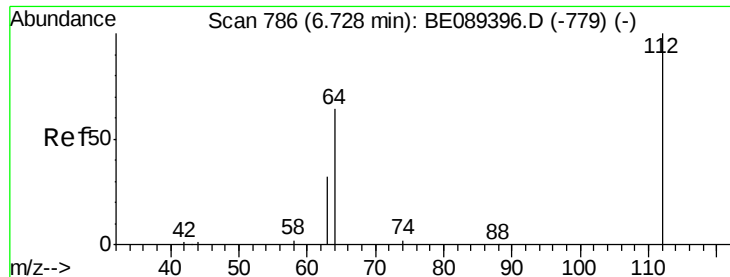




#3
 2-Fluorophenol
 Concen: 0.96 ng
 RT: 6.74 min Scan# 787
 Delta R.T. 0.01 min
 Lab File: BE089407.D
 Acq: 29 Jan 2015 3:02

Instrument :
 BNA_E
 ClientSampleId :
 SSTDCCC001

Tgt Ion: 112 Resp: 40229
 Ion Ratio Lower Upper
 112 100
 64 62.4 51.7 77.5
 63 30.1 25.7 38.5

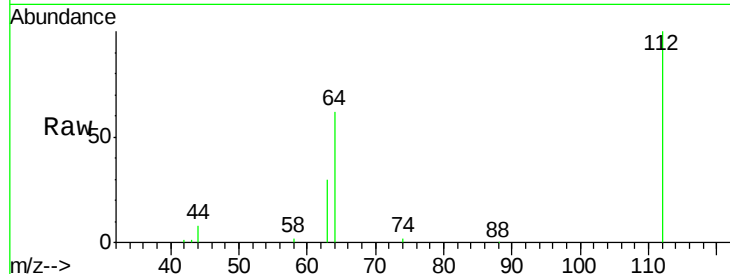


Abundance Ion 112.00 (111.70 to 112.70): BE0
 Ion 64.00 (63.70 to 64.70): BE0
 Ion 63.00 (62.70 to 63.70): BE0

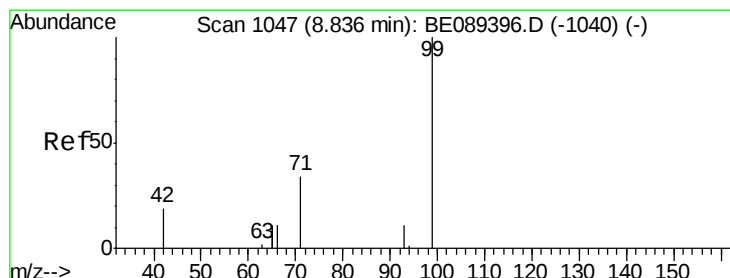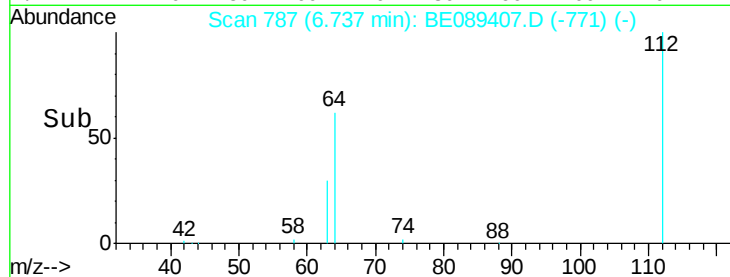
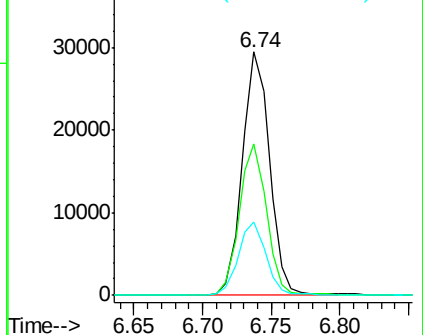



#4
 Phenol-d6
 Concen: 0.95 ng
 RT: 8.85 min Scan# 1048
 Delta R.T. 0.01 min
 Lab File: BE089407.D
 Acq: 29 Jan 2015 3:02

Tgt Ion: 99 Resp: 49368
 Ion Ratio Lower Upper
 99 100
 42 20.3 15.3 22.9
 71 33.6 27.0 40.6

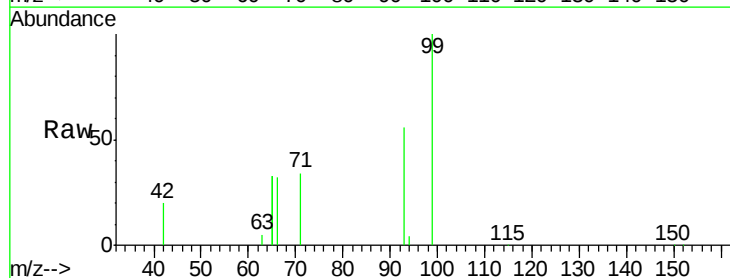

Abundance Ion 99.00 (98.70 to 99.70): BE0
 Ion 42.00 (41.70 to 42.70): BE0
 Ion 71.00 (70.70 to 71.70): BE0

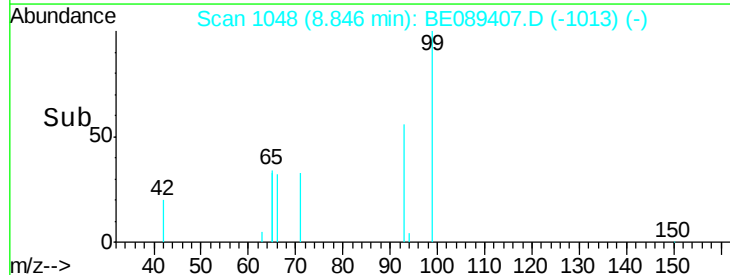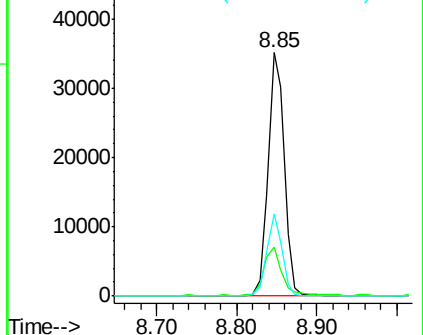

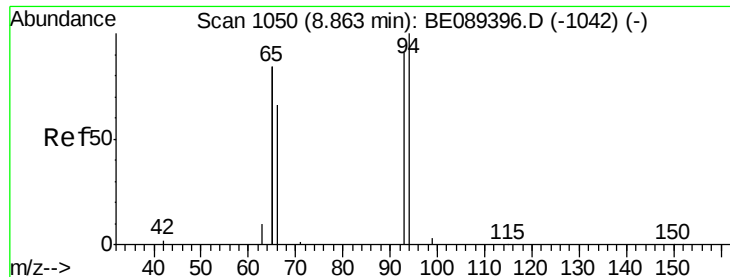

#5

Phenol

Concen: 0.96 ng

RT: 8.87 min Scan# 1051

Delta R.T. 0.01 min

Lab File: BE089407.D

Acq: 29 Jan 2015 3:02

Instrument :

BNA_E

ClientSampleId :

SSTDCCC001





Tgt Ion: 94 Resp: 52785

Ion Ratio Lower Upper

94 100

65 139.1 148.6 188.6#

66 48.8 46.2 86.2

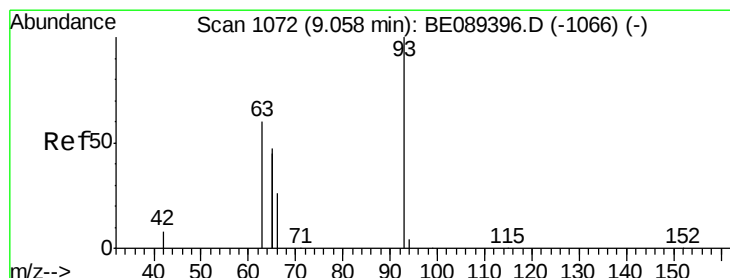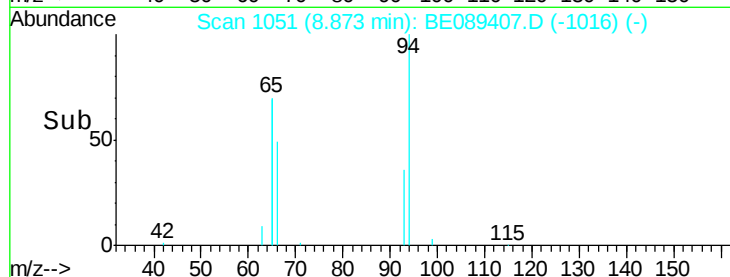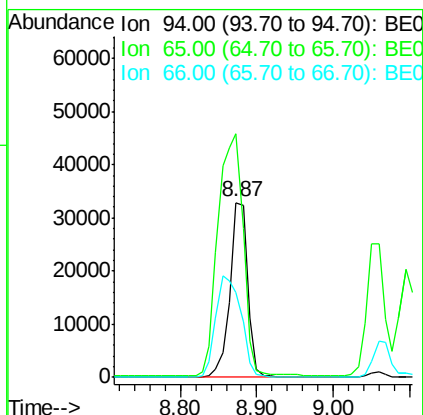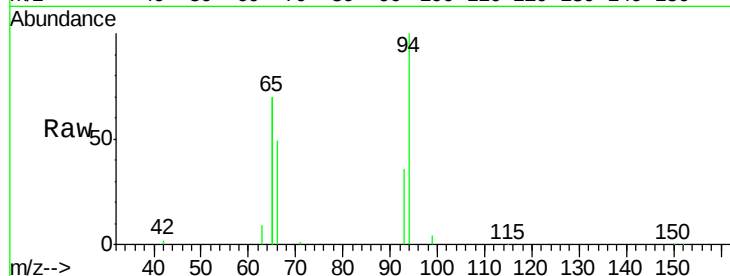

#6

bis(2-Chloroethyl)ether

Concen: 0.94 ng

RT: 9.06 min Scan# 1072

Delta R.T. 0.00 min

Lab File: BE089407.D

Acq: 29 Jan 2015 3:02




Tgt Ion: 93 Resp: 38677


Ion Ratio Lower Upper

93 100

63 72.8 58.9 88.3

95 0.0 0.0 0.0

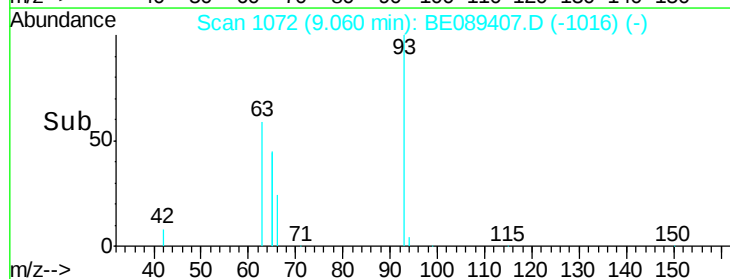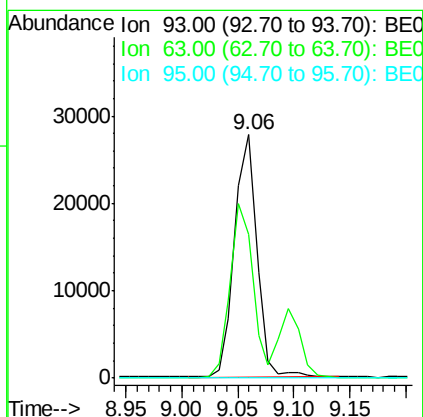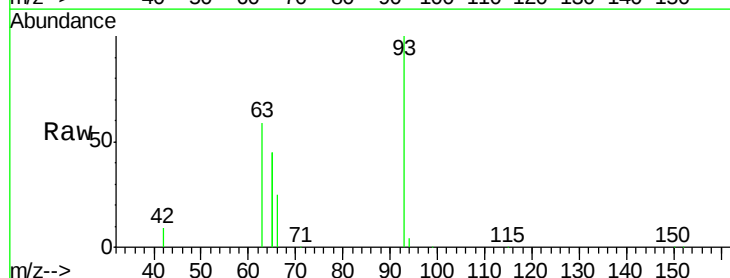



#7

Naphthalene-d8

Concen: 5.00 ng

RT: 12.50 min Scan# 1562

Delta R.T. 0.00 min

Lab File: BE089407.D

Acq: 29 Jan 2015 3:02

Instrument :

BNA_E

ClientSampleId :

SSTDCCC001


Tgt Ion: 136 Resp: 469028

Ion Ratio Lower Upper

136 100

137 10.9 8.7 13.1




54 9.1 7.4 11.0

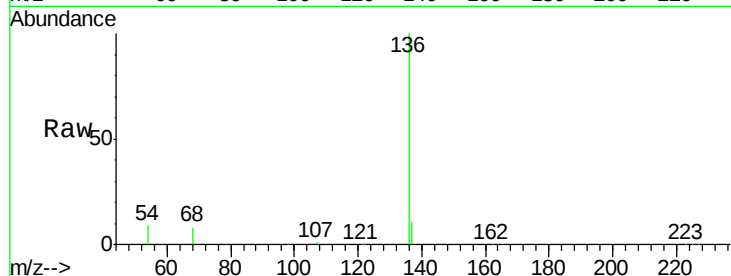

Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

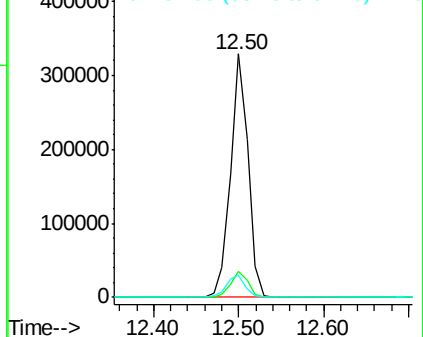

#8

Nitrobenzene-d5

Concen: 0.95 ng

RT: 10.85 min Scan# 1349

Delta R.T. 0.00 min

Lab File: BE089407.D

Acq: 29 Jan 2015 3:02


Tgt Ion: 82 Resp: 31290

Ion Ratio Lower Upper

82 100

128 42.9 33.6 50.4



54 45.6 37.7 56.5




Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0

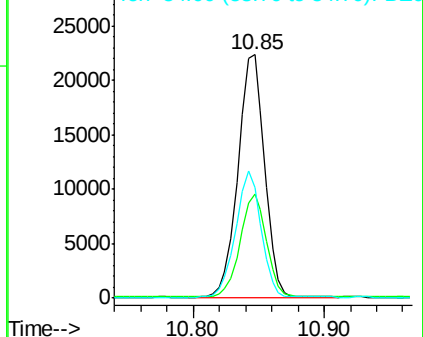

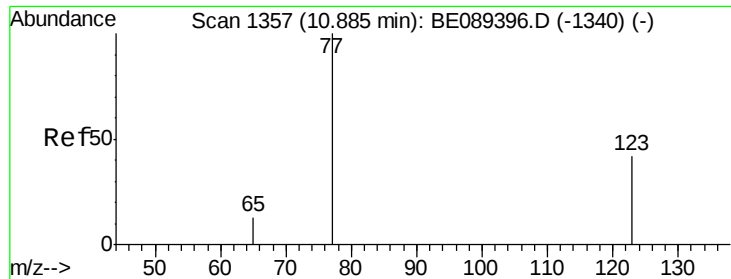

#9

Nitrobenzene

Concen: 0.95 ng

RT: 10.89 min Scan# 1358

Delta R.T. 0.00 min

Lab File: BE089407.D

Acq: 29 Jan 2015 3:02

Instrument :

BNA_E

ClientSampleId :

SSTDCCC001


Tgt Ion: 77 Resp: 35361

Ion Ratio Lower Upper

77 100

123 44.5 34.7 52.1




65 13.3 10.6 15.8

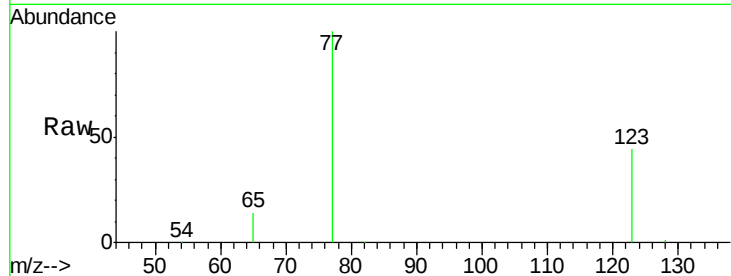

Abundance Ion 77.00 (76.70 to 77.70): BE0

Ion 123.00 (122.70 to 123.70): BE0

Ion 65.00 (64.70 to 65.70): BE0

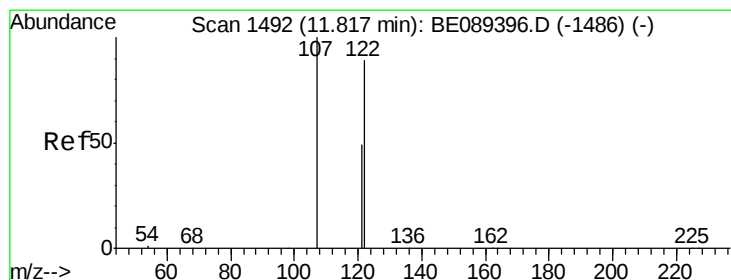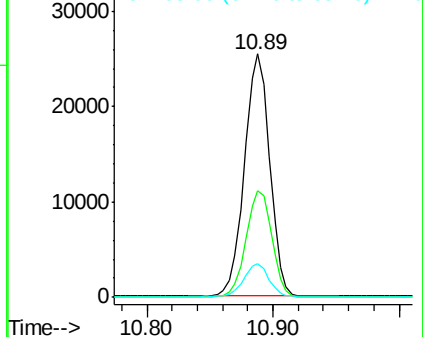

#10

2,4-Dimethylphenol

Concen: 0.98 ng

RT: 11.82 min Scan# 1492

Delta R.T. 0.00 min

Lab File: BE089407.D

Acq: 29 Jan 2015 3:02


Tgt Ion: 122 Resp: 27856

Ion Ratio Lower Upper

122 100

107 123.9 89.4 134.2



121 57.6 43.6 65.4




Abundance Ion 122.00 (121.70 to 122.70): E

Ion 107.00 (106.70 to 107.70): E

Ion 121.00 (120.70 to 121.70): E

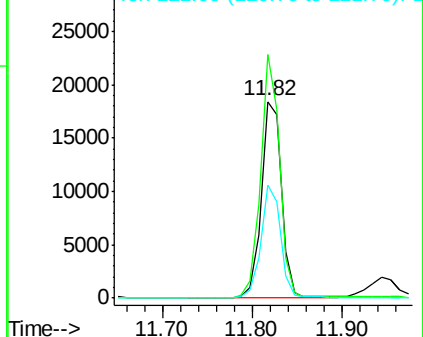


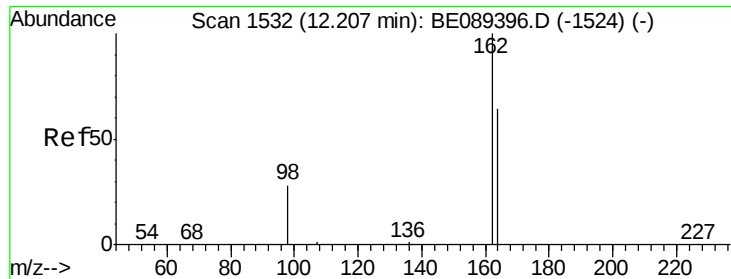




#11
 2,4-Dichlorophenol
 Concen: 0.97 ng
 RT: 12.21 min Scan# 1532
 Delta R.T. 0.00 min
 Lab File: BE089407.D
 Acq: 29 Jan 2015 3:02

Instrument :
 BNA_E
 ClientSampleId :
 SSTDCCC001

Tgt Ion:162 Resp: 21203
 Ion Ratio Lower Upper
 162 100
 164 62.2 44.6 84.6
 98 38.9 8.7 48.7

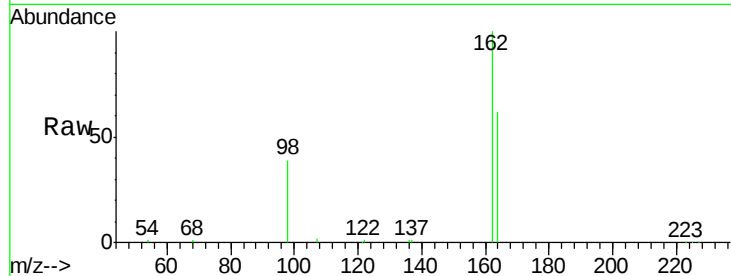


Abundance Ion 162.00 (161.70 to 162.70): E
 Ion 164.00 (163.70 to 164.70): E
 Ion 98.00 (97.70 to 98.70): BE0


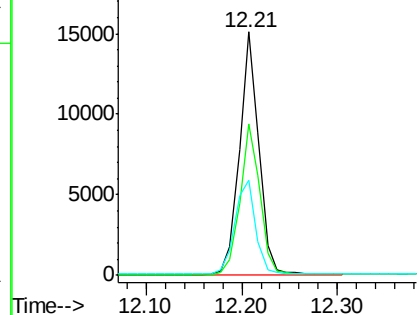



#12
 Hexachlorobutadiene
 Concen: 0.91 ng
 RT: 12.89 min Scan# 1602
 Delta R.T. 0.00 min
 Lab File: BE089407.D
 Acq: 29 Jan 2015 3:02

Tgt Ion:225 Resp: 14188
 Ion Ratio Lower Upper
 225 100
 223 62.5 50.2 75.4
 227 63.9 50.5 75.7



Abundance Ion 225.00 (224.70 to 225.70): E
 Ion 223.00 (222.70 to 223.70): E
 Ion 227.00 (226.70 to 227.70): E

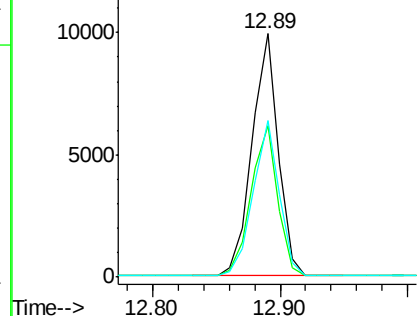



#13

Acenaphthene-d10

Concen: 5.00 ng

RT: 12.21 min Scan# 1532

Delta R.T. 0.00 min

Lab File: BE089407.D

Acq: 29 Jan 2015 3:02

Instrument :

BNA_E

ClientSampleId :

SSTDCCC001


Tgt Ion:164 Resp: 13436

Ion Ratio Lower Upper

164 100

162 160.8 123.9 185.9




160 0.0 0.0 0.0

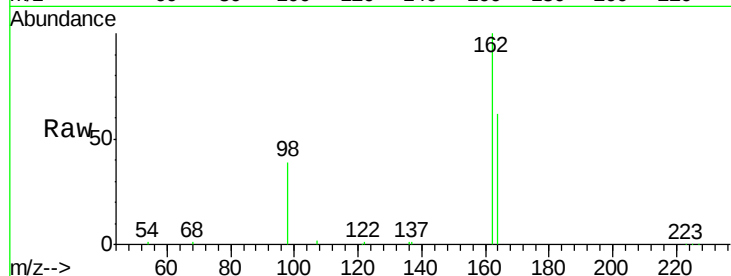

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

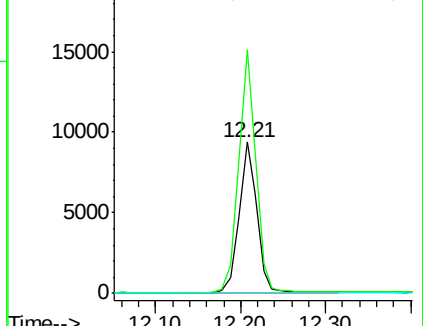

#14

2,4,6-Tribromophenol

Concen: 0.37 ng

RT: 18.58 min Scan# 3035

Delta R.T. 0.00 min

Lab File: BE089407.D

Acq: 29 Jan 2015 3:02


Tgt Ion:330 Resp: 4222

Ion Ratio Lower Upper

330 100

332 96.4 77.5 116.3



141 39.7 32.4 48.6




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E




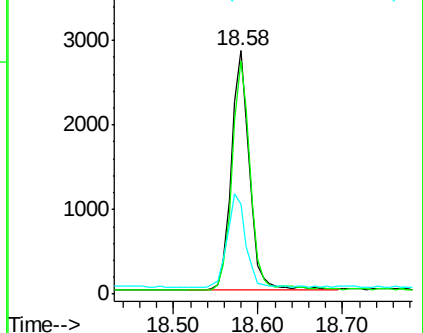


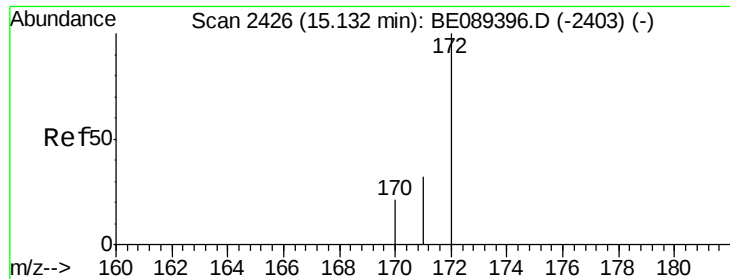

#15
2-Fluorobiphenyl
Concen: 0.37 ng
RT: 15.13 min Scan# 2425
Delta R.T. -0.00 min
Lab File: BE089407.D
Acq: 29 Jan 2015 3:02




Instrument :
BNA_E
ClientSampleId :
SSTDCCC001


Tgt Ion:172 Resp: 52862
Ion Ratio Lower Upper
172 100
171 32.9 25.6 38.4
170 22.0 17.0 25.4

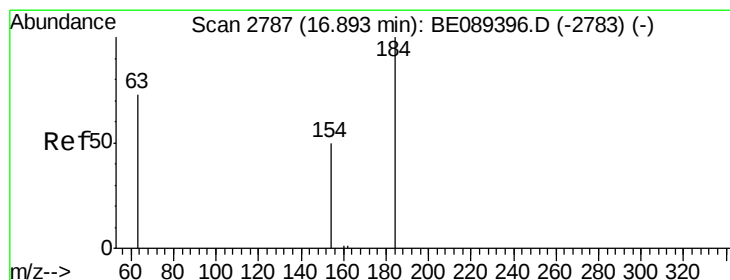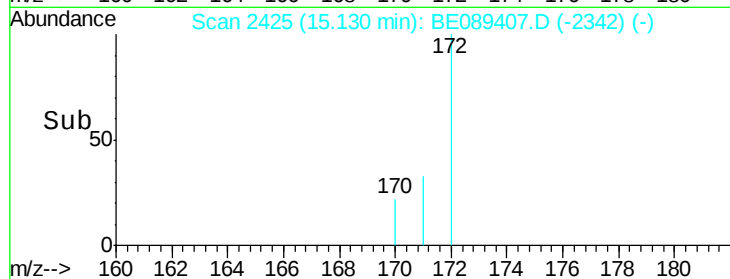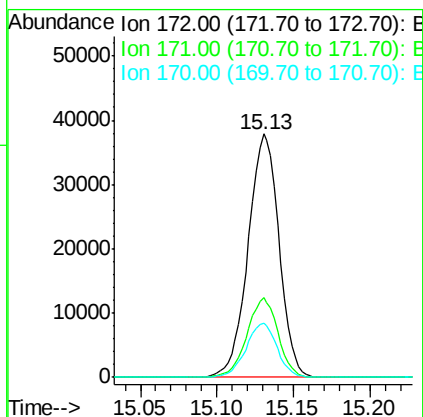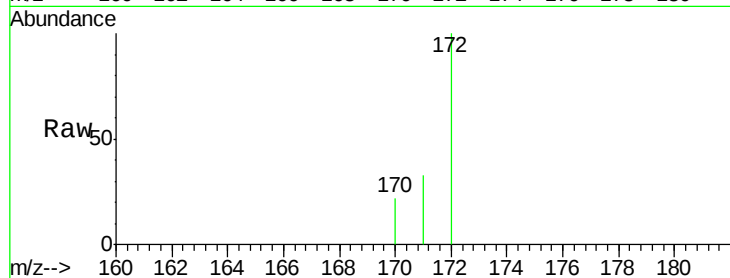

#16
2,4-Dinitrophenol
Concen: 0.96 ng
RT: 16.90 min Scan# 2788
Delta R.T. 0.01 min
Lab File: BE089407.D
Acq: 29 Jan 2015 3:02

Tgt Ion:184 Resp: 674
Ion Ratio Lower Upper
184 100
63 70.4 66.9 100.3
154 51.9 45.1 67.7

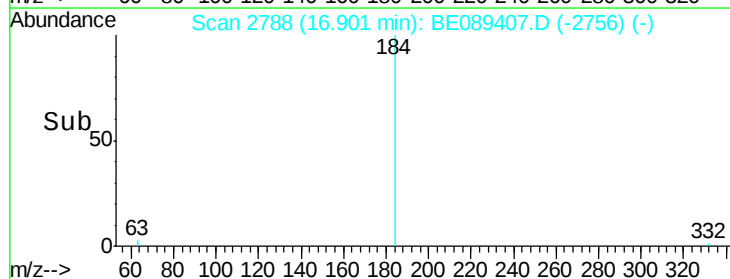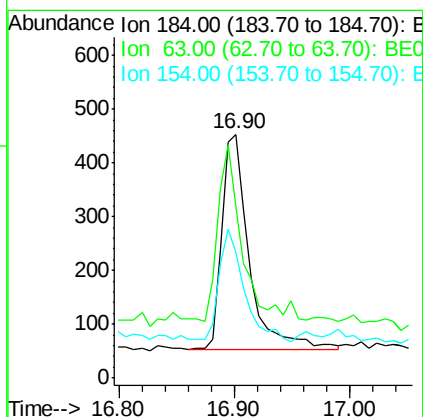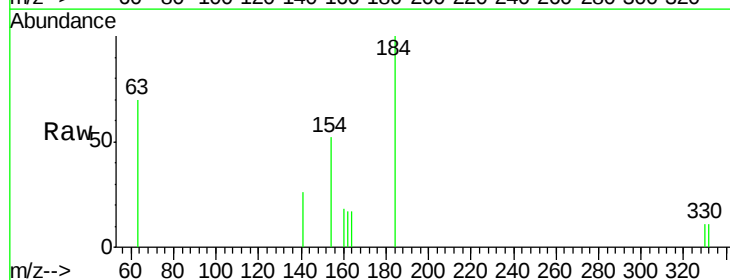


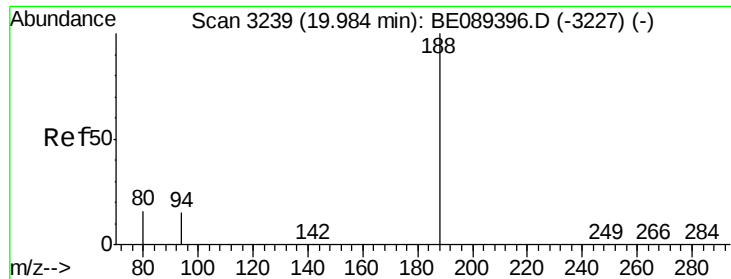




#17
Phenanthrene-d10
Concen: 5.00 ng
RT: 19.99 min Scan# 3240
Delta R.T. 0.01 min
Lab File: BE089407.D
Acq: 29 Jan 2015 3:02

Instrument :
BNA_E
ClientSampleId :
SSTDCCC001

Tgt Ion:188 Resp: 371458
Ion Ratio Lower Upper
188 100
94 12.9 12.0 18.0
80 12.9 13.2 19.8#




Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BE0
Ion 80.00 (79.70 to 80.70): BE0

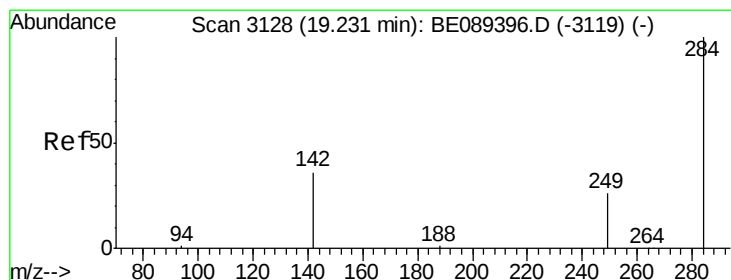
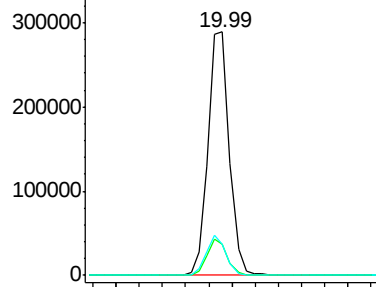



#18
Hexachlorobenzene
Concen: 0.92 ng
RT: 19.23 min Scan# 3128
Delta R.T. 0.00 min
Lab File: BE089407.D
Acq: 29 Jan 2015 3:02

Tgt Ion:284 Resp: 15782
Ion Ratio Lower Upper
284 100
142 36.9 30.7 46.1
249 29.2 23.4 35.2



Abundance Ion 284.00 (283.70 to 284.70): E
Ion 142.00 (141.70 to 142.70): E
Ion 249.00 (248.70 to 249.70): E

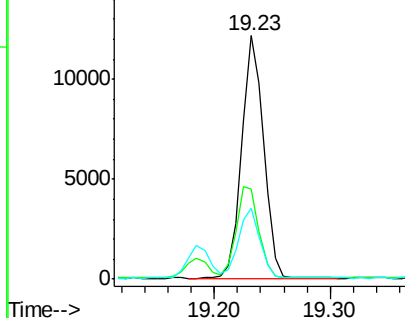


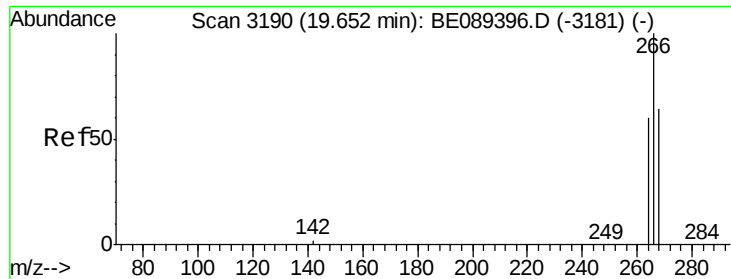




#19
 Pentachlorophenol
 Concen: 0.78 ng
 RT: 19.65 min Scan# 3190
 Delta R.T. 0.00 min
 Lab File: BE089407.D
 Acq: 29 Jan 2015 3:02

Instrument :
 BNA_E
 ClientSampleId :
 SSTDCCC001

Tgt Ion: 266 Resp: 2588
 Ion Ratio Lower Upper
 266 100
 268 60.8 52.5 78.7
 264 60.4 48.8 73.2

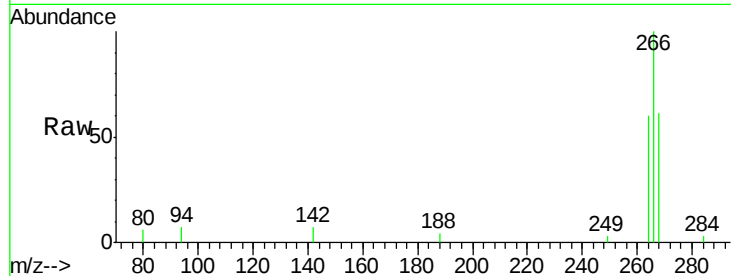


Abundance Ion 265.70 (265.40 to 266.40): E
 Ion 268.00 (267.70 to 268.70): E
 Ion 264.00 (263.70 to 264.70): E


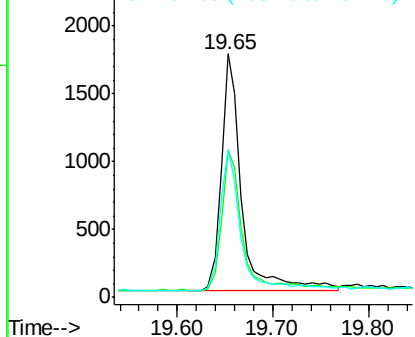



#20
 Chrysene-d12
 Concen: 5.00 ng
 RT: 23.84 min Scan# 3873
 Delta R.T. -0.00 min
 Lab File: BE089407.D
 Acq: 29 Jan 2015 3:02

Tgt Ion: 240 Resp: 476823
 Ion Ratio Lower Upper
 240 100
 120 8.8 7.1 10.7
 236 24.7 19.5 29.3



Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

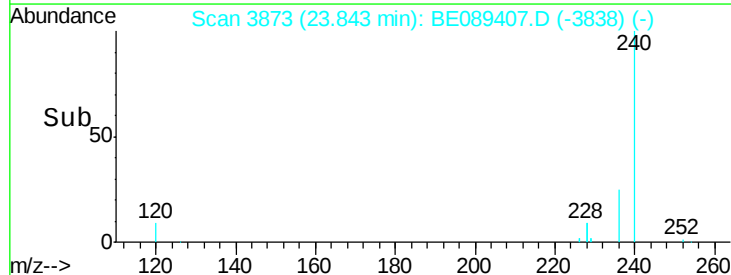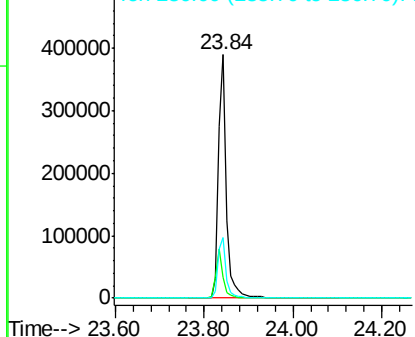

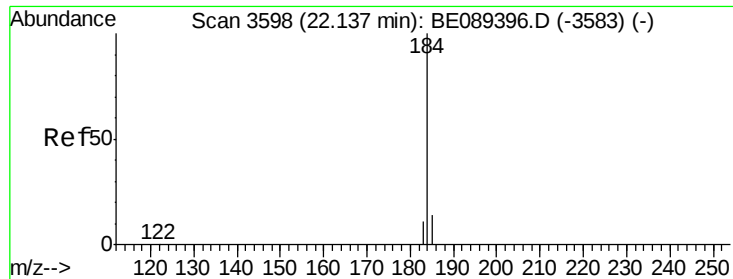

#21

Benzidine

Concen: 0.80 ng

RT: 22.14 min Scan# 3599

Delta R.T. 0.00 min

Lab File: BE089407.D

Acq: 29 Jan 2015 3:02

Instrument :

BNA_E

ClientSampleId :

SSTDCCC001





Tgt Ion:184 Resp: 45101

Ion Ratio Lower Upper

184 100

185 14.8 11.4 17.0

183 10.6 8.7 13.1

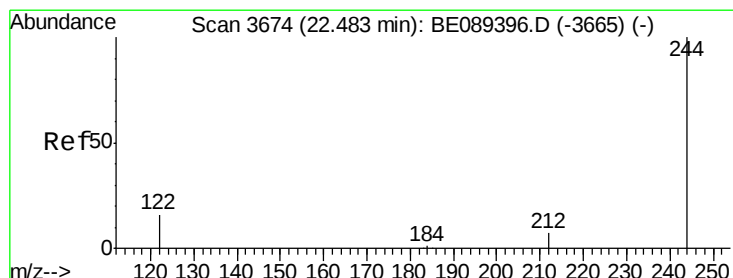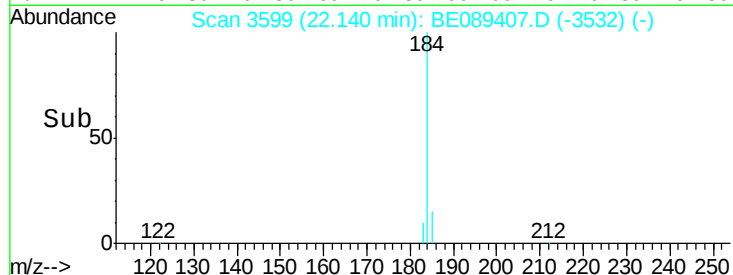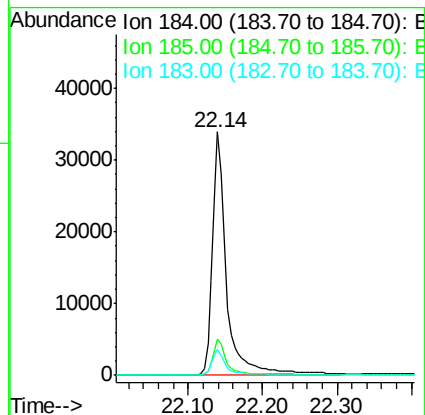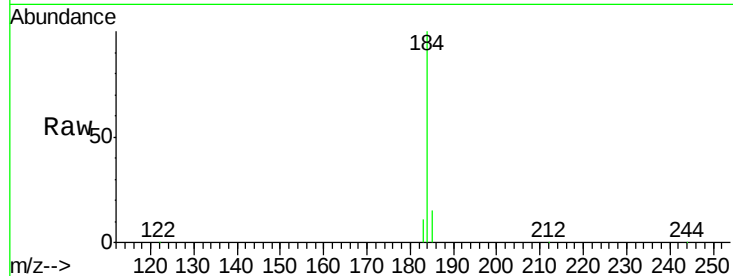

#22

Terphenyl-d14

Concen: 1.05 ng

RT: 22.48 min Scan# 3674

Delta R.T. -0.00 min

Lab File: BE089407.D

Acq: 29 Jan 2015 3:02




Tgt Ion:244 Resp: 55510


Ion Ratio Lower Upper

244 100

212 7.1 5.9 8.9

122 16.4 12.8 19.2

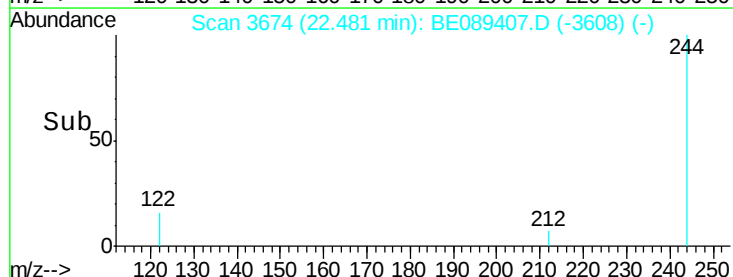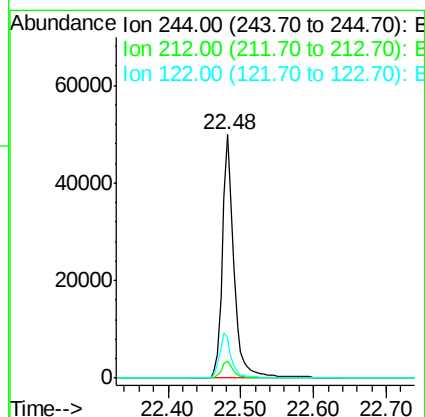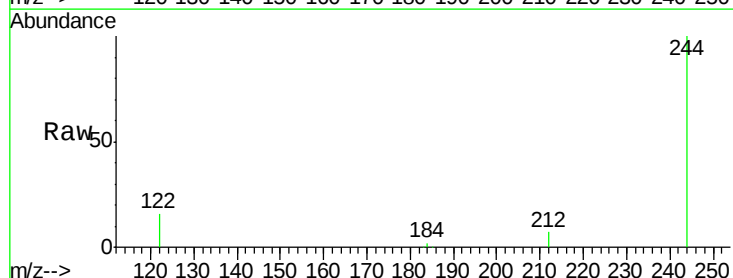

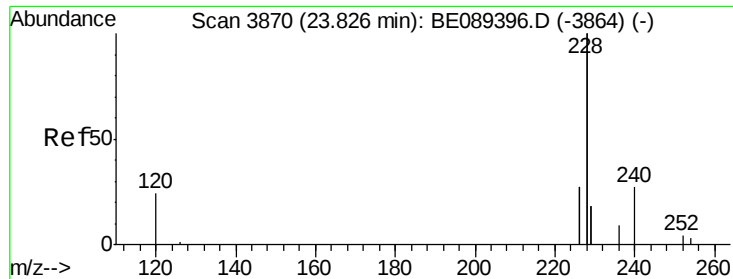

#23

Benzo(a)anthracene

Concen: 1.04 ng

RT: 23.83 min Scan# 3871

Delta R.T. -0.00 min

Lab File: BE089407.D

Acq: 29 Jan 2015 3:02

Instrument :

BNA_E

ClientSampleId :

SSTDCCC001


Tgt Ion:228 Resp: 461240

Ion Ratio Lower Upper

228 100

226 26.9 21.8 32.6




229 18.2 14.5 21.7

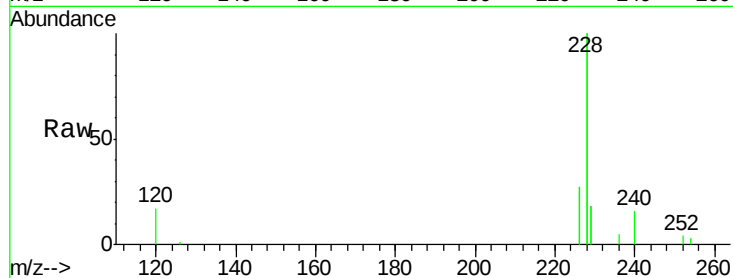

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

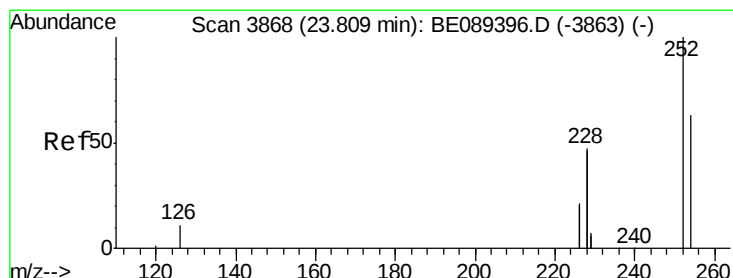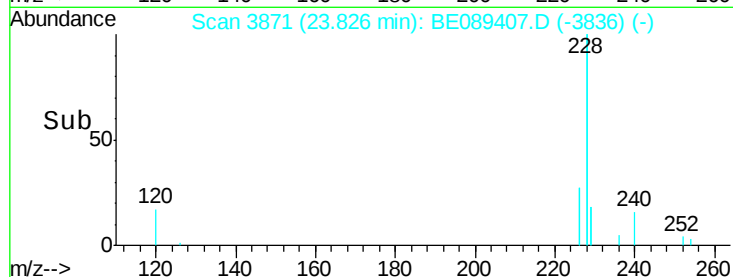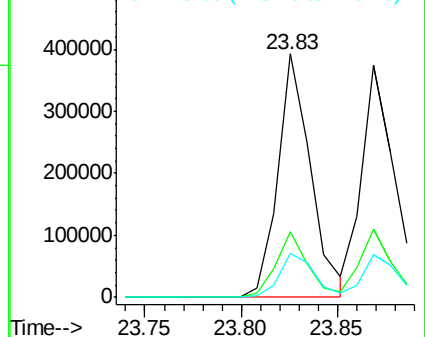

#24

3,3'-Dichlorobenzidine

Concen: 1.22 ng

RT: 23.81 min Scan# 3869

Delta R.T. -0.00 min

Lab File: BE089407.D

Acq: 29 Jan 2015 3:02


Tgt Ion:252 Resp: 42751

Ion Ratio Lower Upper

252 100

254 60.6 50.2 75.4



126 14.1 9.8 14.6

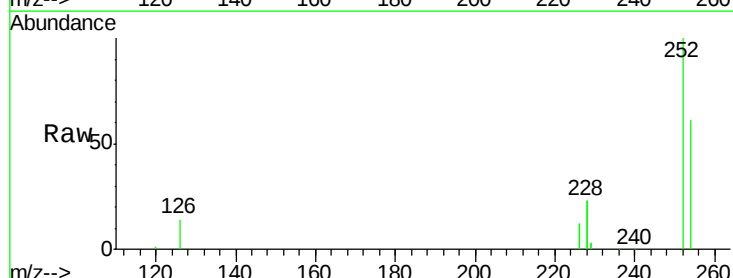


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 254.00 (253.70 to 254.70): E

Ion 126.00 (125.70 to 126.70): E

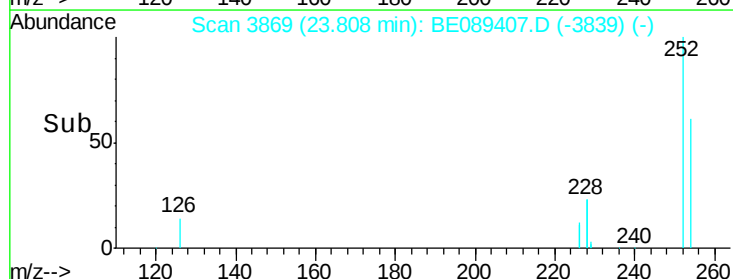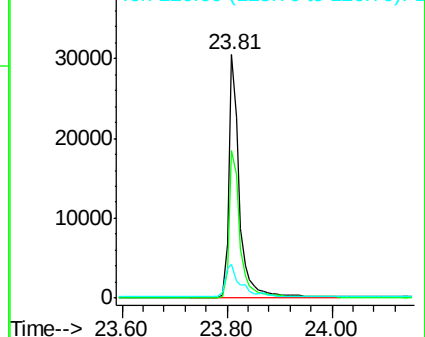

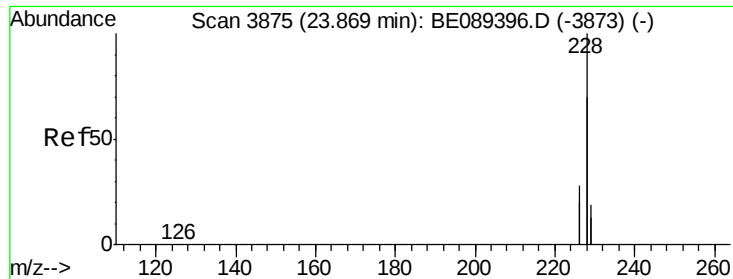

#25

Chrysene

Concen: 0.93 ng

RT: 23.87 min Scan# 3876

Delta R.T. -0.00 min

Lab File: BE089407.D

Acq: 29 Jan 2015 3:02

Instrument :

BNA_E

ClientSampleId :

SSTDCCC001


Tgt Ion:228 Resp: 504799

Ion Ratio Lower Upper

228 100

226 29.3 22.7 34.1




229 18.6 15.2 22.8

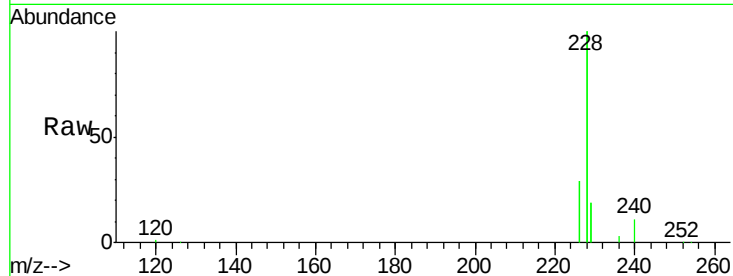

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

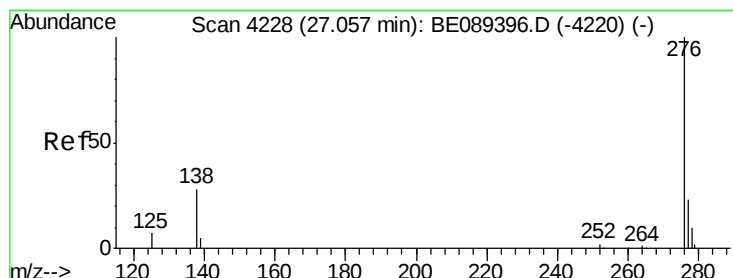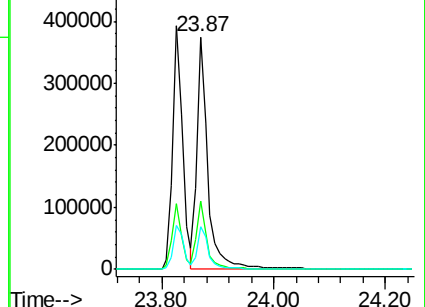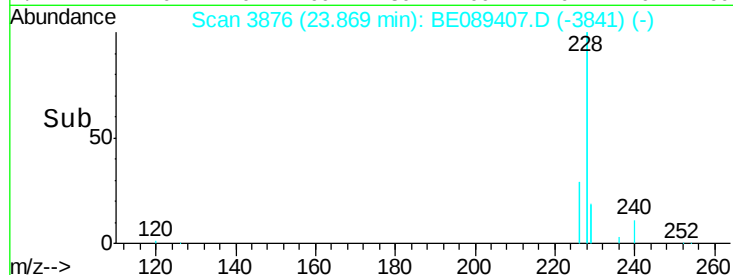

#26

Indeno(1,2,3-cd)pyrene

Concen: 1.16 ng

RT: 27.06 min Scan# 4229

Delta R.T. -0.00 min

Lab File: BE089407.D

Acq: 29 Jan 2015 3:02


Tgt Ion:276 Resp: 145951

Ion Ratio Lower Upper

276 100

138 33.4 0.0 0.0#



277 24.3 0.0 0.0#

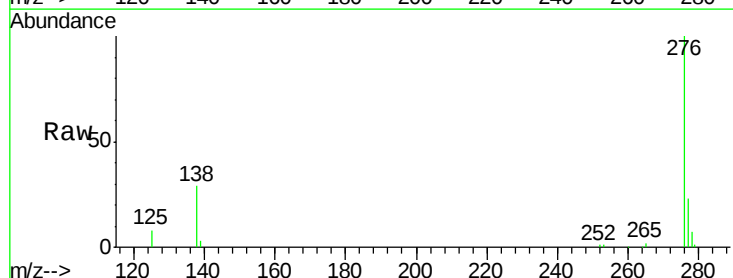


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

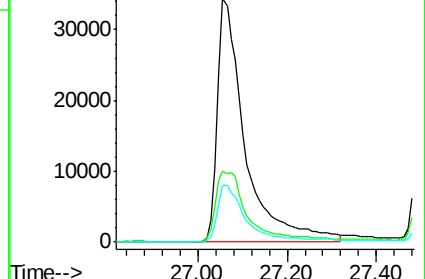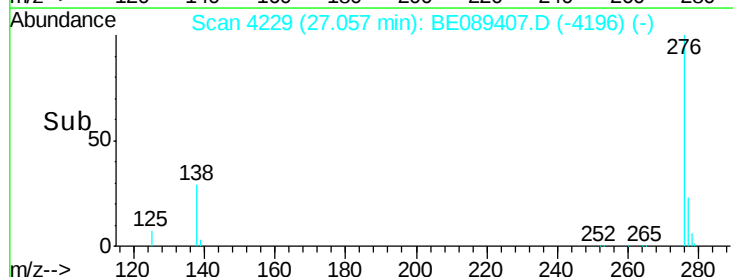




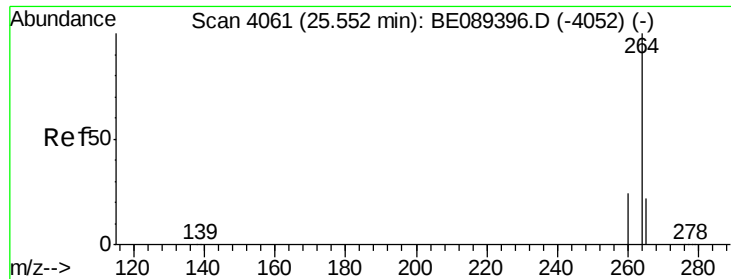


#27
Perylene-d12
Concen: 5.00 ng
RT: 25.55 min Scan# 4062
Delta R.T. -0.00 min
Lab File: BE089407.D
Acq: 29 Jan 2015 3:02

Instrument :
BNA_E
ClientSampleId :
SSTDCCC001

Tgt Ion: 264 Resp: 550235




Ion	Ratio	Lower	Upper
264	100		
260	23.9	18.9	28.3
265	21.7	17.5	26.3

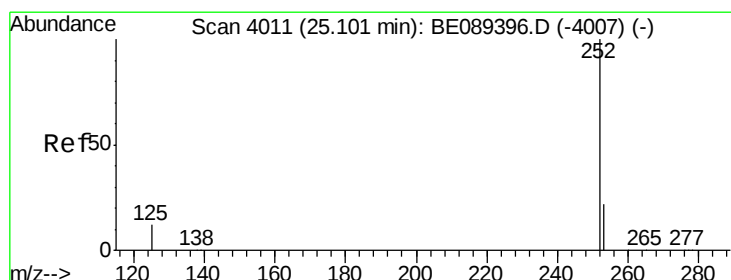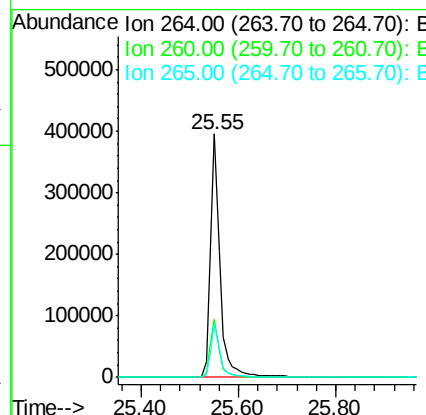


#28
Benzo(b)fluoranthene
Concen: 1.30 ng
RT: 25.10 min Scan# 4012
Delta R.T. -0.00 min
Lab File: BE089407.D
Acq: 29 Jan 2015 3:02

Tgt Ion: 252 Resp: 93925

Ion	Ratio	Lower	Upper
252	100		
253	22.7	17.6	26.4
125	11.5	9.8	14.6

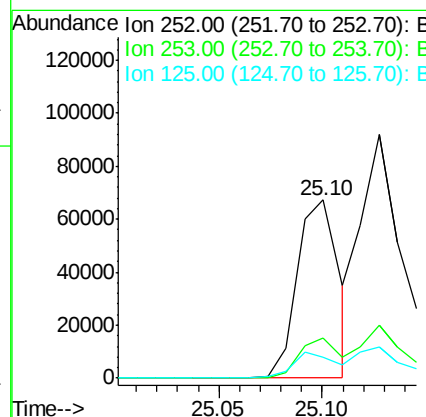

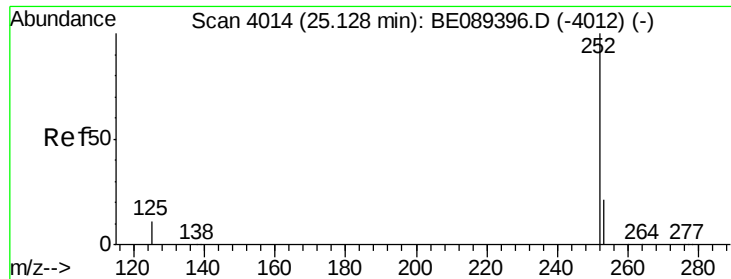

#29

Benzo(k)fluoranthene

Concen: 0.93 ng

RT: 25.13 min Scan# 4015

Delta R.T. -0.00 min

Lab File: BE089407.D

Acq: 29 Jan 2015 3:02

Instrument :

BNA_E

ClientSampleId :

SSTDCCC001


Tgt Ion:252 Resp: 162986

Ion Ratio Lower Upper

252 100

253 21.9 17.3 25.9




125 12.6 10.2 15.4

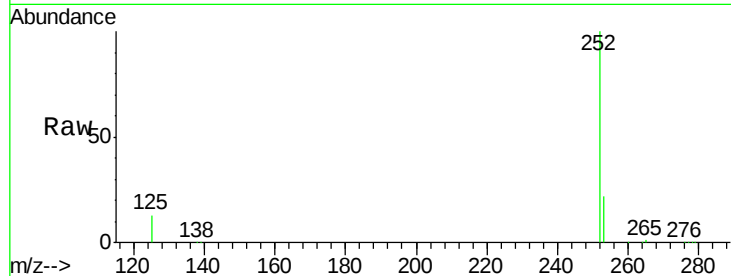

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

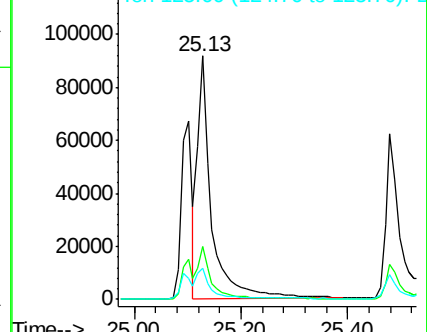

#30

Benzo(a)pyrene

Concen: 1.22 ng

RT: 25.48 min Scan# 4054

Delta R.T. -0.00 min

Lab File: BE089407.D

Acq: 29 Jan 2015 3:02


Tgt Ion:252 Resp: 103428

Ion Ratio Lower Upper

252 100

253 21.4 17.5 26.3



125 15.2 12.2 18.4




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

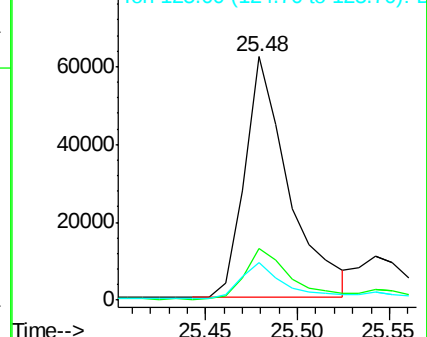

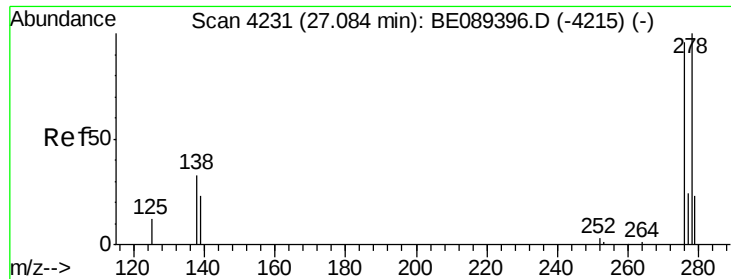

#31

Dibenzo(a,h)anthracene

Concen: 1.25 ng

RT: 27.09 min Scan# 4233

Delta R.T. 0.01 min

Lab File: BE089407.D


Acq: 29 Jan 2015 3:02

Instrument :

BNA_E

ClientSampleId :

SSTDCCC001




Tgt Ion: 278 Resp: 112829

Ion Ratio Lower Upper

278 100

139 18.6 18.5 27.7

279 23.9 18.6 28.0

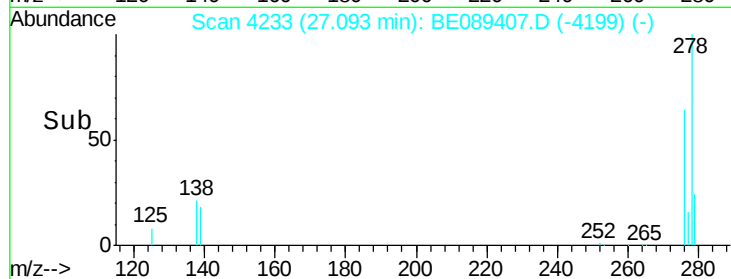

Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

