


Data Path : Z:\HPCHEM1\BNA\_E\Data\BE012815\  
 Data File : BE089391.D  
 Acq On : 28 Jan 2015 16:38  
 Operator : TP/IZ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG012815.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Jan 29 04:12:23 2015

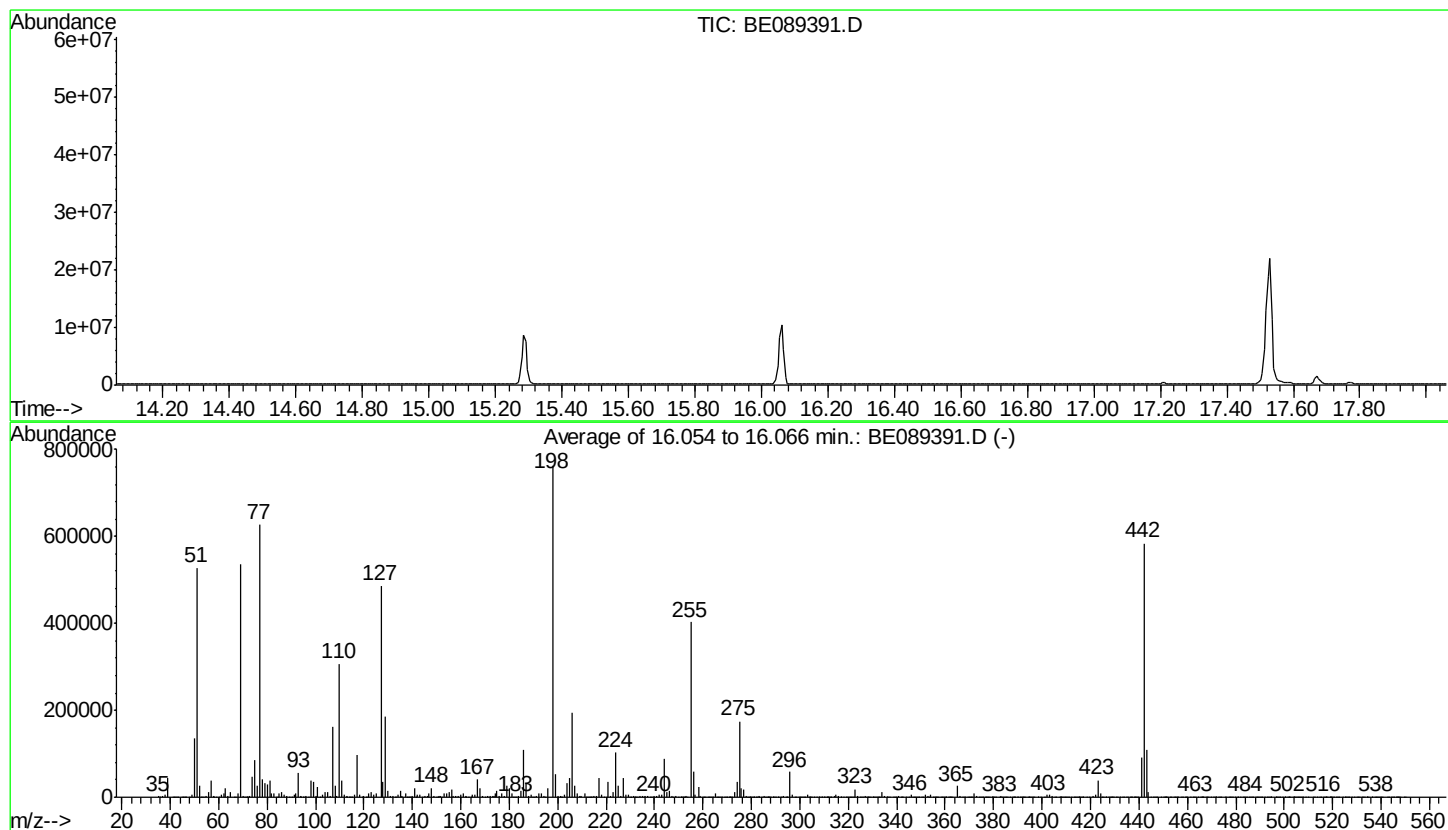

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2490

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 69.1      | 527623  | PASS             |
| 68          | 69           | 0.00         | 2            | 1.7       | 9078    | PASS             |
| 69          | 198          | 0.00         | 100          | 70.3      | 536585  | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 3046    | PASS             |
| 127         | 198          | 10           | 80           | 63.7      | 486083  | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 763029  | PASS             |
| 199         | 198          | 5            | 9            | 7.1       | 54511   | PASS             |
| 275         | 198          | 10           | 60           | 22.8      | 173794  | PASS             |
| 365         | 198          | 1            | 100          | 3.4       | 25736   | PASS             |
| 441         | 442          | 0.01         | 24           | 15.7      | 91890   | PASS             |
| 442         | 198          | 50           | 100          | 76.5      | 583893  | PASS             |
| 443         | 442          | 15           | 24           | 18.8      | 109981  | PASS             |