


Data Path : Z:\HPCHEM1\BNA\_E\Data\BE012815\  
Data File : BE089408.D  
Acq On : 29 Jan 2015 3:40  
Operator : TP/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_E\METHODS\SIM-BE012815.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Thu Jan 29 04:21:19 2015

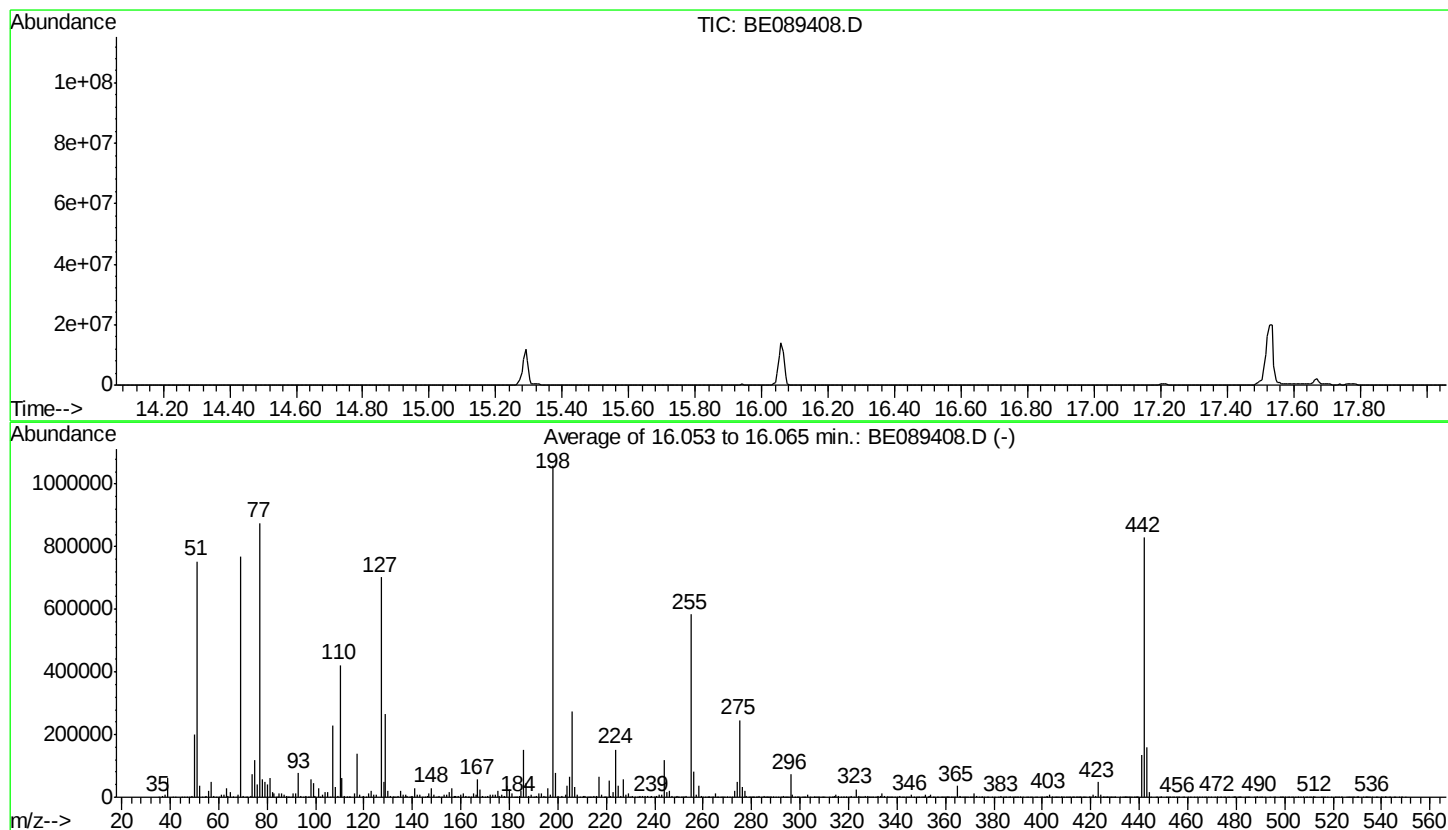

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2488

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 71.2         | 753767     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.3          | 9877       | PASS                |
| 69             | 198             | 0.00            | 100             | 72.4         | 767098     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.4          | 3085       | PASS                |
| 127            | 198             | 10              | 80              | 66.3         | 702281     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.7          | 7407       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 1059131    | PASS                |
| 199            | 198             | 5               | 9               | 7.2          | 75789      | PASS                |
| 275            | 198             | 10              | 60              | 23.3         | 247207     | PASS                |
| 365            | 198             | 1               | 100             | 3.5          | 36635      | PASS                |
| 441            | 442             | 0.01            | 24              | 16.2         | 134096     | PASS                |
| 442            | 198             | 50              | 100             | 78.2         | 828490     | PASS                |
| 443            | 442             | 15              | 24              | 19.1         | 158271     | PASS                |