

Data Path : Z:\HPCHEM1\BNA E\DATA\BE012818\
 Data File : BE095212.D
 Acq On : 28 Jan 2018 18:21
 Operator : SJ/JU
 Sample : J1221-13
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Jan 29 06:59:42 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 29 06:58:46 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2390	0.40	ng/ul	0.00
2) Naphthalene-d8	11.27	136	7488	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	4779	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.71
16) Chrysene-d12	21.80	240	10704	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	502317	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3411	0.28	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	10399	0.00	ng/ul	0.00
Target Compounds						
					Ovalue	
17) Pyrene	20.08	202	3735	0.104	ng/ul	95
18) Benzo(a)anthracene	21.79	228	758	0.023	ng/ul#	32
19) Chrysene	21.84	228	950	0.027	ng/ul#	49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE012818\
Data File : BE095212.D
Acq On : 28 Jan 2018 18:21
Operator : SJ/JU
Sample : J1221-13
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Jan 29 06:59:42 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 29 06:58:46 2018
Response via : Initial Calibration




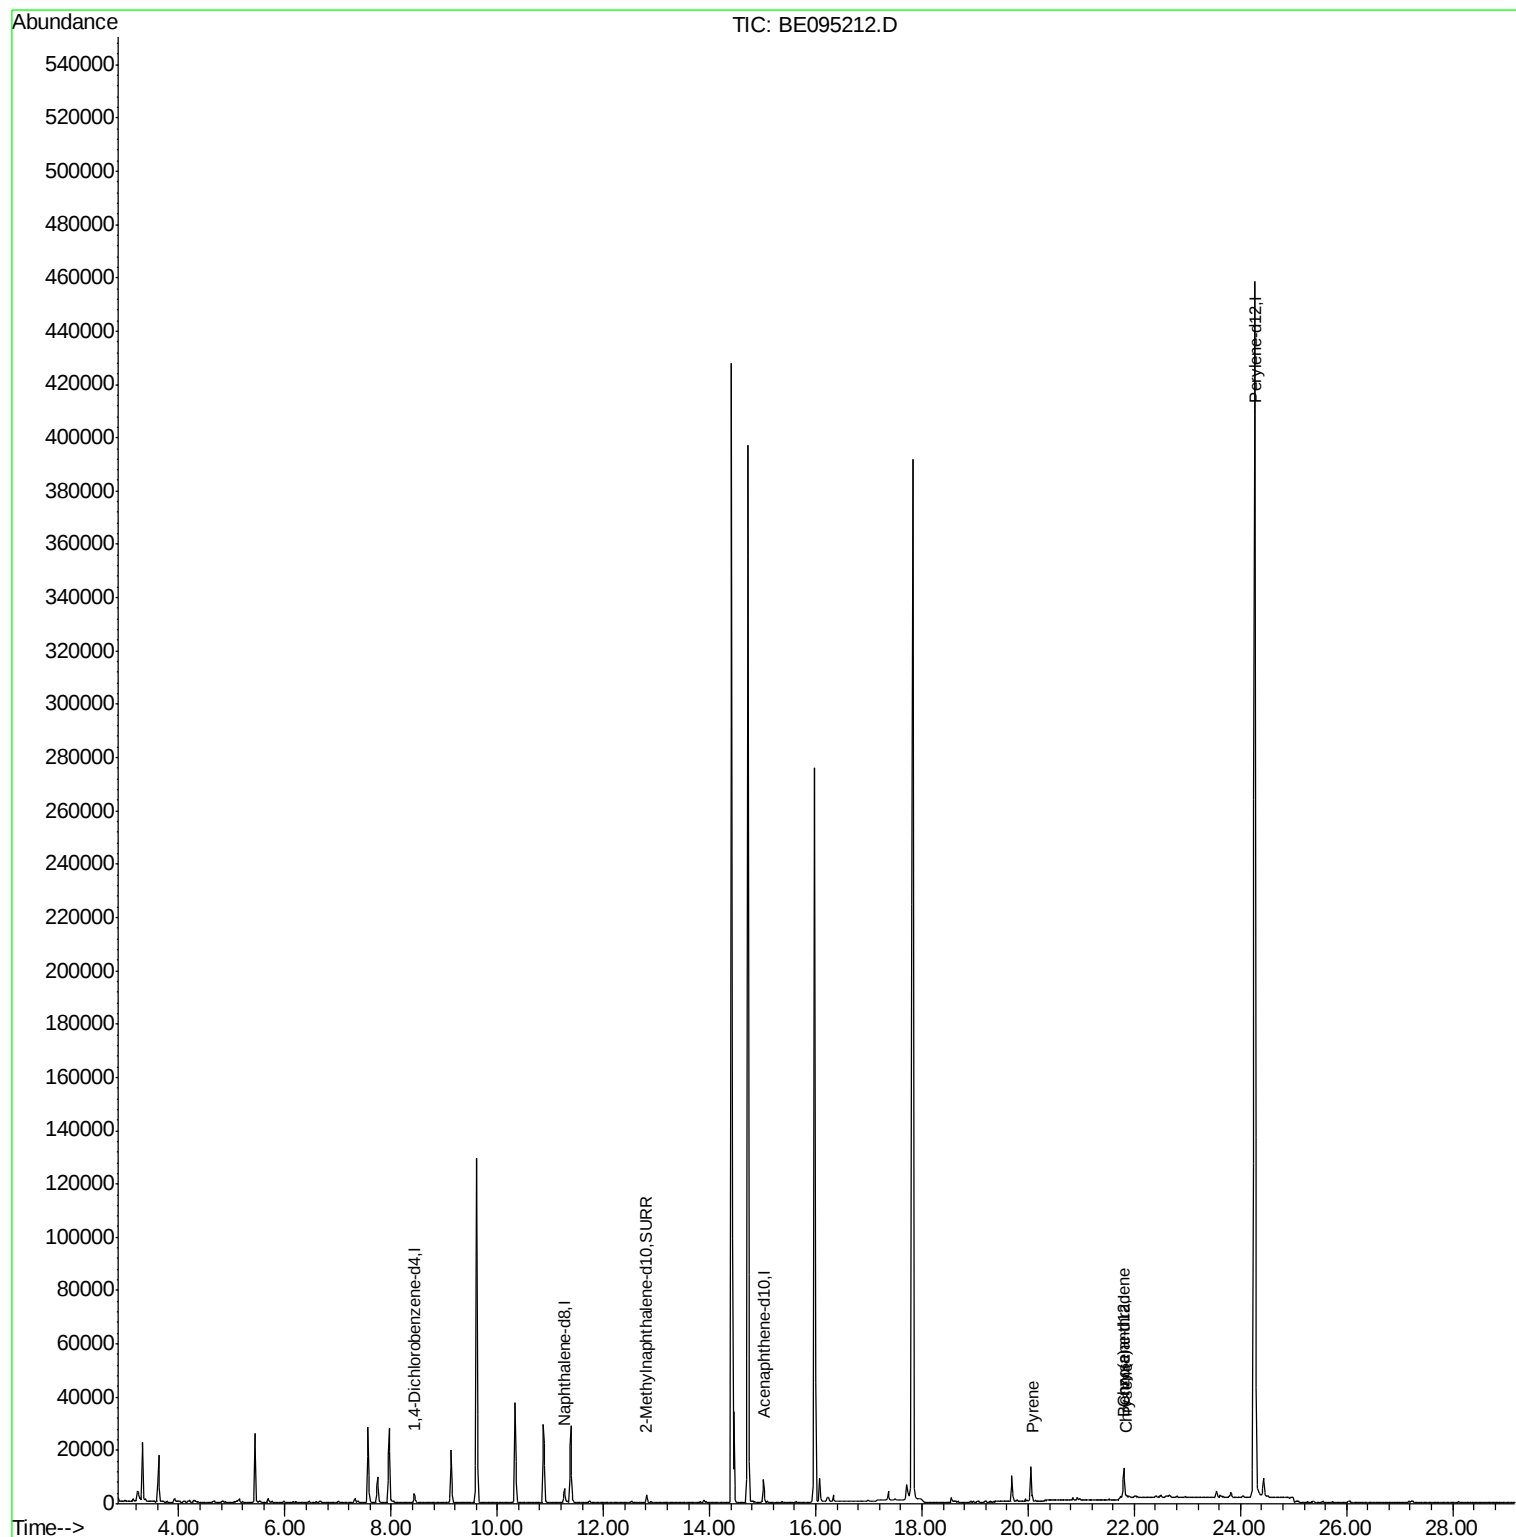


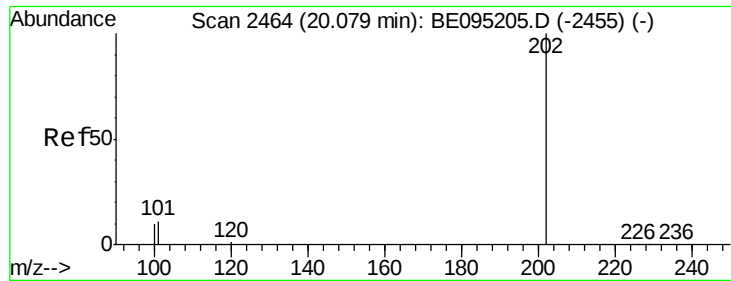

#17
 Pvrene
 Concen: 0.104 ng/ul
 RT: 20.08 min Scan# 2464
 Delta R.T. -0.00 min
 Lab File: BE095212.D
 Acq: 28 Jan 2018 18:21




Instrument :
 BNA_E
 ClientSampleId :




Tot Ion:202 Resp: 3735
 Ion Ratio Lower Upper
 202 100
 101 18.7 18.2 27.4
 100 18.7 15.6 23.4

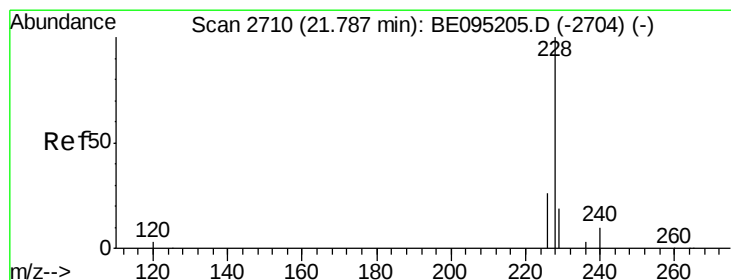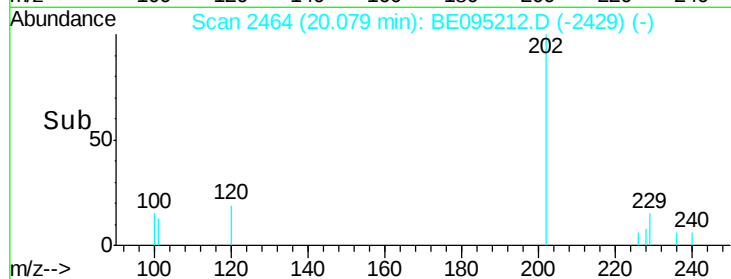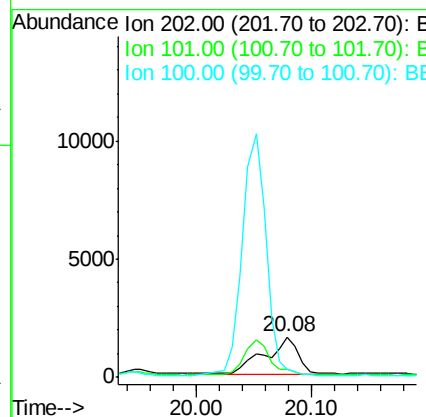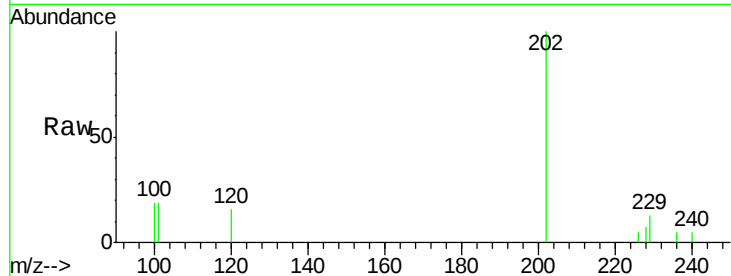

#18
 Benzo(a)anthracene
 Concen: 0.023 ng/ul
 RT: 21.79 min Scan# 2710
 Delta R.T. -0.00 min
 Lab File: BE095212.D
 Acq: 28 Jan 2018 18:21

Tgt Ion:228 Resp: 758
 Ion Ratio Lower Upper
 228 100
 229 69.2 22.8 34.2#
 226 47.2 17.0 25.6#

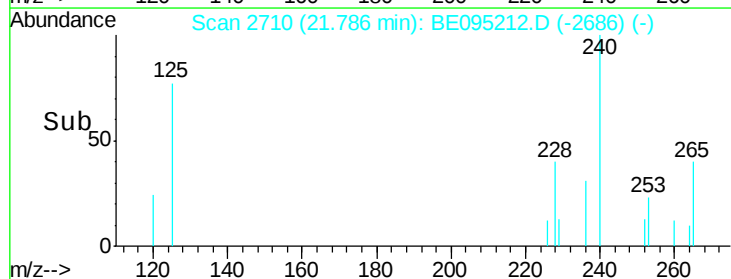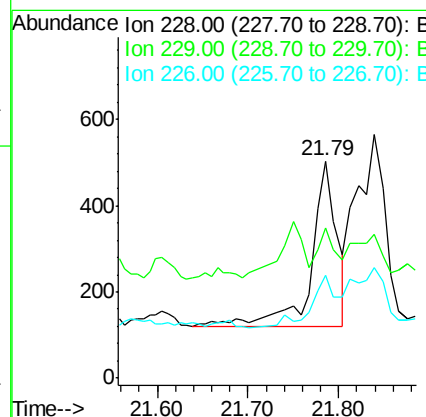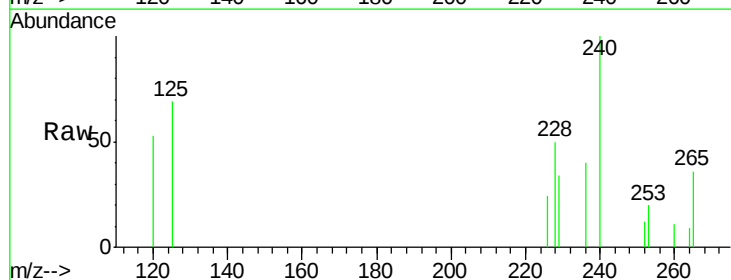

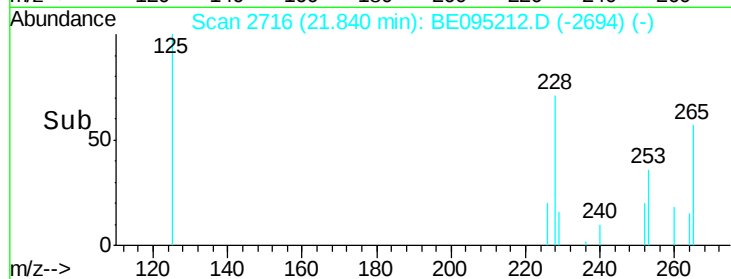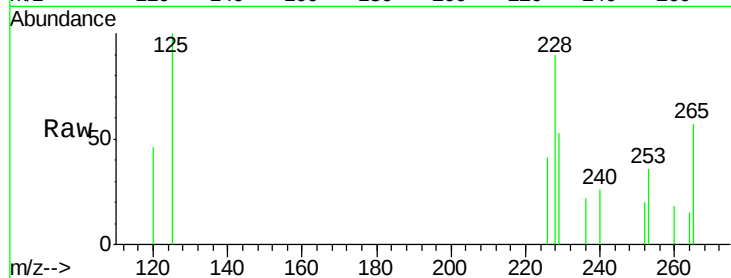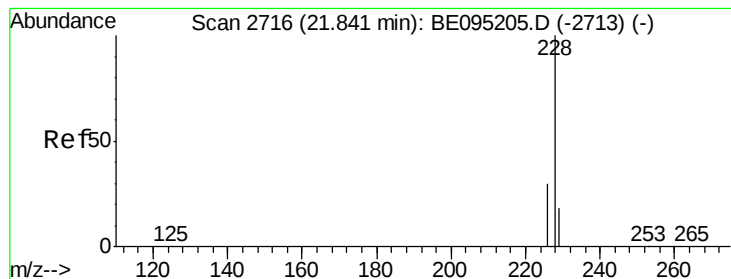

#19

Chrysene

Concen: 0.027 ng/ul

RT: 21.84 min Scan# 2716

Delta R.T. -0.00 min

Lab File: BE095212.D

Acq: 28 Jan 2018 18:21

Instrument :

BNA_E

ClientSampleId :

Tot Ion: 228 Resp: 950

Ion Ratio Lower Upper

228 100

226 45.5 23.4 35.0#

229 59.1 17.7 26.5#

