

Data Path : Z:\HPCHEM1\BNA E\DATA\BE012818\
 Data File : BE095214.D
 Acq On : 28 Jan 2018 19:33
 Operator : SJ/JU
 Sample : J1222-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Jan 29 06:59:56 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 29 06:58:46 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2726	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	8662	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	5558	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.71
16) Chrysene-d12	21.80	240	11307	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	633404	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	4734	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	12795	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	20.05	202	2091	0.055	ng/ul#	1
18) Benzo(a)anthracene	21.81	228	788	0.022	ng/ul#	27
19) Chrysene	21.81	228	785	0.021	ng/ul#	33


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE012818\
Data File : BE095214.D
Acq On : 28 Jan 2018 19:33
Operator : SJ/JU
Sample : J1222-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Jan 29 06:59:56 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 29 06:58:46 2018
Response via : Initial Calibration




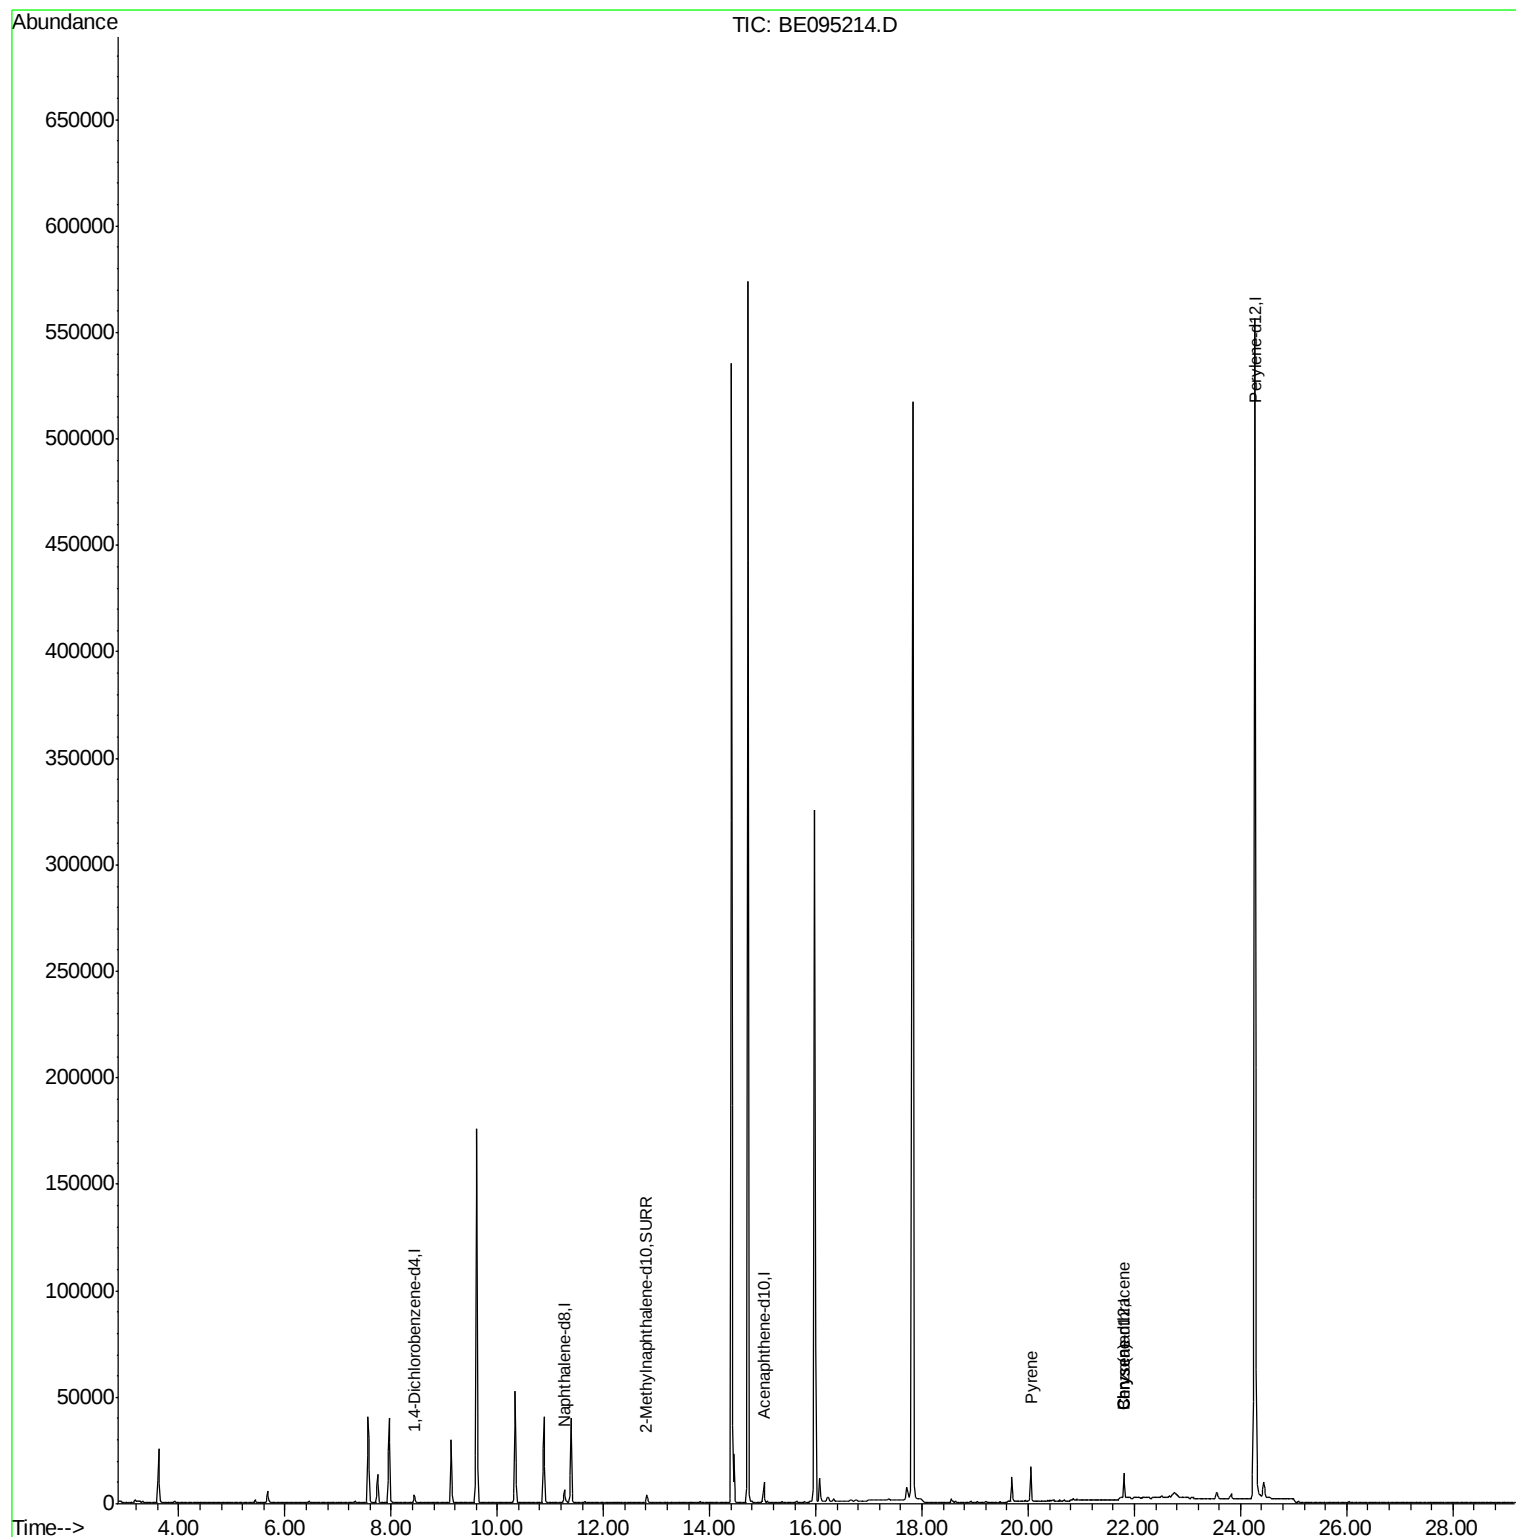


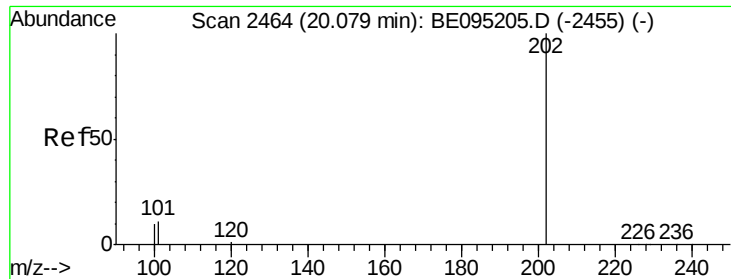

#17
Pvrene
Concen: 0.055 ng/ul
RT: 20.05 min Scan# 2460
Delta R.T. -0.03 min
Lab File: BE095214.D
Acq: 28 Jan 2018 19:33




Instrument :
BNA_E
ClientSampleId :




Tot Ion:202 Resp: 2091
Ion Ratio Lower Upper
202 100
101 153.5 18.2 27.4#
100 1019.3 15.6 23.4#

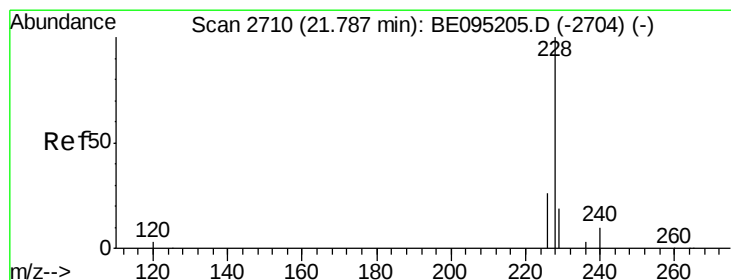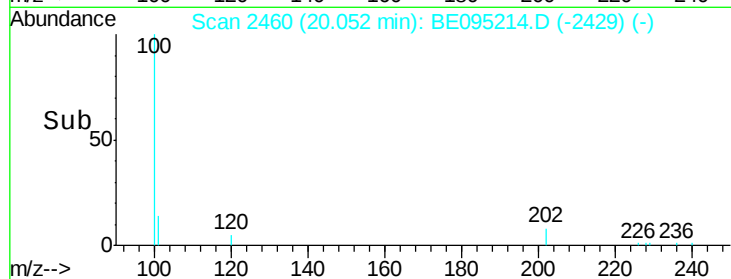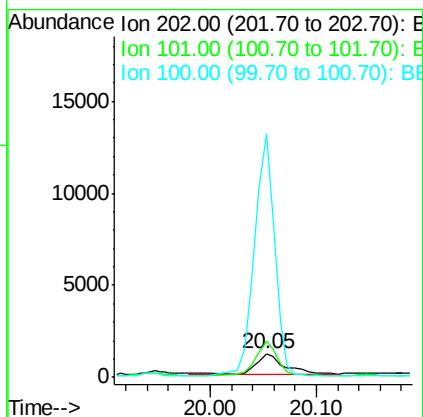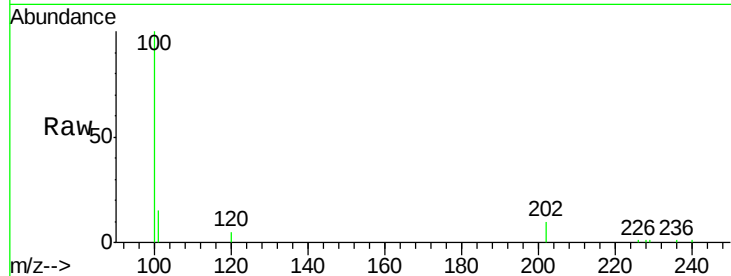

#18
Benzo(a)anthracene
Concen: 0.022 ng/ul
RT: 21.81 min Scan# 2713
Delta R.T. 0.03 min
Lab File: BE095214.D
Acq: 28 Jan 2018 19:33

Tgt Ion:228 Resp: 788
Ion Ratio Lower Upper
228 100
229 70.9 22.8 34.2#
226 50.9 17.0 25.6#

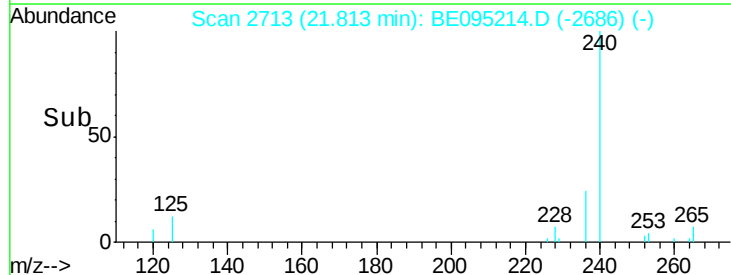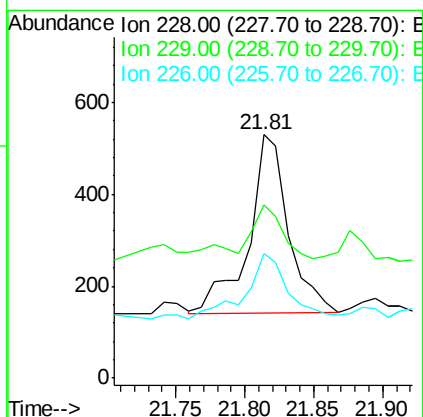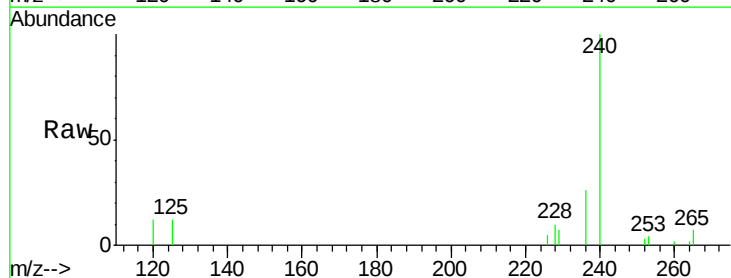

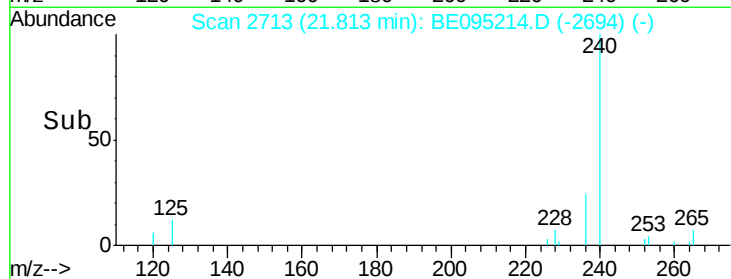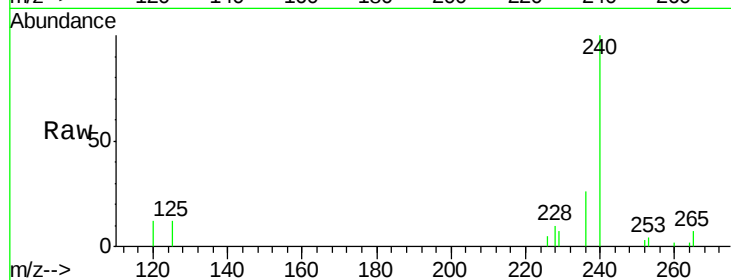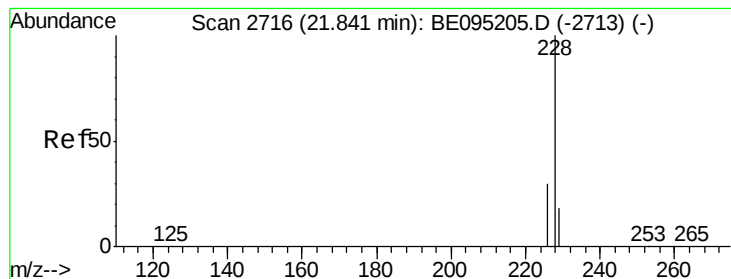

#19

Chrysene

Concen: 0.021 ng/ul

RT: 21.81 min Scan# 2713

Delta R.T. -0.03 min

Lab File: BE095214.D

Acq: 28 Jan 2018 19:33

Instrument :

BNA_E

ClientSampleId :

Tot Ion: 228 Resp: 785

Ion Ratio Lower Upper

228 100

226 50.9 23.4 35.0#

229 70.9 17.7 26.5#

