

Data Path : Z:\HPCHEM1\BNA E\DATA\BE012818\
 Data File : BE095216.D
 Acq On : 28 Jan 2018 20:44
 Operator : SJ/JU
 Sample : J1222-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Jan 29 07:00:12 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 29 06:58:46 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2699	0.40	ng/ul	0.00
2) Naphthalene-d8	11.27	136	8734	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	5614	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.71
16) Chrysene-d12	21.80	240	12325	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	616950	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	4323	0.30	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	12345	0.00	ng/ul	0.00
Target Compounds						
7) Acenaphthylene	14.74	152	839	0.031	ng/ul#	76
17) Pyrene	20.05	202	2842	0.069	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE012818\
Data File : BE095216.D
Acq On : 28 Jan 2018 20:44
Operator : SJ/JU
Sample : J1222-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Jan 29 07:00:12 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 29 06:58:46 2018
Response via : Initial Calibration

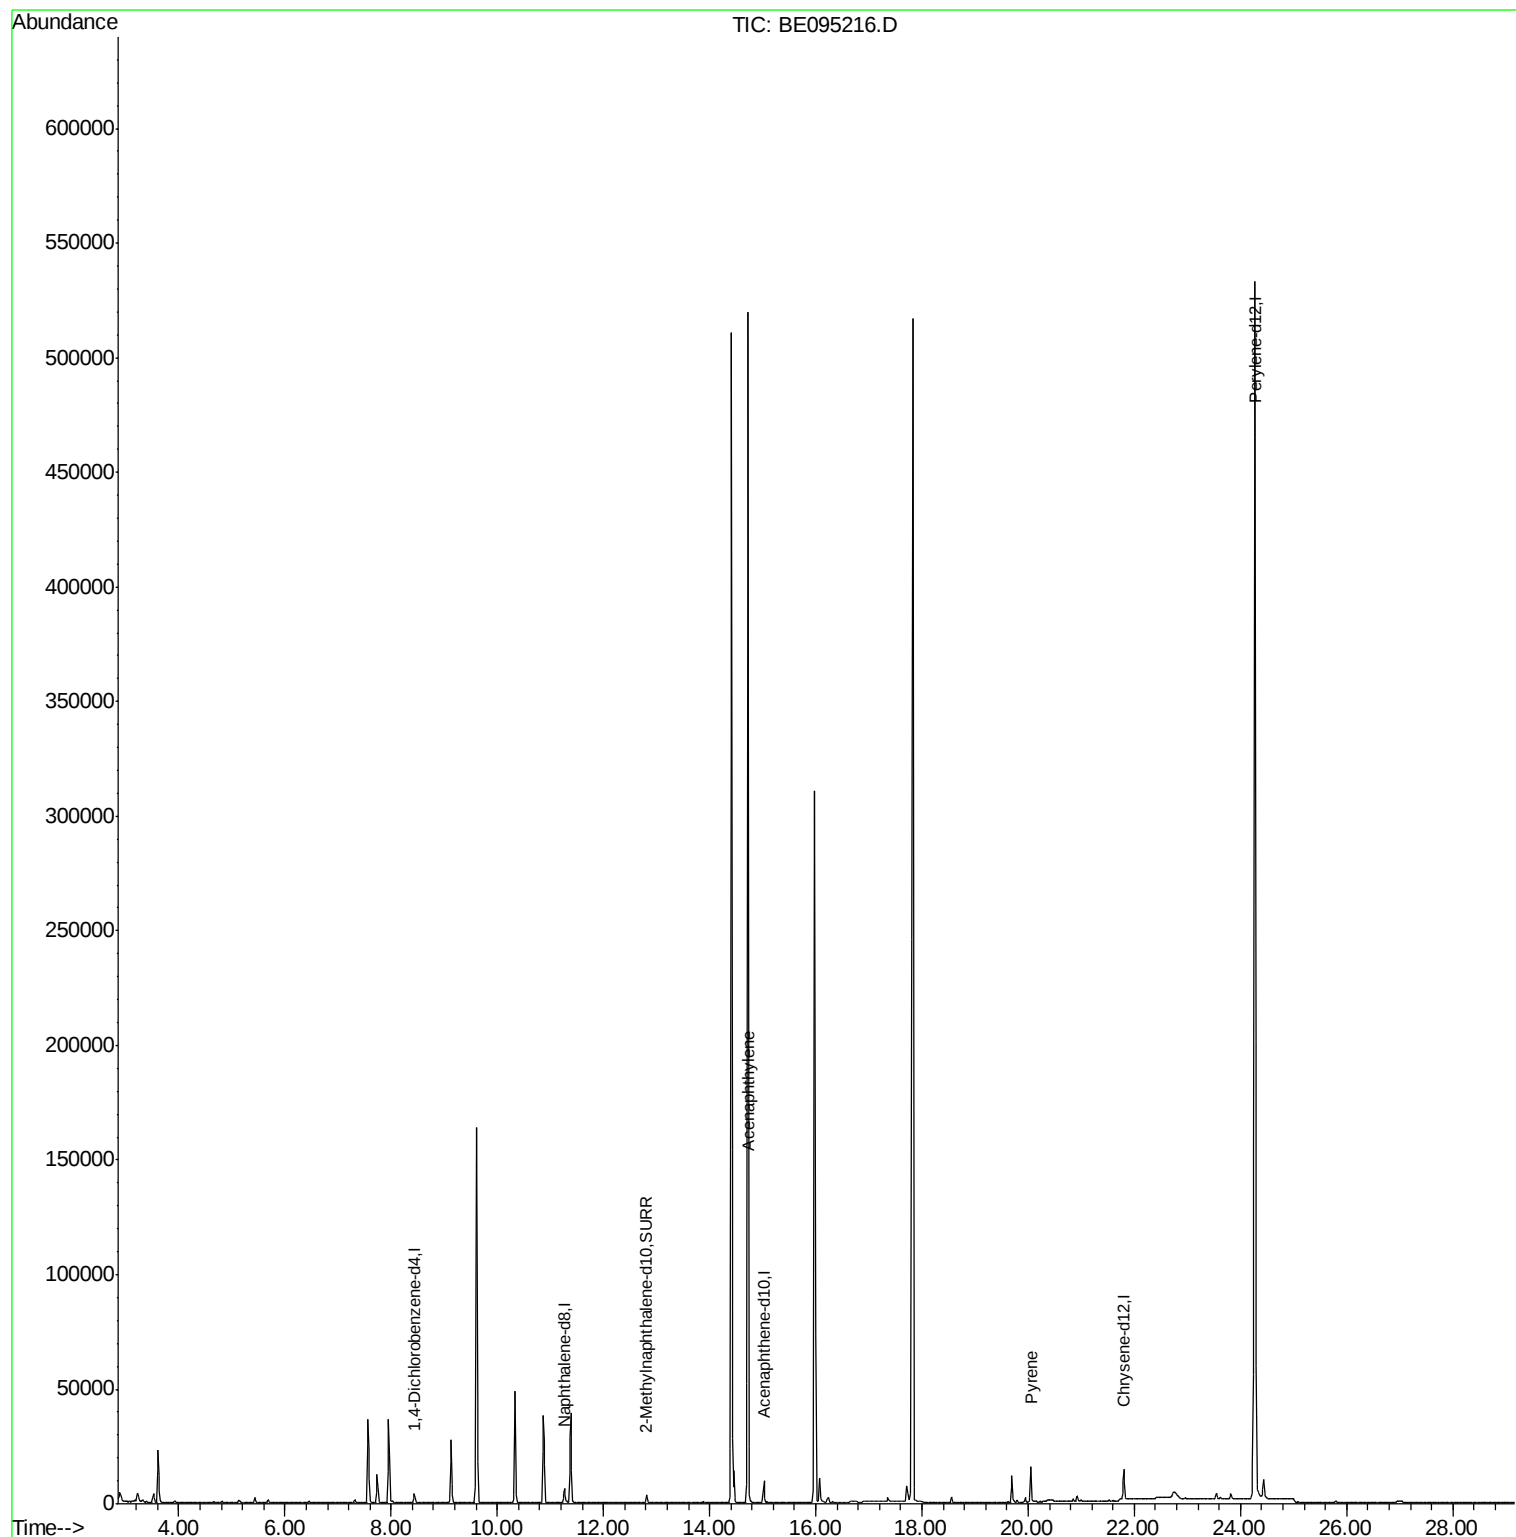

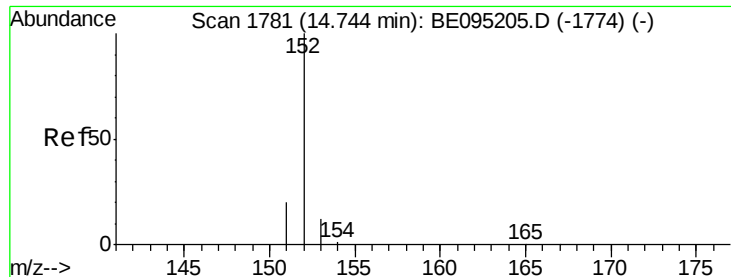

#7

Acenaphthylene

Concen: 0.031 ng/ul

RT: 14.74 min Scan# 1781

Delta R.T. 0.00 min

Lab File: BE095216.D

Acq: 28 Jan 2018 20:44

Instrument :

BNA_E

ClientSampleId :


Tot Ion:152 Resp: 839

Ion Ratio Lower Upper

152 100

151 32.3 17.1 25.7#




153 26.5 12.8 19.2#

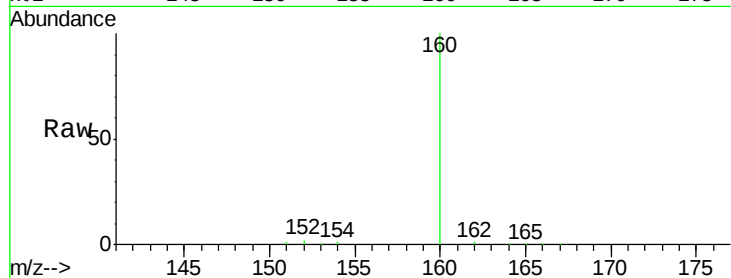

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

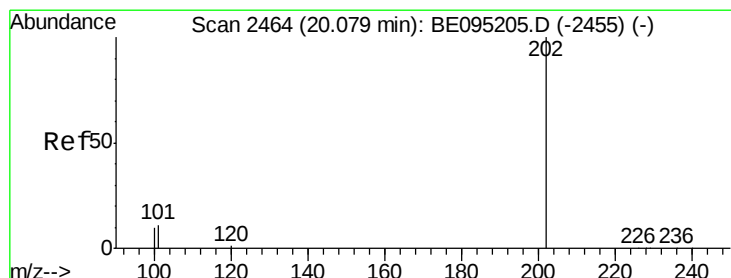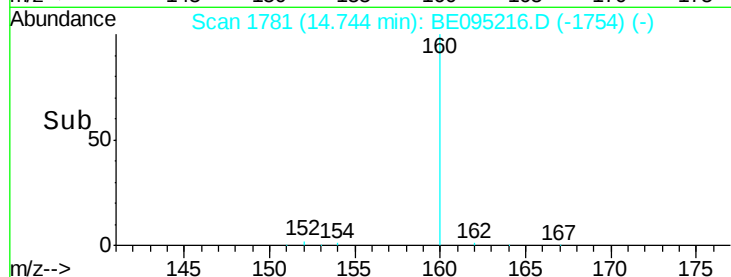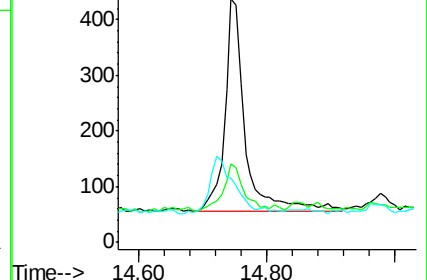

#17

Pyrene

Concen: 0.069 ng/ul

RT: 20.05 min Scan# 2461

Delta R.T. -0.03 min

Lab File: BE095216.D

Acq: 28 Jan 2018 20:44


Tgt Ion:202 Resp: 2842

Ion Ratio Lower Upper

202 100

101 162.7 18.2 27.4#

100 1066.8 15.6 23.4#

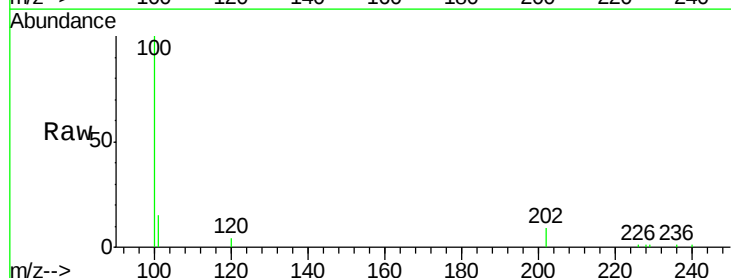

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

