

Data Path : Z:\HPCHEM1\BNA E\DATA\BE012818\
 Data File : BE095218.D
 Acq On : 28 Jan 2018 21:56
 Operator : SJ/JU
 Sample : J1222-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Jan 29 07:00:27 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 29 06:58:46 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2738	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	8619	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	5599	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.71
16) Chrysene-d12	21.80	240	11663	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	710793	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	4981	0.35	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	13782	0.00	ng/ul	0.00
Target Compounds						
3) Naphthalene	11.31	128	686	0.028	ng/ul#	68
5) 2-Methylnaphthalene	12.89	142	365	0.023	ng/ul	98
17) Pyrene	20.05	202	2855	0.073	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE012818\
Data File : BE095218.D
Acq On : 28 Jan 2018 21:56
Operator : SJ/JU
Sample : J1222-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Jan 29 07:00:27 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 29 06:58:46 2018
Response via : Initial Calibration

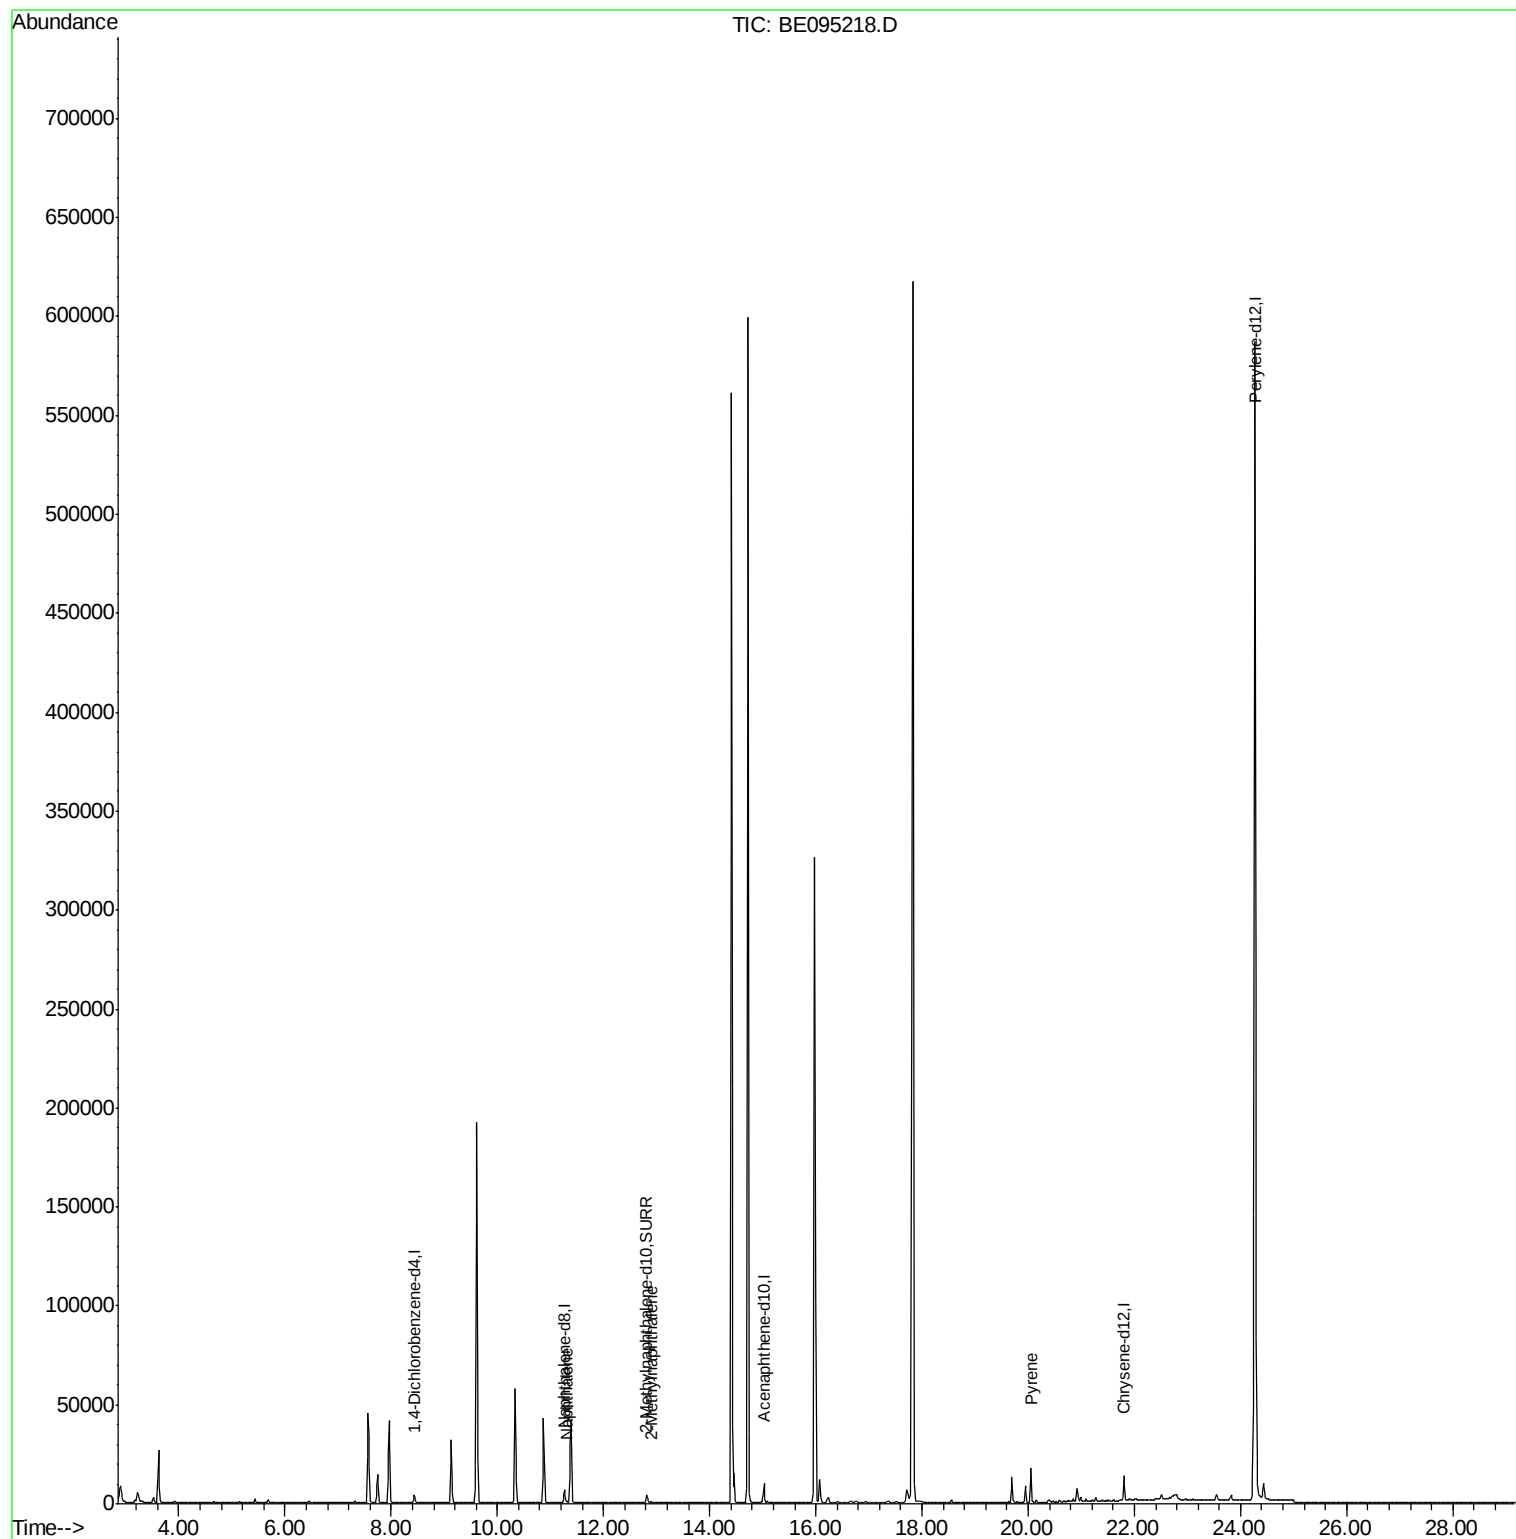

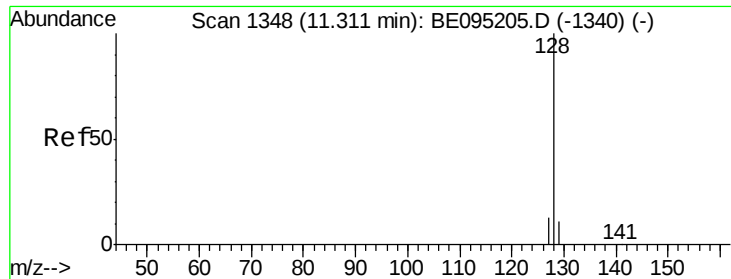

#3

Naphthalene

Concen: 0.028 ng/ul

RT: 11.31 min Scan# 1348

Delta R.T. -0.00 min

Lab File: BE095218.D

Acq: 28 Jan 2018 21:56

Instrument :

BNA_E

ClientSampleId :





Tot Ion:128 Resp: 686

Ion Ratio Lower Upper

128 100

129 23.6 11.3 16.9#

127 23.1 4.0 6.0#

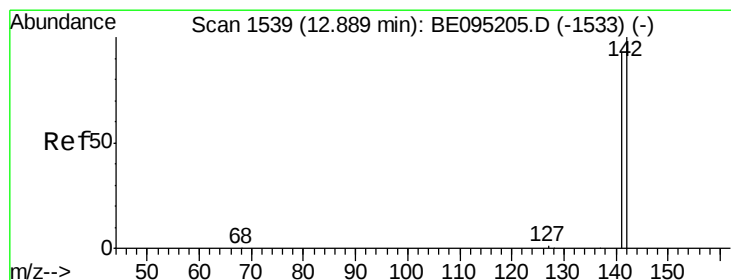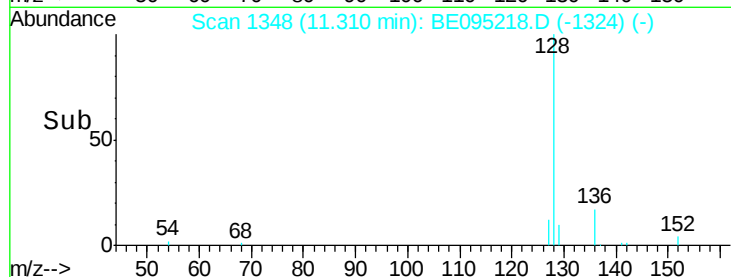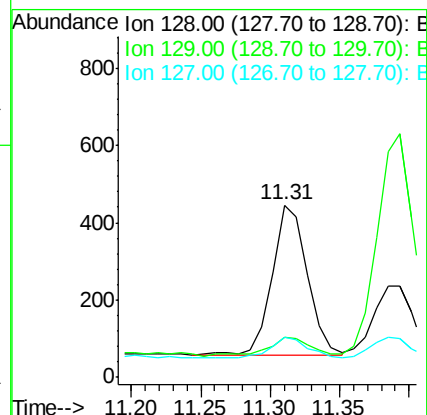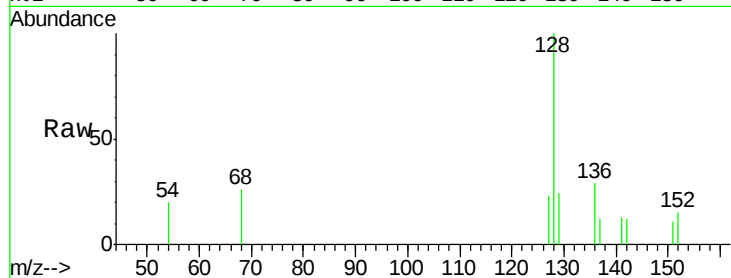

#5

2-Methylnaphthalene

Concen: 0.023 ng/ul

RT: 12.89 min Scan# 1539

Delta R.T. -0.00 min

Lab File: BE095218.D




Acq: 28 Jan 2018 21:56


Tgt Ion:142 Resp: 365

Ion Ratio Lower Upper

142 100

141 88.5 72.6 108.8

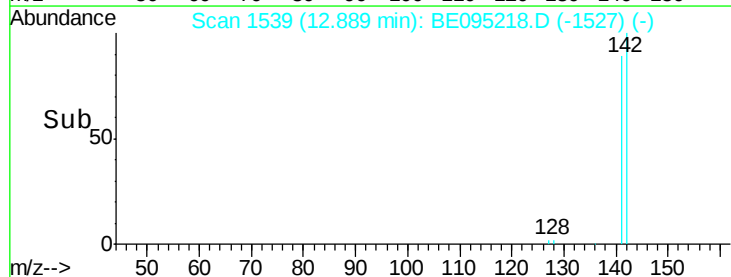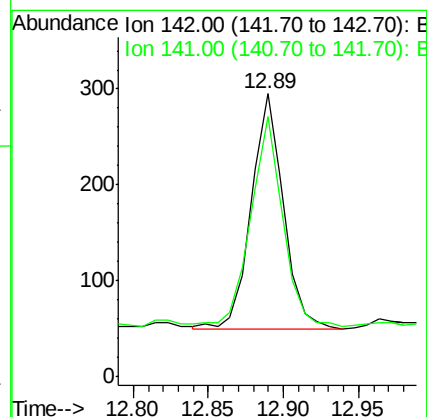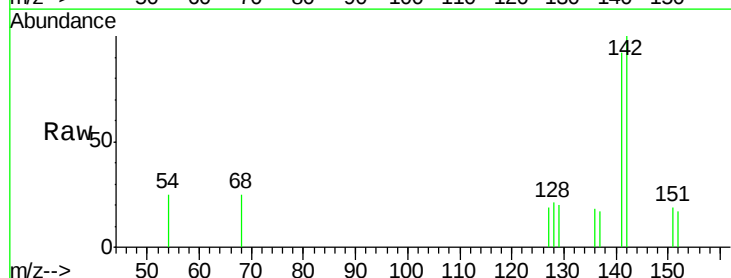

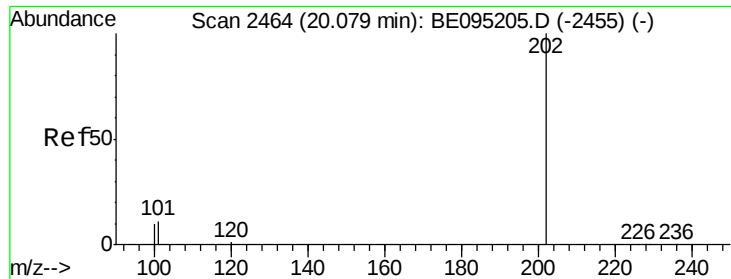

#17
 Pvrene
 Concen: 0.073 ng/ul
 RT: 20.05 min Scan# 2460
 Delta R.T. -0.03 min
 Lab File: BE095218.D
 Acq: 28 Jan 2018 21:56

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion: 202 Resp: 2855
 Ion Ratio Lower Upper
 202 100
 101 165.1 18.2 27.4#
 100 1123.8 15.6 23.4#

