

Data Path : Z:\HPCHEM1\BNA E\DATA\BE012818\
 Data File : BE095237.D
 Acq On : 29 Jan 2018 9:13
 Operator : SJ/JU
 Sample : J1222-17
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Jan 29 12:14:03 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 29 08:11:22 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	3295	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	10845	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	6969	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.71
16) Chrysene-d12	21.80	240	14513	0.40	ng/ul	0.00
20) Perylene-d12	24.28	264	1008727	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	6754	0.38	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	18094	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	20.06	202	4087	0.084	ng/ul#	1
18) Benzo(a)anthracene	21.79	228	988	0.022	ng/ul#	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE012818\
Data File : BE095237.D
Acq On : 29 Jan 2018 9:13
Operator : SJ/JU
Sample : J1222-17
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Jan 29 12:14:03 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 29 08:11:22 2018
Response via : Initial Calibration




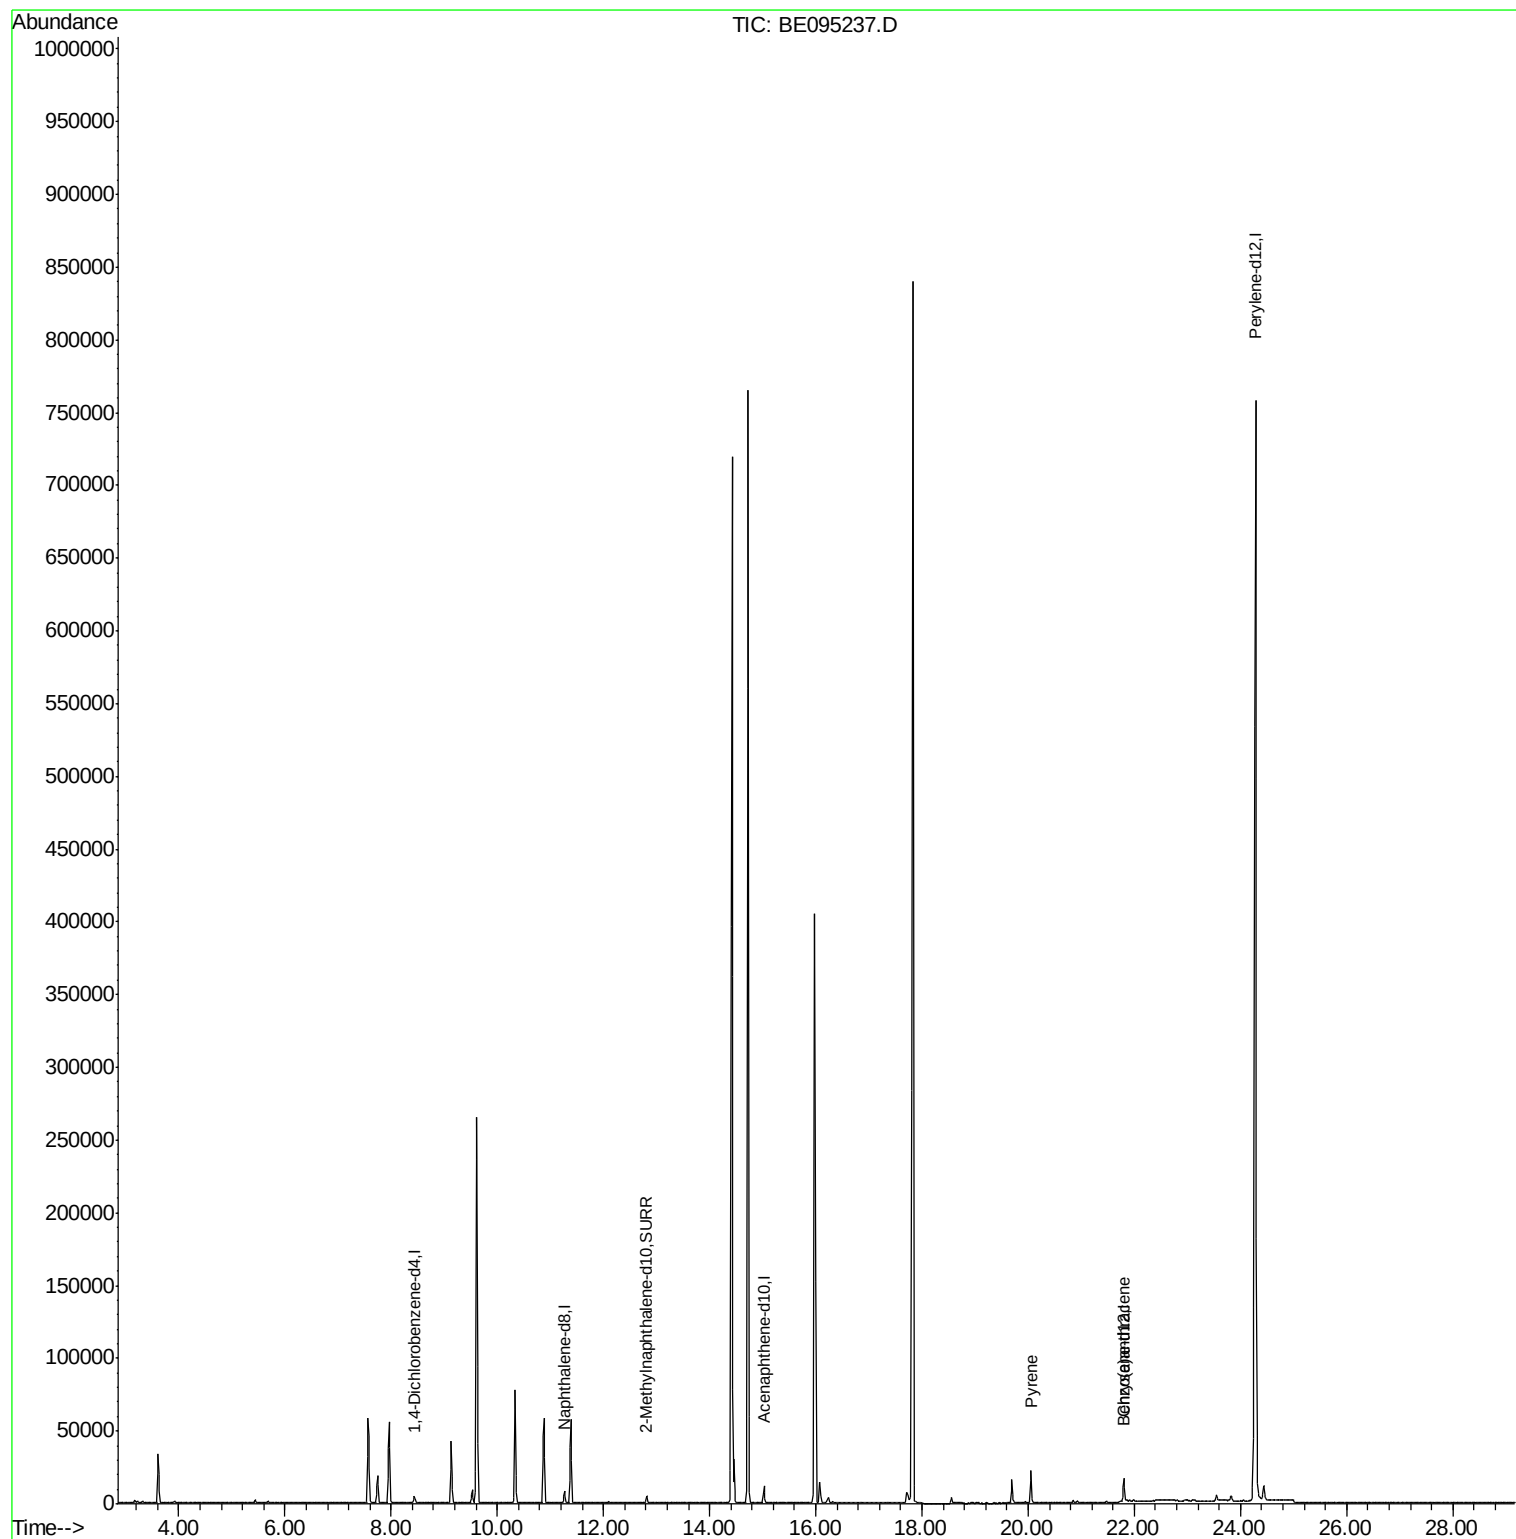


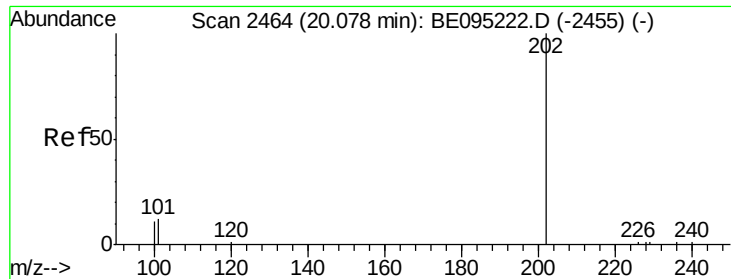

#17
 Pvrene
 Concen: 0.084 ng/ul
 RT: 20.06 min Scan# 2462
 Delta R.T. -0.02 min
 Lab File: BE095237.D
 Acq: 29 Jan 2018 9:13

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:202 Resp: 4087
 Ion Ratio Lower Upper
 202 100
 101 155.9 18.2 27.4#
 100 966.5 15.6 23.4#

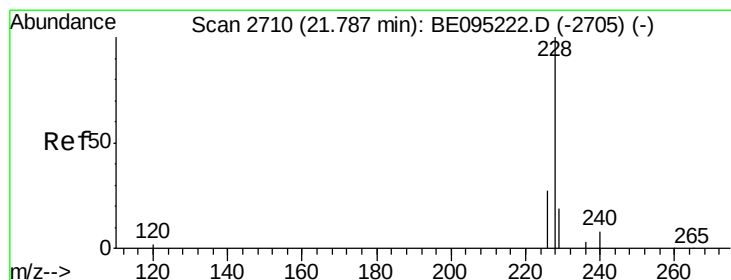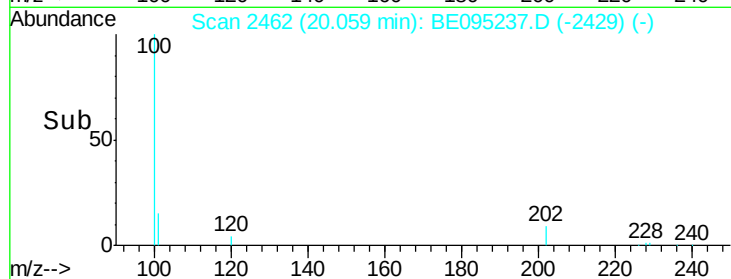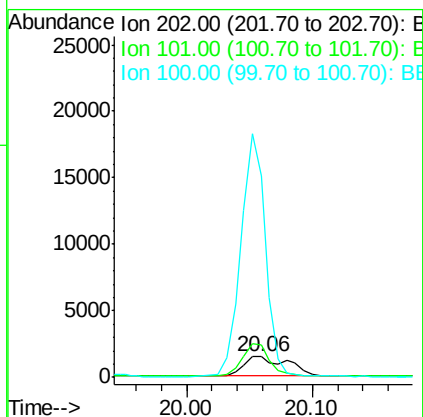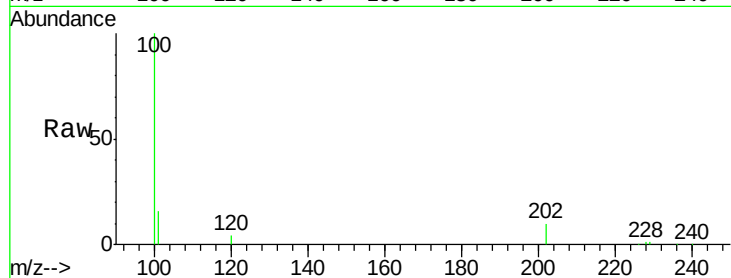

#18
 Benzo(a)anthracene
 Concen: 0.022 ng/ul
 RT: 21.79 min Scan# 2711
 Delta R.T. -0.00 min
 Lab File: BE095237.D
 Acq: 29 Jan 2018 9:13

Tgt Ion:228 Resp: 988
 Ion Ratio Lower Upper
 228 100
 229 44.0 22.8 34.2#
 226 39.7 17.0 25.6#

