

Data Path : Z:\HPCHEM1\BNA\_E\Data\BE012915\  
 Data File : BE089427.D  
 Acq On : 30 Jan 2015 00:58  
 Operator : TP/IZ  
 Sample : G1110-11  
 Misc :  
 ALS Vial : 23 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 MPE-9

Quant Time: Jan 30 07:37:16 2015  
 Quant Method : Z:\HPCHEM1\BNA\_E\METHODS\SIM-BE012915.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jan 30 03:48:17 2015  
 Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc | Units | Dev(Min) |
|---------------------------|-------|------|----------|------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 9.58  | 152  | 125135   | 5.00 | ng    | 0.00     |
| 7) Naphthalene-d8         | 12.50 | 136  | 477927   | 5.00 | ng    | 0.00     |
| 13) Acenaphthene-d10      | 16.68 | 164  | 224817   | 5.00 | ng    | 0.00     |
| 17) Phenanthrene-d10      | 19.99 | 188  | 438636   | 5.00 | ng    | 0.00     |
| 20) Chrysene-d12          | 23.84 | 240  | 557623   | 5.00 | ng    | 0.00     |
| 27) Perylene-d12          | 25.55 | 264  | 595665   | 5.00 | ng    | 0.00     |

|                             |       |     |        |       |    |      |
|-----------------------------|-------|-----|--------|-------|----|------|
| System Monitoring Compounds |       |     |        |       |    |      |
| 3) 2-Fluorophenol           | 6.74  | 112 | 156464 | 3.32  | ng | 0.00 |
| 4) Phenol-d6                | 8.85  | 99  | 156513 | 2.80  | ng | 0.00 |
| 8) Nitrobenzene-d5          | 10.85 | 82  | 200283 | 5.15  | ng | 0.00 |
| 14) 2,4,6-Tribromophenol    | 18.58 | 330 | 78671  | 12.68 | ng | 0.00 |
| 15) 2-Fluorobiphenyl        | 15.13 | 172 | 335097 | 5.34  | ng | 0.00 |
| 22) Terphenyl-d14           | 22.48 | 244 | 629463 | 9.77  | ng | 0.00 |


|                            |       |     |       |      |    |        |
|----------------------------|-------|-----|-------|------|----|--------|
| Target Compounds           |       |     |       |      |    | Qvalue |
| 2) n-Nitrosodimethylamine  | 3.56  | 42  | 45    | 0.00 | ng | # 1    |
| 5) Phenol                  | 8.88  | 94  | 17907 | 0.29 | ng | 94     |
| 6) bis(2-Chloroethyl)ether | 9.07  | 93  | 469   | 0.01 | ng | # 1    |
| 9) Nitrobenzene            | 10.85 | 77  | 696   | 0.02 | ng | # 42   |
| 10) 2,4-Dimethylphenol     | 11.83 | 122 | 83    | 0.00 | ng | # 73   |
| 11) 2,4-Dichlorophenol     | 12.21 | 162 | 61    | 0.00 | ng | # 39   |
| 16) 2,4-Dinitrophenol      | 16.88 | 184 | 4     | 0.00 | ng | # 19   |
| 18) Hexachlorobenzene      | 19.23 | 284 | 26    | 0.00 | ng | # 1    |
| 19) Pentachlorophenol      | 19.65 | 266 | 68    | 0.02 | ng | # 77   |
| 21) Benzidine              | 22.14 | 184 | 152   | 0.00 | ng | # 1    |
| 23) Benzo(a)anthracene     | 23.84 | 228 | 9174  | 0.02 | ng | # 75   |
| 24) 3,3'-Dichlorobenzidine | 23.79 | 252 | 173   | 0.01 | ng | # 1    |
| 25) Chrysene               | 23.84 | 228 | 9174  | 0.02 | ng | # 76   |
| 26) Indeno(1,2,3-cd)pyrene | 27.06 | 276 | 671   | 0.01 | ng | # 100  |
| 28) Benzo(b)fluoranthene   | 25.10 | 252 | 419   | 0.01 | ng | # 1    |
| 29) Benzo(k)fluoranthene   | 25.13 | 252 | 717   | 0.00 | ng | # 1    |
| 30) Benzo(a)pyrene         | 25.48 | 252 | 493   | 0.01 | ng | # 1    |
| 31) Dibenzo(a,h)anthracene | 27.10 | 278 | 322   | 0.00 | ng | # 1    |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA\_E\Data\BE012915\  
Data File : BE089427.D  
Acq On : 30 Jan 2015 00:58  
Operator : TP/IZ  
Sample : G1110-11  
Misc :  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
MPE-9

Quant Time: Jan 30 07:37:16 2015  
Quant Method : Z:\HPCHEM1\BNA\_E\METHODS\SIM-BE012915.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jan 30 03:48:17 2015  
Response via : Initial Calibration

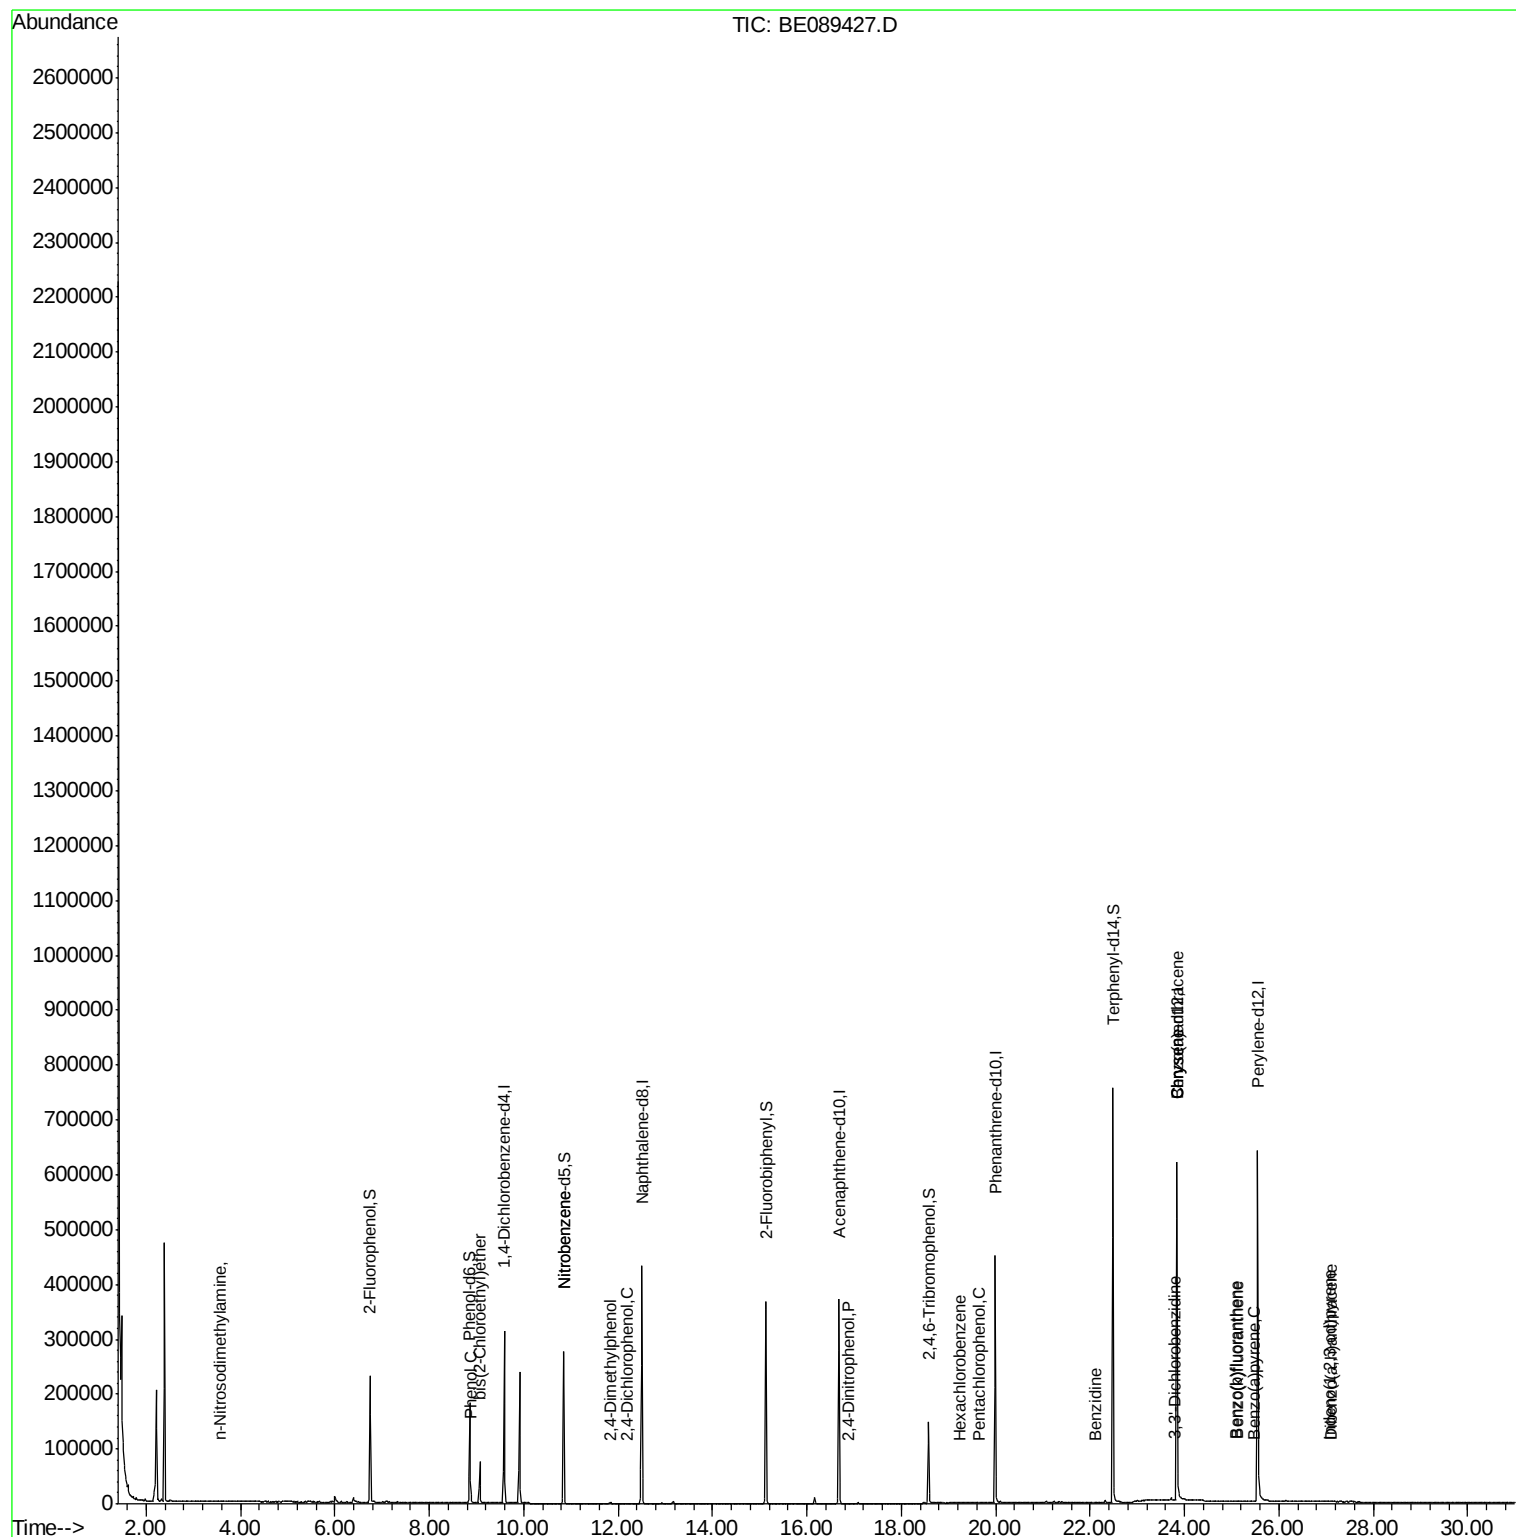



#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 9.58 min Scan# 1131

Delta R.T. -0.00 min

Lab File: BE089427.D

Acq: 30 Jan 2015 00:58

Instrument :

BNA\_E

ClientSampleId :

MPE-9


Tgt Ion:152 Resp: 125135

Ion Ratio Lower Upper

152 100

150 159.3 126.1 189.1




115 71.8 57.1 85.7



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

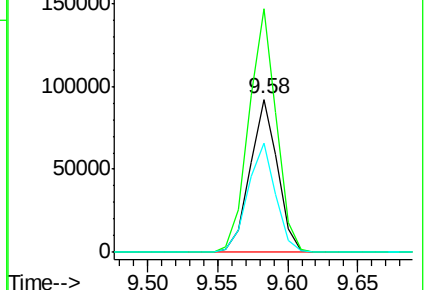

#2

n-Nitrosodimethylamine

Concen: 0.00 ng

RT: 3.56 min Scan# 319

Delta R.T. -0.01 min

Lab File: BE089427.D

Acq: 30 Jan 2015 00:58


Tgt Ion: 42 Resp: 45

Ion Ratio Lower Upper

42 100

74 43.1 90.2 135.2#



44 1304.7 19.4 29.2#




Abundance Ion 42.00 (41.70 to 42.70): BE0

Ion 74.00 (73.70 to 74.70): BE0

Ion 44.00 (43.70 to 44.70): BE0



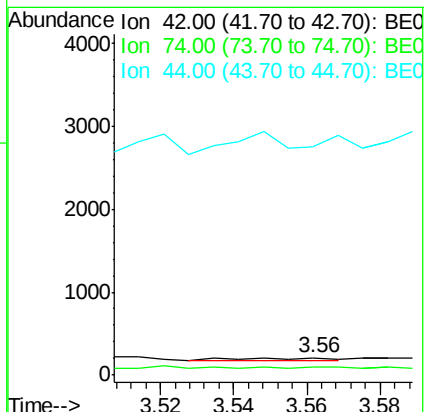



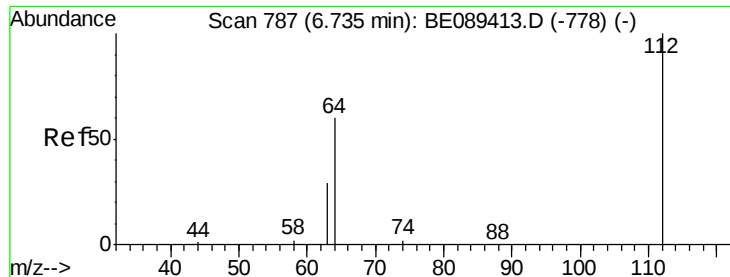

#3  
 2-Fluorophenol  
 Concen: 3.32 ng  
 RT: 6.74 min Scan# 788  
 Delta R.T. 0.01 min  
 Lab File: BE089427.D  
 Acq: 30 Jan 2015 00:58




Instrument :  
 BNA\_E  
 ClientSampleId :  
 MPE-9


|          |       |       |        |
|----------|-------|-------|--------|
| Tgt Ion: | 112   | Resp: | 156464 |
| Ion      | Ratio | Lower | Upper  |
| 112      | 100   |       |        |
| 64       | 62.2  | 48.2  | 72.4   |
| 63       | 30.9  | 23.5  | 35.3   |

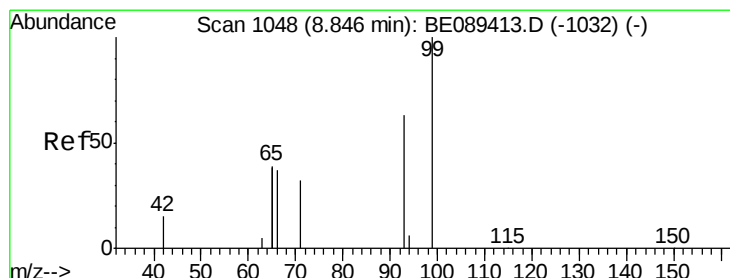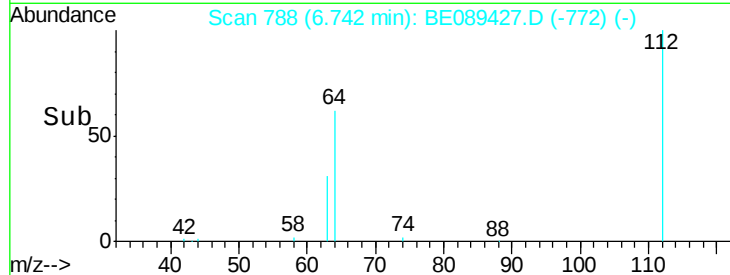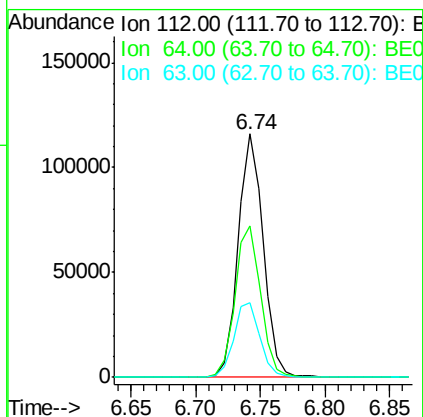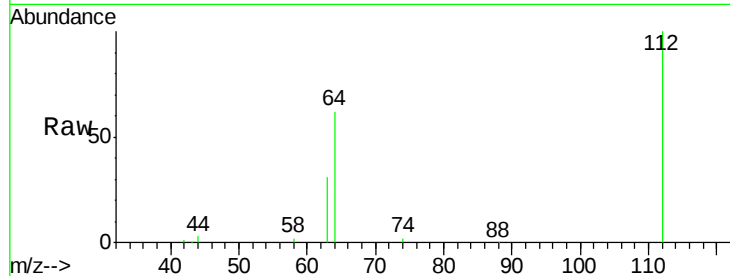

#4  
 Phenol-d6  
 Concen: 2.80 ng  
 RT: 8.85 min Scan# 1049  
 Delta R.T. 0.01 min  
 Lab File: BE089427.D  
 Acq: 30 Jan 2015 00:58

|          |       |       |        |
|----------|-------|-------|--------|
| Tgt Ion: | 99    | Resp: | 156513 |
| Ion      | Ratio | Lower | Upper  |
| 99       | 100   |       |        |
| 42       | 14.2  | 11.9  | 17.9   |
| 71       | 33.1  | 25.8  | 38.6   |

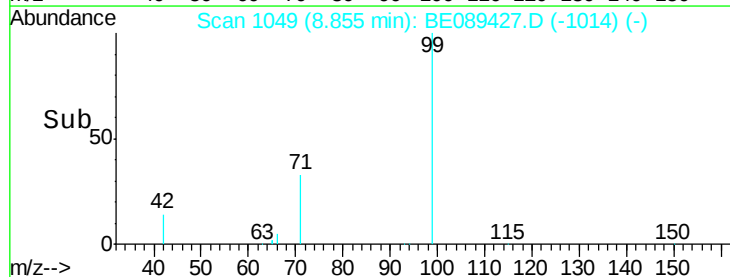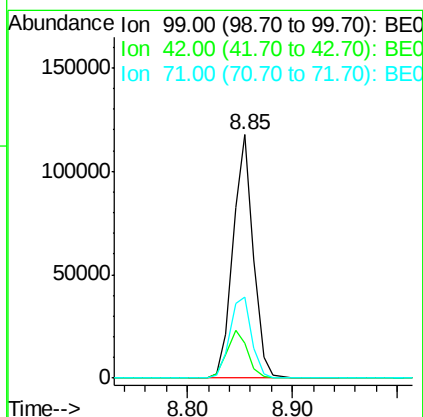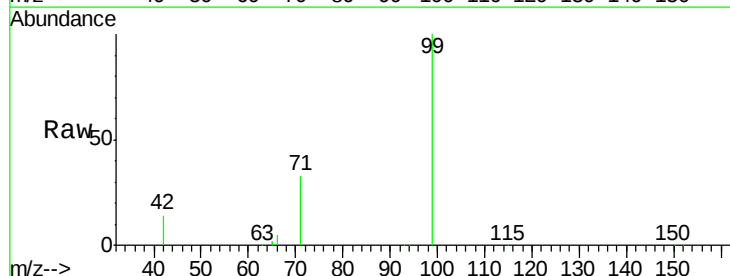

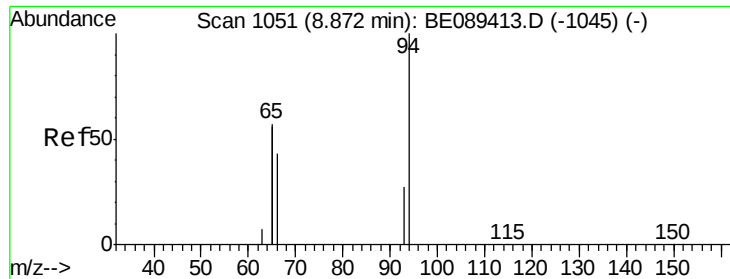

#5

Phenol

Concen: 0.29 ng

RT: 8.88 min Scan# 1052

Delta R.T. 0.01 min

Lab File: BE089427.D

Acq: 30 Jan 2015 00:58

Instrument :

BNA\_E

ClientSampleId :

MPE-9





Tgt Ion: 94 Resp: 17907

Ion Ratio Lower Upper

94 100

65 108.3 93.3 133.3

66 37.4 23.6 63.6

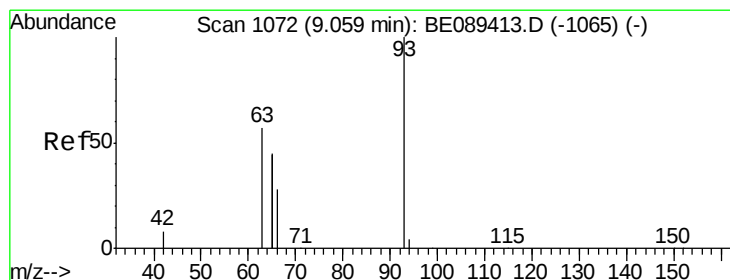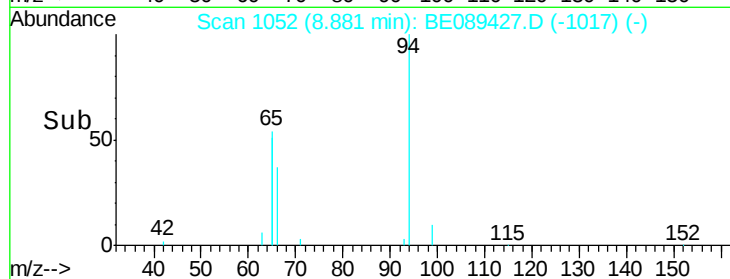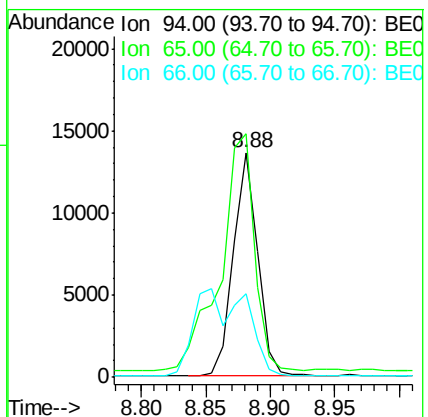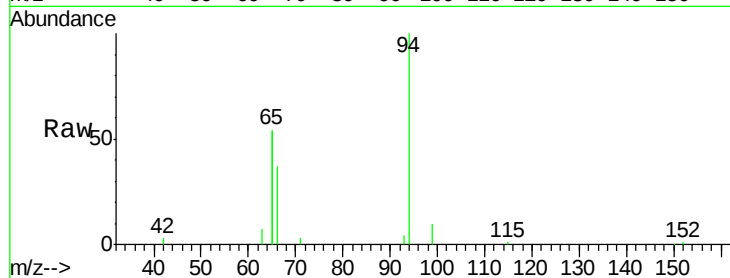

#6

bis(2-Chloroethyl)ether

Concen: 0.01 ng

RT: 9.07 min Scan# 1073

Delta R.T. 0.01 min

Lab File: BE089427.D

Acq: 30 Jan 2015 00:58




Tgt Ion: 93 Resp: 469


Ion Ratio Lower Upper

93 100

63 569.7 58.6 88.0#

95 0.0 0.0 0.0

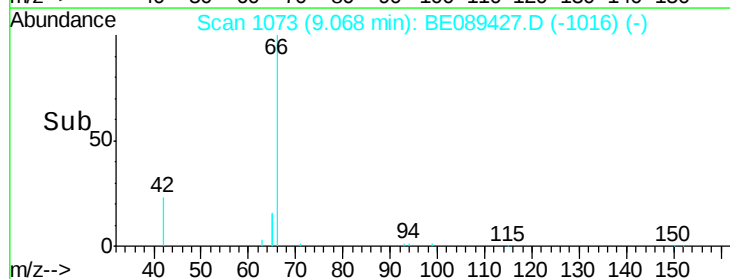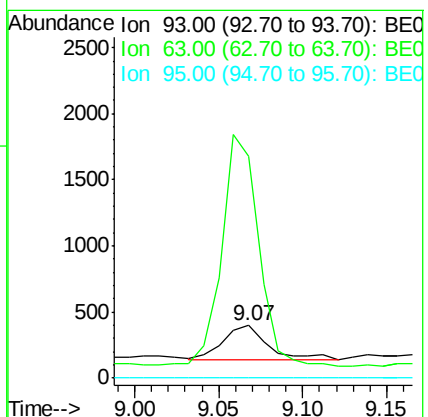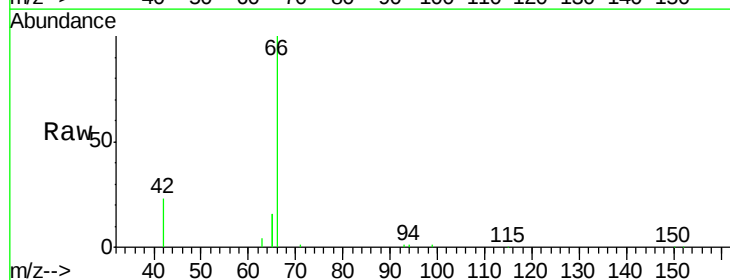



#7

Naphthalene-d8

Concen: 5.00 ng

RT: 12.50 min Scan# 1562

Delta R.T. -0.00 min

Lab File: BE089427.D

Acq: 30 Jan 2015 00:58

Instrument :

BNA\_E

ClientSampleId :

MPE-9


Tgt Ion: 136 Resp: 477927

Ion Ratio Lower Upper

136 100

137 10.7 8.6 12.8




54 9.4 7.5 11.3



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

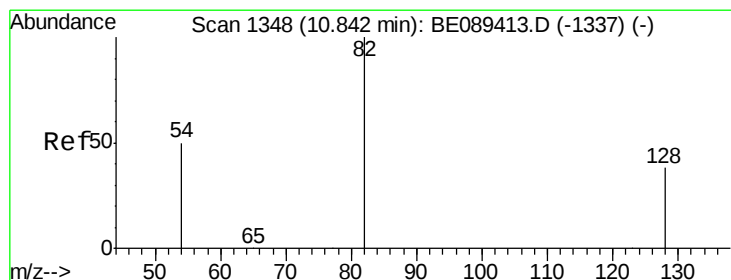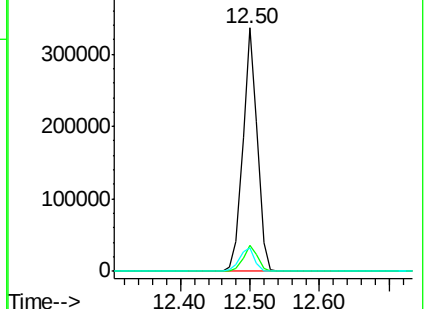

#8

Nitrobenzene-d5

Concen: 5.15 ng

RT: 10.85 min Scan# 1349

Delta R.T. 0.00 min

Lab File: BE089427.D

Acq: 30 Jan 2015 00:58


Tgt Ion: 82 Resp: 200283

Ion Ratio Lower Upper

82 100

128 40.2 31.0 46.4



54 47.9 39.8 59.6




Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0

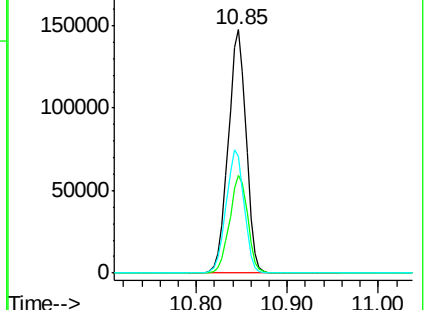

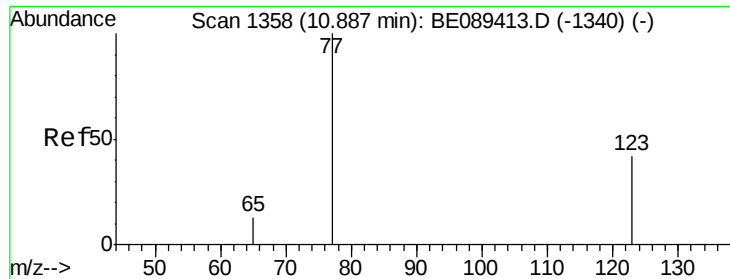

#9

Nitrobenzene

Concen: 0.02 ng

RT: 10.85 min Scan# 1349

Delta R.T. -0.04 min

Lab File: BE089427.D

Acq: 30 Jan 2015 00:58

Instrument :

BNA\_E

ClientSampleId :

MPE-9


Tgt Ion: 77 Resp: 696

Ion Ratio Lower Upper

77 100

123 1.7 32.8 49.2#

65 31.3 11.0 16.6#



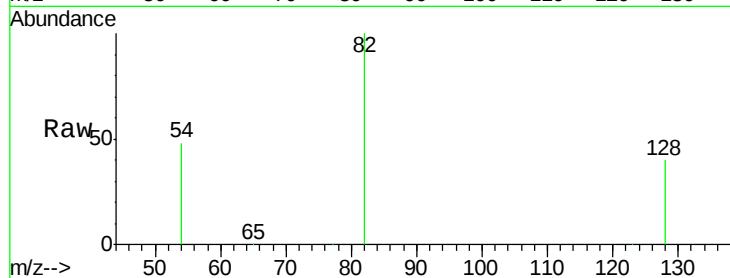


Abundance Ion 77.00 (76.70 to 77.70): BE089413.D (-1340) (-)

Ion 123.00 (122.70 to 123.70): BE089413.D (-1340) (-)

Ion 65.00 (64.70 to 65.70): BE089413.D (-1340) (-)

Time-->

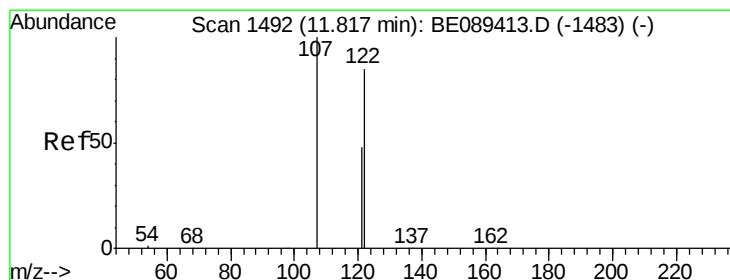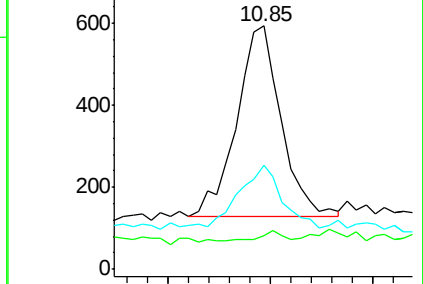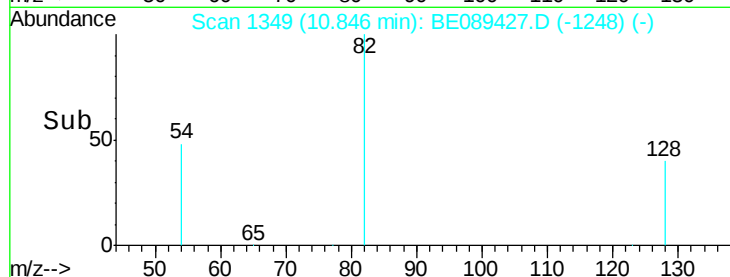

#10

2,4-Dimethylphenol

Concen: 0.00 ng

RT: 11.83 min Scan# 1493

Delta R.T. 0.01 min

Lab File: BE089427.D

Acq: 30 Jan 2015 00:58


Tgt Ion: 122 Resp: 83

Ion Ratio Lower Upper

122 100

107 127.3 94.6 142.0

121 106.4 45.8 68.6#


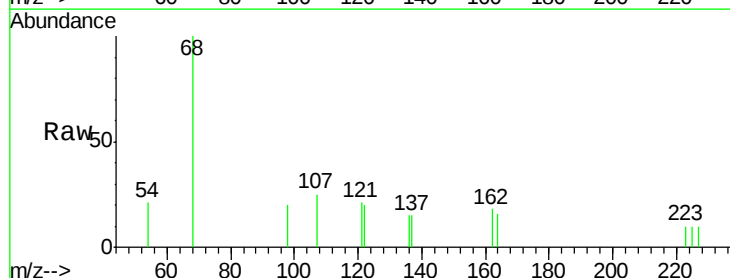



Abundance Ion 122.00 (121.70 to 122.70): BE089413.D (-1483) (-)

Ion 107.00 (106.70 to 107.70): BE089413.D (-1483) (-)

Ion 121.00 (120.70 to 121.70): BE089413.D (-1483) (-)

Time-->



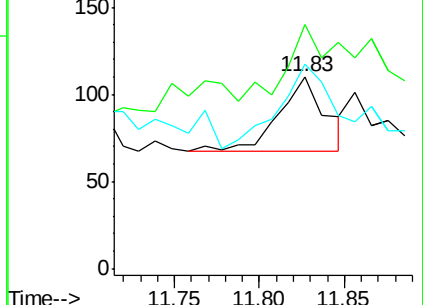
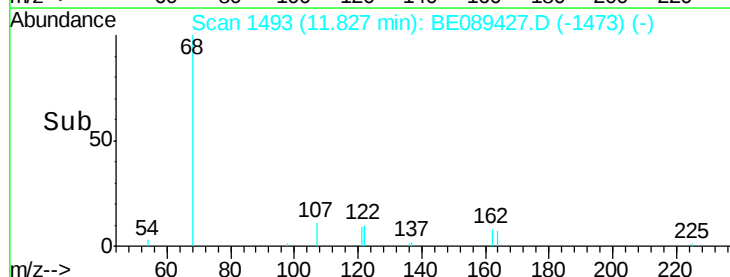




#11  
 2,4-Dichlorophenol  
 Concen: 0.00 ng  
 RT: 12.21 min Scan# 1532  
 Delta R.T. -0.00 min  
 Lab File: BE089427.D  
 Acq: 30 Jan 2015 00:58




Instrument :  
 BNA\_E  
 ClientSampled :  
 MPE-9


Tgt Ion:162 Resp: 61  
 Ion Ratio Lower Upper  
 162 100  
 164 77.8 46.1 86.1  
 98 122.2 16.2 56.2#

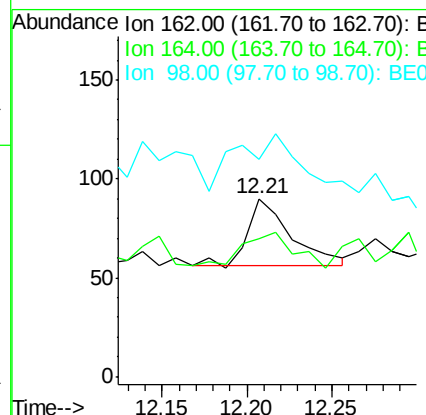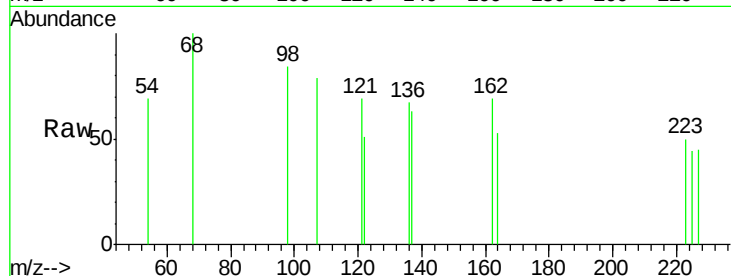

#13  
 Acenaphthene-d10  
 Concen: 5.00 ng  
 RT: 16.68 min Scan# 2755  
 Delta R.T. -0.00 min  
 Lab File: BE089427.D  
 Acq: 30 Jan 2015 00:58

Tgt Ion:164 Resp: 224817  
 Ion Ratio Lower Upper  
 164 100  
 162 95.7 77.0 115.6  
 160 43.7 35.0 52.4



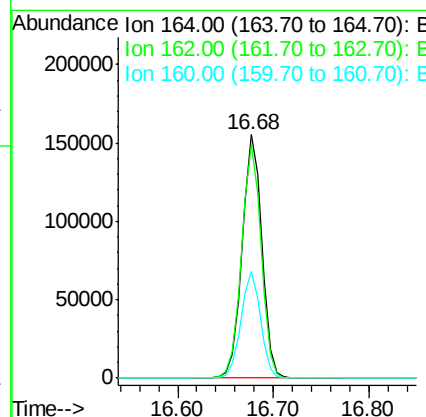





#14  
 2,4,6-Tribromophenol  
 Concen: 12.68 ng  
 RT: 18.58 min Scan# 3035  
 Delta R.T. 0.01 min  
 Lab File: BE089427.D  
 Acq: 30 Jan 2015 00:58




Instrument :  
 BNA\_E  
 ClientSampleId :  
 MPE-9


Tgt Ion: 330 Resp: 78671  
 Ion Ratio Lower Upper  
 330 100  
 332 97.2 76.0 114.0  
 141 42.8 35.6 53.4

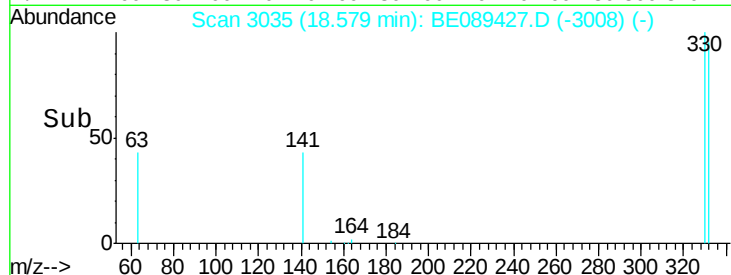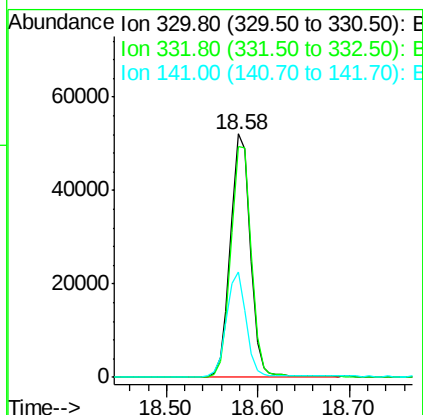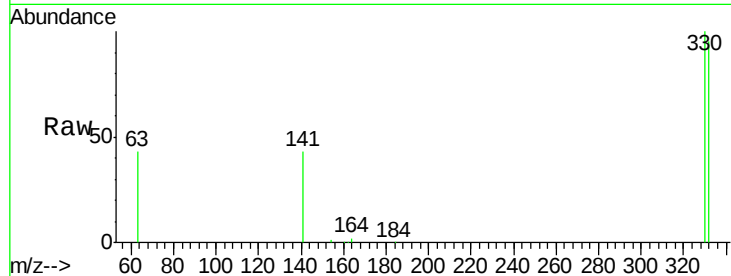

#15  
 2-Fluorobiphenyl  
 Concen: 5.34 ng  
 RT: 15.13 min Scan# 2425  
 Delta R.T. 0.00 min  
 Lab File: BE089427.D  
 Acq: 30 Jan 2015 00:58

Tgt Ion: 172 Resp: 335097  
 Ion Ratio Lower Upper  
 172 100  
 171 33.8 26.6 39.8  
 170 22.7 17.1 25.7


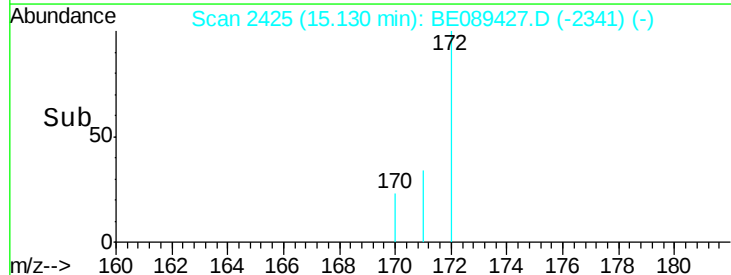
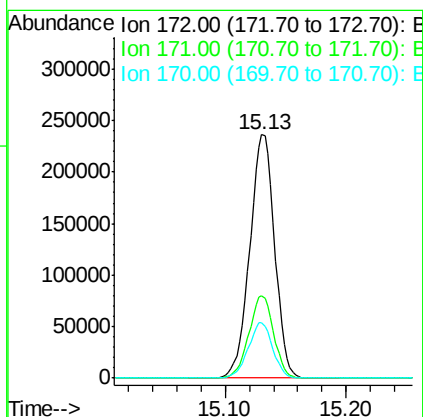





#16  
2,4-Dinitrophenol  
Concen: 0.00 ng  
RT: 16.88 min Scan# 2785  
Delta R.T. -0.01 min  
Lab File: BE089427.D  
Acq: 30 Jan 2015 00:58




Instrument :  
BNA\_E  
ClientSampleId :  
MPE-9


Tgt Ion:184 Resp: 4  
Ion Ratio Lower Upper  
184 100  
63 206.9 79.0 118.4#  
154 104.2 55.8 83.6#

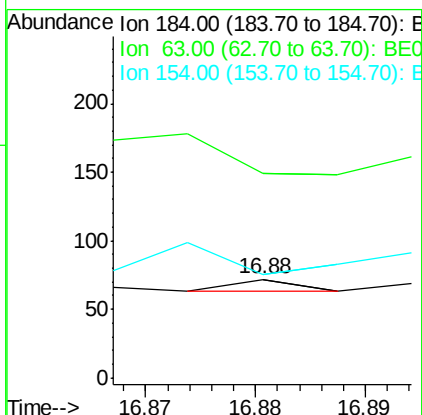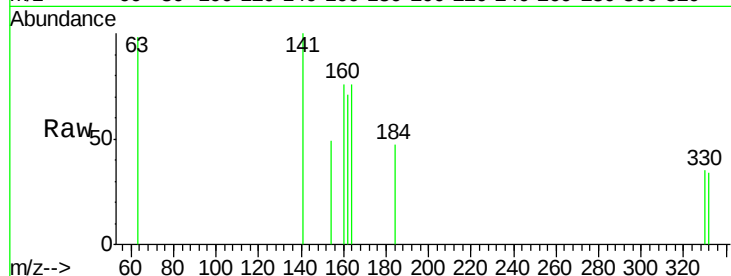

#17  
Phenanthrene-d10  
Concen: 5.00 ng  
RT: 19.99 min Scan# 3240  
Delta R.T. 0.01 min  
Lab File: BE089427.D  
Acq: 30 Jan 2015 00:58

Tgt Ion:188 Resp: 438636  
Ion Ratio Lower Upper  
188 100  
94 14.3 13.0 19.6  
80 14.8 14.2 21.4



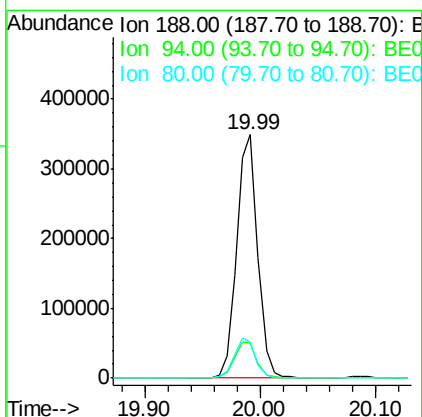





#18  
Hexachlorobenzene  
Concen: 0.00 ng  
RT: 19.23 min Scan# 3128  
Delta R.T. -0.00 min  
Lab File: BE089427.D  
Acq: 30 Jan 2015 00:58




Instrument :  
BNA\_E  
ClientSampled :  
MPE-9


Tgt Ion:284 Resp: 26  
Ion Ratio Lower Upper  
284 100  
142 218.1 28.3 42.5#  
249 88.9 19.9 29.9#

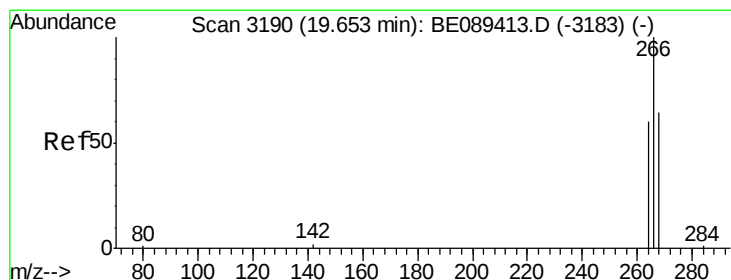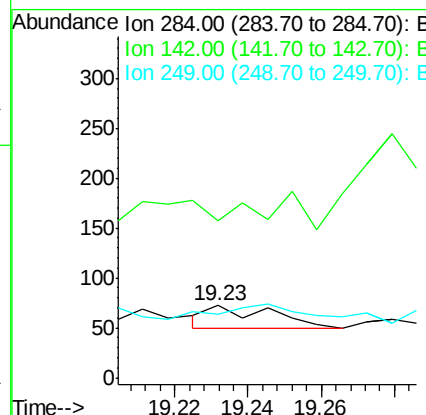

#19  
Pentachlorophenol  
Concen: 0.02 ng  
RT: 19.65 min Scan# 3190  
Delta R.T. 0.00 min  
Lab File: BE089427.D  
Acq: 30 Jan 2015 00:58

Tgt Ion:266 Resp: 68  
Ion Ratio Lower Upper  
266 100  
268 80.7 51.9 77.9#  
264 79.8 48.5 72.7#

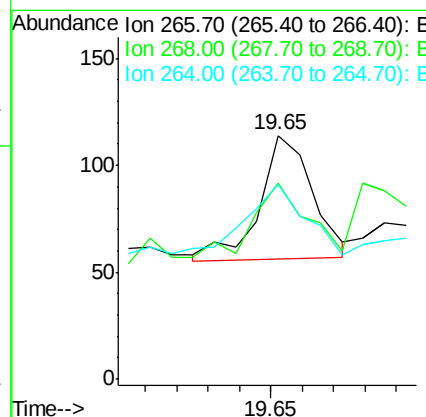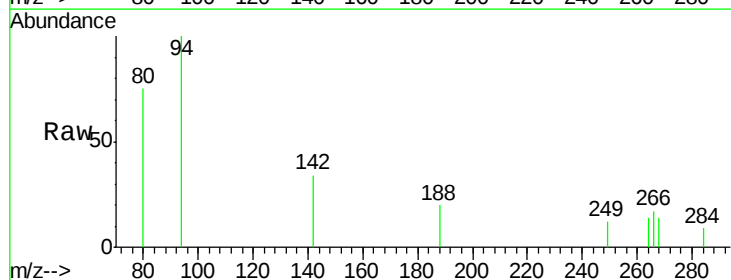

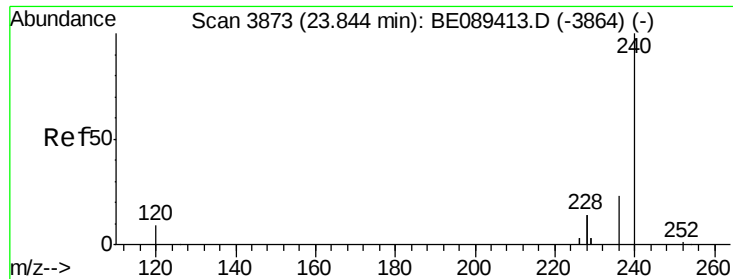

#20

Chrysene-d12

Concen: 5.00 ng

RT: 23.84 min Scan# 3873

Delta R.T. -0.00 min

Lab File: BE089427.D

Acq: 30 Jan 2015 00:58

Instrument :

BNA\_E

ClientSampleId :

MPE-9


Tgt Ion:240 Resp: 557623

Ion Ratio Lower Upper

240 100

120 7.8 6.9 10.3




236 22.9 18.2 27.2

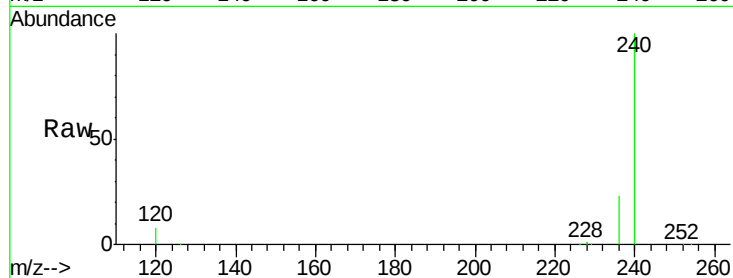

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

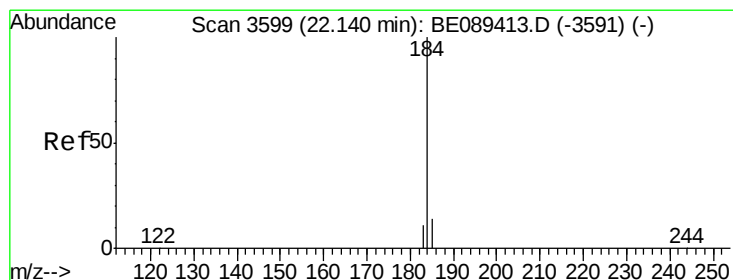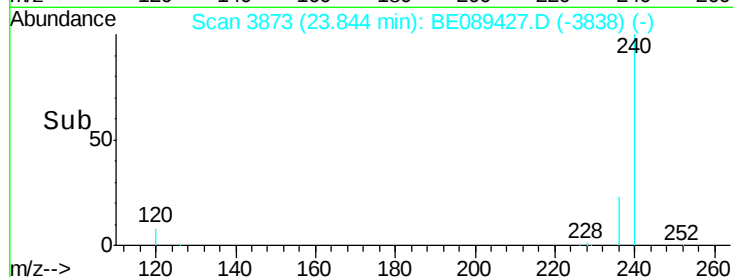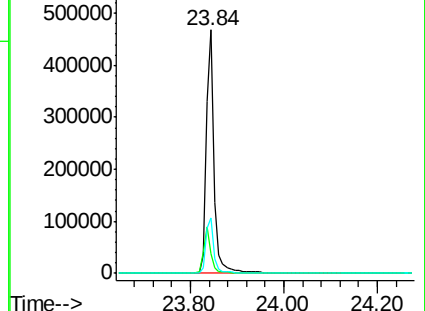

#21

Benzidine

Concen: 0.00 ng

RT: 22.14 min Scan# 3598

Delta R.T. -0.00 min

Lab File: BE089427.D

Acq: 30 Jan 2015 00:58


Tgt Ion:184 Resp: 152

Ion Ratio Lower Upper

184 100

185 111.1 11.0 16.6#



183 111.6 8.6 13.0#

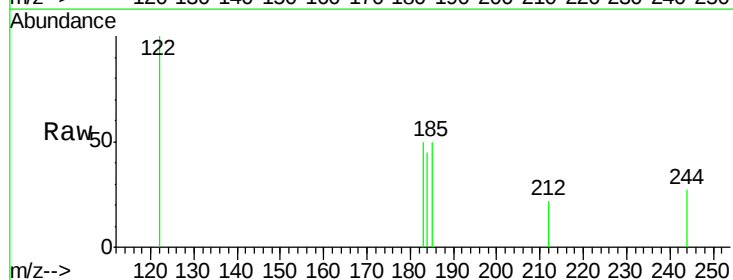


Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E



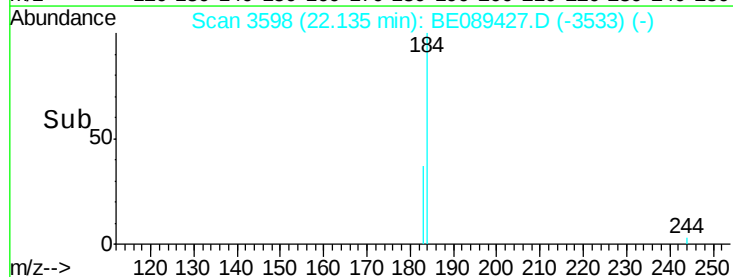
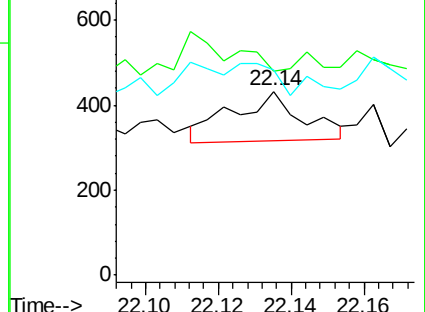


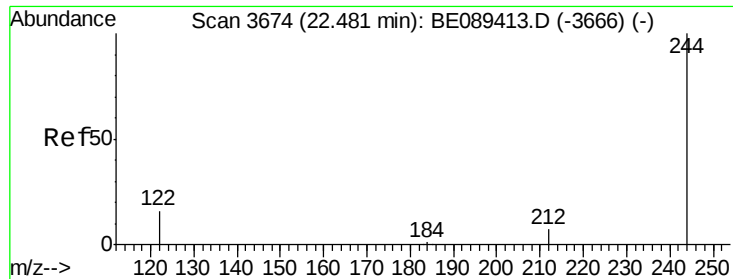

#22  
 Terphenyl-d14  
 Concen: 9.77 ng  
 RT: 22.48 min Scan# 3674  
 Delta R.T. -0.00 min  
 Lab File: BE089427.D  
 Acq: 30 Jan 2015 00:58




Instrument :  
 BNA\_E  
 ClientSampleId :  
 MPE-9


Tgt Ion: 244 Resp: 629463  
 Ion Ratio Lower Upper  
 244 100  
 212 6.9 5.4 8.0  
 122 17.9 13.2 19.8

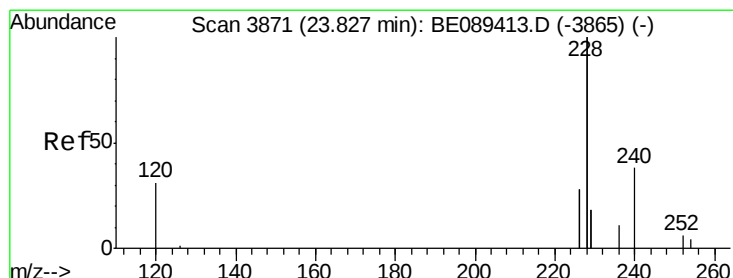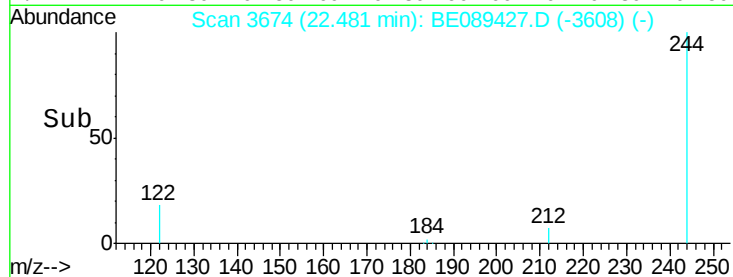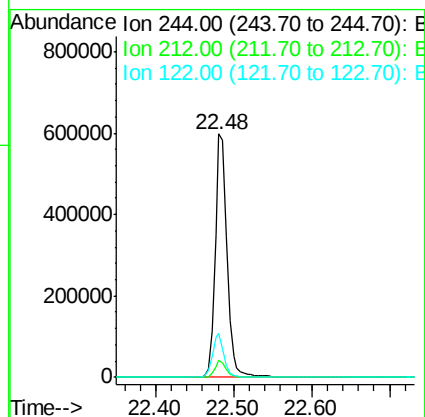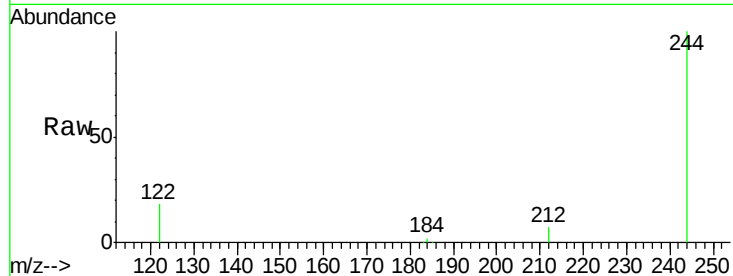

#23  
 Benzo(a)anthracene  
 Concen: 0.02 ng  
 RT: 23.84 min Scan# 3872  
 Delta R.T. 0.01 min  
 Lab File: BE089427.D  
 Acq: 30 Jan 2015 00:58

Tgt Ion: 228 Resp: 9174  
 Ion Ratio Lower Upper  
 228 100  
 226 30.6 22.6 33.8  
 229 42.7 14.5 21.7#


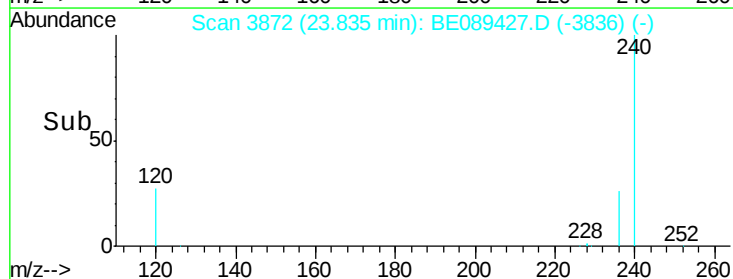
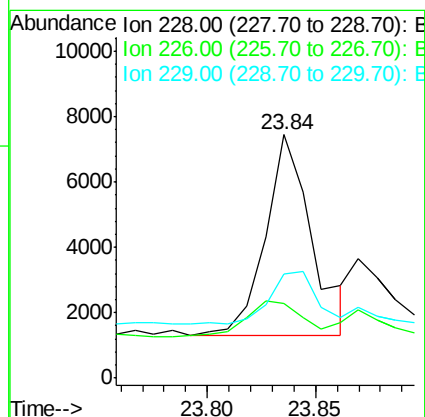
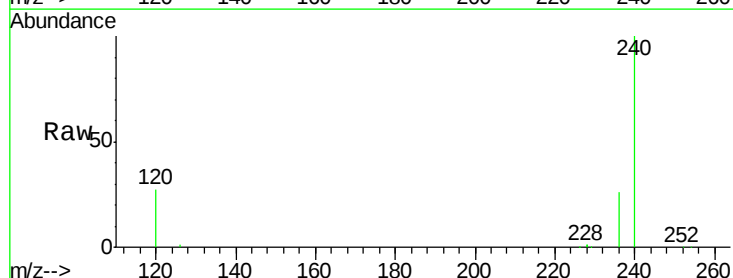


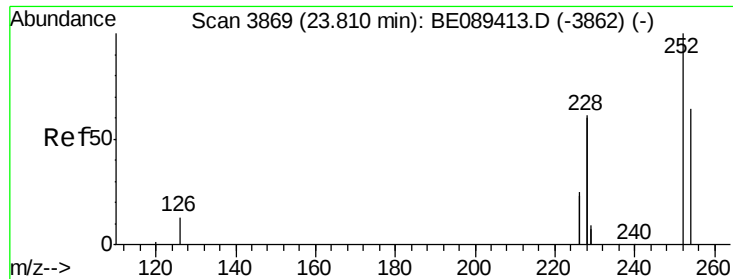

#24  
 3,3'-Dichlorobenzidine  
 Concen: 0.01 ng  
 RT: 23.79 min Scan# 3867  
 Delta R.T. -0.02 min  
 Lab File: BE089427.D  
 Acq: 30 Jan 2015 00:58




Instrument :  
 BNA\_E  
 ClientSampleId :  
 MPE-9


Tgt Ion: 252 Resp: 173  
 Ion Ratio Lower Upper  
 252 100  
 254 81.0 51.1 76.7#  
 126 199.4 11.5 17.3#

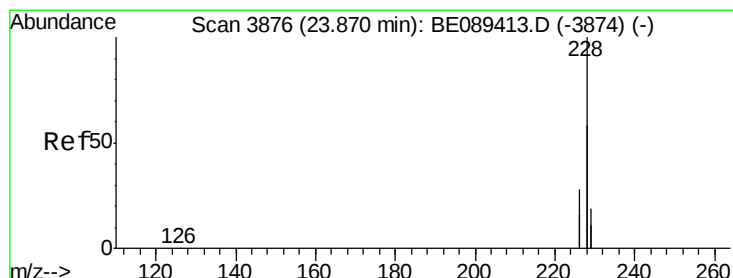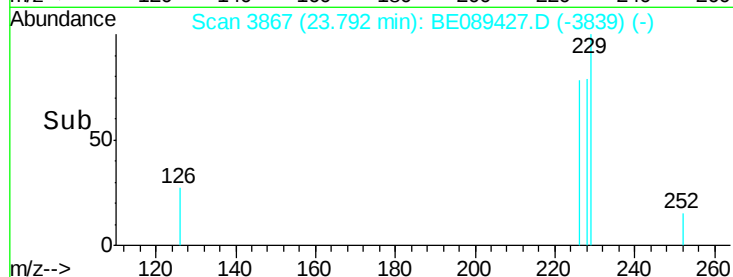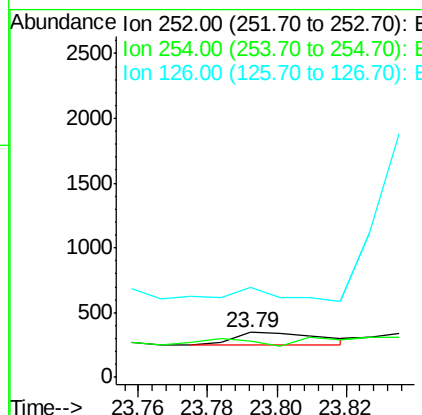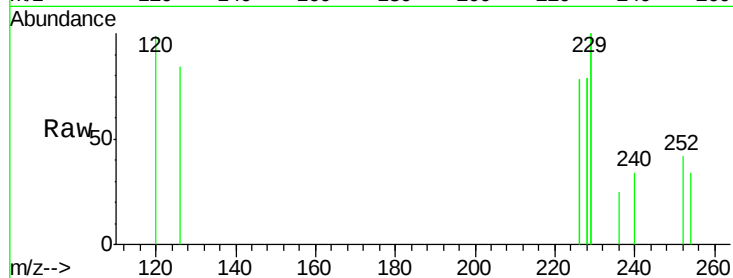

#25  
 Chrysene  
 Concen: 0.02 ng  
 RT: 23.84 min Scan# 3872  
 Delta R.T. -0.03 min  
 Lab File: BE089427.D  
 Acq: 30 Jan 2015 00:58

Tgt Ion: 228 Resp: 9174  
 Ion Ratio Lower Upper  
 228 100  
 226 30.6 22.6 33.8  
 229 42.7 15.5 23.3#

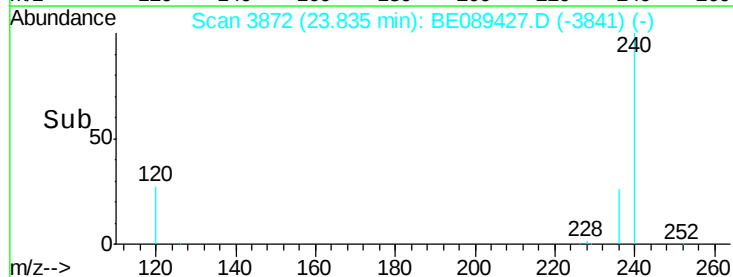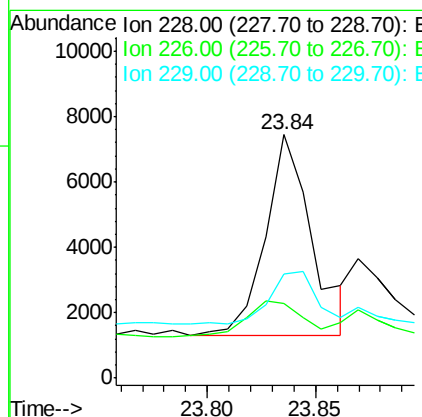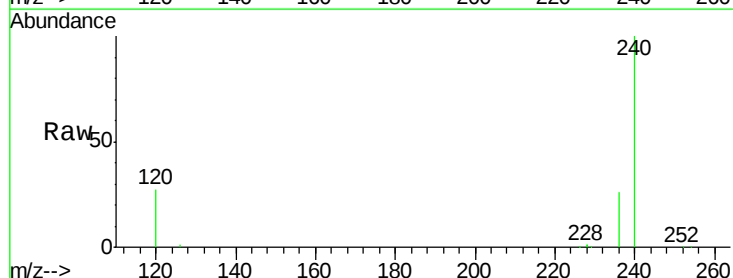



#26

Indeno(1,2,3-cd)pyrene

Concen: 0.01 ng

RT: 27.06 min Scan# 4229

Delta R.T. 0.00 min

Lab File: BE089427.D

Acq: 30 Jan 2015 00:58

Instrument :

BNA\_E

ClientSampleId :

MPE-9


Tgt Ion: 276 Resp: 671

Ion Ratio Lower Upper

276 100

138 34.1 0.0 0.0#




277 42.2 0.0 0.0#

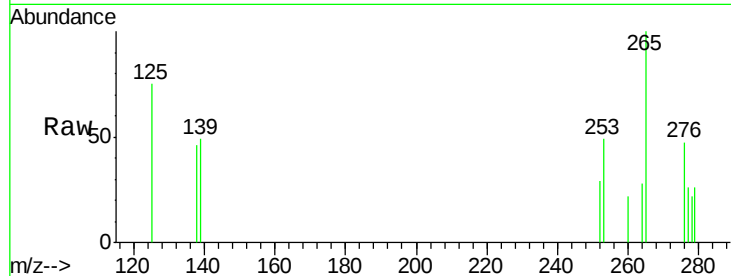

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

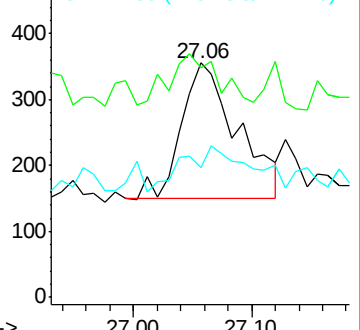

#27

Perylene-d12

Concen: 5.00 ng

RT: 25.55 min Scan# 4062

Delta R.T. -0.00 min

Lab File: BE089427.D

Acq: 30 Jan 2015 00:58


Tgt Ion: 264 Resp: 595665

Ion Ratio Lower Upper

264 100

260 24.1 19.4 29.0



265 21.2 17.1 25.7




Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E




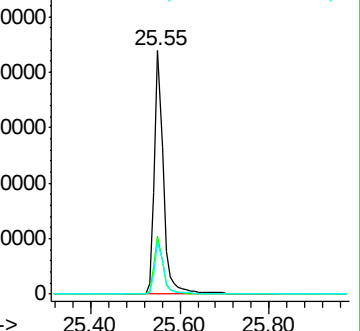




#28  
Benzo(b)fluoranthene  
Concen: 0.01 ng  
RT: 25.10 min Scan# 4012  
Delta R.T. 0.00 min  
Lab File: BE089427.D  
Acq: 30 Jan 2015 00:58




Instrument :  
BNA\_E  
ClientSampleId :  
MPE-9


Tgt Ion: 252 Resp: 419  
Ion Ratio Lower Upper  
252 100  
253 86.2 17.6 26.4#  
125 169.2 10.5 15.7#

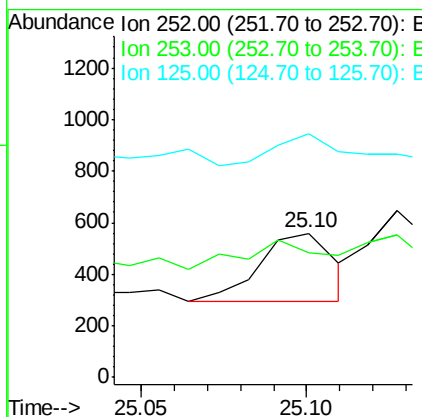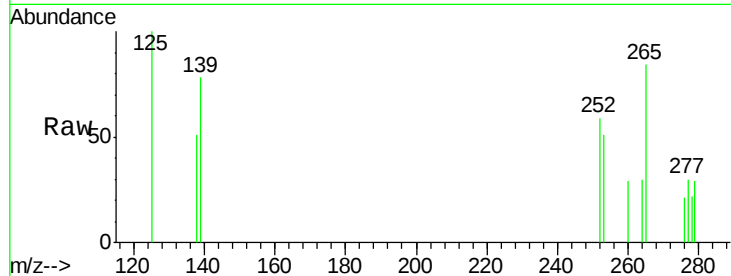

#29  
Benzo(k)fluoranthene  
Concen: 0.00 ng  
RT: 25.13 min Scan# 4015  
Delta R.T. 0.00 min  
Lab File: BE089427.D  
Acq: 30 Jan 2015 00:58

Tgt Ion: 252 Resp: 717  
Ion Ratio Lower Upper  
252 100  
253 85.2 17.4 26.2#  
125 134.0 11.0 16.6#

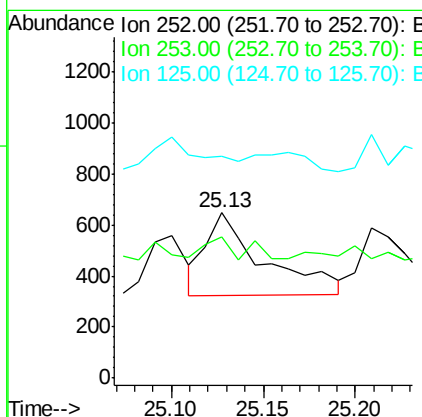



#30

Benzo(a)pyrene

Concen: 0.01 ng

RT: 25.48 min Scan# 4054

Delta R.T. 0.00 min

Lab File: BE089427.D

Acq: 30 Jan 2015 00:58

Instrument :

BNA\_E

ClientSampleId :

MPE-9


Tgt Ion: 252 Resp: 493

Ion Ratio Lower Upper

252 100

253 86.1 17.3 25.9#

125 138.8 13.0 19.6#




Abundance Ion 252.00 (251.70 to 252.70): E


Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

Time-->



Time-->



#31

Dibenzo(a,h)anthracene

Concen: 0.00 ng

RT: 27.10 min Scan# 4234

Delta R.T. 0.02 min

Lab File: BE089427.D

Acq: 30 Jan 2015 00:58


Tgt Ion: 278 Resp: 322

Ion Ratio Lower Upper

278 100

139 135.4 17.2 25.8#

279 70.9 19.2 28.8#




Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

Time-->



Time-->