


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE012915\
 Data File : BE089408.D
 Acq On : 29 Jan 2015 9:58
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-BE012915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 30 17:07:09 2015

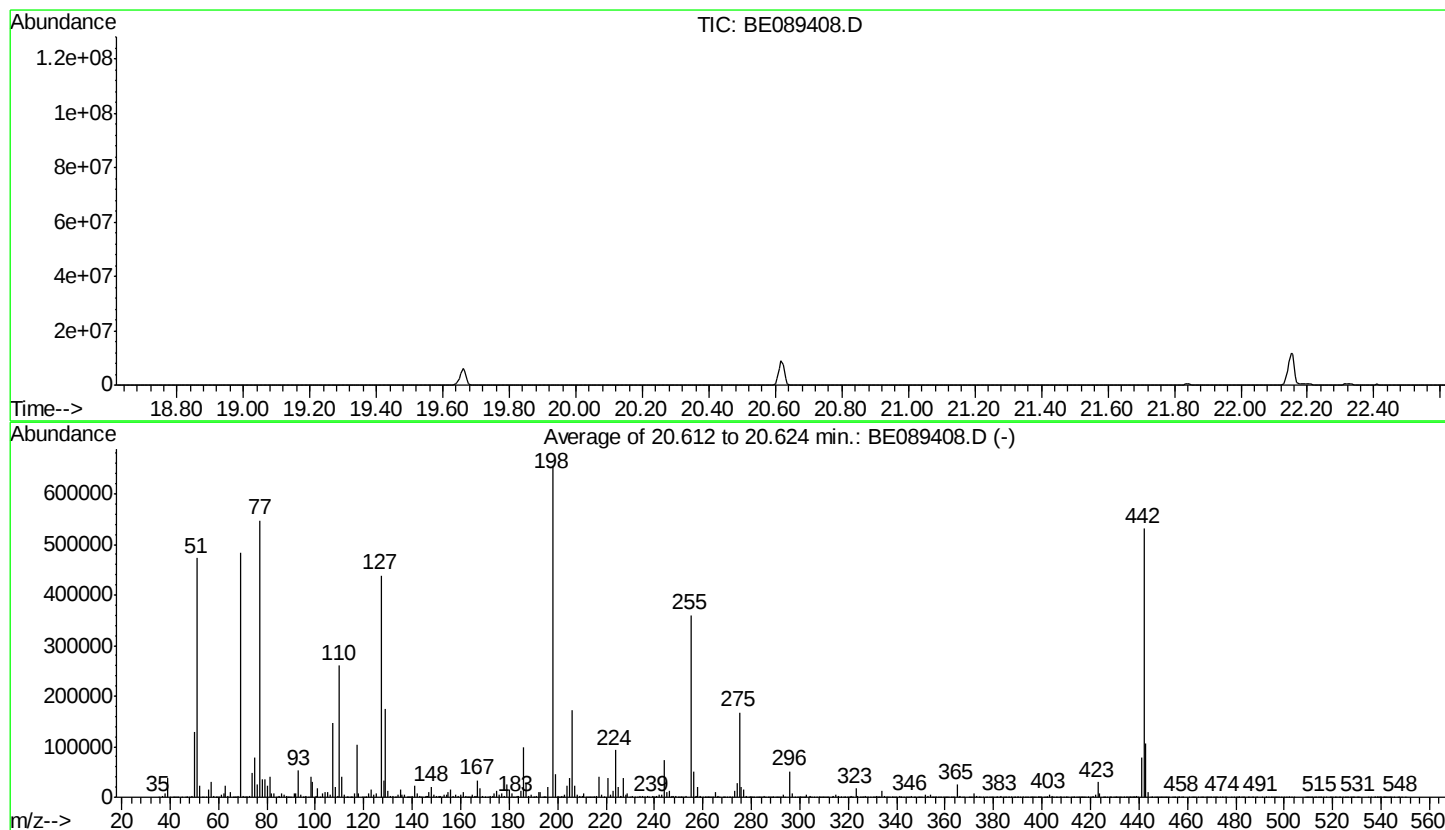

AutoFind: Scans 3272, 3273, 3274; Background Corrected with Scan 3261

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	72.1	472950	PASS
68	69	0.00	2	0.4	1712	PASS
69	198	0.00	100	73.6	482581	PASS
70	69	0.00	2	0.5	2636	PASS
127	198	10	80	66.9	439084	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	655978	PASS
199	198	5	9	7.0	45966	PASS
275	198	10	60	25.7	168298	PASS
365	198	1	100	3.7	24572	PASS
441	442	0.01	24	14.7	78146	PASS
442	198	50	100	81.1	531689	PASS
443	442	15	24	20.2	107315	PASS