


Data Path : Z:\HPCHEM1\BNA\_E\Data\BE012915\  
 Data File : BE089424.D  
 Acq On : 29 Jan 2015 21:41  
 Operator : TP/IZ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_E\METHODS\SIM-BE012915.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Jan 30 17:07:09 2015

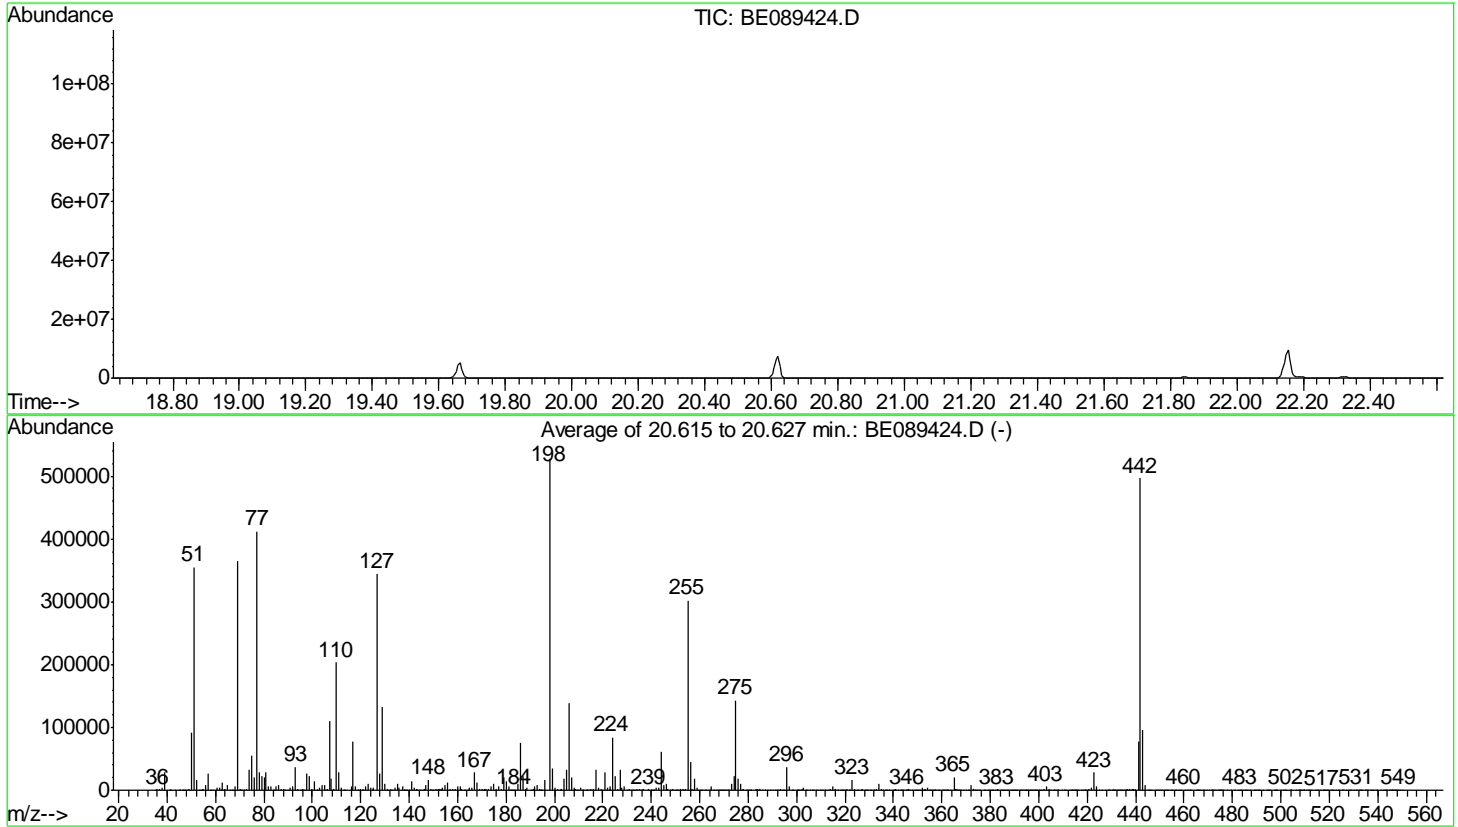

AutoFind: Scans 3272, 3273, 3274; Background Corrected with Scan 3265

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	67.3	355138	PASS
68	69	0.00	2	1.5	5440	PASS
69	198	0.00	100	69.3	365711	PASS
70	69	0.00	2	0.6	2342	PASS
127	198	10	80	65.4	344989	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	527808	PASS
199	198	5	9	6.4	33968	PASS
275	198	10	60	27.2	143485	PASS
365	198	1	100	4.1	21458	PASS
441	442	0.01	24	15.5	77037	PASS
442	198	50	100	94.1	496661	PASS
443	442	15	24	19.4	96581	PASS