

Data Path : Z:\HPCHEM1\BNA E\DATA\BE012918\
 Data File : BE095245.D
 Acq On : 29 Jan 2018 14:09
 Operator : SJ/JU
 Sample : J1233-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6B07

Quant Time: Jan 30 04:44:24 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 30 04:43:36 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2301	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	7339	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	5095	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.71
16) Chrysene-d12	21.80	240	10233	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	697561	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	4707	0.39	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	13405	0.00	ng/ul	0.00
Target Compounds						
3) Naphthalene	11.31	128	1241	0.060	ng/ul#	81
5) 2-Methylnaphthalene	12.89	142	6923	0.504	ng/ul	100
8) Acenaphthene	15.08	153	7692	0.404	ng/ul	93
9) Fluorene	16.03	166	4731	0.241	ng/ul#	77
17) Pyrene	20.05	202	2695	0.078	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE012918\
Data File : BE095245.D
Acq On : 29 Jan 2018 14:09
Operator : SJ/JU
Sample : J1233-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6B07

Quant Time: Jan 30 04:44:24 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 30 04:43:36 2018
Response via : Initial Calibration

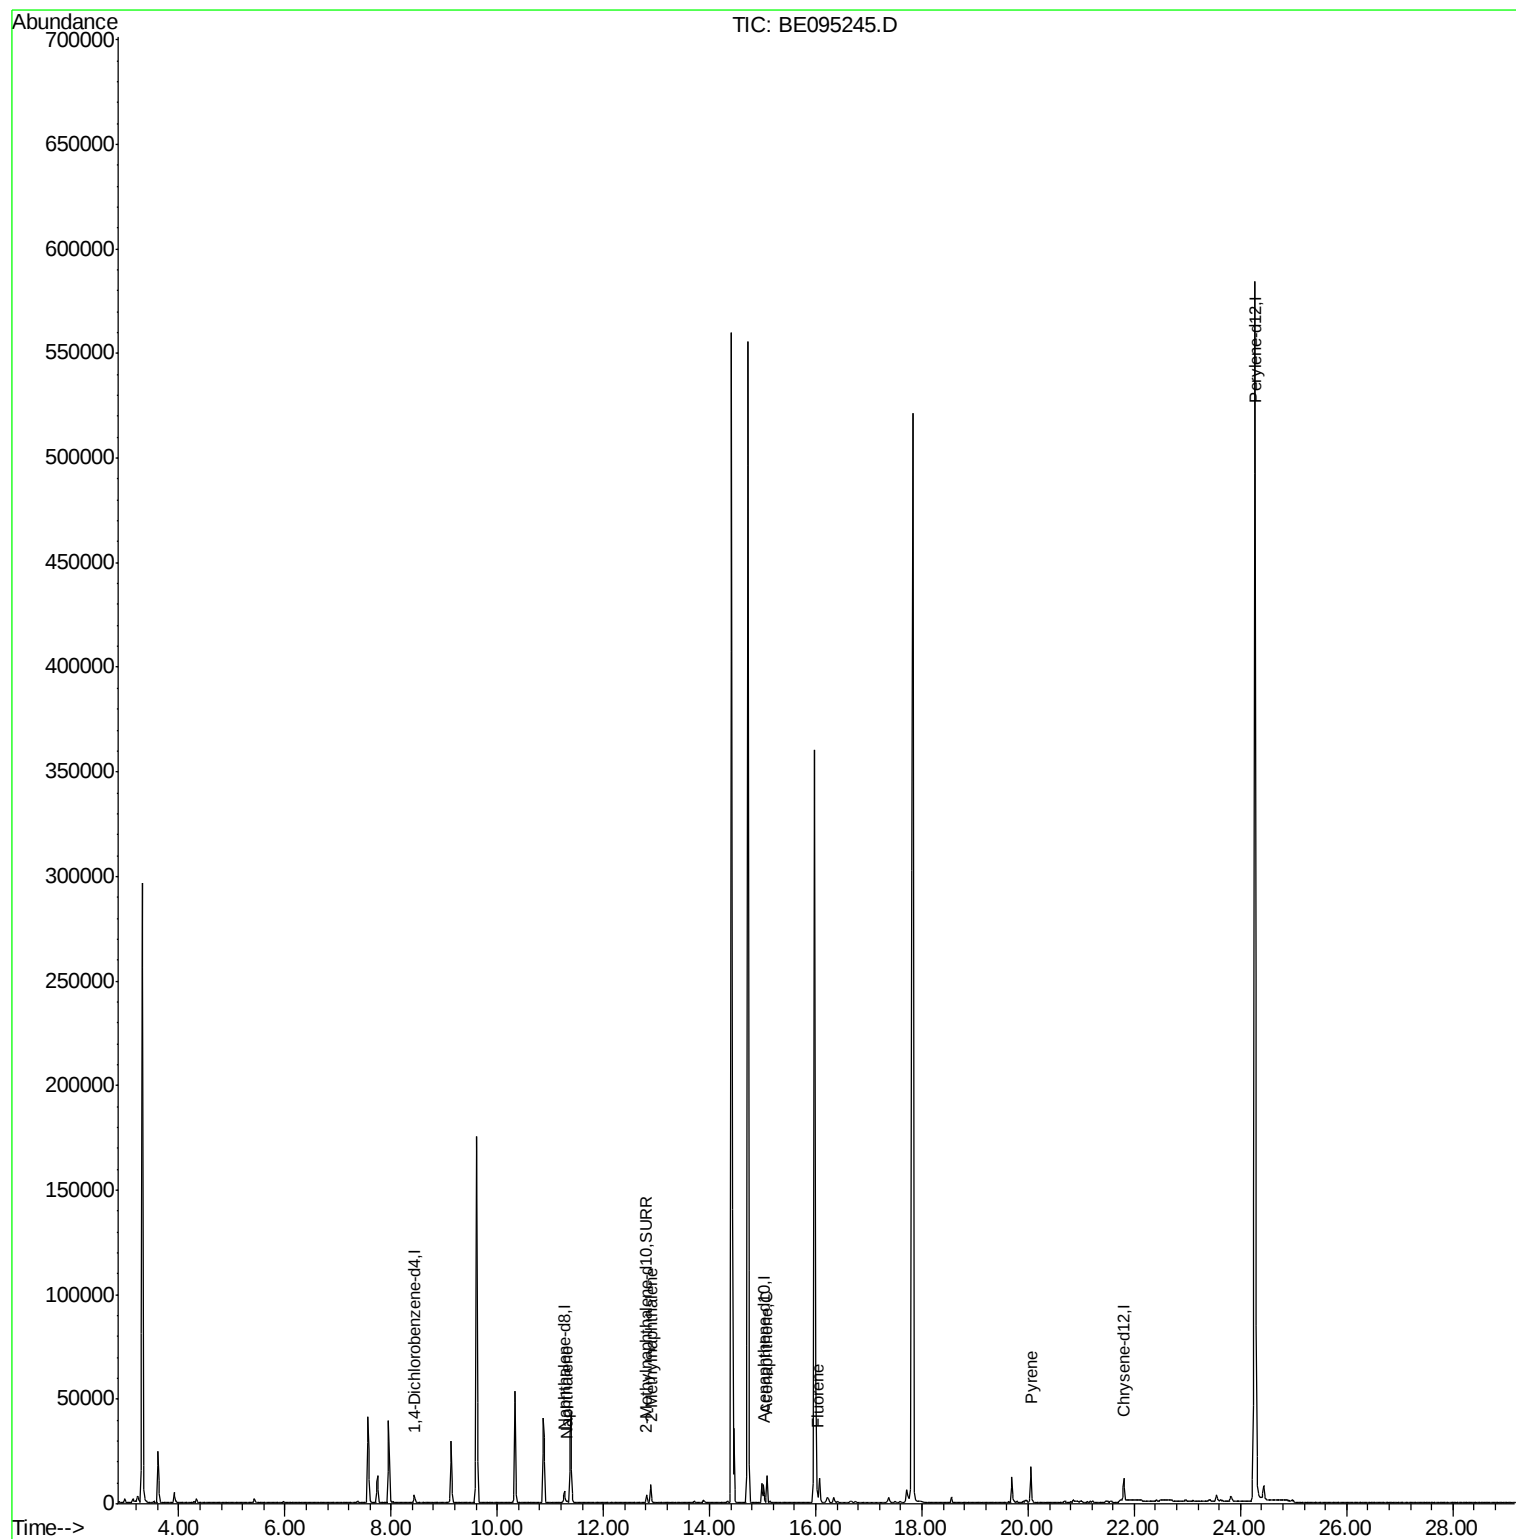

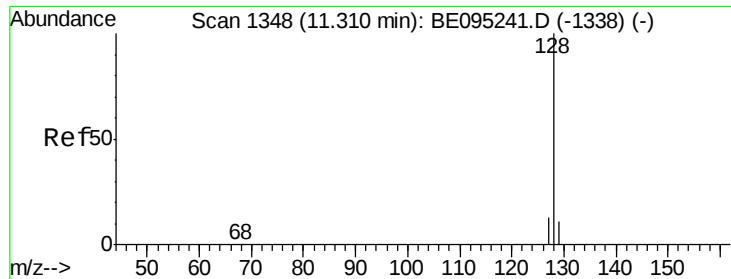

#3

Naphthalene

Concen: 0.060 ng/ul

RT: 11.31 min Scan# 1349

Delta R.T. 0.00 min

Lab File: BE095245.D

Acq: 29 Jan 2018 14:09

Instrument :

BNA_E

ClientSampleId :

F6B07


Tot Ion:128 Resp: 1241

Ion Ratio Lower Upper

128 100

129 18.6 11.3 16.9#




127 18.6 4.0 6.0#

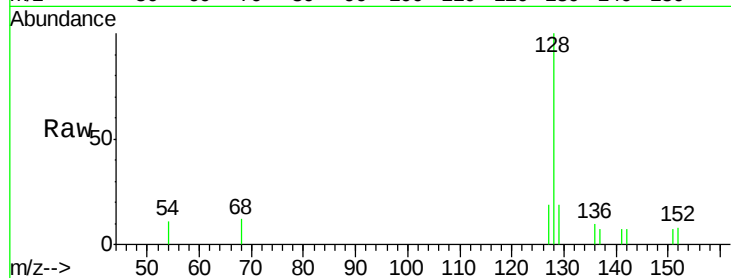

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

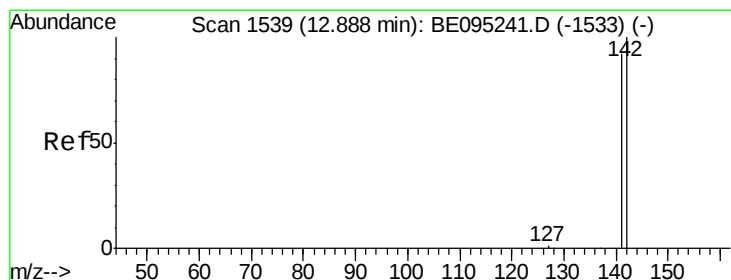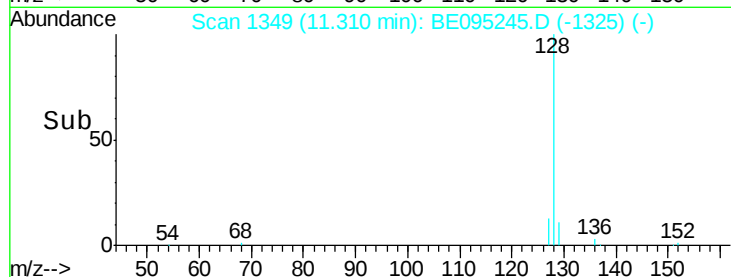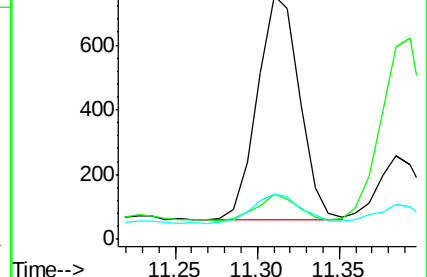

#5

2-Methylnaphthalene

Concen: 0.504 ng/ul

RT: 12.89 min Scan# 1540

Delta R.T. 0.00 min

Lab File: BE095245.D


Acq: 29 Jan 2018 14:09

Tgt Ion:142 Resp: 6923

Ion Ratio Lower Upper



142 100


141 90.6 72.6 108.8

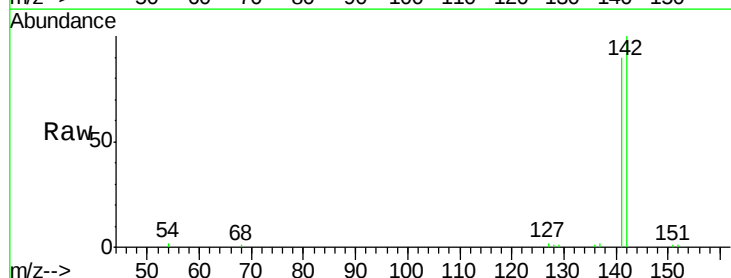

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

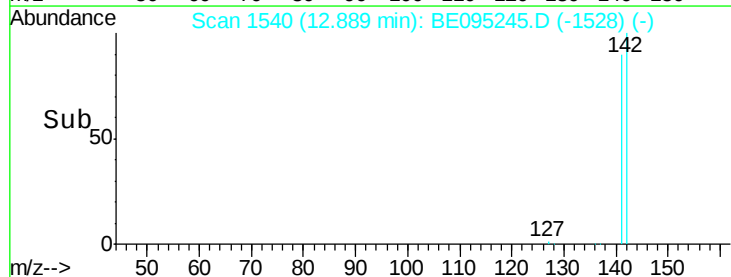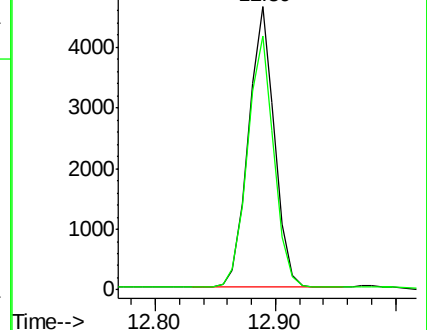

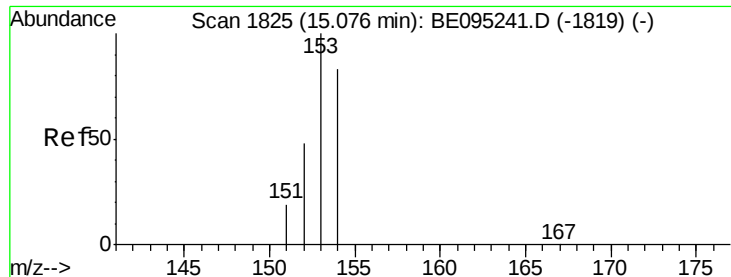

#8

Acenaphthene

Concen: 0.404 ng/ul

RT: 15.08 min Scan# 1826

Delta R.T. -0.00 min

Lab File: BE095245.D

Acq: 29 Jan 2018 14:09

Instrument :

BNA_E

ClientSampleId :

F6B07


Tot Ion:153 Resp: 7692

Ion Ratio Lower Upper

153 100

152 51.7 36.0 54.0




154 84.4 72.0 108.0

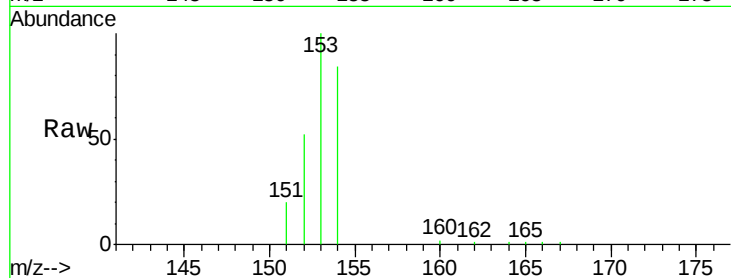

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

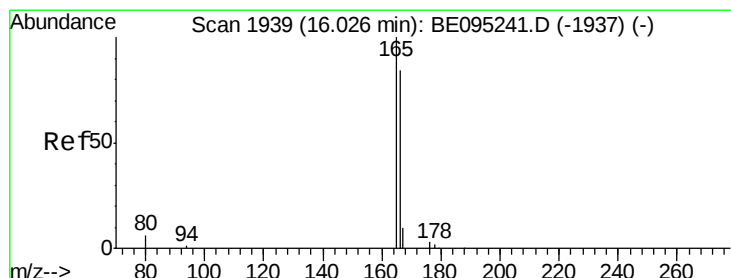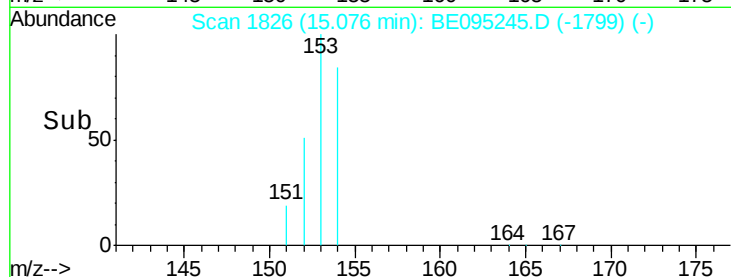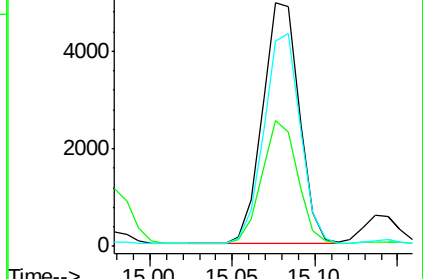

#9

Fluorene

Concen: 0.241 ng/ul

RT: 16.03 min Scan# 1940

Delta R.T. 0.00 min

Lab File: BE095245.D

Acq: 29 Jan 2018 14:09


Tgt Ion:166 Resp: 4731

Ion Ratio Lower Upper

166 100

165 116.8 73.4 110.2#



167 14.2 14.6 22.0#

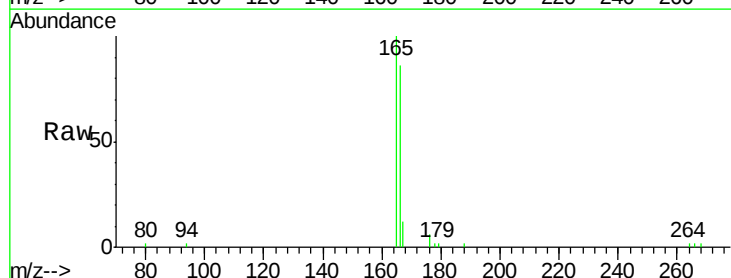


Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

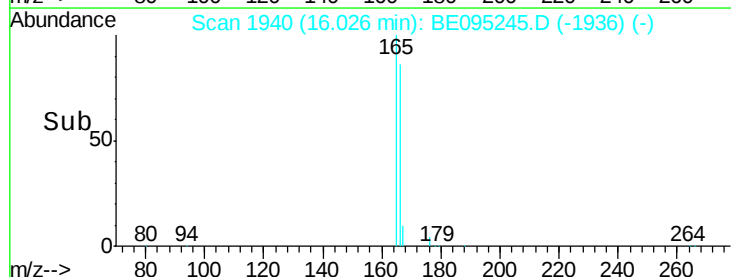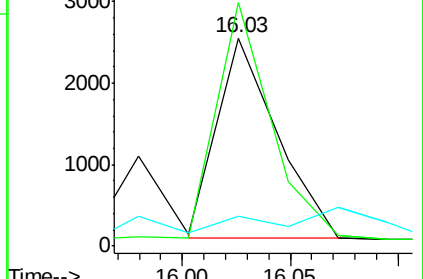

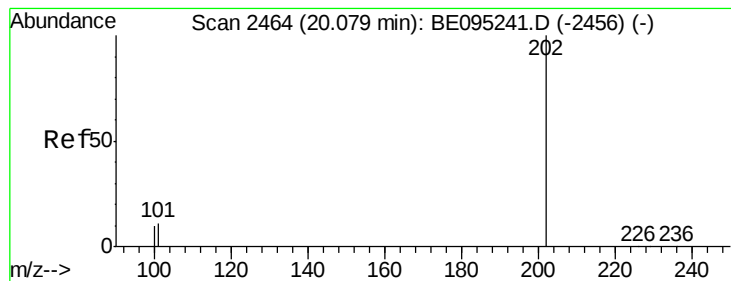

#17

Pvrene

Concen: 0.078 ng/ul

RT: 20.05 min Scan# 2461

Delta R.T. -0.03 min

Lab File: BE095245.D

Acq: 29 Jan 2018 14:09

Instrument :

BNA_E

ClientSampleId :

F6B07


Tot Ion: 202 Resp: 2695

Ion Ratio Lower Upper

202 100

101 167.0 18.2 27.4#

100 1157.9 15.6 23.4#

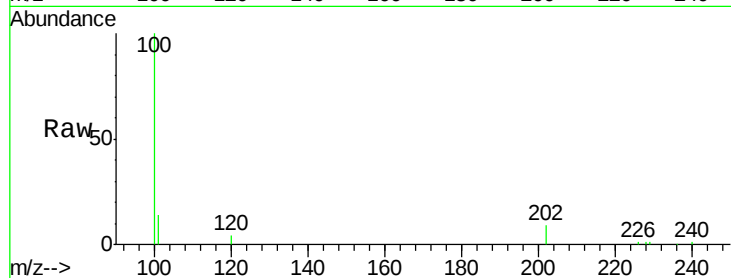

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BE

