

Data Path : Z:\HPCHEM1\BNA E\DATA\BE012918\
 Data File : BE095246.D
 Acq On : 29 Jan 2018 14:45
 Operator : SJ/JU
 Sample : J1233-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6B10

Quant Time: Jan 30 04:44:33 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 30 04:43:36 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2510	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	7797	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	5209	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.71
16) Chrysene-d12	21.80	240	10688	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	610939	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	4323	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	11860	0.00	ng/ul	0.00
Target Compounds						
3) Naphthalene	11.31	128	10179	0.466	ng/ul#	88
5) 2-Methylnaphthalene	12.89	142	6988	0.479	ng/ul	100
7) Acenaphthylene	14.74	152	619	0.025	ng/ul#	55
8) Acenaphthene	15.08	153	11376	0.585	ng/ul	98
9) Fluorene	16.02	166	8892	0.443	ng/ul#	73
17) Pyrene	20.08	202	32554	0.908	ng/ul#	80
18) Benzo(a)anthracene	21.79	228	6254	0.187	ng/ul#	87
19) Chrysene	21.84	228	4950	0.143	ng/ul	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE012918\
Data File : BE095246.D
Acq On : 29 Jan 2018 14:45
Operator : SJ/JU
Sample : J1233-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6B10

Quant Time: Jan 30 04:44:33 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 30 04:43:36 2018
Response via : Initial Calibration

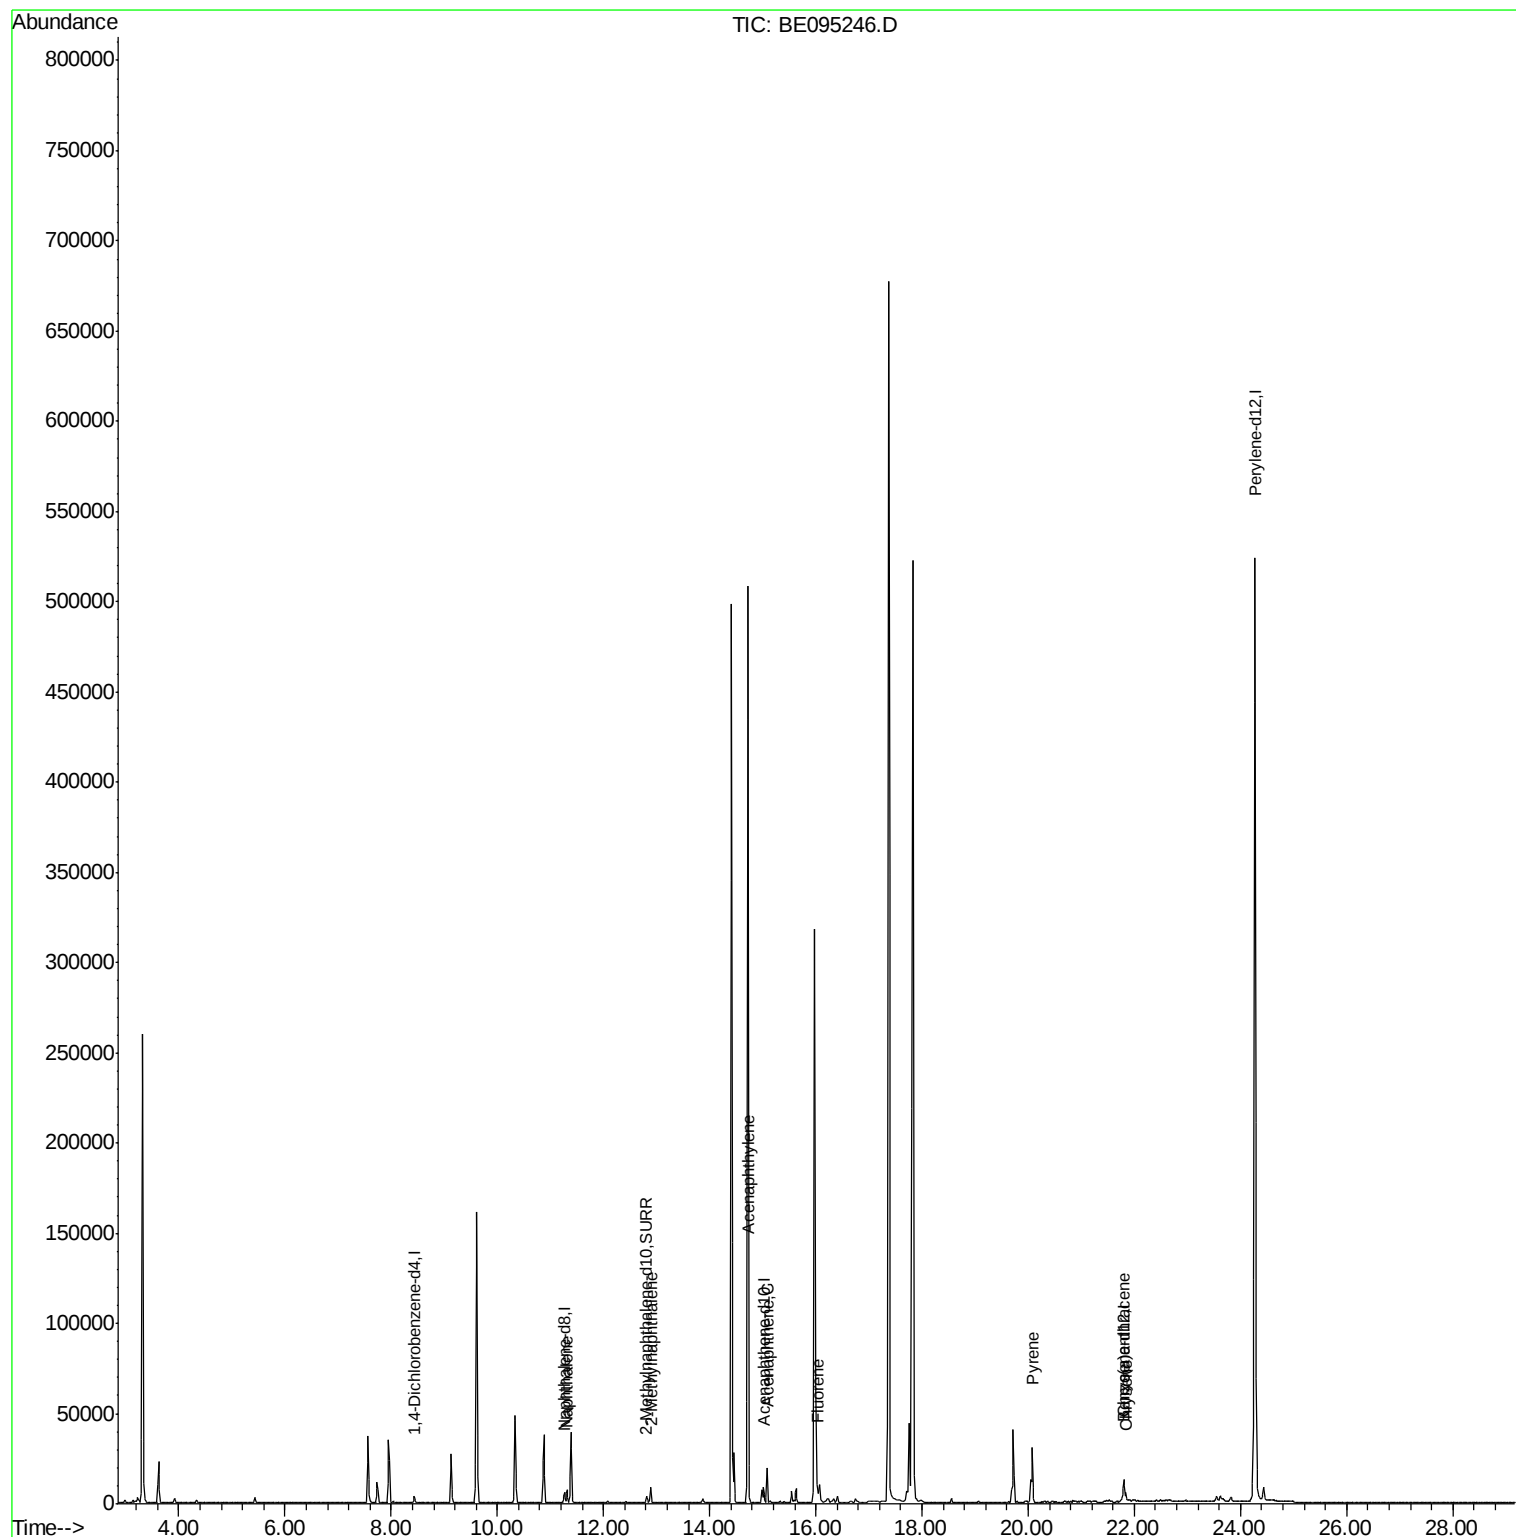

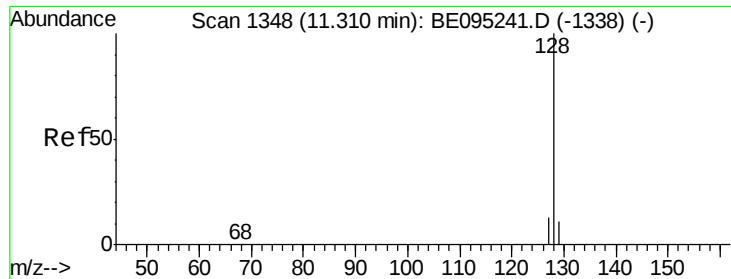

#3

Naphthalene

Concen: 0.466 ng/ul

RT: 11.31 min Scan# 1348

Delta R.T. 0.00 min

Lab File: BE095246.D

Acq: 29 Jan 2018 14:45

Instrument :

BNA_E

ClientSampleId :

F6B10


Tot Ion:128 Resp: 10179

Ion Ratio Lower Upper

128 100

129 11.9 11.3 16.9




127 14.7 4.0 6.0#

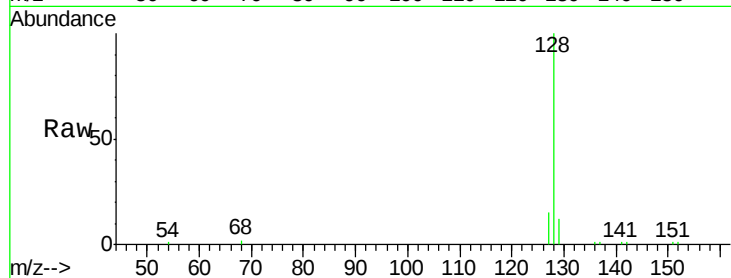

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

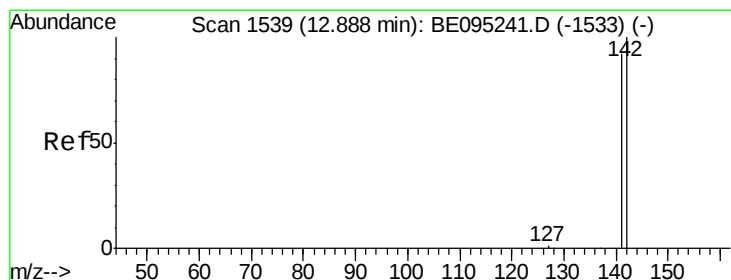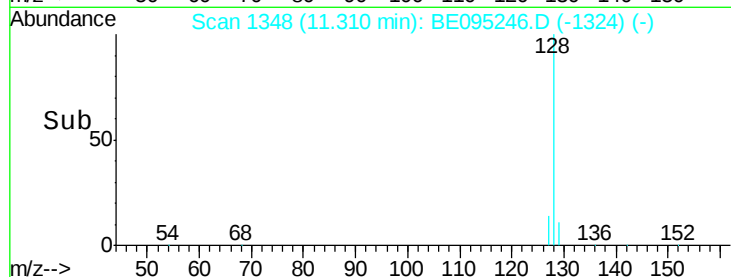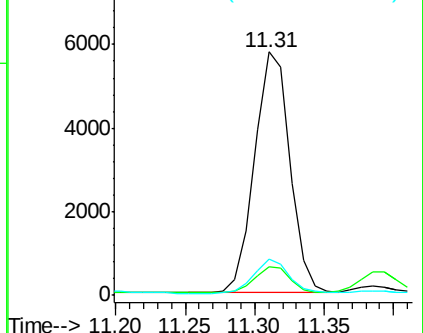

#5

2-Methylnaphthalene

Concen: 0.479 ng/ul

RT: 12.89 min Scan# 1539

Delta R.T. 0.00 min

Lab File: BE095246.D


Acq: 29 Jan 2018 14:45

Tgt Ion:142 Resp: 6988

Ion Ratio Lower Upper



142 100


141 91.1 72.6 108.8

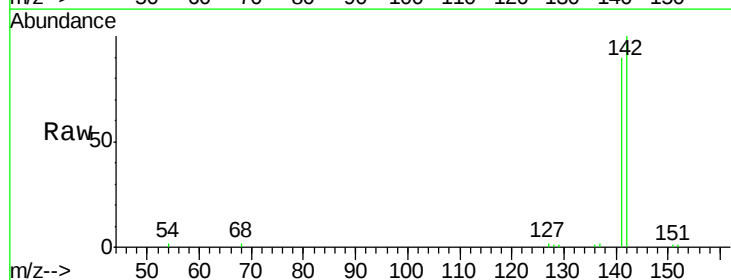

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

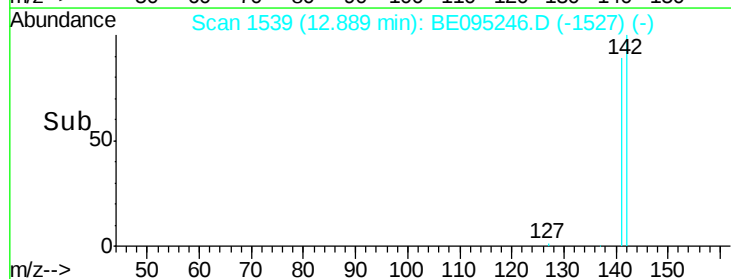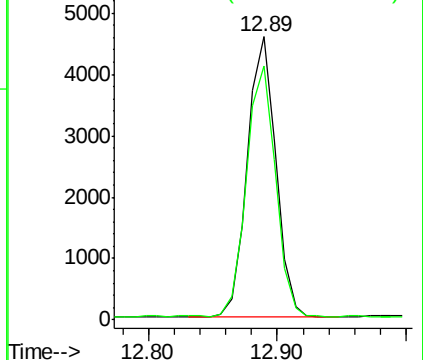

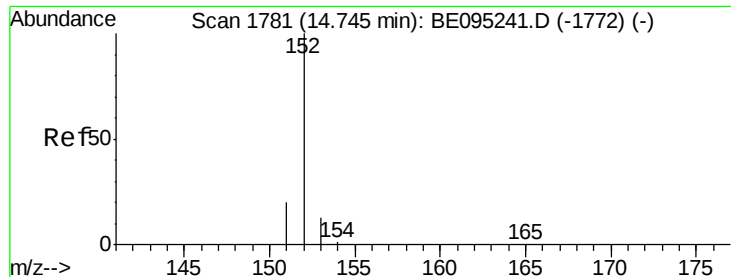

#7

Acenaphthylene

Concen: 0.025 ng/ul

RT: 14.74 min Scan# 1781

Delta R.T. -0.00 min

Lab File: BE095246.D

Acq: 29 Jan 2018 14:45

Instrument :

BNA_E

ClientSampleId :

F6B10


Tot Ion:152 Resp: 619

Ion Ratio Lower Upper

152 100

151 37.3 17.1 25.7#




153 41.1 12.8 19.2#

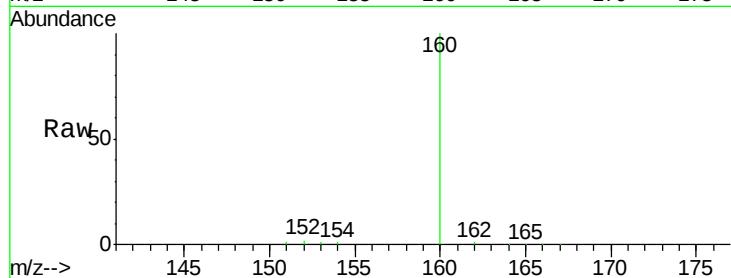

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

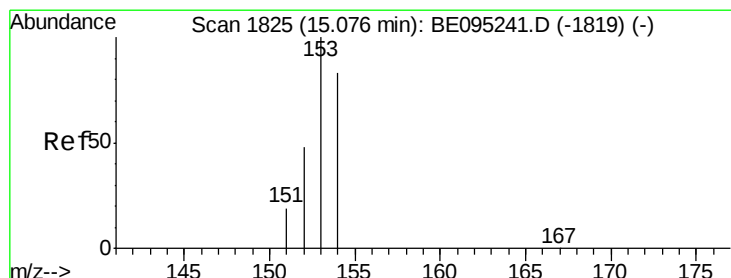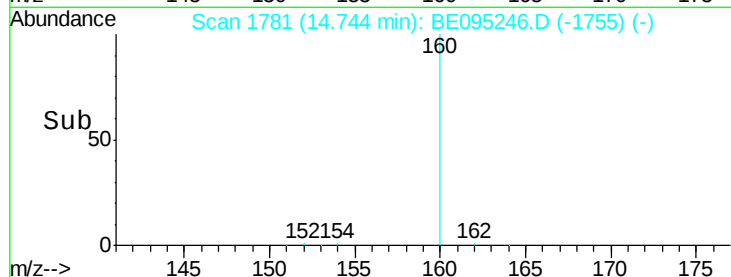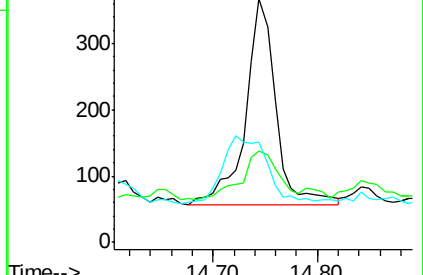

#8

Acenaphthene

Concen: 0.585 ng/ul

RT: 15.08 min Scan# 1826

Delta R.T. 0.01 min

Lab File: BE095246.D

Acq: 29 Jan 2018 14:45


Tgt Ion:153 Resp: 11376

Ion Ratio Lower Upper

153 100

152 47.9 36.0 54.0



154 89.3 72.0 108.0

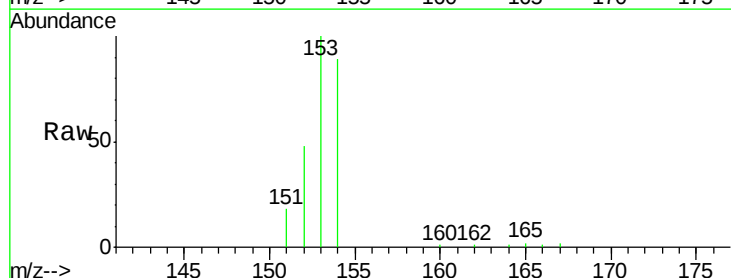


Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

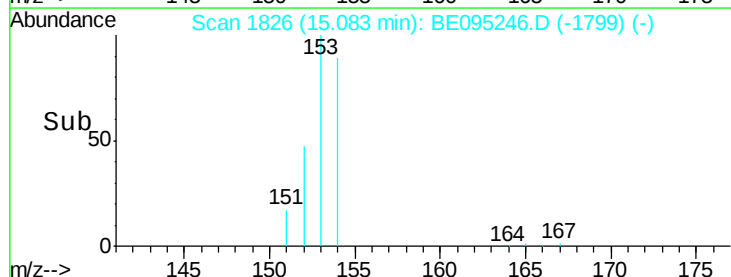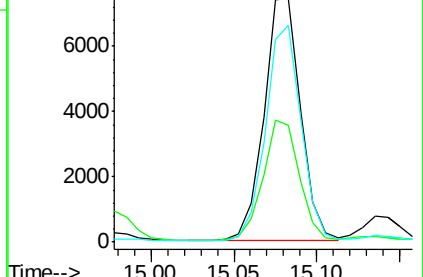

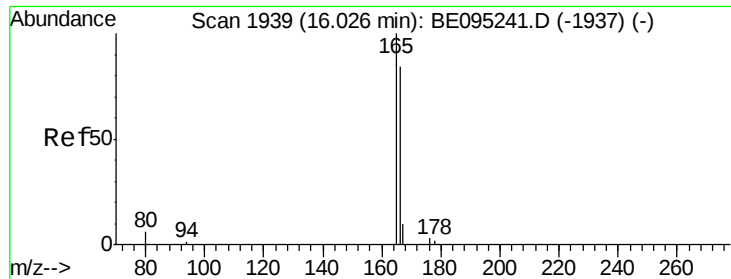

#9

Fluorene

Concen: 0.443 ng/ul

RT: 16.02 min Scan# 1939

Delta R.T. -0.00 min

Lab File: BE095246.D

Acq: 29 Jan 2018 14:45

Instrument :

BNA_E

ClientSampleId :

F6B10





Tot Ion:166 Resp: 8892

Ion Ratio Lower Upper

166 100

165 120.7 73.4 110.2#

167 13.8 14.6 22.0#

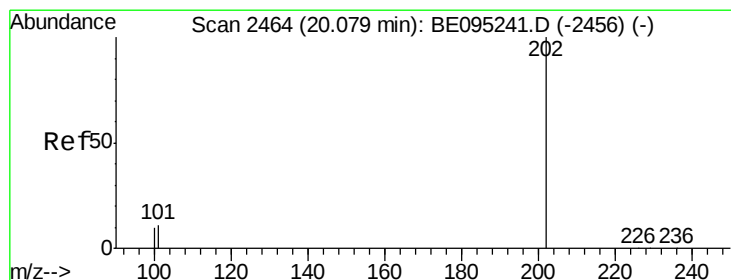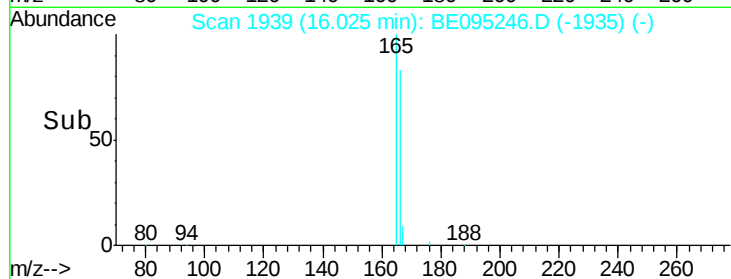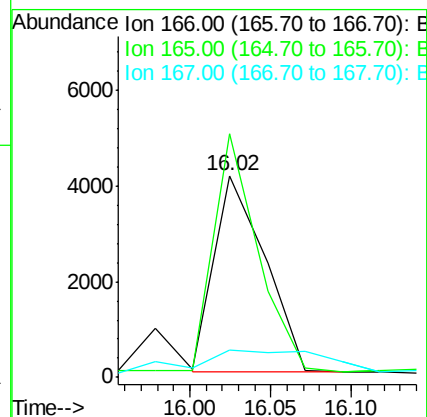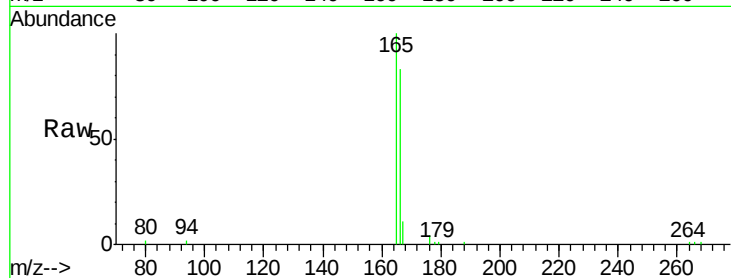

#17

Pyrene

Concen: 0.908 ng/ul

RT: 20.08 min Scan# 2464

Delta R.T. 0.00 min

Lab File: BE095246.D

Acq: 29 Jan 2018 14:45




Tgt Ion:202 Resp: 32554


Ion Ratio Lower Upper

202 100

101 12.2 18.2 27.4#

100 11.2 15.6 23.4#

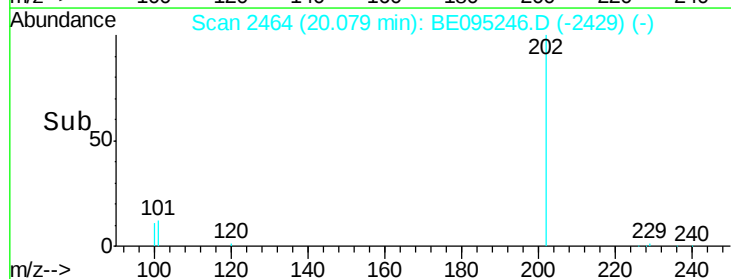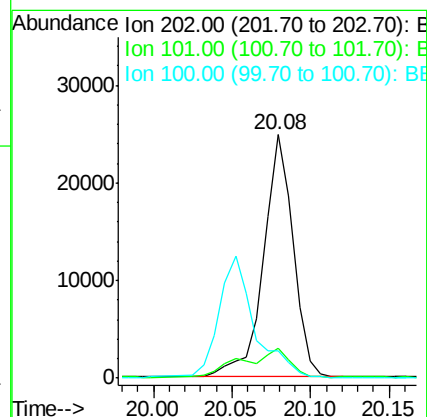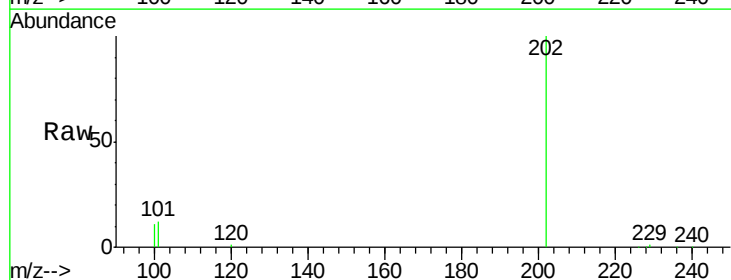

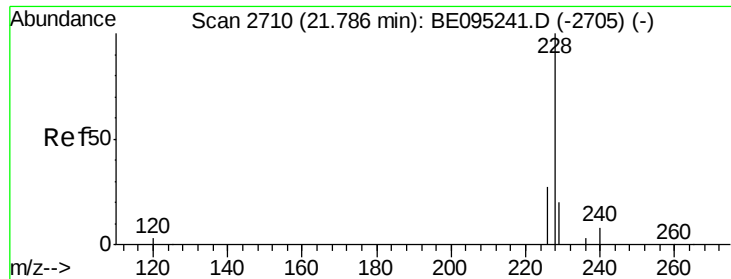

#18

Benzo(a)anthracene

Concen: 0.187 ng/ul

RT: 21.79 min Scan# 2710

Delta R.T. 0.00 min

Lab File: BE095246.D

Acq: 29 Jan 2018 14:45

Instrument :

BNA_E

ClientSampleId :

F6B10


Tot Ion:228 Resp: 6254

Ion Ratio Lower Upper




228 100

229 23.7 22.8 34.2

226 29.4 17.0 25.6#

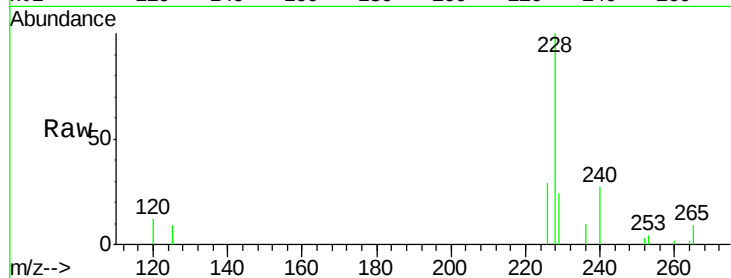

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 229.00 (228.70 to 229.70): E
Ion 226.00 (225.70 to 226.70): E

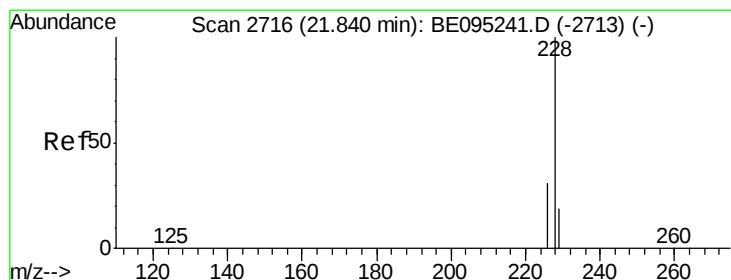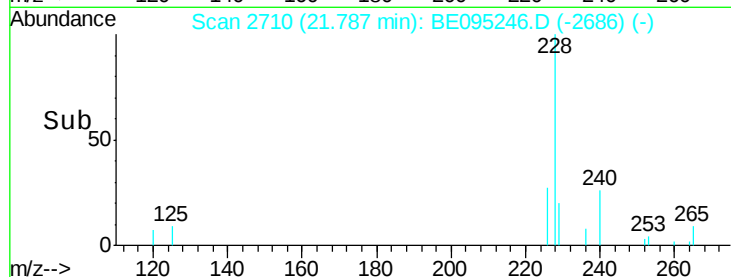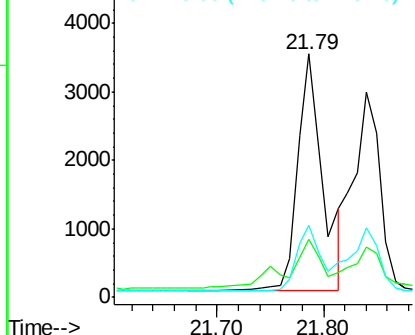

#19

Chrysene

Concen: 0.143 ng/ul

RT: 21.84 min Scan# 2716

Delta R.T. 0.00 min

Lab File: BE095246.D

Acq: 29 Jan 2018 14:45


Tgt Ion:228 Resp: 4950

Ion Ratio Lower Upper

228 100

226 34.0 23.4 35.0

229 24.6 17.7 26.5

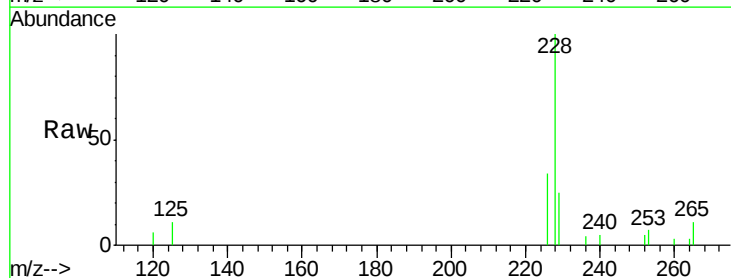

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

