

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE012918\
 Data File : BE095265.D
 Acq On : 30 Jan 2018 2:08
 Operator : SJ/JU
 Sample : J1244-05
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6B46

Manual Integrations
 APPROVED

Sohil
 1/30/2018 3:32:54 PM

Quant Time: Jan 30 06:54:58 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 30 06:14:31 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2187	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	6627	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	4139	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8616	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	9513	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	10100	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2494	0.23	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	6810	0.21	ng/ul	0.00
Target Compounds						
7) Acenaphthylene	14.74	152	406	0.020	ng/ul#	69
17) Pyrene	20.08	202	687m	0.022	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE012918\
Data File : BE095265.D
Acq On : 30 Jan 2018 2:08
Operator : SJ/JU
Sample : J1244-05
Misc :
ALS Vial : 25 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
F6B46

Manual Integrations
APPROVED

Sohil
1/30/2018 3:32:54 PM

Quant Time: Jan 30 06:54:58 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 30 06:14:31 2018
Response via : Initial Calibration

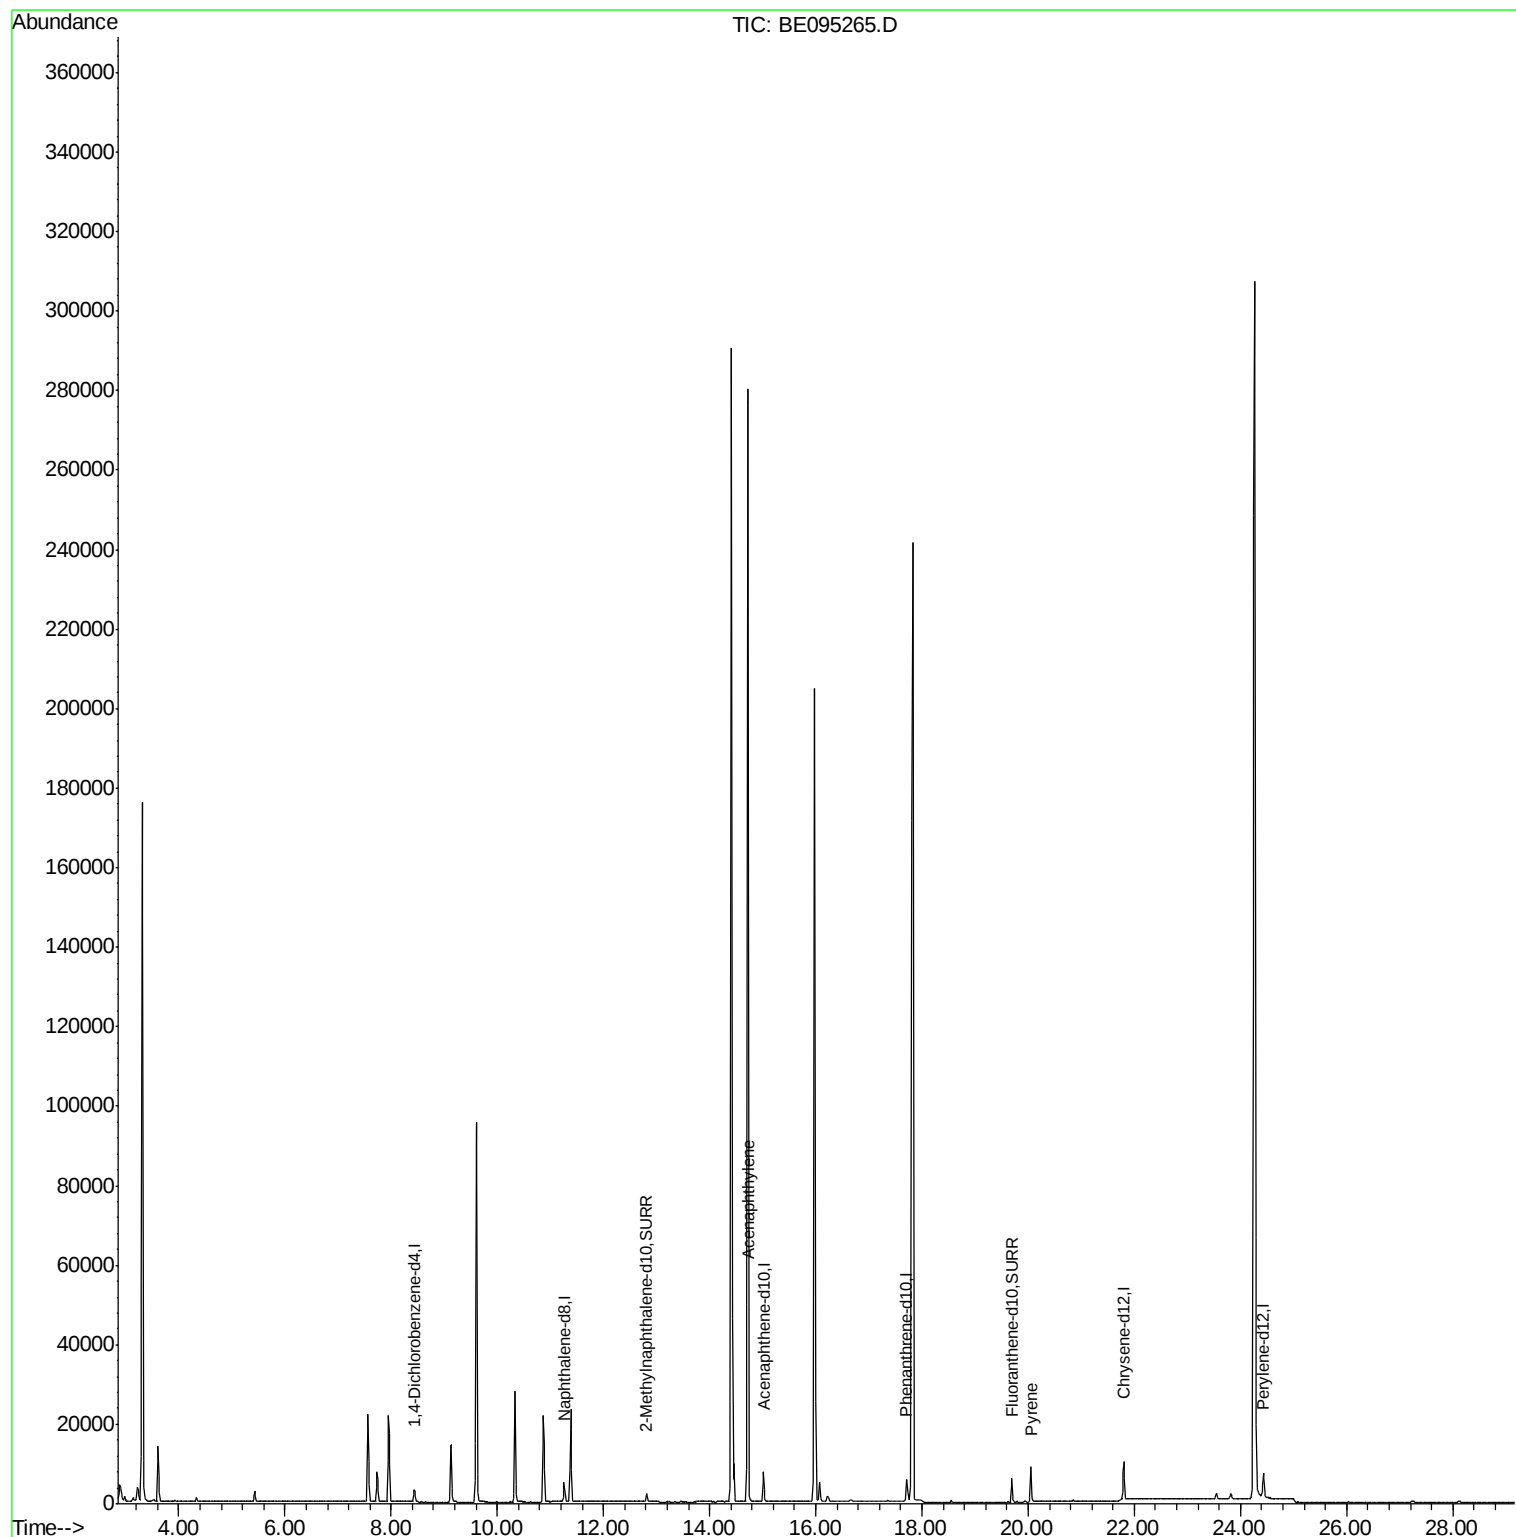

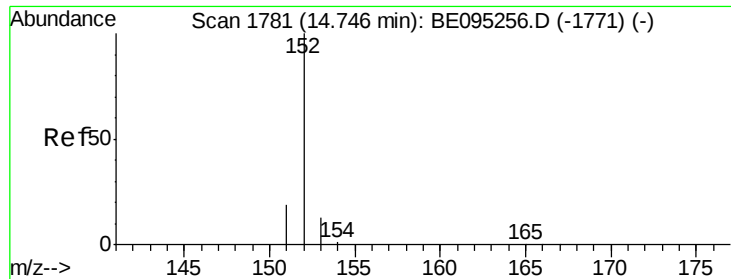

#7

Acenaphthylene

Concen: 0.020 ng/ul

RT: 14.74 min Scan# 1781

Delta R.T. -0.00 min

Lab File: BE095265.D

Acq: 30 Jan 2018 2:08

Instrument :

BNA_E





ClientSampleId :

F6B46

Tgt Ion:	152	Resp:	406
Ion Ratio	Lower	Upper	
152	100		
151	33.5	17.1	25.7#
153	31.9	12.8	19.2#

Manual Integrations
APPROVED

Sohil
1/30/2018 3:32:54 PM

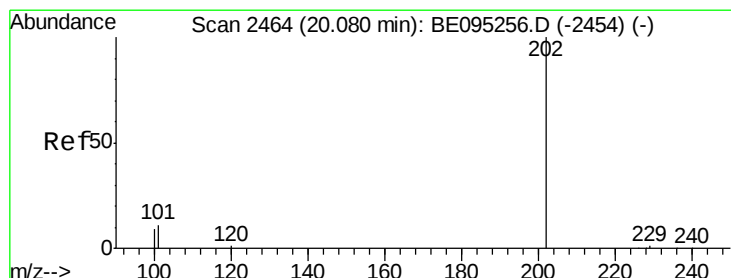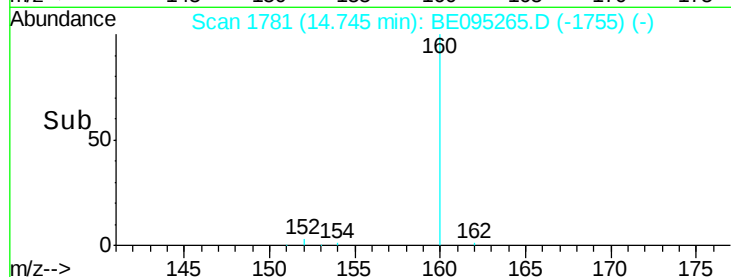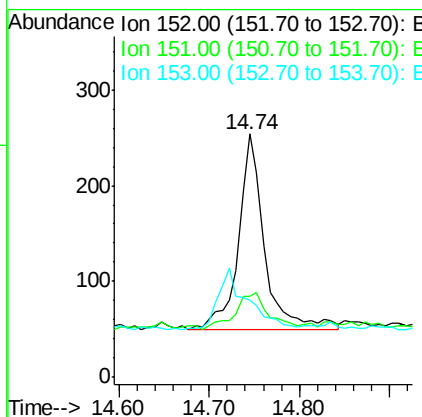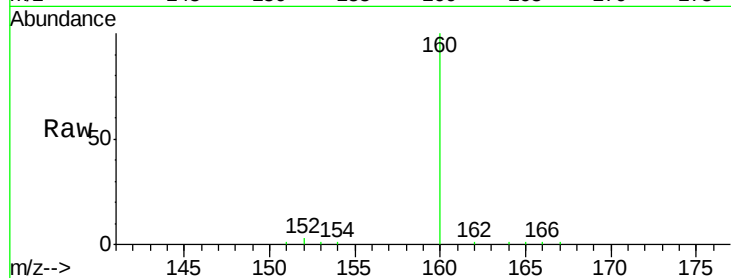

#17

Pyrene

Concen: 0.022 ng/ul m

RT: 20.08 min Scan# 2464

Delta R.T. -0.00 min

Lab File: BE095265.D

Acq: 30 Jan 2018 2:08

Tgt Ion:	202	Resp:	687
Ion Ratio	Lower	Upper	
202	100		
101	23.4	18.2	27.4
100	24.7	15.6	23.4#

