


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE013015\
 Data File : BE089454.D
 Acq On : 31 Jan 2015 1:50
 Operator : TP/IZ
 Sample : DFTPP
 Misc : G
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE013015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jan 31 05:05:18 2015

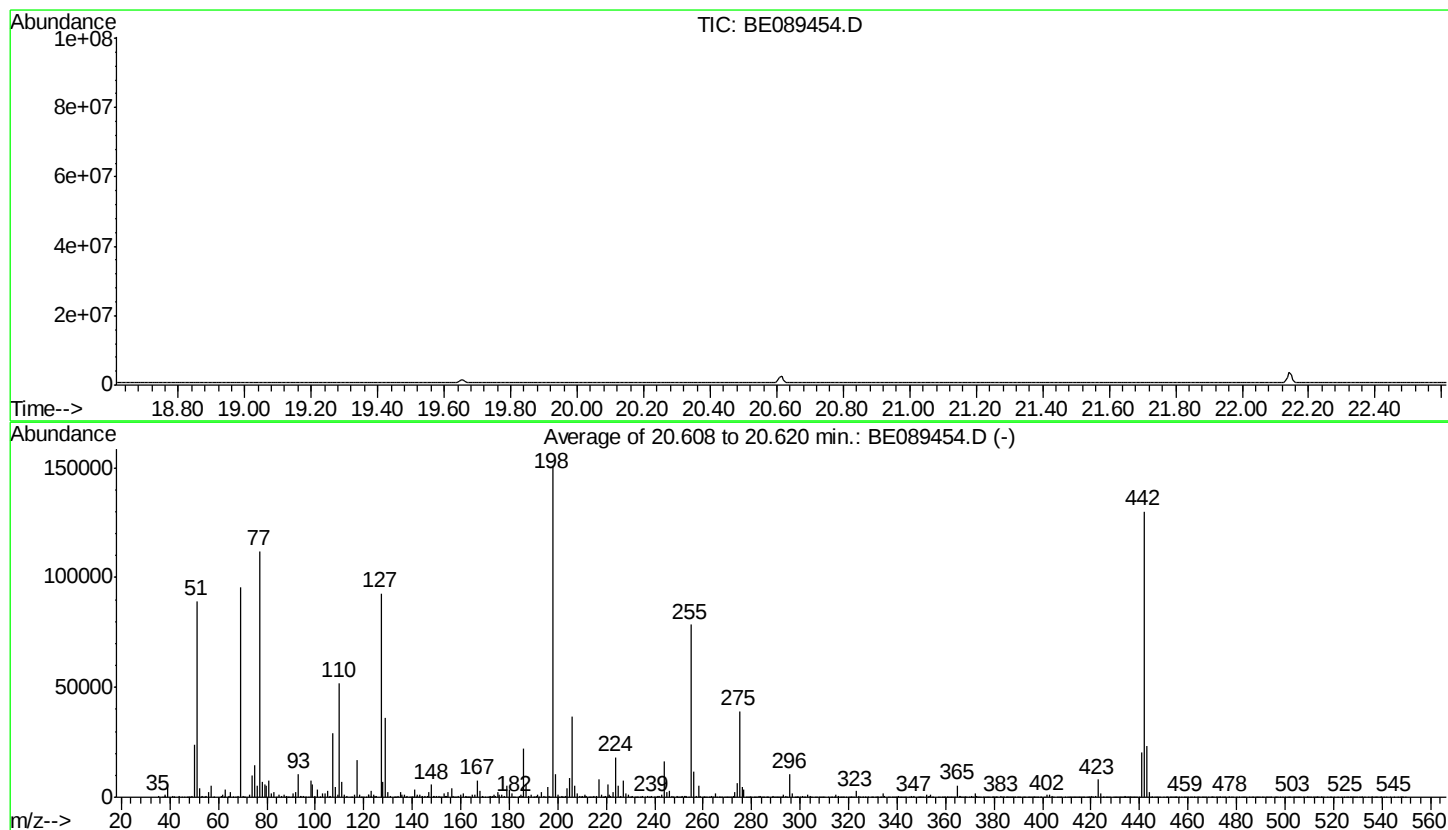

AutoFind: Scans 3271, 3272, 3273; Background Corrected with Scan 3264

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.2	89458	PASS
68	69	0.00	2	0.9	843	PASS
69	198	0.00	100	63.4	95709	PASS
70	69	0.00	2	0.4	419	PASS
127	198	10	80	61.4	92685	PASS
197	198	0.00	2	0.2	269	PASS
198	198	100	100	100.0	150994	PASS
199	198	5	9	7.1	10659	PASS
275	198	10	60	25.9	39152	PASS
365	198	1	100	3.6	5421	PASS
441	442	0.01	24	15.7	20459	PASS
442	198	50	100	86.2	130141	PASS
443	442	15	24	18.1	23584	PASS