


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE013015\
 Data File : BE089471.D
 Acq On : 31 Jan 2015 14:51
 Operator : TP/IZ
 Sample : DFTPP
 Misc : MDL-SOIL-0.1/0.2
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE013015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jan 31 05:05:18 2015

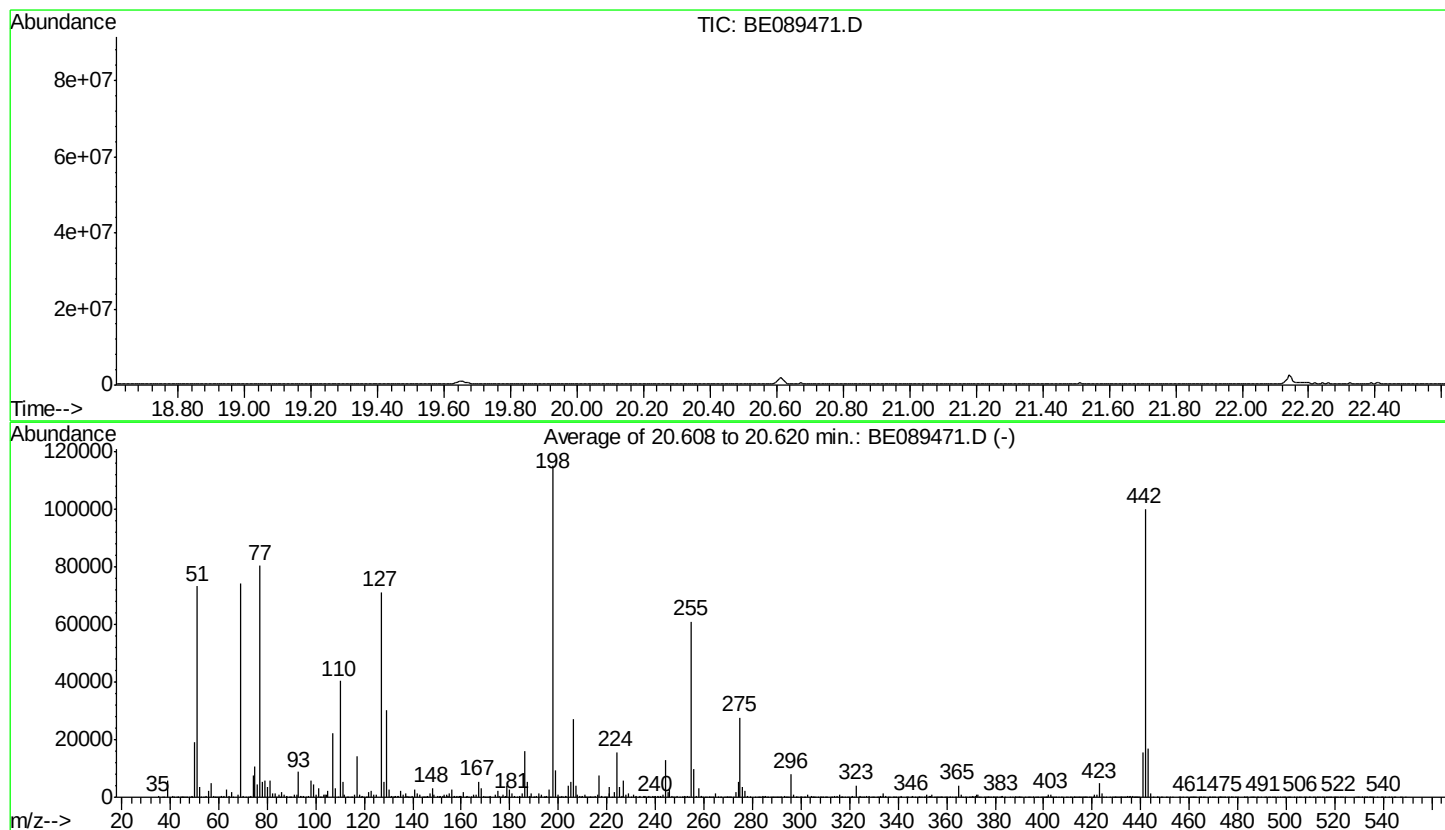

AutoFind: Scans 3271, 3272, 3273; Background Corrected with Scan 3262

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	63.6	73123	PASS
68	69	0.00	2	1.0	727	PASS
69	198	0.00	100	64.3	73934	PASS
70	69	0.00	2	0.4	313	PASS
127	198	10	80	61.9	71139	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	114912	PASS
199	198	5	9	8.2	9369	PASS
275	198	10	60	24.0	27586	PASS
365	198	1	100	3.5	4068	PASS
441	442	0.01	24	15.6	15613	PASS
442	198	50	100	87.1	100037	PASS
443	442	15	24	17.1	17066	PASS