


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE013015\
Data File : BE089484.D
Acq On : 1 Feb 2015 1:54
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE013015.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Jan 31 05:05:18 2015

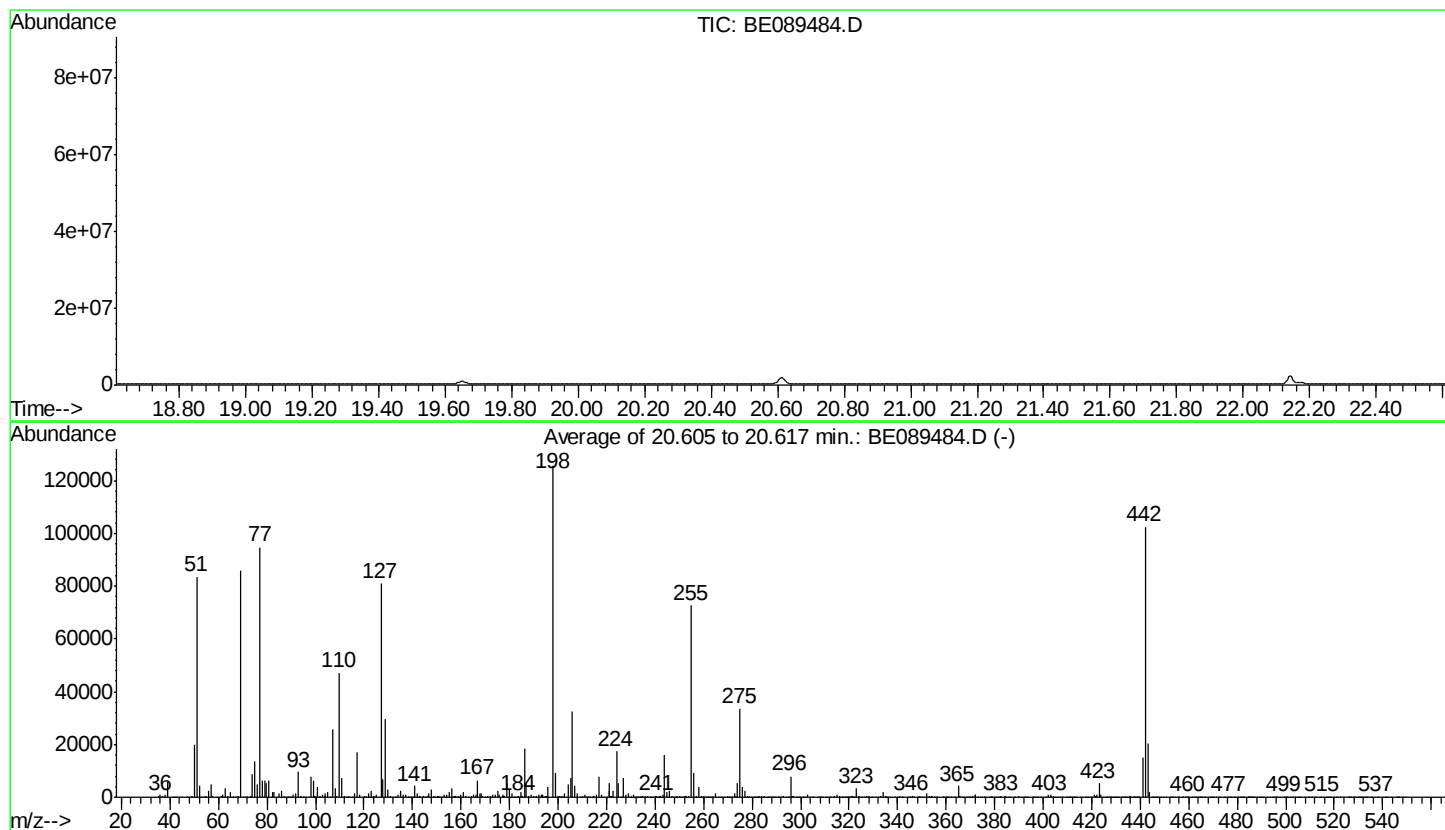

AutoFind: Scans 3271, 3272, 3273; Background Corrected with Scan 3262

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	66.4	83429	PASS
68	69	0.00	2	0.7	613	PASS
69	198	0.00	100	68.5	85989	PASS
70	69	0.00	2	0.2	180	PASS
127	198	10	80	64.4	80862	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	125617	PASS
199	198	5	9	7.3	9114	PASS
275	198	10	60	26.7	33517	PASS
365	198	1	100	3.5	4366	PASS
441	442	0.01	24	14.6	14974	PASS
442	198	50	100	81.5	102322	PASS
443	442	15	24	19.9	20324	PASS