


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE013015\
 Data File : BE089494.D
 Acq On : 1 Feb 2015 10:57
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE013015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jan 31 05:05:18 2015

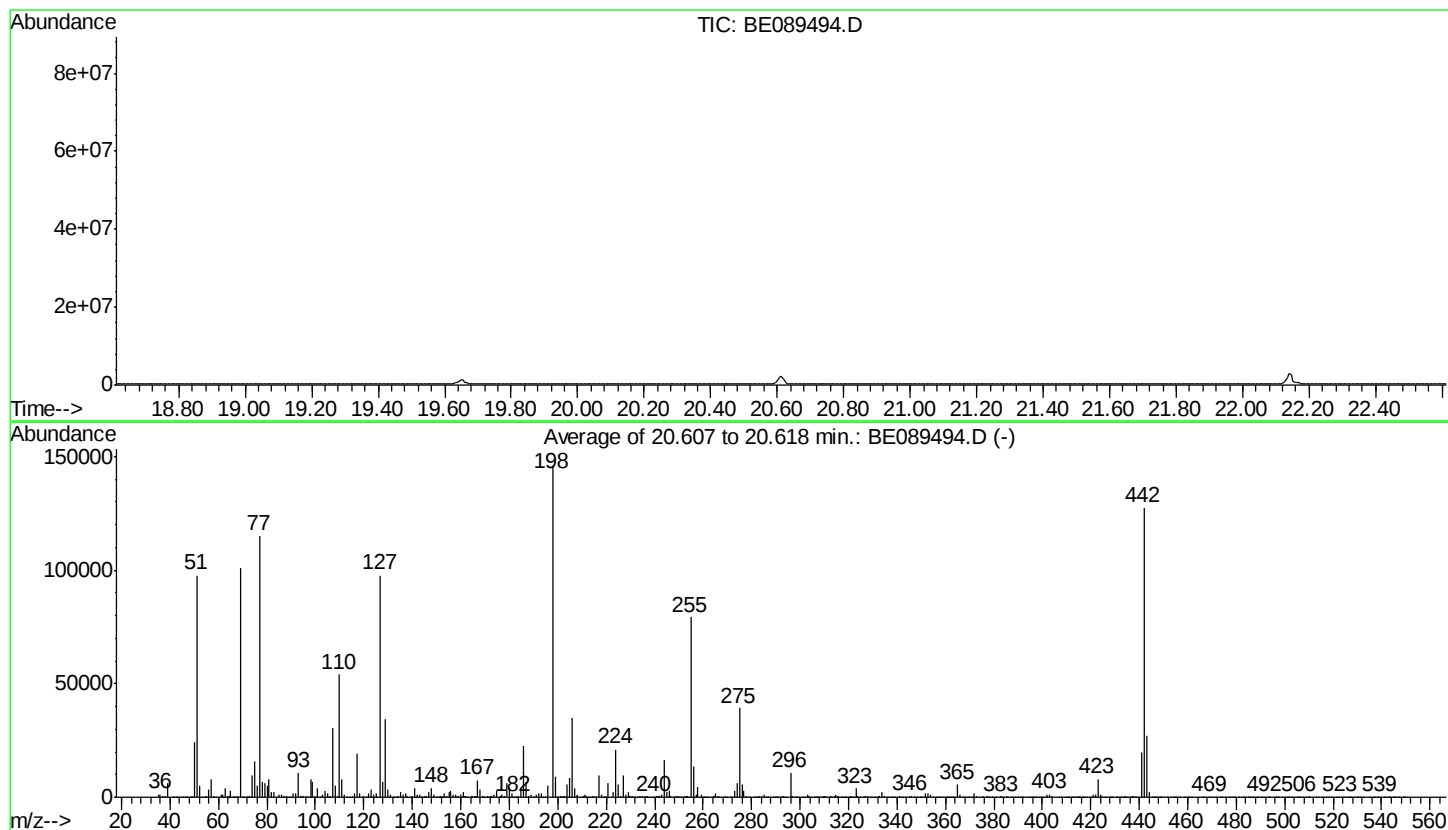

AutoFind: Scans 3271, 3272, 3273; Background Corrected with Scan 3259

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	66.9	97637	PASS
68	69	0.00	2	0.7	700	PASS
69	198	0.00	100	69.1	100866	PASS
70	69	0.00	2	0.2	214	PASS
127	198	10	80	66.9	97621	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	145960	PASS
199	198	5	9	6.0	8763	PASS
275	198	10	60	27.0	39445	PASS
365	198	1	100	3.8	5582	PASS
441	442	0.01	24	15.5	19809	PASS
442	198	50	100	87.4	127545	PASS
443	442	15	24	21.1	26952	PASS