




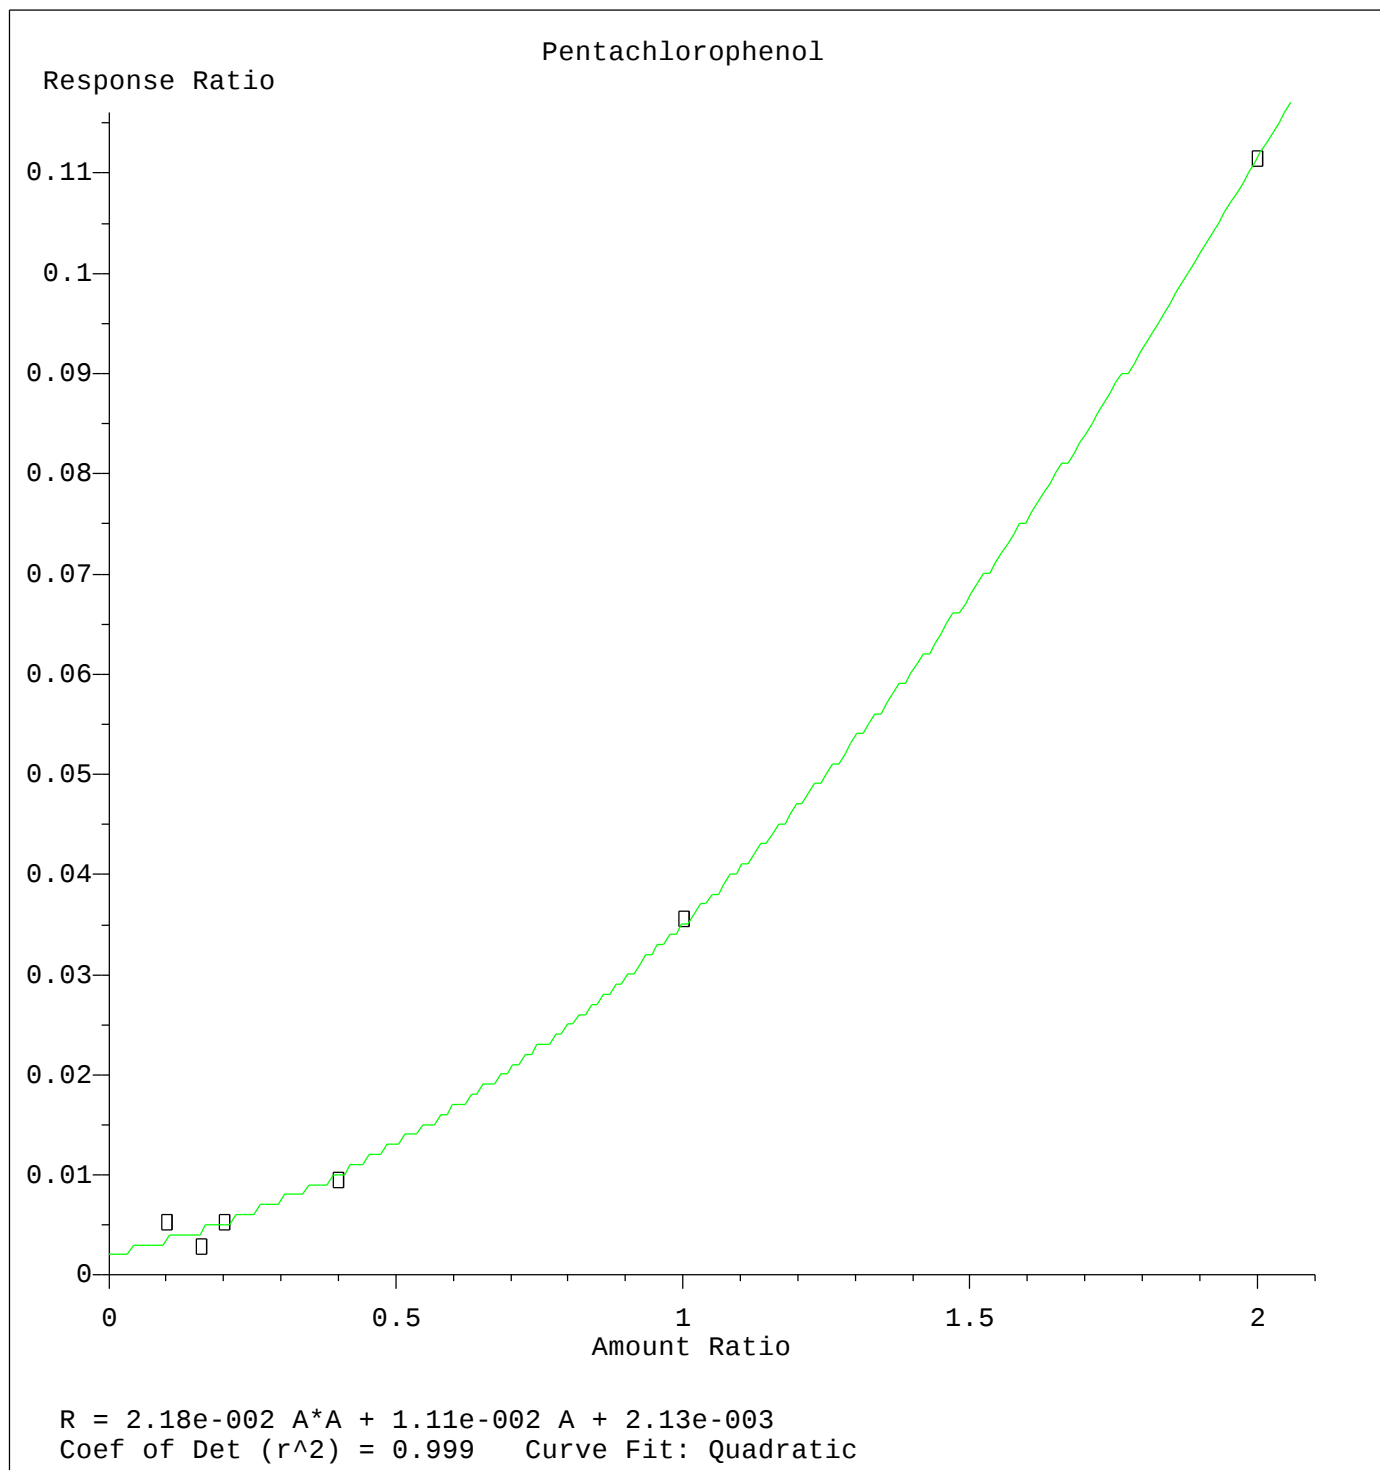

Method Name: Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE013015.M
Calibration Table Last Updated: Sat Jan 31 05:00:59 2015

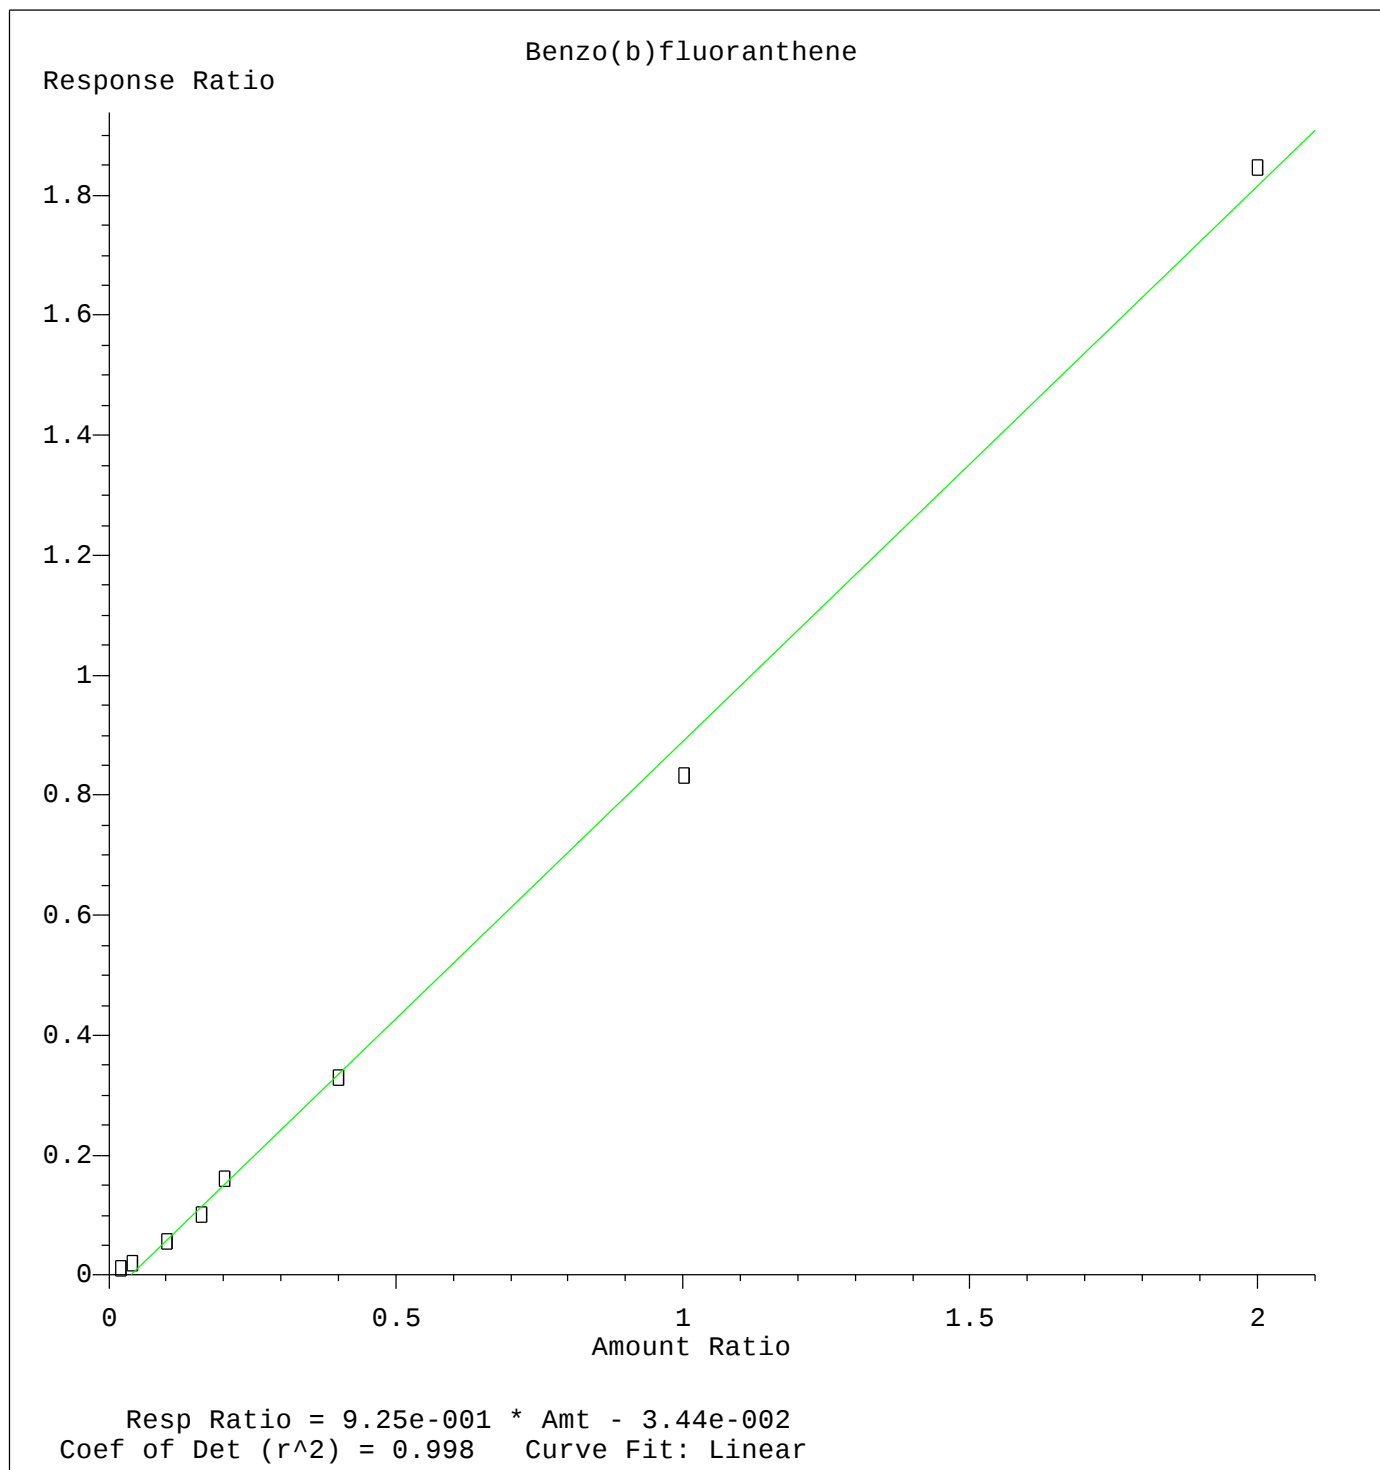


Method Name: Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE013015.M
Calibration Table Last Updated: Sat Jan 31 05:03:42 2015

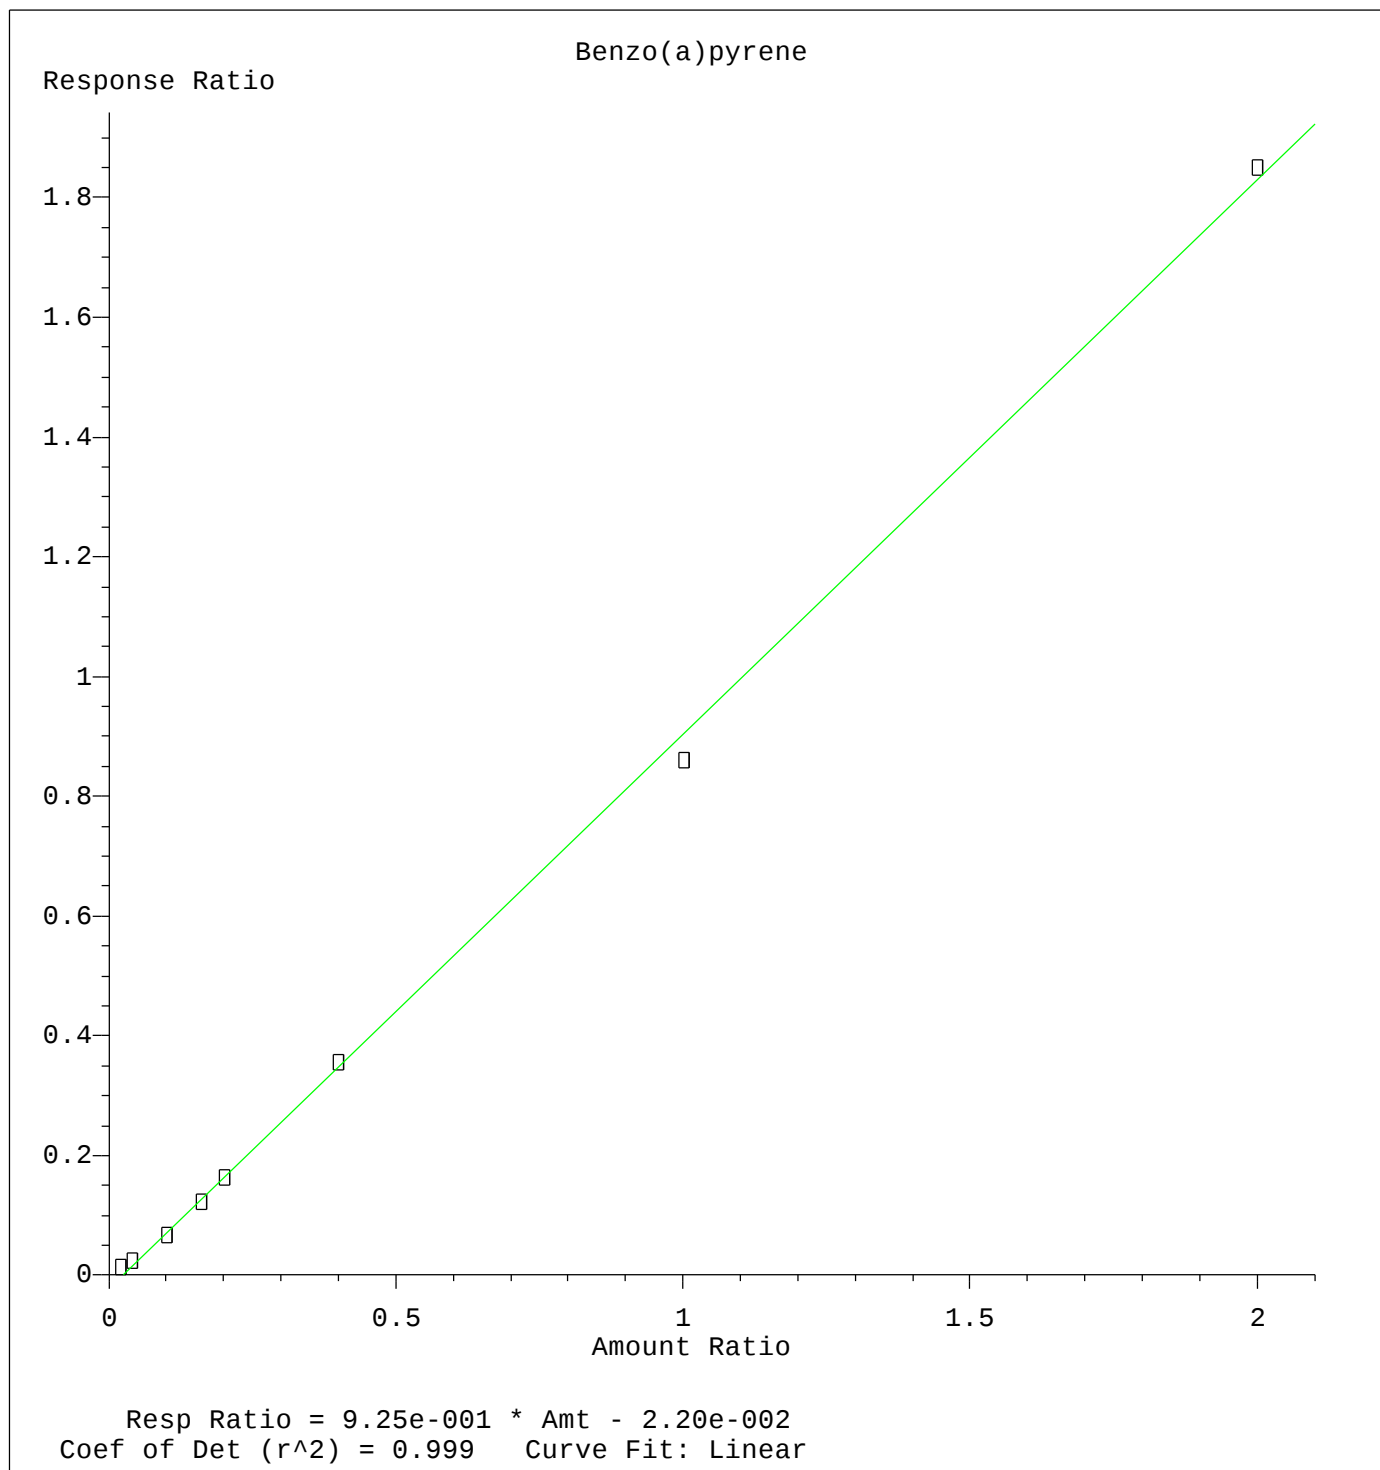

Method Name: Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE013015.M
Calibration Table Last Updated: Sat Jan 31 05:04:19 2015

Dibenzo(a,h)anthracene

Response Ratio

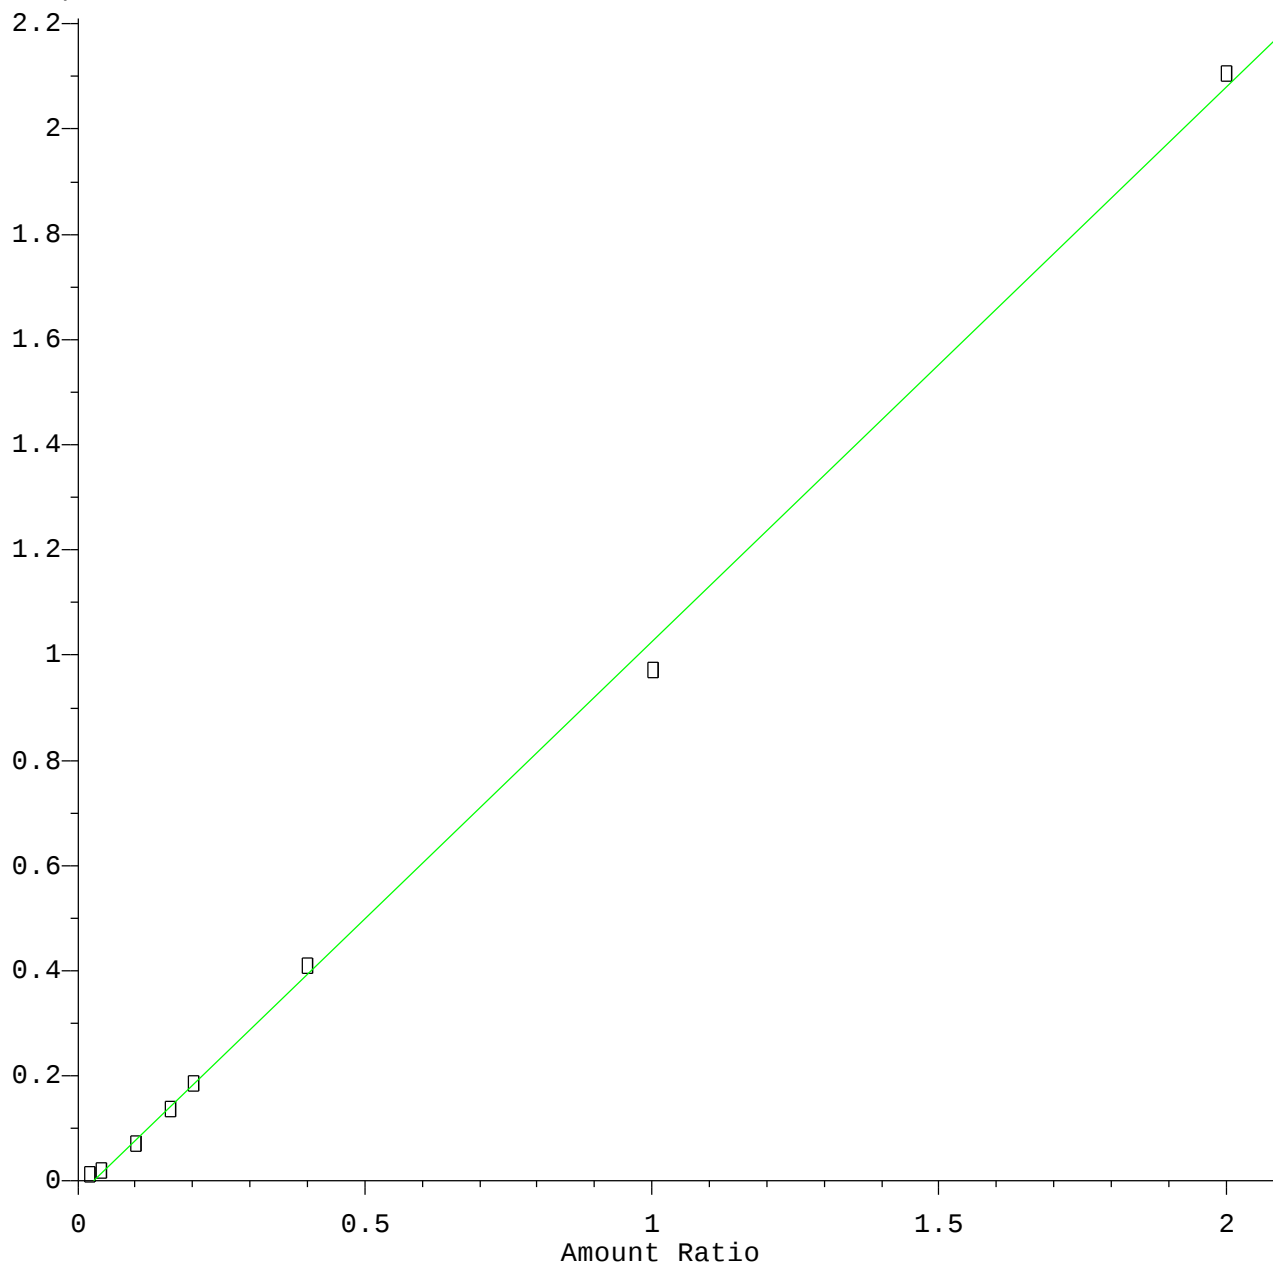

Resp Ratio = $1.05 \times 10^0 \times \text{Amt} - 2.77 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE013015.M
Calibration Table Last Updated: Sat Jan 31 05:04:57 2015