


Data Path : Z:\HPCHEM1\BNA_E\Data\BE013015\
 Data File : BE089432.D
 Acq On : 30 Jan 2015 4:15
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE013015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jan 31 05:05:18 2015

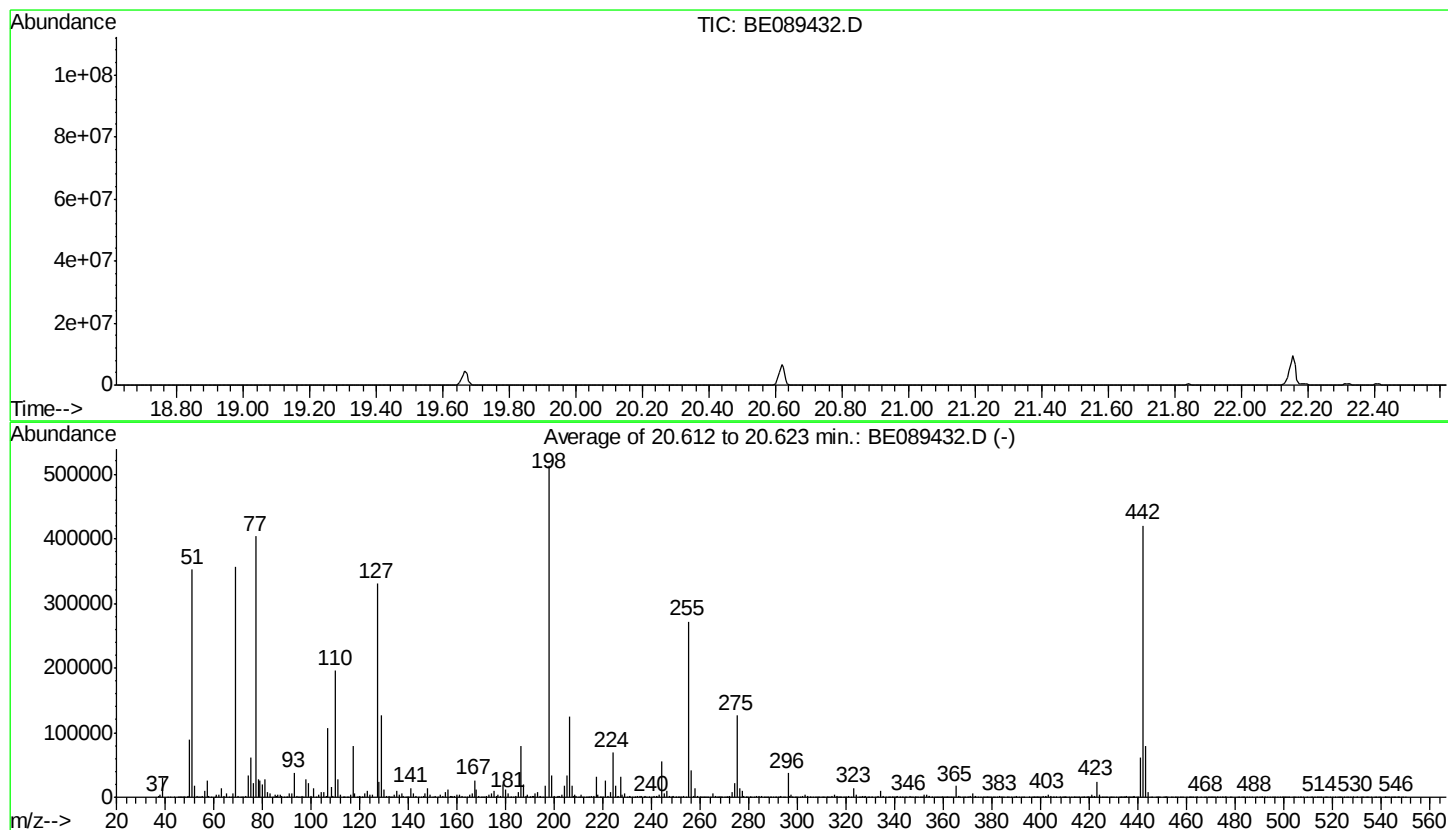

AutoFind: Scans 3272, 3273, 3274; Background Corrected with Scan 3259

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	68.6	351990	PASS
68	69	0.00	2	1.9	6809	PASS
69	198	0.00	100	69.6	356935	PASS
70	69	0.00	2	0.7	2436	PASS
127	198	10	80	64.5	330730	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	513057	PASS
199	198	5	9	6.6	33848	PASS
275	198	10	60	24.7	126485	PASS
365	198	1	100	3.4	17270	PASS
441	442	0.01	24	14.5	61068	PASS
442	198	50	100	81.9	420408	PASS
443	442	15	24	19.0	79868	PASS