


Data Path : Z:\HPCHEM1\BNA_E\Data\BE013015\
 Data File : BE089441.D
 Acq On : 30 Jan 2015 16:38
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE013015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jan 31 05:05:18 2015

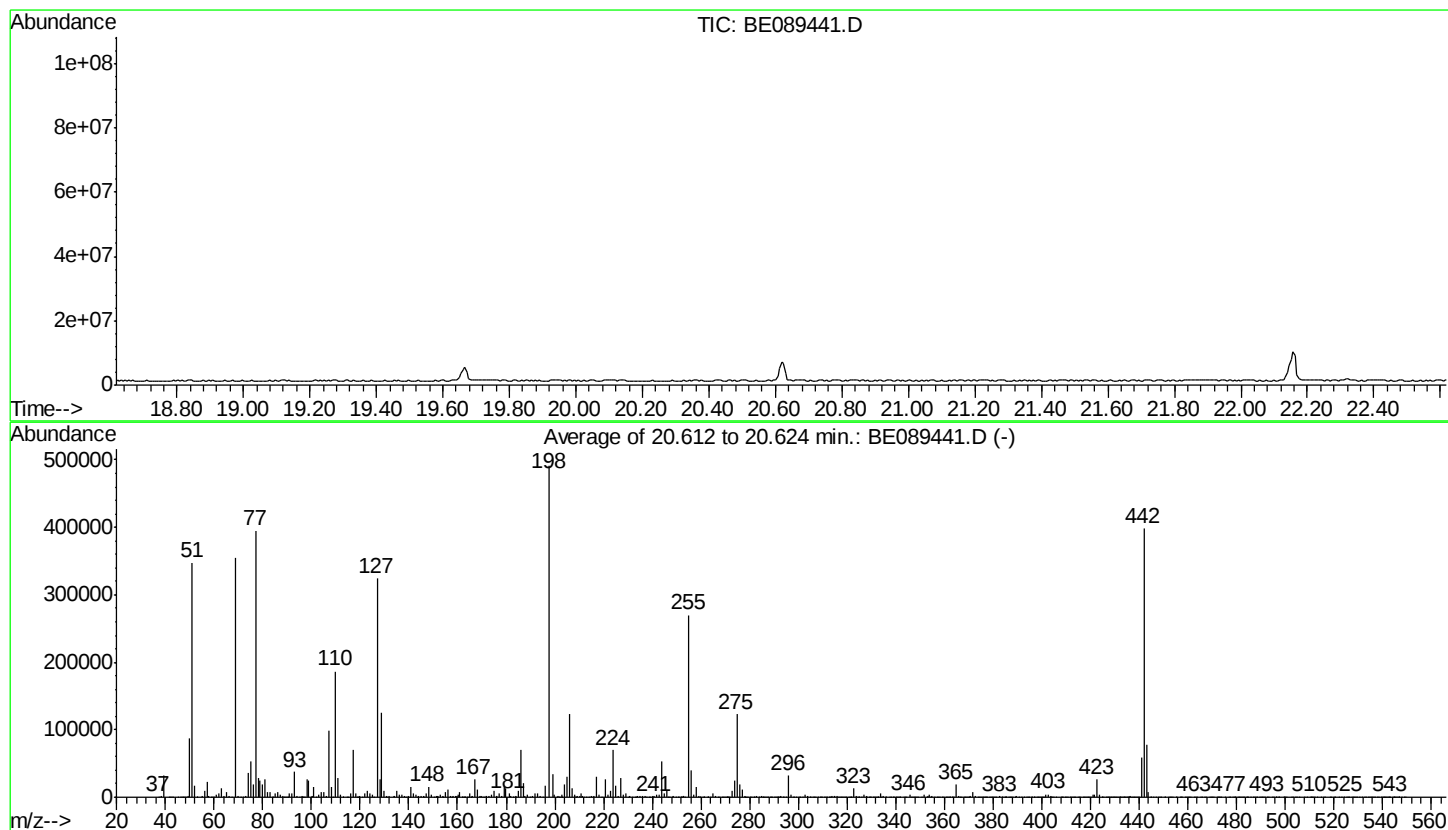

AutoFind: Scans 3272, 3273, 3274; Background Corrected with Scan 3263

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	70.8	347900	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	72.2	354615	PASS
70	69	0.00	2	0.6	2180	PASS
127	198	10	80	65.9	323808	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	491404	PASS
199	198	5	9	6.9	33765	PASS
275	198	10	60	24.9	122527	PASS
365	198	1	100	3.8	18624	PASS
441	442	0.01	24	14.6	58061	PASS
442	198	50	100	81.0	398075	PASS
443	442	15	24	19.7	78485	PASS