

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013018\
 Data File : BE095284.D
 Acq On : 30 Jan 2018 14:15
 Operator : SJ/JU
 Sample : J1243-17DL 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Jan 31 01:25:50 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 31 01:22:09 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2300	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	6996	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	4300	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	9026	0.40	ng/ul	0.00
16) Chrysene-d12	21.81	240	9690	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	9831	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	870	0.08	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	2305	0.07	ng/ul	0.00
Target Compounds				Ovalue		
3) Naphthalene	11.31	128	6628	0.338	ng/ul#	90
5) 2-Methylnaphthalene	12.89	142	1990	0.152	ng/ul	100
8) Acenaphthene	15.08	153	1011	0.063	ng/ul#	93
9) Fluorene	16.03	166	502	0.030	ng/ul#	73
11) Pentachlorophenol	17.36	266	134	0.077	ng/ul	93
12) Phenanthrene	17.75	178	2117	0.070	ng/ul#	89
15) Fluoranthene	19.72	202	902	0.023	ng/ul	88
17) Pyrene	20.08	202	1150	0.035	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013018\
Data File : BE095284.D
Acq On : 30 Jan 2018 14:15
Operator : SJ/JU
Sample : J1243-17DL 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Jan 31 01:25:50 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 01:22:09 2018
Response via : Initial Calibration

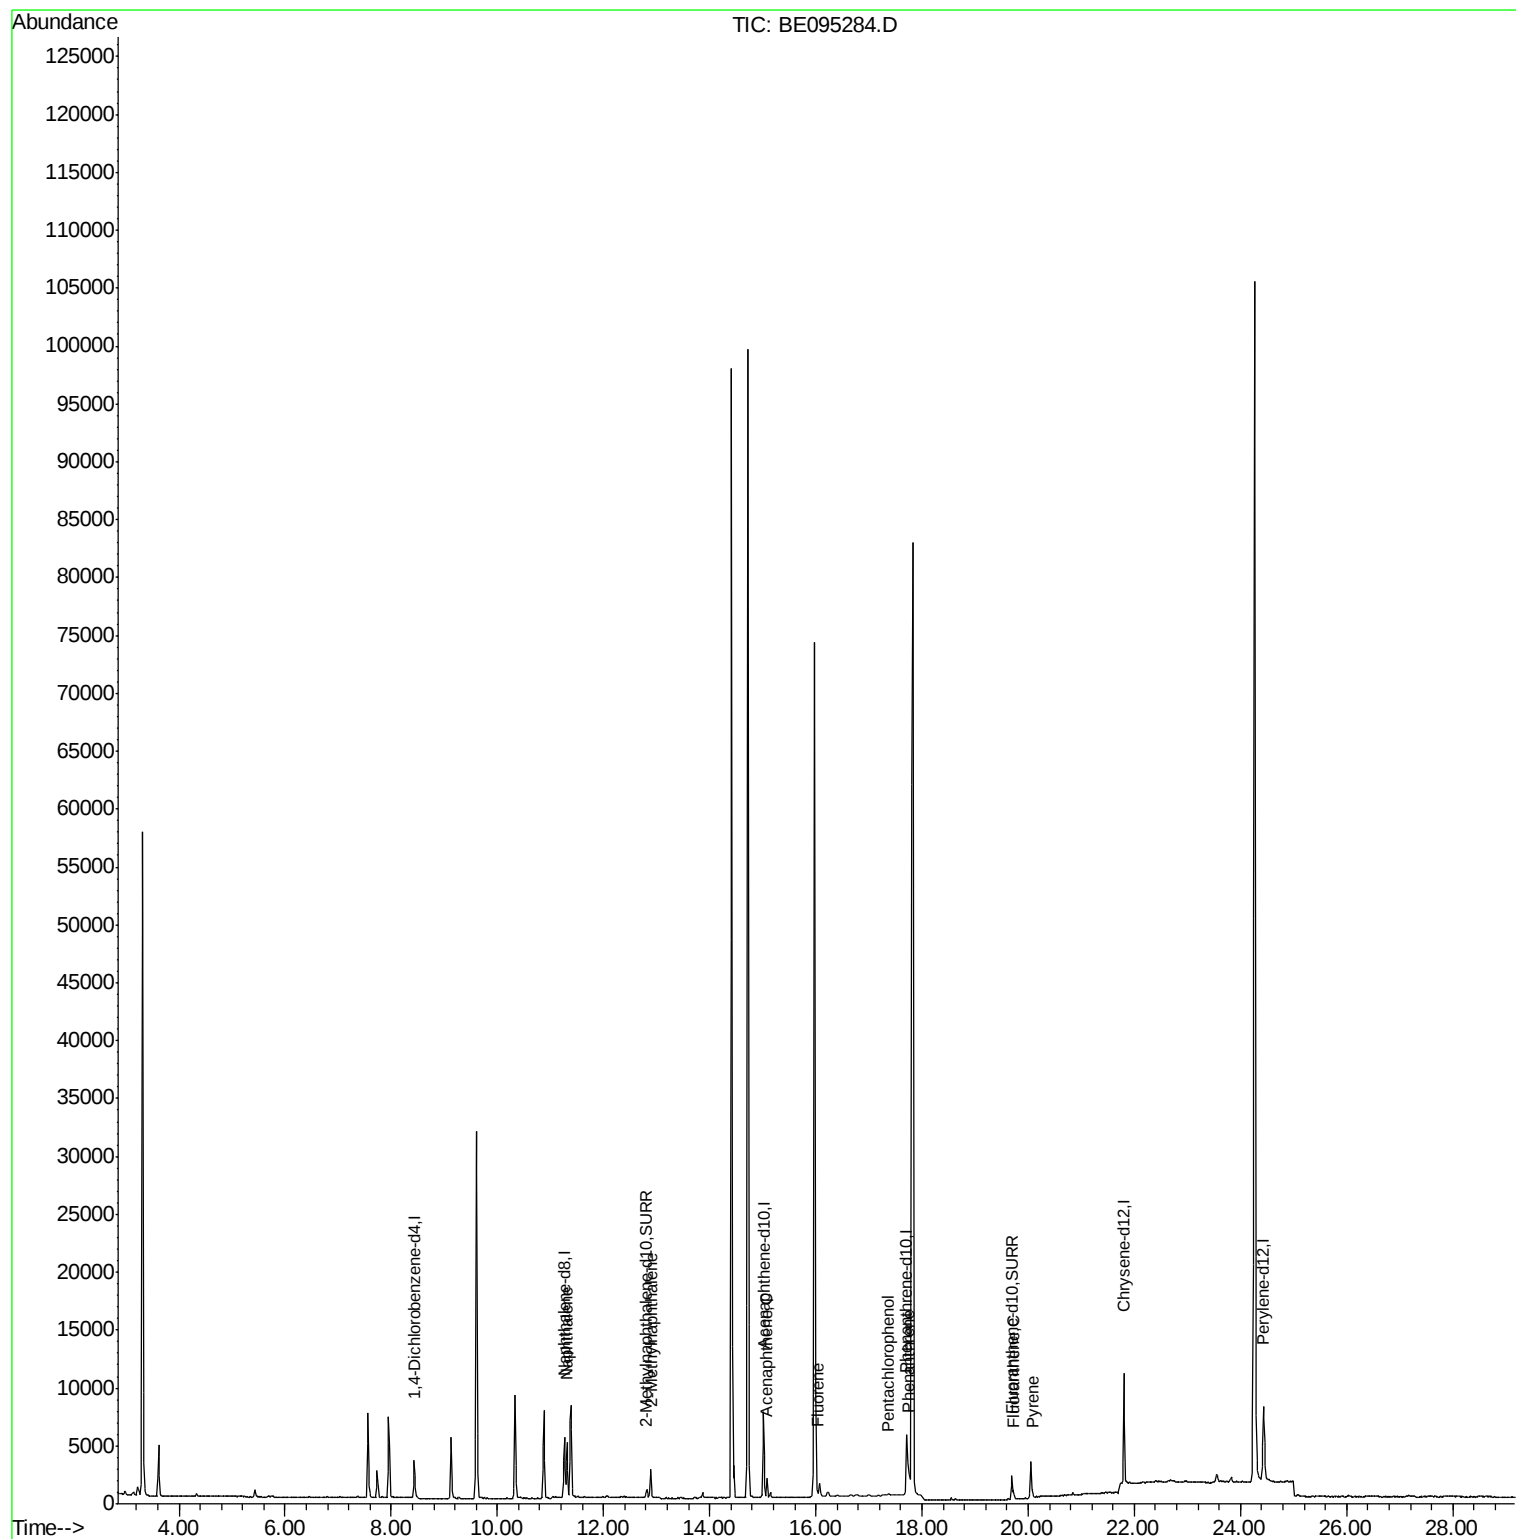

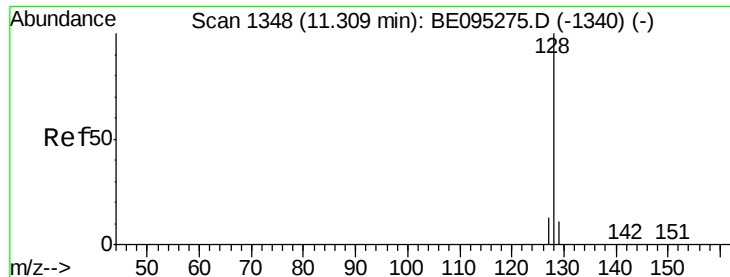

#3

Naphthalene

Concen: 0.338 ng/ul

RT: 11.31 min Scan# 1348

Delta R.T. 0.00 min

Lab File: BE095284.D

Acq: 30 Jan 2018 14:15

Instrument :

BNA_E

ClientSampleId :


Tot Ion:128 Resp: 6628

Ion Ratio Lower Upper

128 100

129 12.3 11.3 16.9




127 14.1 4.0 6.0#

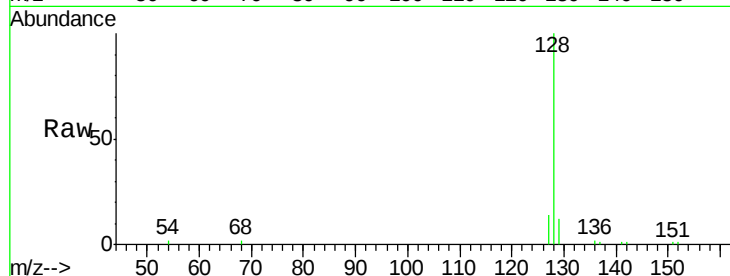

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

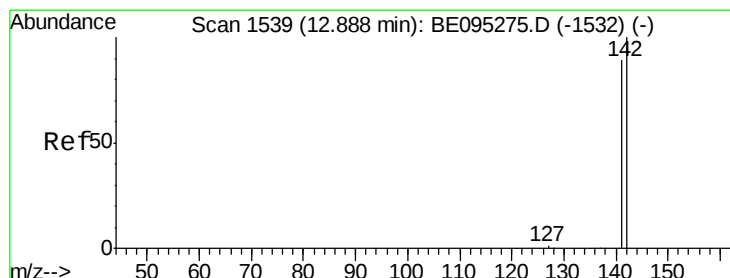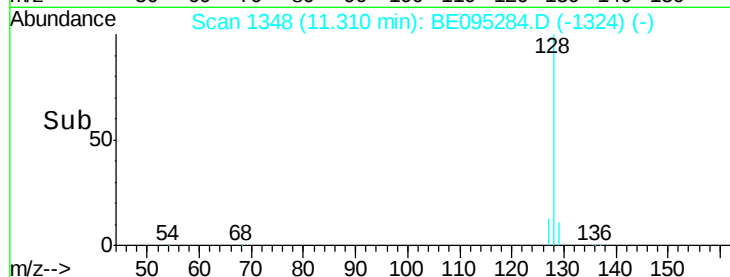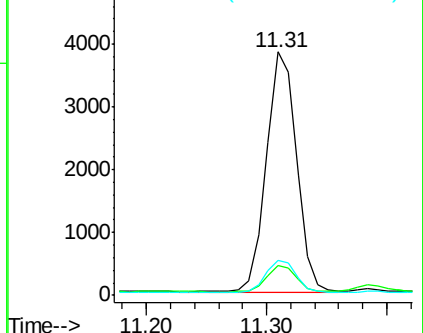

#5

2-Methylnaphthalene

Concen: 0.152 ng/ul

RT: 12.89 min Scan# 1539

Delta R.T. 0.00 min

Lab File: BE095284.D


Acq: 30 Jan 2018 14:15

Tgt Ion:142 Resp: 1990

Ion Ratio Lower Upper



142 100


141 90.9 72.6 108.8

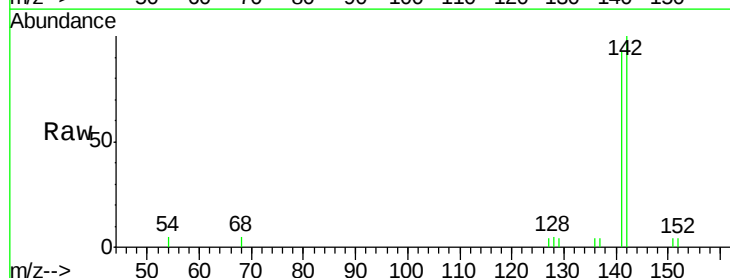

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

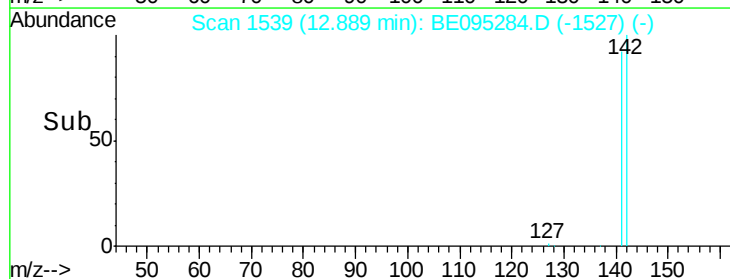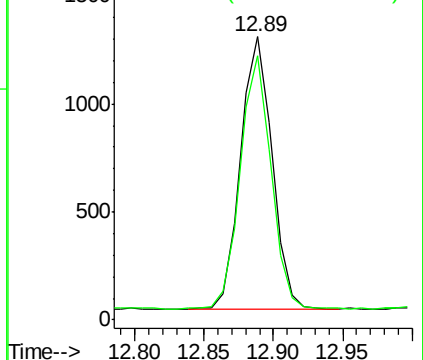

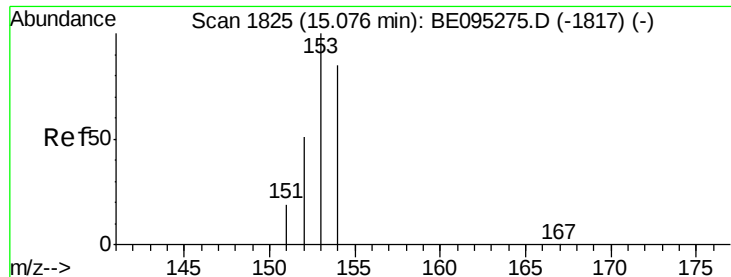

#8

Acenaphthene

Concen: 0.063 ng/ul

RT: 15.08 min Scan# 1825

Delta R.T. 0.00 min

Lab File: BE095284.D

Acq: 30 Jan 2018 14:15

Instrument :

BNA_E

ClientSampleId :


Tot Ion:153 Resp: 1011

Ion Ratio Lower Upper

153 100

152 54.8 36.0 54.0#

154 86.6 72.0 108.0

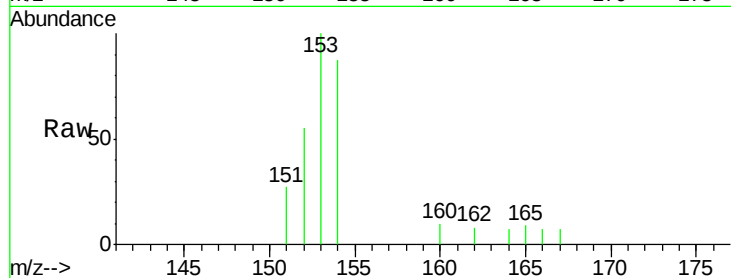

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

15.08



600

400

200

0

Time--> 15.00 15.05 15.10

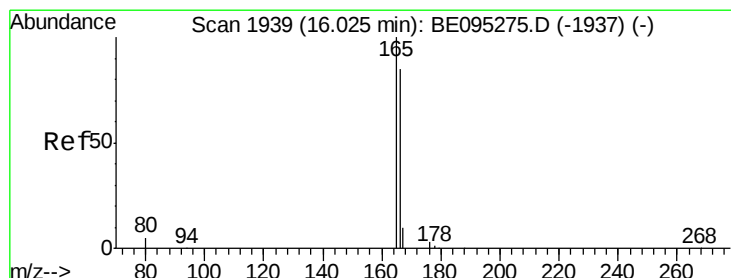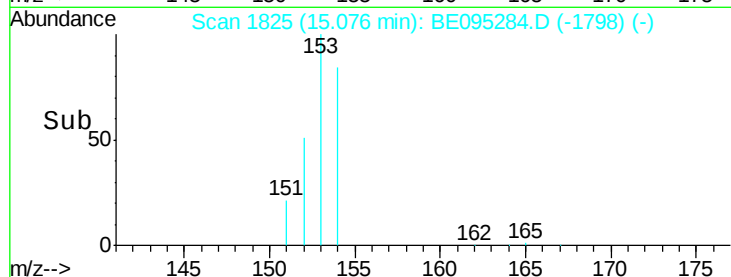

#9

Fluorene

Concen: 0.030 ng/ul

RT: 16.03 min Scan# 1939

Delta R.T. 0.00 min

Lab File: BE095284.D

Acq: 30 Jan 2018 14:15


Tgt Ion:166 Resp: 502

Ion Ratio Lower Upper

166 100

165 118.4 73.4 110.2#

167 27.5 14.6 22.0#

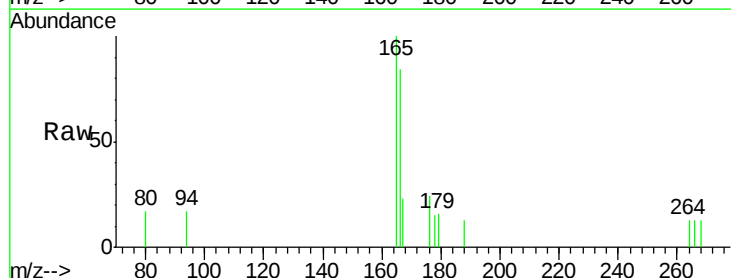

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

16.03


300


200

100

0

Time--> 16.00 16.05




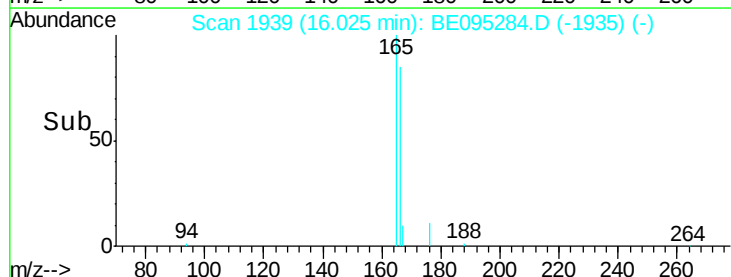


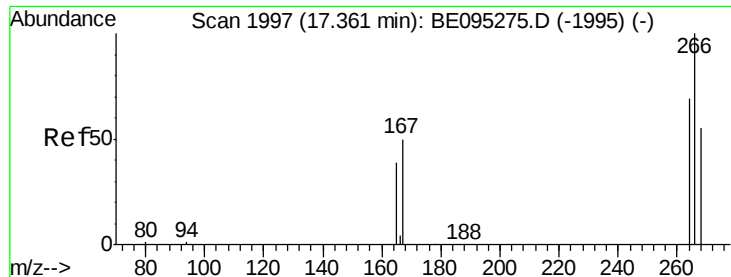

#11
 Pentachlorophenol
 Concen: 0.077 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. 0.00 min
 Lab File: BE095284.D
 Acq: 30 Jan 2018 14:15




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:266 Resp: 134
 Ion Ratio Lower Upper
 266 100
 264 64.2 47.9 71.9
 268 56.0 49.8 74.8

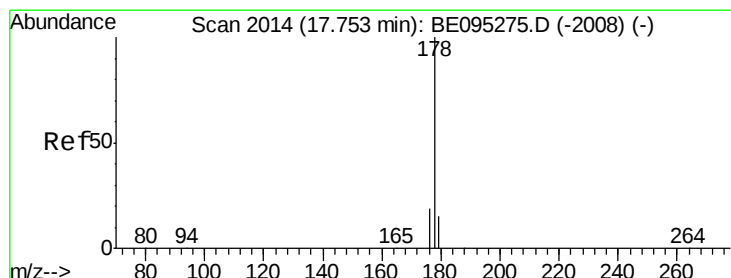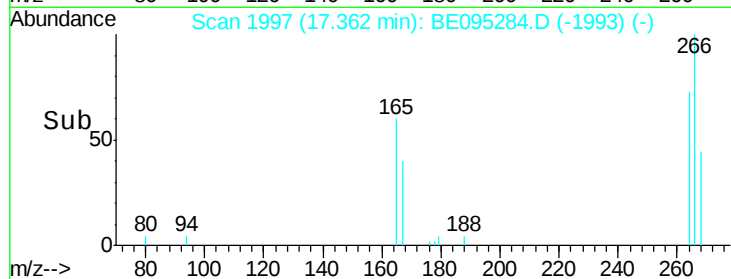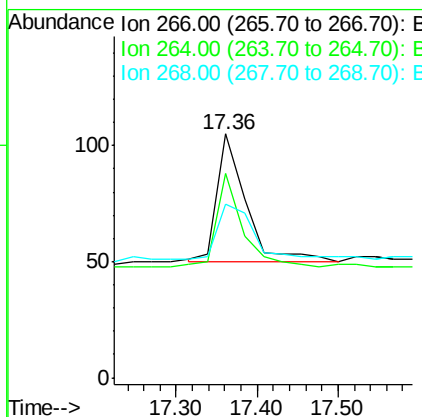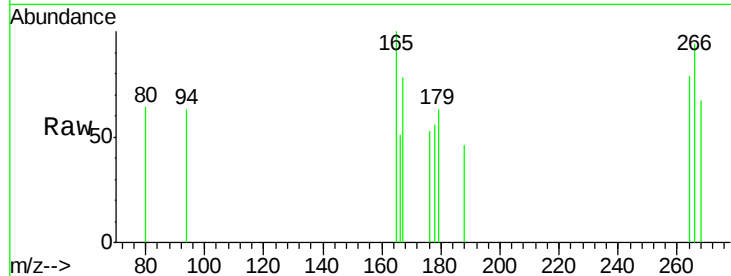

#12
 Phenanthrene
 Concen: 0.070 ng/ul
 RT: 17.75 min Scan# 2014
 Delta R.T. 0.00 min
 Lab File: BE095284.D
 Acq: 30 Jan 2018 14:15

Tgt Ion:178 Resp: 2117
 Ion Ratio Lower Upper
 178 100
 179 19.1 18.4 27.6
 176 23.5 13.6 20.4#

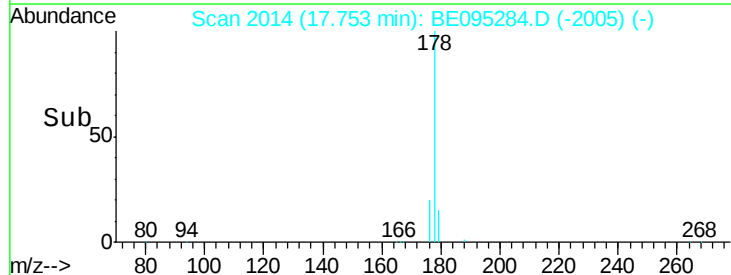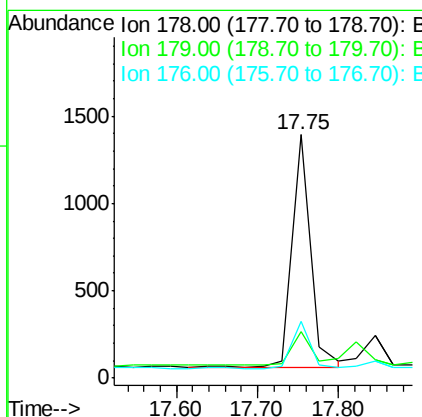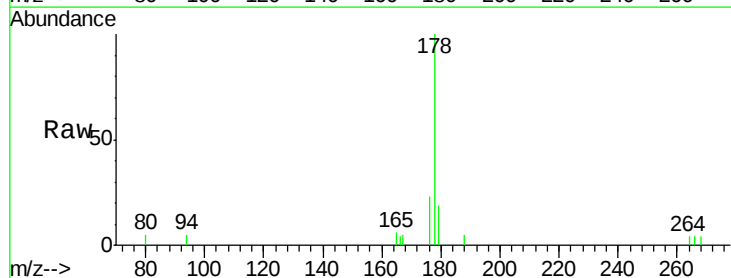

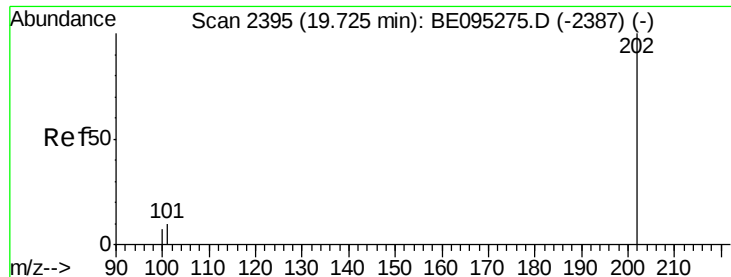

#15

Fluoranthene

Concen: 0.023 ng/ul

RT: 19.72 min Scan# 2395

Delta R.T. -0.00 min

Lab File: BE095284.D

Acq: 30 Jan 2018 14:15

Instrument :

BNA_E

ClientSampleId :


Tot Ion:202 Resp: 902

Ion Ratio Lower Upper

202 100

101 17.4 0.0 30.3




100 15.7 0.0 39.5

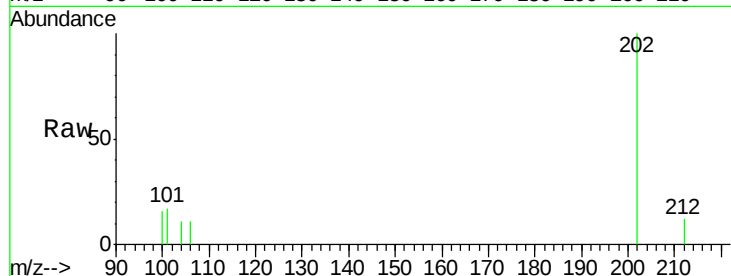

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BE

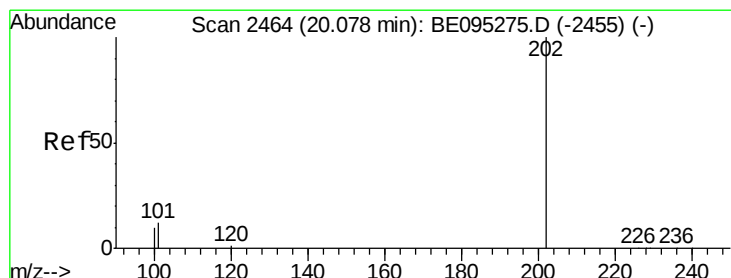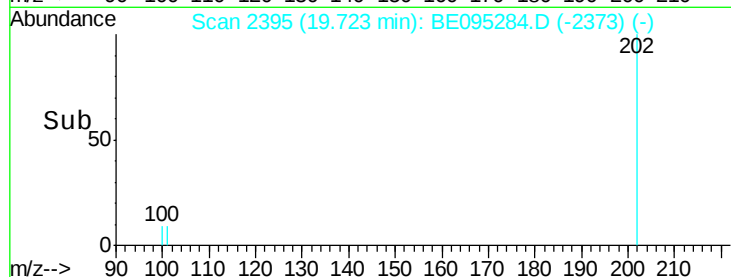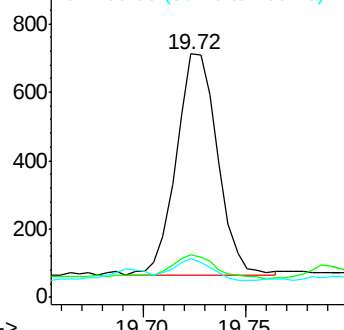

#17

Pyrene

Concen: 0.035 ng/ul

RT: 20.08 min Scan# 2464

Delta R.T. 0.00 min

Lab File: BE095284.D

Acq: 30 Jan 2018 14:15


Tgt Ion:202 Resp: 1150

Ion Ratio Lower Upper

202 100

101 21.9 18.2 27.4

100 21.7 15.6 23.4

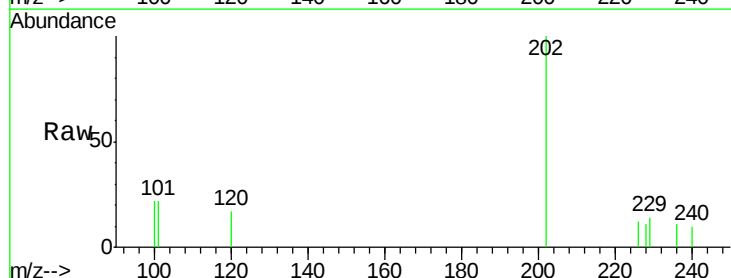

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BE

