

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013018\
 Data File : BE095287.D
 Acq On : 30 Jan 2018 16:03
 Operator : SJ/JU
 Sample : J1233-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Jan 31 01:26:23 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 31 01:22:09 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2308	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	7009	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	4285	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8616	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	9539	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	348819	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2455	0.22	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	6270	0.19	ng/ul	0.00
Target Compounds						
					Ovalue	
3) Naphthalene	11.31	128	744	0.038	ng/ul#	68
5) 2-Methylnaphthalene	12.89	142	637	0.049	ng/ul	99
7) Acenaphthylene	14.75	152	19605	0.951	ng/ul	97
8) Acenaphthene	15.08	153	949	0.059	ng/ul#	84
11) Pentachlorophenol	17.36	266	193608	116.015	ng/ul	96
12) Phenanthrene	17.75	178	17813	0.615	ng/ul#	88
13) Anthracene	17.85	178	49910	1.882	ng/ul#	92
15) Fluoranthene	19.73	202	575244	15.331	ng/ul	81
17) Pyrene	20.08	202	613114	19.155	ng/ul#	75
18) Benzo(a)anthracene	21.79	228	117547	3.941	ng/ul#	86
19) Chrysene	21.85	228	219055	7.073	ng/ul	95
23) Benzo(a)pyrene	24.21	252	197666	0.180	ng/ul#	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013018\
Data File : BE095287.D
Acq On : 30 Jan 2018 16:03
Operator : SJ/JU
Sample : J1233-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Jan 31 01:26:23 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 01:22:09 2018
Response via : Initial Calibration

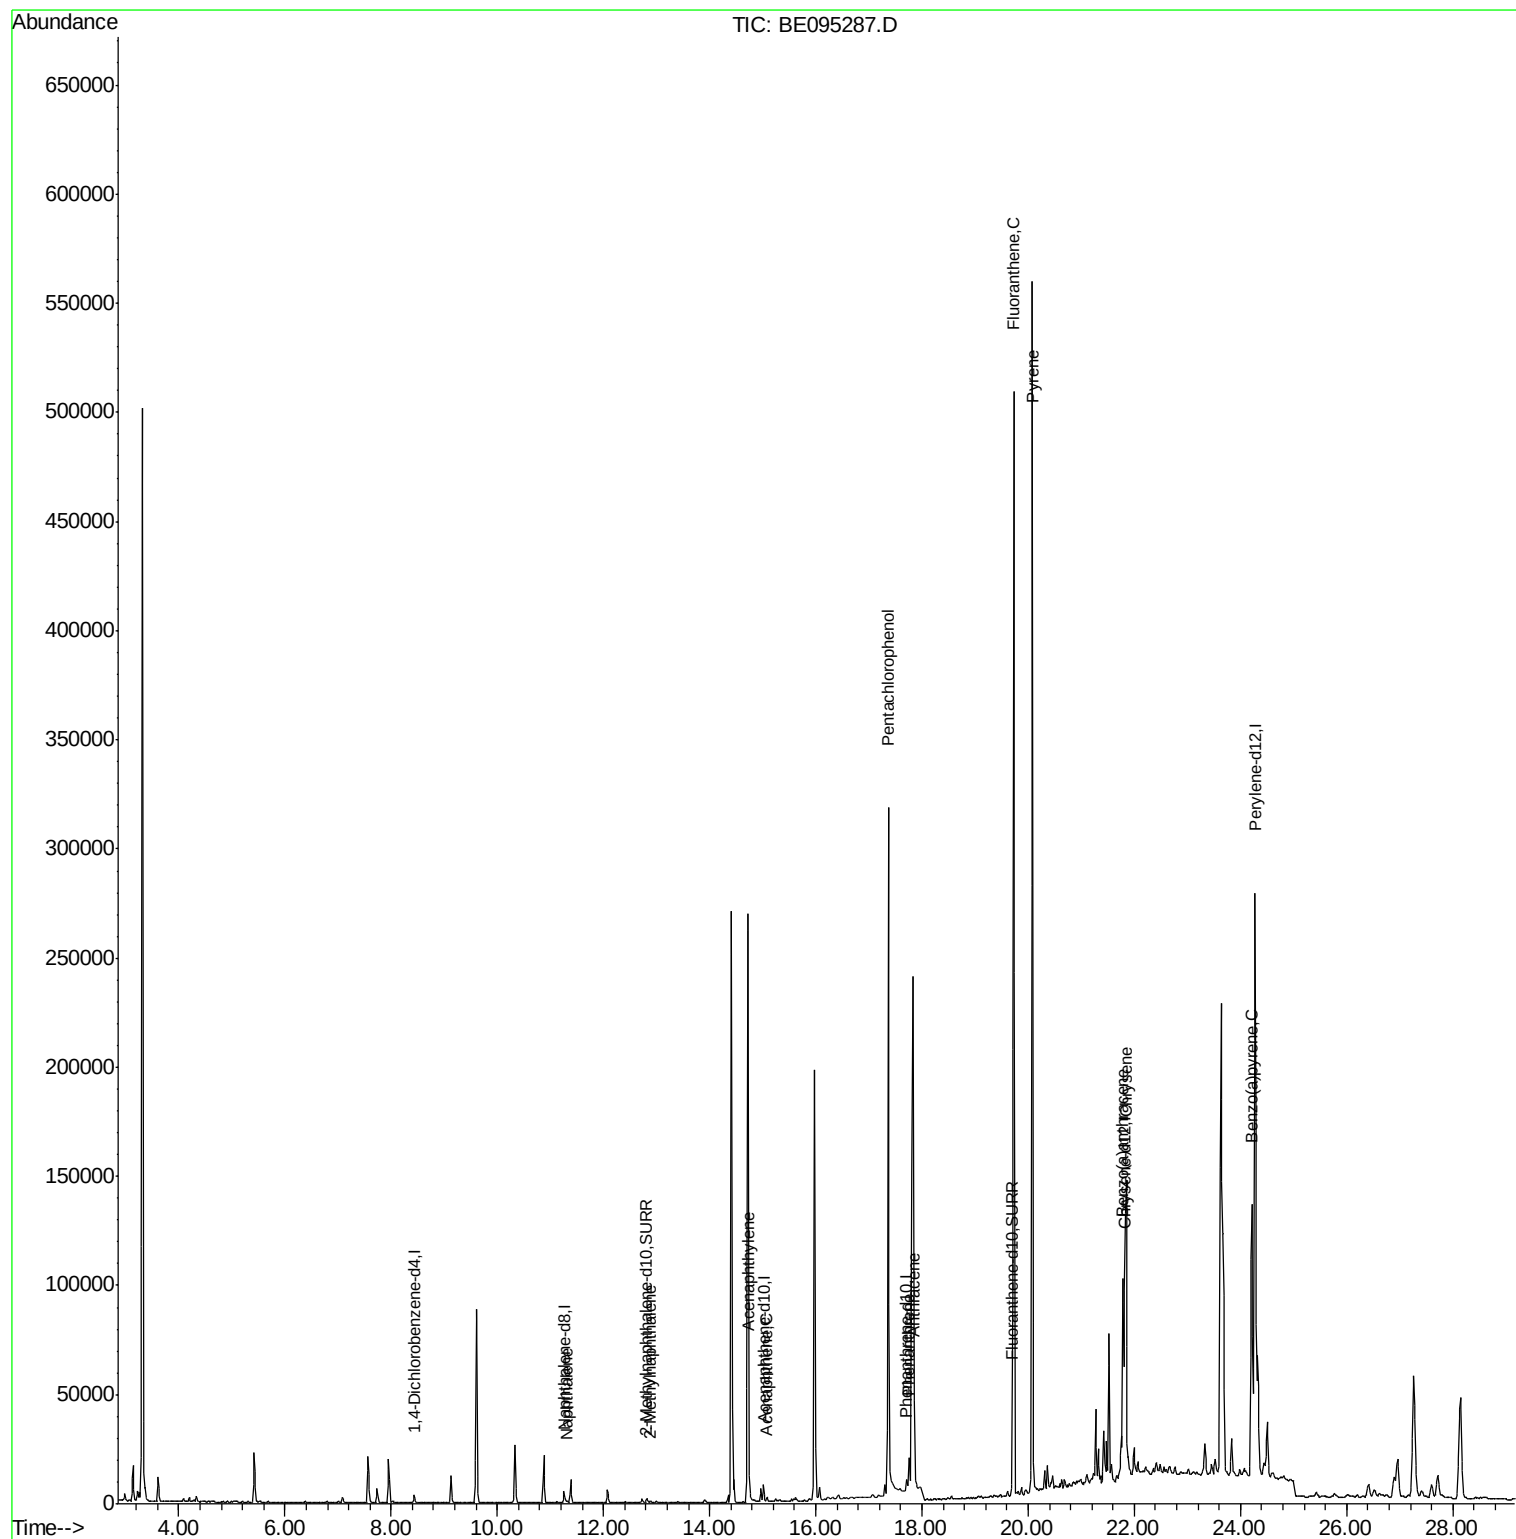

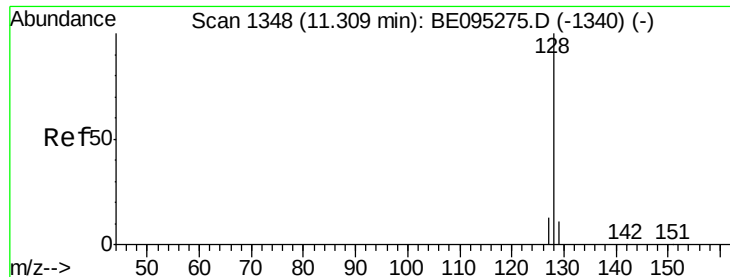

#3

Naphthalene

Concen: 0.038 ng/ul

RT: 11.31 min Scan# 1348

Delta R.T. -0.00 min

Lab File: BE095287.D

Acq: 30 Jan 2018 16:03

Instrument :

BNA_E

ClientSampleId :


Tot Ion:128 Resp: 744

Ion Ratio Lower Upper

128 100

129 24.2 11.3 16.9#




127 21.9 4.0 6.0#

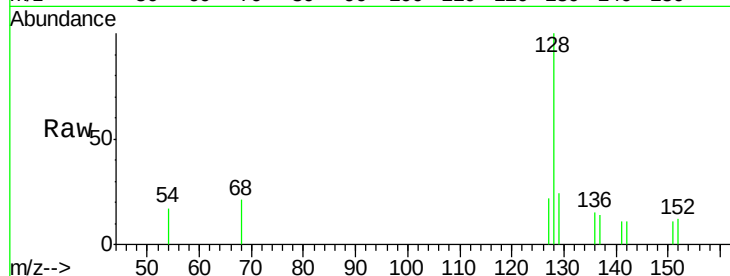

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

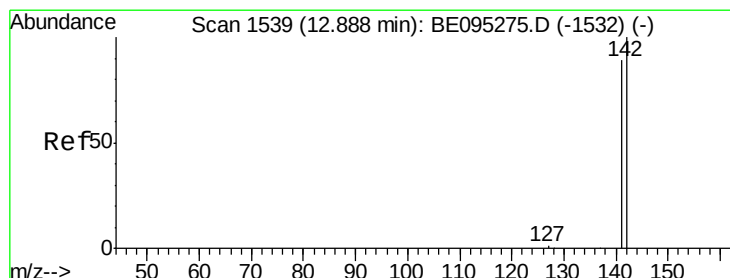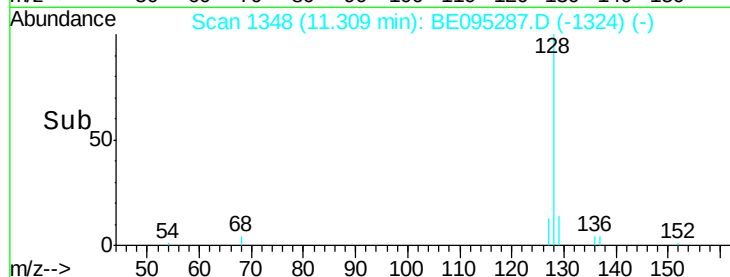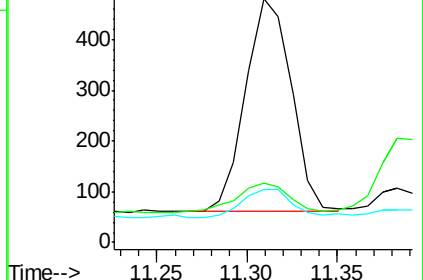

#5

2-Methylnaphthalene

Concen: 0.049 ng/ul

RT: 12.89 min Scan# 1539

Delta R.T. -0.00 min

Lab File: BE095287.D


Acq: 30 Jan 2018 16:03

Tgt Ion:142 Resp: 637

Ion Ratio Lower Upper



142 100


141 89.3 72.6 108.8

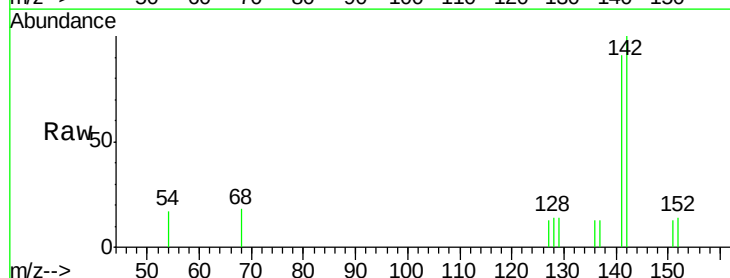

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

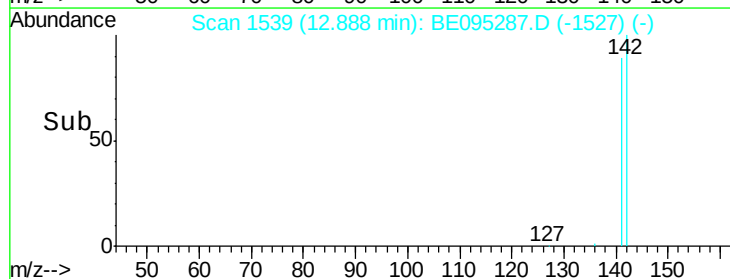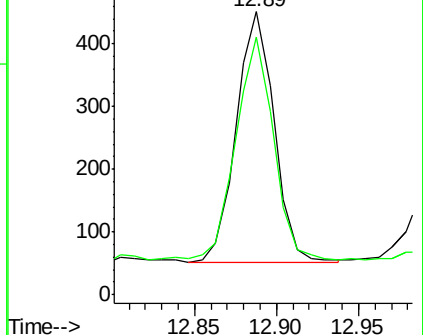

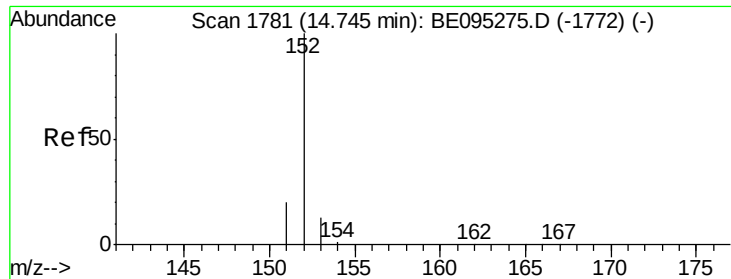

#7

Acenaphthylene

Concen: 0.951 ng/ul

RT: 14.75 min Scan# 1781

Delta R.T. 0.00 min

Lab File: BE095287.D

Acq: 30 Jan 2018 16:03

Instrument :

BNA_E

ClientSampleId :


Tot Ion:152 Resp: 19605

Ion Ratio Lower Upper

152 100

151 21.9 17.1 25.7




153 13.8 12.8 19.2

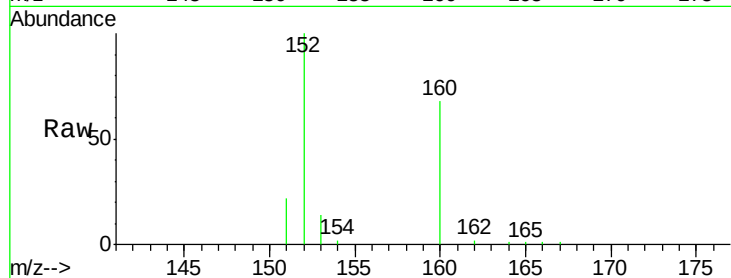

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

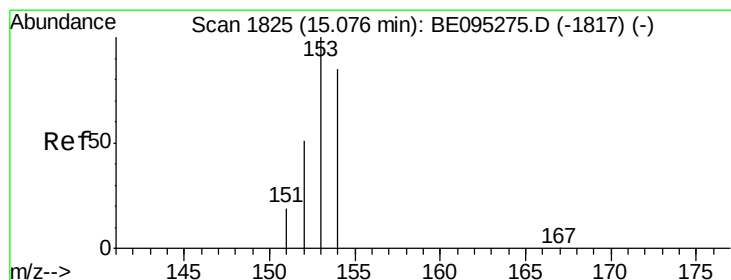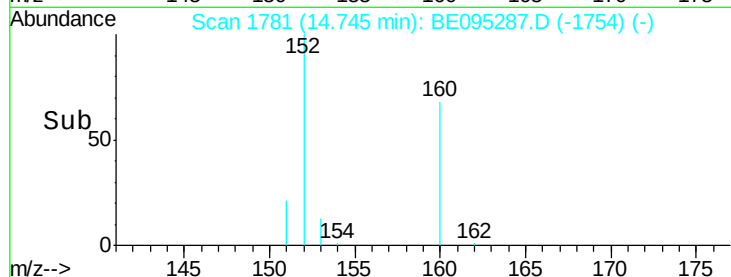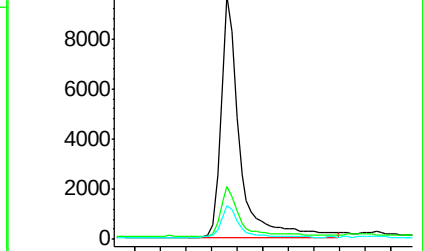

#8

Acenaphthene

Concen: 0.059 ng/ul

RT: 15.08 min Scan# 1825

Delta R.T. 0.00 min

Lab File: BE095287.D

Acq: 30 Jan 2018 16:03


Tgt Ion:153 Resp: 949

Ion Ratio Lower Upper

153 100

152 70.4 36.0 54.0#



154 86.0 72.0 108.0

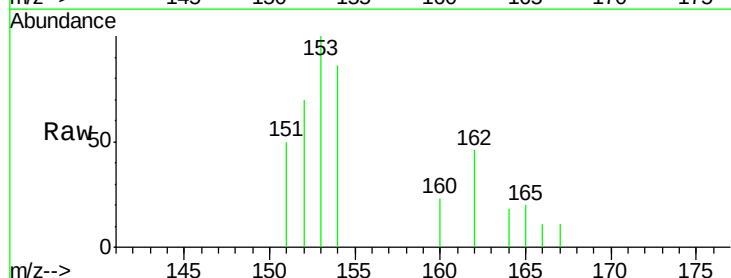


Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E



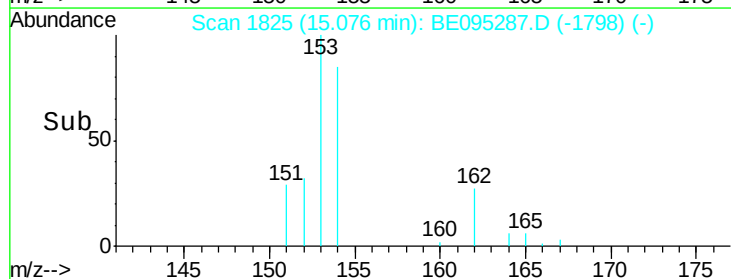
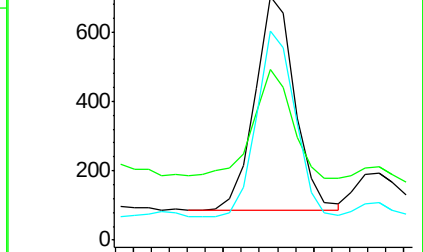


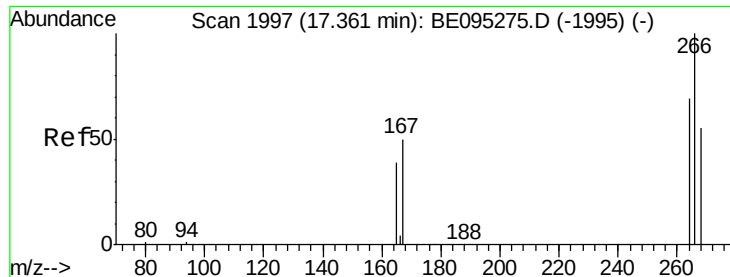

#11
 Pentachlorophenol
 Concen: 116.015 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. 0.00 min
 Lab File: BE095287.D
 Acq: 30 Jan 2018 16:03




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:266 Resp: 193608
 Ion Ratio Lower Upper
 266 100
 264 65.7 47.9 71.9
 268 62.0 49.8 74.8

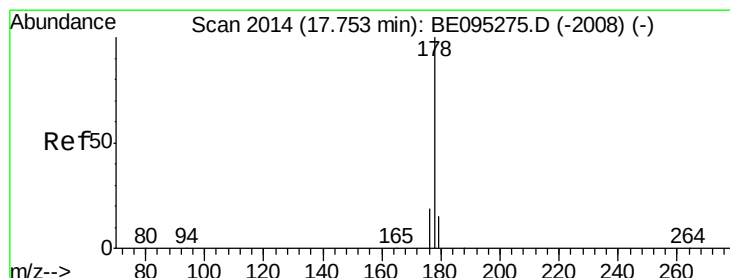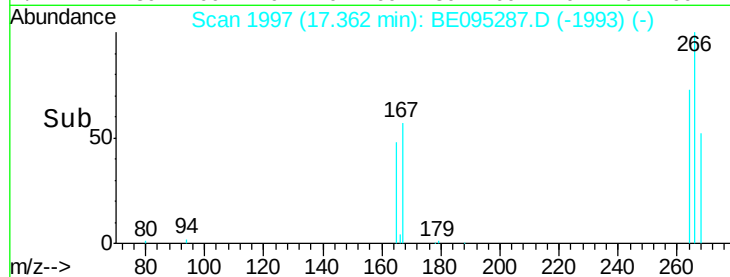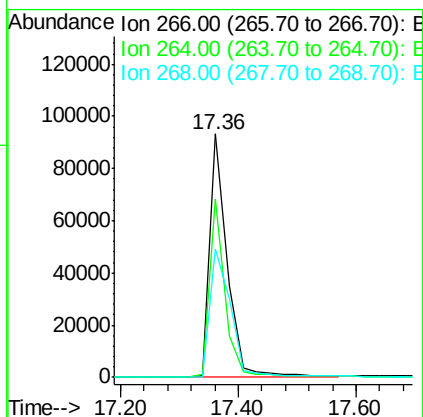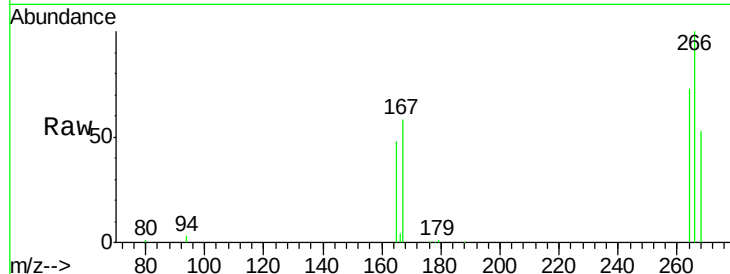

#12
 Phenanthrene
 Concen: 0.615 ng/ul
 RT: 17.75 min Scan# 2014
 Delta R.T. 0.00 min
 Lab File: BE095287.D
 Acq: 30 Jan 2018 16:03

Tgt Ion:178 Resp: 17813
 Ion Ratio Lower Upper
 178 100
 179 17.8 18.4 27.6#
 176 22.5 13.6 20.4#

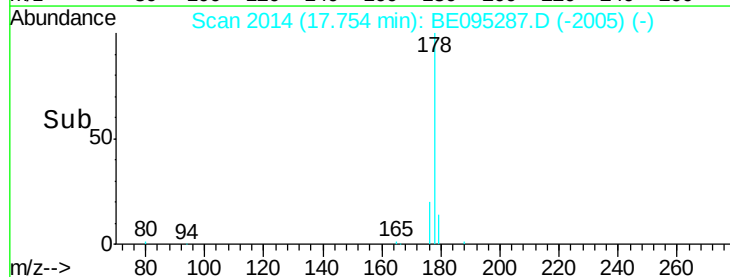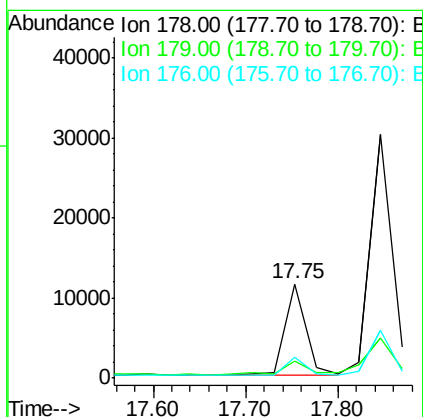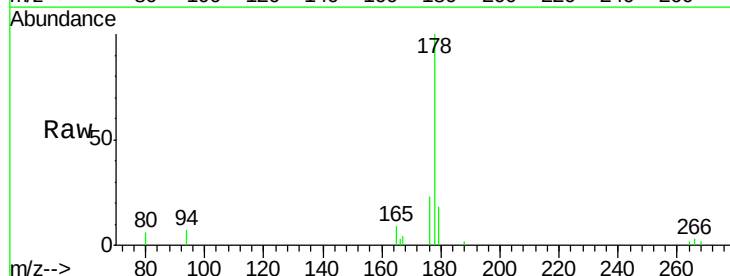

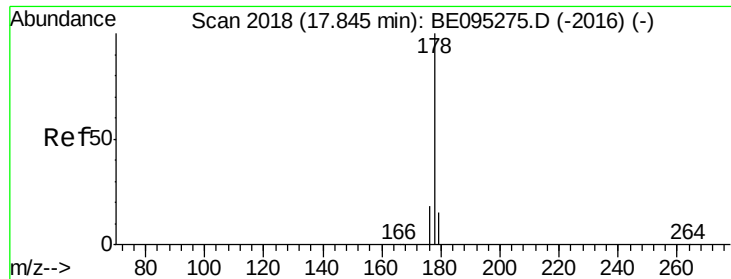

#13

Anthracene

Concen: 1.882 ng/ul

RT: 17.85 min Scan# 2018

Delta R.T. 0.00 min

Lab File: BE095287.D

Acq: 30 Jan 2018 16:03

Instrument :

BNA_E

ClientSampleId :





Tot Ion:178 Resp: 49910

Ion Ratio Lower Upper

178 100

179 16.5 18.1 27.1#

176 19.6 14.7 22.1

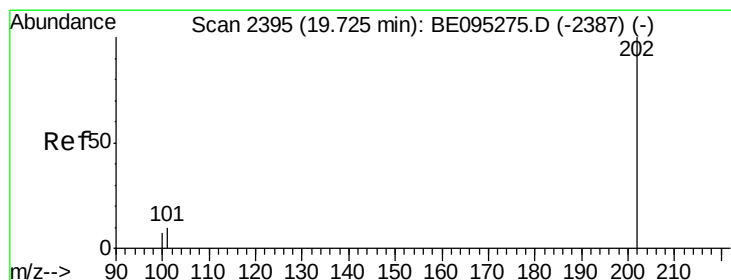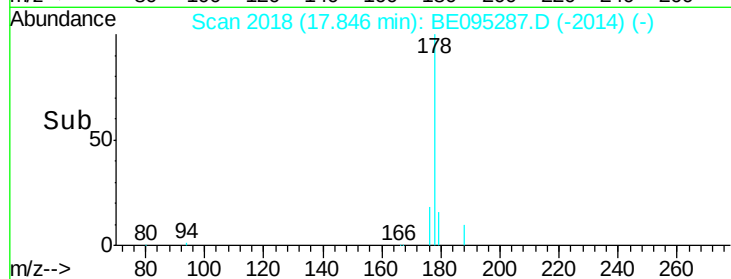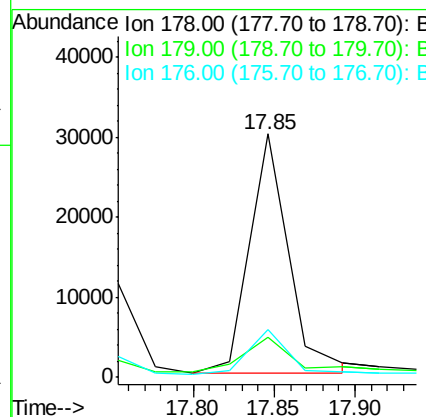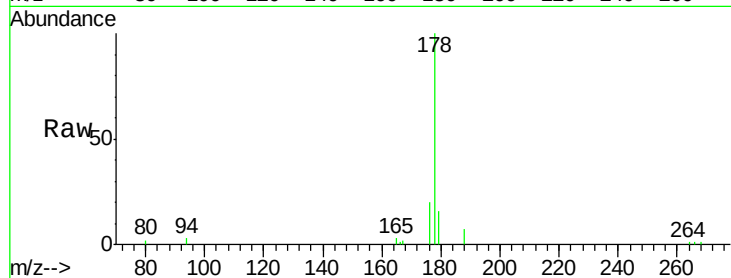

#15

Fluoranthene

Concen: 15.331 ng/ul

RT: 19.73 min Scan# 2396

Delta R.T. 0.00 min

Lab File: BE095287.D

Acq: 30 Jan 2018 16:03




Tgt Ion:202 Resp: 575244


Ion Ratio Lower Upper

202 100

101 9.0 0.0 30.3

100 7.2 0.0 39.5

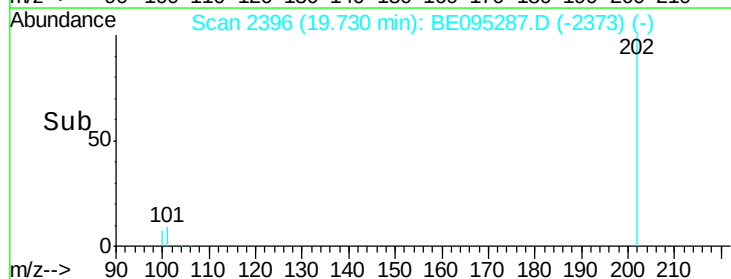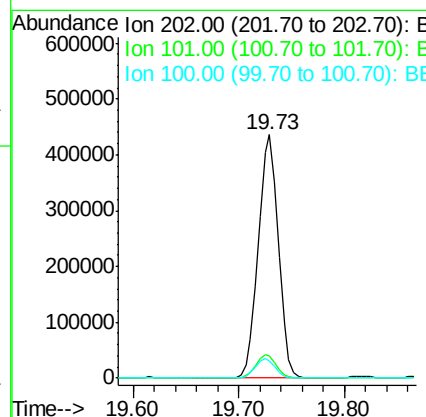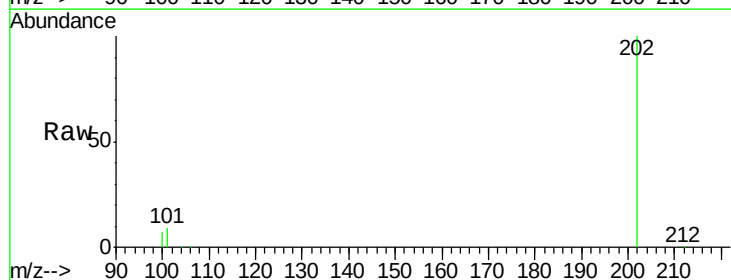

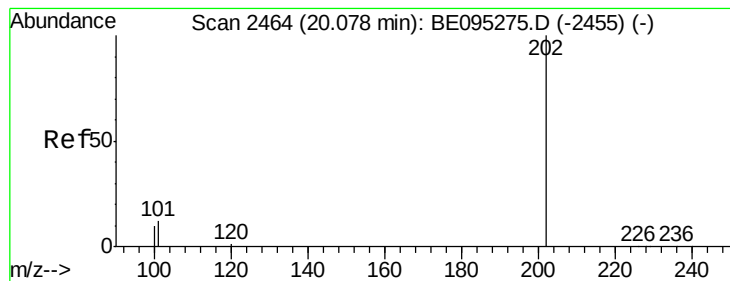

#17

Pvrene

Concen: 19.155 ng/ul

RT: 20.08 min Scan# 2465

Delta R.T. 0.01 min

Lab File: BE095287.D

Acq: 30 Jan 2018 16:03

Instrument :

BNA_E

ClientSampleId :


Tot Ion:202 Resp: 613114

Ion Ratio Lower Upper

202 100

101 10.4 18.2 27.4#




100 8.9 15.6 23.4#

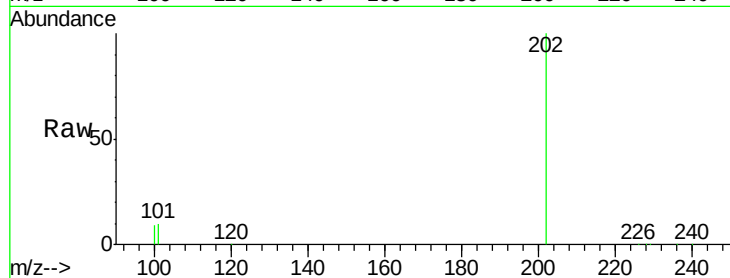

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

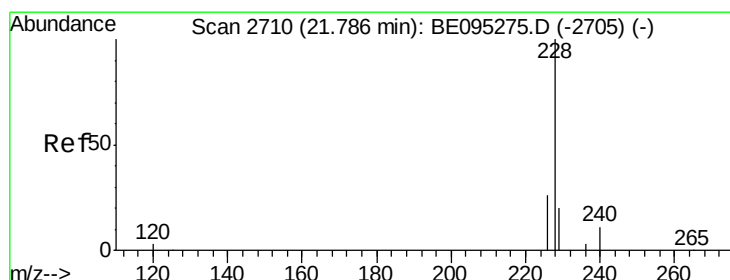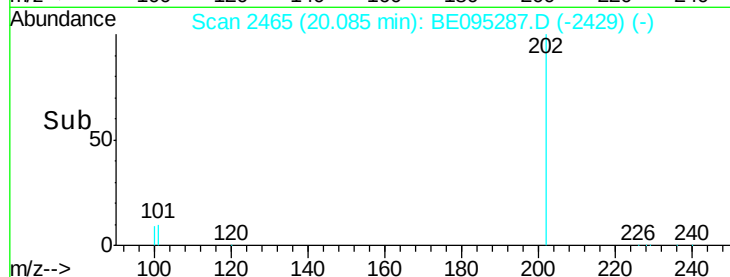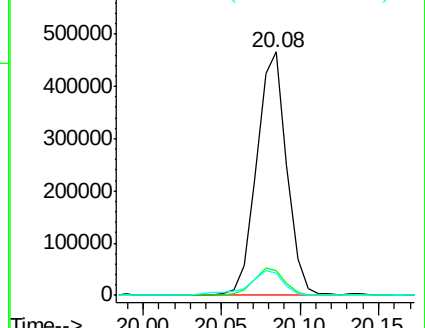

#18

Benzo(a)anthracene

Concen: 3.941 ng/ul

RT: 21.79 min Scan# 2710

Delta R.T. 0.00 min

Lab File: BE095287.D

Acq: 30 Jan 2018 16:03


Tgt Ion:228 Resp: 117547

Ion Ratio Lower Upper

228 100

229 23.5 22.8 34.2



226 30.7 17.0 25.6#

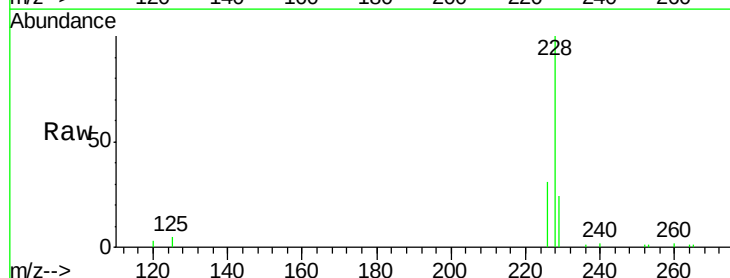


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

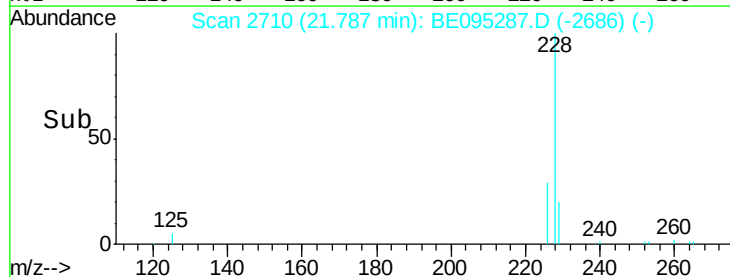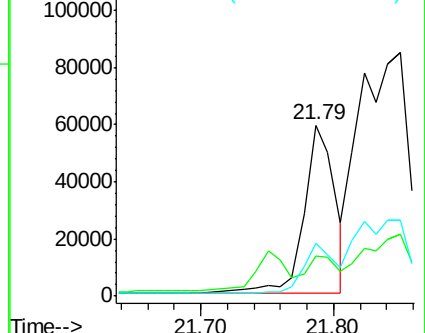

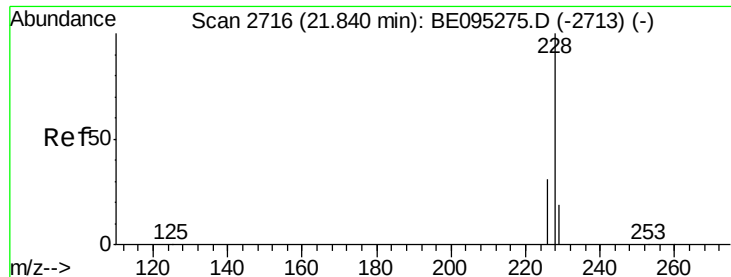

#19

Chrysene

Concen: 7.073 ng/ul

RT: 21.85 min Scan# 2717

Delta R.T. 0.01 min

Lab File: BE095287.D

Acq: 30 Jan 2018 16:03

Instrument :

BNA_E

ClientSampleId :


Tot Ion:228 Resp: 219055

Ion Ratio Lower Upper




228 100

226 31.0 23.4 35.0

229 25.5 17.7 26.5

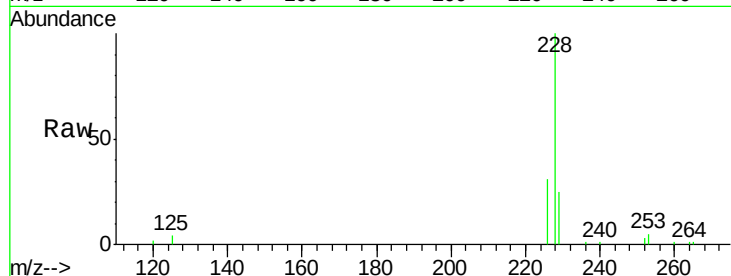

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

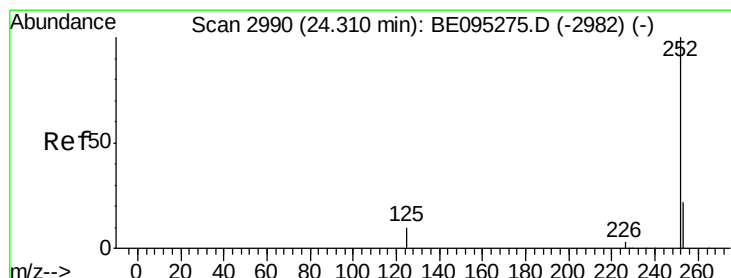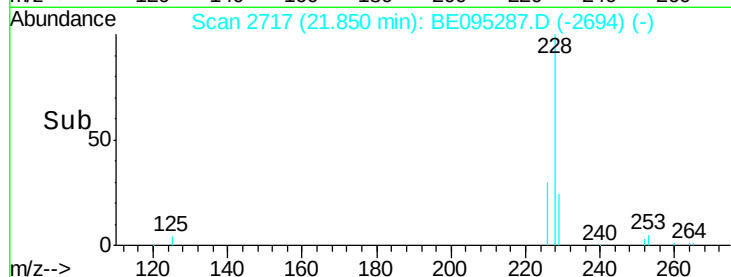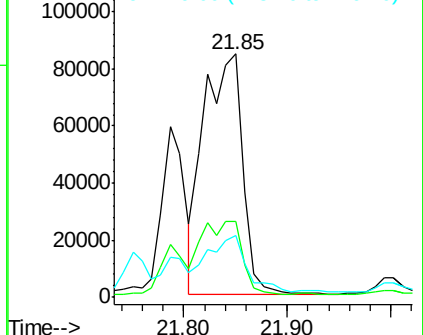

#23

Benzo(a)pyrene

Concen: 0.180 ng/ul

RT: 24.21 min Scan# 2979

Delta R.T. -0.10 min

Lab File: BE095287.D

Acq: 30 Jan 2018 16:03


Tgt Ion:252 Resp: 197666

Ion Ratio Lower Upper

252 100

253 23.3 28.5 42.7#

125 15.2 18.1 27.1#

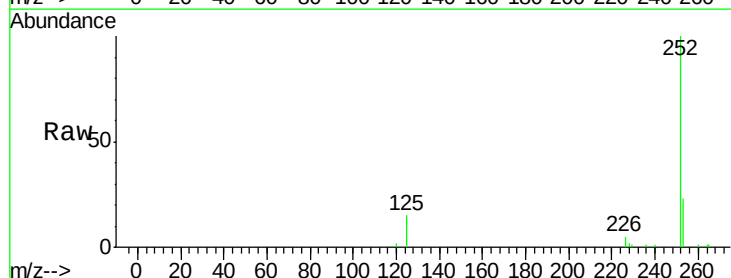

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

