

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013018\
 Data File : BE095291.D
 Acq On : 30 Jan 2018 18:26
 Operator : SJ/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Jan 31 01:27:03 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 31 01:22:09 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2372	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	7272	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	4273	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8822	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	9902	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	9389	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	4978	0.42	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	13005	0.39	ng/ul	0.00
Target Compounds				Ovalue		
3) Naphthalene	11.31	128	8086	0.397	ng/ul#	89
5) 2-Methylnaphthalene	12.89	142	5764	0.424	ng/ul	100
7) Acenaphthylene	14.74	152	8786	0.427	ng/ul	96
8) Acenaphthene	15.08	153	6439	0.404	ng/ul	94
9) Fluorene	16.03	166	6826	0.415	ng/ul#	76
11) Pentachlorophenol	17.36	266	845	0.495	ng/ul	95
12) Phenanthrene	17.75	178	12468	0.420	ng/ul#	88
13) Anthracene	17.85	178	12090	0.445	ng/ul#	92
15) Fluoranthene	19.73	202	14427	0.376	ng/ul	83
17) Pyrene	20.08	202	16830	0.507	ng/ul#	79
18) Benzo(a)anthracene	21.79	228	13495	0.436	ng/ul#	86
19) Chrysene	21.84	228	12786	0.398	ng/ul	96
21) Benzo(b)fluoranthene	23.62	252	12450	0.376	ng/ul	87
22) Benzo(k)fluoranthene	23.67	252	12280	0.405	ng/ul#	88
23) Benzo(a)pyrene	24.32	252	11935	0.404	ng/ul#	80
24) Indeno(1,2,3-cd)pyrene	27.24	276	13474	0.415	ng/ul#	78
25) Dibenzo(a,h)anthracene	27.27	278	10917	0.411	ng/ul#	90
26) Benzo(g,h,i)perylene	28.12	276	11264	0.410	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013018\
Data File : BE095291.D
Acq On : 30 Jan 2018 18:26
Operator : SJ/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Jan 31 01:27:03 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 01:22:09 2018
Response via : Initial Calibration

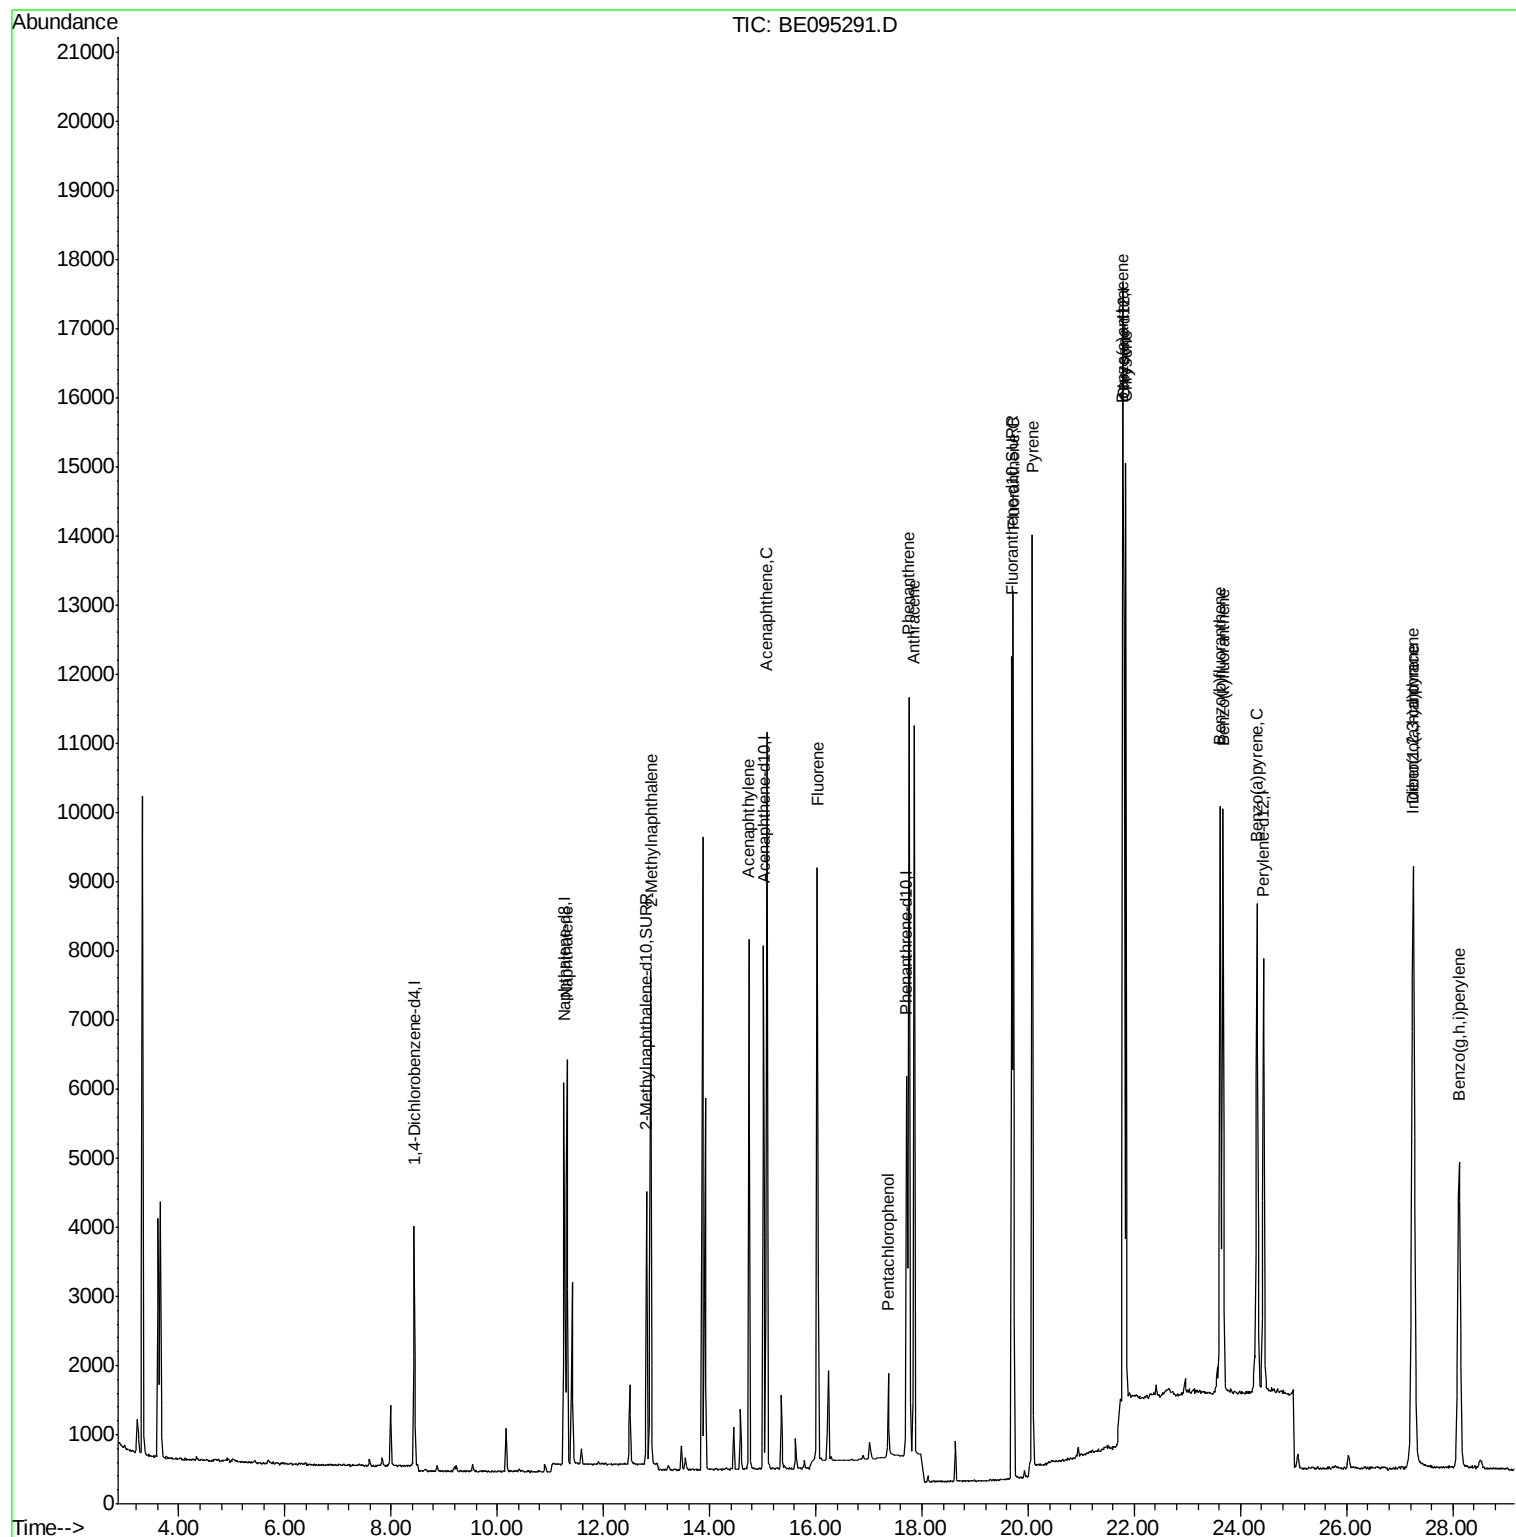



#3

Naphthalene

Concen: 0.397 ng/ul

RT: 11.31 min Scan# 1349

Delta R.T. 0.00 min

Lab File: BE095291.D

Acq: 30 Jan 2018 18:26

Instrument :

BNA_E

ClientSampleId :


Tot Ion:128 Resp: 8086

Ion Ratio Lower Upper

128 100

129 11.8 11.3 16.9




127 13.7 4.0 6.0#



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

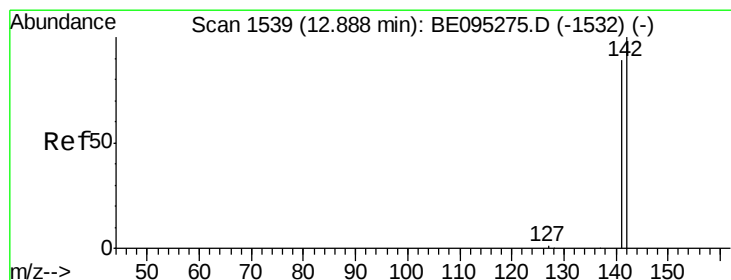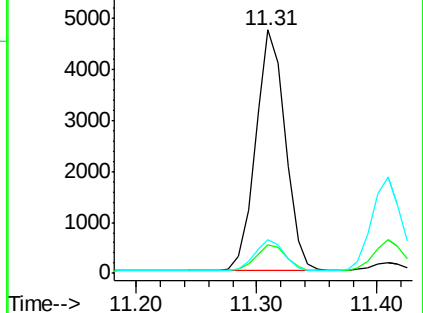

#5

2-Methylnaphthalene

Concen: 0.424 ng/ul

RT: 12.89 min Scan# 1540

Delta R.T. 0.00 min

Lab File: BE095291.D


Acq: 30 Jan 2018 18:26

Tgt Ion:142 Resp: 5764

Ion Ratio Lower Upper



142 100


141 90.5 72.6 108.8

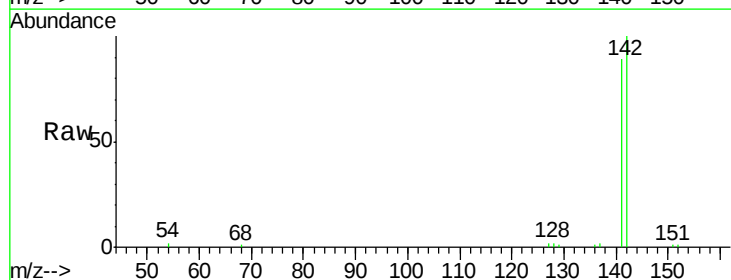

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

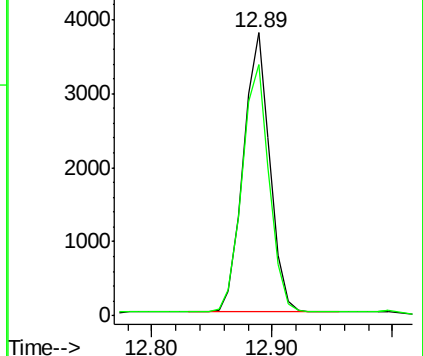



#7

Acenaphthylene

Concen: 0.427 ng/ul

RT: 14.74 min Scan# 1782

Delta R.T. 0.00 min

Lab File: BE095291.D

Acq: 30 Jan 2018 18:26

Instrument :

BNA_E

ClientSampleId :


Tot Ion:152 Resp: 8786

Ion Ratio Lower Upper




152 100

151 19.7 17.1 25.7

153 14.0 12.8 19.2



Abundance Ion 152.00 (151.70 to 152.70): E
Ion 151.00 (150.70 to 151.70): E
Ion 153.00 (152.70 to 153.70): E

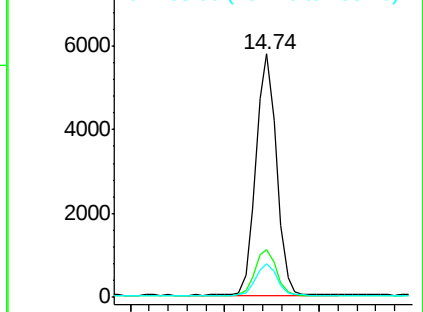

#8

Acenaphthene

Concen: 0.404 ng/ul

RT: 15.08 min Scan# 1826

Delta R.T. 0.00 min

Lab File: BE095291.D

Acq: 30 Jan 2018 18:26


Tgt Ion:153 Resp: 6439

Ion Ratio Lower Upper



153 100


152 49.4 36.0 54.0

154 84.5 72.0 108.0



Abundance Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E
Ion 154.00 (153.70 to 154.70): E

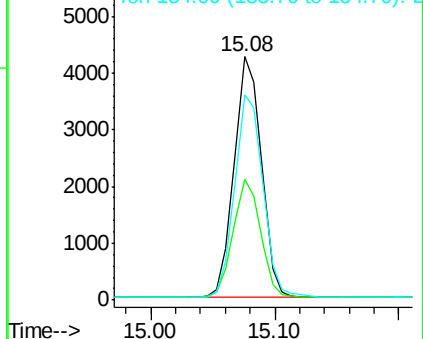

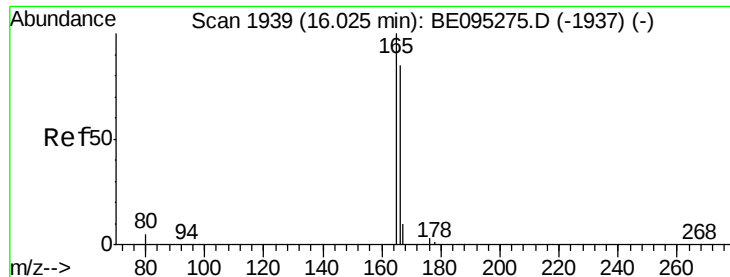

#9

Fluorene

Concen: 0.415 ng/ul

RT: 16.03 min Scan# 1940

Delta R.T. 0.00 min

Lab File: BE095291.D

Acq: 30 Jan 2018 18:26

Instrument :

BNA_E

ClientSampleId :


Tot Ion:166 Resp: 6826

Ion Ratio Lower Upper

166 100

165 116.4 73.4 110.2#




167 12.5 14.6 22.0#

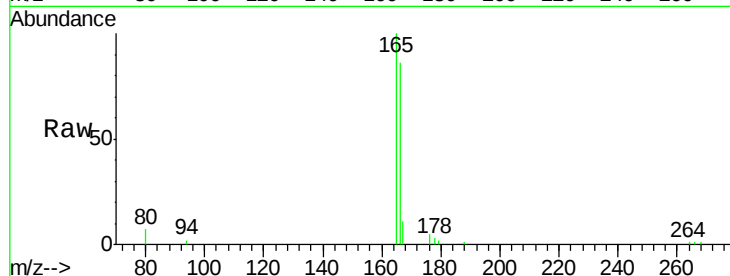

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

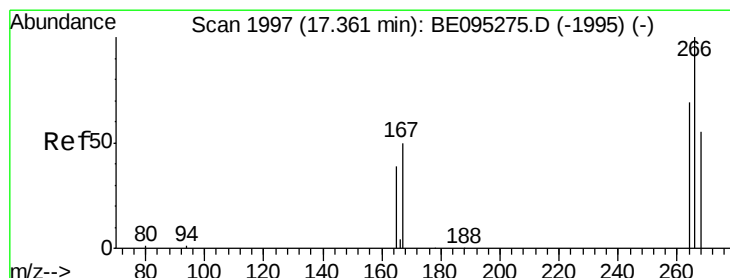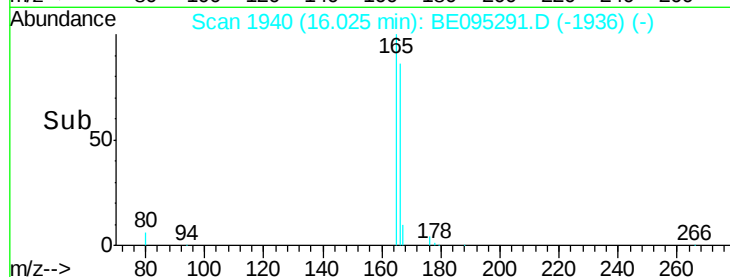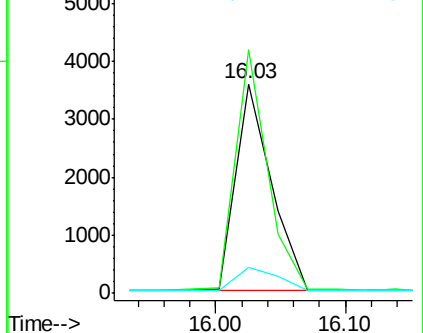

#11

Pentachlorophenol

Concen: 0.495 ng/ul

RT: 17.36 min Scan# 1998

Delta R.T. 0.00 min

Lab File: BE095291.D

Acq: 30 Jan 2018 18:26


Tgt Ion:266 Resp: 845

Ion Ratio Lower Upper

266 100

264 63.8 47.9 71.9



268 59.2 49.8 74.8

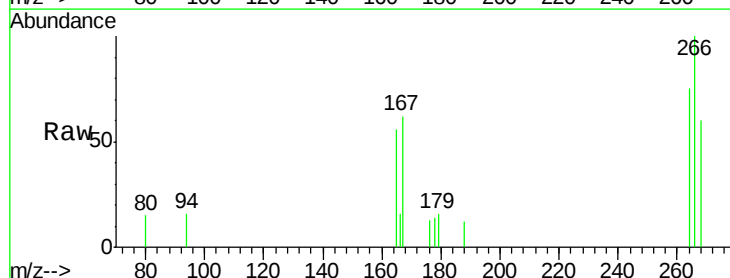


Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

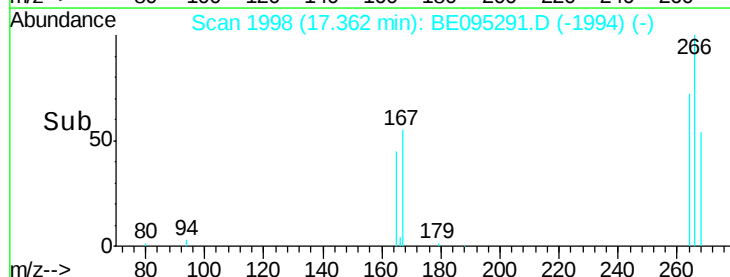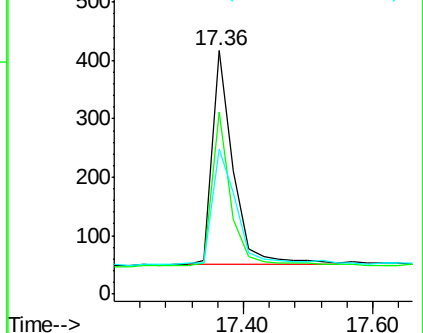



#12

Phenanthrene

Concen: 0.420 ng/ul

RT: 17.75 min Scan# 2015

Delta R.T. 0.00 min

Lab File: BE095291.D

Acq: 30 Jan 2018 18:26

Instrument :

BNA_E

ClientSampleId :


Tot Ion:178 Resp: 12468

Ion Ratio Lower Upper




178 100

179 15.2 18.4 27.6#

176 20.1 13.6 20.4



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

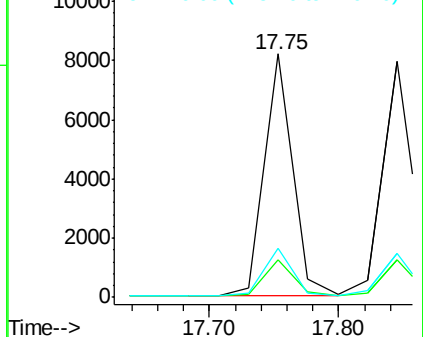

#13

Anthracene

Concen: 0.445 ng/ul

RT: 17.85 min Scan# 2019

Delta R.T. 0.00 min

Lab File: BE095291.D

Acq: 30 Jan 2018 18:26


Tgt Ion:178 Resp: 12090

Ion Ratio Lower Upper



178 100


179 16.0 18.1 27.1#

176 18.5 14.7 22.1



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

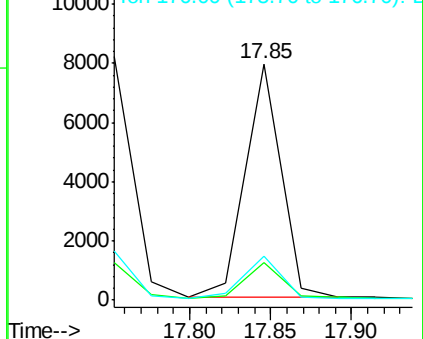



#15

Fluoranthene

Concen: 0.376 ng/ul

RT: 19.73 min Scan# 2397

Delta R.T. 0.00 min

Lab File: BE095291.D

Acq: 30 Jan 2018 18:26

Instrument :

BNA_E

ClientSampleId :


Tot Ion:202 Resp: 14427

Ion Ratio Lower Upper

202 100

101 9.6 0.0 30.3




100 7.8 0.0 39.5



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BE

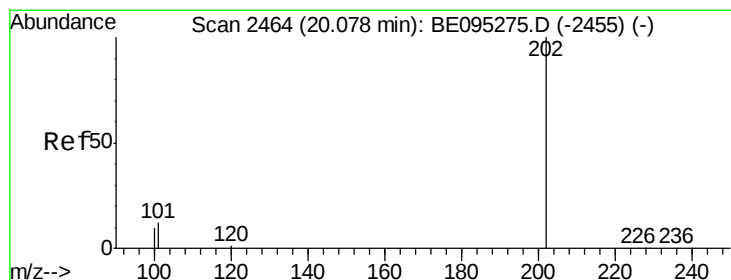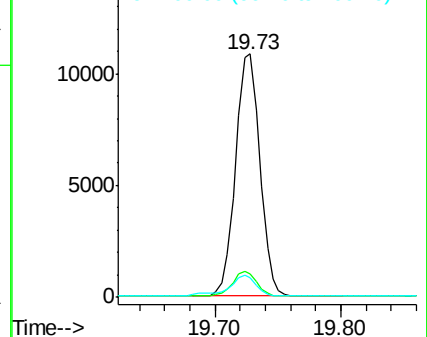

#17

Pyrene

Concen: 0.507 ng/ul

RT: 20.08 min Scan# 2465

Delta R.T. 0.00 min

Lab File: BE095291.D

Acq: 30 Jan 2018 18:26


Tgt Ion:202 Resp: 16830

Ion Ratio Lower Upper

202 100

101 12.2 18.2 27.4#



100 10.2 15.6 23.4#

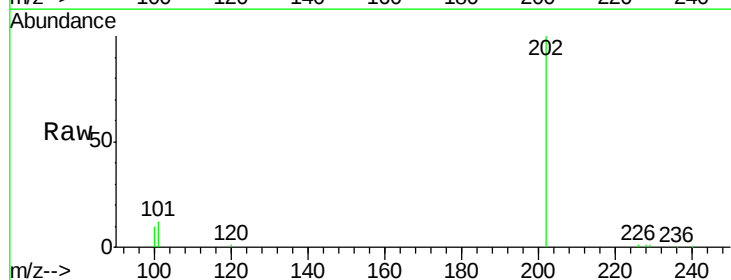


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BE

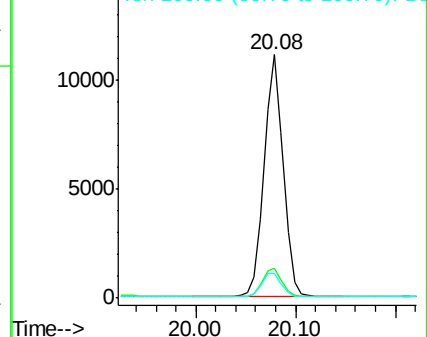



#18

Benzo(a)anthracene

Concen: 0.436 ng/ul

RT: 21.79 min Scan# 2711

Delta R.T. 0.00 min

Lab File: BE095291.D

Acq: 30 Jan 2018 18:26

Instrument :

BNA_E

ClientSampleId :


Tot Ion:228 Resp: 13495

Ion Ratio Lower Upper

228 100

229 20.6 22.8 34.2#




226 27.6 17.0 25.6#

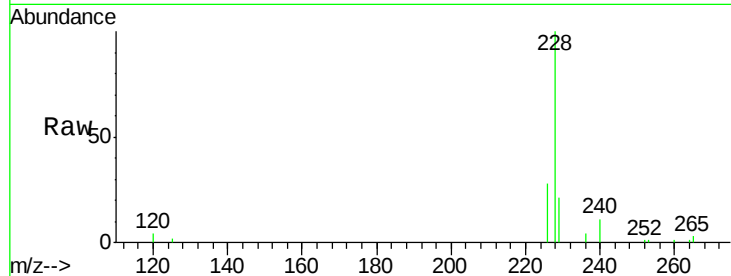

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

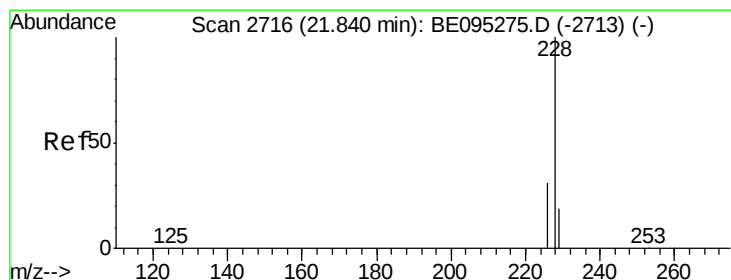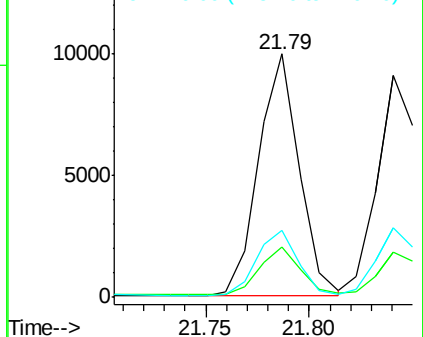

#19

Chrysene

Concen: 0.398 ng/ul

RT: 21.84 min Scan# 2717

Delta R.T. 0.00 min

Lab File: BE095291.D

Acq: 30 Jan 2018 18:26


Tgt Ion:228 Resp: 12786

Ion Ratio Lower Upper

228 100

226 31.1 23.4 35.0



229 20.1 17.7 26.5




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E




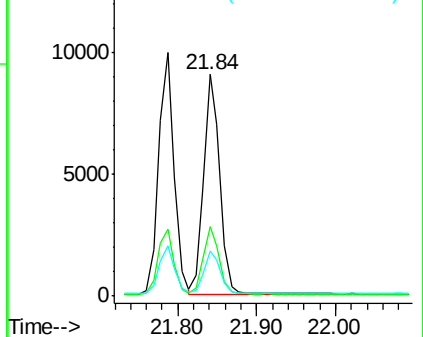




#21
Benzo(b)fluoranthene
Concen: 0.376 ng/ul
RT: 23.62 min Scan# 2914
Delta R.T. 0.00 min
Lab File: BE095291.D
Acq: 30 Jan 2018 18:26




Instrument :
BNA_E
ClientSampleId :


Tot Ion:252 Resp: 12450
Ion Ratio Lower Upper
252 100
253 23.5 0.0 64.2
125 13.3 0.0 35.0

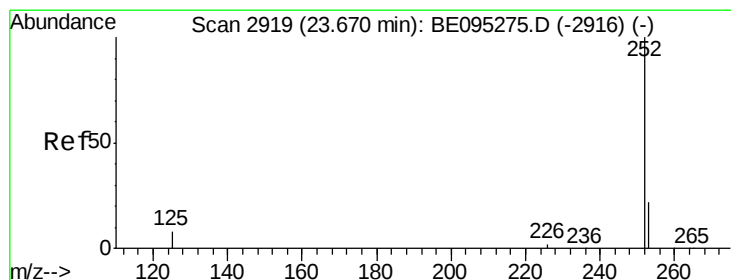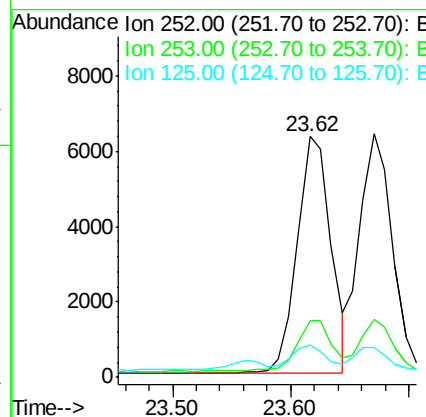

#22
Benzo(k)fluoranthene
Concen: 0.405 ng/ul
RT: 23.67 min Scan# 2920
Delta R.T. 0.00 min
Lab File: BE095291.D
Acq: 30 Jan 2018 18:26

Tgt Ion:252 Resp: 12280
Ion Ratio Lower Upper
252 100
253 23.8 24.5 36.7#
125 12.3 13.7 20.5#

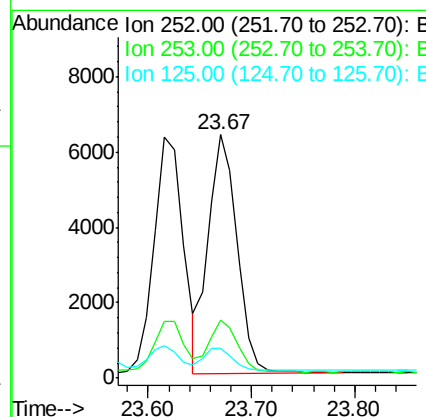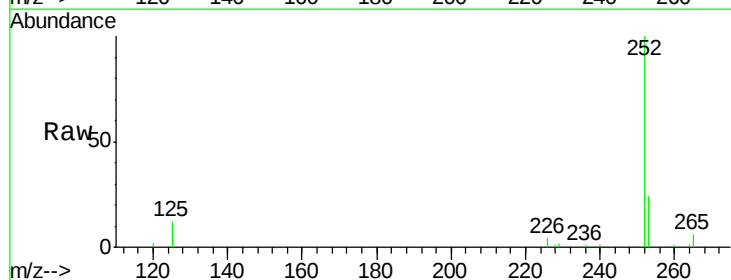



#23

Benzo(a)pyrene

Concen: 0.404 ng/ul

RT: 24.32 min Scan# 2992

Delta R.T. 0.01 min

Lab File: BE095291.D

Acq: 30 Jan 2018 18:26

Instrument :

BNA_E

ClientSampleId :


Tot Ion:252 Resp: 11935

Ion Ratio Lower Upper

252 100

253 23.1 28.5 42.7#




125 13.5 18.1 27.1#

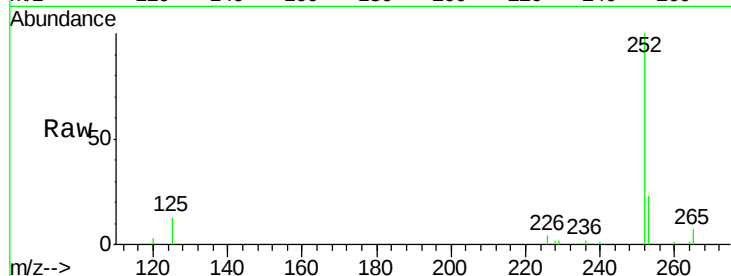

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

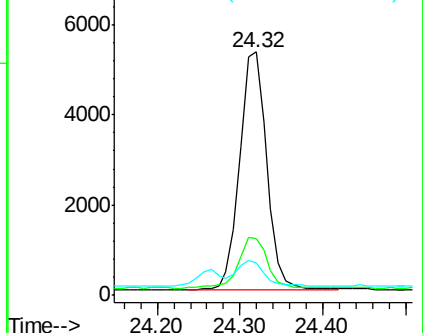

#24

Indeno(1,2,3-cd)pyrene

Concen: 0.415 ng/ul

RT: 27.24 min Scan# 3555

Delta R.T. 0.01 min

Lab File: BE095291.D

Acq: 30 Jan 2018 18:26


Tgt Ion:276 Resp: 13474

Ion Ratio Lower Upper

276 100

138 22.9 28.0 42.0#



227 0.0 8.0 12.0#




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 227.00 (226.70 to 227.70): E




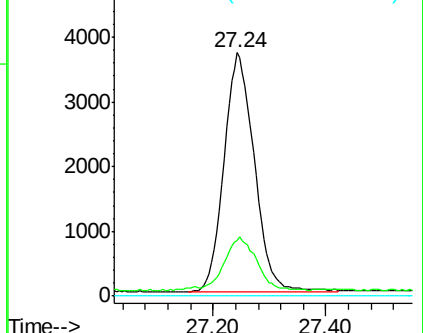




#25
Dibenzo(a,h)anthracene
Concen: 0.411 ng/ul
RT: 27.27 min Scan# 3560
Delta R.T. 0.00 min
Lab File: BE095291.D
Acq: 30 Jan 2018 18:26

Instrument :
BNA_E
ClientSampleId :

Tot Ion:278 Resp: 10917
Ion Ratio Lower Upper
278 100
139 17.9 17.4 26.0
279 25.8 25.9 38.9#

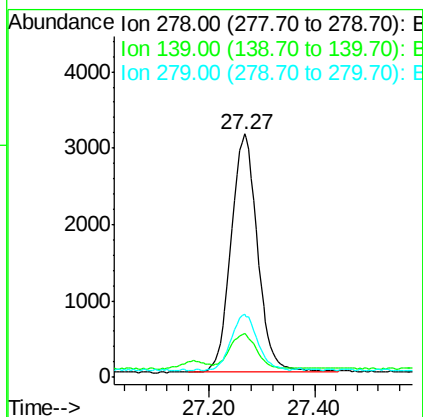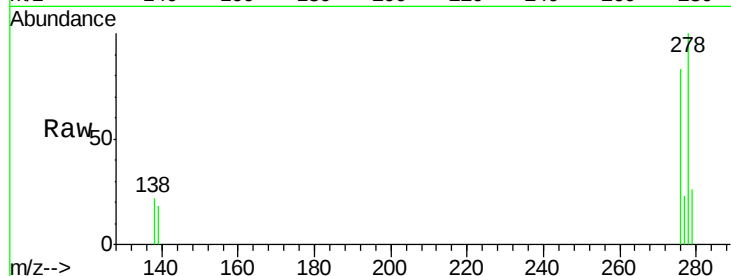

#26
Benzo(g,h,i)perylene
Concen: 0.410 ng/ul
RT: 28.12 min Scan# 3747
Delta R.T. 0.00 min
Lab File: BE095291.D
Acq: 30 Jan 2018 18:26

Tgt Ion:276 Resp: 11264
Ion Ratio Lower Upper
276 100
138 22.0 21.8 32.8
277 24.3 20.5 30.7

