


Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013018\
 Data File : BE095281.D
 Acq On : 30 Jan 2018 12:28
 Operator : SJ/JU
 Sample : J1233-17DL 5X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1




Quant Time: Jan 31 02:55:23 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 31 01:22:09 2018
 Response via : Initial Calibration

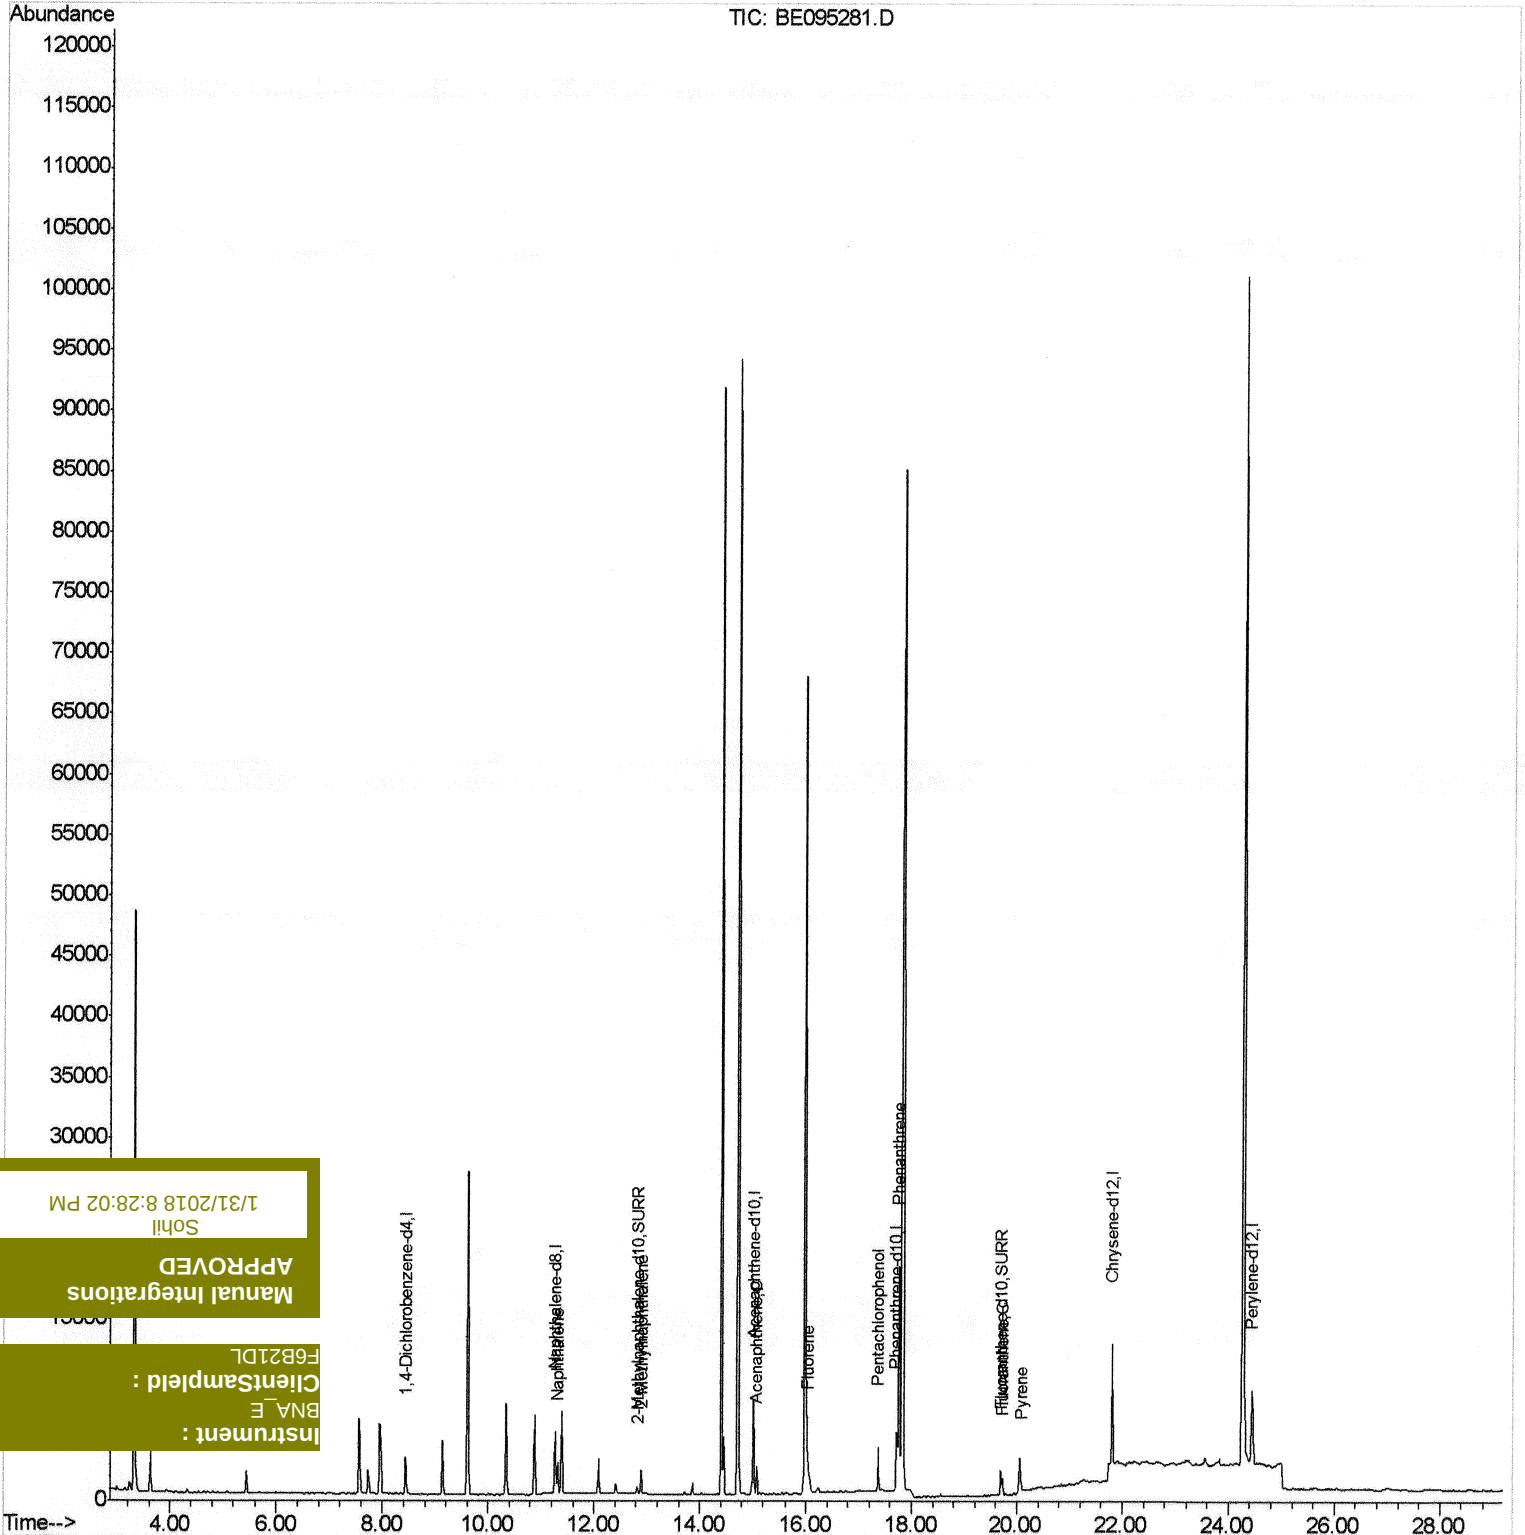

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013018\
 Data File : BE095281.D
 Acq On : 30 Jan 2018 12:28
 Operator : SJ/JU
 Sample : J1233-17DL 5X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jan 31 01:25:17 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 31 01:22:09 2018
 Response via : Initial Calibration

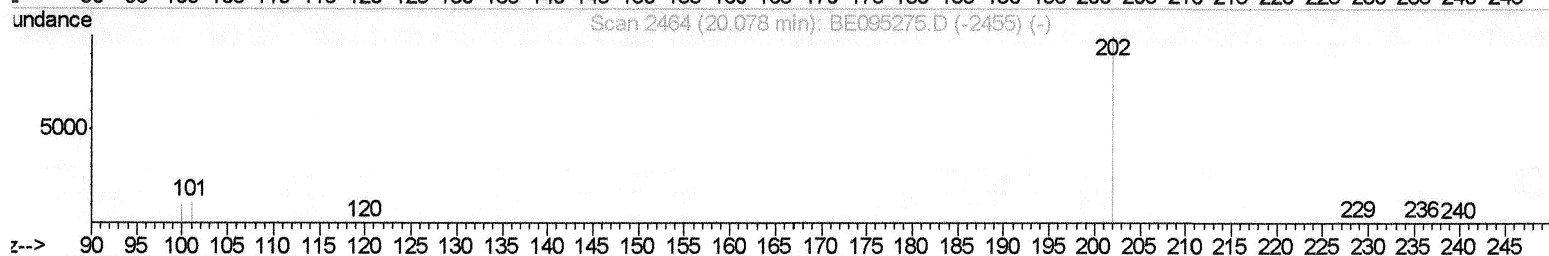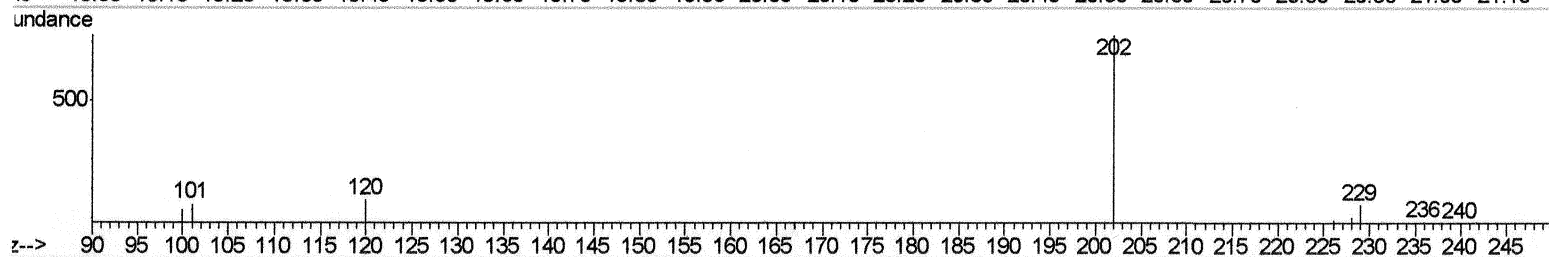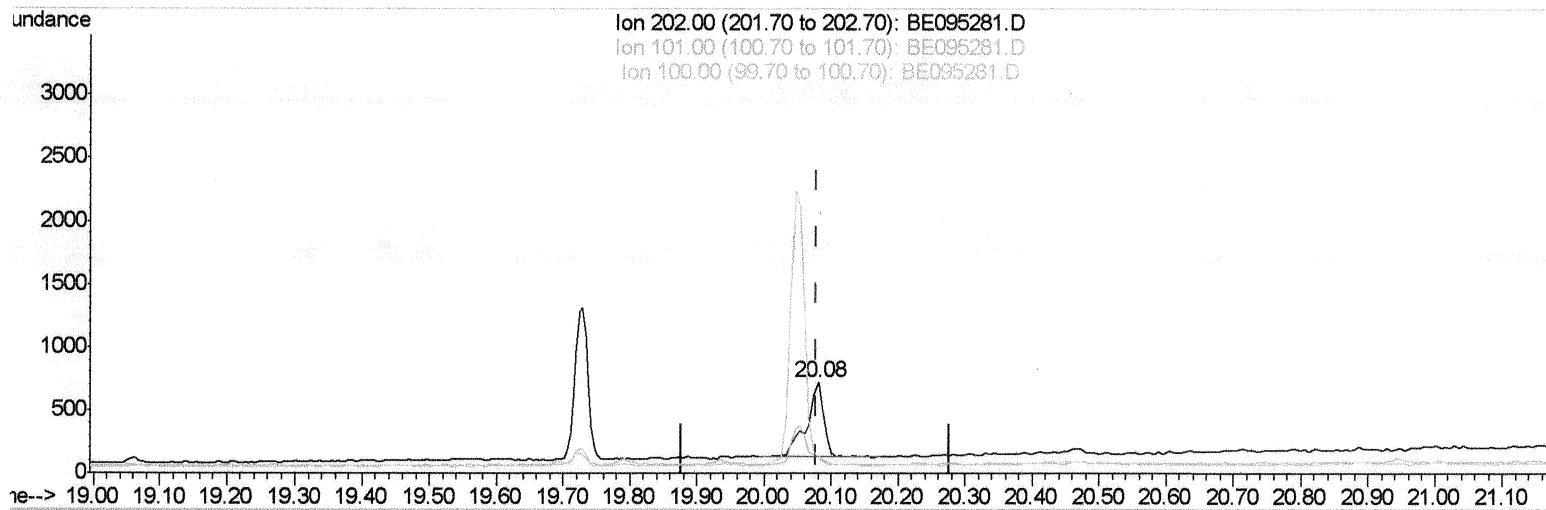

TIC: BE095281.D

(17) Pyrene

20.079min (+0.001) 0.04ng/ul

1/31/2018 8:28:02 PM
 Sohll

APPROVED
 Manual Integrations




101.00 22.80 20.42

Client Sample : F6821DL
 BNA_E
 Instrument : 4

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013018\
 Data File : BE095281.D
 Acq On : 30 Jan 2018 12:28
 Operator : SJ/JU
 Sample : J1233-17DL 5X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jan 31 01:25:17 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 31 01:22:09 2018
 Response via : Initial Calibration

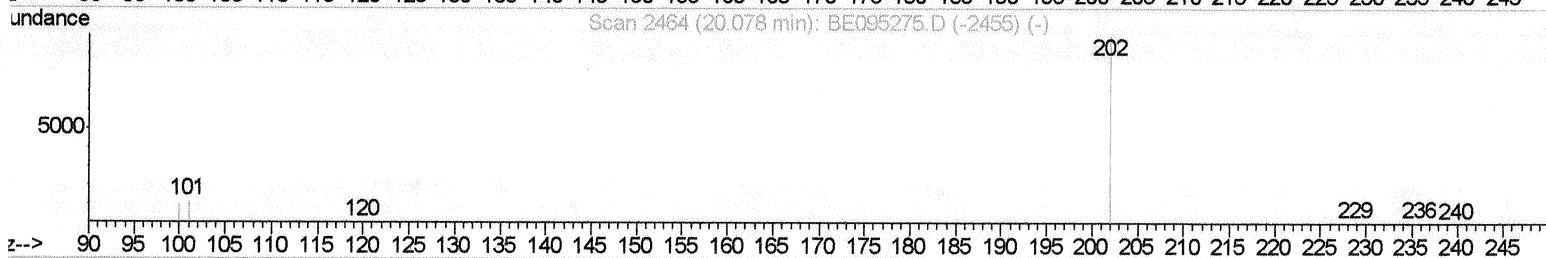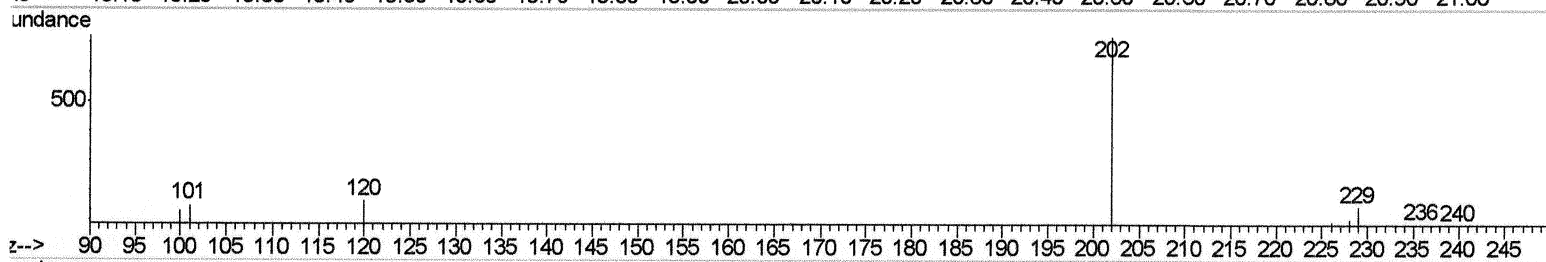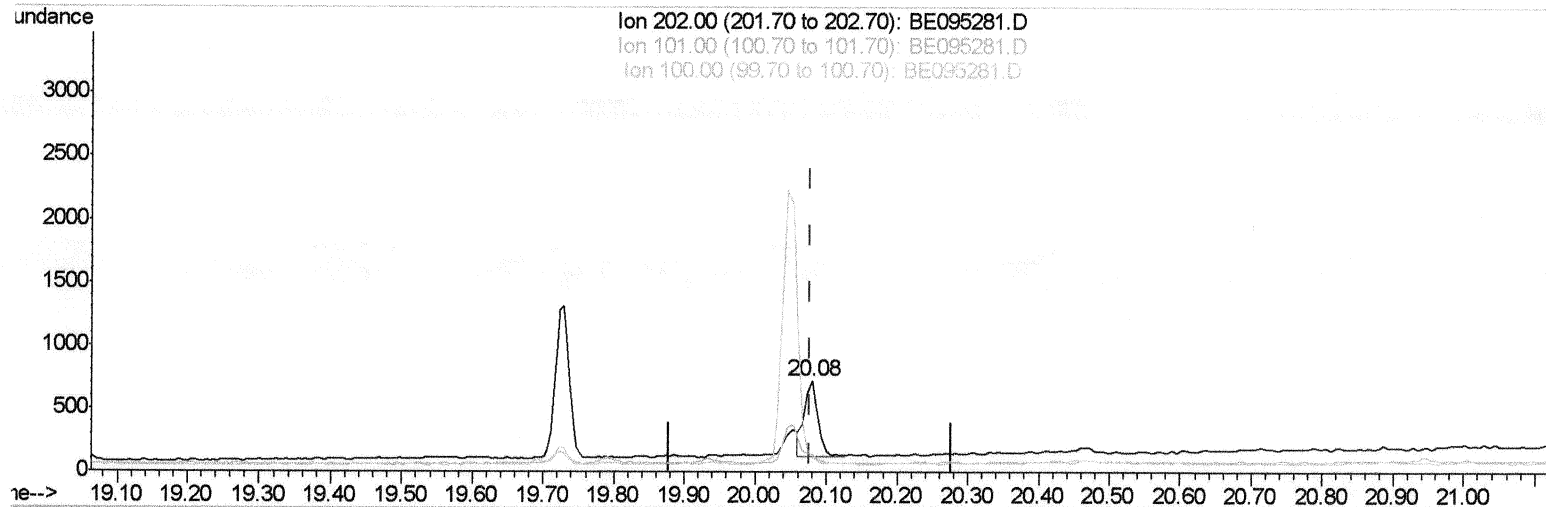

(17) Pyrene

20.079min (+0.001) 0.02ng/ul m > 50 2/1/18

1/31/2018 8:28:02 PM

Sohil

APPROVED

Manual Integrations

Client Sampled :
 BNA_E

Instrument :

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013018\
 Data File : BE095281.D
 Acq On : 30 Jan 2018 12:28
 Operator : SJ/JU
 Sample : J1233-17DL 5X
 Disc :
 ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jan 31 02:55:23 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 31 01:22:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2231	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	6805	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	4322	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8918	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	9530	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	9628	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	784	0.07	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	2197	0.06	ng/ul	0.00
Target Compounds						
3) Naphthalene	11.31	128	3531	0.185	ng/ul#	91
5) 2-Methylnaphthalene	12.89	142	1565	0.123	ng/ul	100
8) Acenaphthene	15.08	153	1341	0.083	ng/ul	93
9) Fluorene	16.02	166	3207	0.193	ng/ul#	74
11) Pentachlorophenol	17.36	266	2180	1.262	ng/ul	96
12) Phenanthrene	17.75	178	22098	0.737	ng/ul#	87
15) Fluoranthene	19.73	202	1655	0.043	ng/ul	84
17) Pyrene	20.08	202	796m)	0.025	ng/ul	

52 2/1/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed

1/31/2018 8:28:02 PM
Sohil

Manual Integrations
APPROVED

Instrument : BNA_E
Client Sampled : F6B21DL