


Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013018\
 Data File : BE095292.D
 Acq On : 31 Jan 2018 00:06
 Operator : SJ/JU
 Sample : J1233-20DL 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1




Quant Time: Jan 31 03:48:58 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 31 03:40:45 2018
 Response via : Initial Calibration

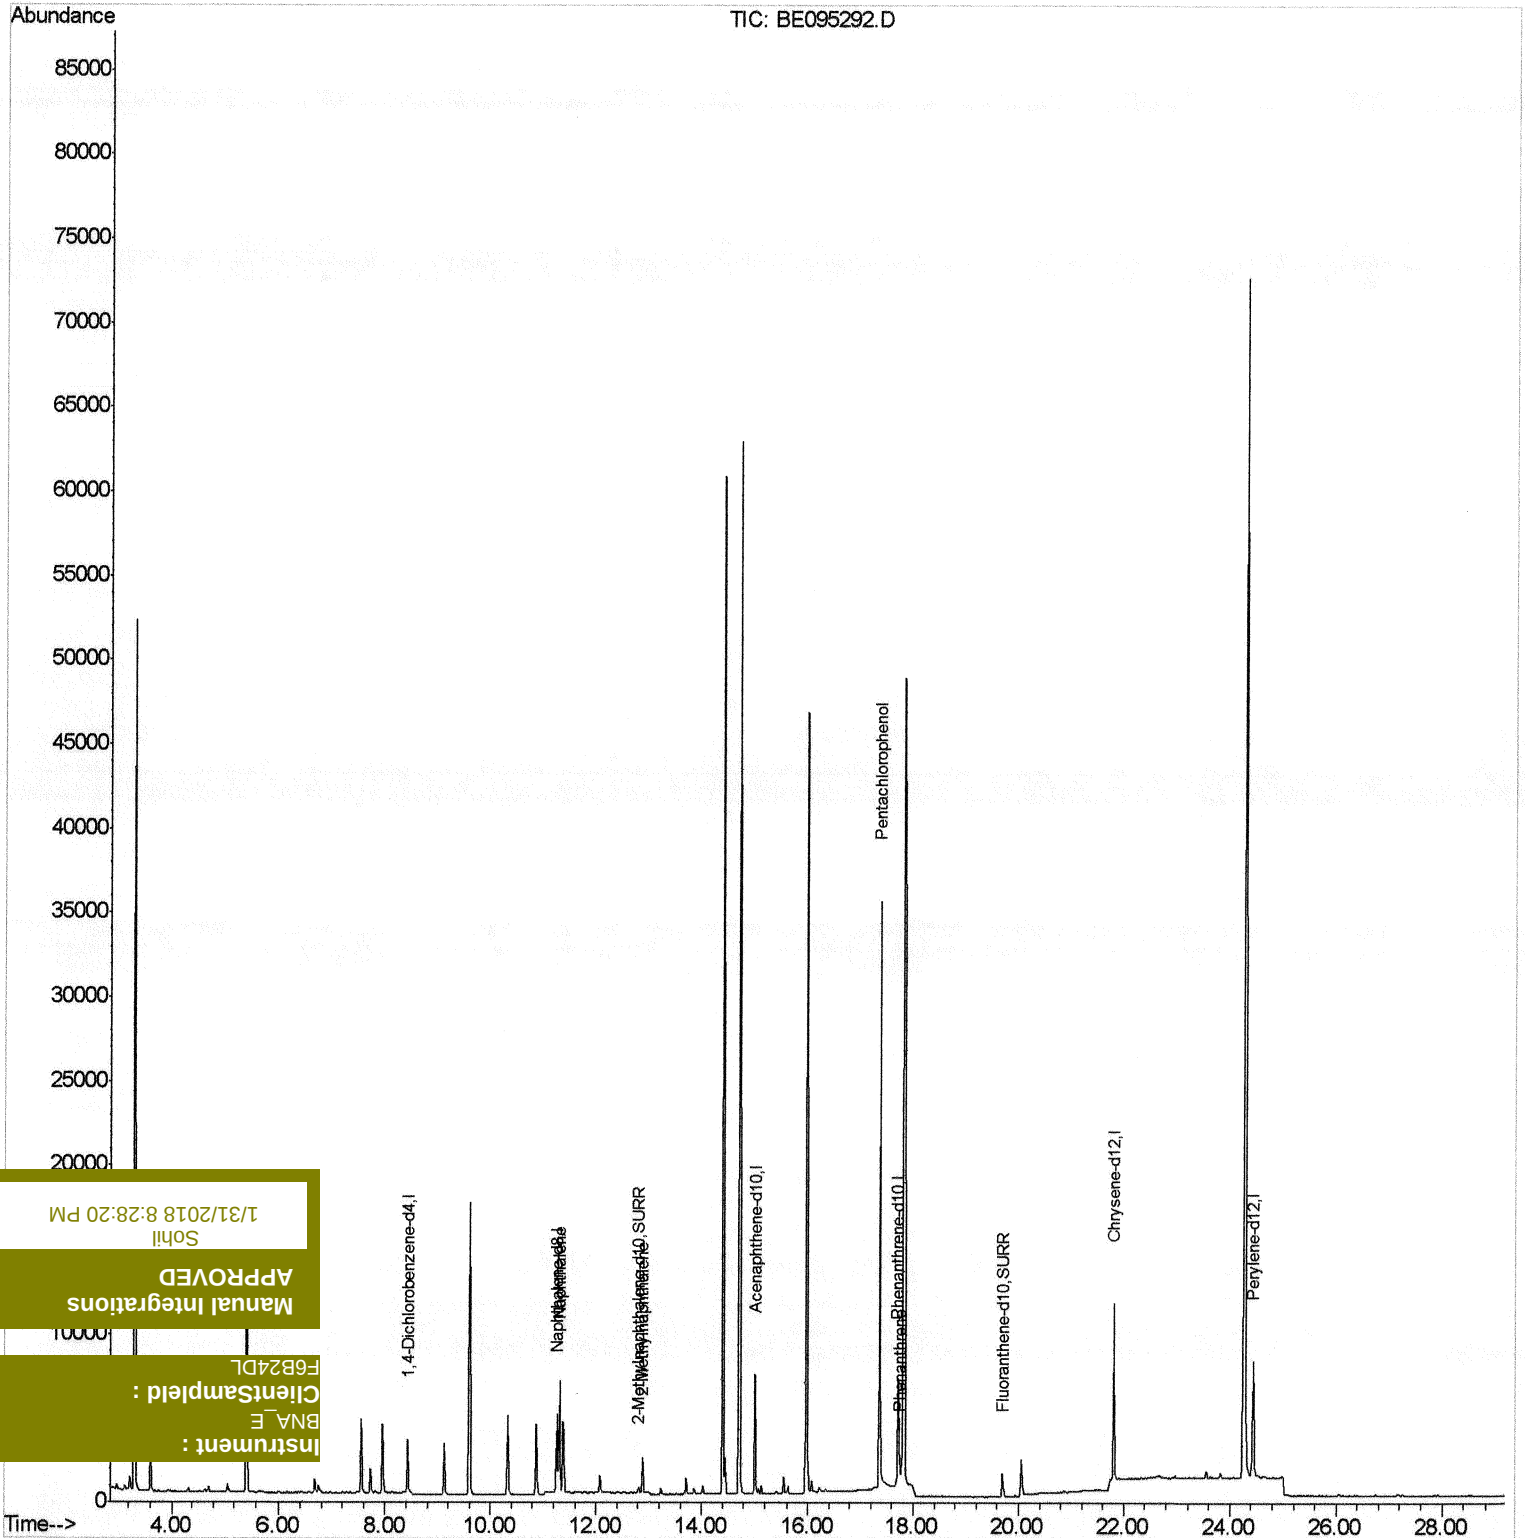

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013018\
 Data File : BE095292.D
 Acq On : 31 Jan 2018 00:06
 Operator : SJ/JU
 Sample : J1233-20DL 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Quant Time: Jan 31 03:43:40 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 31 03:40:45 2018
 Response via : Initial Calibration

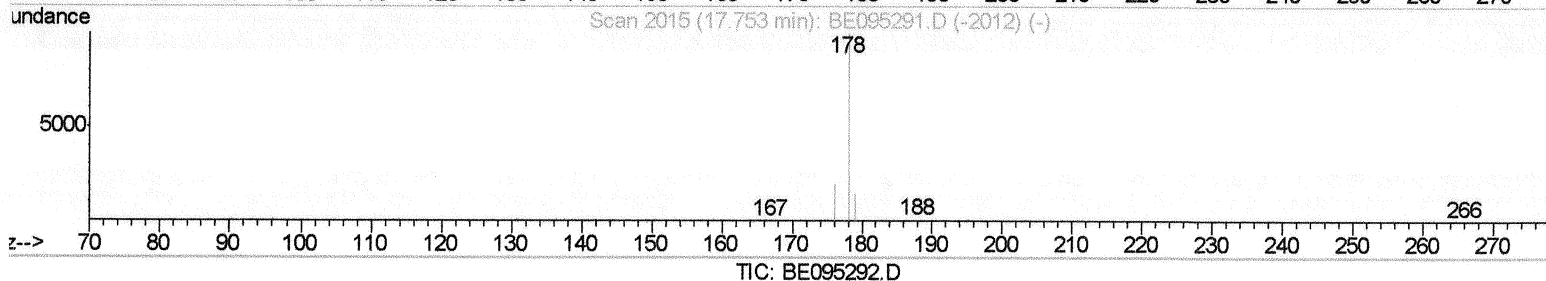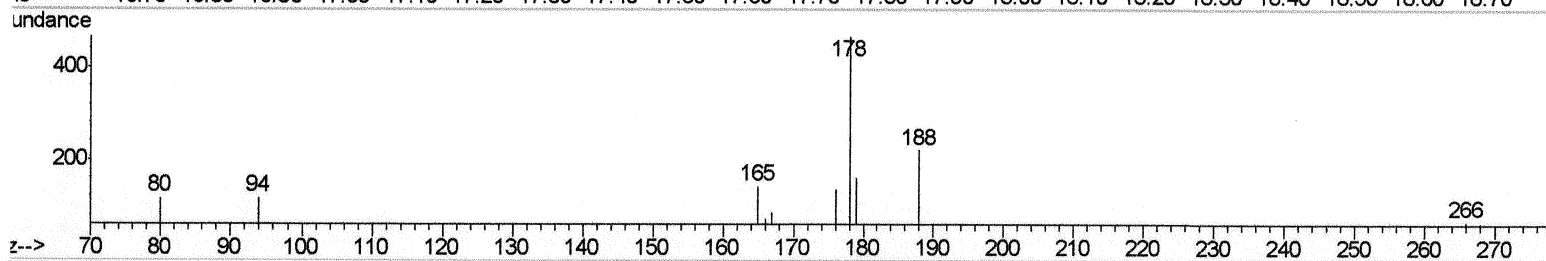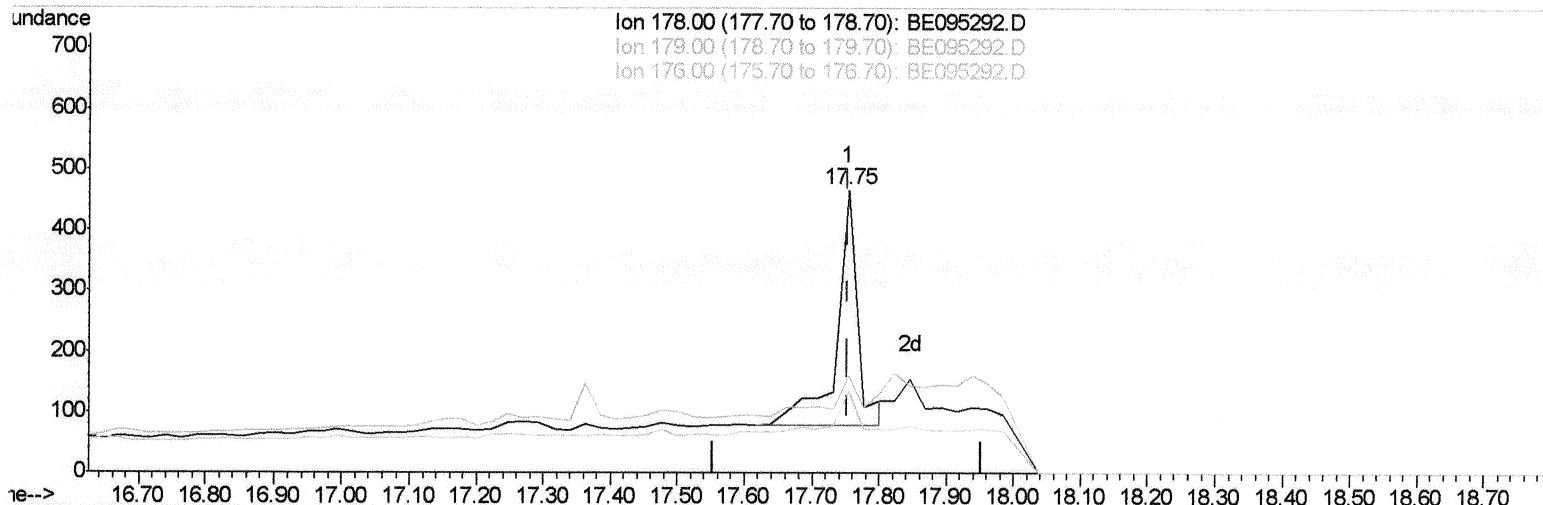

(12) Phenanthrene

17.754min (+0.000) 0.03ng/ul

1/31/2018 8:28:20 PM

Sohil

APPROVED

Manual Integrations




#8 Client Sampled :

Instrument :

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013018\
 Data File : BE095292.D
 Acq On : 31 Jan 2018 00:06
 Operator : SJ/JU
 Sample : J1233-20DL 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Quant Time: Jan 31 03:43:40 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 31 03:40:45 2018
 Response via : Initial Calibration

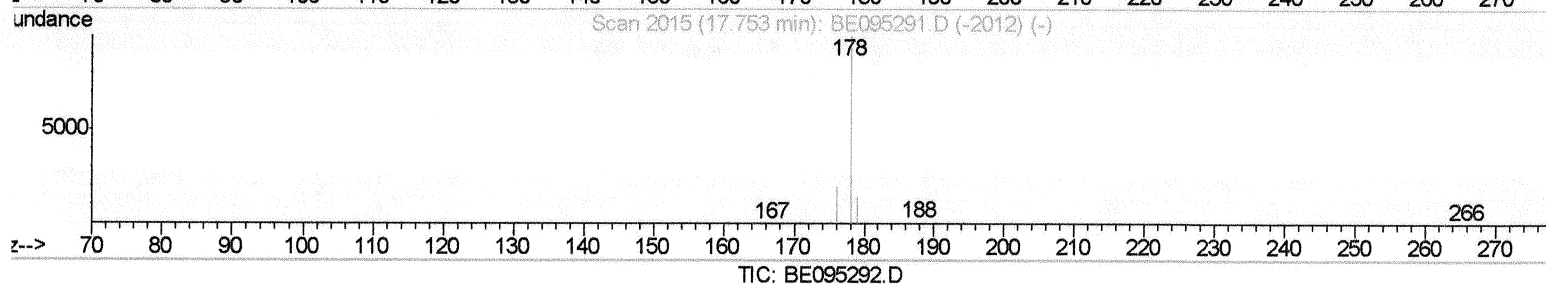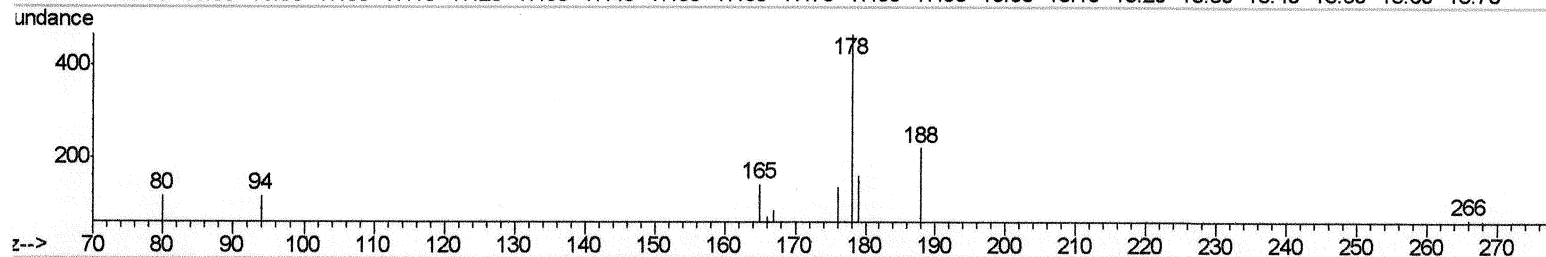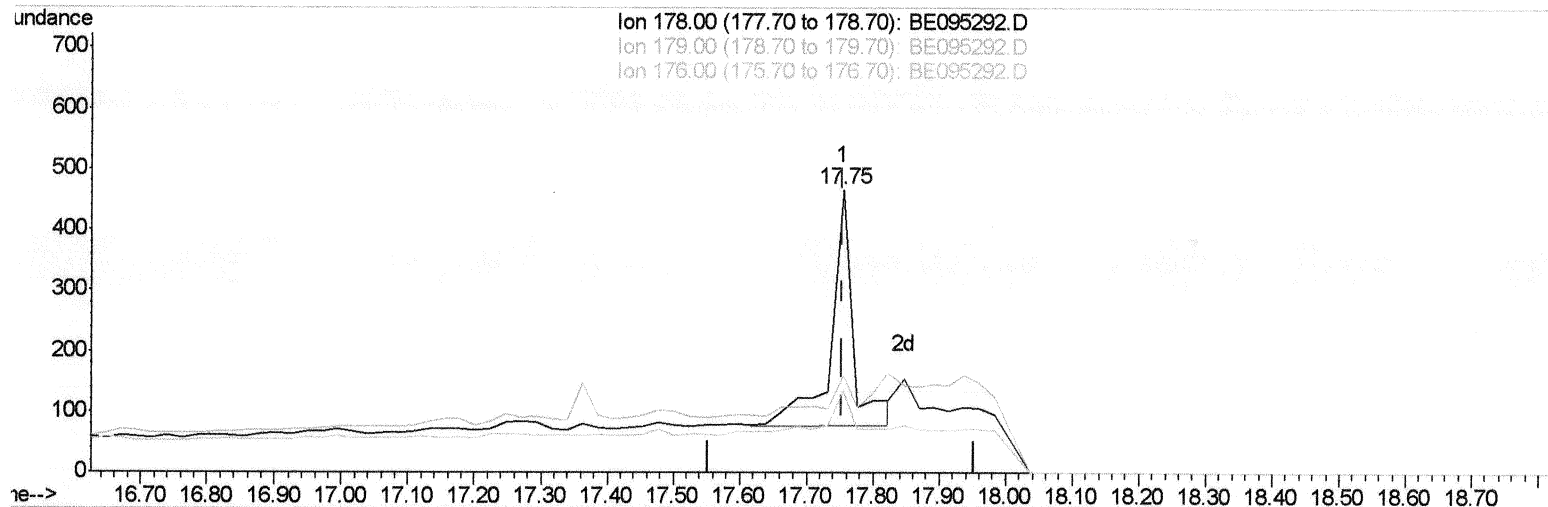

(12) Phenanthrene

17.754min (+0.000) 0.03ng/ul m > SJ 2/1/18

1/31/2018 8:28:20 PM

Sohil

APPROVED

Manual Integrations

Client Sampled :
 BNA_E

Instrument :

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013018\
 Data File : BE095292.D
 Acq On : 31 Jan 2018 00:06
 Operator : SJ/JU
 Sample : J1233-20DL 10X
 Disc :
 ALS Vial : 18 Sample Multiplier: 1

Quant Time: Jan 31 03:48:58 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 31 03:40:45 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	2233	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	6528	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3912	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	9616	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	10473	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	10583	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	501	0.05	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	1494	0.04	ng/ul	0.00
Target Compounds						
3) Naphthalene	11.31	128	9657	0.528	ng/ul#	89
5) 2-Methylnaphthalene	12.88	142	1740	0.143	ng/ul	98
11) Pentachlorophenol	17.36	266	20524	11.020	ng/ul	96
12) Phenanthrene	17.75	178	937m	0.029	ng/ul	

SJ 2/1/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed

1/31/2018 8:28:20 PM

Sohil

Manual Integrations
 APPROVED

Instrument : BNA_E
 Client Sample : F6B24DL