


Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013018\
 Data File : BE095319.D
 Acq On : 31 Jan 2018 16:10
 Operator : SJ/JU
 Sample : J1244-19
 Misc :
 ALS Vial : 43 Sample Multiplier: 1


Quant Time: Jan 31 17:53:45 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 31 11:55:47 2018
 Response via : Initial Calibration

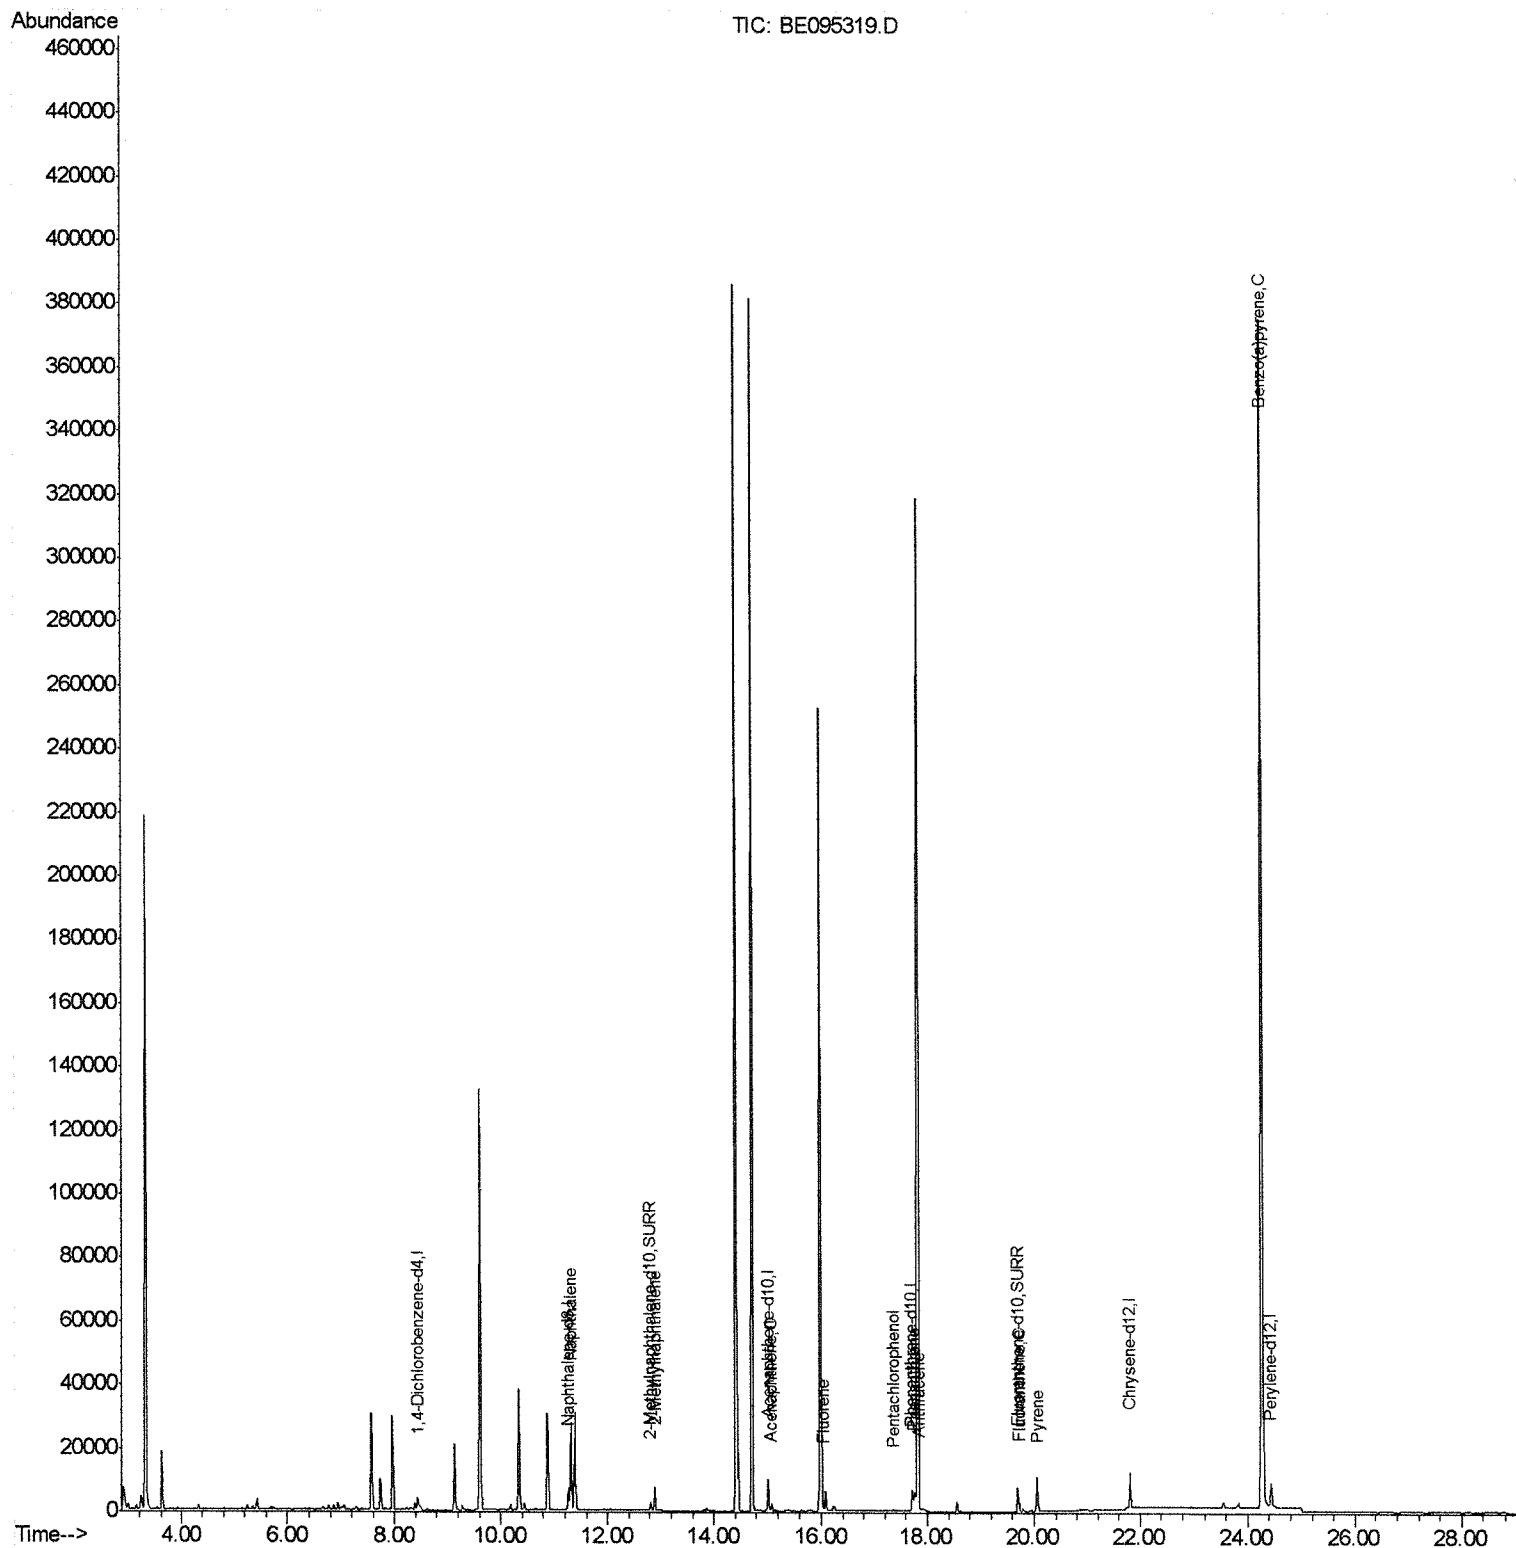

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013018\
 Data File : BE095319.D
 Acq On : 31 Jan 2018 16:10
 Operator : SJ/JU
 Sample : J1244-19
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Quant Time: Jan 31 16:50:22 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 31 11:55:47 2018
 Response via : Initial Calibration

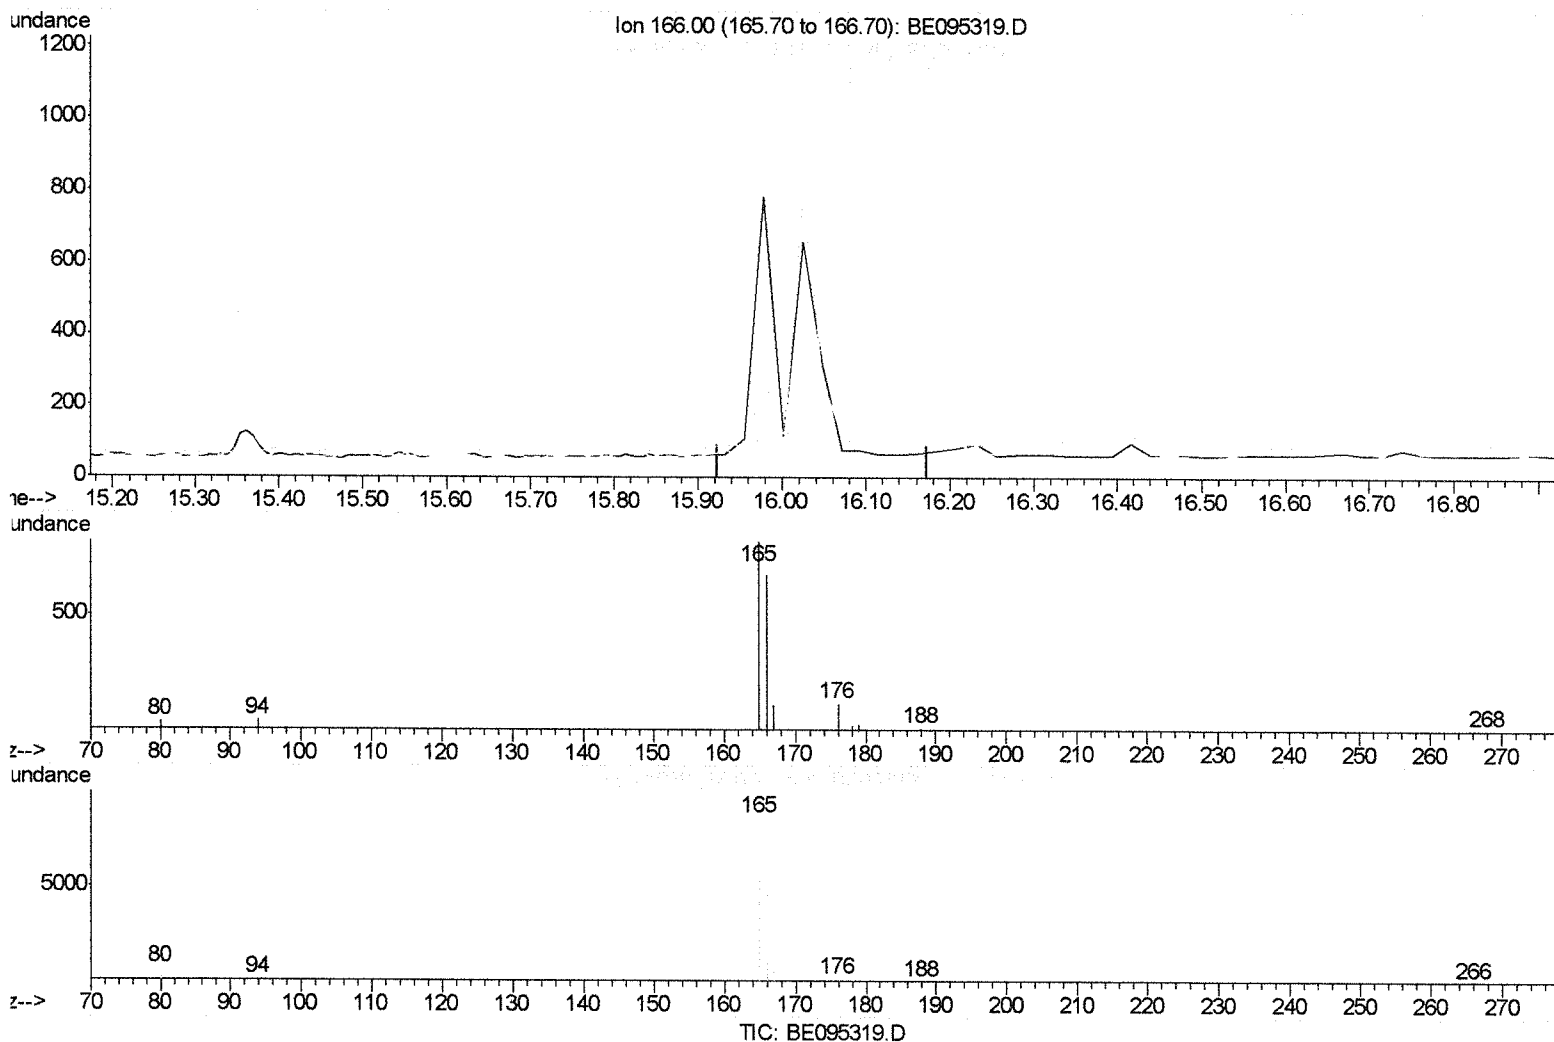

(9) Fluorene

16.024min (-16.024) 0.00ng/ul


response 0

Ion	Exp%	Act%
166.00	100	0.00
165.00	91.80	0.00#
167.00	18.30	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013018\
 Data File : BE095319.D
 Acq On : 31 Jan 2018 16:10
 Operator : SJ/JU
 Sample : J1244-19
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Quant Time: Jan 31 16:50:22 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 31 11:55:47 2018
 Response via : Initial Calibration

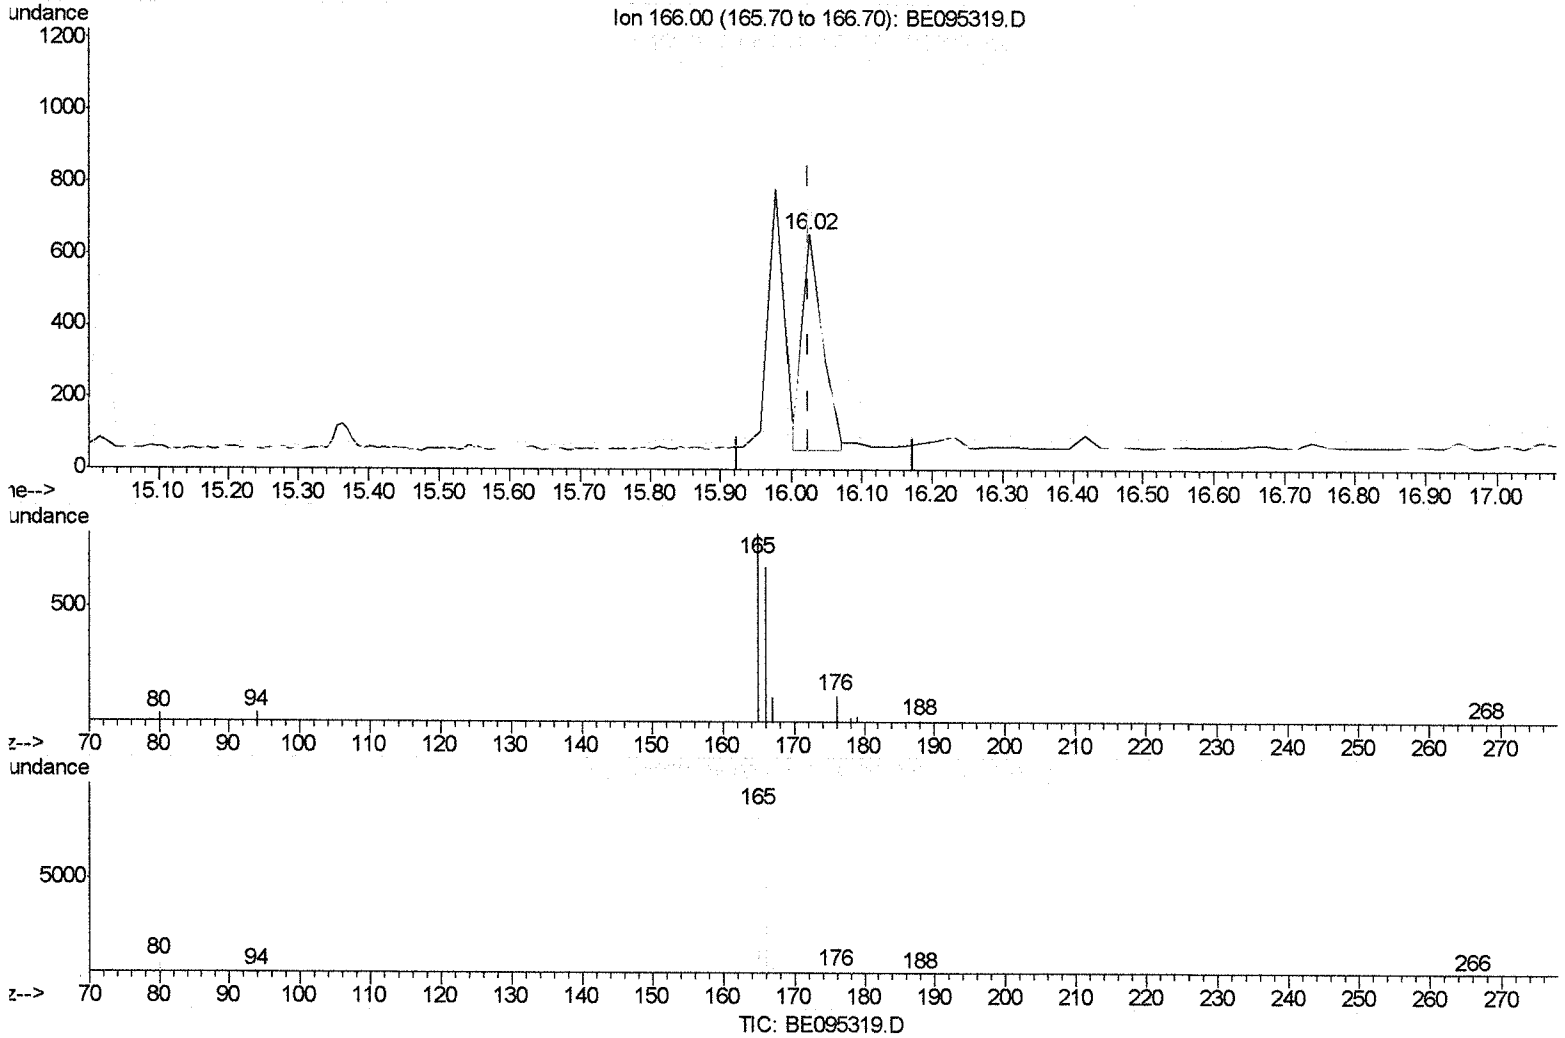

(9) Fluorene

16.025min (+0.000) 0.06ng/ul m) SJ 2/1/18

response 1218

Ion	Exp%	Act%
166.00	100	100
165.00	91.80	120.46#
167.00	18.30	21.83
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013018\
 Data File : BE095319.D
 Acq On : 31 Jan 2018 16:10
 Operator : SJ/JU
 Sample : J1244-19
 Disc :
 ALS Vial : 43 Sample Multiplier: 1

Quant Time: Jan 31 17:53:45 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 31 11:55:47 2018
 Response via : Initial Calibration



Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2652	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	8531	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	5488	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	10949	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	11154	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	12285	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.81	152	3370	0.24	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	8412	0.20	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
3) Naphthalene	11.31	128	37145	1.555	ng/ul#	88
5) 2-Methylnaphthalene	12.89	142	5989	0.375	ng/ul	99
8) Acenaphthene	15.08	153	1317	0.064	ng/ul#	93
9) Fluorene	16.02	166	1218m>	0.058	ng/ul	
11) Pentachlorophenol	17.36	266	303	0.143	ng/ul	95
12) Phenanthrene	17.75	178	6405	0.174	ng/ul#	88
13) Anthracene	17.84	178	1113	0.033	ng/ul#	89
15) Fluoranthene	19.72	202	2931	0.061	ng/ul	86
17) Pyrene	20.08	202	3428	0.092	ng/ul#	89
23) Benzo(a)pyrene	24.27	252	2330	0.060	ng/ul#	49

SJ 2/1/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed