

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE013117\
 Data File : BE092690.D
 Acq On : 31 Jan 2017 17:06
 Operator : SJ/MA
 Sample : PB96577BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 PB96577BL

Quant Time: Feb 01 02:21:01 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE011617.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 17 10:14:01 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.14	152	10717	5.00	ng	0.00
7) Naphthalene-d8	10.91	136	47483	5.00	ng	0.00
12) Acenaphthene-d10	14.78	164	29072	5.00	ng	0.00
18) Phenanthrene-d10	17.53	188	59723	5.00	ng	0.00
24) Chrysene-d12	21.72	240	70227	5.00	ng	0.00
31) Perylene-d12	24.06	264	77387	5.00	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.64	112	24642	10.30	ng	-0.01
5) Phenol-d6	7.31	99	29072	9.91	ng	-0.02
8) Nitrobenzene-d5	9.32	82	12866	4.17	ng	-0.02
13) 2,4,6-Tribromophenol	16.31	330	4344	5.11	ng	0.01
14) 2-Fluorobiphenyl	13.41	172	31534	4.41	ng	-0.01
26) Terphenyl-d14	20.14	244	44383	4.47	ng	-0.02
Target Compounds						
3) n-Nitrosodimethylamine	3.87	42	58	0.03	ng	# 14
19) Hexachlorobenzene	16.66	284	115	Below Cal		# 1
29) Bis(2-ethylhexyl)phthalate	21.61	149	302	0.23	ng	# 71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE013117\
Data File : BE092690.D
Acq On : 31 Jan 2017 17:06
Operator : SJ/MA
Sample : PB96577BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB96577BL

Quant Time: Feb 01 02:21:01 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE011617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 17 10:14:01 2017
Response via : Initial Calibration

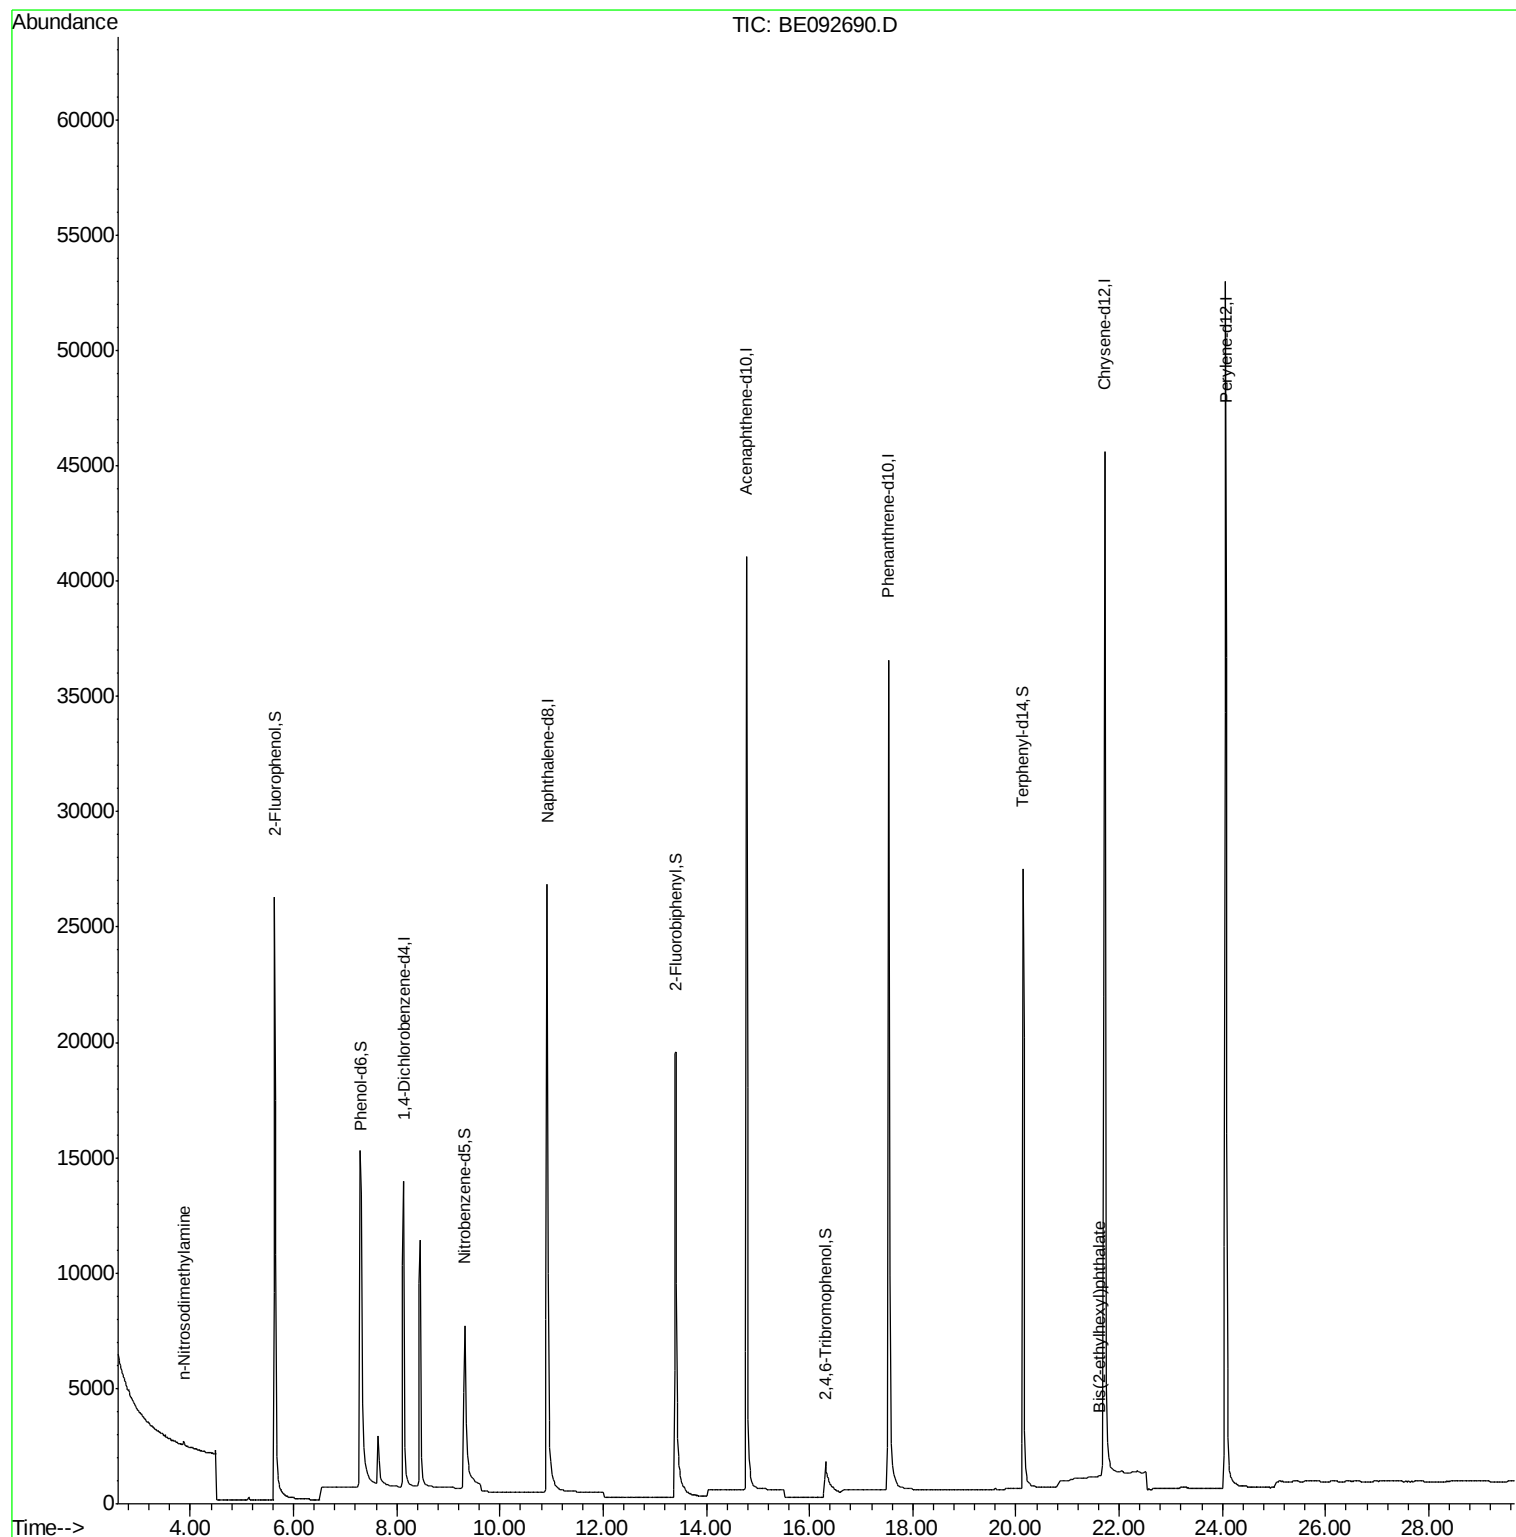

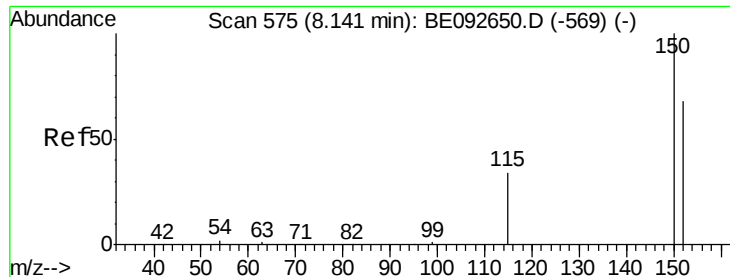

#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 8.14 min Scan# 575

Delta R.T. 0.00 min

Lab File: BE092690.D

Acq: 31 Jan 2017 17:06

Instrument :

BNA_E

ClientSampleId :

PB96577BL


Tgt Ion:152 Resp: 10717

Ion Ratio Lower Upper

152 100

150 134.9 106.0 159.0




115 40.2 31.2 46.8

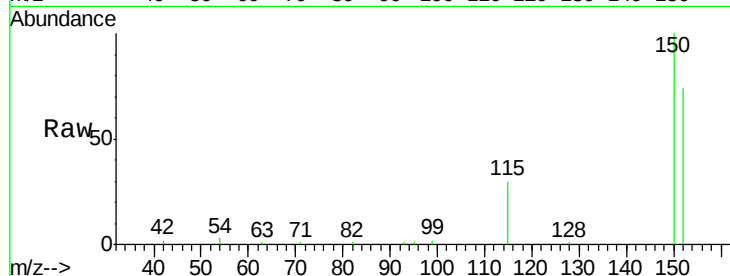

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

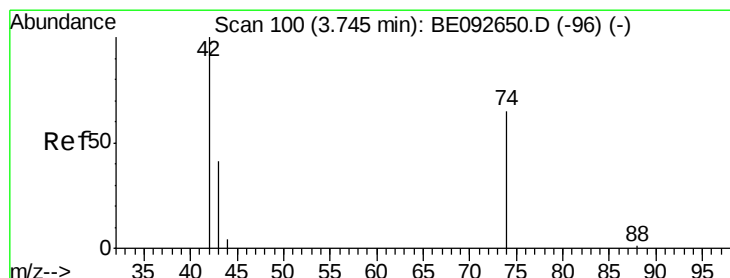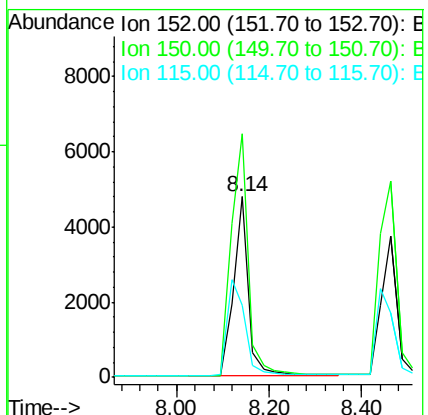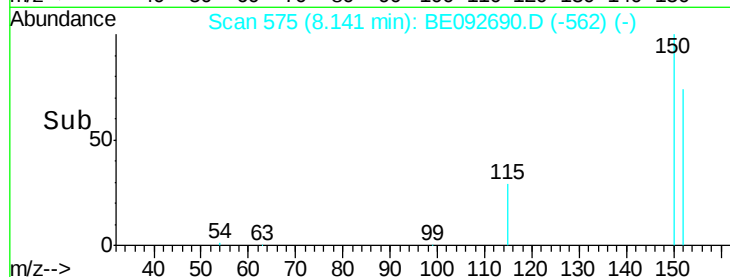

#3

n-Nitrosodimethylamine

Concen: 0.03 ng

RT: 3.87 min Scan# 111

Delta R.T. 0.13 min

Lab File: BE092690.D

Acq: 31 Jan 2017 17:06


Tgt Ion: 42 Resp: 58

Ion Ratio Lower Upper

42 100

74 13.8 86.0 129.0#



44 0.0 5.1 7.7#

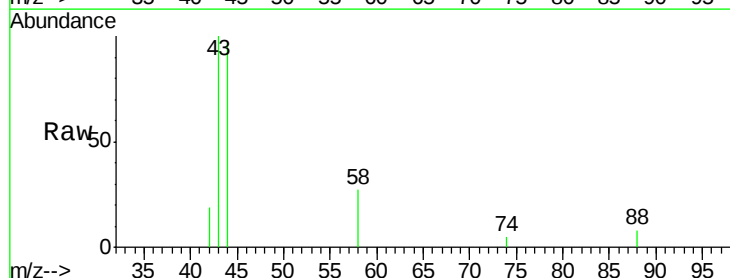


Abundance Ion 42.00 (41.70 to 42.70): BE0

Ion 74.00 (73.70 to 74.70): BE0

Ion 44.00 (43.70 to 44.70): BE0

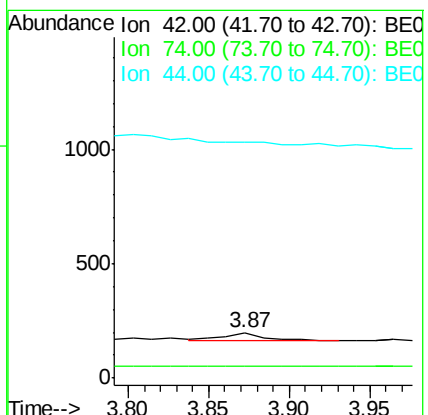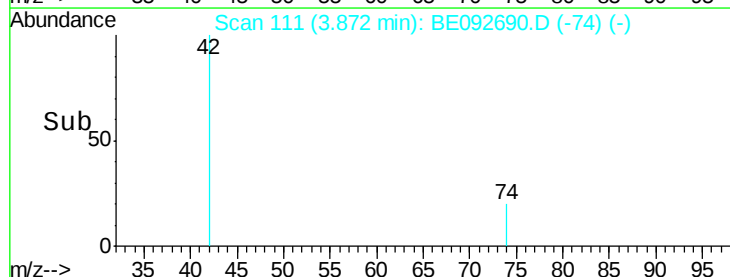

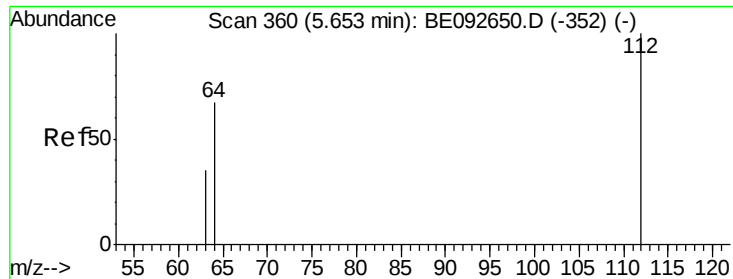

#4

2-Fluorophenol

Concen: 10.30 ng

RT: 5.64 min Scan# 358

Delta R.T. -0.01 min

Lab File: BE092690.D

Acq: 31 Jan 2017 17:06

Instrument :

BNA_E

ClientSampleId :

PB96577BL


Tgt Ion: 112 Resp: 24642

Ion Ratio Lower Upper

112 100

64 69.0 53.5 80.3




63 36.9 27.9 41.9

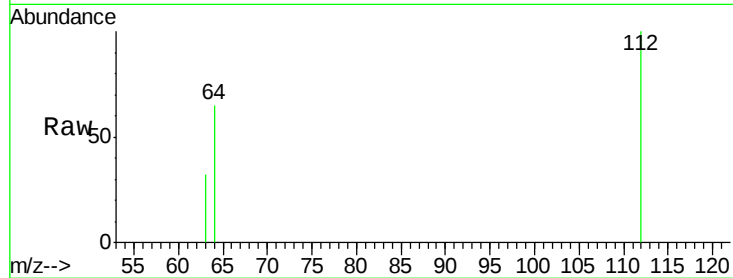

Abundance Ion 112.00 (111.70 to 112.70): BE0

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

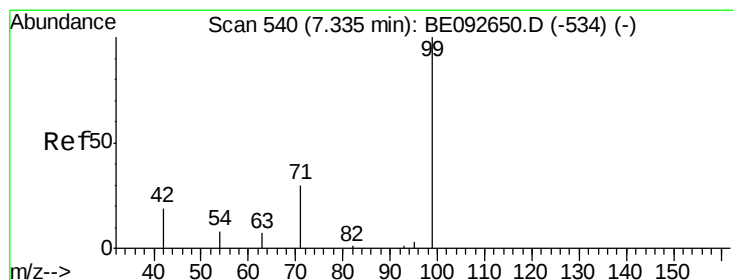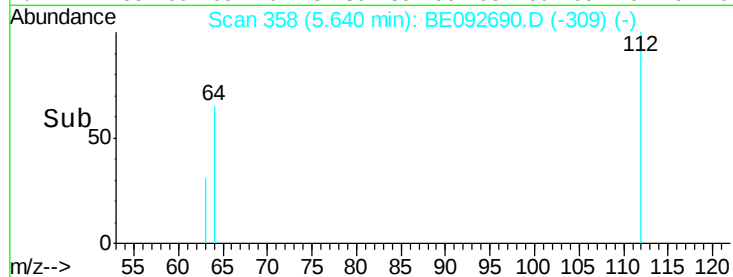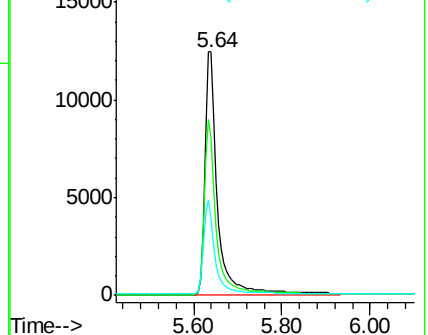

#5

Phenol-d6

Concen: 9.91 ng

RT: 7.31 min Scan# 539

Delta R.T. -0.02 min

Lab File: BE092690.D

Acq: 31 Jan 2017 17:06


Tgt Ion: 99 Resp: 29072

Ion Ratio Lower Upper

99 100

42 0.0 16.0 24.0#



71 0.0 30.6 45.8#

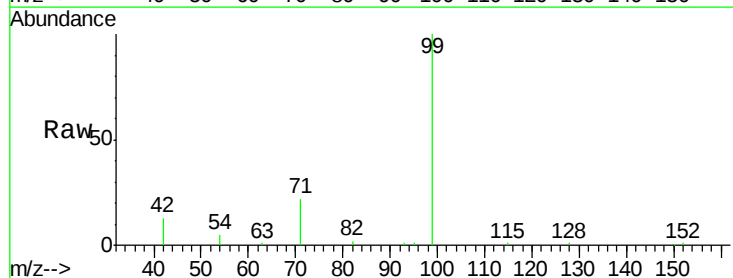


Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

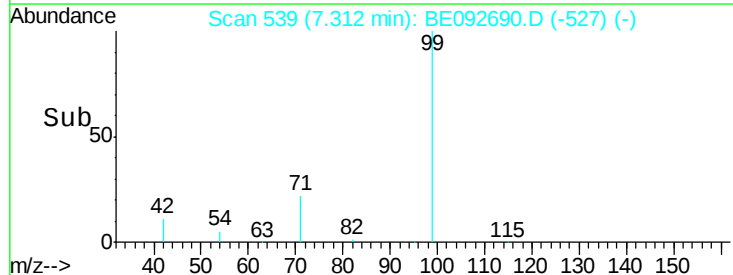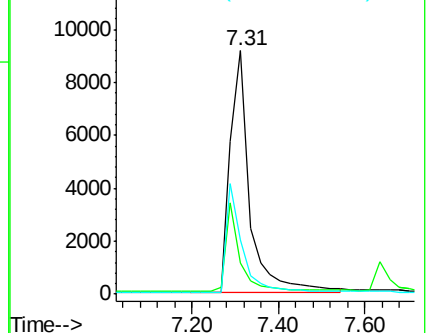

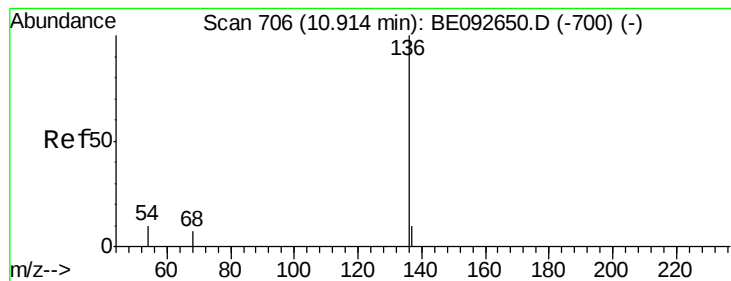

#7

Naphthalene-d8

Concen: 5.00 ng

RT: 10.91 min Scan# 706

Delta R.T. 0.00 min

Lab File: BE092690.D

Acq: 31 Jan 2017 17:06

Instrument :

BNA_E

ClientSampleId :

PB96577BL

Tgt Ion:136 Resp: 47483





Ion Ratio Lower Upper

136 100

137 11.2 8.2 12.4

54 8.0 9.6 14.4#

68 5.7 6.7 10.1#

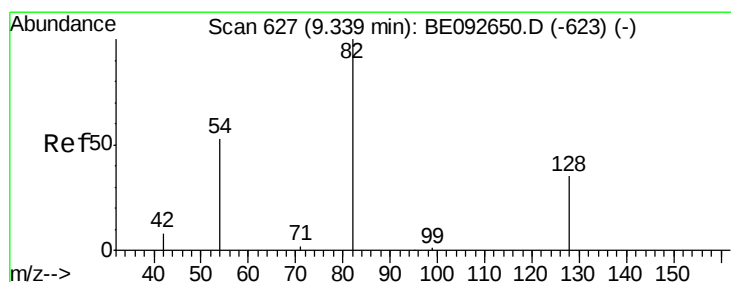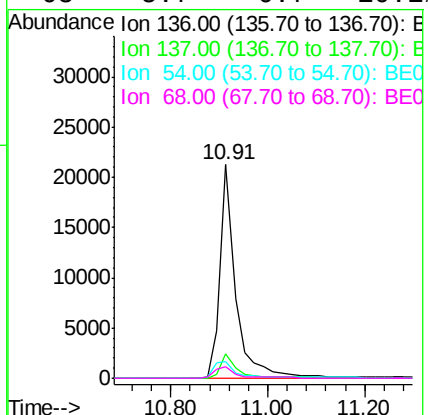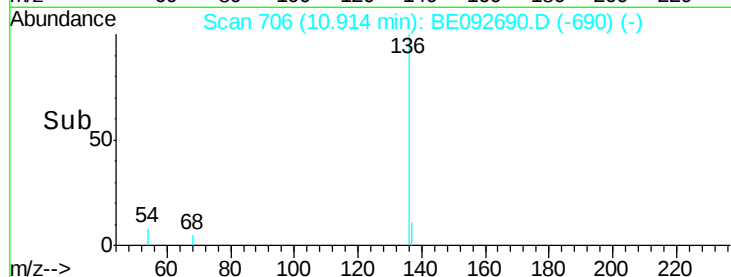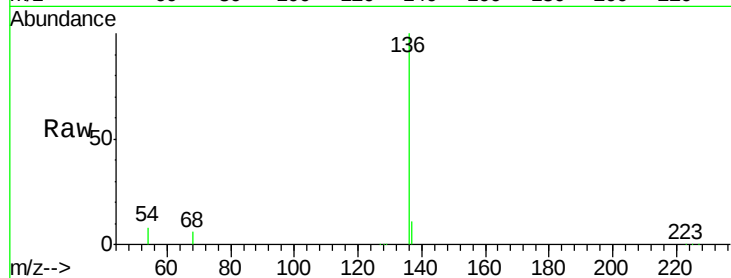

#8

Nitrobenzene-d5

Concen: 4.17 ng

RT: 9.32 min Scan# 626

Delta R.T. -0.02 min

Lab File: BE092690.D

Acq: 31 Jan 2017 17:06




Tgt Ion: 82 Resp: 12866


Ion Ratio Lower Upper

82 100

128 42.5 39.0 58.4

54 51.5 44.8 67.2

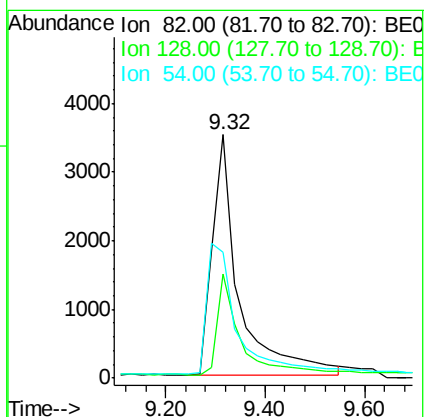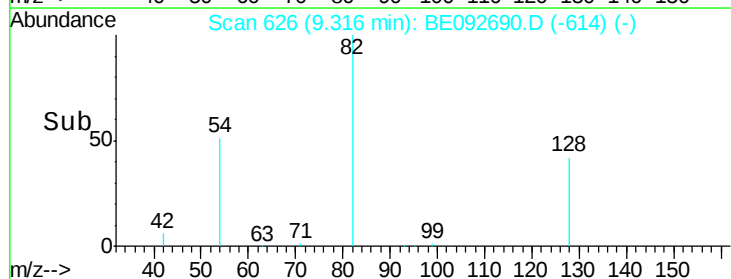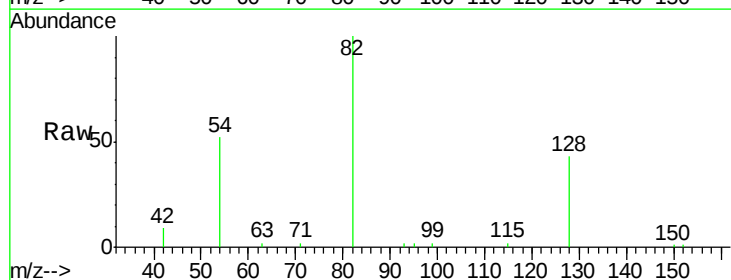

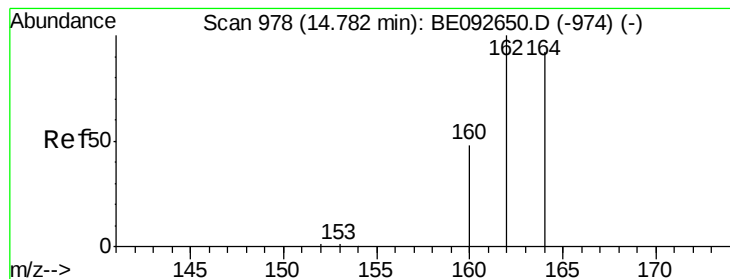

#12

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.78 min Scan# 978

Delta R.T. -0.00 min

Lab File: BE092690.D

Acq: 31 Jan 2017 17:06

Instrument :

BNA_E

ClientSampleId :

PB96577BL





Tgt Ion:164 Resp: 29072

Ion Ratio Lower Upper

164 100

162 107.9 71.4 107.0#

160 50.3 27.4 41.2#

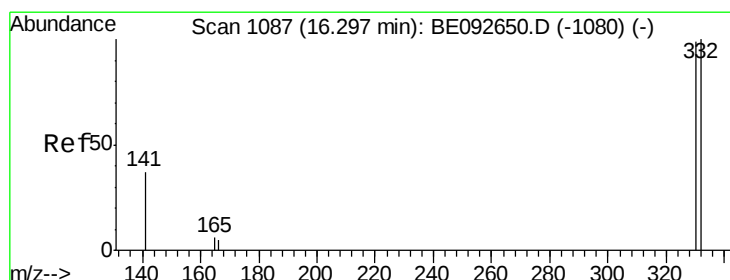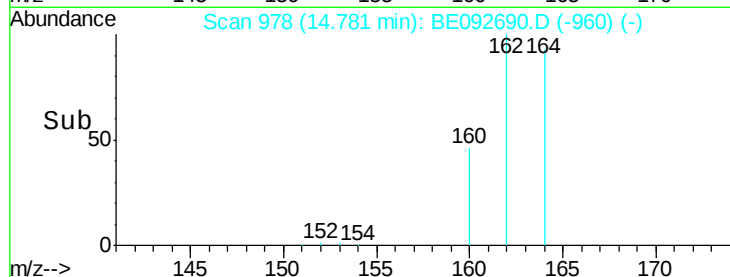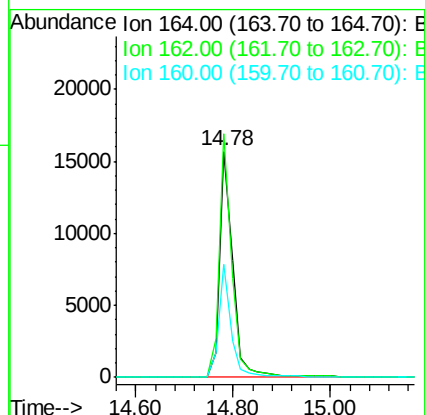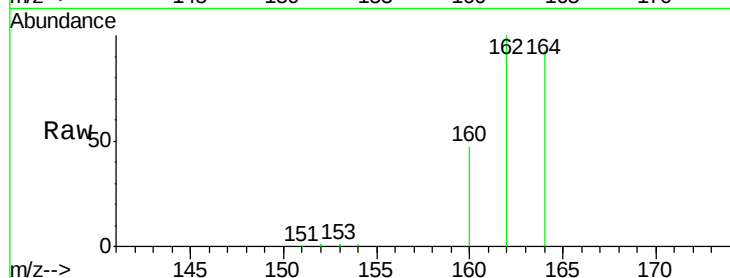

#13

2,4,6-Tribromophenol

Concen: 5.11 ng

RT: 16.31 min Scan# 1088

Delta R.T. 0.01 min

Lab File: BE092690.D

Acq: 31 Jan 2017 17:06




Tgt Ion:330 Resp: 4344


Ion Ratio Lower Upper

330 100

332 96.9 75.4 113.0

141 44.9 31.0 46.6

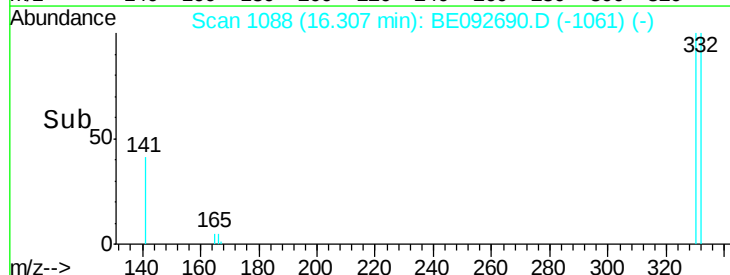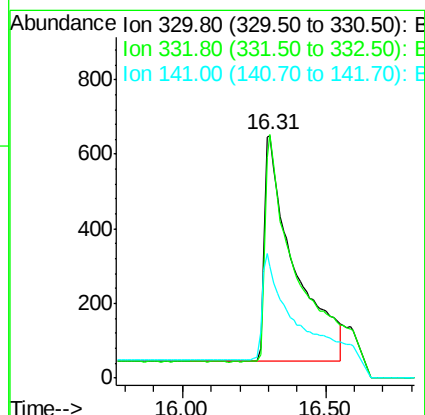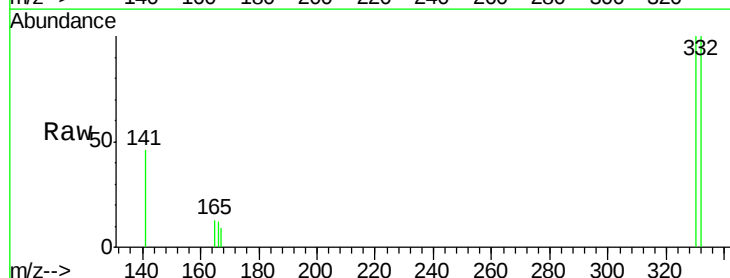

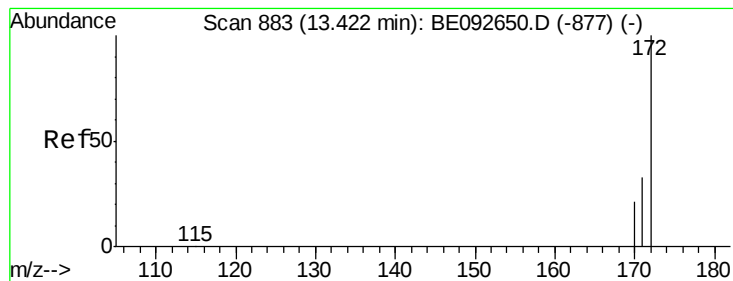

#14

2-Fluorobiphenyl

Concen: 4.41 ng

RT: 13.41 min Scan# 882

Delta R.T. -0.01 min

Lab File: BE092690.D

Acq: 31 Jan 2017 17:06

Instrument :

BNA_E

ClientSampleId :

PB96577BL





Tgt Ion:172 Resp: 31534

Ion Ratio Lower Upper

172 100

171 31.8 30.1 45.1

170 20.1 21.8 32.6#

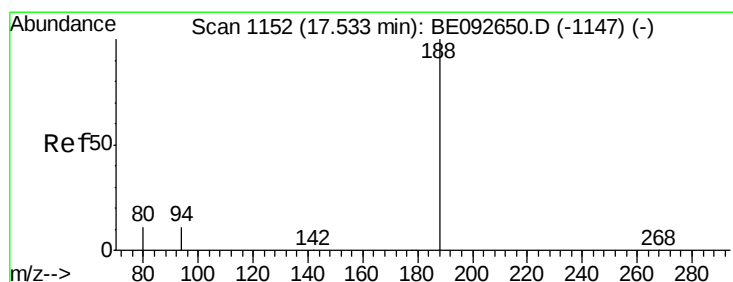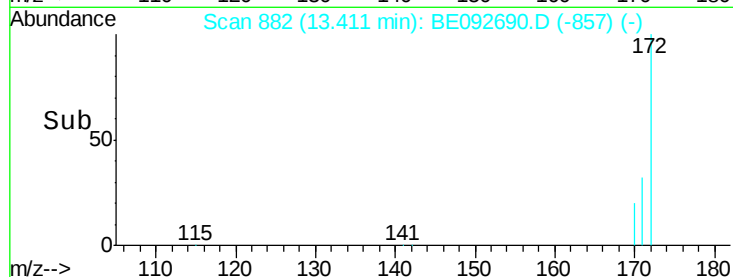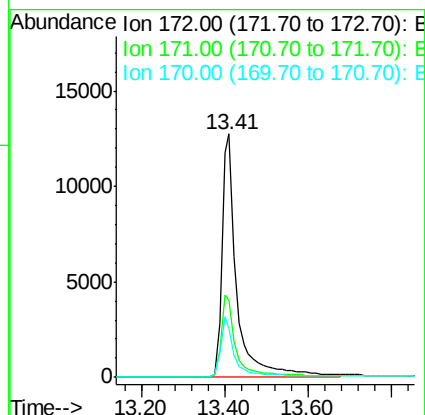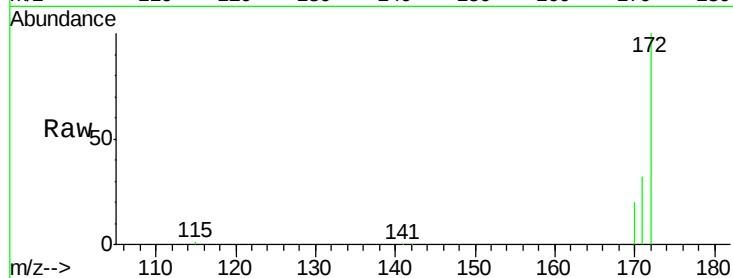

#18

Phenanthrene-d10

Concen: 5.00 ng

RT: 17.53 min Scan# 1152

Delta R.T. 0.00 min

Lab File: BE092690.D

Acq: 31 Jan 2017 17:06




Tgt Ion:188 Resp: 59723


Ion Ratio Lower Upper

188 100

94 10.7 3.2 4.8#

80 10.5 2.6 3.8#

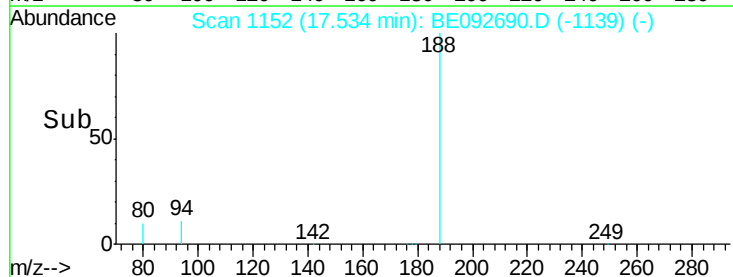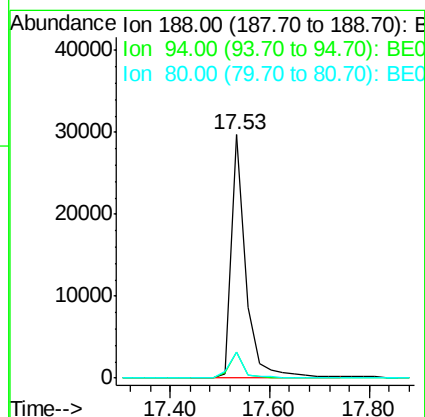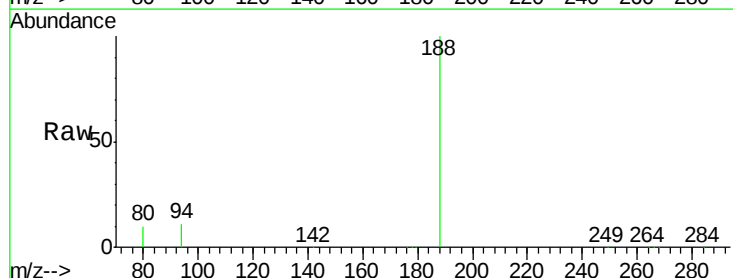

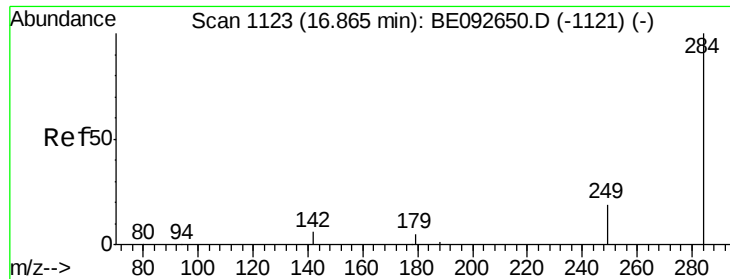

#19

Hexachlorobenzene

Concen: Below Cal

RT: 16.66 min Scan# 1114

Delta R.T. -0.21 min

Lab File: BE092690.D

Acq: 31 Jan 2017 17:06

Instrument :

BNA_E

ClientSampleId :

PB96577BL


Tgt Ion:284 Resp: 115

Ion Ratio Lower Upper

284 100

142 370.4 29.1 43.7#




249 0.0 27.9 41.9#

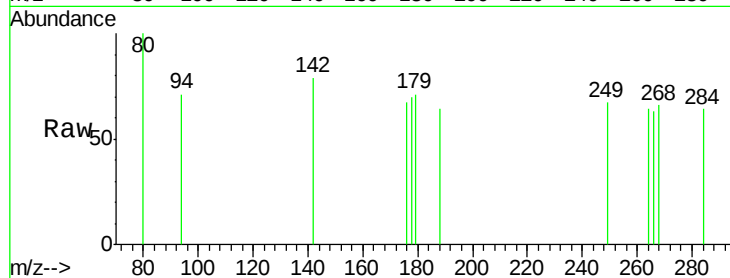

Abundance Ion 283.80 (283.50 to 284.50): E

Ion 142.00 (141.70 to 142.70): E

Ion 249.00 (248.70 to 249.70): E

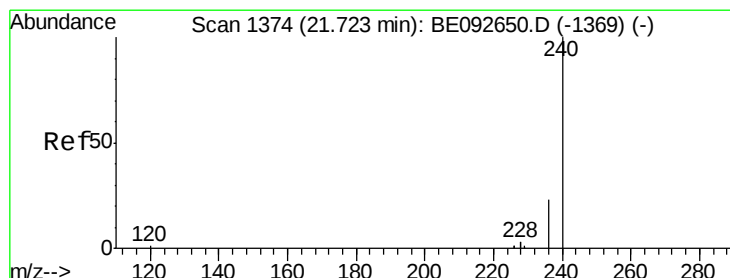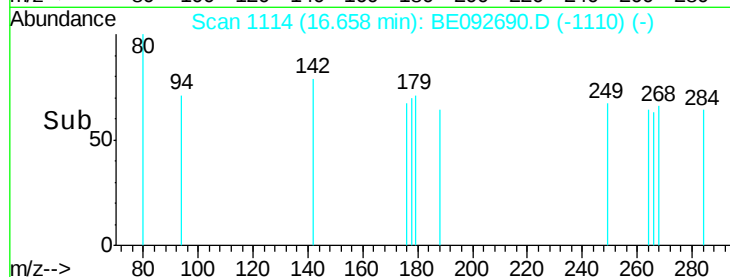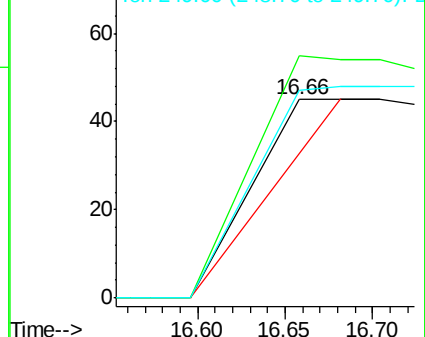

#24

Chrysene-d12

Concen: 5.00 ng

RT: 21.72 min Scan# 1374

Delta R.T. 0.00 min

Lab File: BE092690.D

Acq: 31 Jan 2017 17:06


Tgt Ion:240 Resp: 70227

Ion Ratio Lower Upper

240 100

120 1.6 2.6 4.0#



236 22.3 24.6 37.0#

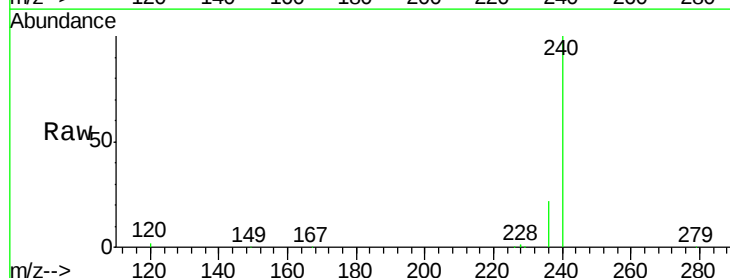


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



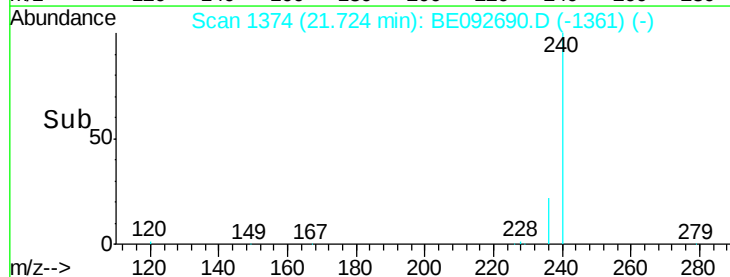
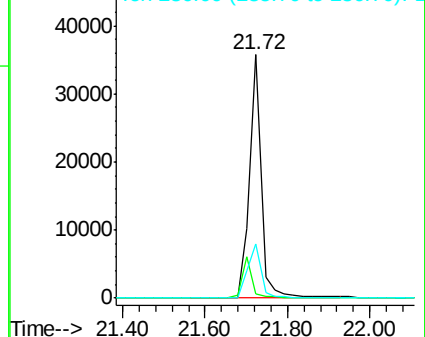


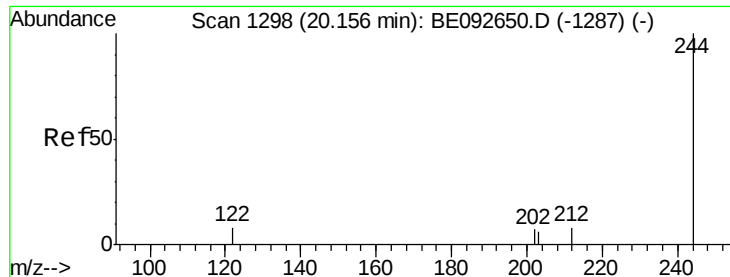

#26
 Terphenyl-d14
 Concen: 4.47 ng
 RT: 20.14 min Scan# 1297
 Delta R.T. -0.02 min
 Lab File: BE092690.D
 Acq: 31 Jan 2017 17:06




Instrument :
 BNA_E
 ClientSampled :
 PB96577BL


Tgt Ion: 244 Resp: 44383
 Ion Ratio Lower Upper
 244 100
 212 10.3 6.7 10.1#
 122 17.2 3.6 5.4#

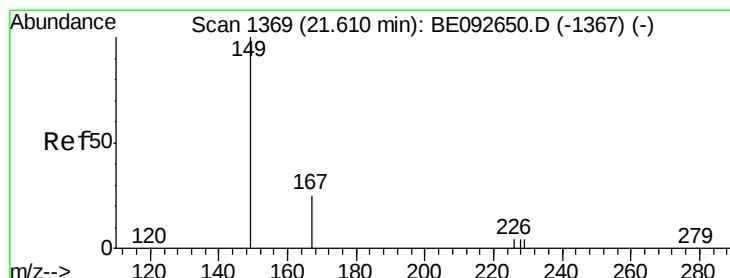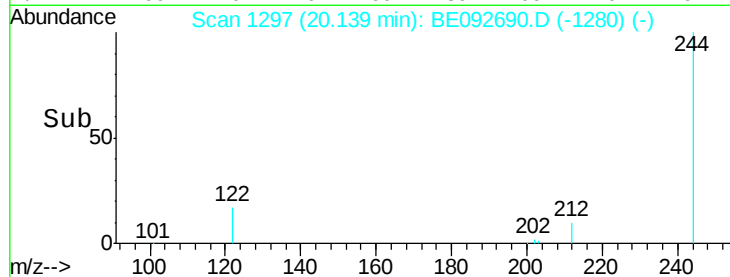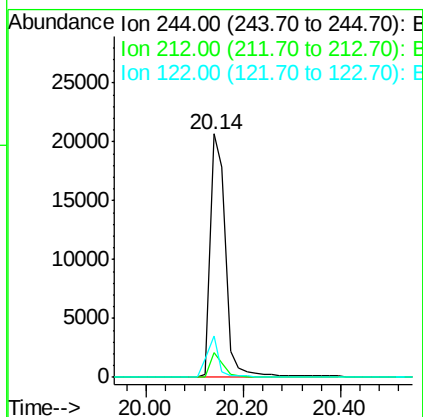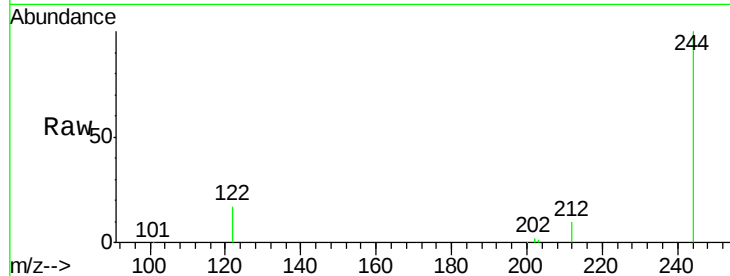

#29
 Bis(2-ethylhexyl)phthalate
 Concen: 0.23 ng
 RT: 21.61 min Scan# 1369
 Delta R.T. 0.00 min
 Lab File: BE092690.D
 Acq: 31 Jan 2017 17:06

Tgt Ion: 149 Resp: 302
 Ion Ratio Lower Upper
 149 100
 167 13.6 16.0 24.0#
 279 0.0 16.0 24.0#

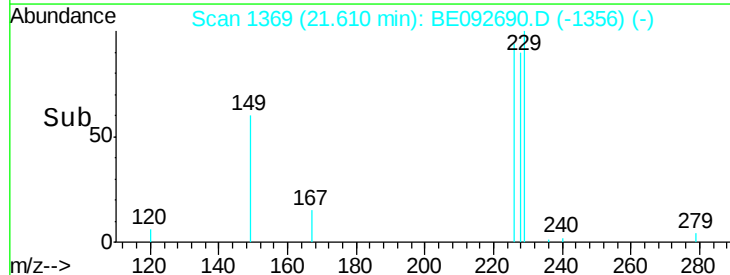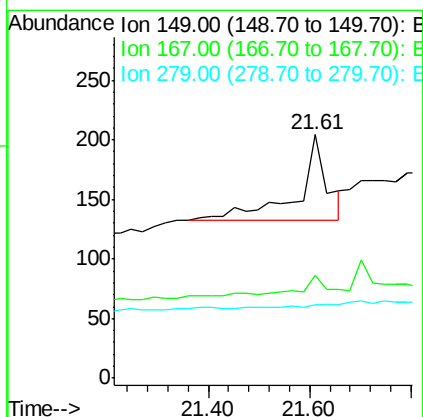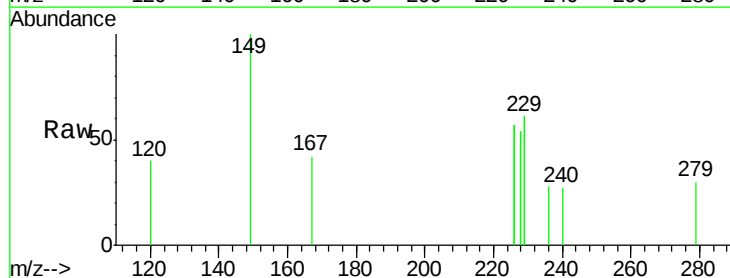

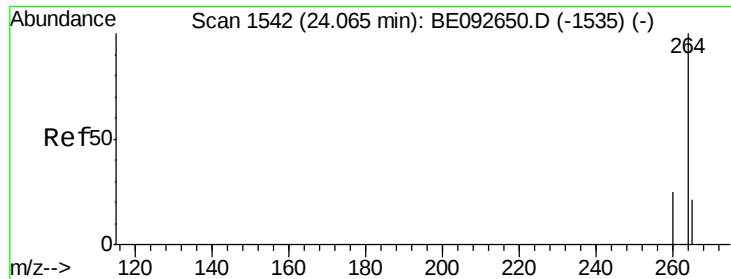

#31

Perylene-d12

Concen: 5.00 ng

RT: 24.06 min Scan# 1542

Delta R.T. -0.00 min

Lab File: BE092690.D


Acq: 31 Jan 2017 17:06

Instrument :

BNA_E

ClientSampleId :

PB96577BL

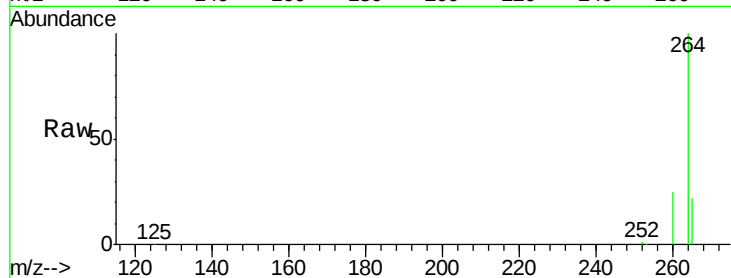

Tgt Ion: 264 Resp: 77387

Ion	Ratio	Lower	Upper
264	100		
260	25.1	20.1	30.1
265	21.7	17.9	26.9

