


Data Path : Z:\HPCHEM1\BNA E\DATA\BE013117\
 Data File : BE092688.D
 Acq On : 31 Jan 2017 15:49
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE011617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 17 10:14:01 2017

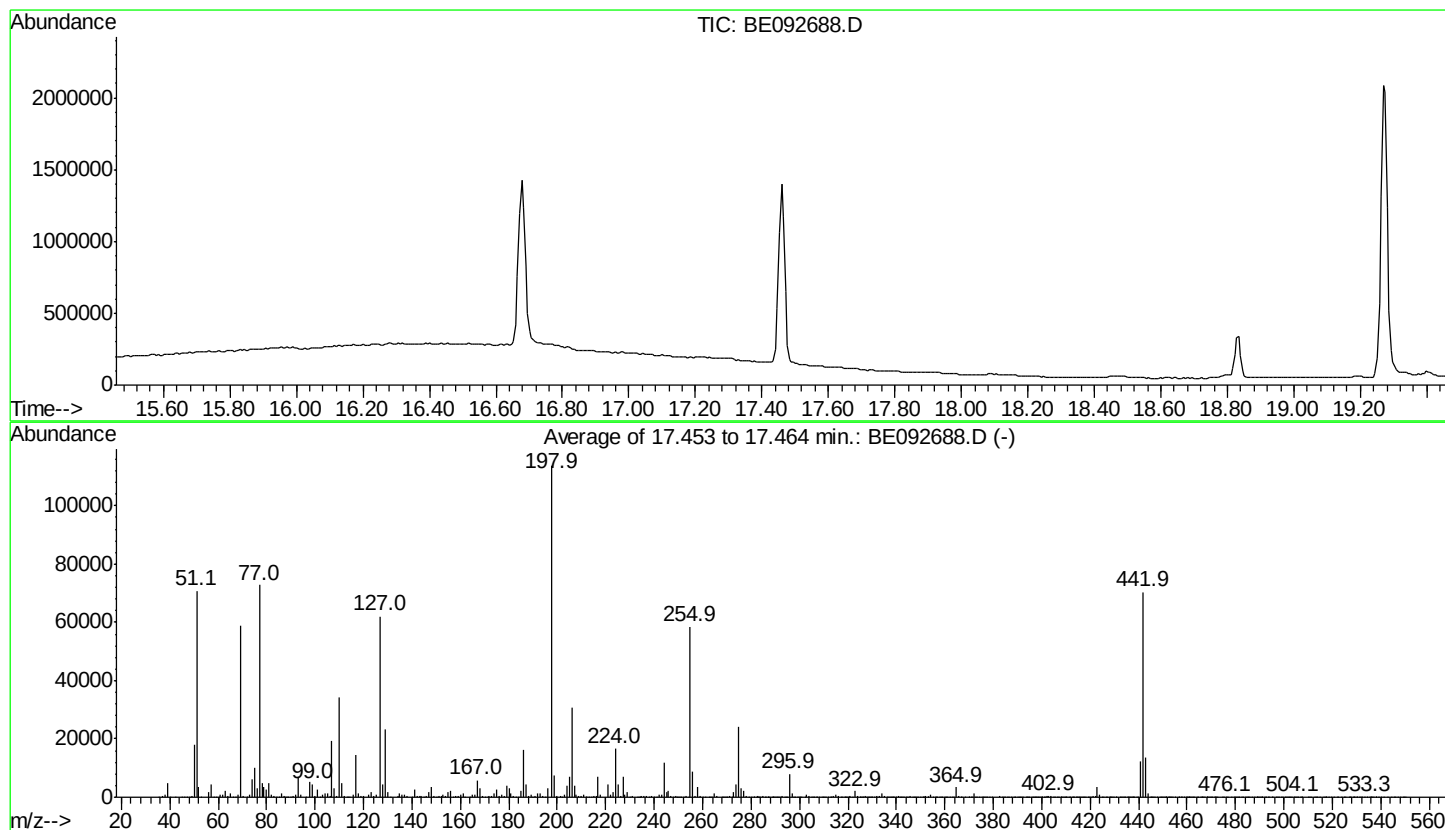

AutoFind: Scans 2530, 2531, 2532; Background Corrected with Scan 2524

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	62.3	70942	PASS
68	69	0.00	2	1.5	873	PASS
69	198	0.00	100	51.9	59052	PASS
70	69	0.00	2	0.5	291	PASS
127	198	10	80	54.4	61951	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	113786	PASS
199	198	5	9	6.8	7690	PASS
275	198	10	60	21.2	24076	PASS
365	198	1	100	3.0	3453	PASS
441	442	0.01	24	17.3	12152	PASS
442	198	50	100	61.8	70312	PASS
443	442	15	24	19.3	13582	PASS