

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013118\
 Data File : BE095330.D
 Acq On : 31 Jan 2018 22:56
 Operator : SJ/JU
 Sample : J1245-18
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6B79

Quant Time: Feb 01 04:06:53 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 01 04:05:22 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2213	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	6806	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	4489	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.71
16) Chrysene-d12	21.80	240	8968	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	649817	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	4556	0.41	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	12663	0.00	ng/ul	0.00
Target Compounds						
3) Naphthalene	11.31	128	409	0.021	ng/ul#	58
17) Pyrene	20.05	202	1976	0.066	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013118\
Data File : BE095330.D
Acq On : 31 Jan 2018 22:56
Operator : SJ/JU
Sample : J1245-18
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6B79

Quant Time: Feb 01 04:06:53 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 04:05:22 2018
Response via : Initial Calibration

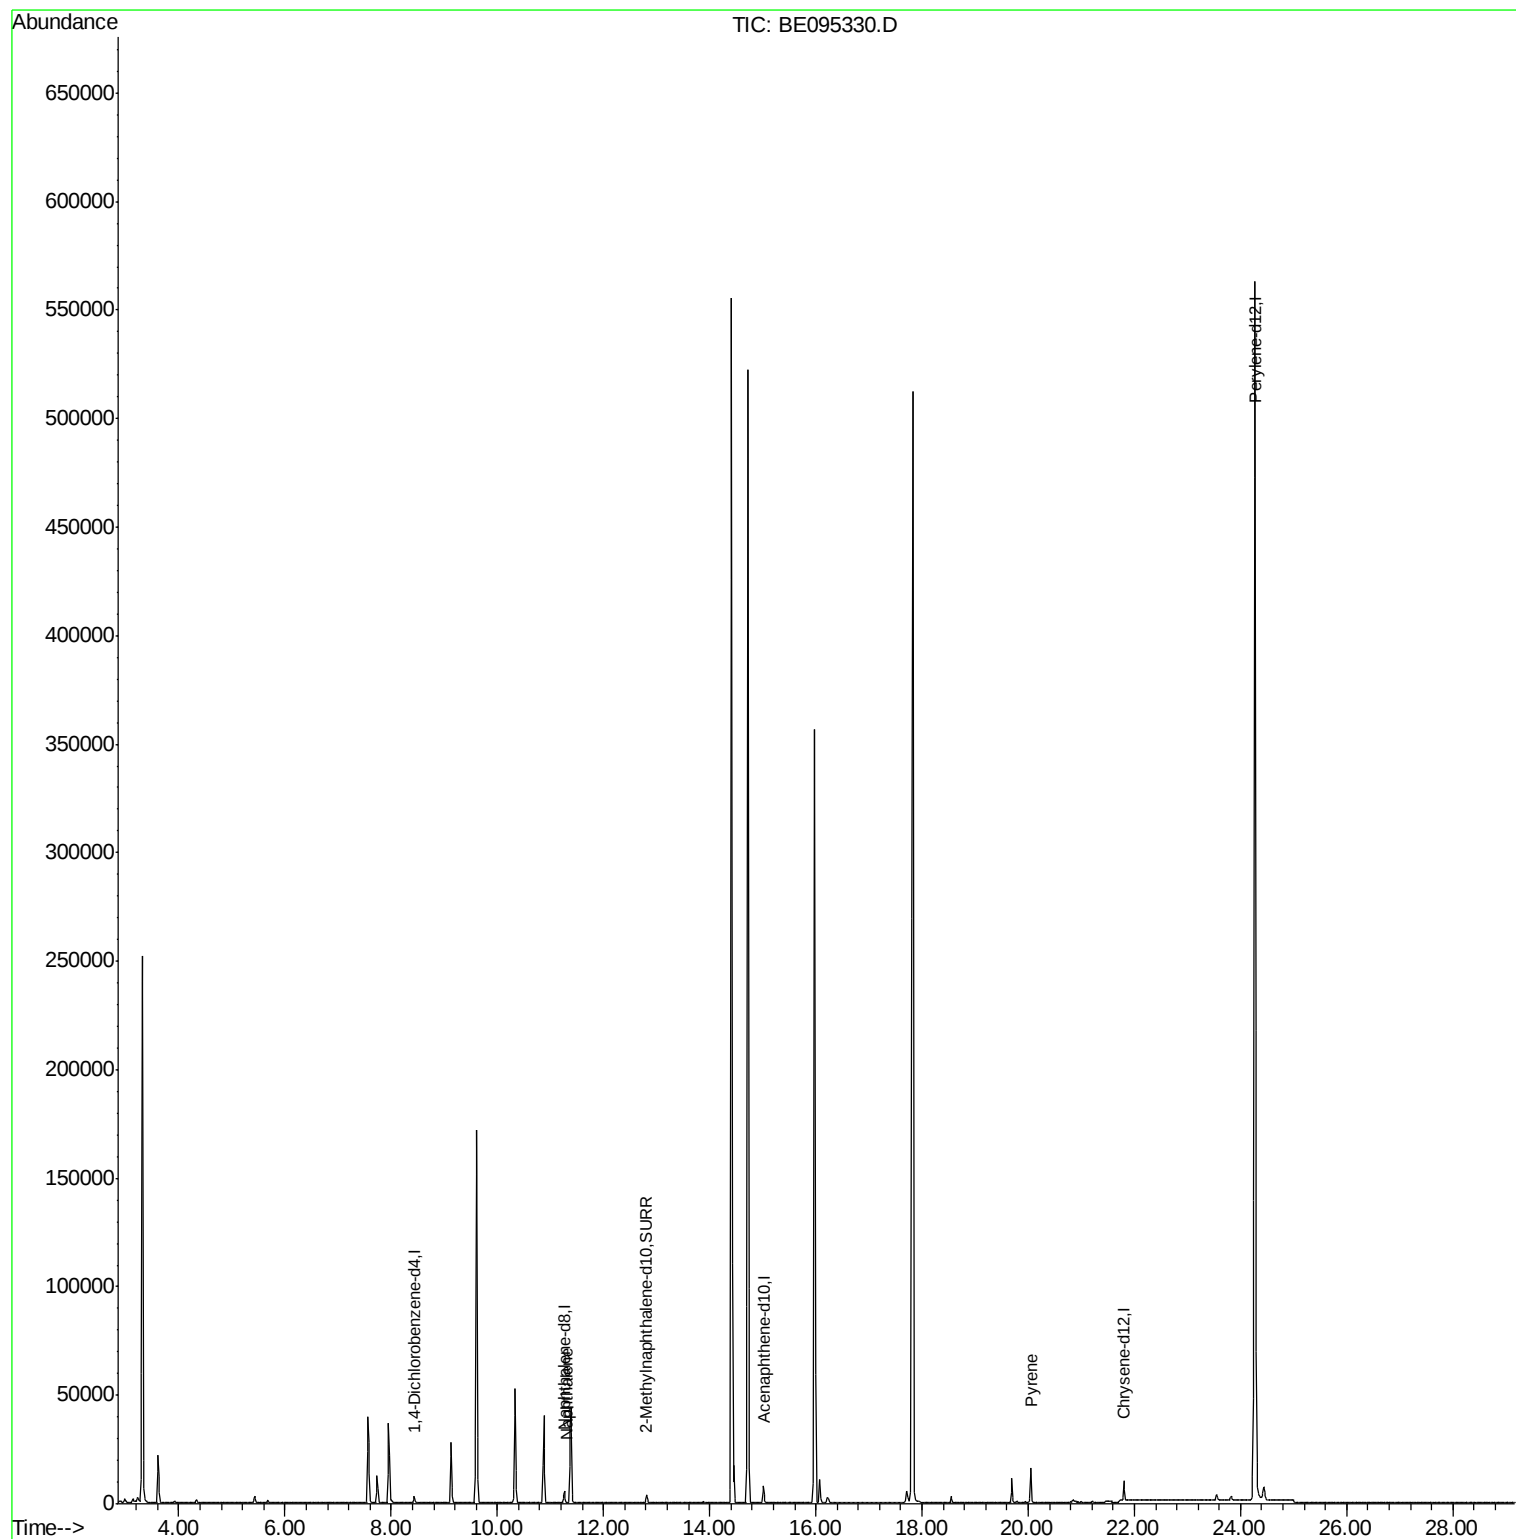

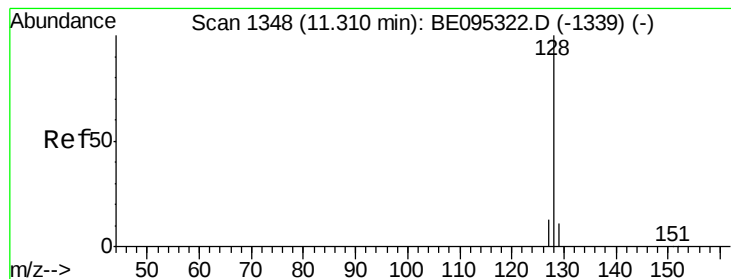

#3

Naphthalene

Concen: 0.021 ng/ul

RT: 11.31 min Scan# 1348

Delta R.T. 0.00 min

Lab File: BE095330.D

Acq: 31 Jan 2018 22:56

Instrument :

BNA_E

ClientSampleId :

F6B79


Tot Ion:128 Resp: 409

Ion Ratio Lower Upper

128 100

129 27.6 11.3 16.9#




127 27.6 4.0 6.0#

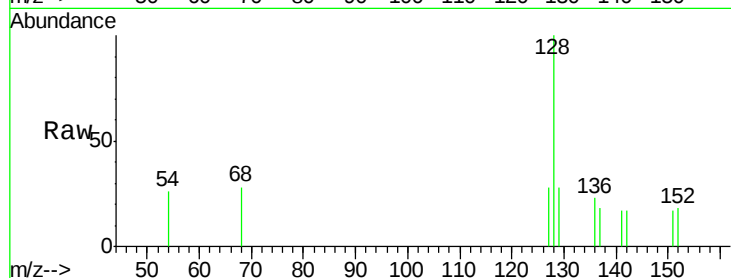

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

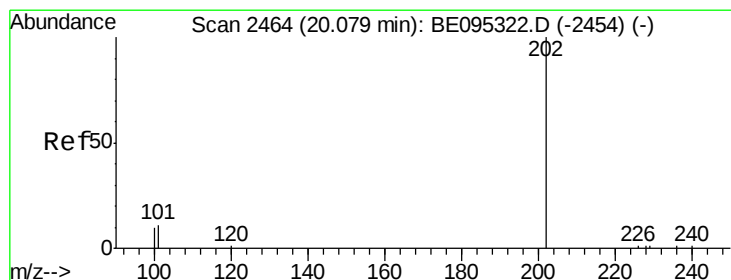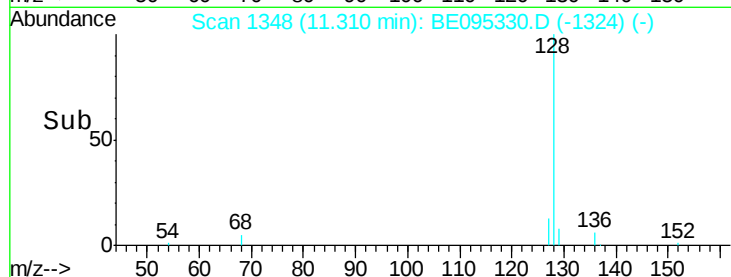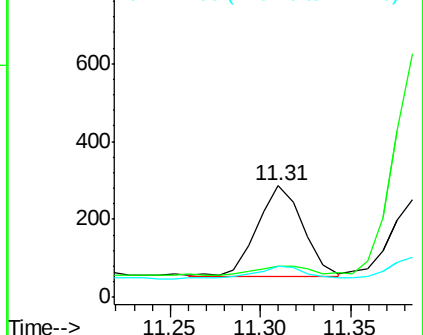

#17

Pyrene

Concen: 0.066 ng/ul

RT: 20.05 min Scan# 2460

Delta R.T. -0.03 min

Lab File: BE095330.D

Acq: 31 Jan 2018 22:56


Tgt Ion:202 Resp: 1976

Ion Ratio Lower Upper

202 100

101 169.9 18.2 27.4#

100 1133.3 15.6 23.4#

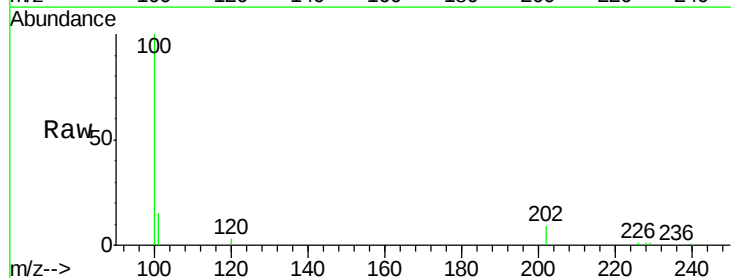

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

