

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013118\
 Data File : BE095334.D
 Acq On : 1 Feb 2018 1:19
 Operator : SJ/JU
 Sample : J1245-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6B71

Quant Time: Feb 01 04:07:23 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 01 04:05:22 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2242	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	6900	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	4515	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.71
16) Chrysene-d12	21.80	240	9063	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	492272	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3774	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	9816	0.00	ng/ul	0.00
Target Compounds						
8) Acenaphthene	15.08	153	774	0.046	ng/ul	92
17) Pyrene	20.05	202	1739	0.057	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013118\
Data File : BE095334.D
Acq On : 1 Feb 2018 1:19
Operator : SJ/JU
Sample : J1245-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6B71

Quant Time: Feb 01 04:07:23 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 04:05:22 2018
Response via : Initial Calibration

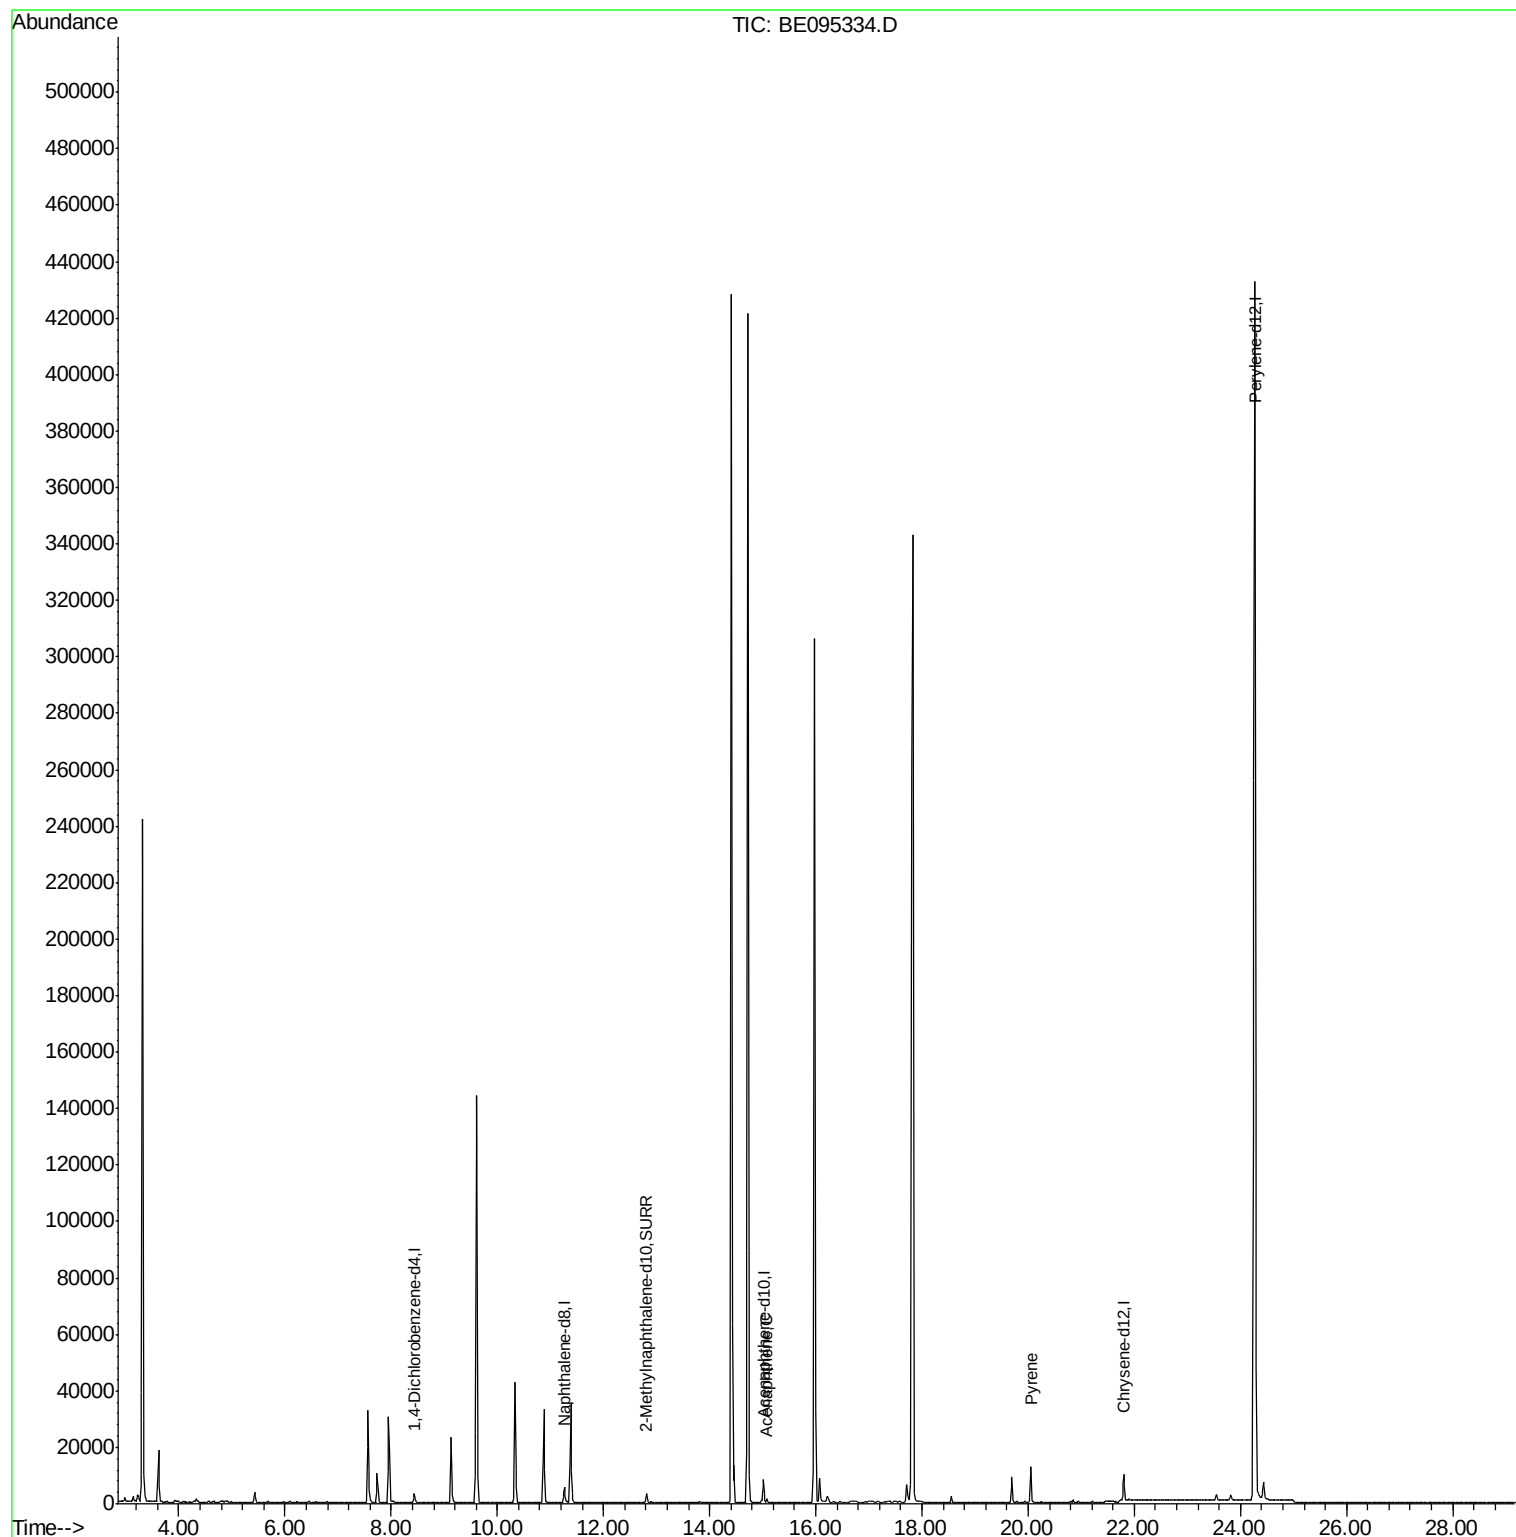

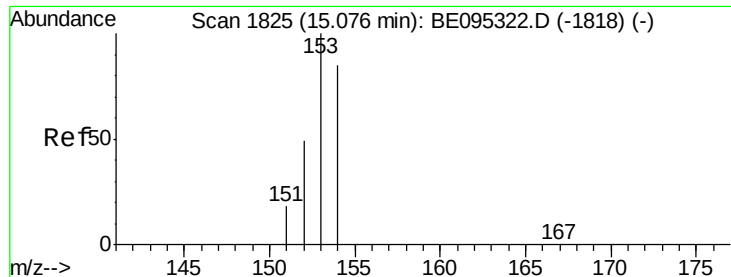

#8

Acenaphthene

Concen: 0.046 ng/ul

RT: 15.08 min Scan# 1825

Delta R.T. -0.00 min

Lab File: BE095334.D

Acq: 1 Feb 2018 1:19

Instrument :

BNA_E

ClientSampleId :

F6B71


Tot Ion:153 Resp: 774

Ion Ratio Lower Upper




153 100

152 53.7 36.0 54.0

154 85.6 72.0 108.0

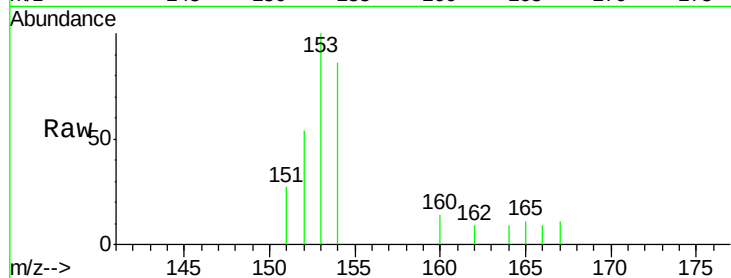

Abundance Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E
Ion 154.00 (153.70 to 154.70): E

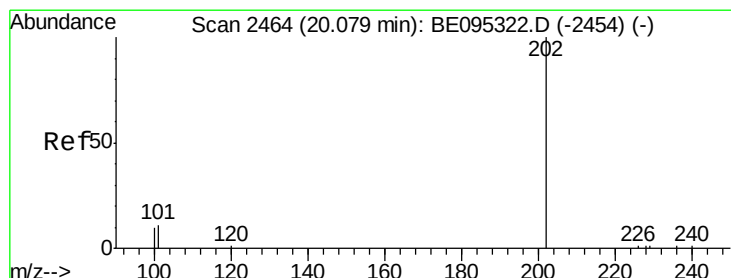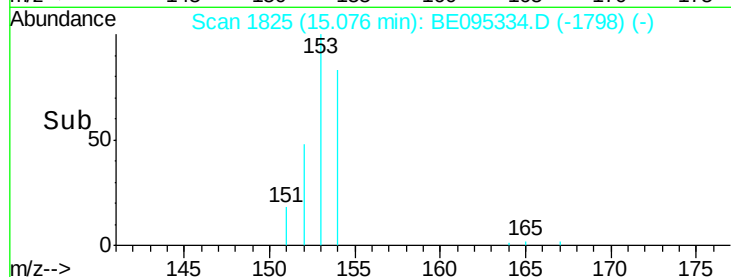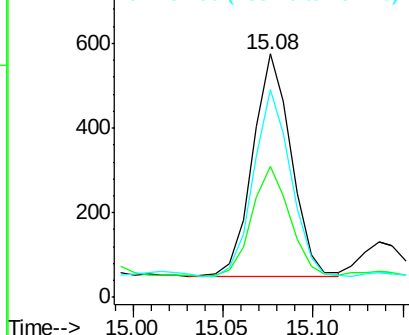

#17

Pyrene

Concen: 0.057 ng/ul

RT: 20.05 min Scan# 2460

Delta R.T. -0.03 min

Lab File: BE095334.D

Acq: 1 Feb 2018 1:19


Tgt Ion:202 Resp: 1739

Ion Ratio Lower Upper

202 100

101 168.1 18.2 27.4#

100 1101.1 15.6 23.4#

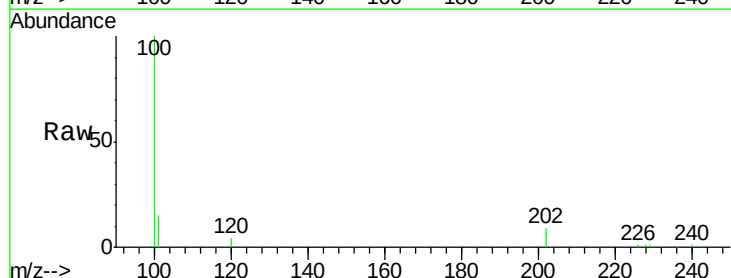

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): E

