

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013118\
 Data File : BE095336.D
 Acq On : 1 Feb 2018 2:31
 Operator : SJ/JU
 Sample : J1245-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6B69

Quant Time: Feb 01 04:07:38 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 01 04:05:22 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2372	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	7618	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	4946	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.71
16) Chrysene-d12	21.81	240	9900	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	631830	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	4850	0.39	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	12267	0.00	ng/ul	0.00
Target Compounds						
5) 2-Methylnaphthalene	12.89	142	348	0.024	ng/ul	99
17) Pyrene	20.05	202	2546	0.077	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013118\
Data File : BE095336.D
Acq On : 1 Feb 2018 2:31
Operator : SJ/JU
Sample : J1245-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6B69

Quant Time: Feb 01 04:07:38 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 04:05:22 2018
Response via : Initial Calibration

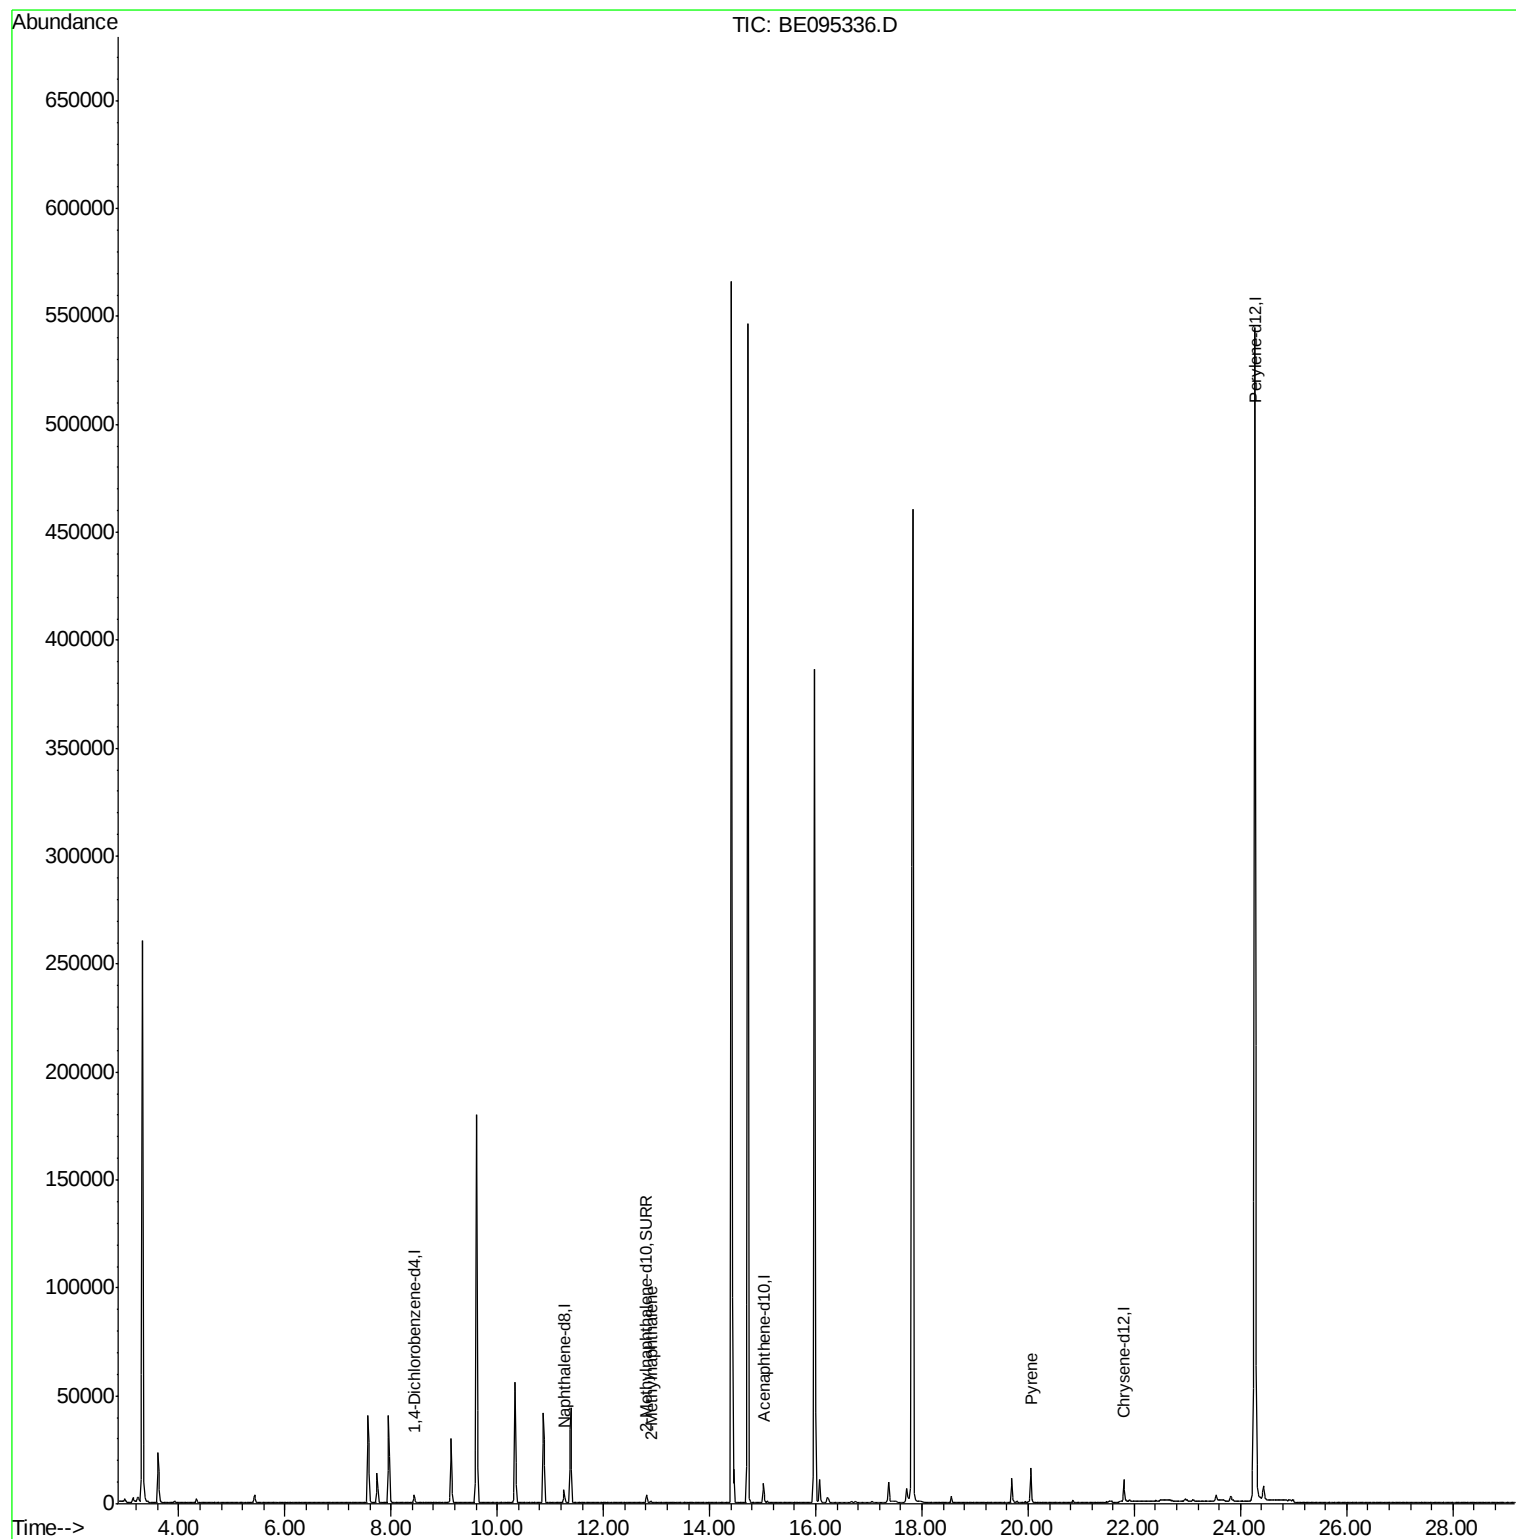

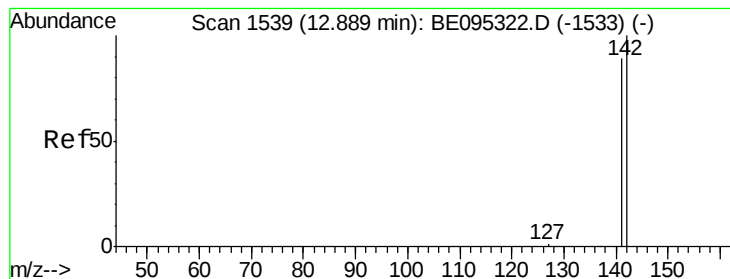

#5

2-Methylnaphthalene

Concen: 0.024 ng/ul

RT: 12.89 min Scan# 1539

Delta R.T. -0.00 min

Lab File: BE095336.D

Acq: 1 Feb 2018 2:31

Instrument :

BNA_E

ClientSampleId :


F6B69

Tot Ion:142 Resp: 348

Ion Ratio Lower Upper

142 100

141 92.0 72.6 108.8

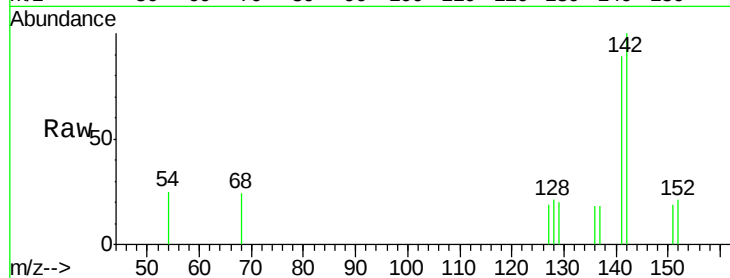

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

12.89

250

200



150

100

50

0

Time-->

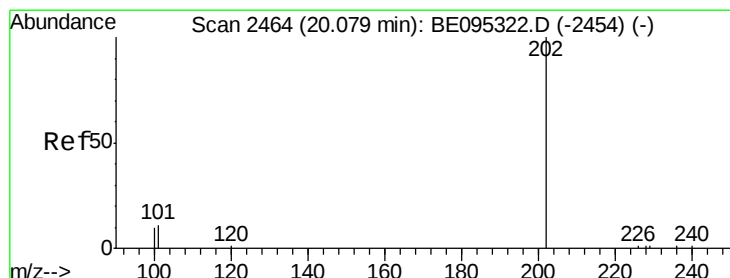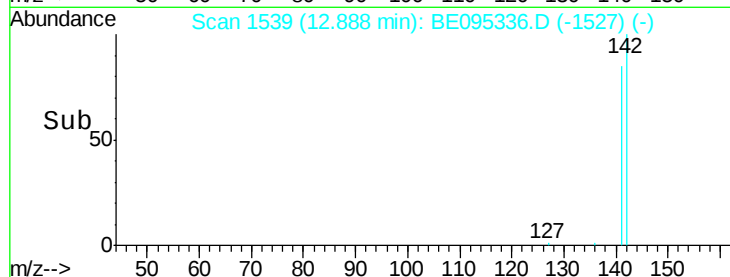

#17

Pyrene

Concen: 0.077 ng/ul

RT: 20.05 min Scan# 2460

Delta R.T. -0.03 min

Lab File: BE095336.D

Acq: 1 Feb 2018 2:31


Tgt Ion:202 Resp: 2546

Ion Ratio Lower Upper

202 100

101 171.6 18.2 27.4#

100 1180.5 15.6 23.4#

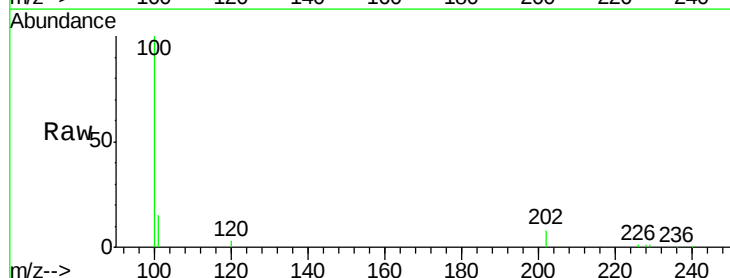

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

20.05

15000

10000

5000

0

Time-->

