

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013118\
 Data File : BE095337.D
 Acq On : 1 Feb 2018 3:07
 Operator : SJ/JU
 Sample : J1245-17
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6B78

Quant Time: Feb 01 04:07:43 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 01 04:05:22 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2310	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	7286	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	4887	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.71
16) Chrysene-d12	21.80	240	9801	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	687546	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	4795	0.40	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	13109	0.00	ng/ul	0.00
Target Compounds						
					Ovalue	
17) Pyrene	20.08	202	8681	0.264	ng/ul#	82
18) Benzo(a)anthracene	21.79	228	2365	0.077	ng/ul#	90
19) Chrysene	21.84	228	2623	0.082	ng/ul#	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013118\
Data File : BE095337.D
Acq On : 1 Feb 2018 3:07
Operator : SJ/JU
Sample : J1245-17
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6B78

Quant Time: Feb 01 04:07:43 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 04:05:22 2018
Response via : Initial Calibration

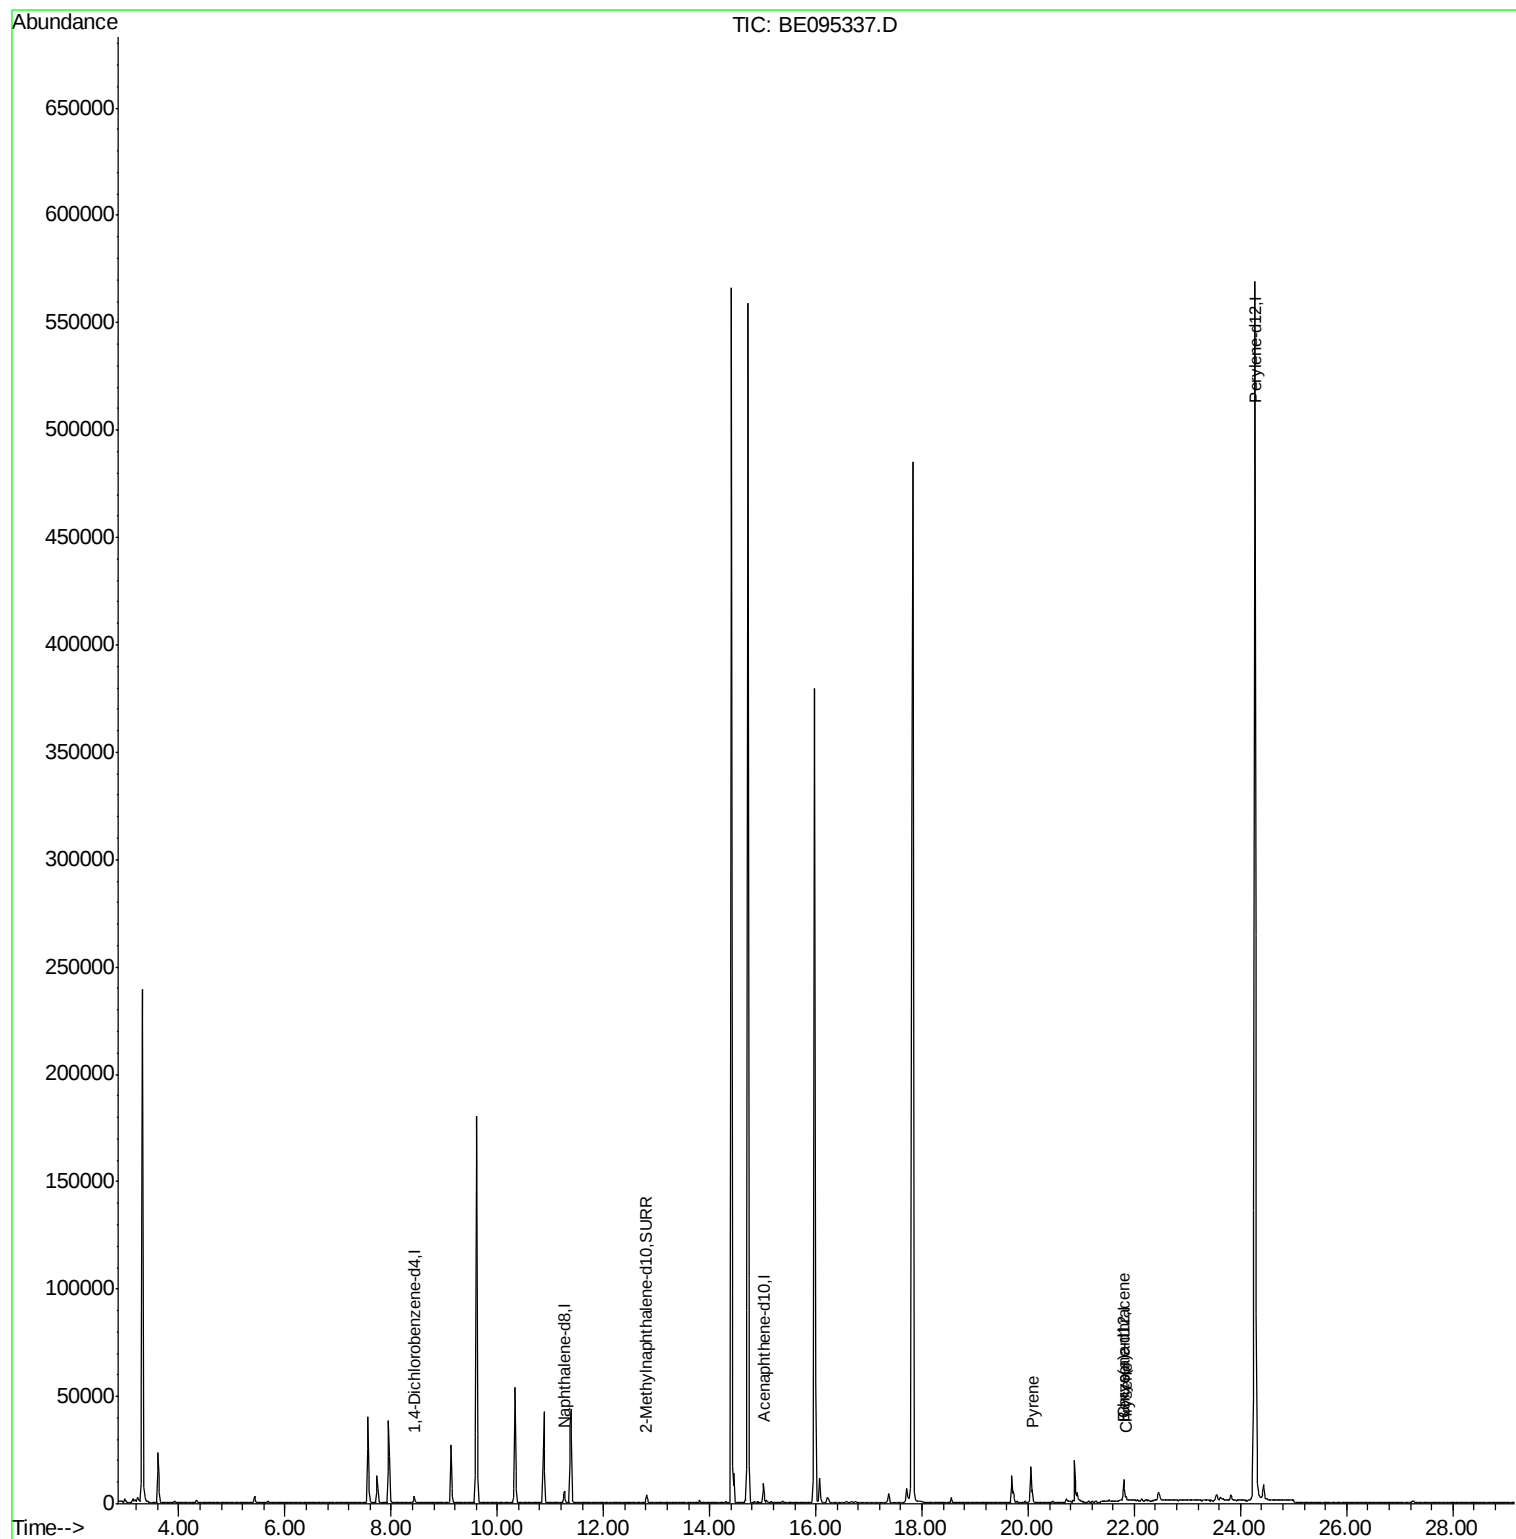

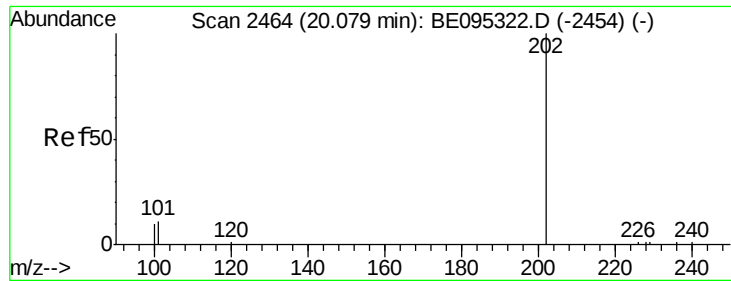

#17

Pvrene

Concen: 0.264 ng/ul

RT: 20.08 min Scan# 2464

Delta R.T. -0.00 min

Lab File: BE095337.D

Acq: 1 Feb 2018 3:07

Instrument :

BNA_E

ClientSampleId :

F6B78


Tot Ion:202 Resp: 8681

Ion Ratio Lower Upper

202 100

101 13.0 18.2 27.4#




100 12.8 15.6 23.4#

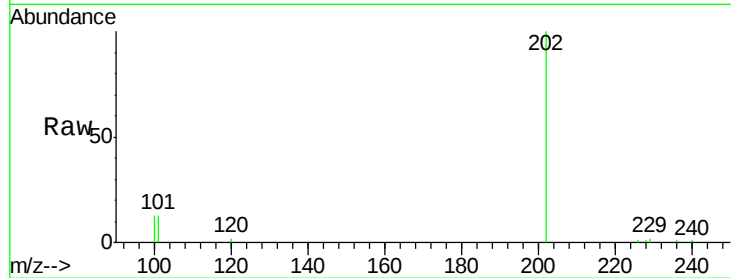

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BE

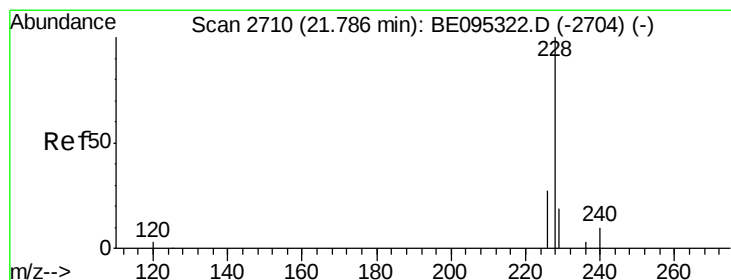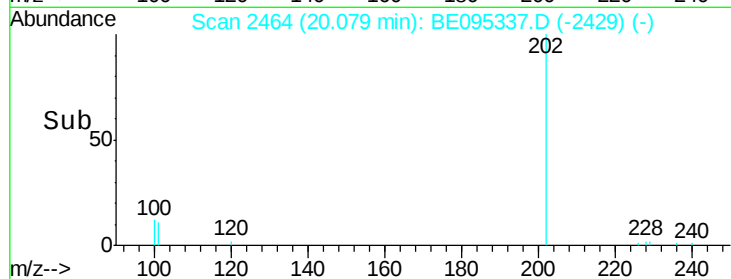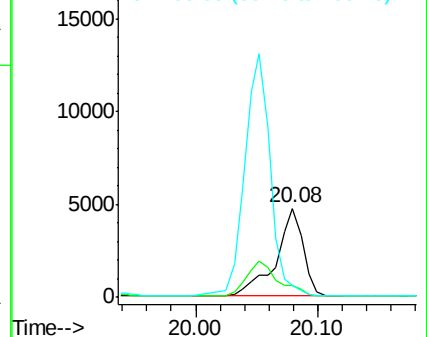

#18

Benzo(a)anthracene

Concen: 0.077 ng/ul

RT: 21.79 min Scan# 2710

Delta R.T. 0.00 min

Lab File: BE095337.D

Acq: 1 Feb 2018 3:07


Tgt Ion:228 Resp: 2365

Ion Ratio Lower Upper

228 100

229 29.5 22.8 34.2



226 31.6 17.0 25.6#



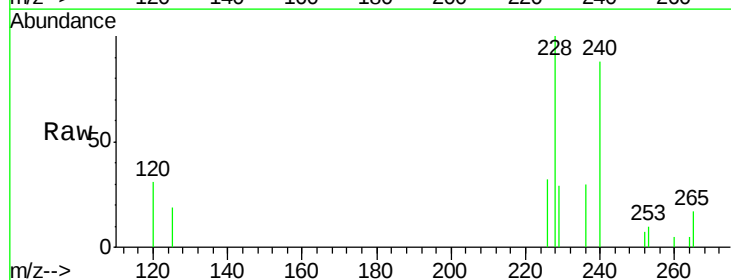


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

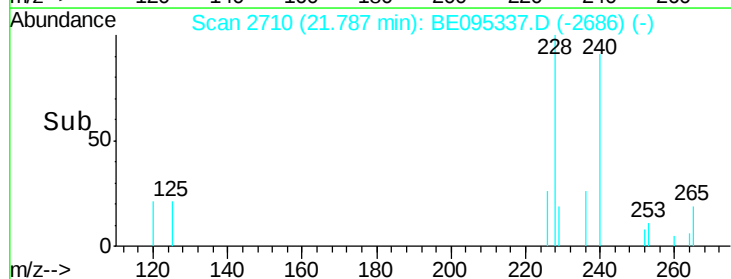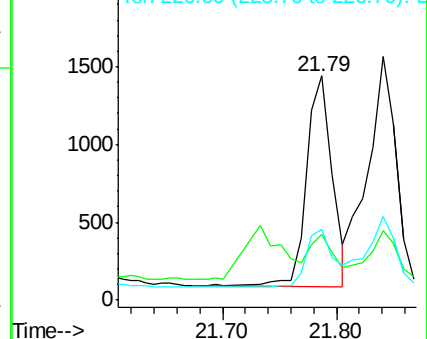

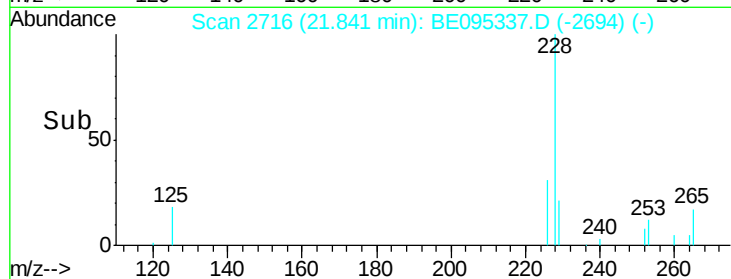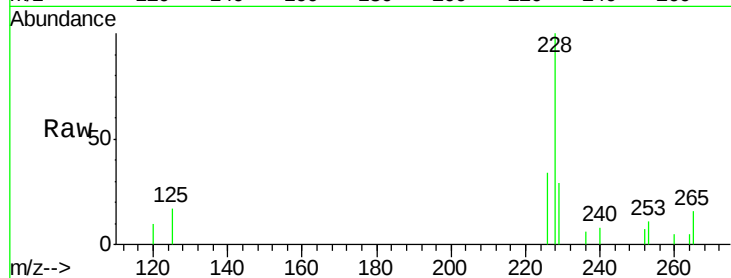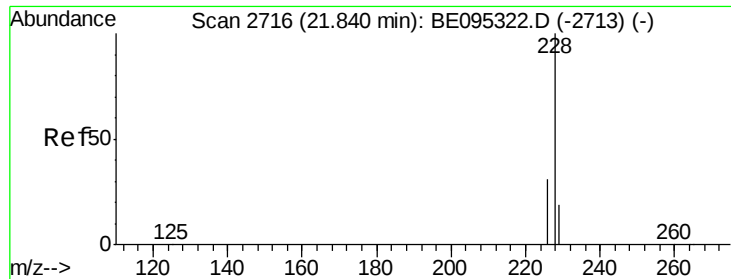

#19

Chrysene

Concen: 0.082 ng/ul

RT: 21.84 min Scan# 2716

Delta R.T. 0.00 min

Lab File: BE095337.D

Acq: 1 Feb 2018 3:07

Instrument :

BNA_E

ClientSampleId :

F6B78

Tot Ion:228 Resp: 2623

Ion Ratio Lower Upper

228 100

226 34.2 23.4 35.0

229 28.6 17.7 26.5#

