

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013118\
 Data File : BE095339.D
 Acq On : 1 Feb 2018 4:18
 Operator : SJ/JU
 Sample : J1245-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6B62

Quant Time: Feb 01 06:27:52 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 01 06:27:03 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2280	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	7076	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	4653	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.71
16) Chrysene-d12	21.80	240	9195	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	535845	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	4084	0.35	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	10492	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	20.08	202	1160	0.038	ng/ul#	Ovalue 94




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013118\
Data File : BE095339.D
Acq On : 1 Feb 2018 4:18
Operator : SJ/JU
Sample : J1245-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6B62

Quant Time: Feb 01 06:27:52 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 06:27:03 2018
Response via : Initial Calibration

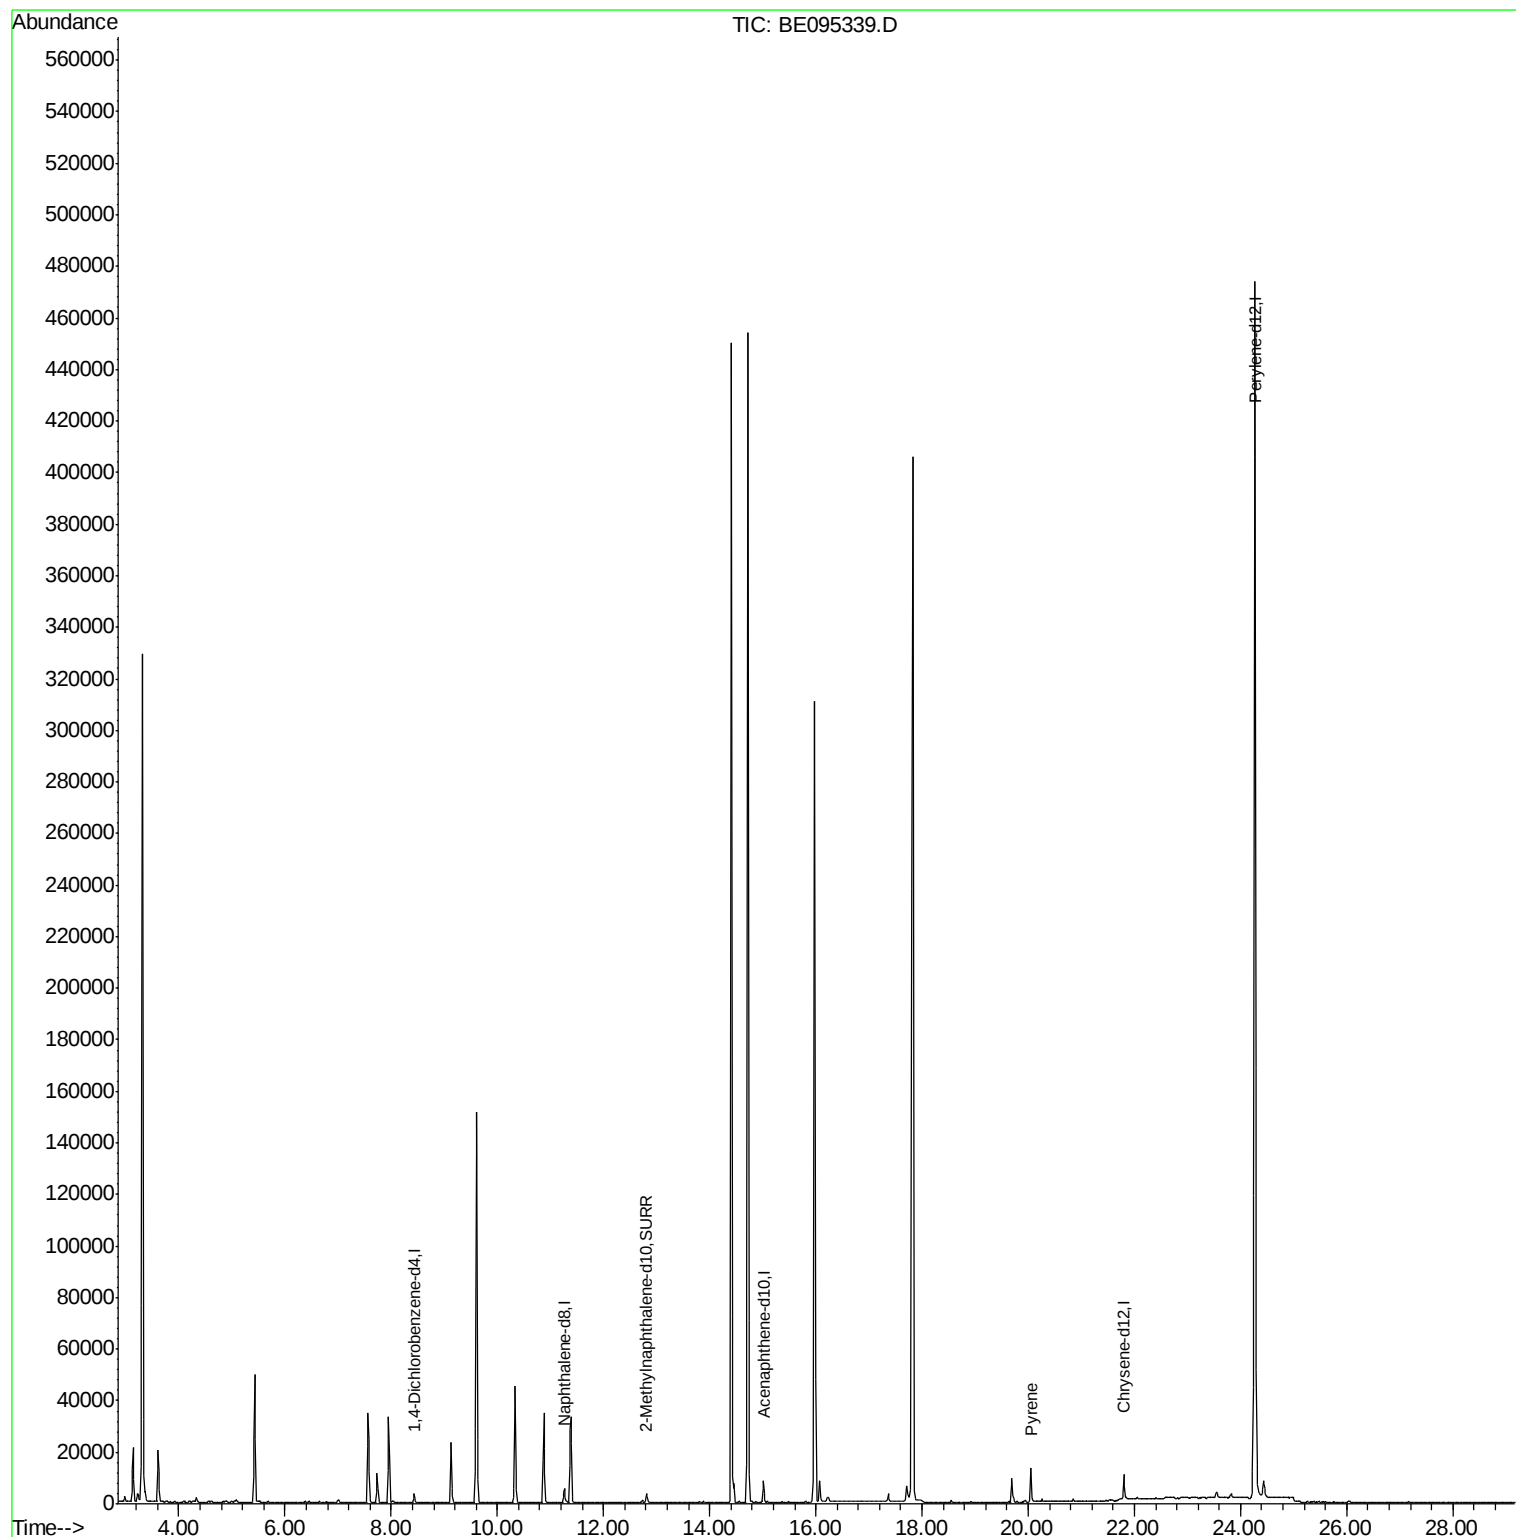

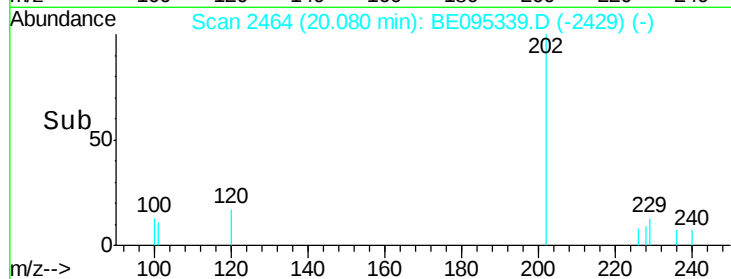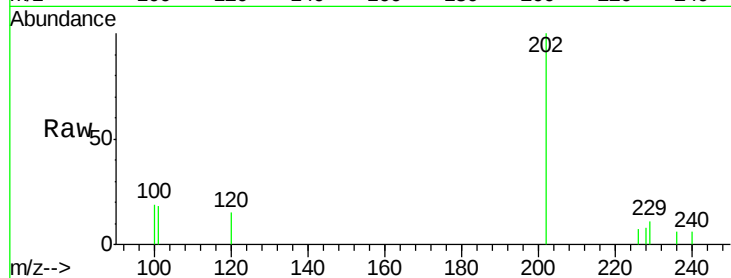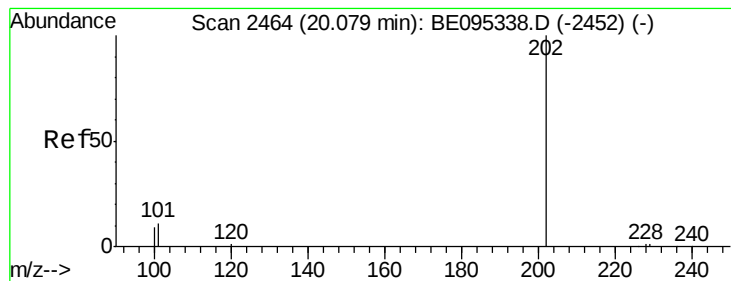

#17

Pvrene

Concen: 0.038 ng/ul

RT: 20.08 min Scan# 2464

Delta R.T. 0.00 min

Lab File: BE095339.D

Acq: 1 Feb 2018 4:18

Instrument :

BNA_E

ClientSampleId :

F6B62

Tot Ion: 202 Resp: 1160

Ion Ratio Lower Upper

202 100

101 18.0 18.2 27.4#

100 18.6 15.6 23.4

